

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012621\
 Data File : PP032979.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jan 2021 19:43
 Operator : DD\AJ
 Sample : M1242-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 0026-SITE-WATER-048-03-04

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:47:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.737	4.010	1070507	909449	18.431	19.333
2) SA Decachlor...	10.569	9.283	732564	692494	18.568	18.485
Target Compounds						
8) L2 AR-1221-1	4.983	0.000	58870	0	96.273	N.D. #
34) L7 AR-1260-4	8.553f	0.000	39564	0	19.202	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012621\
Data File : PP032979.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jan 2021 19:43
Operator : DD\AJ
Sample : M1242-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
0026-SITE-WATER-048-03-04

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:47:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

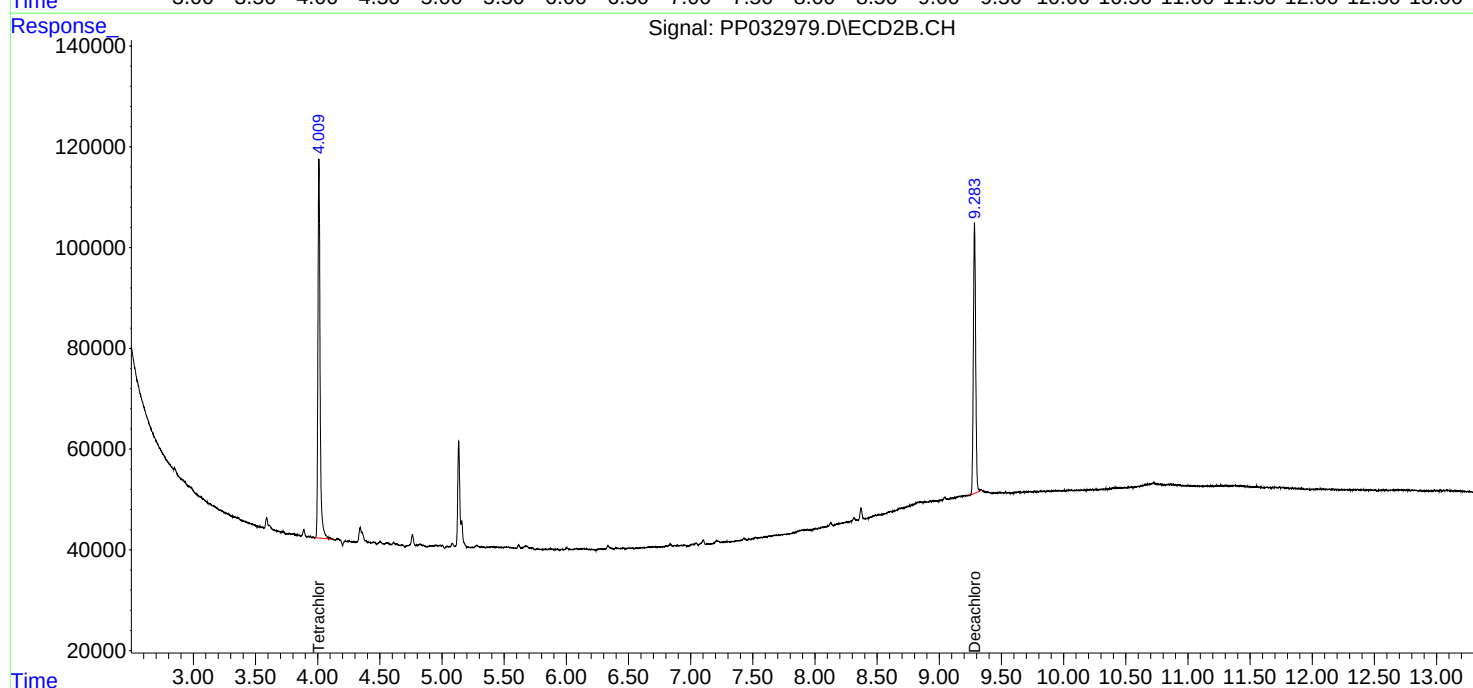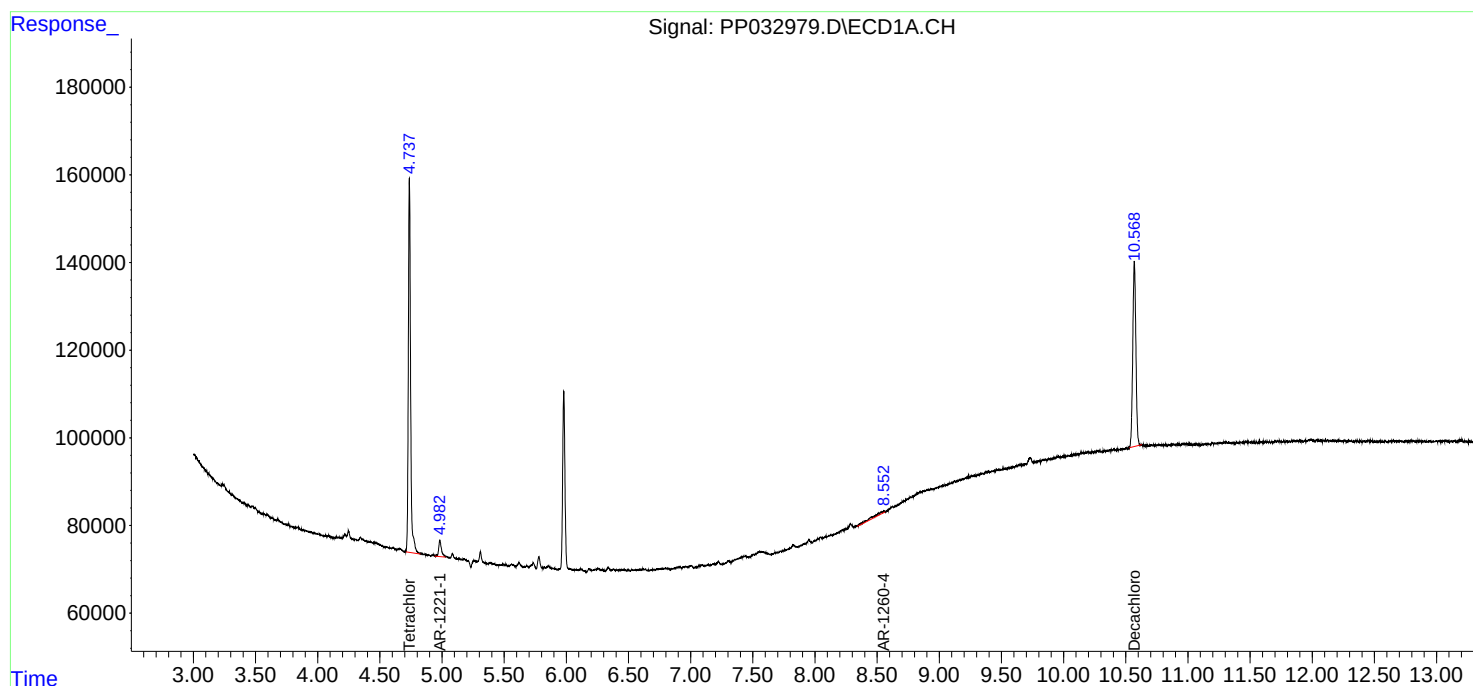


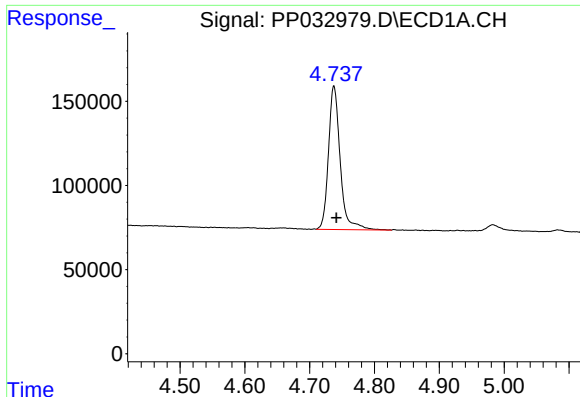

#1 Tetrachloro-m-xylene


R.T.: 4.737 min
Delta R.T.: -0.004 min
Response: 1070507
Conc: 18.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
0026-SITE-WATER-048-03-04

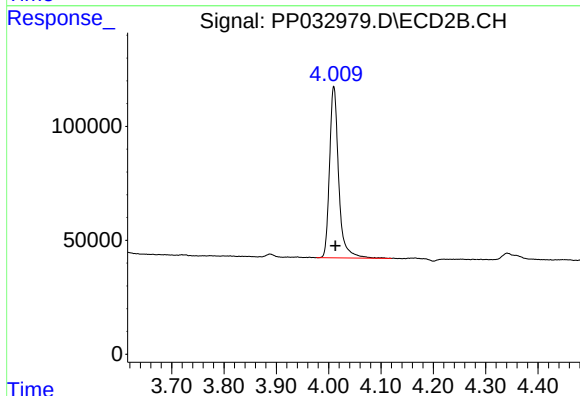


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
Delta R.T.: -0.003 min
Response: 909449
Conc: 19.33 ng/ml

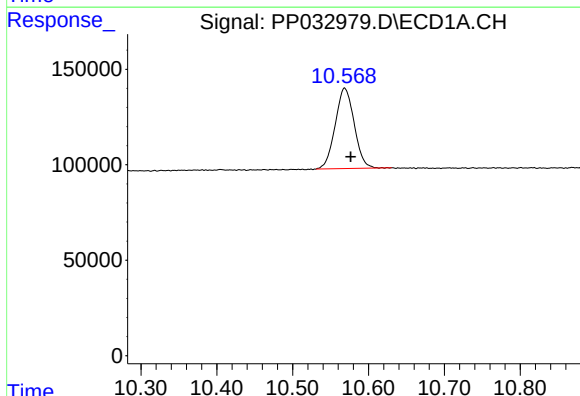


#2 Decachlorobiphenyl

R.T.: 10.569 min
Delta R.T.: -0.008 min
Response: 732564
Conc: 18.57 ng/ml

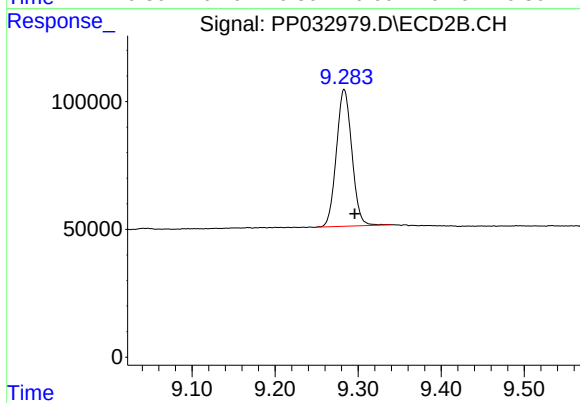

#2 Decachlorobiphenyl


R.T.: 9.283 min
Delta R.T.: -0.013 min
Response: 692494
Conc: 18.49 ng/ml

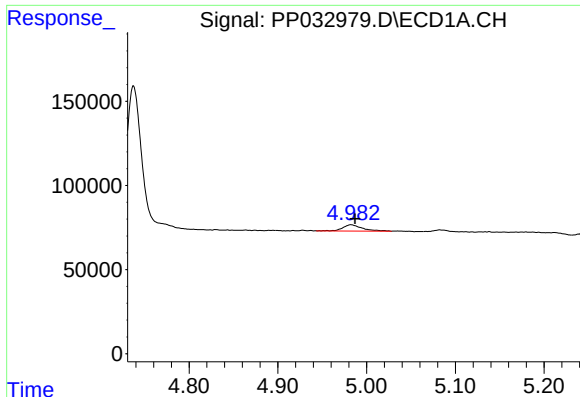

#8 AR-1221-1


R.T.: 4.983 min
Delta R.T.: -0.004 min
Response: 58870
Conc: 96.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
0026-SITE-WATER-048-03-04

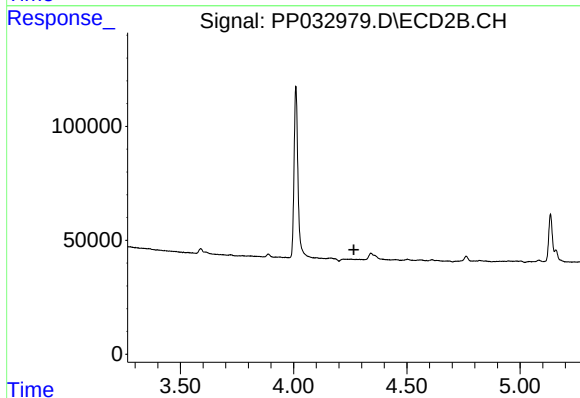


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.266 min
Response: 0
Conc: N.D.

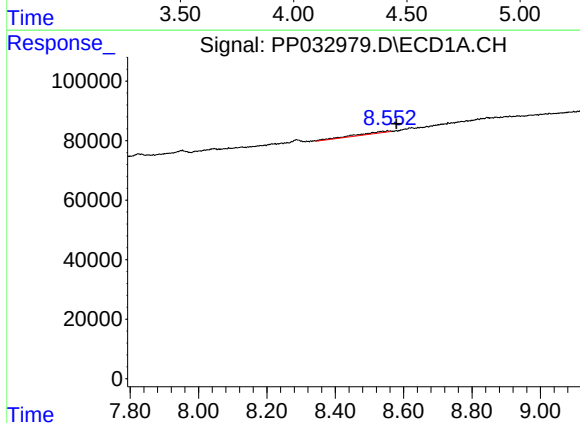

#34 AR-1260-4

R.T.: 8.553 min
Delta R.T.: -0.026 min
Response: 39564
Conc: 19.20 ng/ml

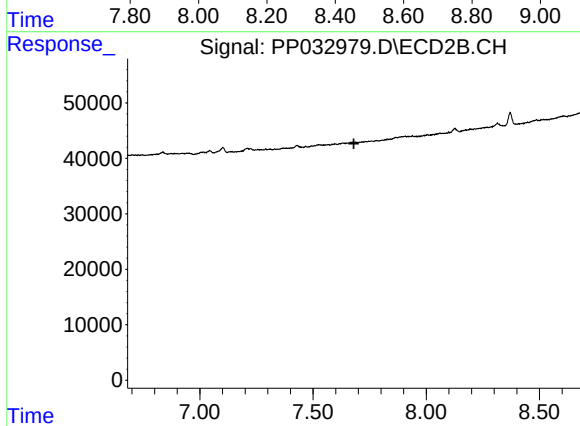

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.680 min
Response: 0
Conc: N.D.