

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012621\
 Data File : PP032972.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jan 2021 17:45
 Operator : DD\AJ
 Sample : M1190-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20796

Manual Integrations
 APPROVED

mohammad
 1/27/2021 5:24:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:43:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.739	4.011	646155	518513	11.125	11.023
2) SA Decachlor...	10.599f	9.314f	632741	557064	16.038m	14.870m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012621\
Data File : PP032972.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jan 2021 17:45
Operator : DD\AJ
Sample : M1190-02
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
20796


Manual Integrations
APPROVED

mohammad
1/27/2021 5:24:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:43:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

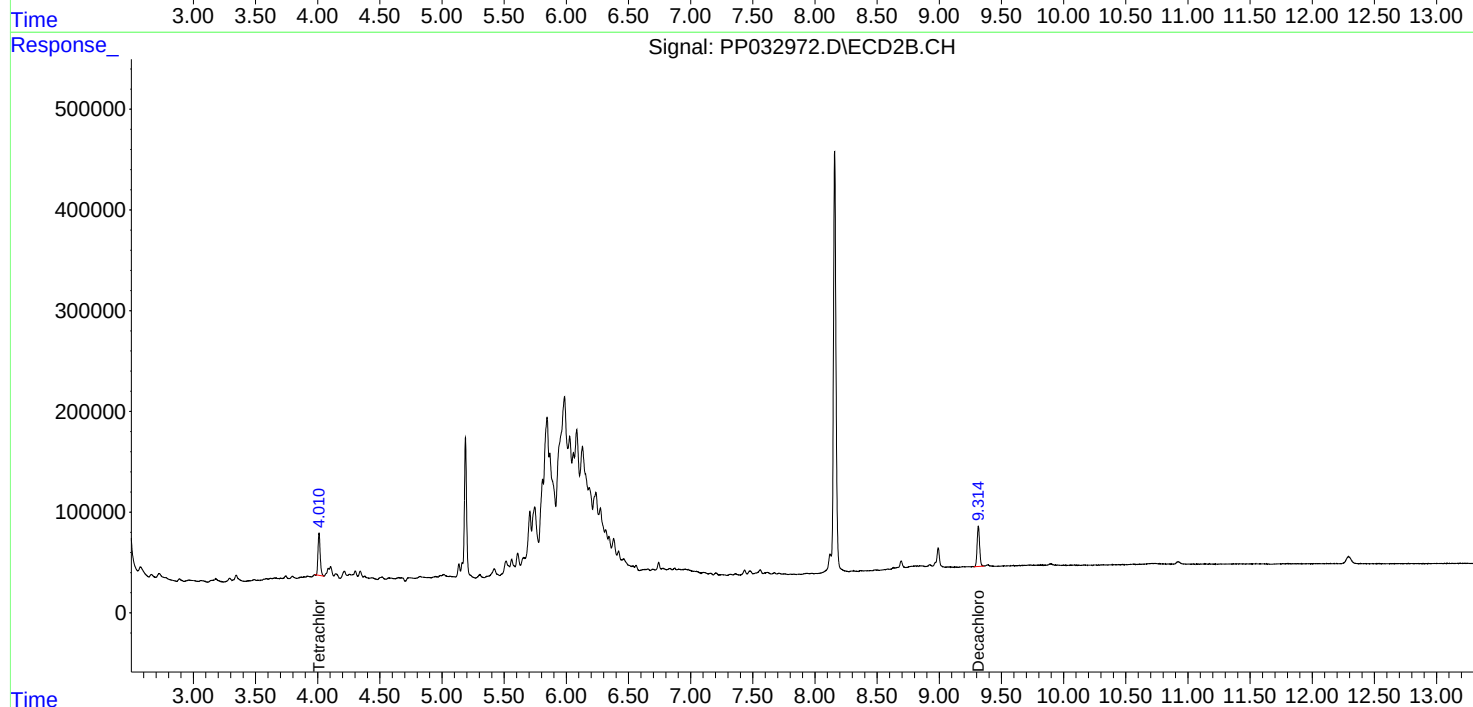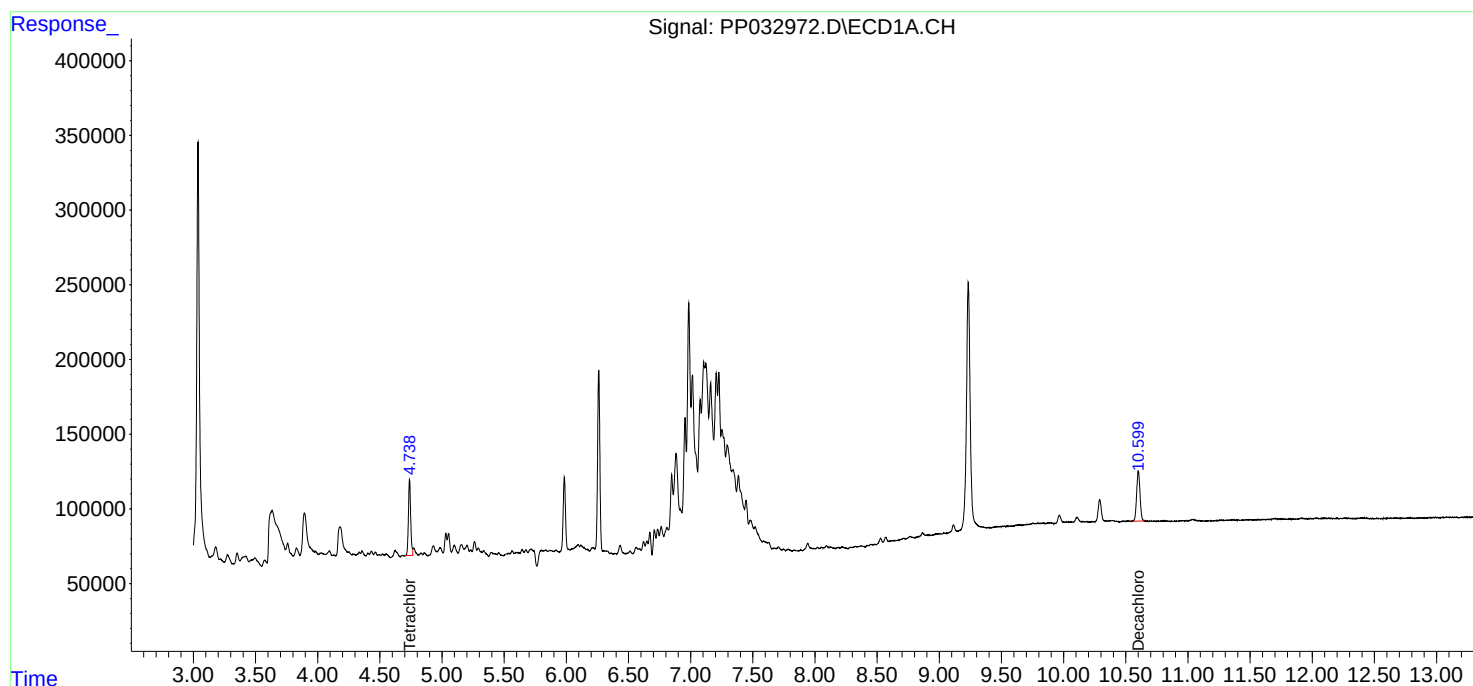

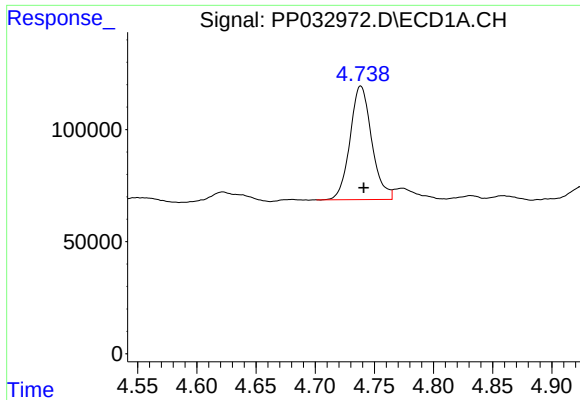


#1 Tetrachloro-m-xylene

R.T.: 4.739 min
Delta R.T.: -0.002 min
Response: 646155
Conc: 11.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
20796


Manual Integrations
APPROVED

mohammad
1/27/2021 5:24:52 PM

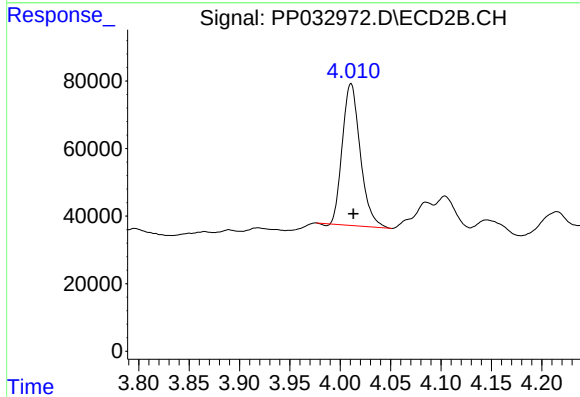


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: -0.002 min
Response: 518513
Conc: 11.02 ng/ml

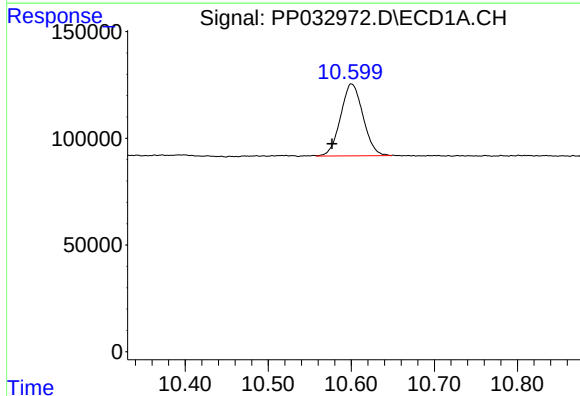

#2 Decachlorobiphenyl

R.T.: 10.599 min
Delta R.T.: 0.022 min
Response: 632741
Conc: 16.04 ng/ml m

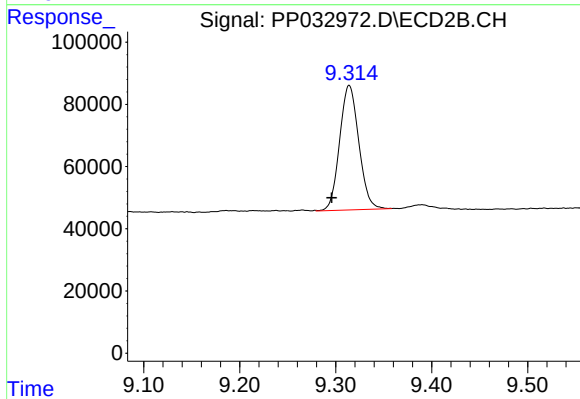

#2 Decachlorobiphenyl

R.T.: 9.314 min
Delta R.T.: 0.018 min
Response: 557064
Conc: 14.87 ng/ml m