

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012622\
 Data File : PP043290.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jan 2022 13:29
 Operator : AJ\MA
 Sample : N1266-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:40:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 25 03:09:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.869	4.034	452401	482593	19.682	21.658
2)	SA Decachlor...	10.787	9.359	273221	342708	19.291	18.383
Target Compounds							
29)	L6 AR-1254-4	7.994	0.000	8849	0	12.554	N.D. #
31)	L7 AR-1260-1	7.863	0.000	1702	0	2.205	N.D. #
34)	L7 AR-1260-4	0.000	7.728	0	217777	N.D.	222.014 #
37)	L8 AR-1262-2	0.000	7.728	0	217777	N.D.	157.138 #
39)	L8 AR-1262-4	0.000	8.339	0	14426	N.D.	7.665 #
42)	L9 AR-1268-2	0.000	8.339	0	14426	N.D.	5.399 #
45)	L9 AR-1268-5	10.471	0.000	9320	0	1.841	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012622\
Data File : PP043290.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jan 2022 13:29
Operator : AJ\MA
Sample : N1266-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:40:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

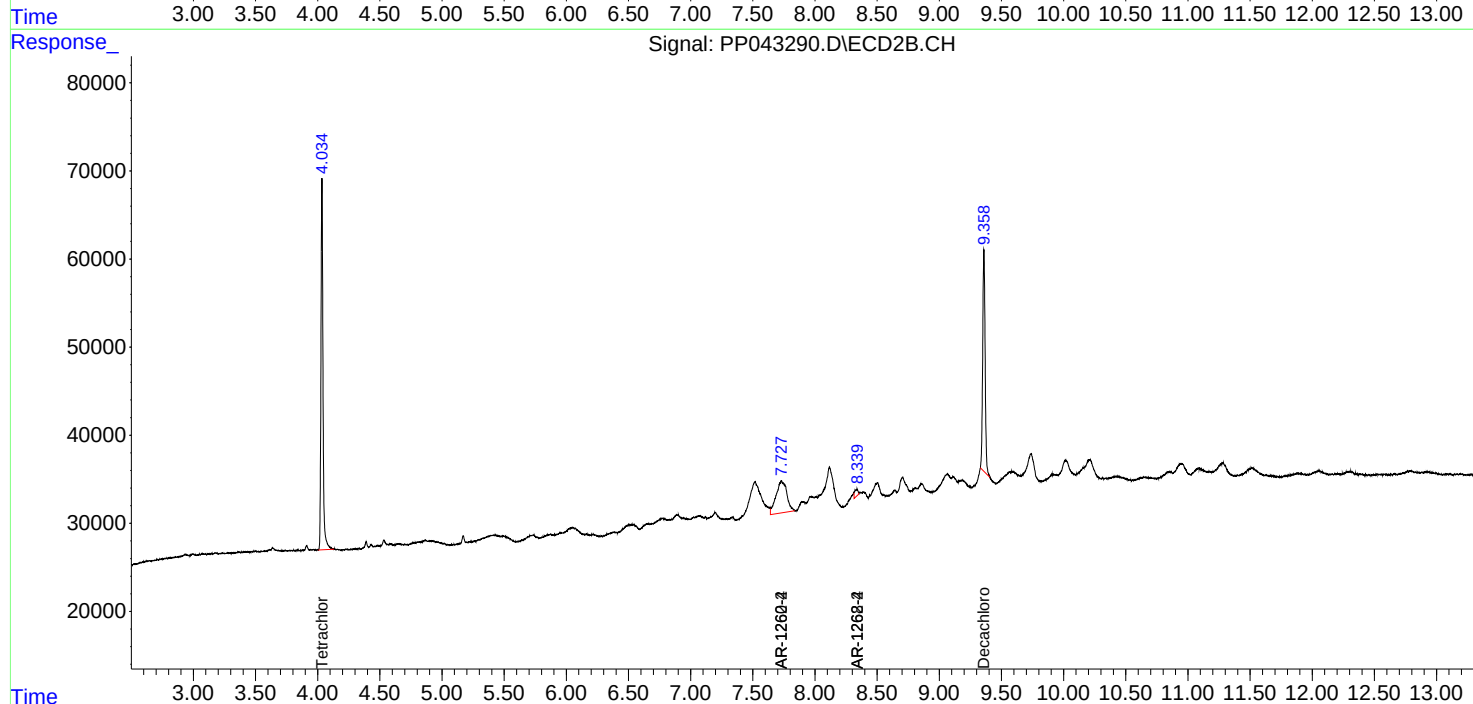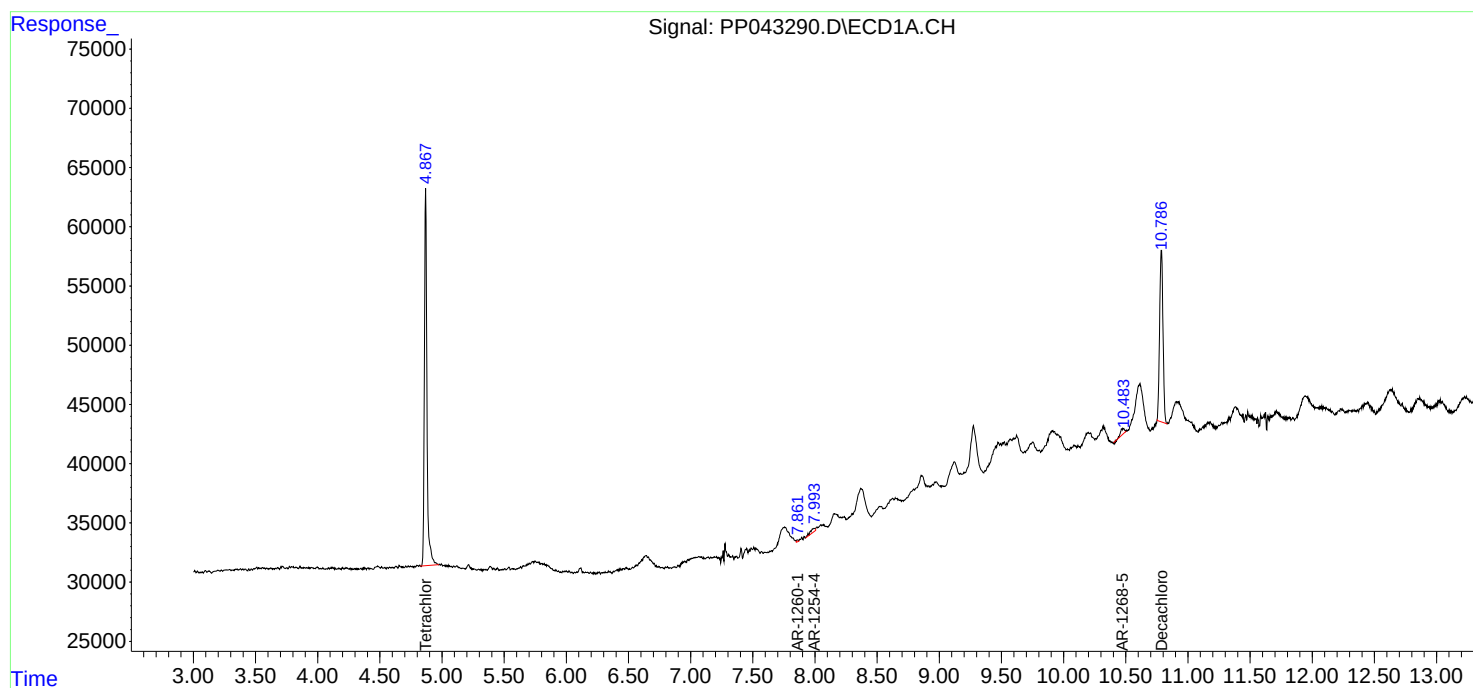


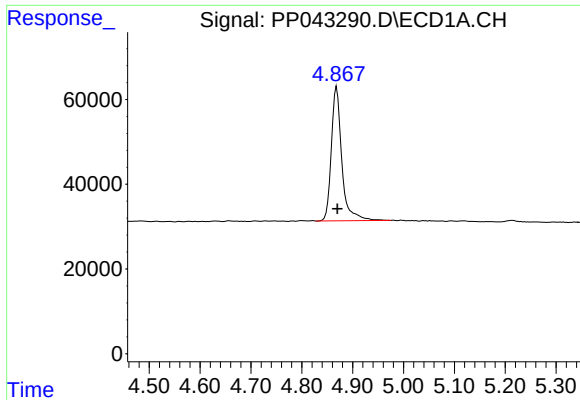

#1 Tetrachloro-m-xylene


R.T.: 4.869 min
Delta R.T.: -0.001 min
Response: 452401
Conc: 19.68 ng/ml

Instrument :
ECD_P
ClientSampleId :

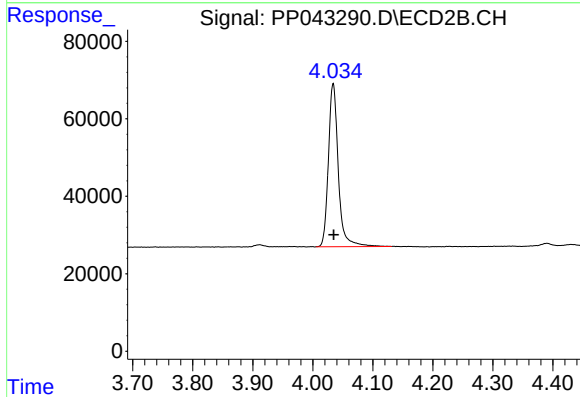


#1 Tetrachloro-m-xylene

R.T.: 4.034 min
Delta R.T.: 0.000 min
Response: 482593
Conc: 21.66 ng/ml

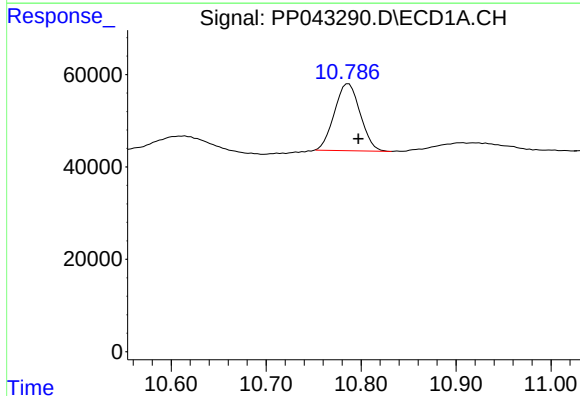


#2 Decachlorobiphenyl

R.T.: 10.787 min
Delta R.T.: -0.010 min
Response: 273221
Conc: 19.29 ng/ml

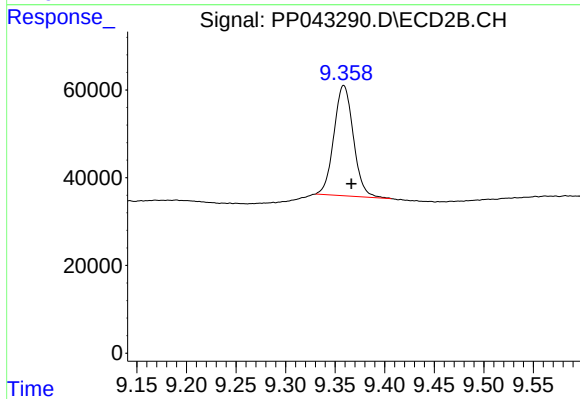

#2 Decachlorobiphenyl


R.T.: 9.359 min
Delta R.T.: -0.008 min
Response: 342708
Conc: 18.38 ng/ml

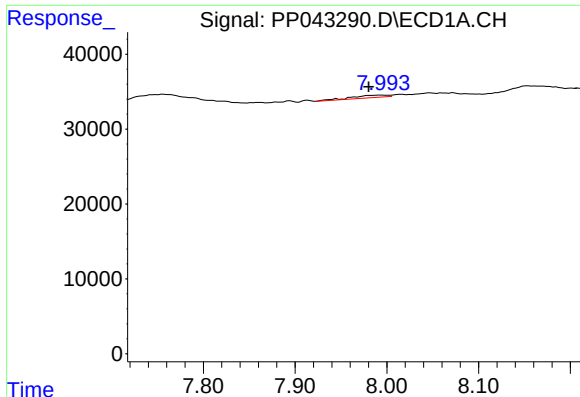

#29 AR-1254-4


R.T.: 7.994 min
Delta R.T.: 0.014 min
Response: 8849
Conc: 12.55 ng/ml

Instrument :
ECD_P
ClientSampleId :

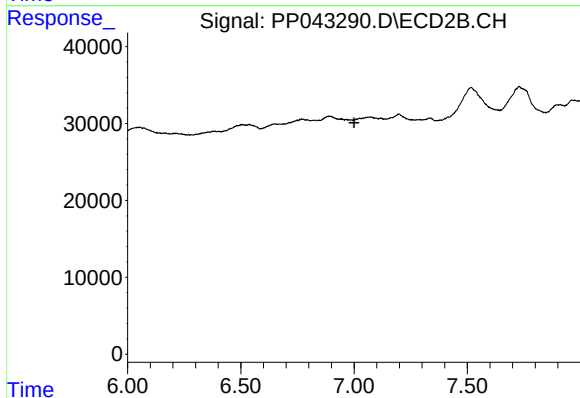


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.000 min
Response: 0
Conc: N.D.

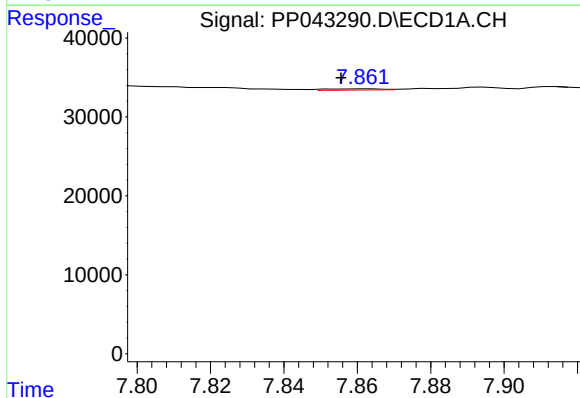


#31 AR-1260-1

R.T.: 7.863 min
Delta R.T.: 0.007 min
Response: 1702
Conc: 2.21 ng/ml

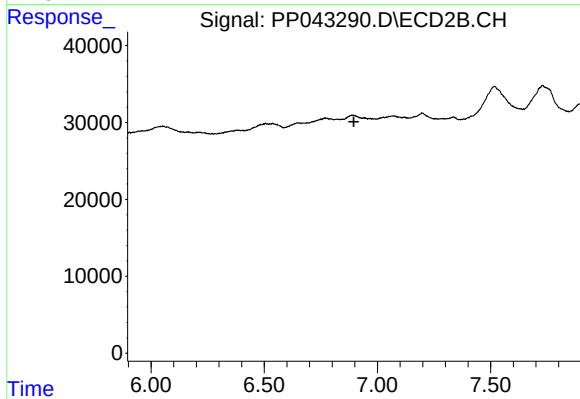

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.896 min
Response: 0
Conc: N.D.

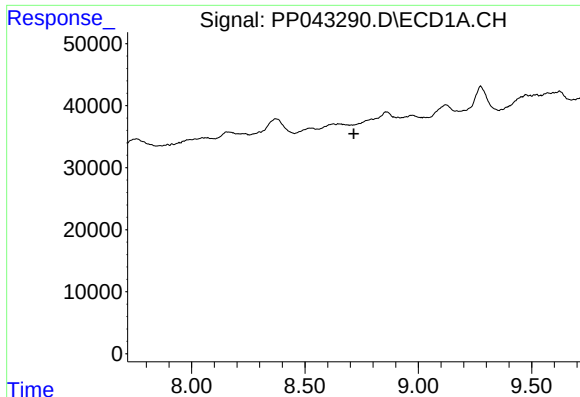

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 8.715 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

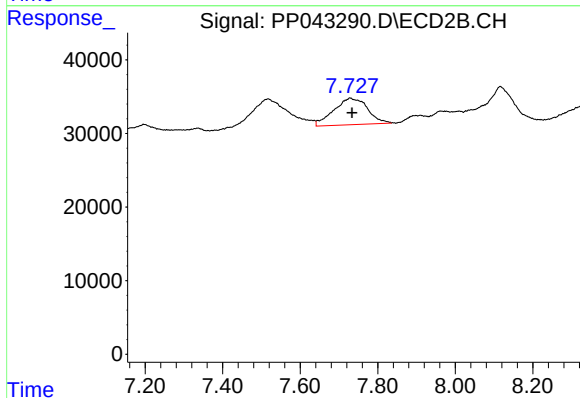


#34 AR-1260-4

R.T.: 7.728 min
Delta R.T.: -0.006 min
Response: 217777
Conc: 222.01 ng/ml

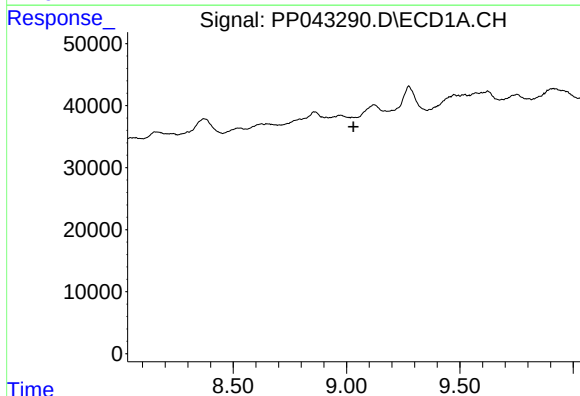


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 9.031 min
Response: 0
Conc: N.D.

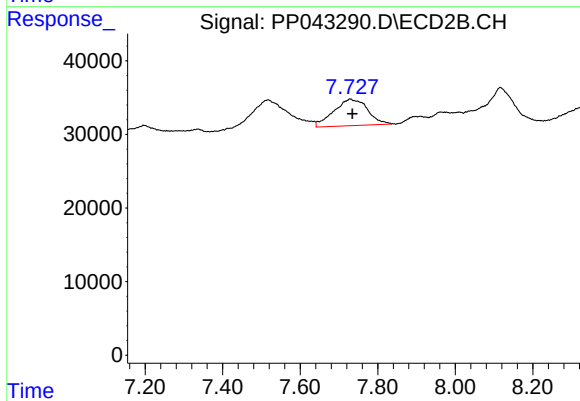

#37 AR-1262-2


R.T.: 7.728 min
Delta R.T.: -0.007 min
Response: 217777
Conc: 157.14 ng/ml

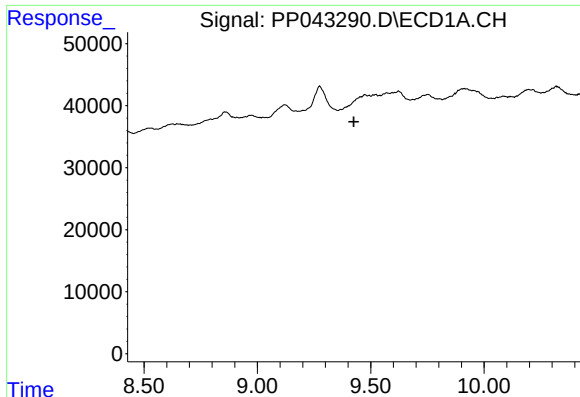

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 9.426 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

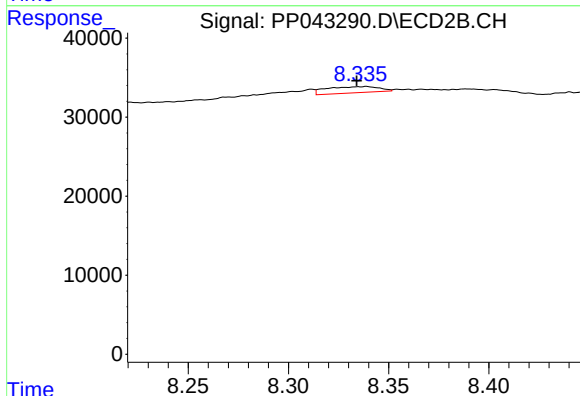


#39 AR-1262-4

R.T.: 8.339 min
Delta R.T.: 0.005 min
Response: 14426
Conc: 7.67 ng/ml

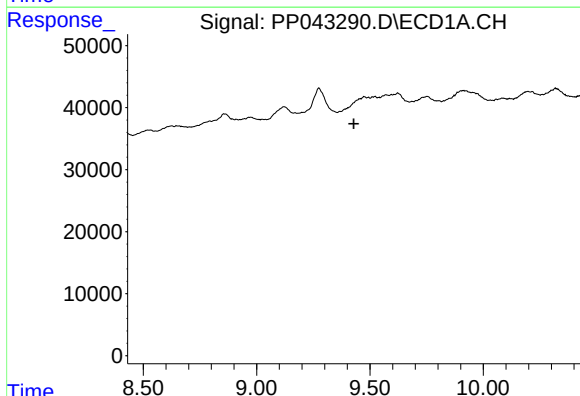


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 9.428 min
Response: 0
Conc: N.D.

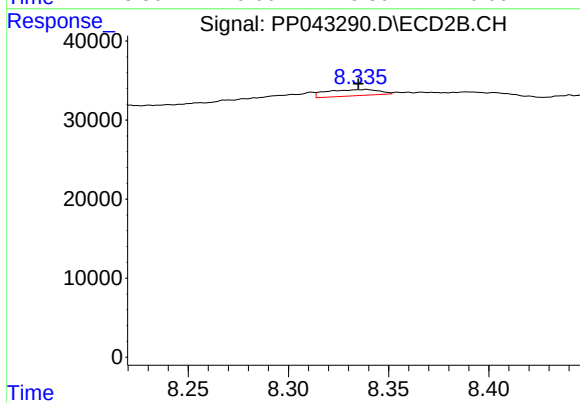

#42 AR-1268-2


R.T.: 8.339 min
Delta R.T.: 0.004 min
Response: 14426
Conc: 5.40 ng/ml

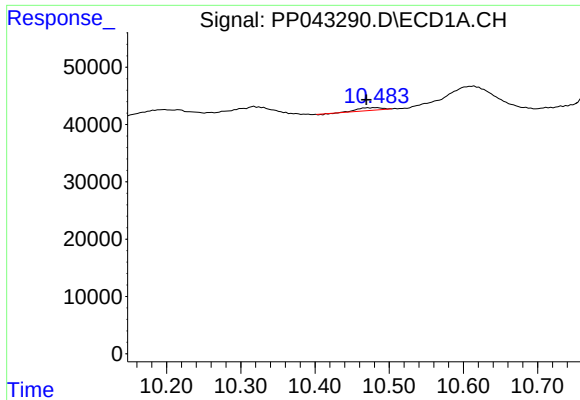

#45 AR-1268-5

R.T.: 10.471 min
Delta R.T.: 0.002 min
Response: 9320
Conc: 1.84 ng/ml

Instrument :
ECD_P
ClientSampleId :

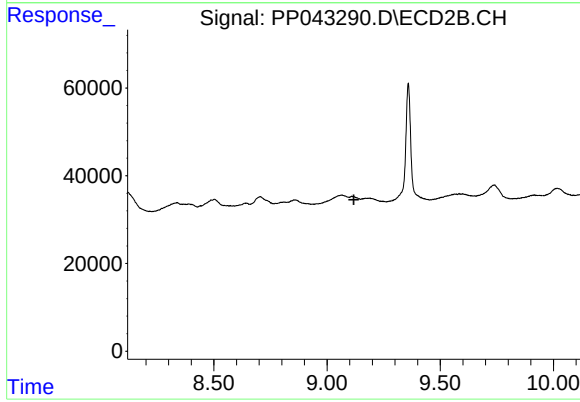

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.119 min
Response: 0
Conc: N.D.