

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012622\
 Data File : PP043304.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jan 2022 17:21
 Operator : AJ\MA
 Sample : N1276-03 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-SF-012522-03

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/28/2022
 Supervised By :Ankita Jodhani 01/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:45:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 25 03:09:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.865	4.032	31846	40288	1.385m	1.808 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012622\
Data File : PP043304.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jan 2022 17:21
Operator : AJ\MA
Sample : N1276-03 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PCB-SF-012522-03


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/28/2022
Supervised By :Ankita Jodhani 01/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:45:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

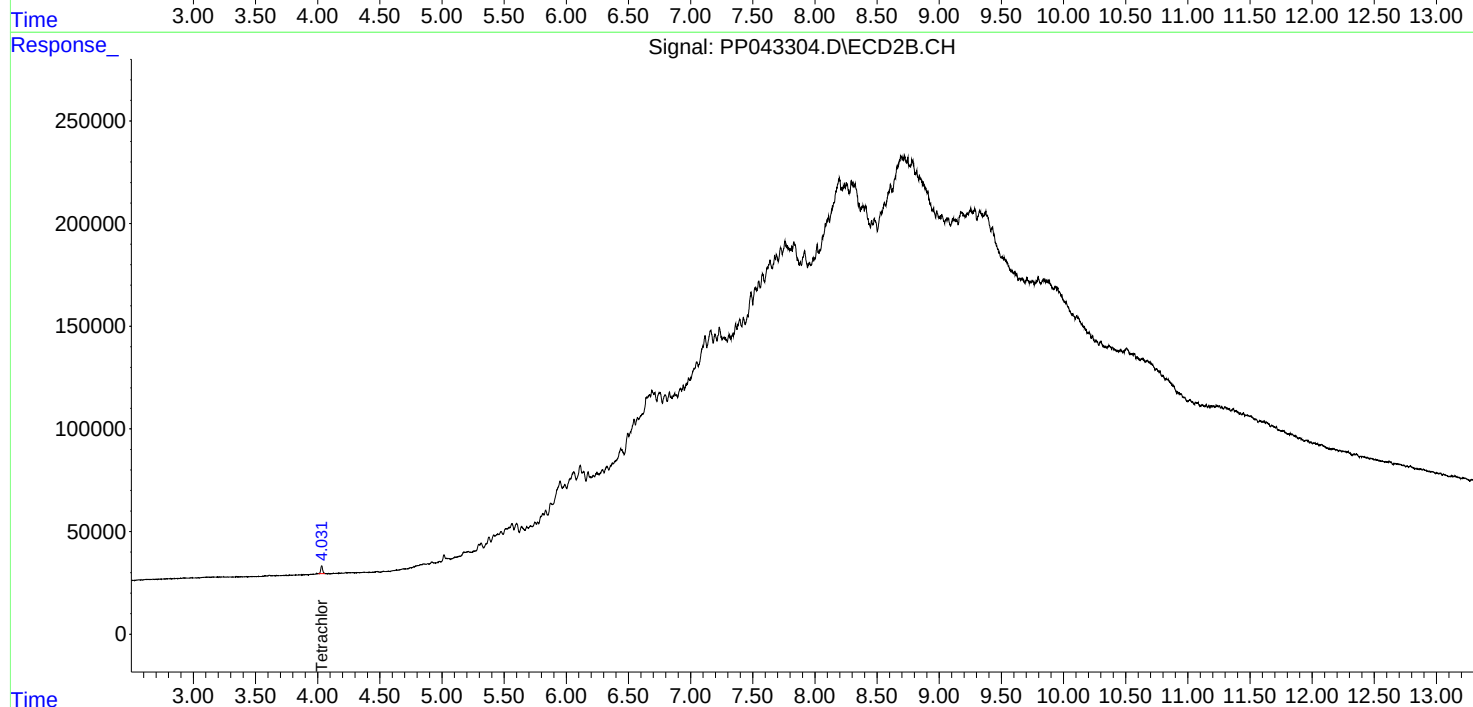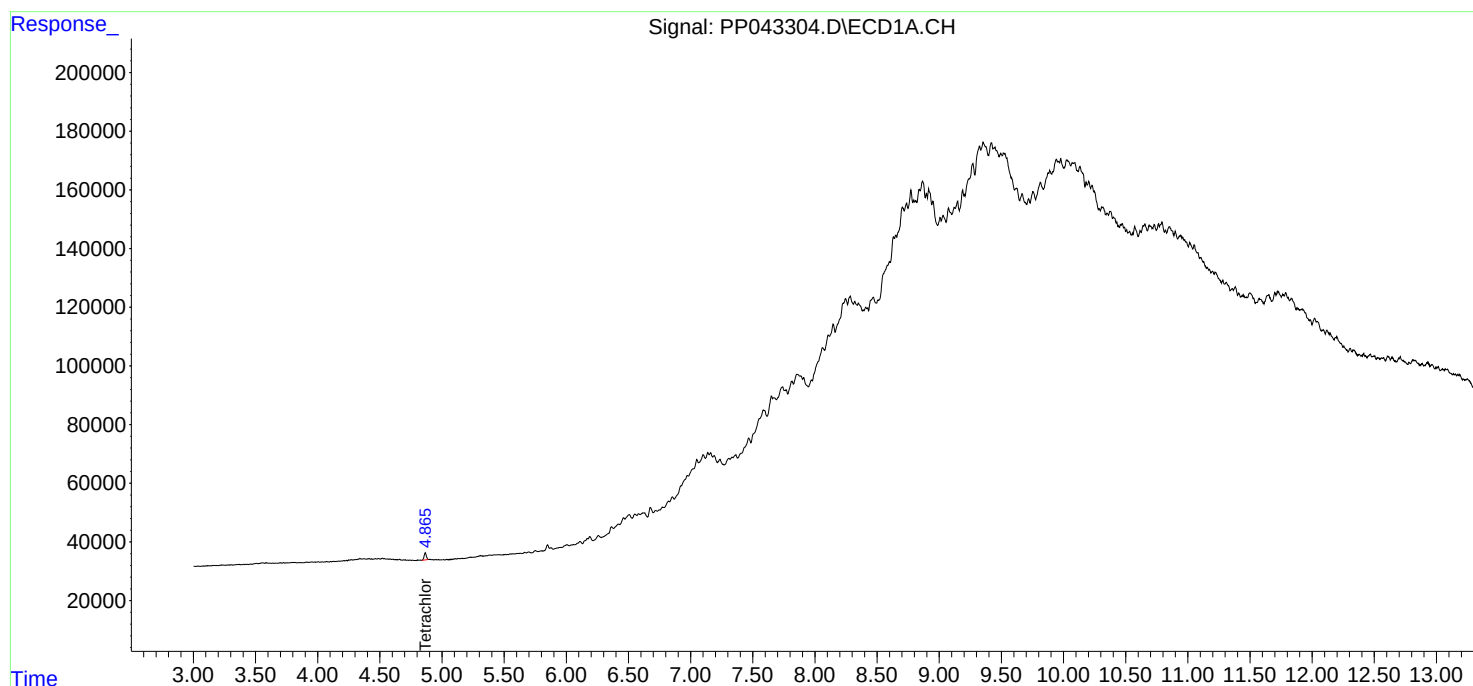

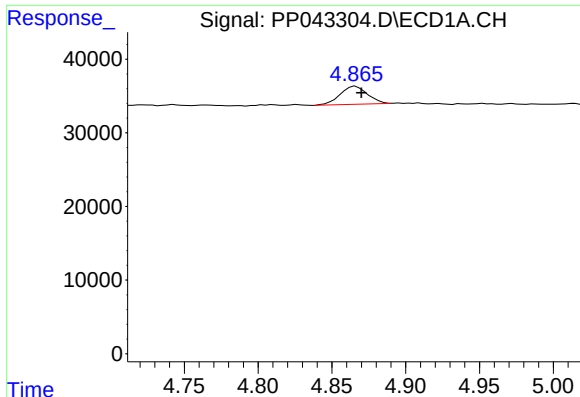


#1 Tetrachloro-m-xylene

R.T.: 4.865 min
Delta R.T.: -0.005 min
Response: 31846
Conc: 1.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-012522-03


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/28/2022
Supervised By :Ankita Jodhani 01/28/2022

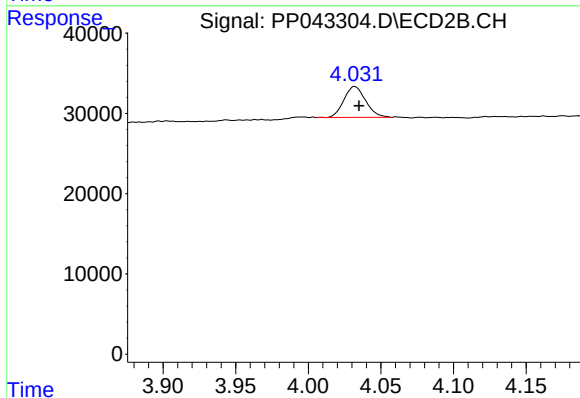


#1 Tetrachloro-m-xylene

R.T.: 4.032 min
Delta R.T.: -0.003 min
Response: 40288
Conc: 1.81 ng/ml

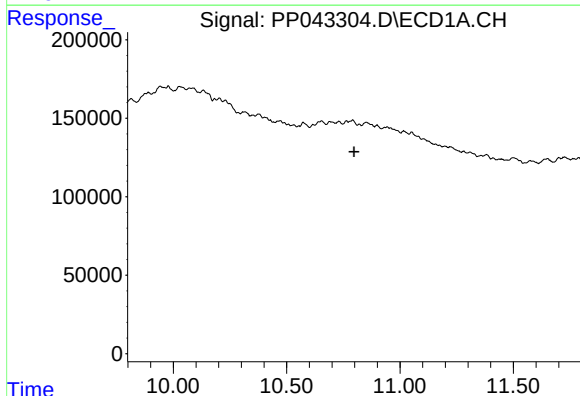

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.797 min
Response: 0
Conc: N.D.

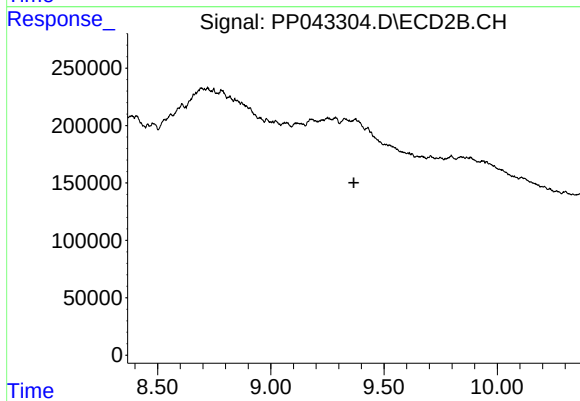

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.366 min
Response: 0
Conc: N.D.