

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012721\
 Data File : PP032991.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jan 2021 15:48
 Operator : DD\AJ
 Sample : M1236-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 J2288R-WO(N)-1-13-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 18:21:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.736	4.008	1405845	1037122	24.205	22.048
2) SA Decachlor...	10.566	9.284	970766	887400	24.605	23.688

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012721\
Data File : PP032991.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jan 2021 15:48
Operator : DD\AJ
Sample : M1236-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
J2288R-WO(N)-1-13-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 18:21:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

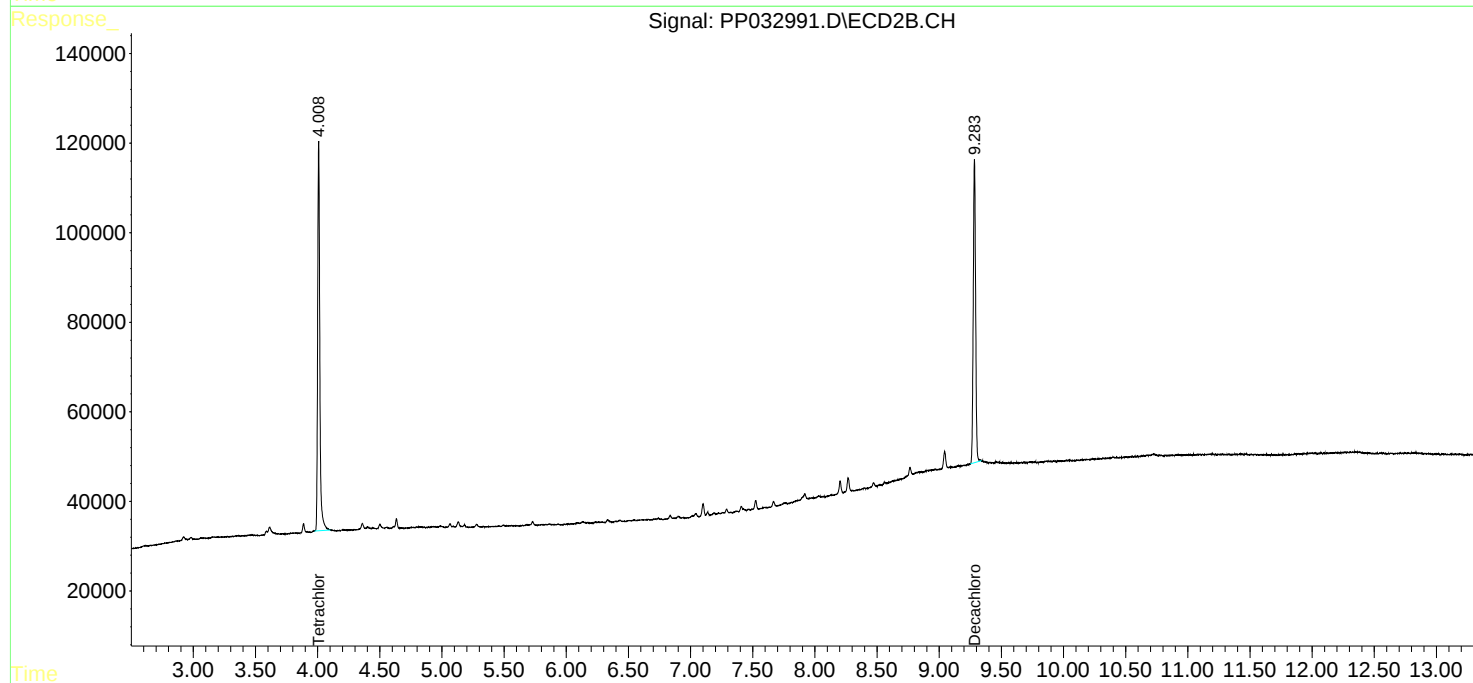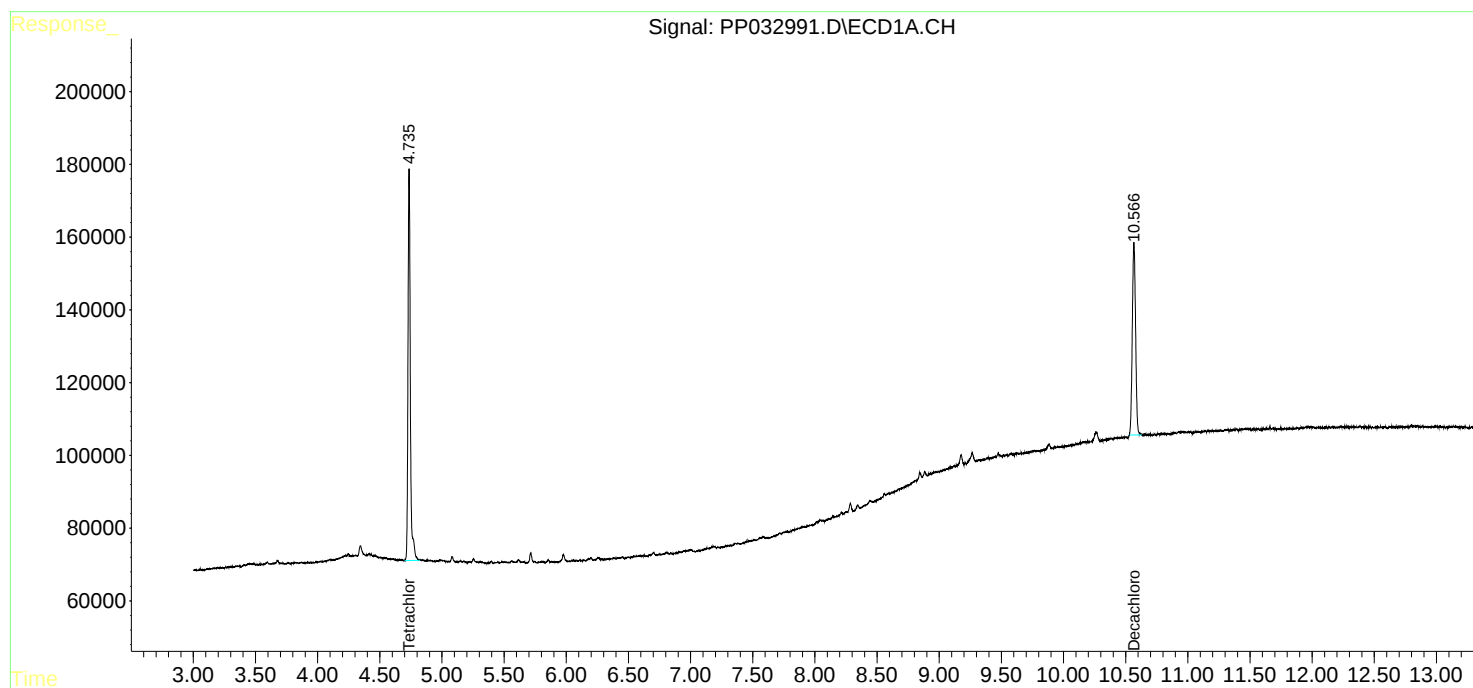


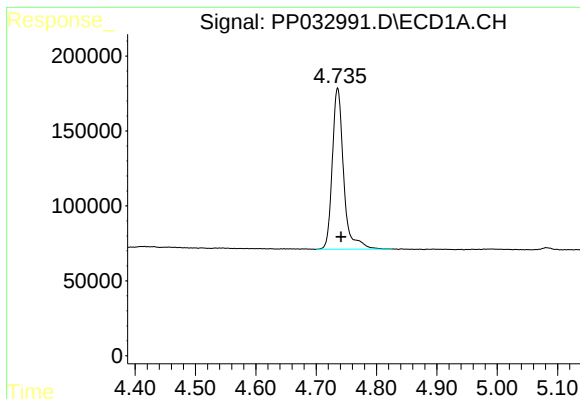

#1 Tetrachloro-m-xylene


R.T.: 4.736 min
Delta R.T.: -0.005 min
Response: 1405845
Conc: 24.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
J2288R-WO(N)-1-13-1

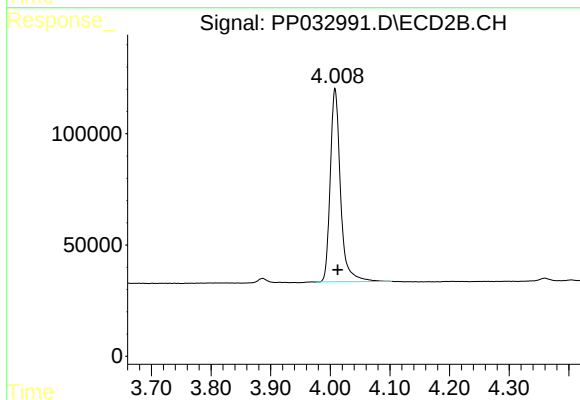


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.005 min
Response: 1037122
Conc: 22.05 ng/ml

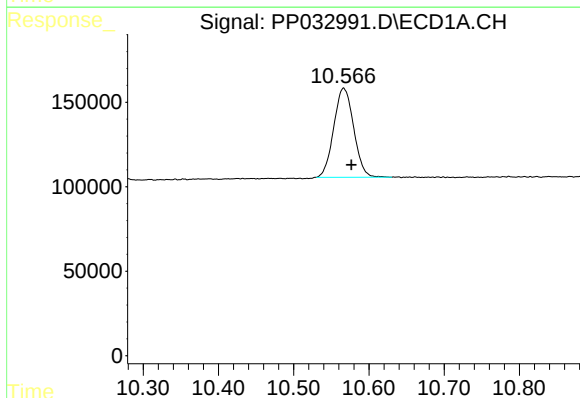

#2 Decachlorobiphenyl

R.T.: 10.566 min
Delta R.T.: -0.010 min
Response: 970766
Conc: 24.61 ng/ml

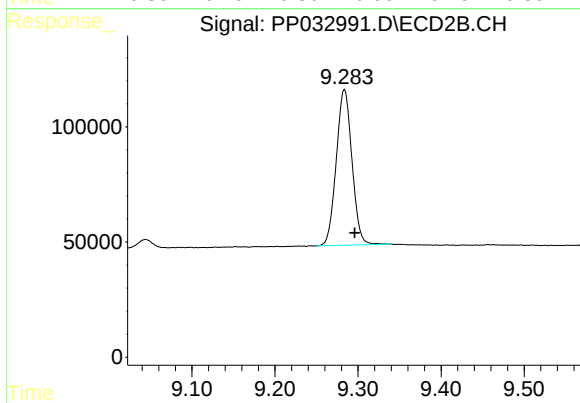

#2 Decachlorobiphenyl

R.T.: 9.284 min
Delta R.T.: -0.012 min
Response: 887400
Conc: 23.69 ng/ml