

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012821\
 Data File : PP033055.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jan 2021 9:40
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 14:29:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 04:07:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.732	4.004	1090664	908792	19.208	19.769
2)	SA Decachlor...	10.561	9.277	810363	730652	22.587	22.236
Target Compounds							
24)	L5 AR-1248-4	6.952	0.000	7915	0	5.031	N.D. #
26)	L6 AR-1254-1	6.952	0.000	7915	0	4.698	N.D. #
32)	L7 AR-1260-2	7.973	0.000	108162	0	44.183	N.D. #
34)	L7 AR-1260-4	8.570	0.000	27477	0	13.458	N.D. #
35)	L7 AR-1260-5	8.884	0.000	36574	0	8.236	N.D. #
37)	L8 AR-1262-2	8.884	0.000	36574	0	7.672	N.D. #
39)	L8 AR-1262-4	9.271	0.000	27779	0	9.999	N.D. #
42)	L9 AR-1268-2	9.271	0.000	27779	0	4.967	N.D. #
43)	L9 AR-1268-3	9.471	0.000	33989	0	6.566	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012821\
Data File : PP033055.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jan 2021 9:40
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 14:29:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 04:07:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

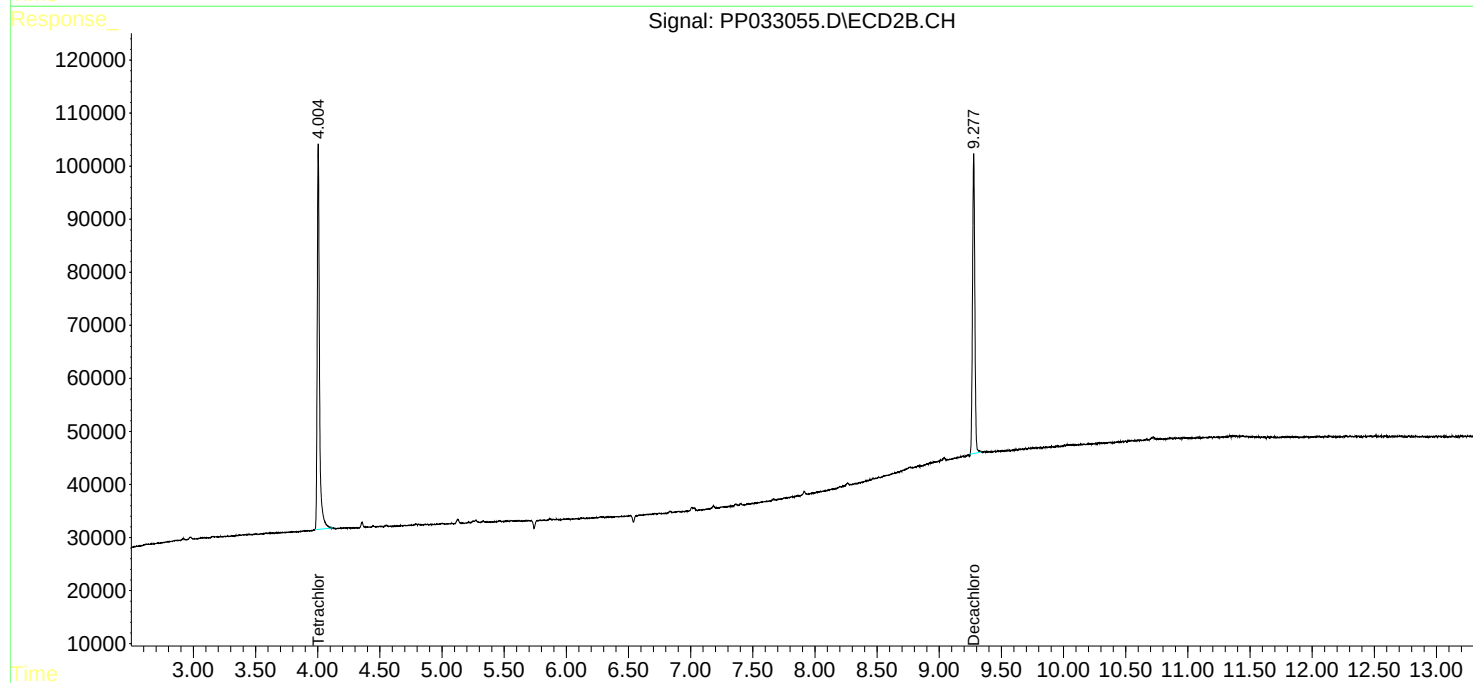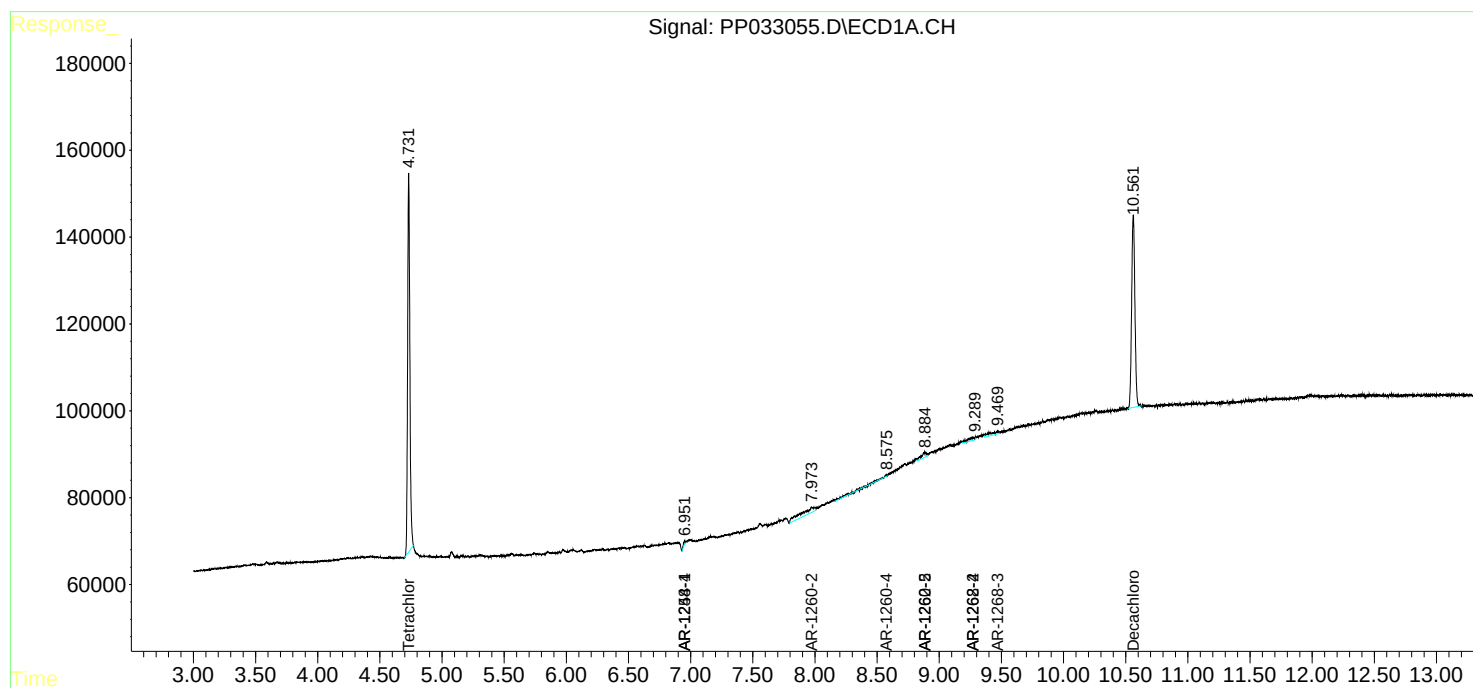


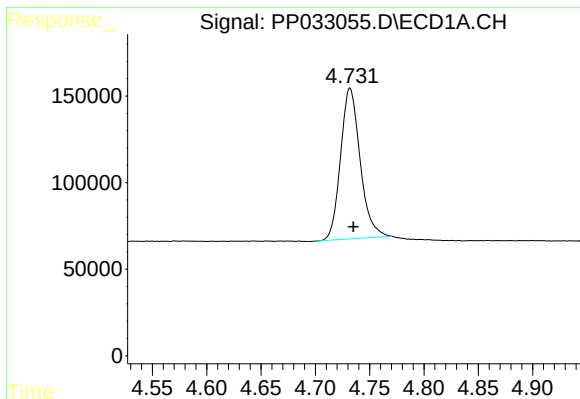

#1 Tetrachloro-m-xylene


R.T.: 4.732 min
Delta R.T.: -0.003 min
Response: 1090664
Conc: 19.21 ng/ml

Instrument :
ECD_P
ClientSampleId :

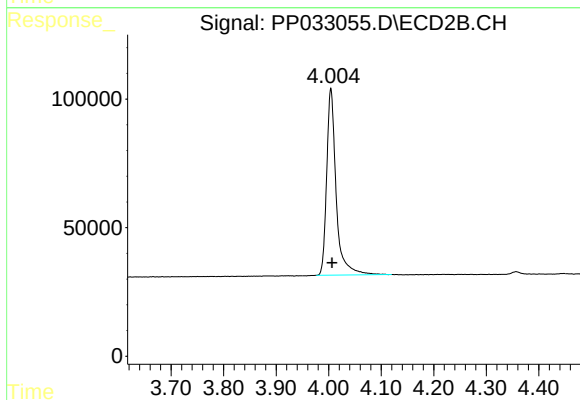


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: -0.002 min
Response: 908792
Conc: 19.77 ng/ml

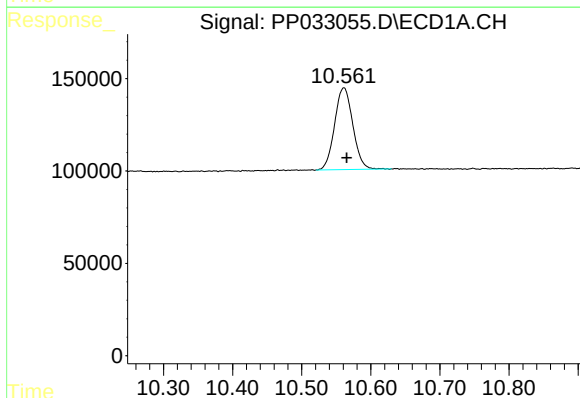


#2 Decachlorobiphenyl

R.T.: 10.561 min
Delta R.T.: -0.004 min
Response: 810363
Conc: 22.59 ng/ml

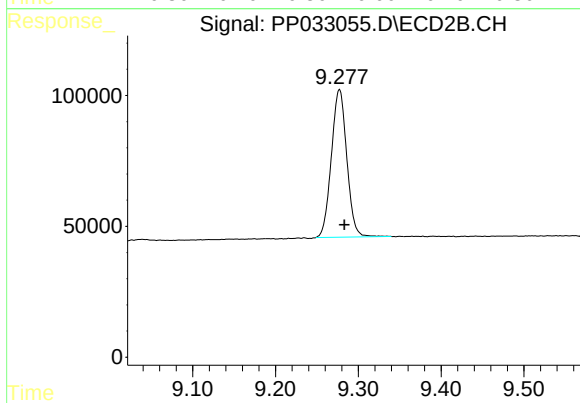

#2 Decachlorobiphenyl


R.T.: 9.277 min
Delta R.T.: -0.006 min
Response: 730652
Conc: 22.24 ng/ml

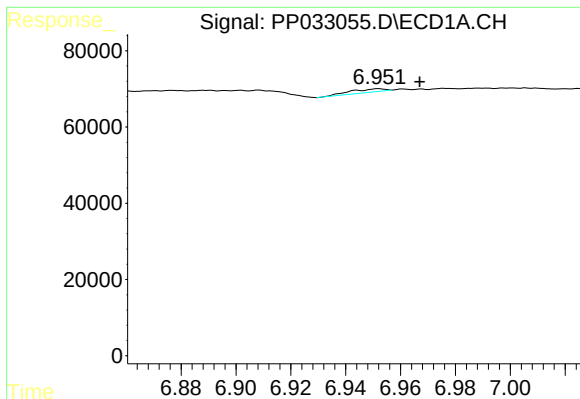

#24 AR-1248-4


R.T.: 6.952 min
Delta R.T.: -0.015 min
Response: 7915
Conc: 5.03 ng/ml

Instrument :
ECD_P
ClientSampleId :

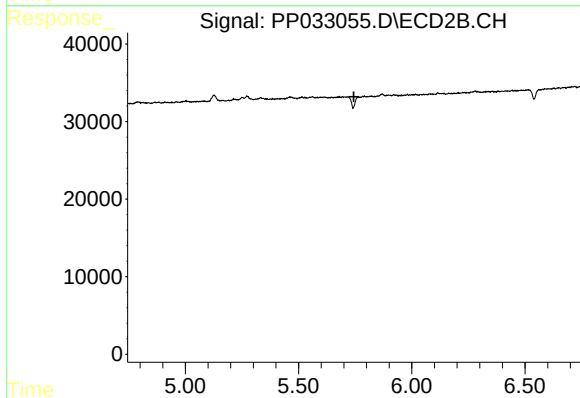


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.744 min
Response: 0
Conc: N.D.

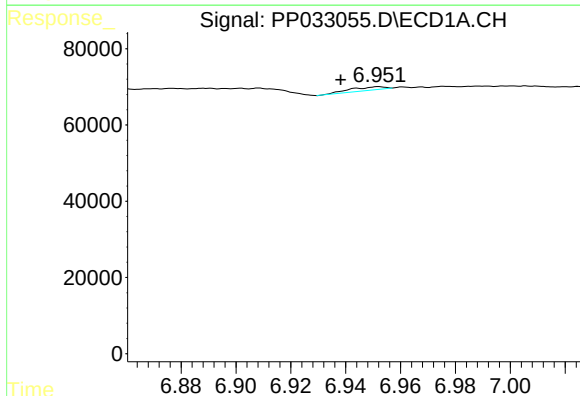


#26 AR-1254-1

R.T.: 6.952 min
Delta R.T.: 0.014 min
Response: 7915
Conc: 4.70 ng/ml

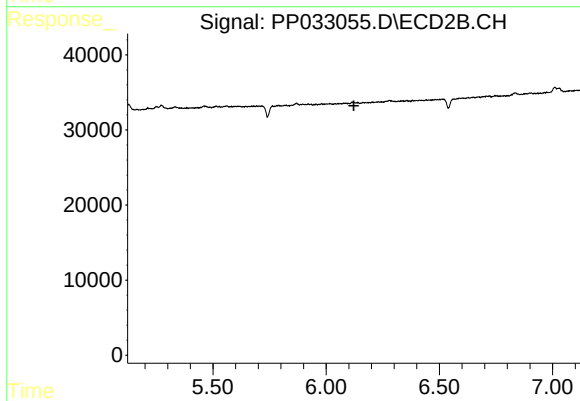

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.123 min
Response: 0
Conc: N.D.

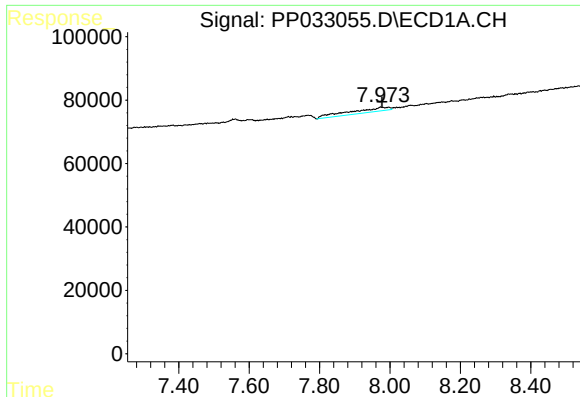

#32 AR-1260-2


R.T.: 7.973 min
Delta R.T.: -0.004 min
Response: 108162
Conc: 44.18 ng/ml

Instrument :
ECD_P
ClientSampleId :

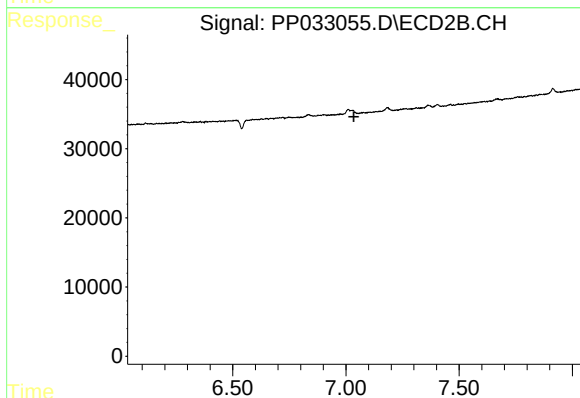


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.035 min
Response: 0
Conc: N.D.

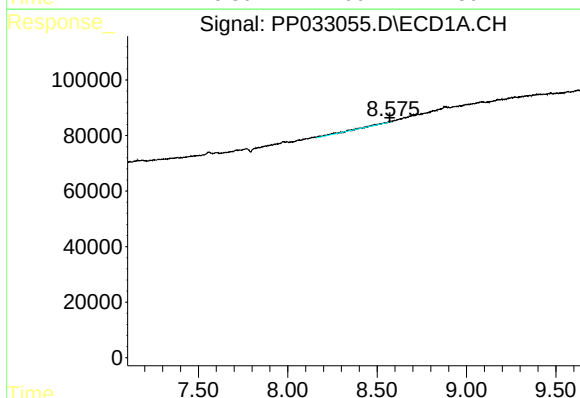


#34 AR-1260-4

R.T.: 8.570 min
Delta R.T.: -0.001 min
Response: 27477
Conc: 13.46 ng/ml

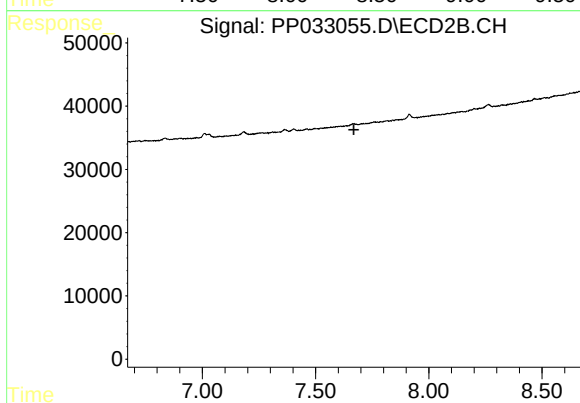

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.669 min
Response: 0
Conc: N.D.

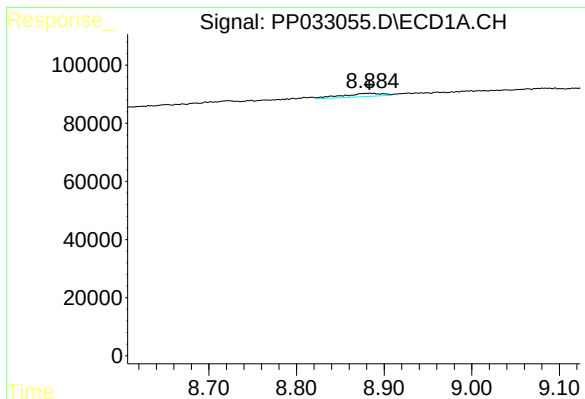

#35 AR-1260-5


R.T.: 8.884 min
Delta R.T.: 0.000 min
Response: 36574
Conc: 8.24 ng/ml

Instrument :
ECD_P
ClientSampleId :

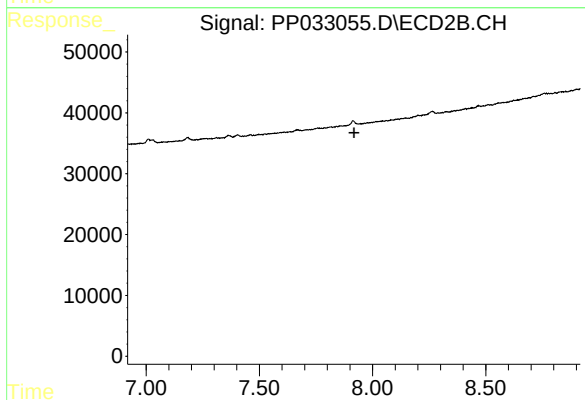


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.918 min
Response: 0
Conc: N.D.

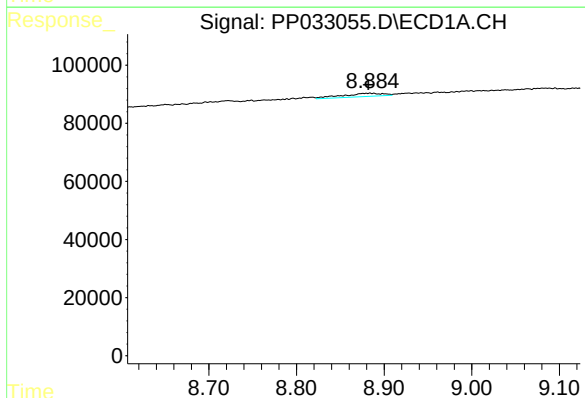


#37 AR-1262-2

R.T.: 8.884 min
Delta R.T.: 0.002 min
Response: 36574
Conc: 7.67 ng/ml

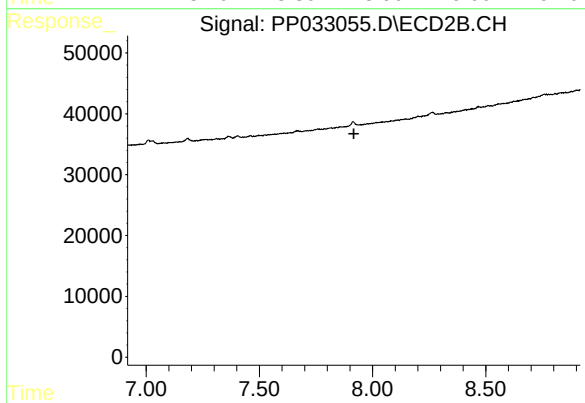

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.917 min
Response: 0
Conc: N.D.

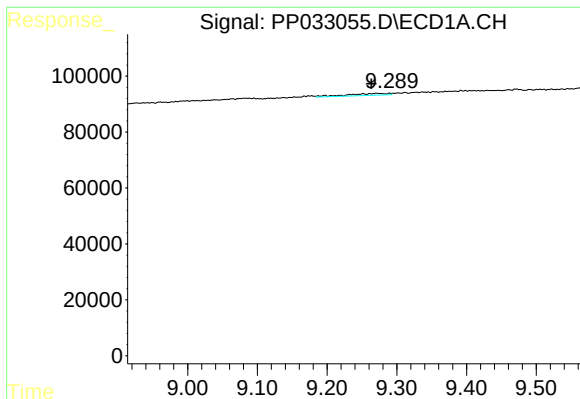

#39 AR-1262-4


R.T.: 9.271 min
Delta R.T.: 0.008 min
Response: 27779
Conc: 10.00 ng/ml

Instrument :
ECD_P
ClientSampleId :

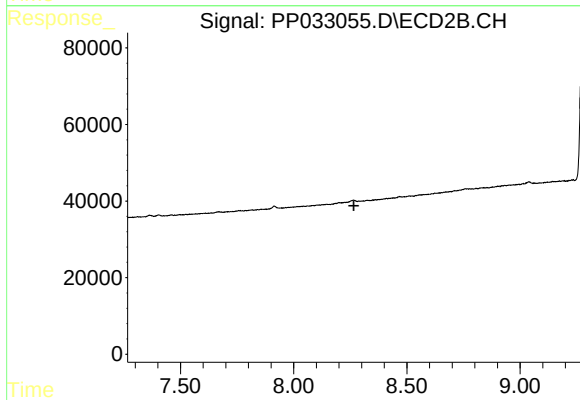


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.266 min
Response: 0
Conc: N.D.

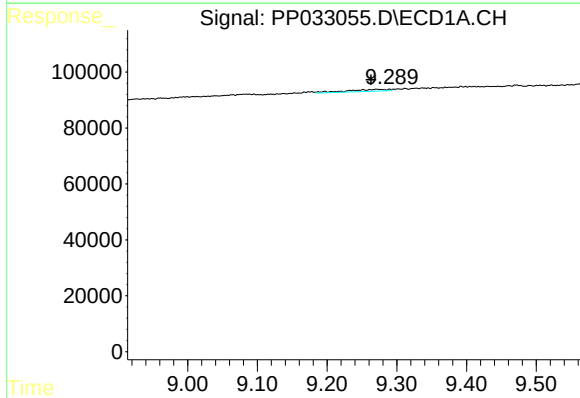


#42 AR-1268-2

R.T.: 9.271 min
Delta R.T.: 0.008 min
Response: 27779
Conc: 4.97 ng/ml

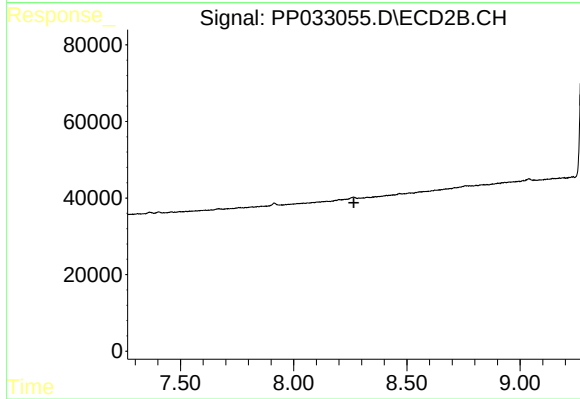

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.266 min
Response: 0
Conc: N.D.

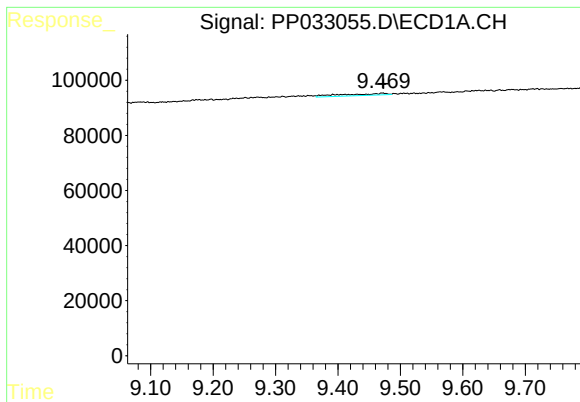

#43 AR-1268-3

R.T.: 9.471 min
Delta R.T.: -0.001 min
Response: 33989
Conc: 6.57 ng/ml

Instrument :
ECD_P
ClientSampleId :

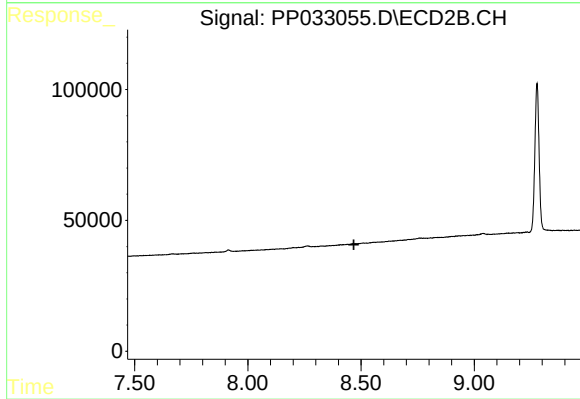

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.468 min
Response: 0
Conc: N.D.