

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012821\
 Data File : PP033042.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jan 2021 23:00
 Operator : DD\AJ
 Sample : PB134369BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB134369BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 04:18:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 04:07:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.734	4.005	1179750	909911	20.777	19.793
2)	SA Decachlor...	10.563	9.279	712068	651511	19.847	19.827

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012821\
Data File : PP033042.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jan 2021 23:00
Operator : DD\AJ
Sample : PB134369BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB134369BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 04:18:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 04:07:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

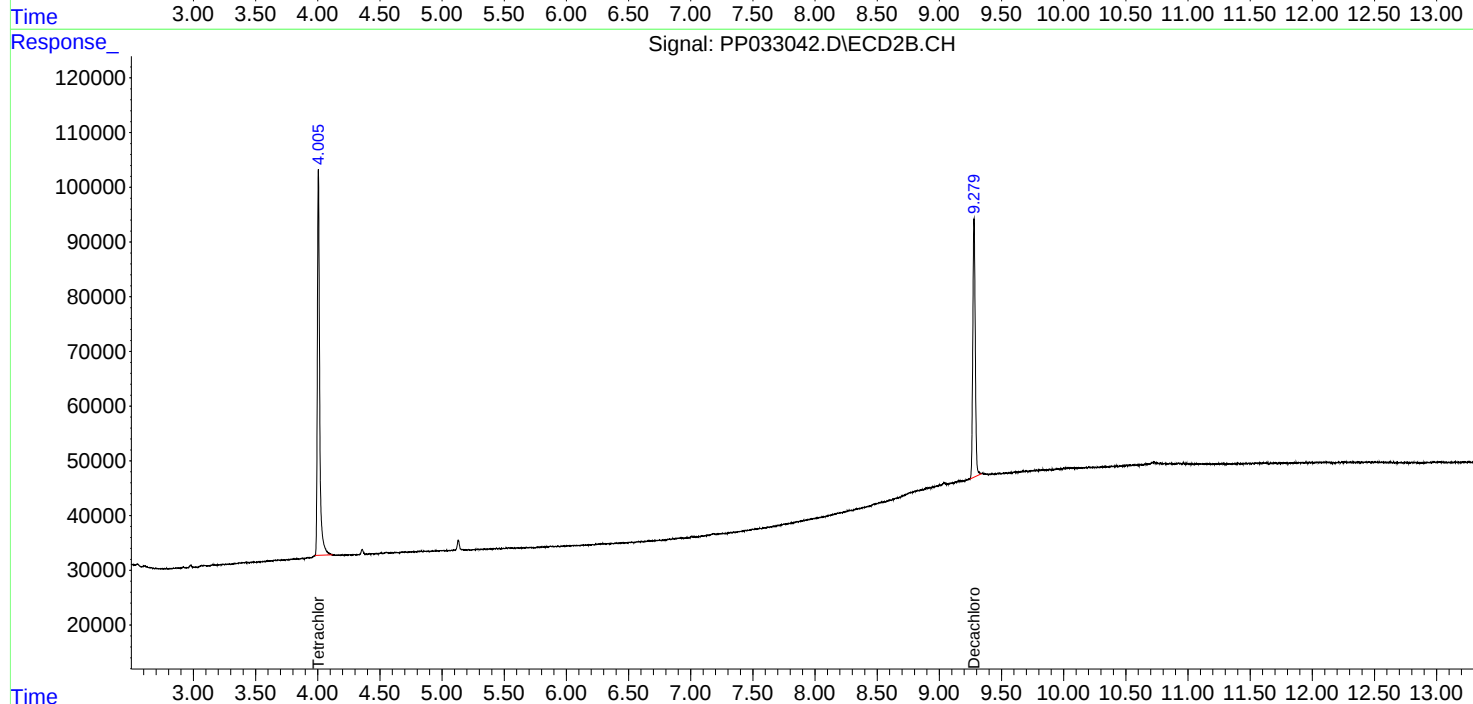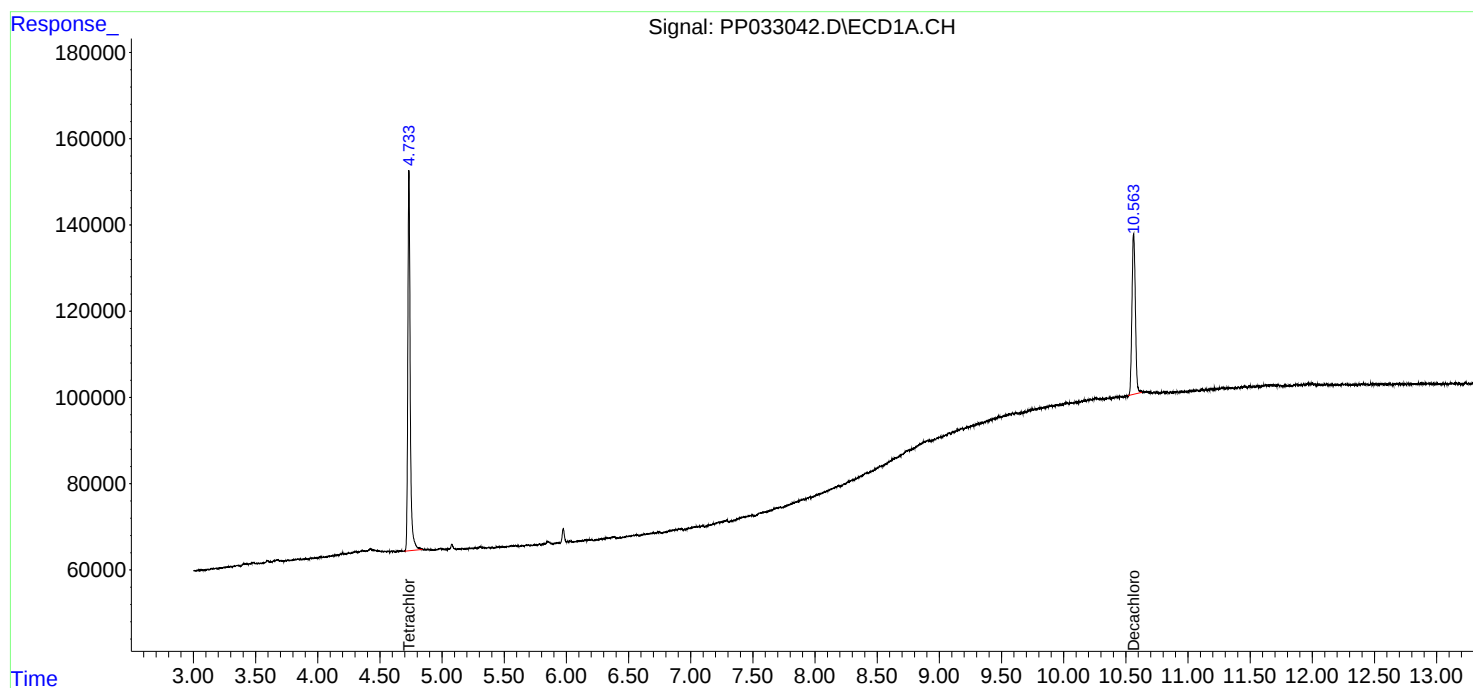


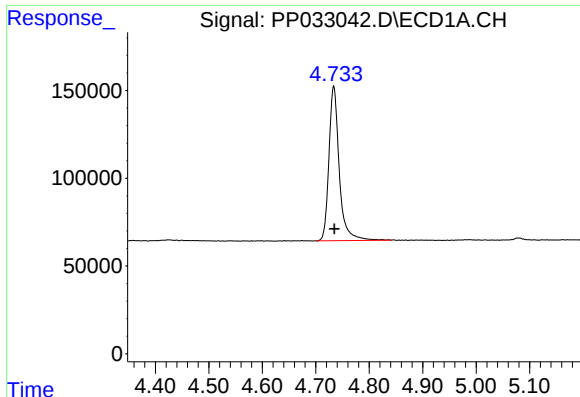

#1 Tetrachloro-m-xylene


R.T.: 4.734 min
Delta R.T.: -0.001 min
Response: 1179750
Conc: 20.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB134369BL

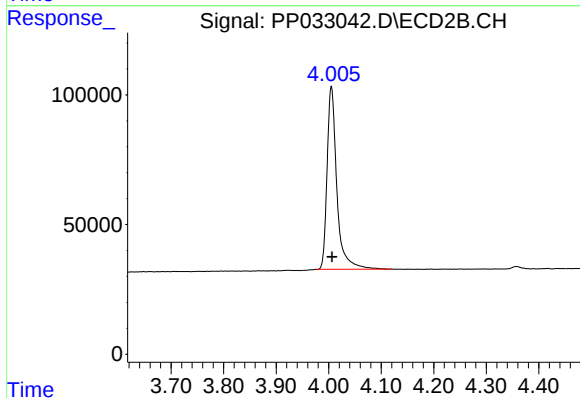


#1 Tetrachloro-m-xylene

R.T.: 4.005 min
Delta R.T.: -0.001 min
Response: 909911
Conc: 19.79 ng/ml

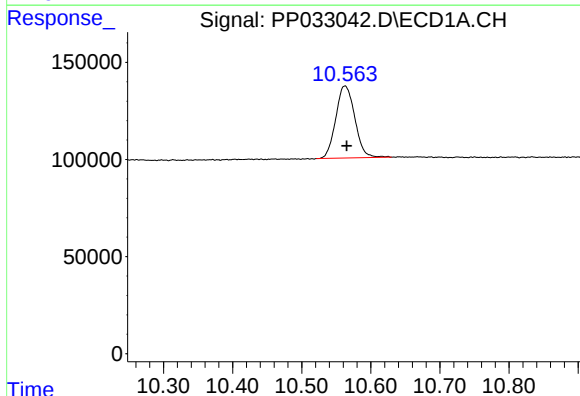

#2 Decachlorobiphenyl

R.T.: 10.563 min
Delta R.T.: -0.003 min
Response: 712068
Conc: 19.85 ng/ml

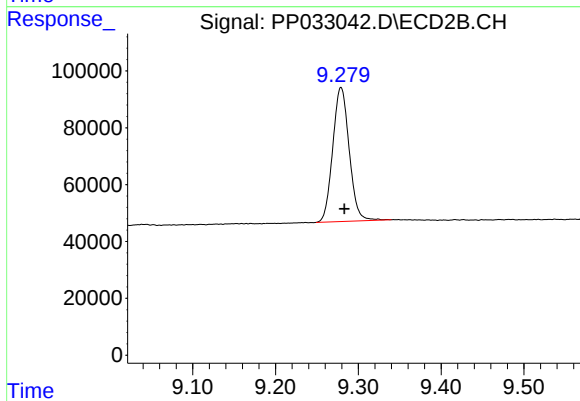

#2 Decachlorobiphenyl

R.T.: 9.279 min
Delta R.T.: -0.004 min
Response: 651511
Conc: 19.83 ng/ml