

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012821\
 Data File : PP033044.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jan 2021 23:33
 Operator : DD\AJ
 Sample : M1260-13
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WOOSPK-054-0002

Manual Integrations
 APPROVED

Ankita
 1/29/2021 1:21:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 04:19:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 04:07:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.733	4.006	1232601	1058115	21.707m	23.017
2) SA Decachlor...	10.562	9.279	964897	805481	26.894	24.513

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012821\
Data File : PP033044.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jan 2021 23:33
Operator : DD\AJ
Sample : M1260-13
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WOOSPK-054-0002


Manual Integrations
APPROVED

Ankita
1/29/2021 1:21:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 04:19:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 04:07:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

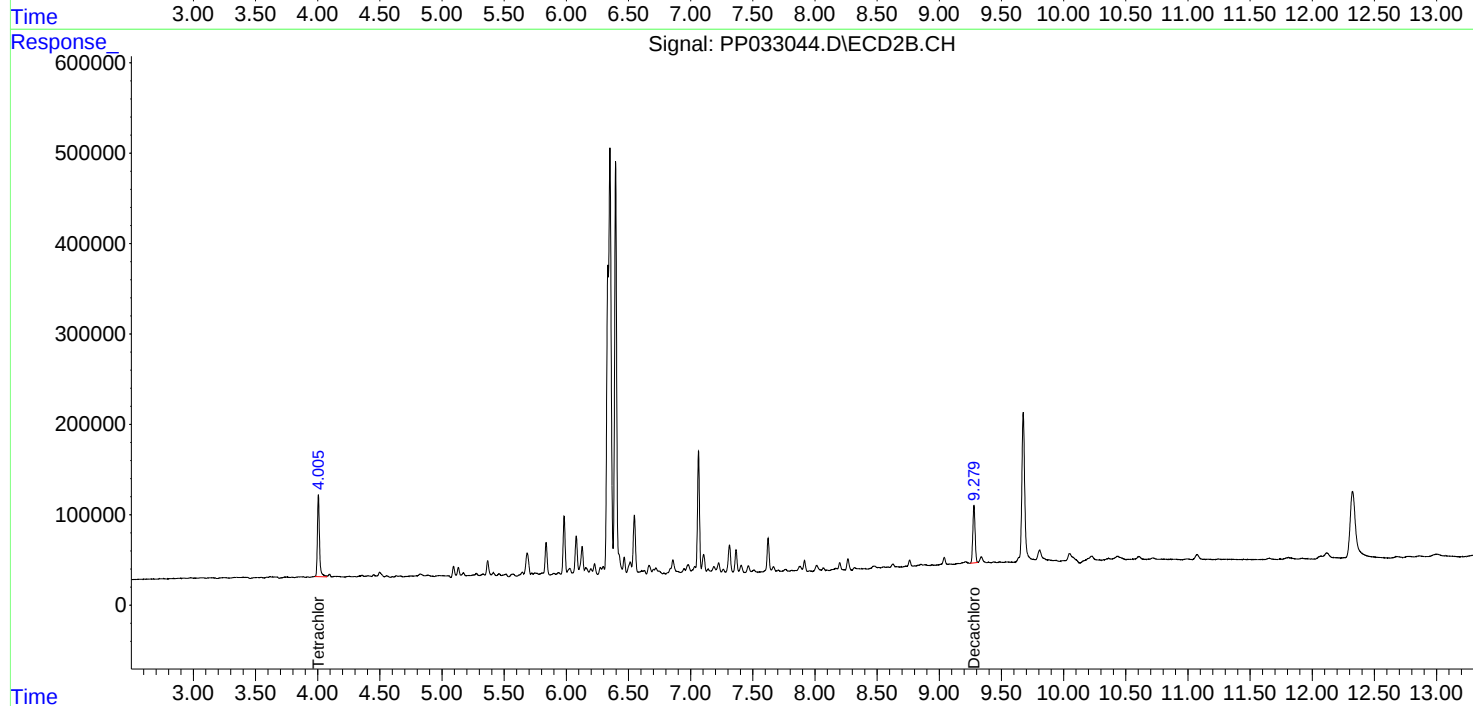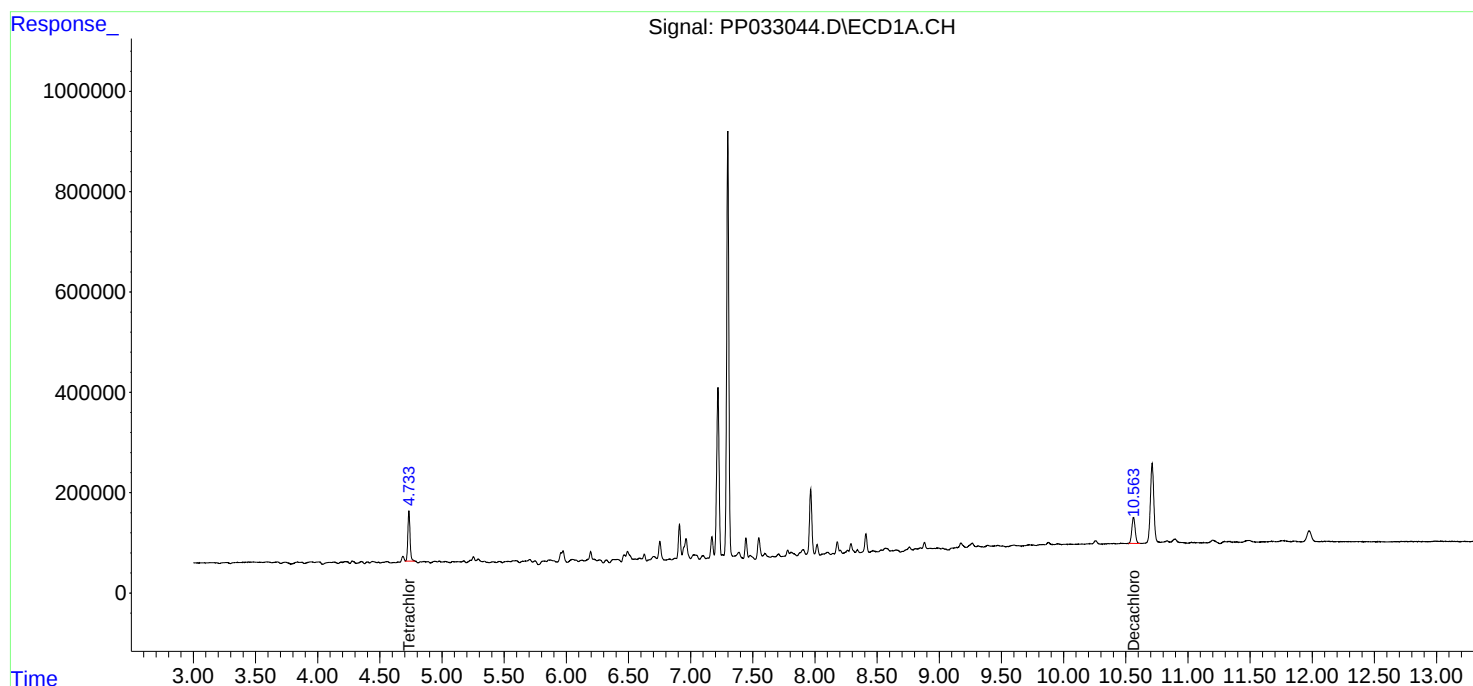

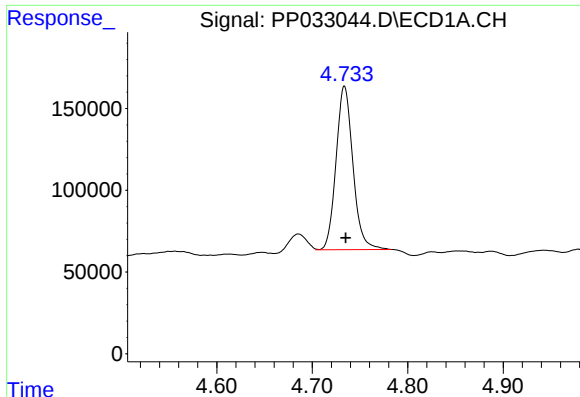


#1 Tetrachloro-m-xylene

R.T.: 4.733 min
Delta R.T.: -0.002 min
Response: 1232601
Conc: 21.71 ng/ml m

Instrument :
ECD_P
ClientSampleId :
WOOSPK-054-0002


Manual Integrations
APPROVED

Ankita
1/29/2021 1:21:21 PM

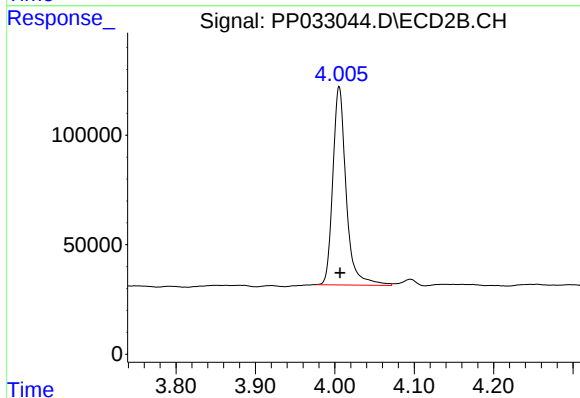


#1 Tetrachloro-m-xylene

R.T.: 4.006 min
Delta R.T.: 0.000 min
Response: 1058115
Conc: 23.02 ng/ml

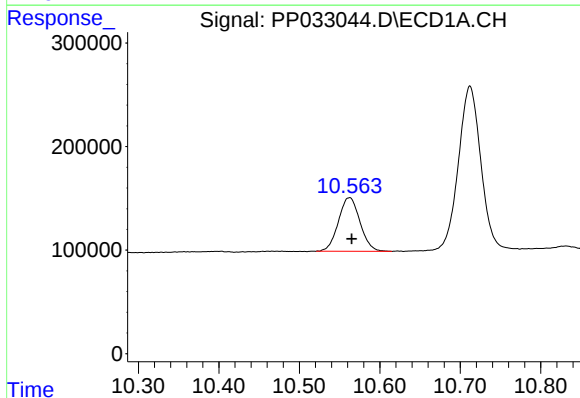

#2 Decachlorobiphenyl

R.T.: 10.562 min
Delta R.T.: -0.003 min
Response: 964897
Conc: 26.89 ng/ml

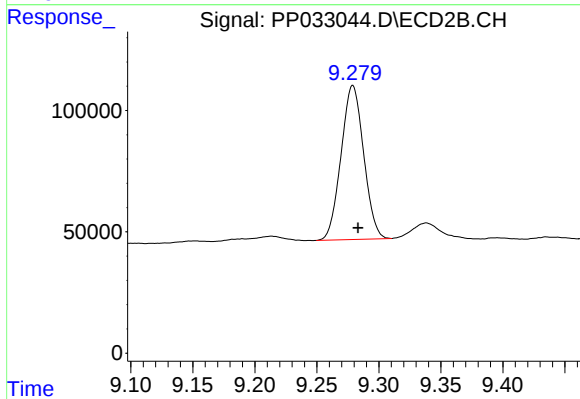

#2 Decachlorobiphenyl

R.T.: 9.279 min
Delta R.T.: -0.004 min
Response: 805481
Conc: 24.51 ng/ml