

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012822\
 Data File : PP043333.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jan 2022 17:42
 Operator : AJ\MA
 Sample : N1319-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 23:38:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 25 03:09:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.865	4.031	553059	522049	24.061	23.429
2)	SA Decachlor...	10.785	9.357	358964	411050	25.344	22.049
Target Compounds							
8)	L2 AR-1221-1	5.101	0.000	27756	0	111.144	N.D. #
9)	L2 AR-1221-2	0.000	4.366f	0	42615	N.D.	177.209 #
30)	L6 AR-1254-5	8.402	0.000	19818	0	24.536	N.D. #
31)	L7 AR-1260-1	0.000	6.889	0	12332	N.D.	10.541 #
32)	L7 AR-1260-2	8.105	0.000	12116	0	14.231	N.D. #
33)	L7 AR-1260-3	8.488	0.000	5196	0	7.878	N.D. #
35)	L7 AR-1260-5	0.000	7.976	0	11048	N.D.	4.993 #
36)	L8 AR-1262-1	8.488	0.000	5196	0	5.230	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012822\
Data File : PP043333.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jan 2022 17:42
Operator : AJ\MA
Sample : N1319-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 23:38:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

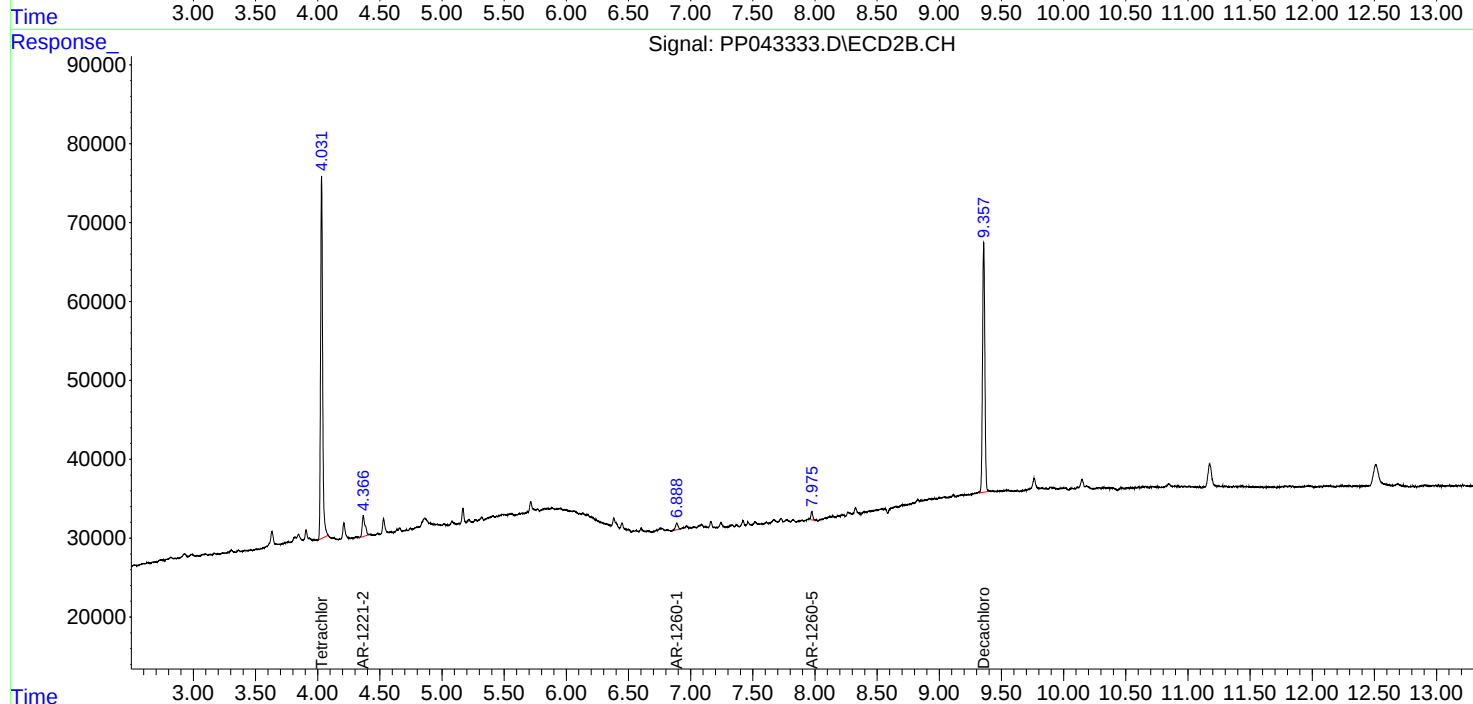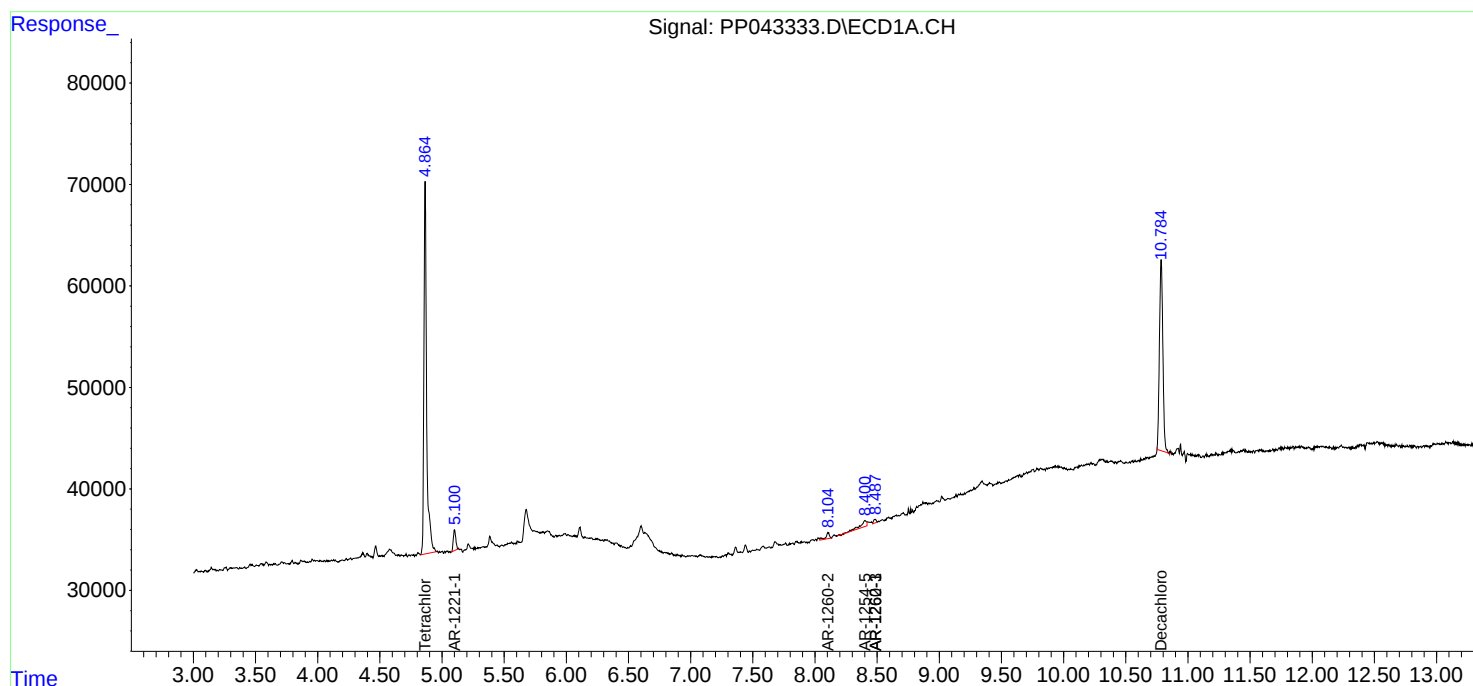


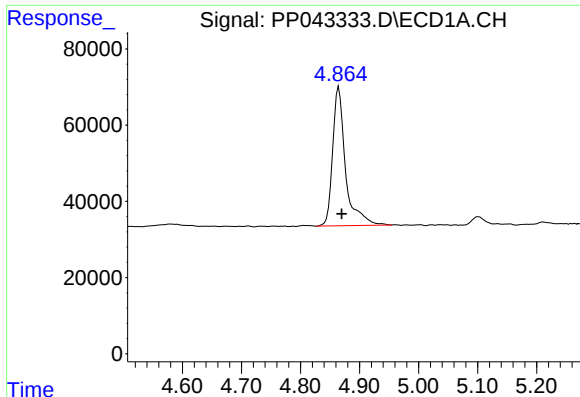

#1 Tetrachloro-m-xylene


R.T.: 4.865 min
Delta R.T.: -0.005 min
Response: 553059
Conc: 24.06 ng/ml

Instrument :
ECD_P
ClientSampleId :

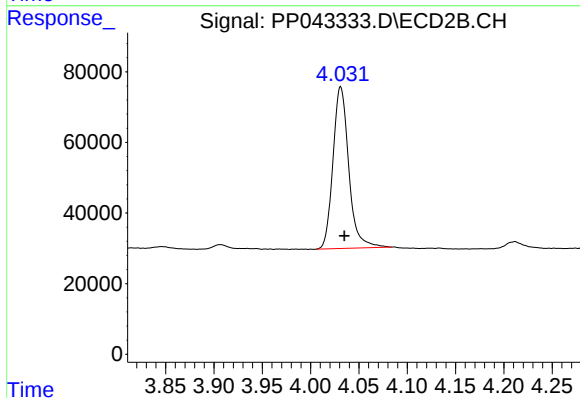


#1 Tetrachloro-m-xylene

R.T.: 4.031 min
Delta R.T.: -0.004 min
Response: 522049
Conc: 23.43 ng/ml

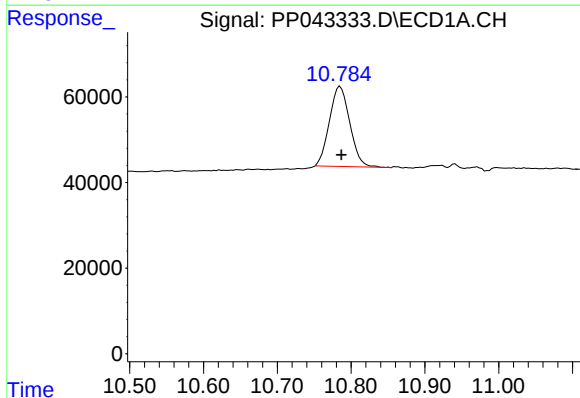


#2 Decachlorobiphenyl

R.T.: 10.785 min
Delta R.T.: -0.002 min
Response: 358964
Conc: 25.34 ng/ml

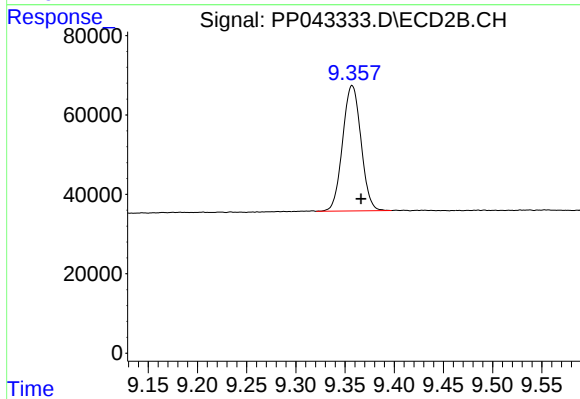

#2 Decachlorobiphenyl


R.T.: 9.357 min
Delta R.T.: -0.009 min
Response: 411050
Conc: 22.05 ng/ml

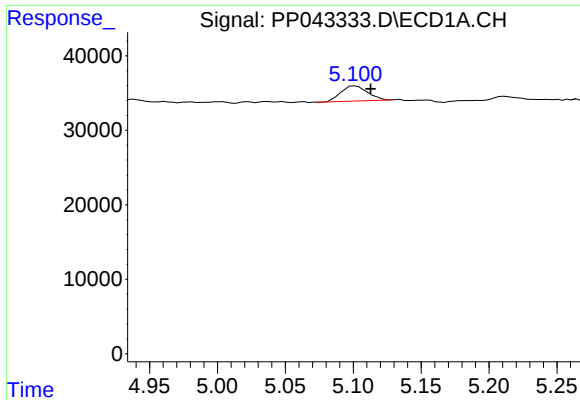

#8 AR-1221-1


R.T.: 5.101 min
Delta R.T.: -0.012 min
Response: 27756
Conc: 111.14 ng/ml

Instrument :
ECD_P
ClientSampleId :

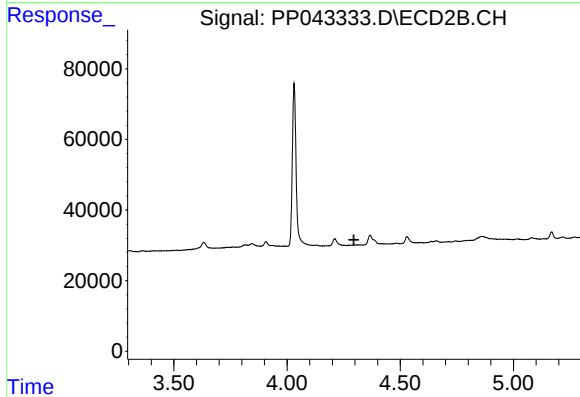


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.295 min
Response: 0
Conc: N.D.

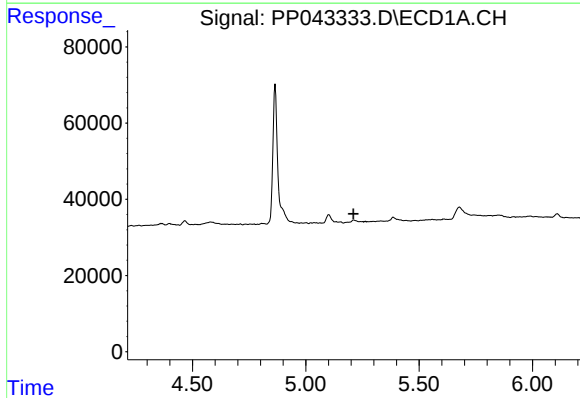


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.211 min
Response: 0
Conc: N.D.

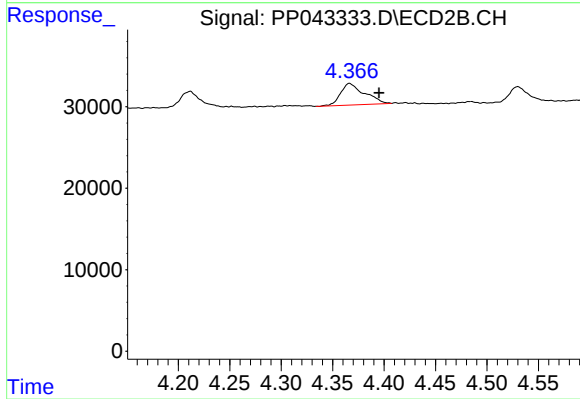

#9 AR-1221-2


R.T.: 4.366 min
Delta R.T.: -0.029 min
Response: 42615
Conc: 177.21 ng/ml

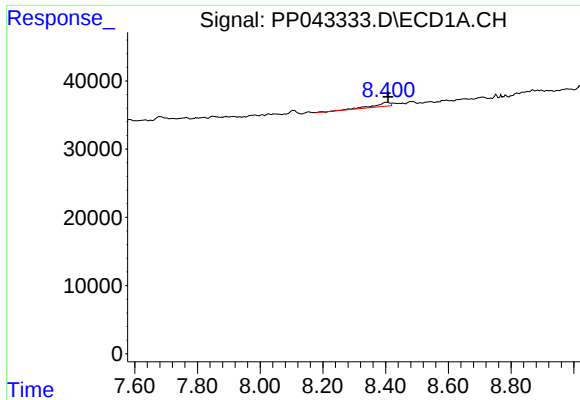

#30 AR-1254-5


R.T.: 8.402 min
Delta R.T.: -0.006 min
Response: 19818
Conc: 24.54 ng/ml

Instrument :
ECD_P
ClientSampleId :

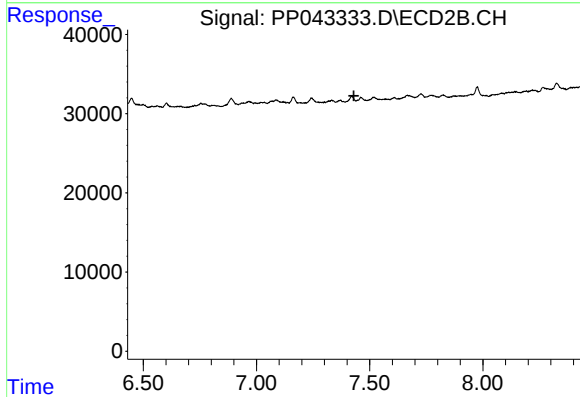


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.430 min
Response: 0
Conc: N.D.

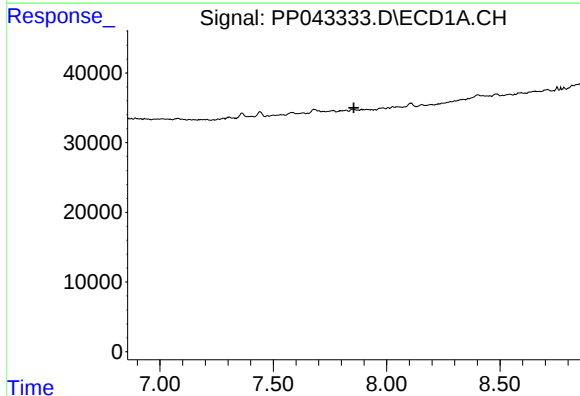


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 7.856 min
Response: 0
Conc: N.D.

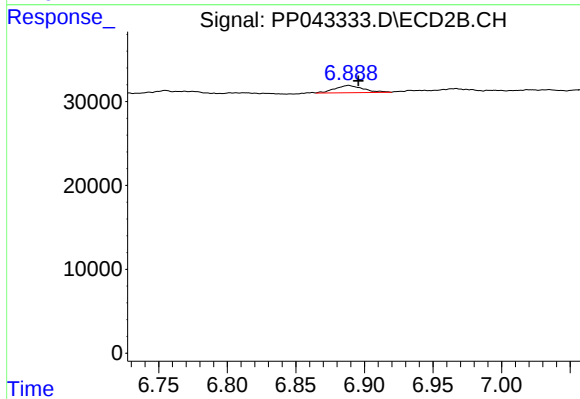

#31 AR-1260-1


R.T.: 6.889 min
Delta R.T.: -0.007 min
Response: 12332
Conc: 10.54 ng/ml

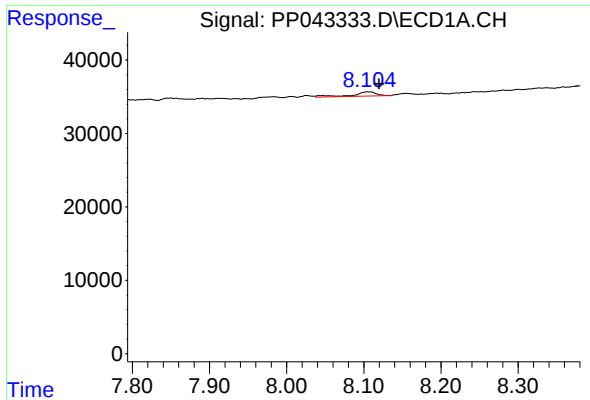

#32 AR-1260-2


R.T.: 8.105 min
Delta R.T.: -0.014 min
Response: 12116
Conc: 14.23 ng/ml

Instrument :
ECD_P
ClientSampleId :

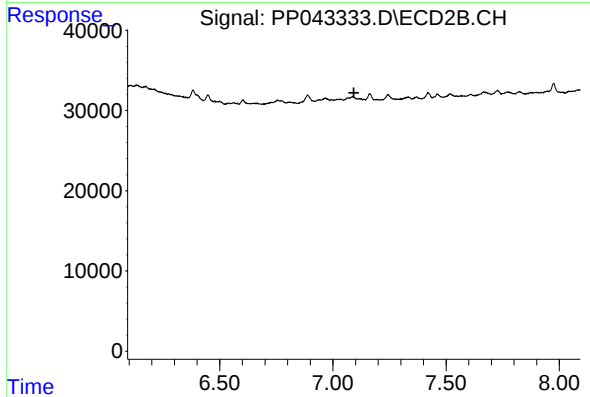


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.093 min
Response: 0
Conc: N.D.

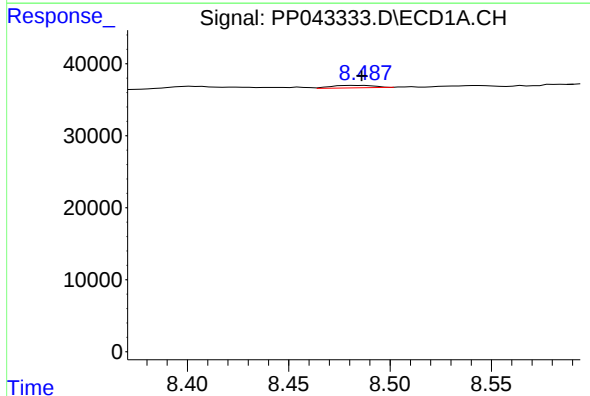


#33 AR-1260-3

R.T.: 8.488 min
Delta R.T.: 0.002 min
Response: 5196
Conc: 7.88 ng/ml

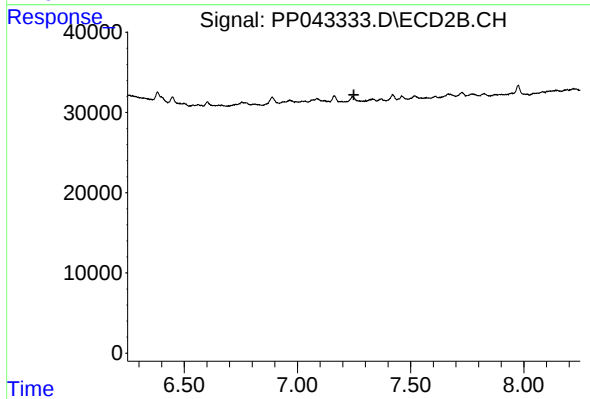

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.250 min
Response: 0
Conc: N.D.

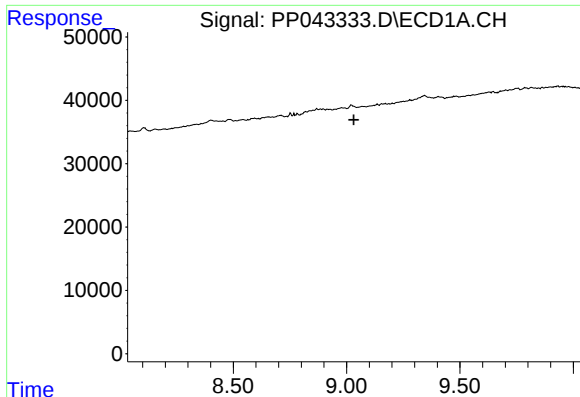

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 9.032 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

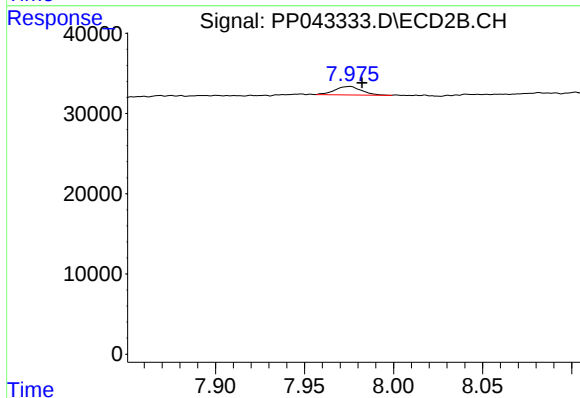


#35 AR-1260-5

R.T.: 7.976 min
Delta R.T.: -0.007 min
Response: 11048
Conc: 4.99 ng/ml

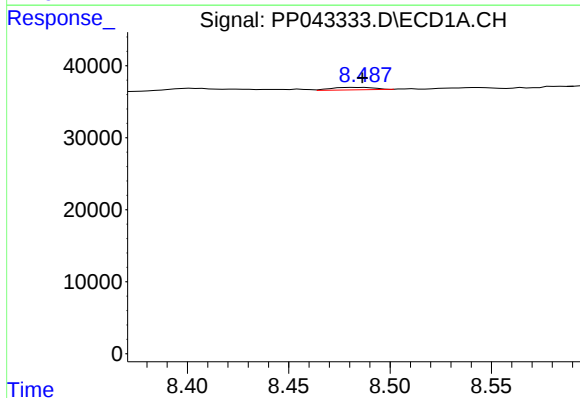

#36 AR-1262-1

R.T.: 8.488 min
Delta R.T.: 0.002 min
Response: 5196
Conc: 5.23 ng/ml

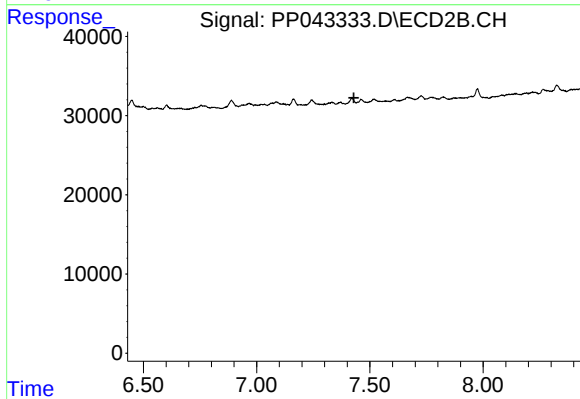

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.429 min
Response: 0
Conc: N.D.