

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012822\
 Data File : PP043311.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jan 2022 10:39
 Operator : AJ\MA
 Sample : PB142323BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB142323BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 23:30:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 25 03:09:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.868	4.034	464481	485888	20.207	21.806
2)	SA Decachlor...	10.789	9.360	368785	462692	26.038	24.819

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012822\
Data File : PP043311.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jan 2022 10:39
Operator : AJ\MA
Sample : PB142323BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB142323BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 23:30:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

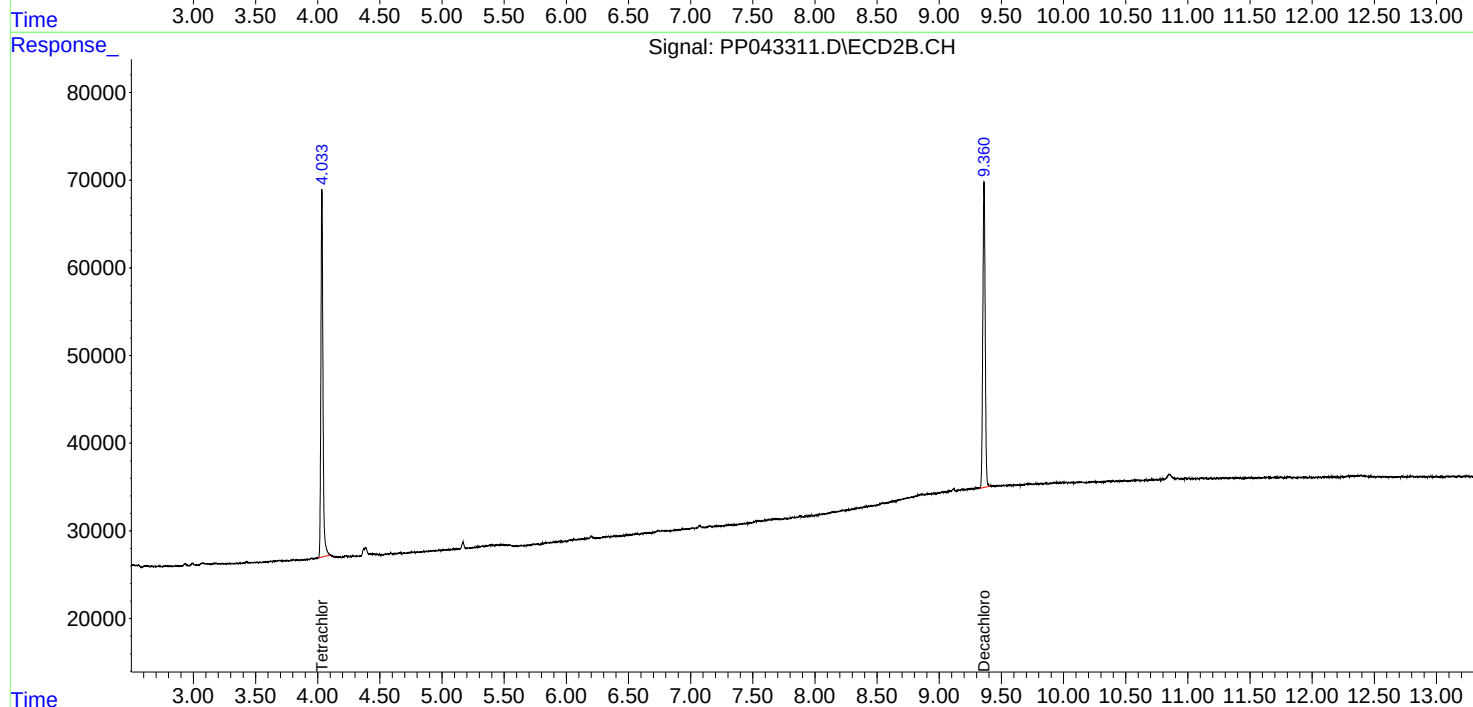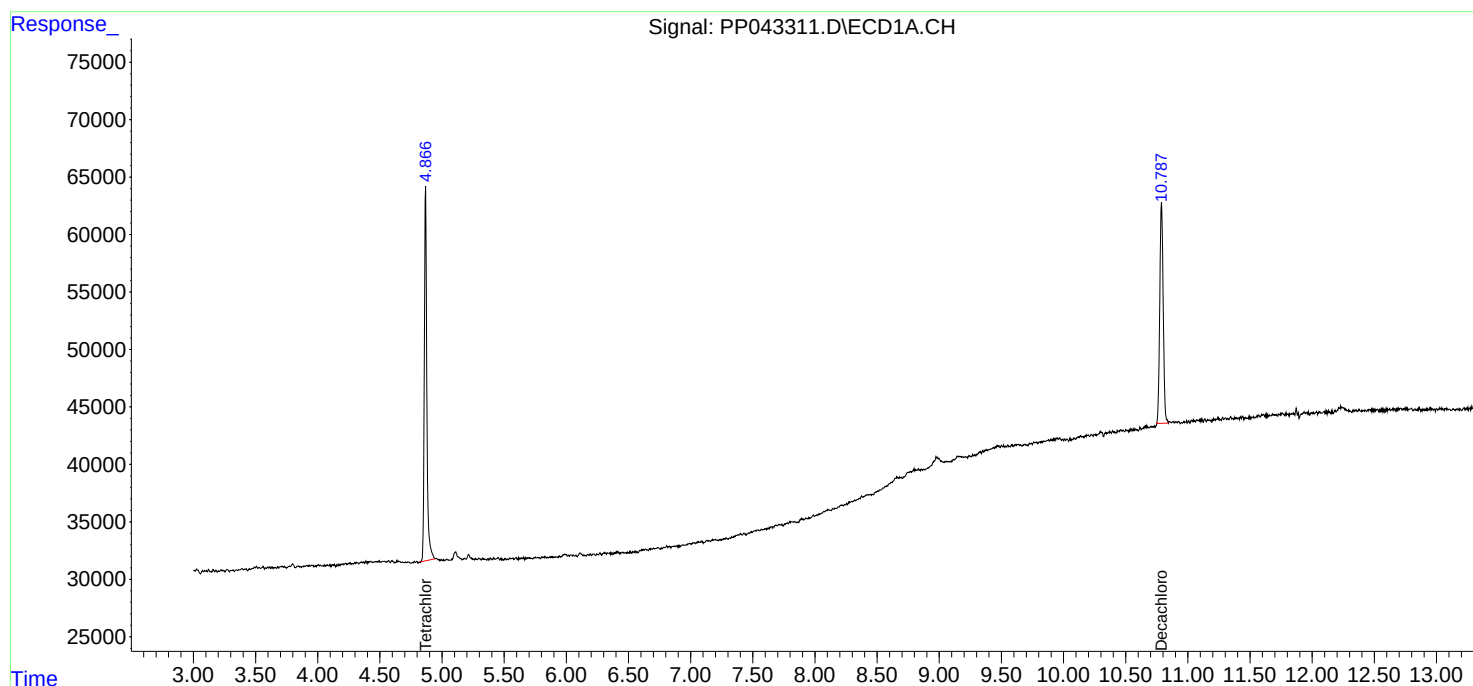


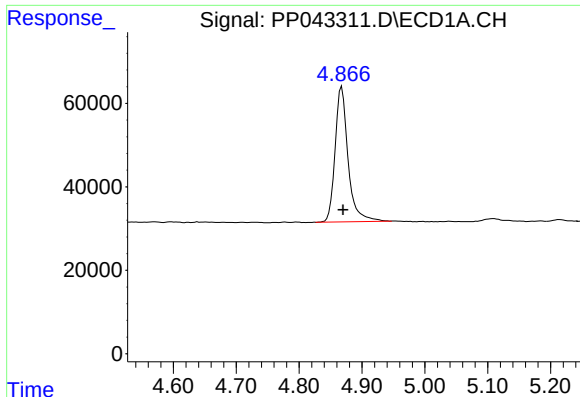

#1 Tetrachloro-m-xylene


R.T.: 4.868 min
Delta R.T.: -0.002 min
Response: 464481
Conc: 20.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB142323BL

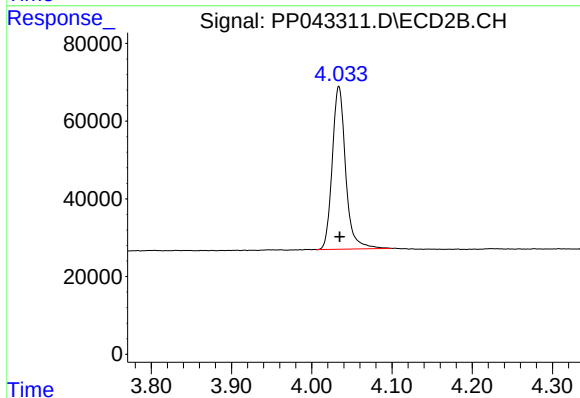


#1 Tetrachloro-m-xylene

R.T.: 4.034 min
Delta R.T.: -0.001 min
Response: 485888
Conc: 21.81 ng/ml

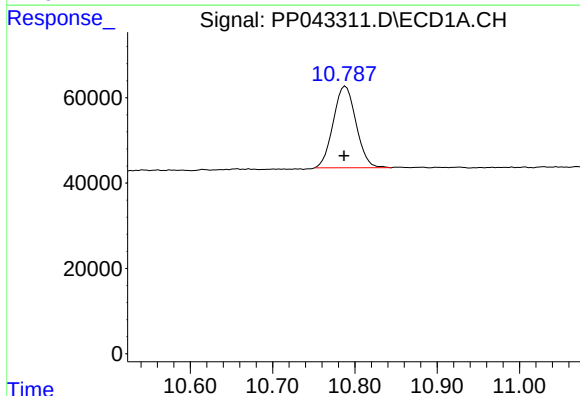

#2 Decachlorobiphenyl

R.T.: 10.789 min
Delta R.T.: 0.002 min
Response: 368785
Conc: 26.04 ng/ml

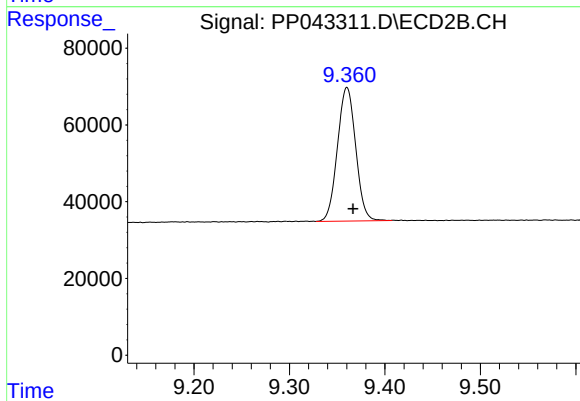

#2 Decachlorobiphenyl

R.T.: 9.360 min
Delta R.T.: -0.006 min
Response: 462692
Conc: 24.82 ng/ml