

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012822\
 Data File : PP043315.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jan 2022 11:45
 Operator : AJ\MA
 Sample : N1276-04RE 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-SF-012522-04

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 23:32:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 25 03:09:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.871	4.037	85163	137982	3.705m	6.192m#
2) SA Decachlor...	10.779	9.361	2084041	25076	147.142m	1.345m#

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012822\
Data File : PP043315.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jan 2022 11:45
Operator : AJ\MA
Sample : N1276-04RE 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PCB-SF-012522-04

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 23:32:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

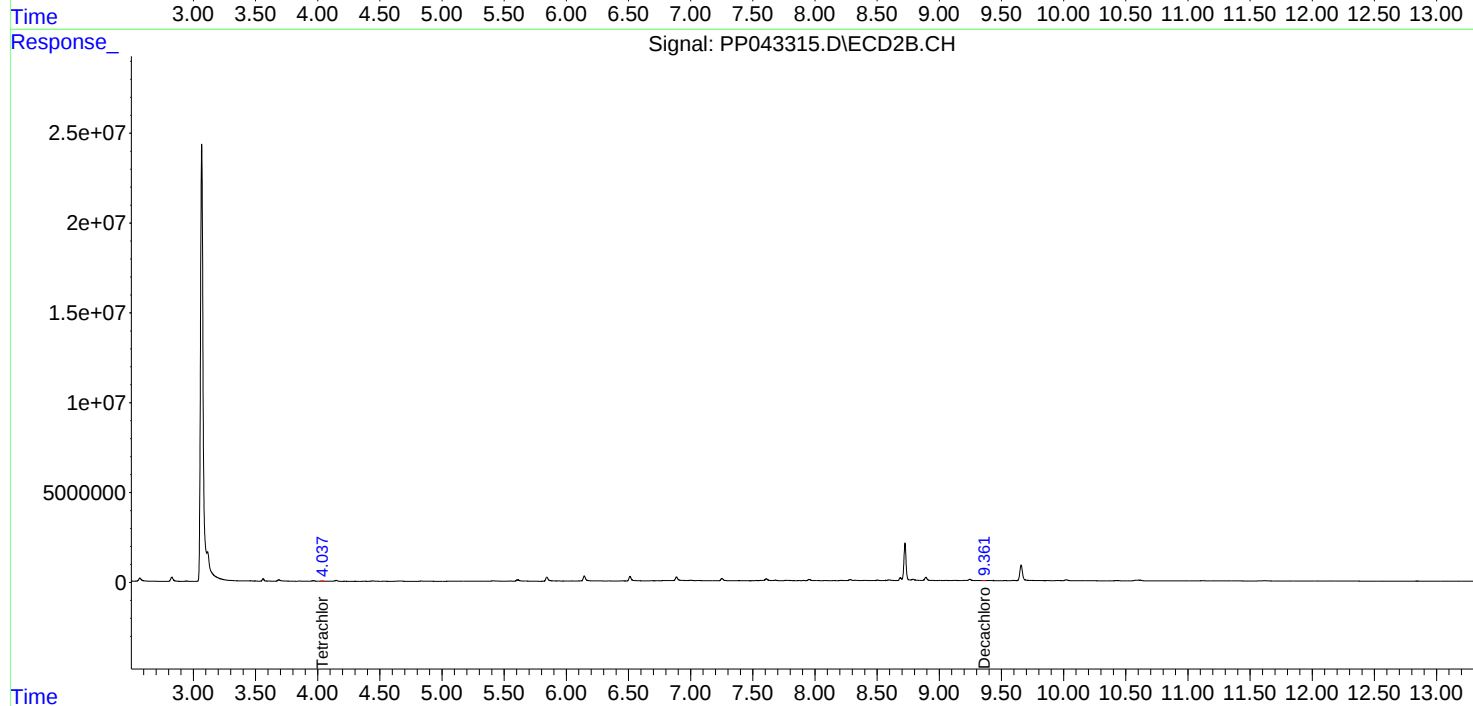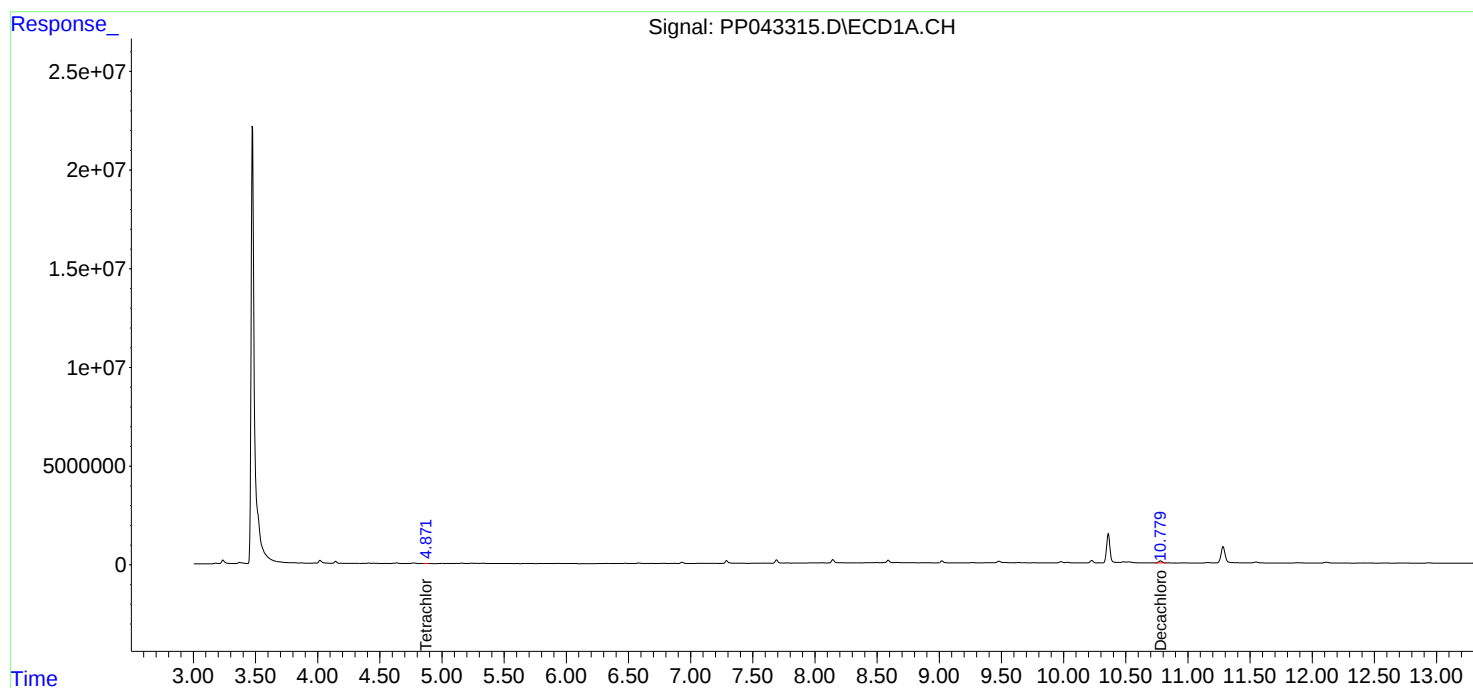


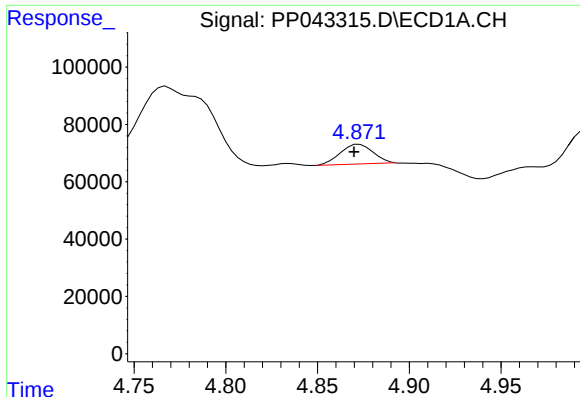

#1 Tetrachloro-m-xylene


R.T.: 4.871 min
Delta R.T.: 0.001 min
Response: 85163
Conc: 3.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-012522-04

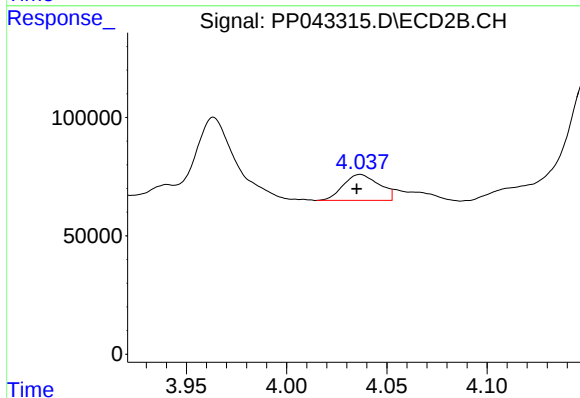


#1 Tetrachloro-m-xylene

R.T.: 4.037 min
Delta R.T.: 0.002 min
Response: 137982
Conc: 6.19 ng/ml m

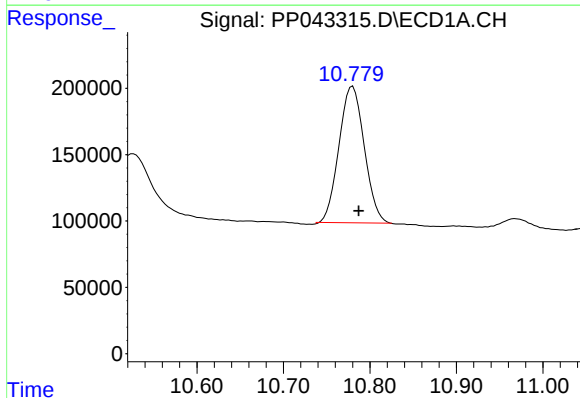

#2 Decachlorobiphenyl

R.T.: 10.779 min
Delta R.T.: -0.008 min
Response: 2084041
Conc: 147.14 ng/ml m

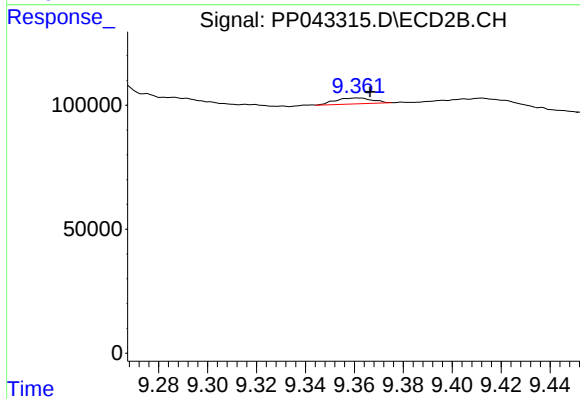

#2 Decachlorobiphenyl

R.T.: 9.361 min
Delta R.T.: -0.006 min
Response: 25076
Conc: 1.35 ng/ml m