

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012822\
 Data File : PP043332.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jan 2022 17:26
 Operator : AJ\MA
 Sample : N1316-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TR-05-012722

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 23:37:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 25 03:09:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.866	4.032	425792	535124	18.524	24.016 #
2) SA Decachlor...	10.784	9.358	316616	351150	22.354m	18.836

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012822\
Data File : PP043332.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jan 2022 17:26
Operator : AJ\MA
Sample : N1316-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TR-05-012722

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 23:37:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

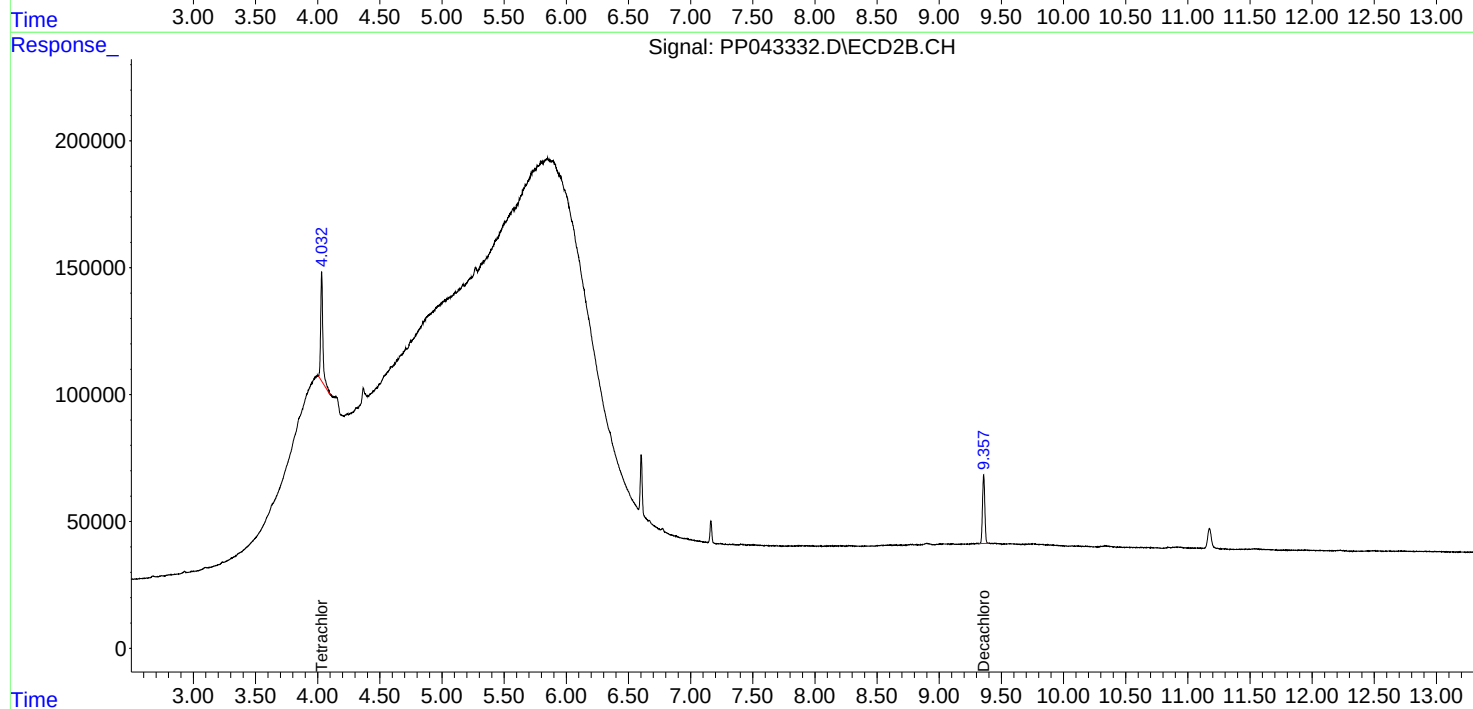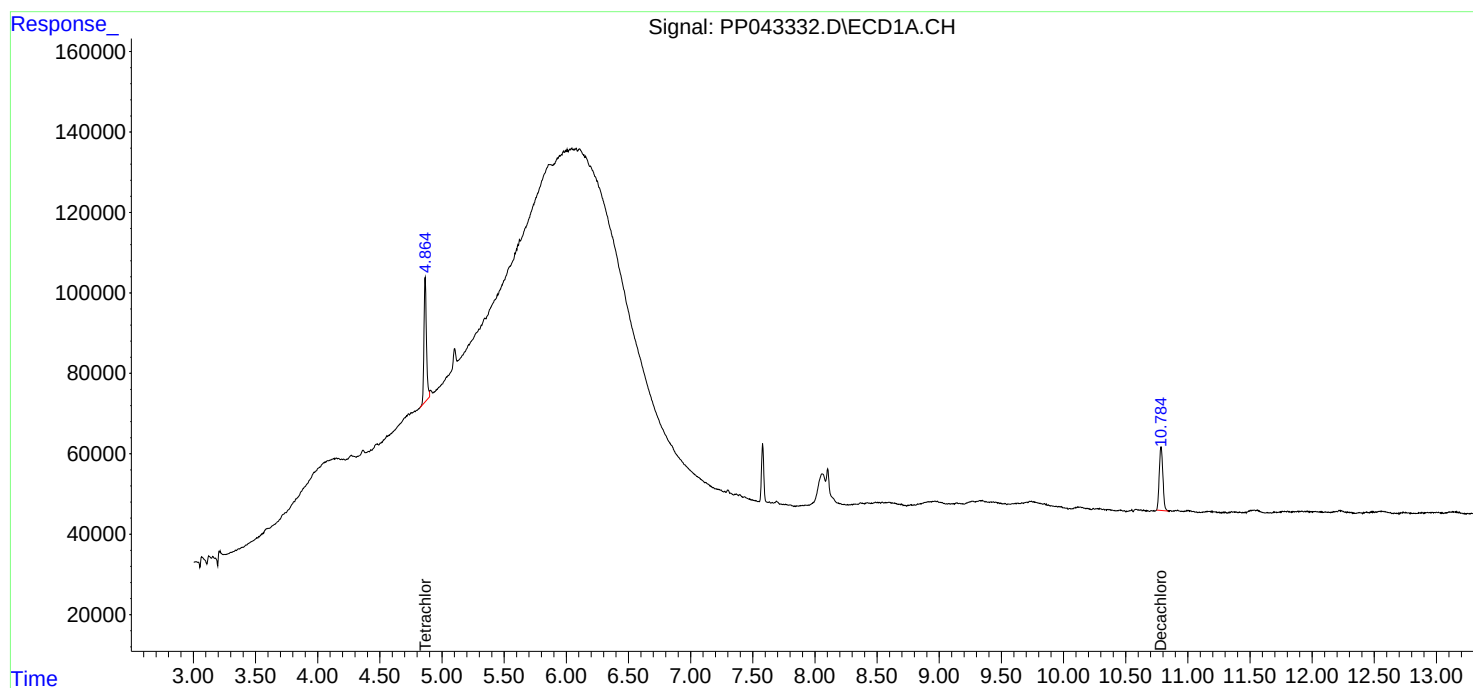


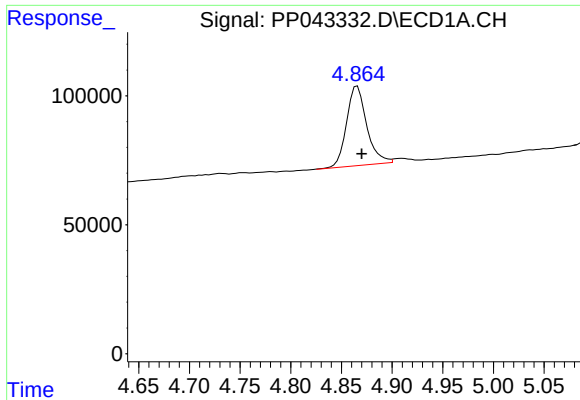

#1 Tetrachloro-m-xylene


R.T.: 4.866 min
Delta R.T.: -0.004 min
Response: 425792
Conc: 18.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
TR-05-012722

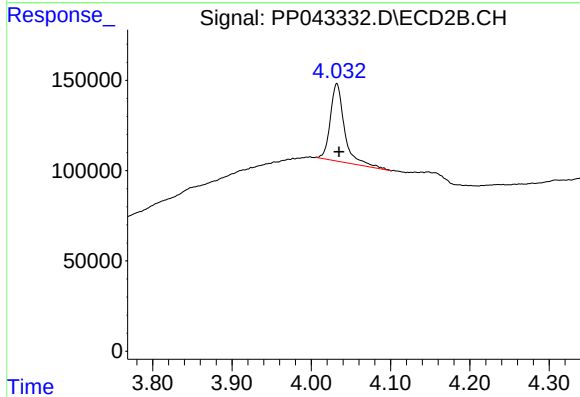


#1 Tetrachloro-m-xylene

R.T.: 4.032 min
Delta R.T.: -0.003 min
Response: 535124
Conc: 24.02 ng/ml

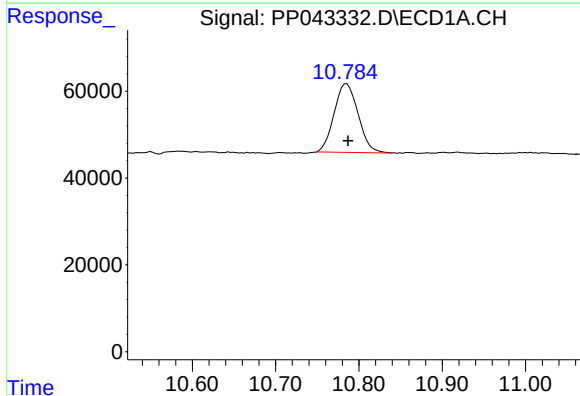

#2 Decachlorobiphenyl

R.T.: 10.784 min
Delta R.T.: -0.003 min
Response: 316616
Conc: 22.35 ng/ml m

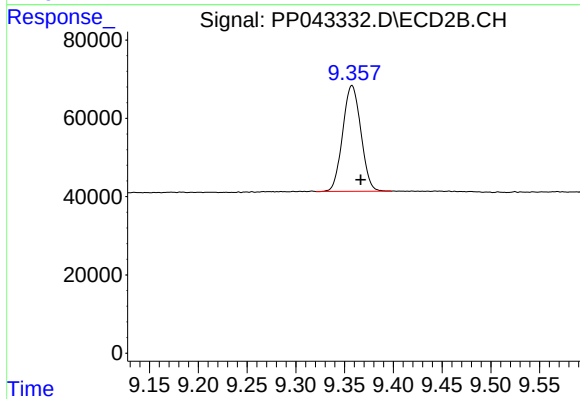

#2 Decachlorobiphenyl

R.T.: 9.358 min
Delta R.T.: -0.009 min
Response: 351150
Conc: 18.84 ng/ml