

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012823\
 Data File : PP055025.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2023 00:19
 Operator : YP\AJ
 Sample : 01329-11
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-8-BORING-2-21-28

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 05:04:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 03:37:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.328	3.574	32036827	29307552	18.425	19.523
2) SA Decachlor...	10.083	8.589	31154456	25087538	17.991	18.576

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012823\
Data File : PP055025.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2023 00:19
Operator : YP\AJ
Sample : 01329-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
COMP-8-BORING-2-21-28

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 05:04:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 03:37:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

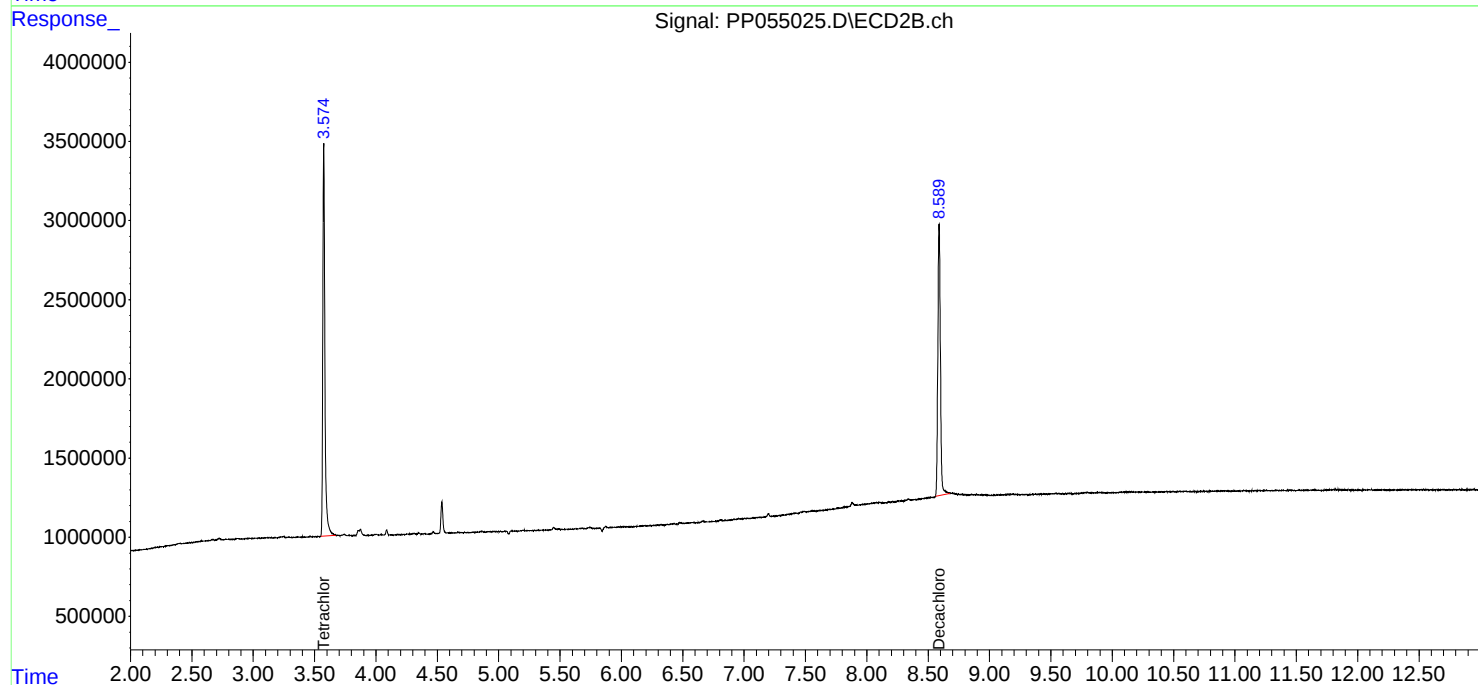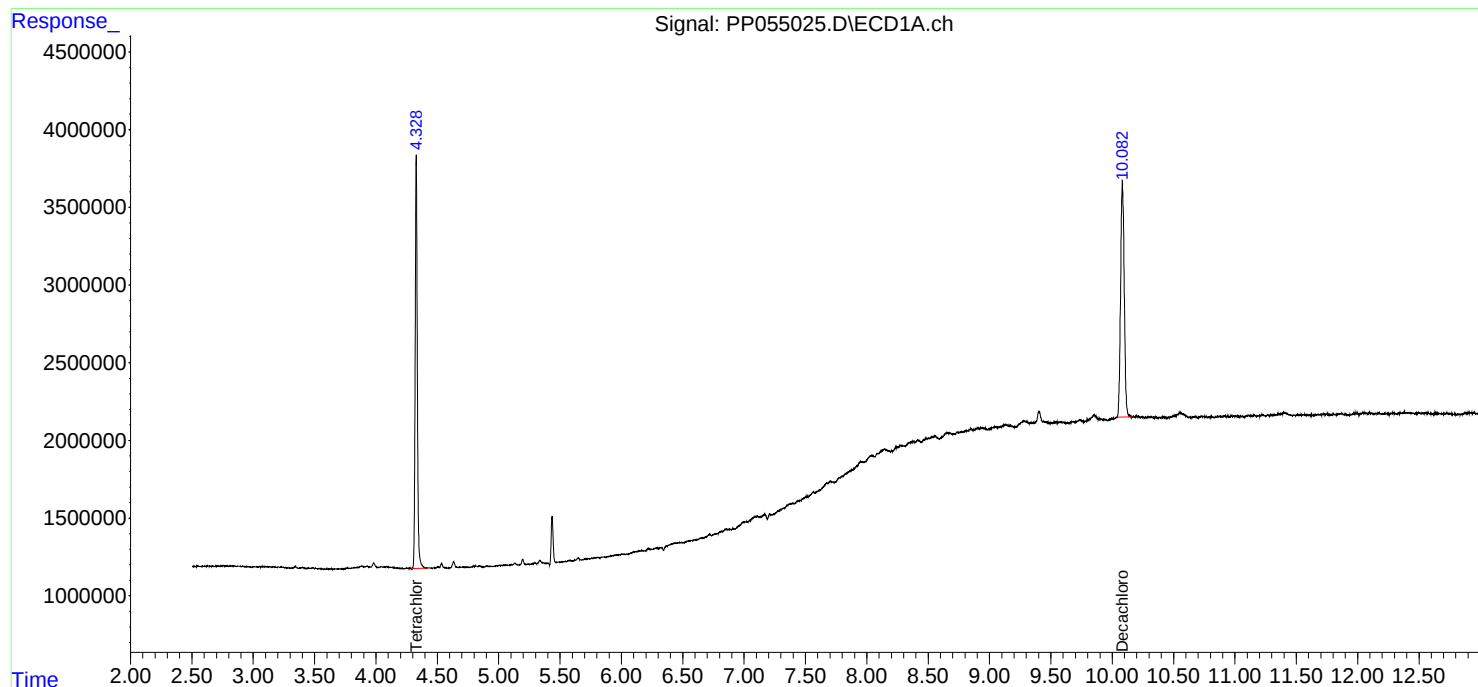


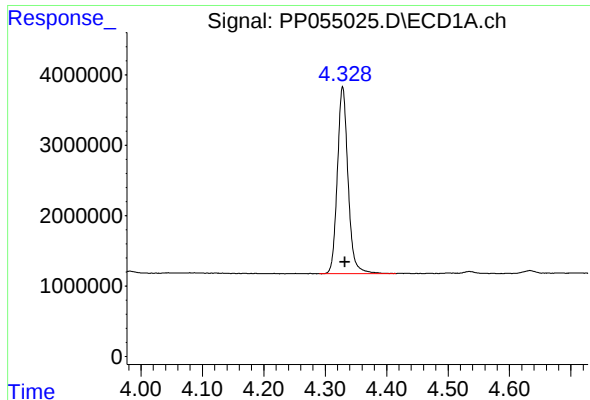

#1 Tetrachloro-m-xylene


R.T.: 4.328 min
Delta R.T.: -0.004 min
Response: 32036827
Conc: 18.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-8-BORING-2-21-28

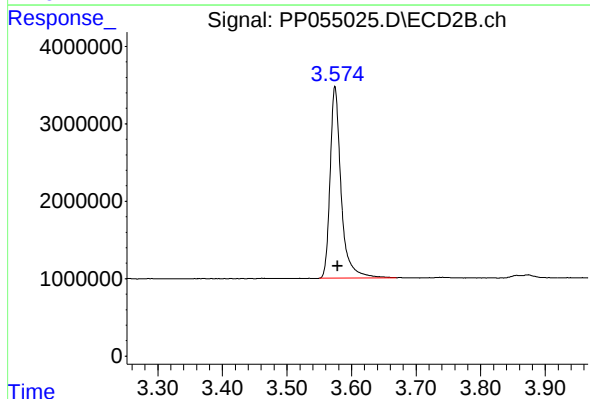


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: -0.004 min
Response: 29307552
Conc: 19.52 ng/ml

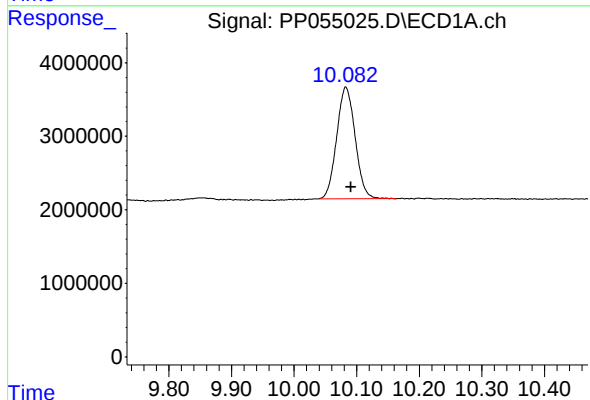

#2 Decachlorobiphenyl

R.T.: 10.083 min
Delta R.T.: -0.008 min
Response: 31154456
Conc: 17.99 ng/ml

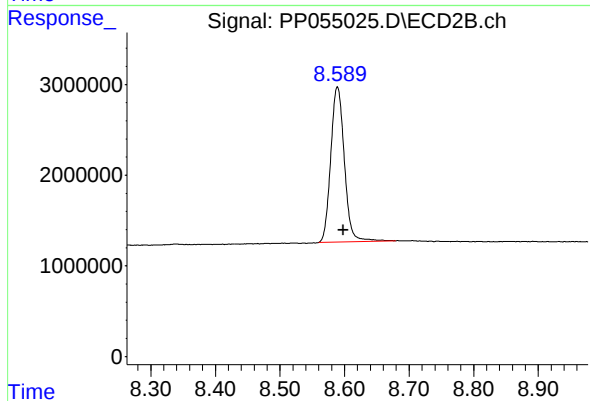

#2 Decachlorobiphenyl

R.T.: 8.589 min
Delta R.T.: -0.009 min
Response: 25087538
Conc: 18.58 ng/ml