

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012921\
 Data File : PP033073.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jan 2021 15:38
 Operator : DD\AJ
 Sample : PB134397BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 00:25:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 04:07:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.733	4.005	1096203	911566	19.305	19.829
2) SA Decachlor...	10.561	9.276	850608	767816	23.708	23.367
Target Compounds						
8) L2 AR-1221-1	4.976	0.000	69211	0	123.936	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012921\
Data File : PP033073.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jan 2021 15:38
Operator : DD\AJ
Sample : PB134397BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 00:25:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 04:07:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

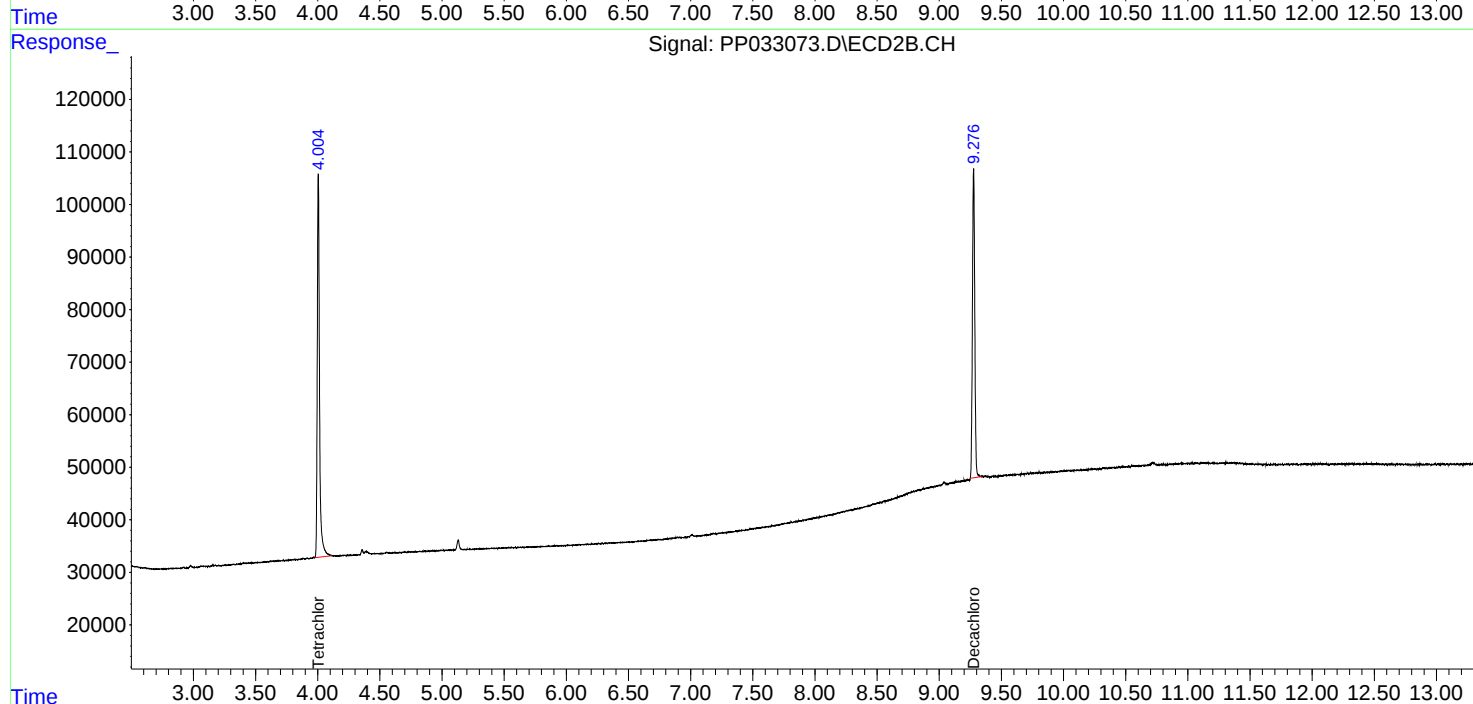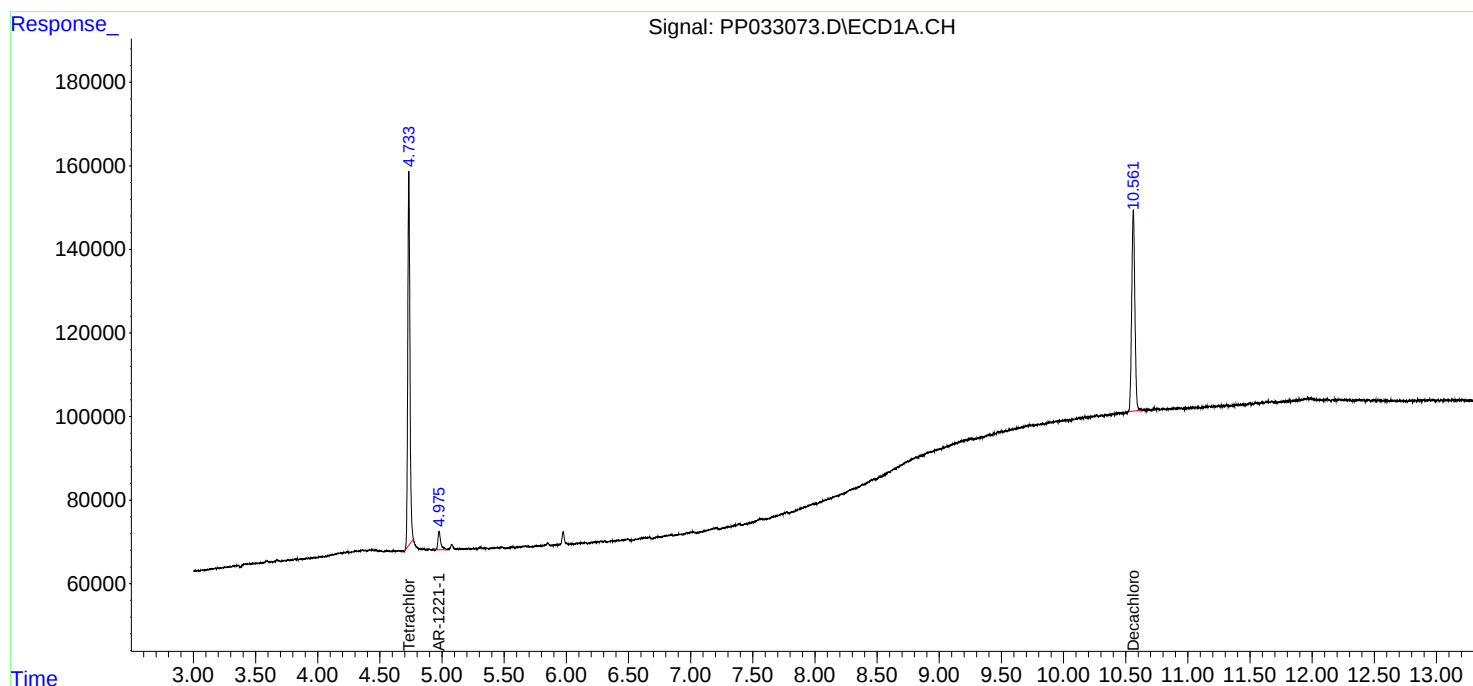


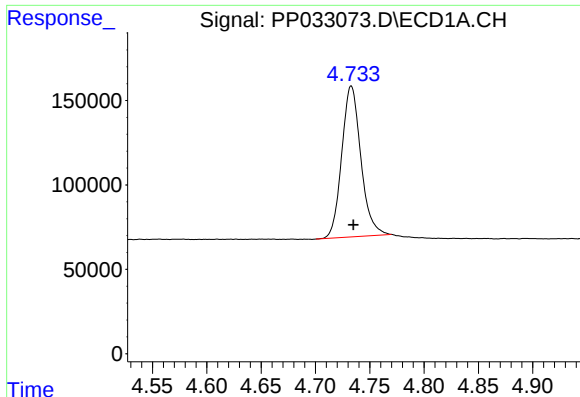

#1 Tetrachloro-m-xylene


R.T.: 4.733 min
Delta R.T.: -0.002 min
Response: 1096203
Conc: 19.31 ng/ml

Instrument :
ECD_P
ClientSampleId :

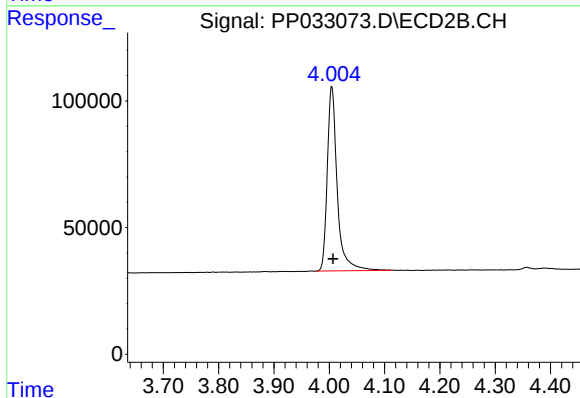


#1 Tetrachloro-m-xylene

R.T.: 4.005 min
Delta R.T.: -0.002 min
Response: 911566
Conc: 19.83 ng/ml

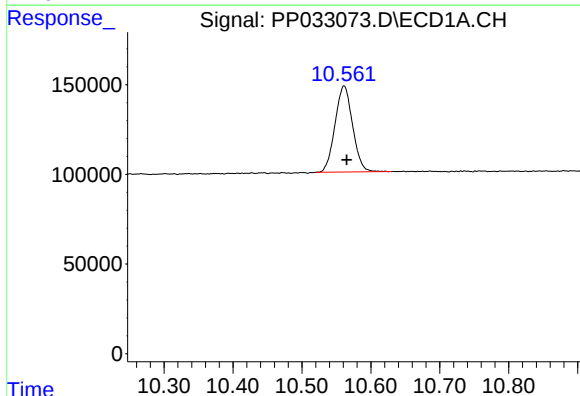


#2 Decachlorobiphenyl

R.T.: 10.561 min
Delta R.T.: -0.004 min
Response: 850608
Conc: 23.71 ng/ml

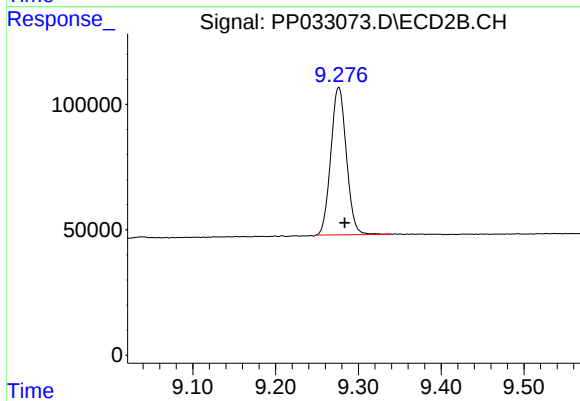

#2 Decachlorobiphenyl


R.T.: 9.276 min
Delta R.T.: -0.007 min
Response: 767816
Conc: 23.37 ng/ml

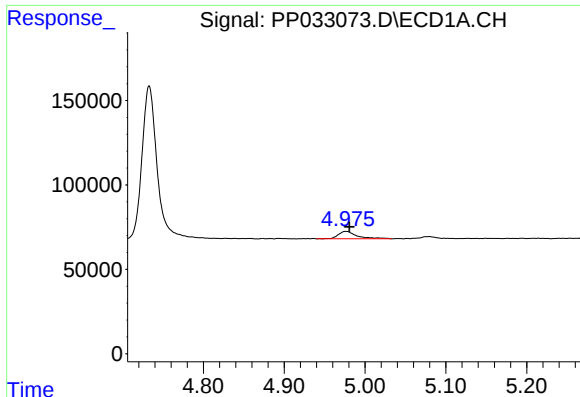

#8 AR-1221-1

R.T.: 4.976 min
Delta R.T.: -0.004 min
Response: 69211
Conc: 123.94 ng/ml

Instrument :
ECD_P
ClientSampleId :

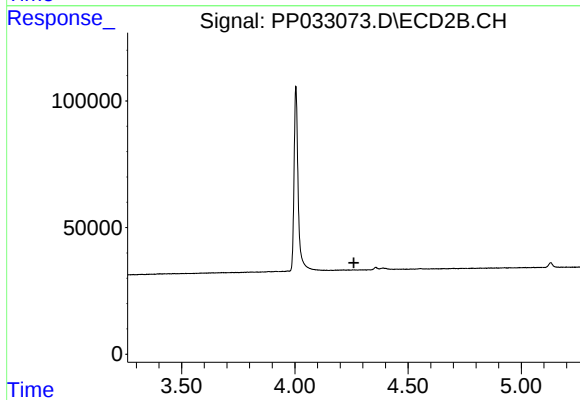

#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.261 min
Response: 0
Conc: N.D.