

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012921\
 Data File : PP033077.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jan 2021 16:45
 Operator : DD\AJ
 Sample : M1279-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S17-02-D

Manual Integrations
 APPROVED

Ankita
 2/3/2021 4:33:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 00:26:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 04:07:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.732	4.004	873137	750863	15.377	16.334
2) SA Decachlor...	10.559	9.275	472673	446135	13.174	13.577m
Target Compounds						
41) L9 AR-1268-1	9.170	8.197	230222	155145	37.237	32.741m
42) L9 AR-1268-2	9.260	8.262	188095	159140	33.629	35.480
43) L9 AR-1268-3	9.469	8.465	122583	102988	23.680	25.055m
44) L9 AR-1268-4	9.880	8.759	21774	45130	13.732	32.933 #
45) L9 AR-1268-5	10.253	9.037	324296	285402	25.031	25.307

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012921\
Data File : PP033077.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jan 2021 16:45
Operator : DD\AJ
Sample : M1279-02
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleID :
S17-02-D


Manual Integrations
APPROVED

Ankita
2/3/2021 4:33:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 00:26:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 04:07:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

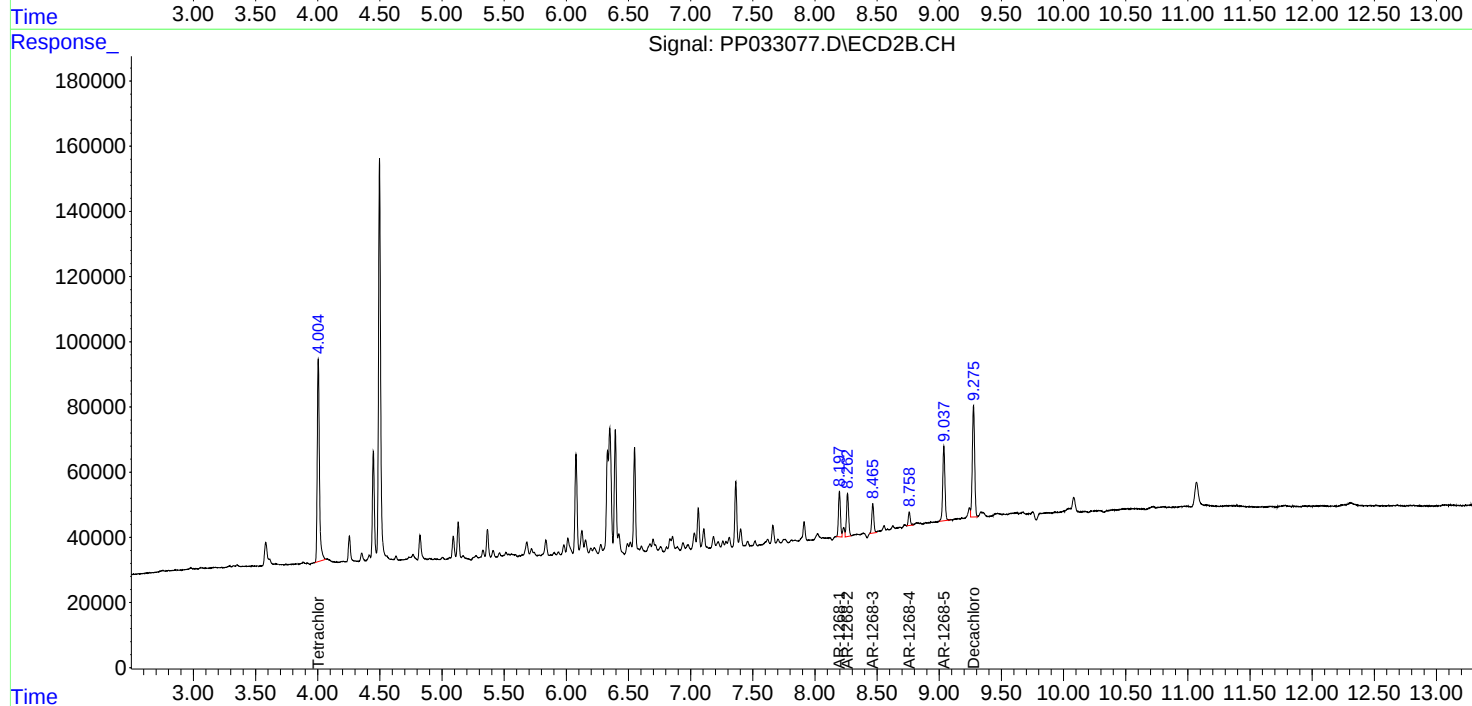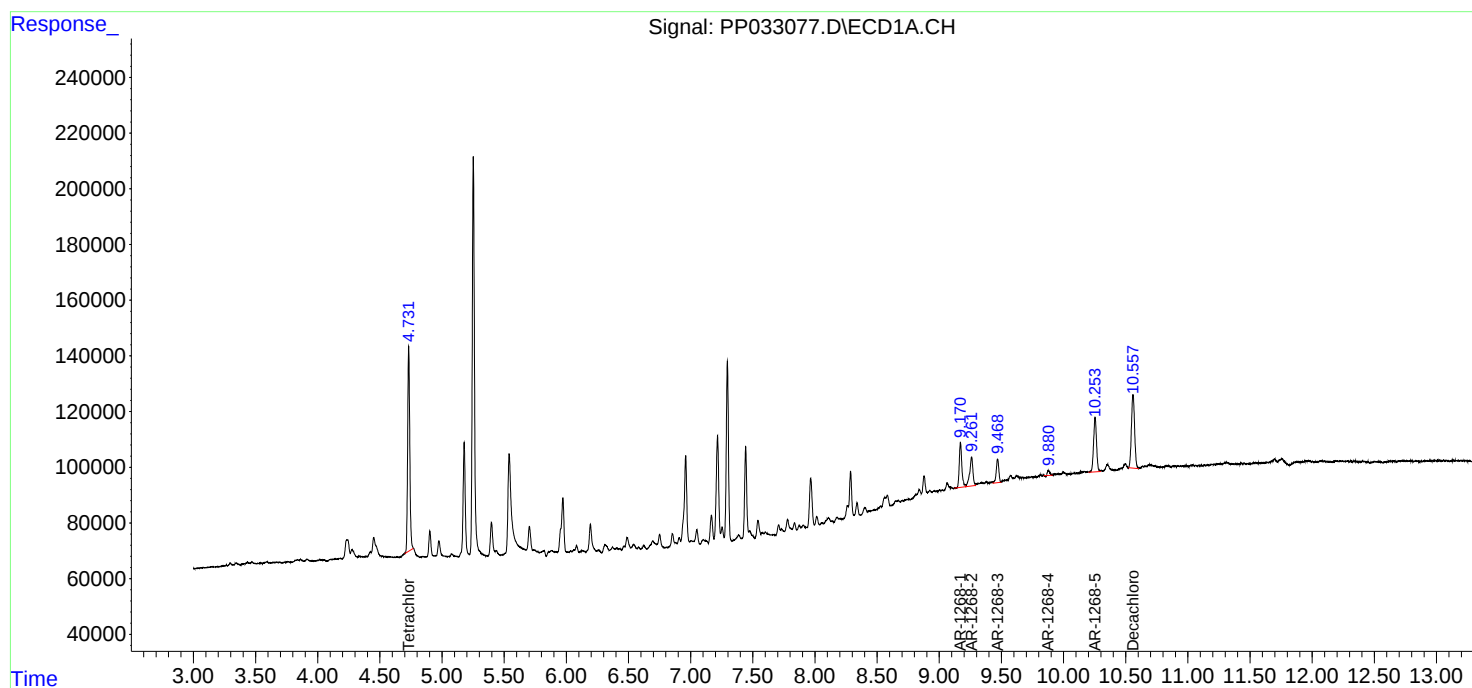

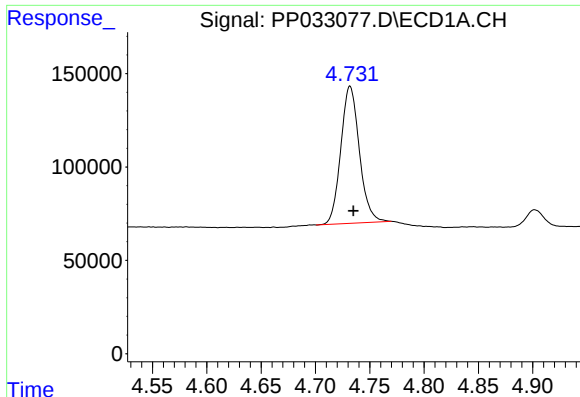


#1 Tetrachloro-m-xylene

R.T.: 4.732 min
Delta R.T.: -0.003 min
Response: 873137
Conc: 15.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
S17-02-D


Manual Integrations
APPROVED

Ankita
2/3/2021 4:33:07 PM

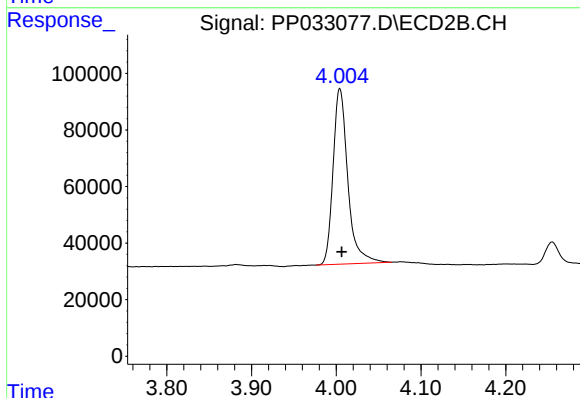


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: -0.002 min
Response: 750863
Conc: 16.33 ng/ml

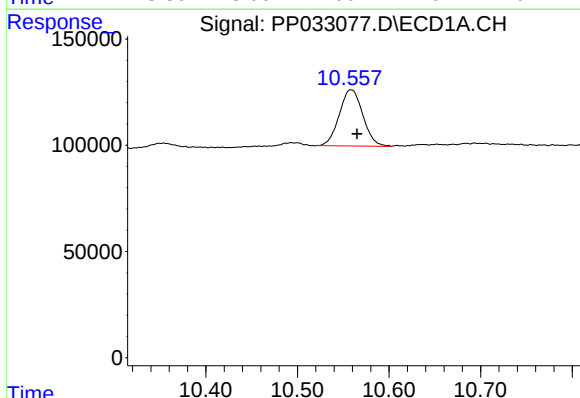


#2 Decachlorobiphenyl

R.T.: 10.559 min
Delta R.T.: -0.007 min
Response: 472673
Conc: 13.17 ng/ml

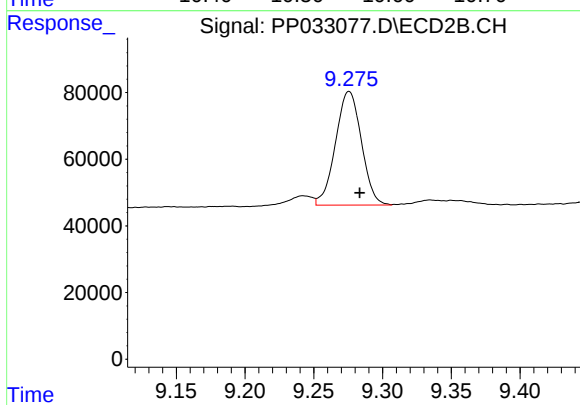

#2 Decachlorobiphenyl

R.T.: 9.275 min
Delta R.T.: -0.008 min
Response: 446135
Conc: 13.58 ng/ml m

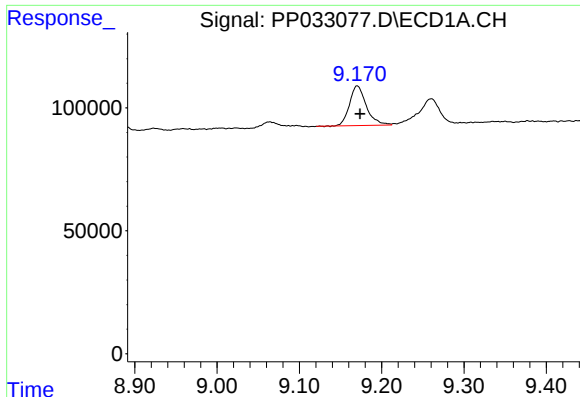


#41 AR-1268-1

R.T.: 9.170 min
Delta R.T.: -0.003 min
Response: 230222
Conc: 37.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
S17-02-D


Manual Integrations
APPROVED

Ankita
2/3/2021 4:33:07 PM

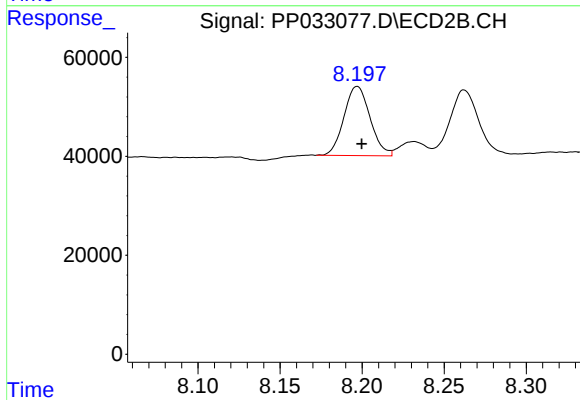


#41 AR-1268-1

R.T.: 8.197 min
Delta R.T.: -0.003 min
Response: 155145
Conc: 32.74 ng/ml m

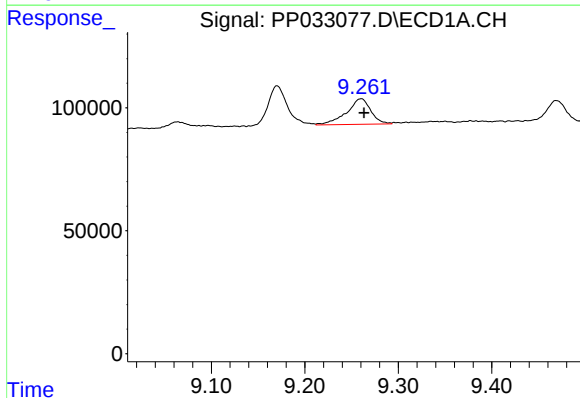


#42 AR-1268-2

R.T.: 9.260 min
Delta R.T.: -0.003 min
Response: 188095
Conc: 33.63 ng/ml

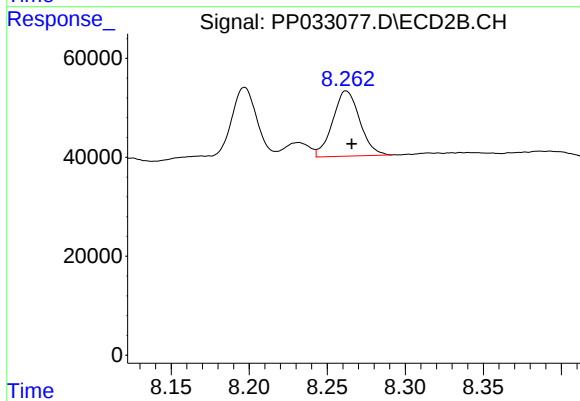

#42 AR-1268-2

R.T.: 8.262 min
Delta R.T.: -0.004 min
Response: 159140
Conc: 35.48 ng/ml

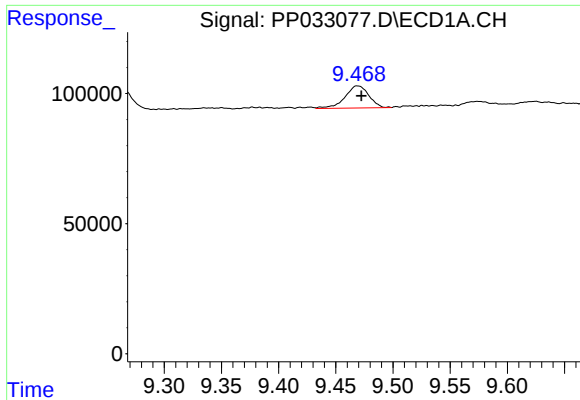


#43 AR-1268-3

R.T.: 9.469 min
Delta R.T.: -0.003 min
Response: 122583
Conc: 23.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
S17-02-D


Manual Integrations
APPROVED

Ankita
2/3/2021 4:33:07 PM

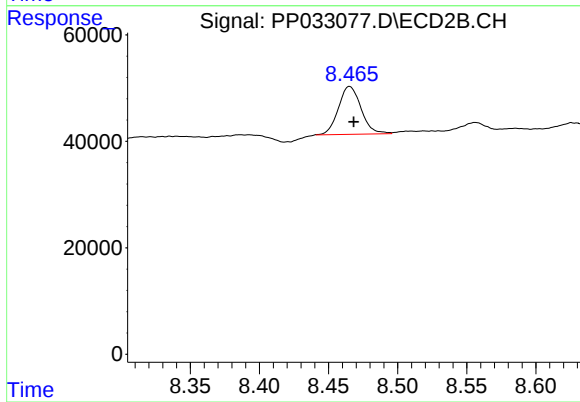


#43 AR-1268-3

R.T.: 8.465 min
Delta R.T.: -0.003 min
Response: 102988
Conc: 25.05 ng/ml m

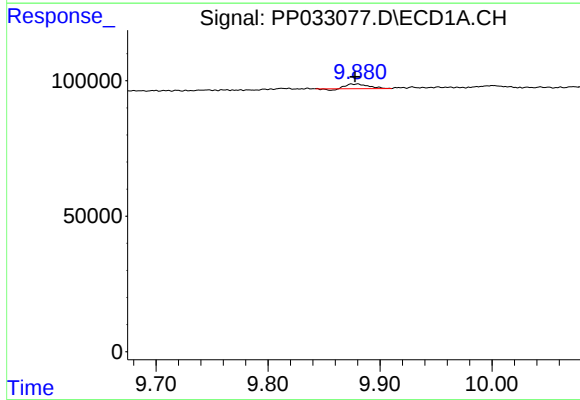


#44 AR-1268-4

R.T.: 9.880 min
Delta R.T.: 0.002 min
Response: 21774
Conc: 13.73 ng/ml

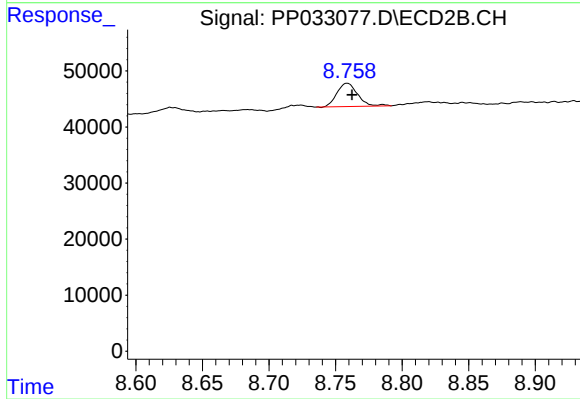

#44 AR-1268-4

R.T.: 8.759 min
Delta R.T.: -0.004 min
Response: 45130
Conc: 32.93 ng/ml

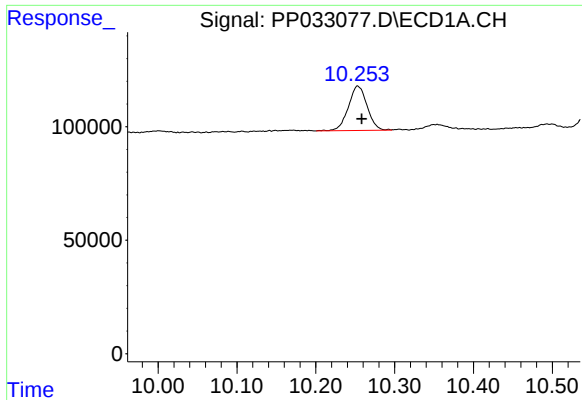


#45 AR-1268-5

R.T.: 10.253 min
Delta R.T.: -0.005 min
Response: 324296
Conc: 25.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
S17-02-D

Manual Integrations
APPROVED

Ankita
2/3/2021 4:33:07 PM

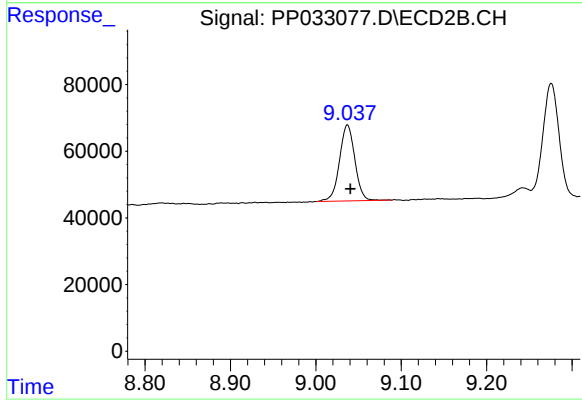

#45 AR-1268-5

R.T.: 9.037 min
Delta R.T.: -0.004 min
Response: 285402
Conc: 25.31 ng/ml