

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012921\
 Data File : PP033109.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jan 2021 2:12
 Operator : DD\AJ
 Sample : M1286-03
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JJ BH 01 2-4

Manual Integrations
 APPROVED

Ankita
 2/3/2021 4:34:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:54:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 04:07:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.731	4.004	1133624	965190	19.964	20.996
2) SA Decachlor...	10.558	9.274	752814	662199	20.983	20.152

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012921\
Data File : PP033109.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jan 2021 2:12
Operator : DD\AJ
Sample : M1286-03
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
JJ BH 01 2-4


Manual Integrations
APPROVED

Ankita
2/3/2021 4:34:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:54:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 04:07:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

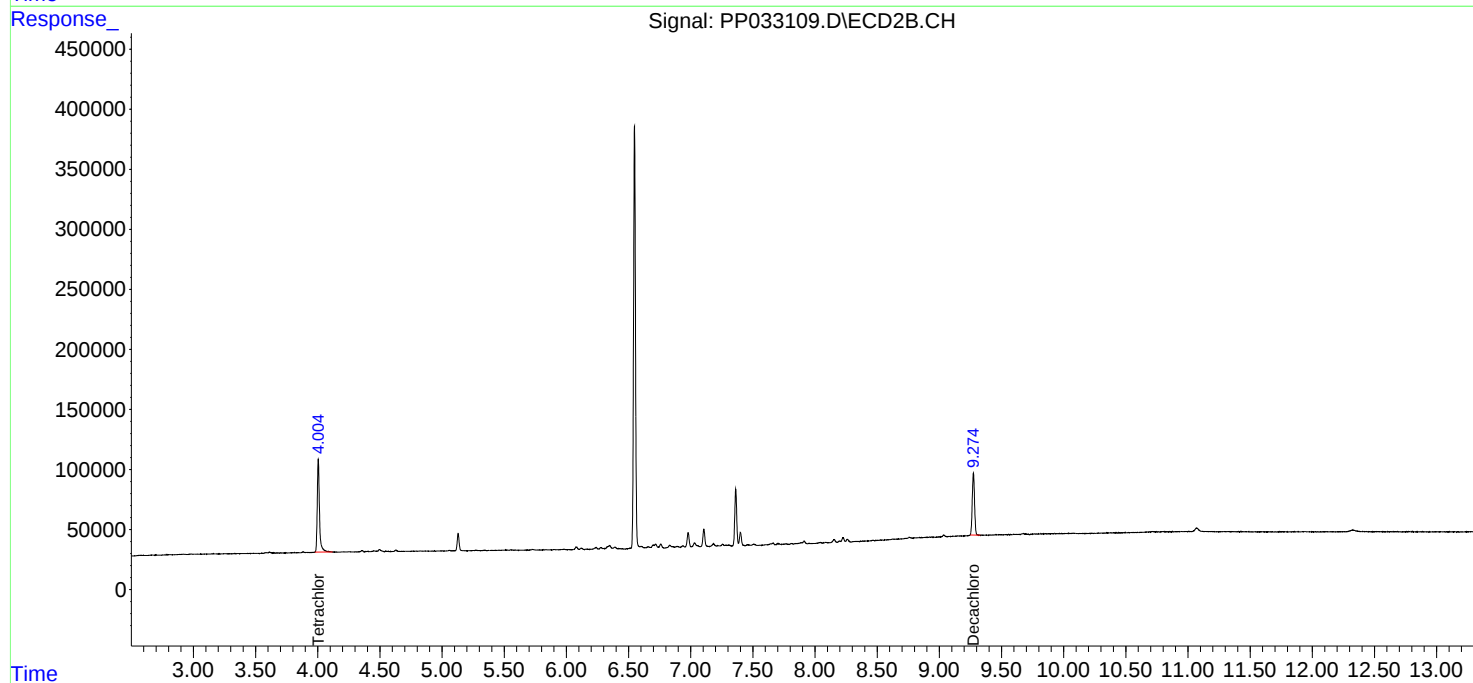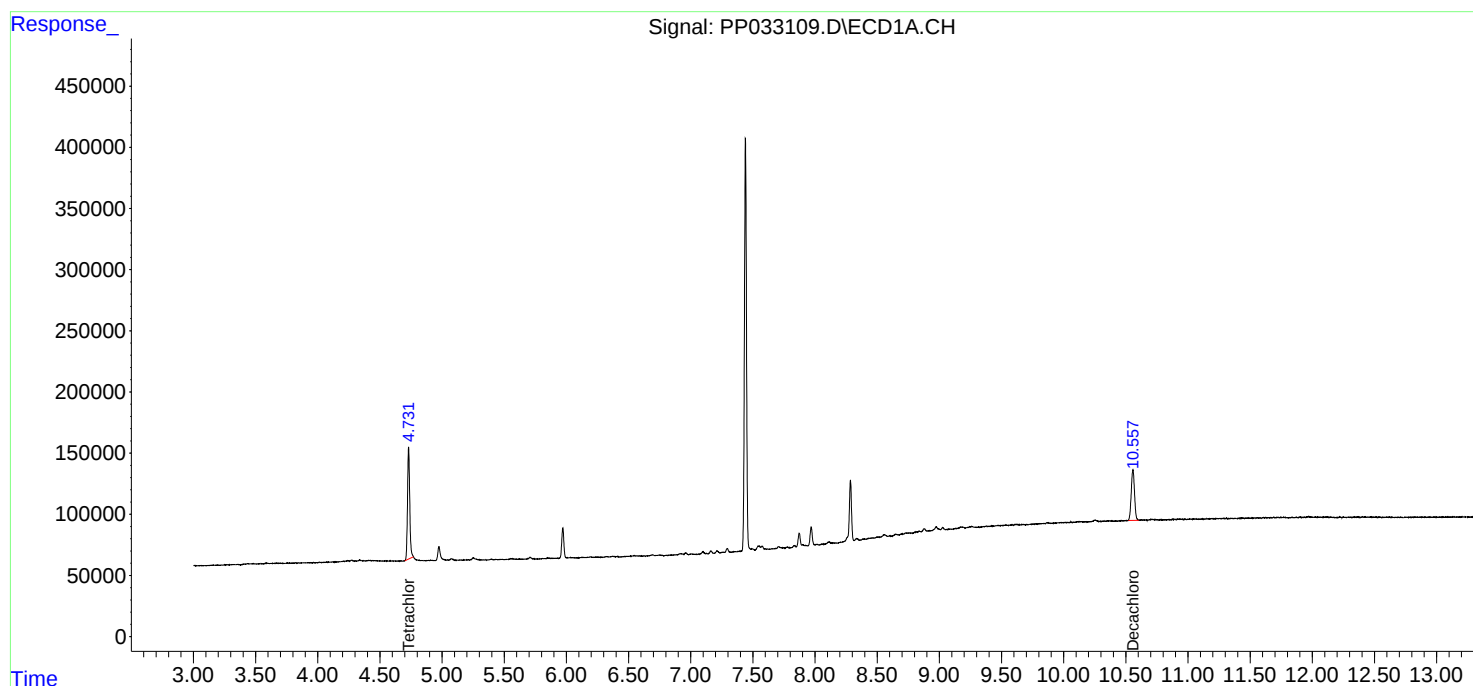

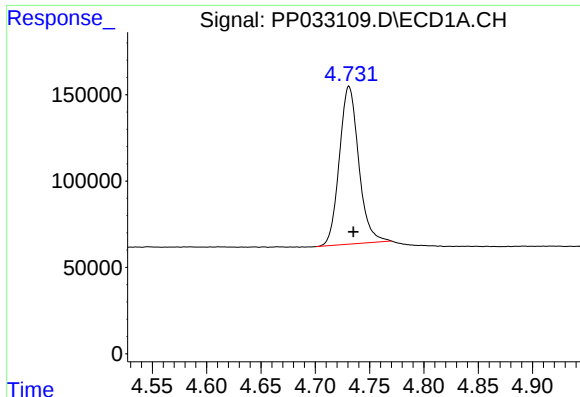


#1 Tetrachloro-m-xylene

R.T.: 4.731 min
Delta R.T.: -0.004 min
Response: 1133624
Conc: 19.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
JJ BH 01 2-4


Manual Integrations
APPROVED

Ankita
2/3/2021 4:34:38 PM

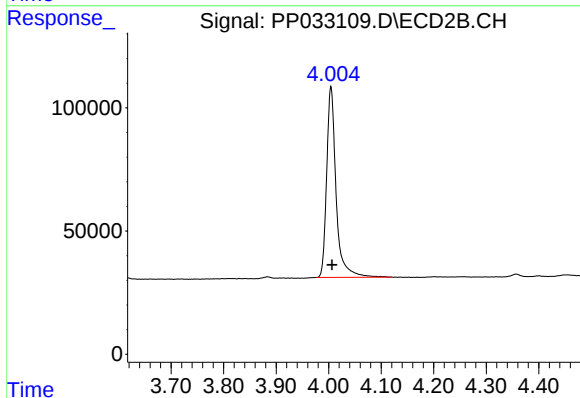


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: -0.002 min
Response: 965190
Conc: 21.00 ng/ml

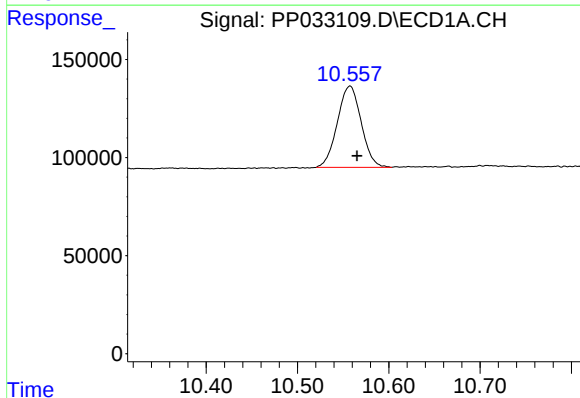

#2 Decachlorobiphenyl

R.T.: 10.558 min
Delta R.T.: -0.008 min
Response: 752814
Conc: 20.98 ng/ml

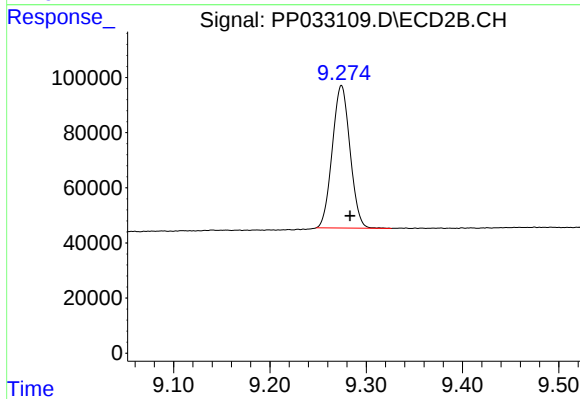

#2 Decachlorobiphenyl

R.T.: 9.274 min
Delta R.T.: -0.009 min
Response: 662199
Conc: 20.15 ng/ml