

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012921\
 Data File : PP033112.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jan 2021 3:02
 Operator : DD\AJ
 Sample : M1286-09
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JJ BH 02 0-1

Manual Integrations
 APPROVED

Ankita
 2/3/2021 4:34:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 02:55:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 04:07:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.731	4.004	1264220	1001231	22.264	21.780
2) SA Decachlor...	10.557	9.273	908483	737014	25.321	22.429

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012921\
Data File : PP033112.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jan 2021 3:02
Operator : DD\AJ
Sample : M1286-09
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
JJ_BH_02_0-1


Manual Integrations
APPROVED

Ankita
2/3/2021 4:34:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 02:55:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 04:07:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

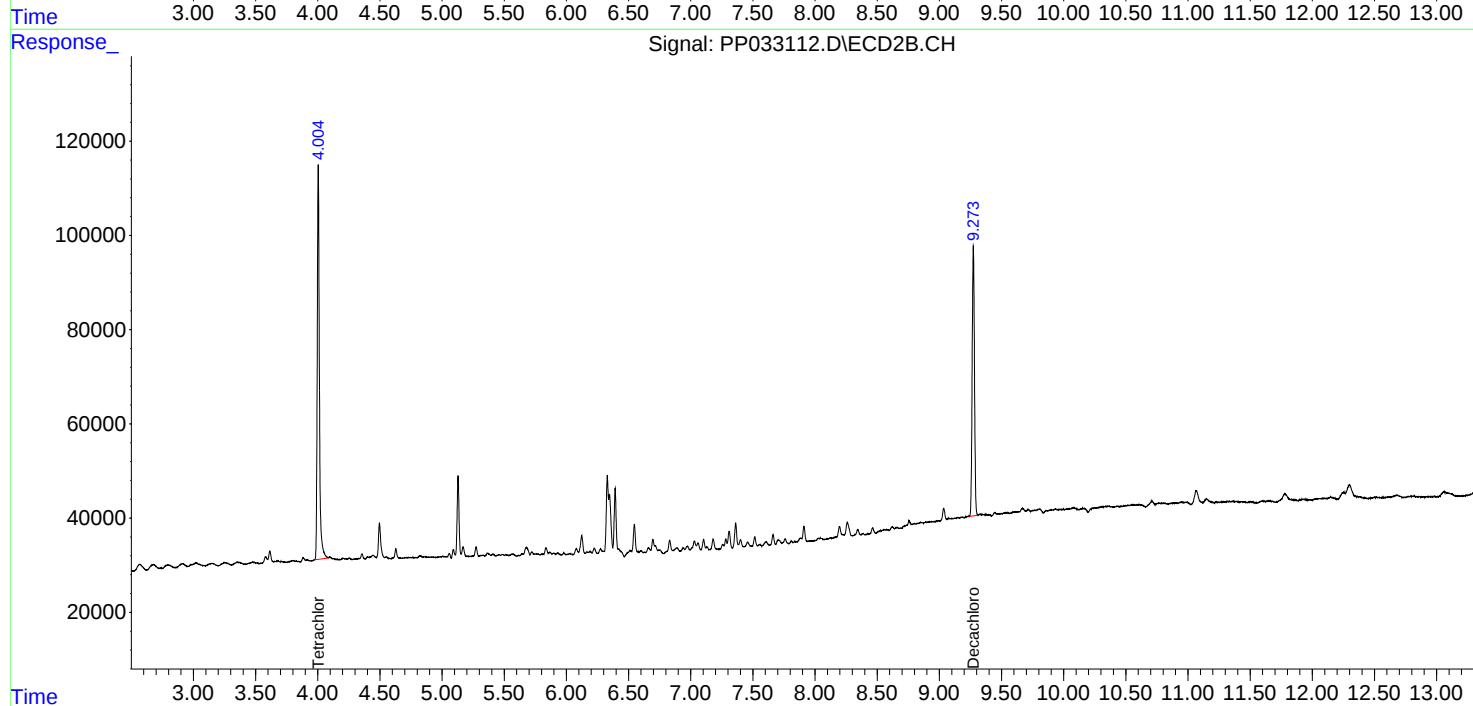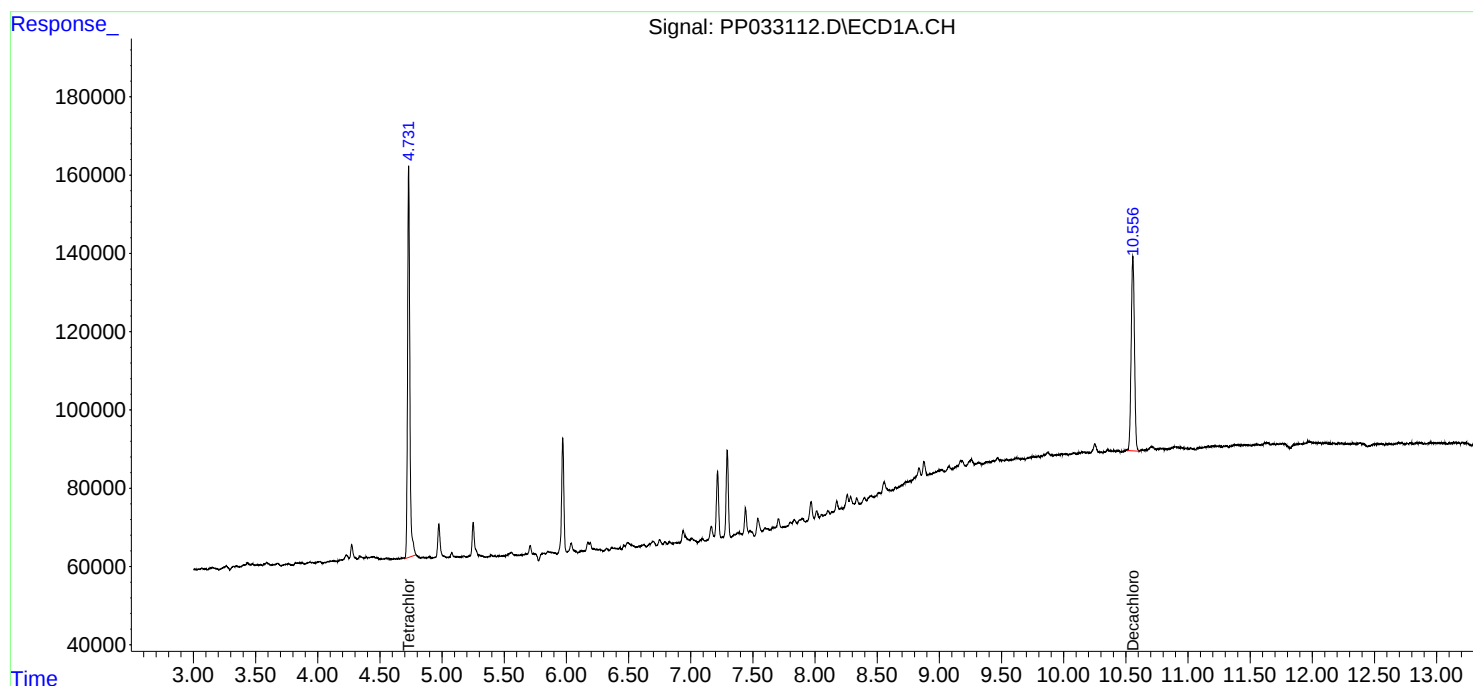

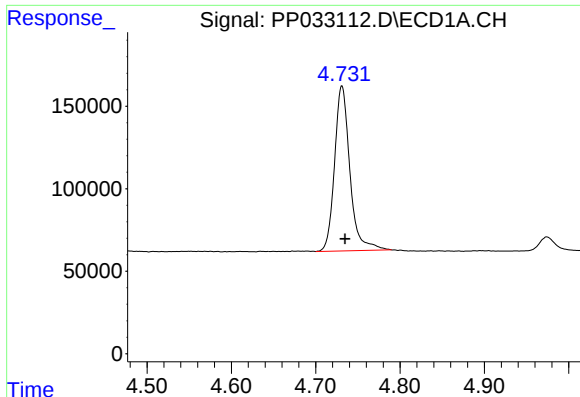


#1 Tetrachloro-m-xylene

R.T.: 4.731 min
Delta R.T.: -0.004 min
Response: 1264220
Conc: 22.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
JJ_BH_02_0-1


Manual Integrations
APPROVED

Ankita
2/3/2021 4:34:42 PM

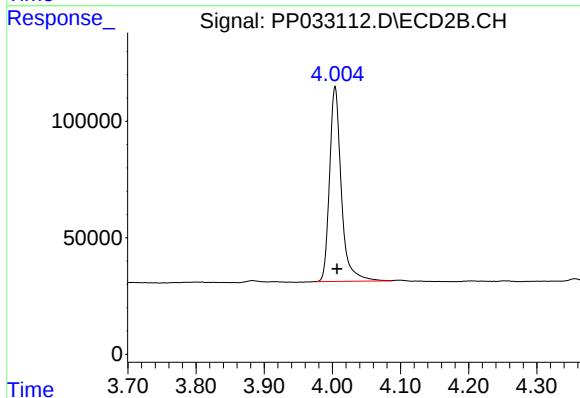


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: -0.003 min
Response: 1001231
Conc: 21.78 ng/ml

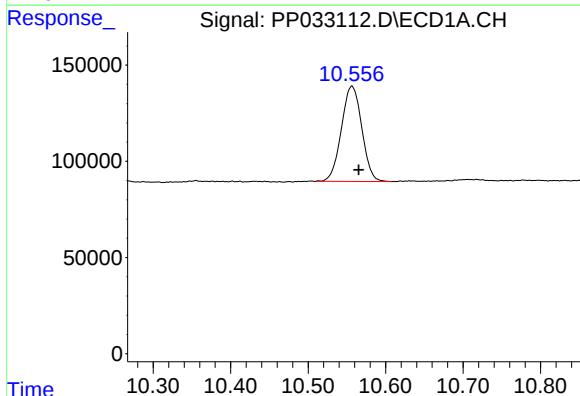

#2 Decachlorobiphenyl

R.T.: 10.557 min
Delta R.T.: -0.009 min
Response: 908483
Conc: 25.32 ng/ml

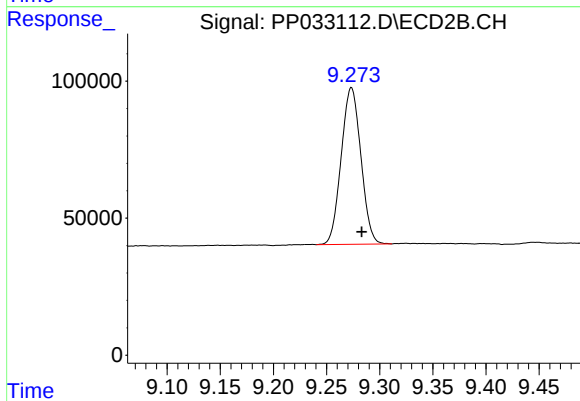

#2 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: -0.010 min
Response: 737014
Conc: 22.43 ng/ml