

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012921\
 Data File : PP033114.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jan 2021 3:35
 Operator : DD\AJ
 Sample : M1286-13
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JJ_BH_02_4-6

Manual Integrations
 APPROVED

Ankita
 2/3/2021 4:34:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:56:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 04:07:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.731	4.004	1012544	923149	17.832m	20.081
2) SA Decachlor...	10.557	9.274	884030	744795	24.640	22.666

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012921\
Data File : PP033114.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jan 2021 3:35
Operator : DD\AJ
Sample : M1286-13
Misc :
ALS Vial : 49 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
JJ_BH_02_4-6


Manual Integrations
APPROVED

Ankita
2/3/2021 4:34:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:56:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 04:07:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

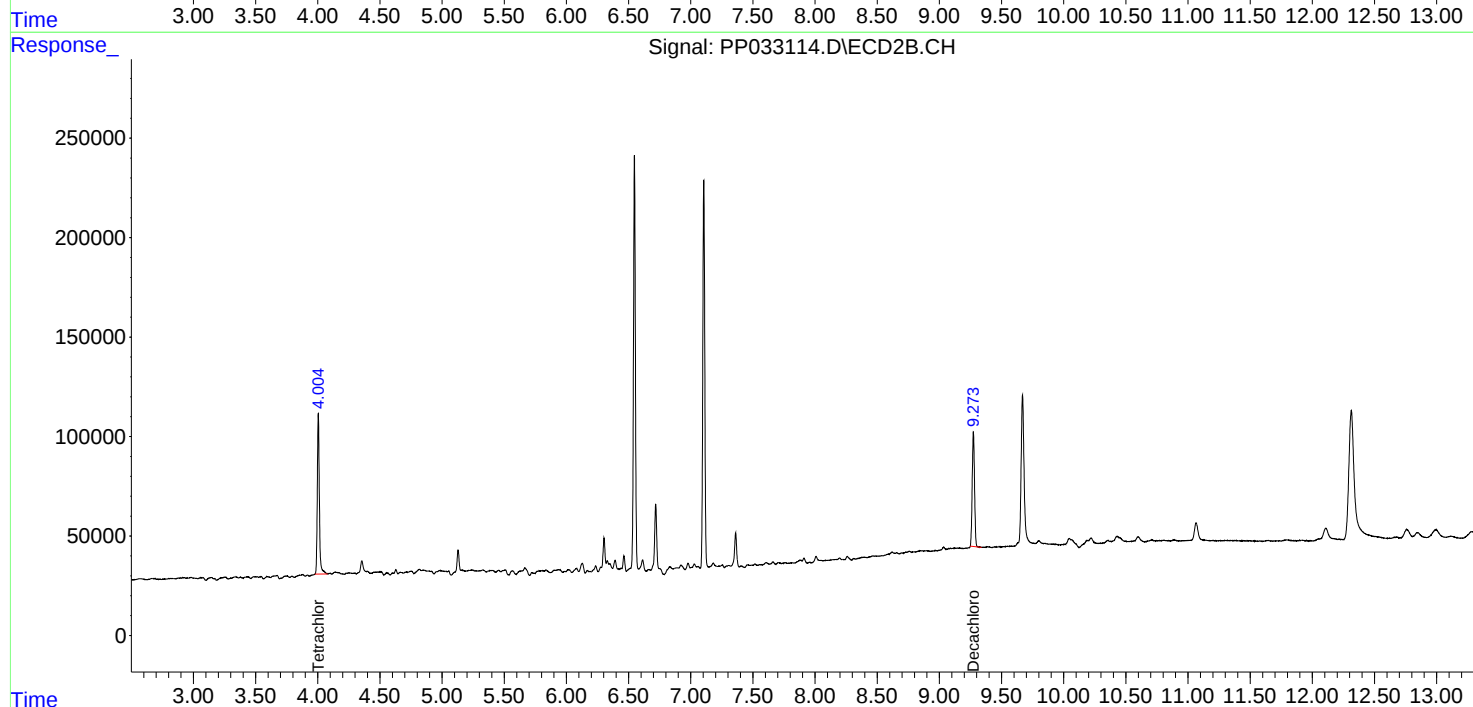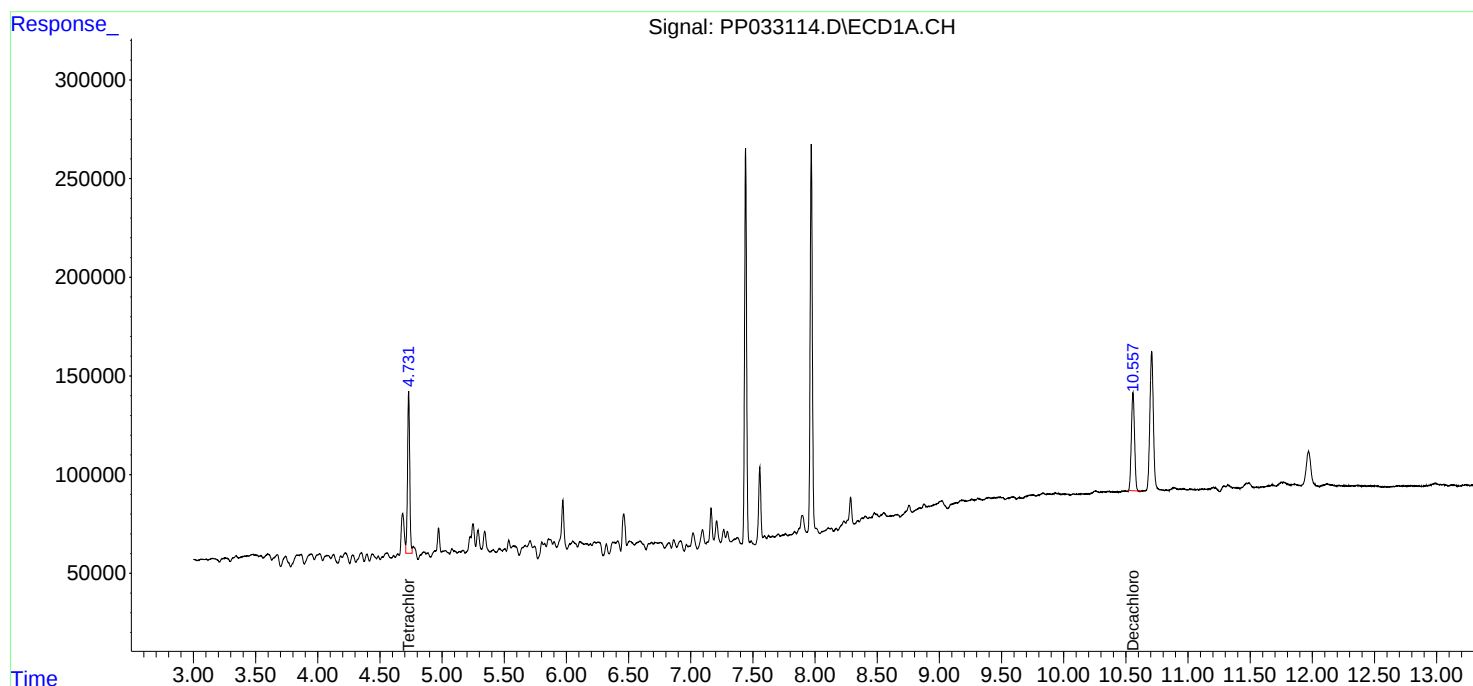

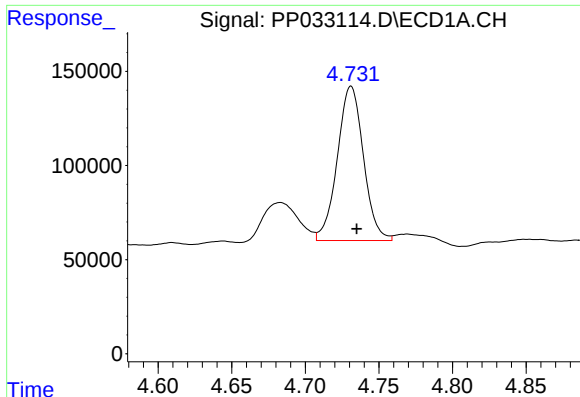

#1 Tetrachloro-m-xylene

R.T.: 4.731 min

Delta R.T.: -0.004 min


Response: 1012544

Conc: 17.83 ng/ml m

Instrument :
ECD_P
ClientSampleId :
JJ_BH_02_4-6

Manual Integrations
APPROVED

Ankita
2/3/2021 4:34:44 PM

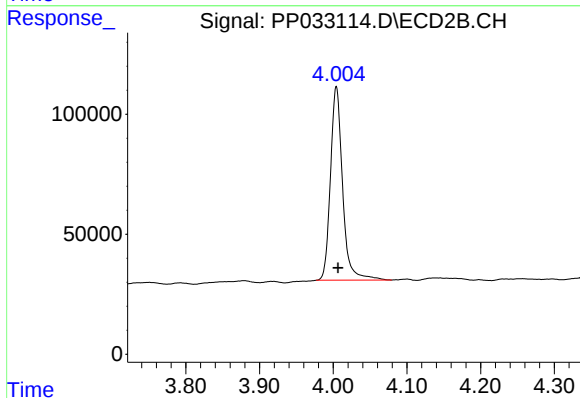


#1 Tetrachloro-m-xylene

R.T.: 4.004 min

Delta R.T.: -0.002 min

Response: 923149

Conc: 20.08 ng/ml

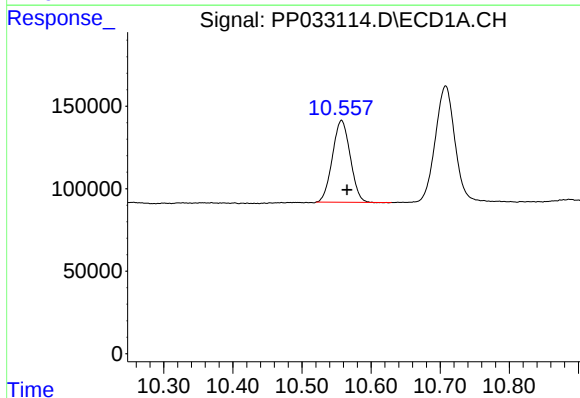


#2 Decachlorobiphenyl

R.T.: 10.557 min

Delta R.T.: -0.008 min

Response: 884030

Conc: 24.64 ng/ml

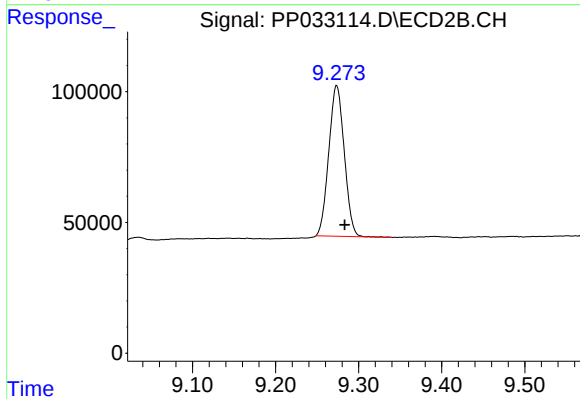

#2 Decachlorobiphenyl

R.T.: 9.274 min

Delta R.T.: -0.010 min

Response: 744795

Conc: 22.67 ng/ml