

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
 Data File : PP069306.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2025 10:55
 Operator : YP\AJ
 Sample : Q1168-07
 Misc : AR1248 LOD 25 PPB
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 12:01:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.536	3.840	27734374	17913570	19.375	20.070
2)	SA Decachlor...	10.280	8.911	21802138	24688934	19.949	22.074
Target Compounds							
3)	L1 AR-1016-1	5.691	4.933	1466687	584451	31.655	17.920 #
4)	L1 AR-1016-2	5.710	4.953	1122886	574055	16.543	12.769
5)	L1 AR-1016-3	5.773	5.132	1006860	463768	23.637	18.637
6)	L1 AR-1016-4	5.872	5.172	1059914	819448	30.283	40.574 #
7)	L1 AR-1016-5	6.163	5.388	1105106	1072098	33.429	39.968
8)	L2 AR-1221-1	4.736	4.045	914818	26704	48.099	2.168 #
9)	L2 AR-1221-2	4.836	4.144	543895	564733	39.722	58.320 #
10)	L2 AR-1221-3	4.836f	4.172f	543895	112750	12.967	3.865 #
11)	L3 AR-1232-1	4.836f	4.172f	543895	112750	16.336	4.802 #
12)	L3 AR-1232-2	0.000	4.953	0	574055	N.D.	24.353 #
13)	L3 AR-1232-3	5.710	5.132	1122886	463768	32.681	35.820
14)	L3 AR-1232-4	5.872	5.215	1059914	907945	59.492	81.898 #
15)	L3 AR-1232-5	5.963	5.388	1111056	1072098	96.930	87.803
16)	L4 AR-1242-1	5.691	4.933	1466687	584451	35.168	20.271 #
17)	L4 AR-1242-2	5.710	4.953	1122886	574055	19.035	14.571
18)	L4 AR-1242-3	5.773	5.132	1006860	463768	27.140	20.608
19)	L4 AR-1242-4	5.872	5.215	1059914	907945	32.320	42.069 #
20)	L4 AR-1242-5	6.605	5.741	1457192	1428471	44.721	49.654
21)	L5 AR-1248-1	5.691	4.933	1466687	584451	45.214	26.553 #
22)	L5 AR-1248-2	5.963	5.172	1111056	819448	26.176	27.256
23)	L5 AR-1248-3	6.163	5.215	1105106	907945	23.519	29.303
24)	L5 AR-1248-4	6.565	5.388	1551986	1072098	28.156	29.020
25)	L5 AR-1248-5	6.605	5.783	1457192	1066730	27.297	28.530
26)	L6 AR-1254-1	6.540	5.741	1059263	1428471	18.306	25.946 #
27)	L6 AR-1254-2	6.760	5.891	1550614	536506	19.324	11.092 #
28)	L6 AR-1254-3	7.124	6.296	1256104	713377	14.902	9.399 #
29)	L6 AR-1254-4	7.406	6.525	1141771	832112	16.744	16.236
30)	L6 AR-1254-5	0.000	6.944	0	109987	N.D.	1.652 #
31)	L7 AR-1260-1	7.337f	6.441	583786	179786	9.990	3.728 #
32)	L7 AR-1260-2	7.548	6.610	939985	370752	12.080	6.048 #
33)	L7 AR-1260-3	0.000	6.771	0	1372426	N.D.	22.814 #
36)	L8 AR-1262-1	0.000	6.944f	0	109987	N.D.	1.549 #
38)	L8 AR-1262-3	0.000	7.799	0	435971	N.D.	8.336 #
39)	L8 AR-1262-4	0.000	7.829	0	232962	N.D.	2.520 #
40)	L8 AR-1262-5	0.000	8.325	0	66853	N.D.	1.399 #
41)	L9 AR-1268-1	0.000	7.799	0	435971	N.D.	3.004 #
42)	L9 AR-1268-2	0.000	7.829	0	232962	N.D.	1.754 #
43)	L9 AR-1268-3	0.000	8.055	0	104452	N.D.	0.918 #
44)	L9 AR-1268-4	0.000	8.325	0	66853	N.D.	1.284 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
Data File : PP069306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2025 10:55
Operator : YP\AJ
Sample : Q1168-07
Misc : AR1248 LOD 25 PPB
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 12:01:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
45) L9	AR-1268-5	0.000	8.637	0	244838	N.D.	0.687 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
Data File : PP069306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2025 10:55
Operator : YP\AJ
Sample : Q1168-07
Misc : AR1248 LOD 25 PPB
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 12:01:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

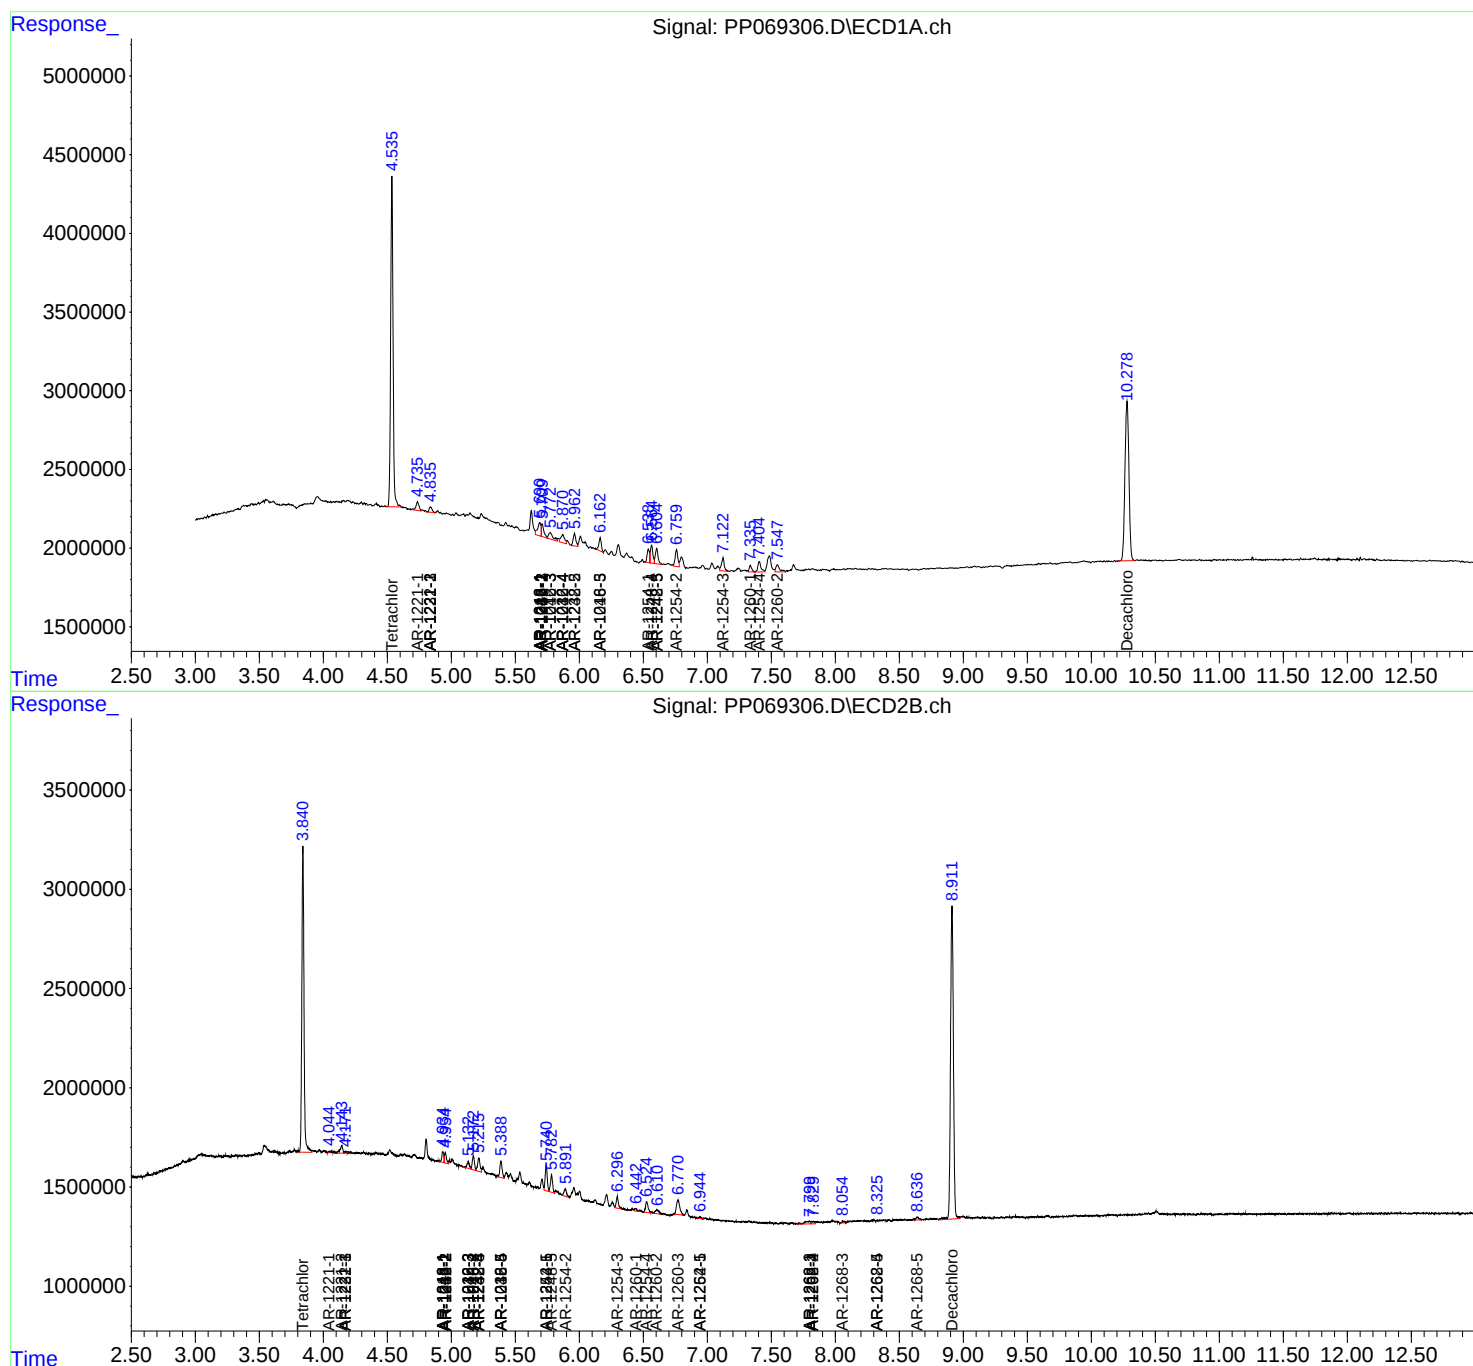


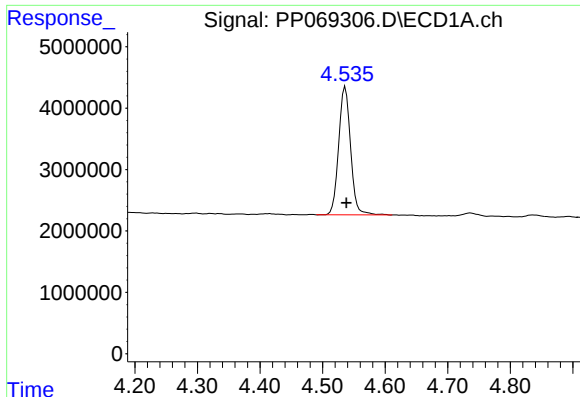

#1 Tetrachloro-m-xylene


R.T.: 4.536 min
Delta R.T.: -0.002 min
Response: 27734374
Conc: 19.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

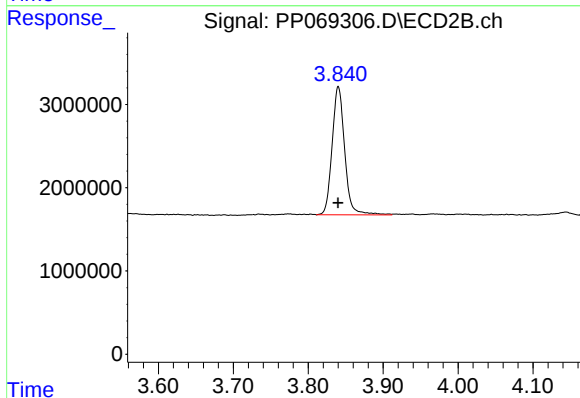


#1 Tetrachloro-m-xylene

R.T.: 3.840 min
Delta R.T.: 0.000 min
Response: 17913570
Conc: 20.07 ng/ml

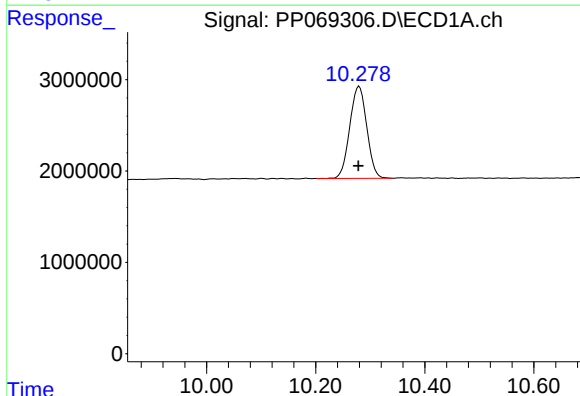


#2 Decachlorobiphenyl

R.T.: 10.280 min
Delta R.T.: 0.001 min
Response: 21802138
Conc: 19.95 ng/ml

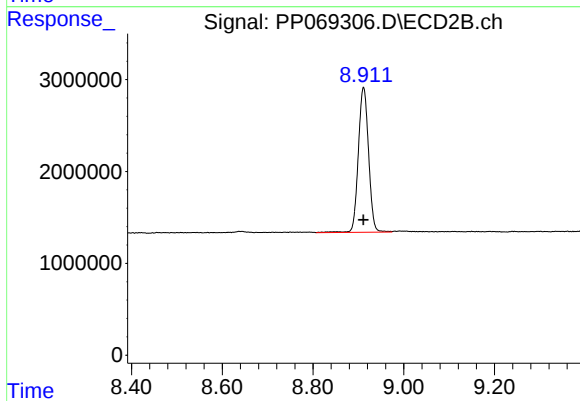

#2 Decachlorobiphenyl


R.T.: 8.911 min
Delta R.T.: 0.000 min
Response: 24688934
Conc: 22.07 ng/ml

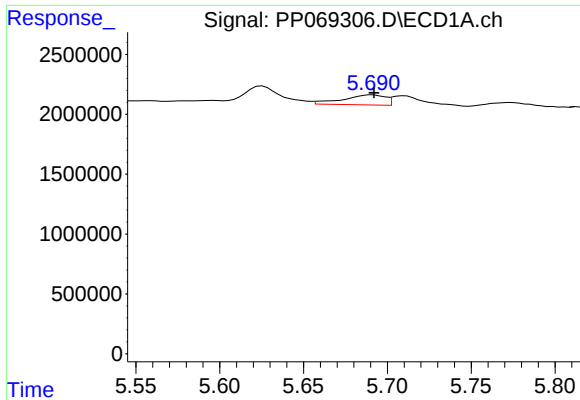

#3 AR-1016-1


R.T.: 5.691 min
Delta R.T.: 0.000 min
Response: 1466687
Conc: 31.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

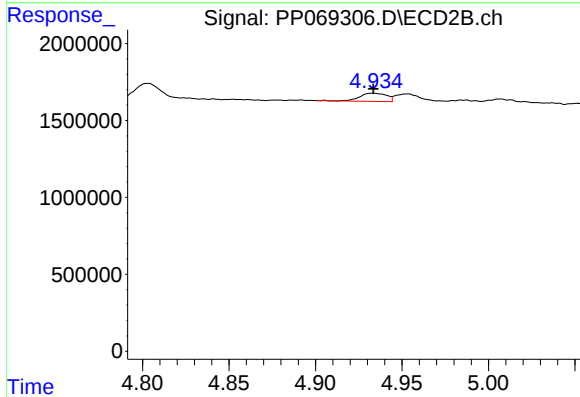


#3 AR-1016-1

R.T.: 4.933 min
Delta R.T.: 0.000 min
Response: 584451
Conc: 17.92 ng/ml

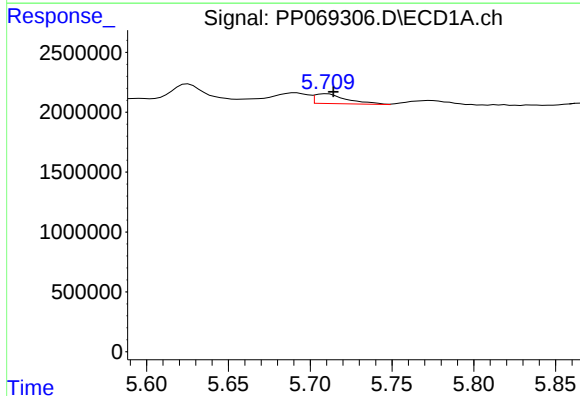


#4 AR-1016-2

R.T.: 5.710 min
Delta R.T.: -0.004 min
Response: 1122886
Conc: 16.54 ng/ml

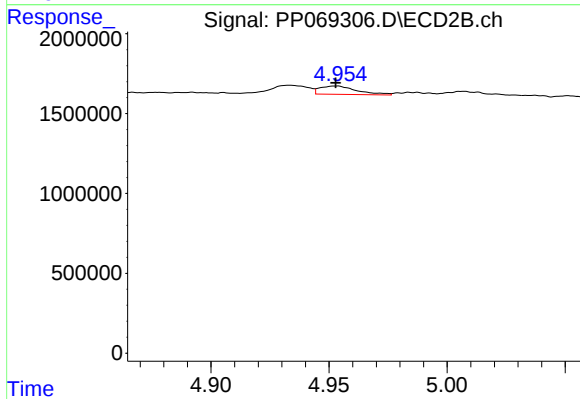

#4 AR-1016-2


R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 574055
Conc: 12.77 ng/ml

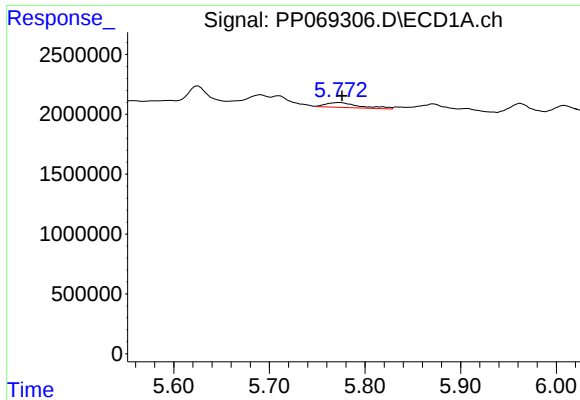

#5 AR-1016-3


R.T.: 5.773 min
Delta R.T.: -0.003 min
Response: 1006860
Conc: 23.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

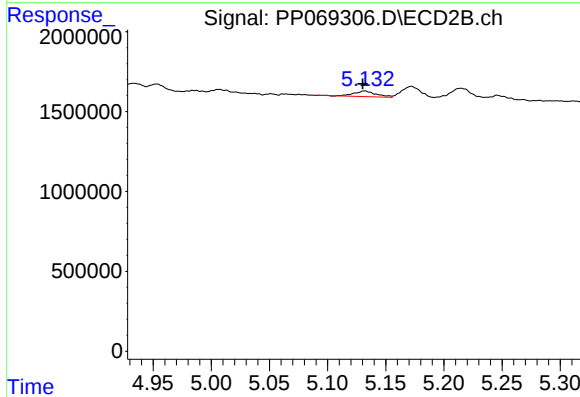


#5 AR-1016-3

R.T.: 5.132 min
Delta R.T.: 0.002 min
Response: 463768
Conc: 18.64 ng/ml

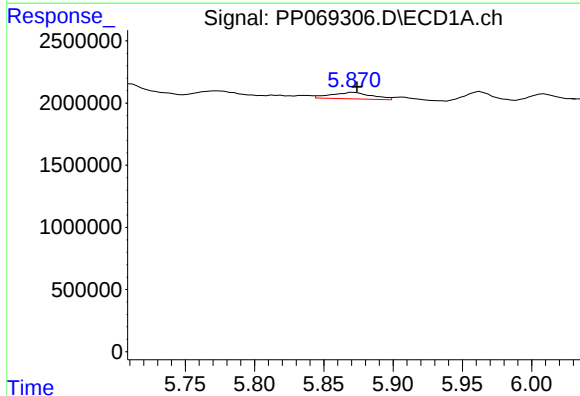


#6 AR-1016-4

R.T.: 5.872 min
Delta R.T.: -0.002 min
Response: 1059914
Conc: 30.28 ng/ml

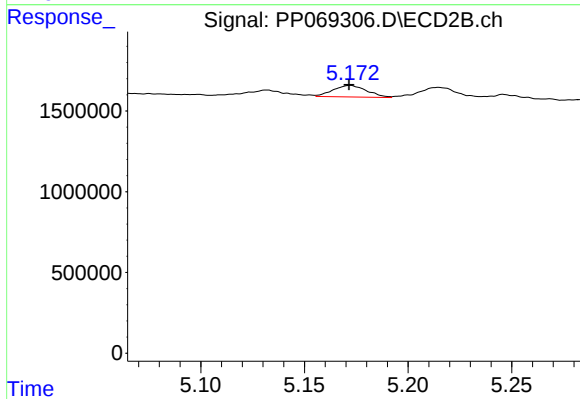

#6 AR-1016-4


R.T.: 5.172 min
Delta R.T.: 0.000 min
Response: 819448
Conc: 40.57 ng/ml

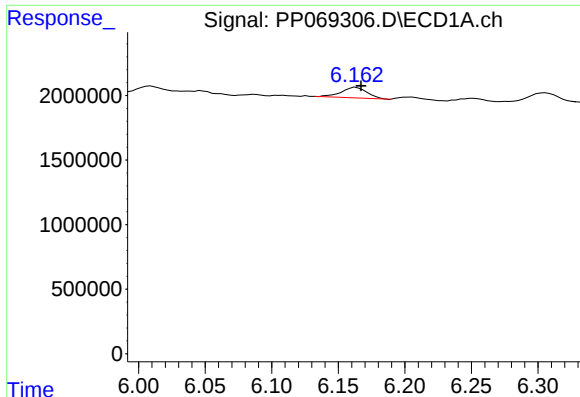

#7 AR-1016-5


R.T.: 6.163 min
Delta R.T.: -0.004 min
Response: 1105106
Conc: 33.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

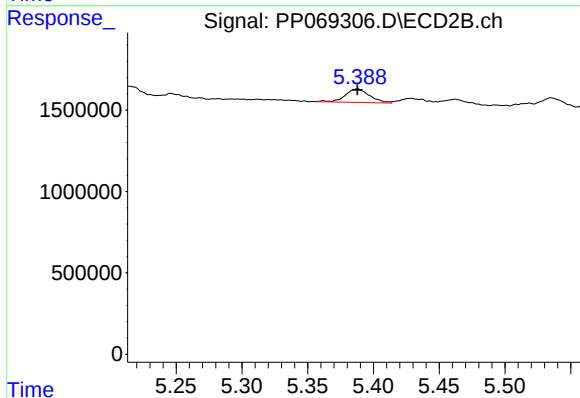


#7 AR-1016-5

R.T.: 5.388 min
Delta R.T.: 0.000 min
Response: 1072098
Conc: 39.97 ng/ml

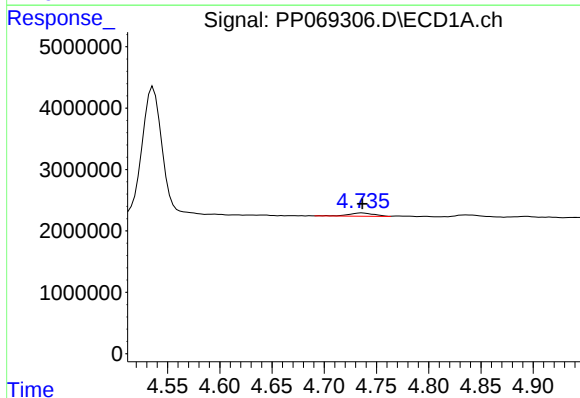


#8 AR-1221-1

R.T.: 4.736 min
Delta R.T.: 0.000 min
Response: 914818
Conc: 48.10 ng/ml

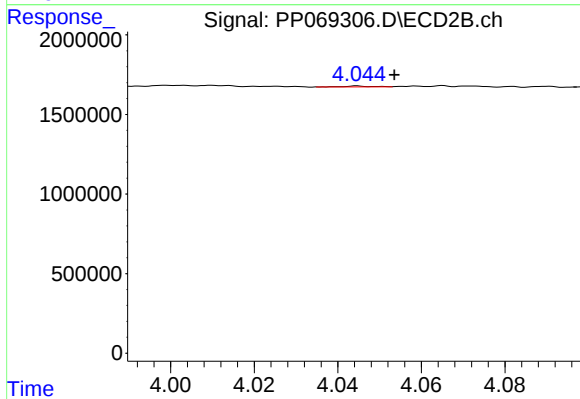

#8 AR-1221-1


R.T.: 4.045 min
Delta R.T.: -0.009 min
Response: 26704
Conc: 2.17 ng/ml

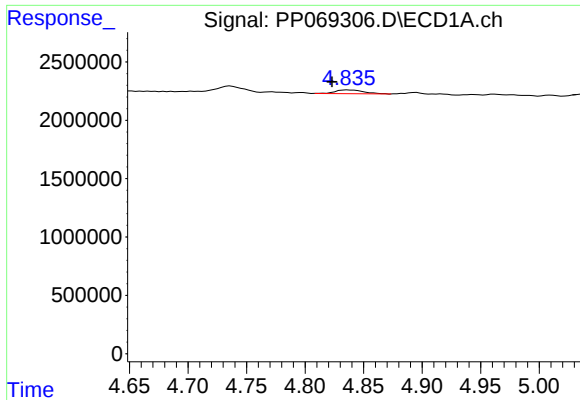

#9 AR-1221-2


R.T.: 4.836 min
Delta R.T.: 0.013 min
Response: 543895
Conc: 39.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

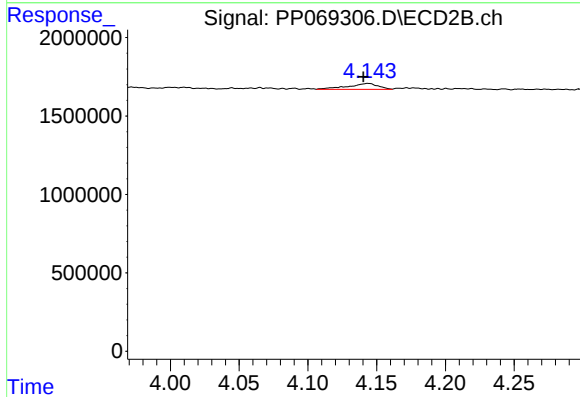


#9 AR-1221-2

R.T.: 4.144 min
Delta R.T.: 0.004 min
Response: 564733
Conc: 58.32 ng/ml

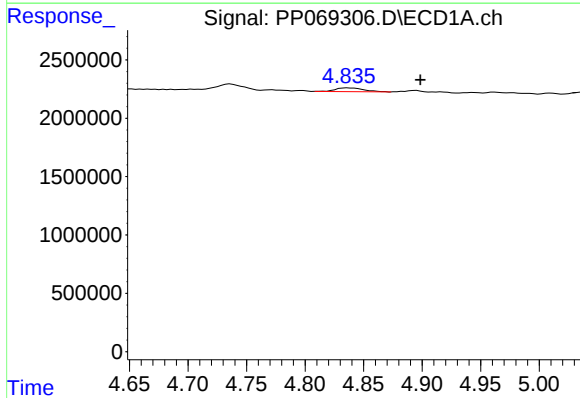


#10 AR-1221-3

R.T.: 4.836 min
Delta R.T.: -0.062 min
Response: 543895
Conc: 12.97 ng/ml

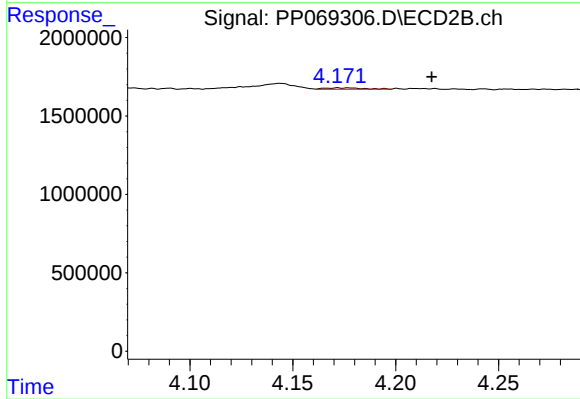

#10 AR-1221-3


R.T.: 4.172 min
Delta R.T.: -0.046 min
Response: 112750
Conc: 3.86 ng/ml

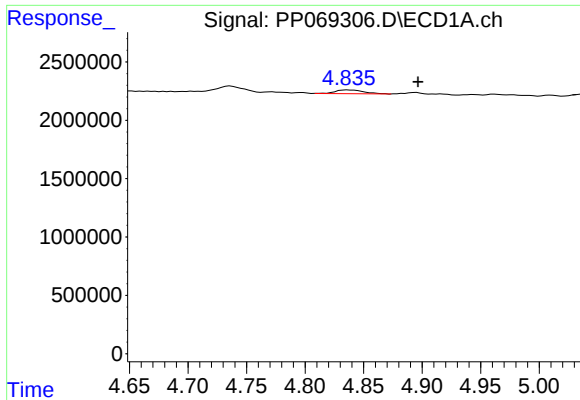

#11 AR-1232-1


R.T.: 4.836 min
Delta R.T.: -0.061 min
Response: 543895
Conc: 16.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

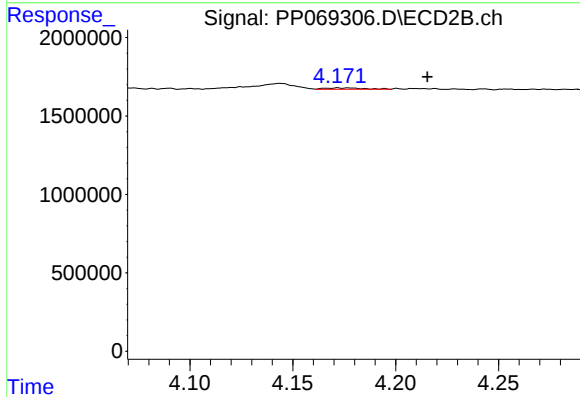


#11 AR-1232-1

R.T.: 4.172 min
Delta R.T.: -0.044 min
Response: 112750
Conc: 4.80 ng/ml

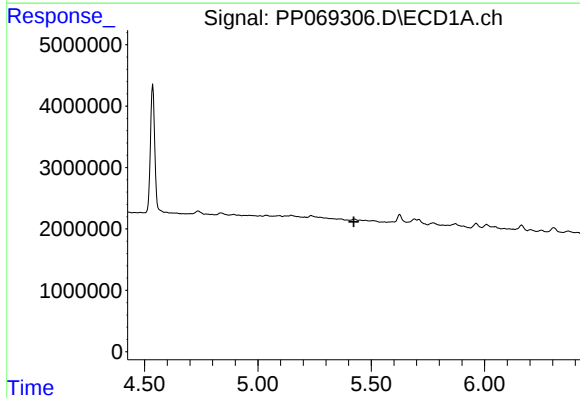


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.424 min
Response: 0
Conc: N.D.

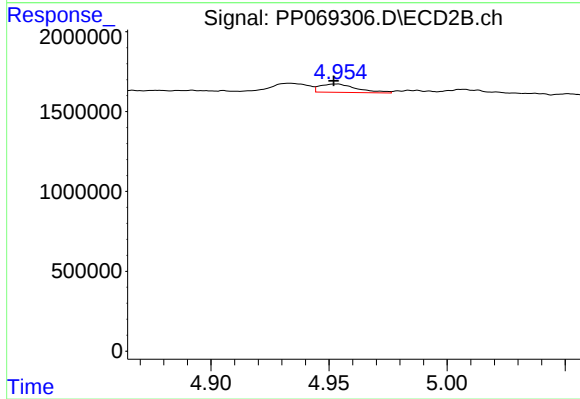

#12 AR-1232-2


R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 574055
Conc: 24.35 ng/ml

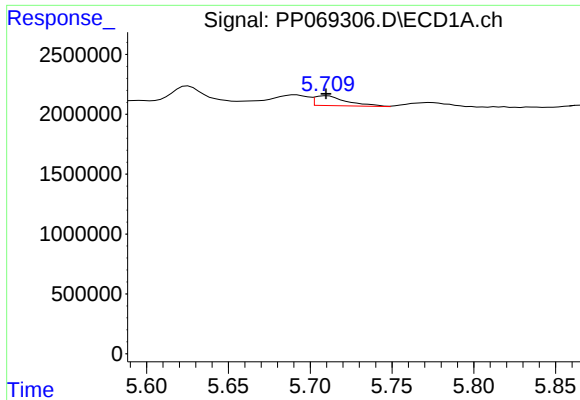

#13 AR-1232-3


R.T.: 5.710 min
Delta R.T.: 0.000 min
Response: 1122886
Conc: 32.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

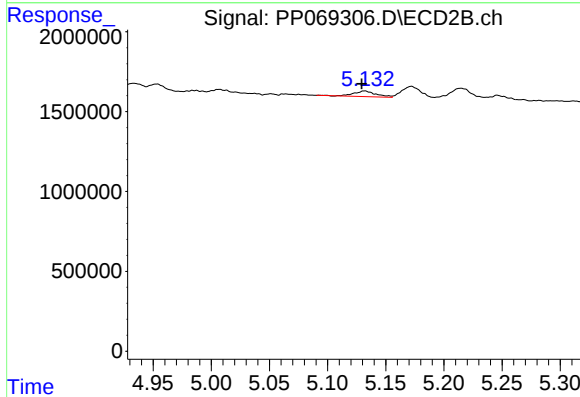


#13 AR-1232-3

R.T.: 5.132 min
Delta R.T.: 0.003 min
Response: 463768
Conc: 35.82 ng/ml

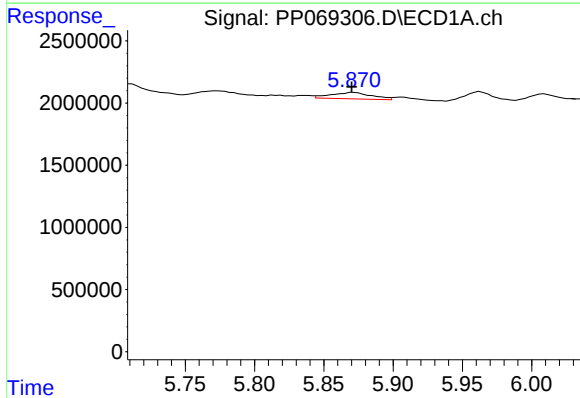


#14 AR-1232-4

R.T.: 5.872 min
Delta R.T.: 0.002 min
Response: 1059914
Conc: 59.49 ng/ml

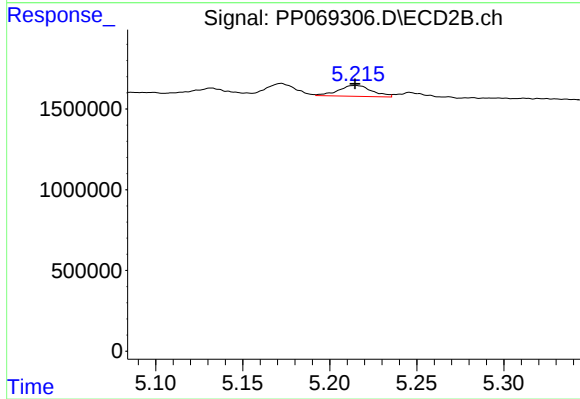

#14 AR-1232-4


R.T.: 5.215 min
Delta R.T.: 0.000 min
Response: 907945
Conc: 81.90 ng/ml

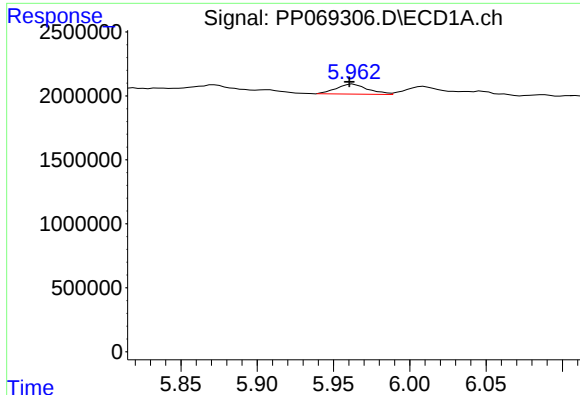

#15 AR-1232-5


R.T.: 5.963 min
Delta R.T.: 0.003 min
Response: 1111056
Conc: 96.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

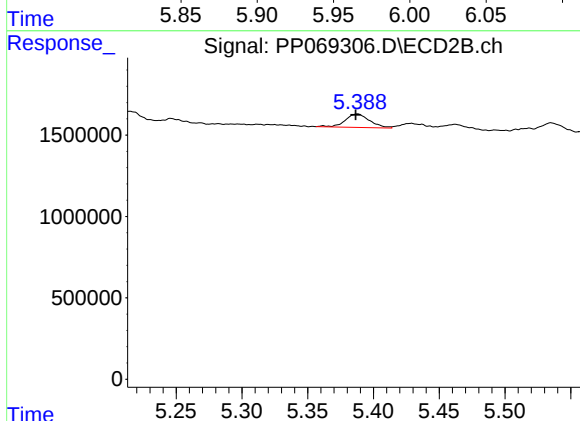


#15 AR-1232-5

R.T.: 5.388 min
Delta R.T.: 0.001 min
Response: 1072098
Conc: 87.80 ng/ml

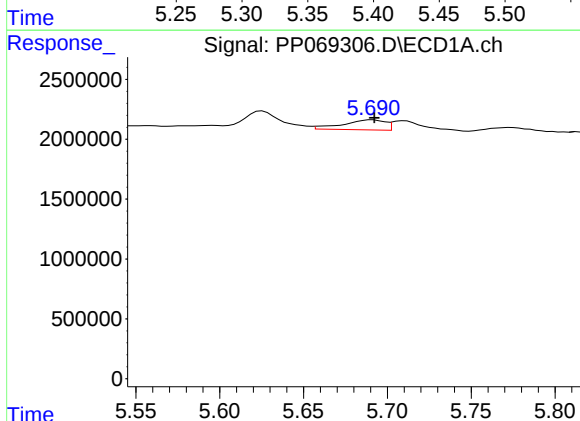


#16 AR-1242-1

R.T.: 5.691 min
Delta R.T.: -0.001 min
Response: 1466687
Conc: 35.17 ng/ml

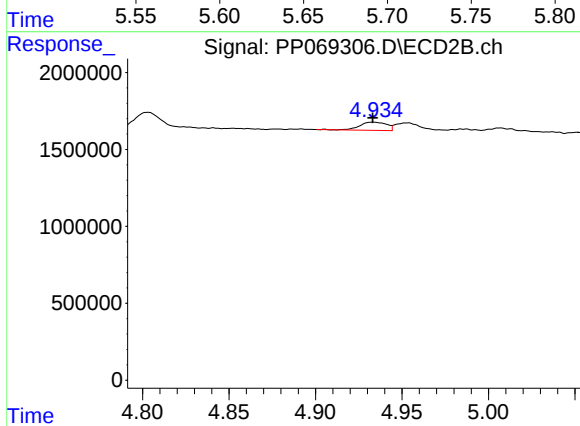

#16 AR-1242-1


R.T.: 4.933 min
Delta R.T.: 0.000 min
Response: 584451
Conc: 20.27 ng/ml

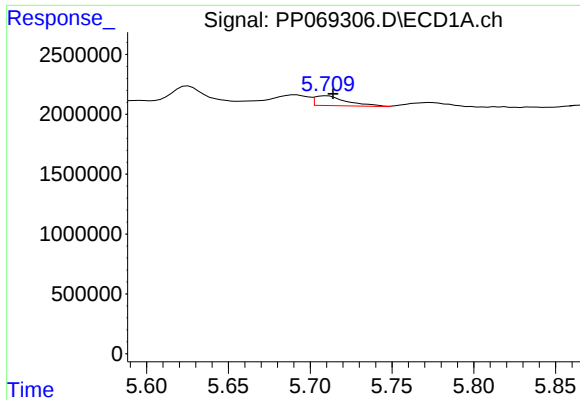

#17 AR-1242-2


R.T.: 5.710 min
Delta R.T.: -0.004 min
Response: 1122886
Conc: 19.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

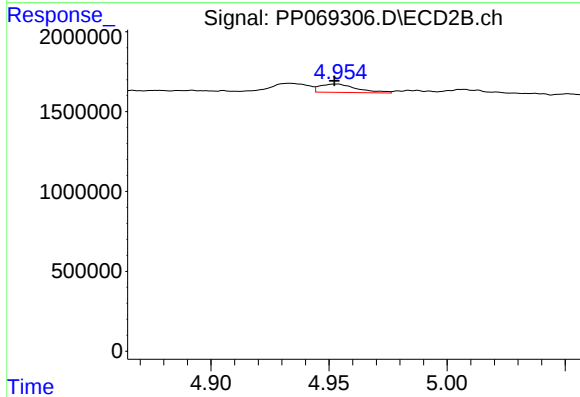


#17 AR-1242-2

R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 574055
Conc: 14.57 ng/ml

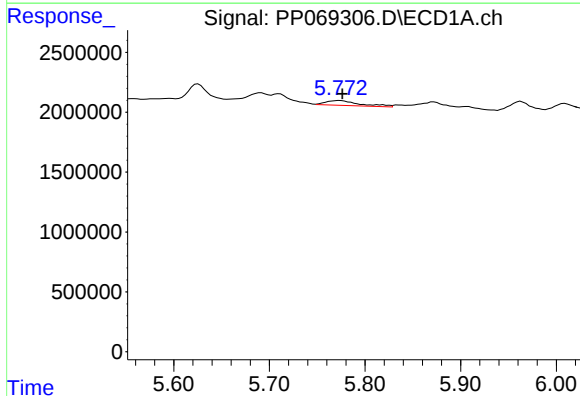


#18 AR-1242-3

R.T.: 5.773 min
Delta R.T.: -0.003 min
Response: 1006860
Conc: 27.14 ng/ml

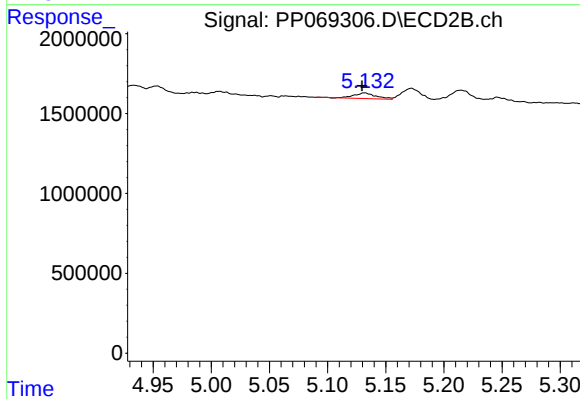

#18 AR-1242-3


R.T.: 5.132 min
Delta R.T.: 0.002 min
Response: 463768
Conc: 20.61 ng/ml

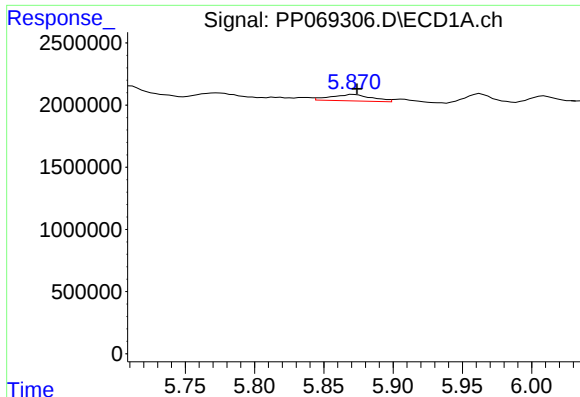

#19 AR-1242-4


R.T.: 5.872 min
Delta R.T.: -0.002 min
Response: 1059914
Conc: 32.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

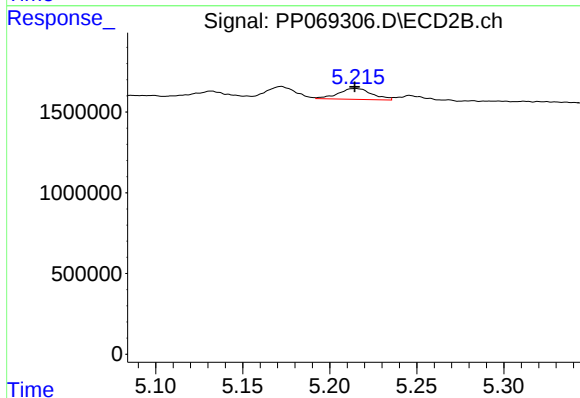


#19 AR-1242-4

R.T.: 5.215 min
Delta R.T.: 0.000 min
Response: 907945
Conc: 42.07 ng/ml

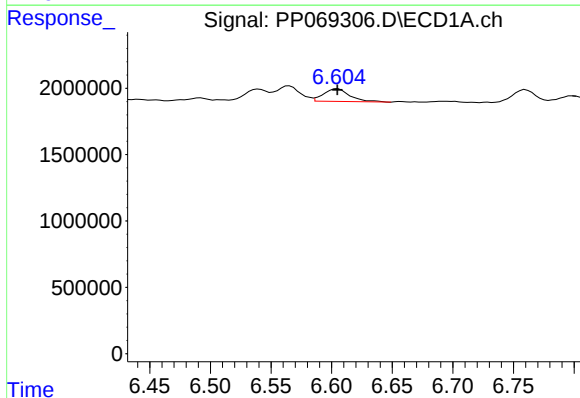


#20 AR-1242-5

R.T.: 6.605 min
Delta R.T.: 0.000 min
Response: 1457192
Conc: 44.72 ng/ml

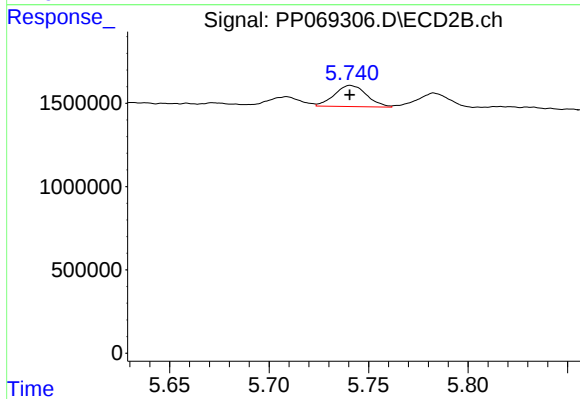

#20 AR-1242-5


R.T.: 5.741 min
Delta R.T.: 0.000 min
Response: 1428471
Conc: 49.65 ng/ml

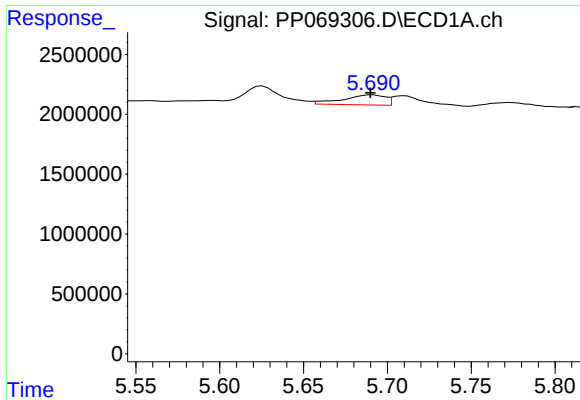

#21 AR-1248-1


R.T.: 5.691 min
Delta R.T.: 0.001 min
Response: 1466687
Conc: 45.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

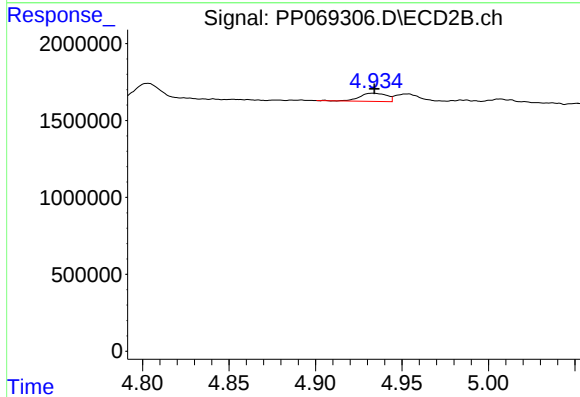


#21 AR-1248-1

R.T.: 4.933 min
Delta R.T.: 0.000 min
Response: 584451
Conc: 26.55 ng/ml

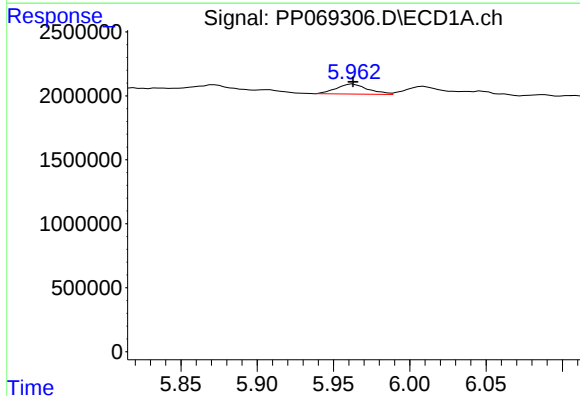


#22 AR-1248-2

R.T.: 5.963 min
Delta R.T.: 0.000 min
Response: 1111056
Conc: 26.18 ng/ml

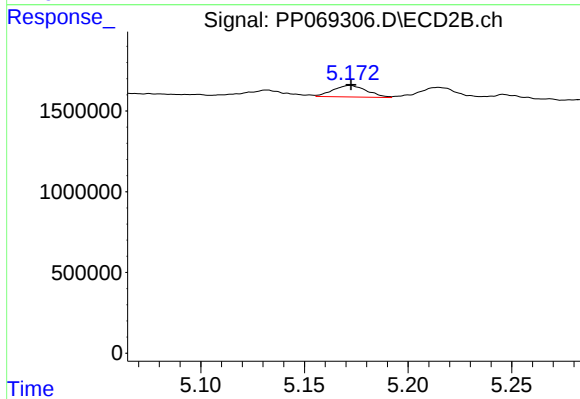

#22 AR-1248-2


R.T.: 5.172 min
Delta R.T.: 0.000 min
Response: 819448
Conc: 27.26 ng/ml

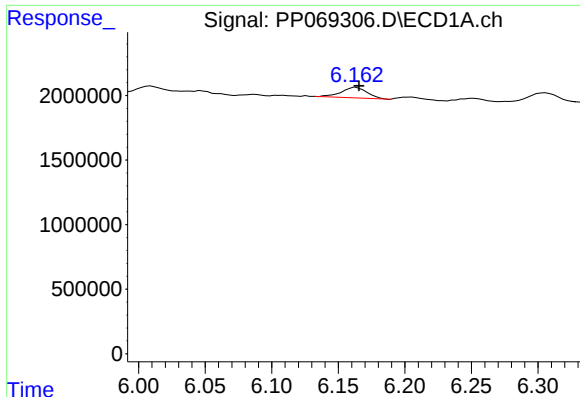

#23 AR-1248-3


R.T.: 6.163 min
Delta R.T.: -0.002 min
Response: 1105106
Conc: 23.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

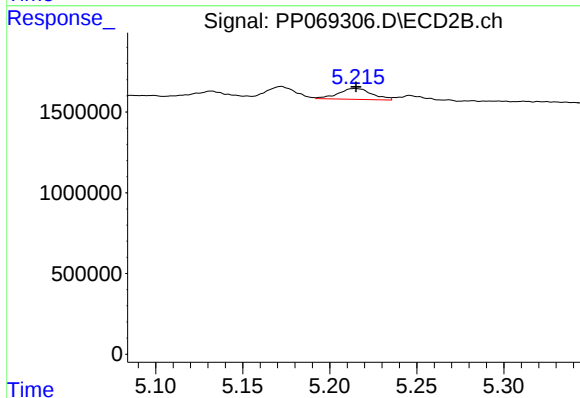


#23 AR-1248-3

R.T.: 5.215 min
Delta R.T.: 0.000 min
Response: 907945
Conc: 29.30 ng/ml

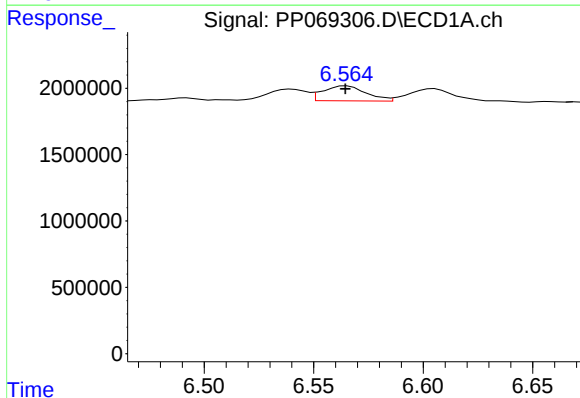


#24 AR-1248-4

R.T.: 6.565 min
Delta R.T.: 0.000 min
Response: 1551986
Conc: 28.16 ng/ml

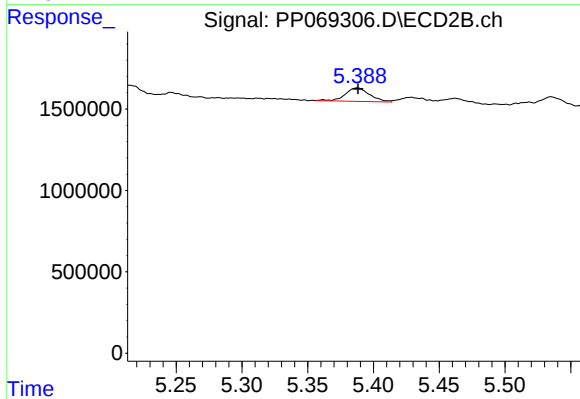

#24 AR-1248-4


R.T.: 5.388 min
Delta R.T.: 0.000 min
Response: 1072098
Conc: 29.02 ng/ml

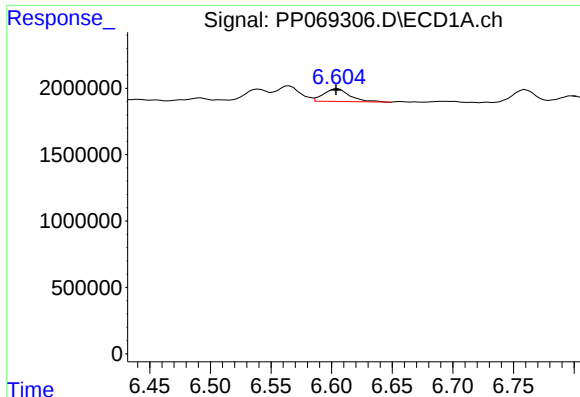

#25 AR-1248-5


R.T.: 6.605 min
Delta R.T.: 0.001 min
Response: 1457192
Conc: 27.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

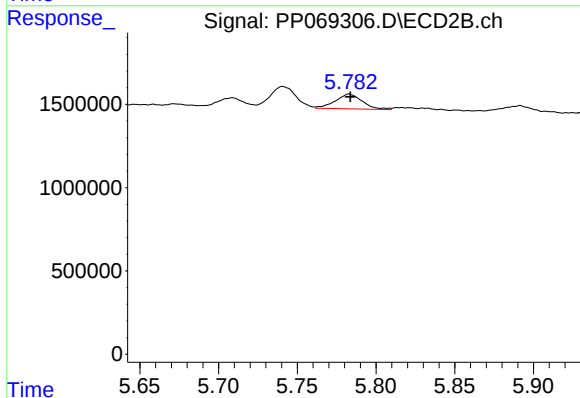


#25 AR-1248-5

R.T.: 5.783 min
Delta R.T.: 0.000 min
Response: 1066730
Conc: 28.53 ng/ml

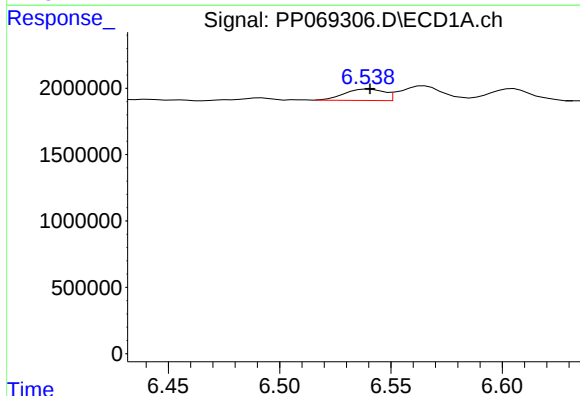


#26 AR-1254-1

R.T.: 6.540 min
Delta R.T.: 0.000 min
Response: 1059263
Conc: 18.31 ng/ml

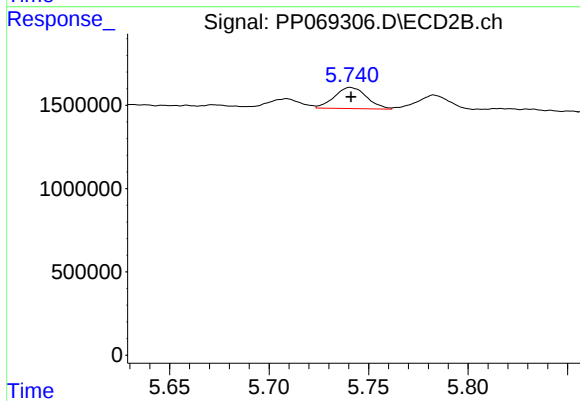

#26 AR-1254-1


R.T.: 5.741 min
Delta R.T.: 0.000 min
Response: 1428471
Conc: 25.95 ng/ml

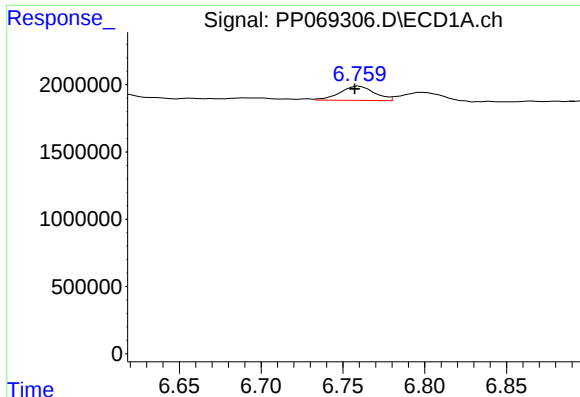

#27 AR-1254-2


R.T.: 6.760 min
Delta R.T.: 0.003 min
Response: 1550614
Conc: 19.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

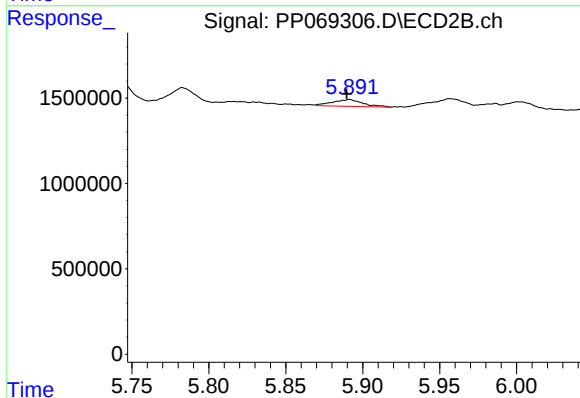


#27 AR-1254-2

R.T.: 5.891 min
Delta R.T.: 0.002 min
Response: 536506
Conc: 11.09 ng/ml

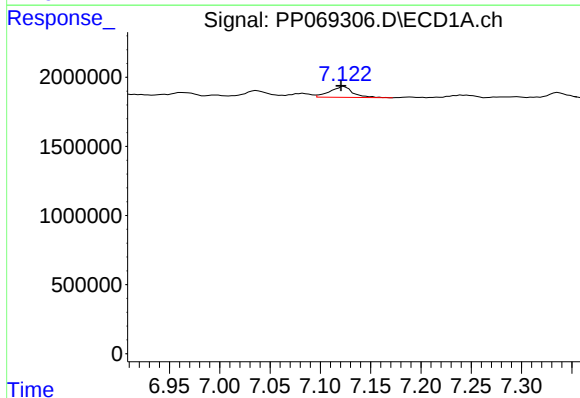


#28 AR-1254-3

R.T.: 7.124 min
Delta R.T.: 0.003 min
Response: 1256104
Conc: 14.90 ng/ml

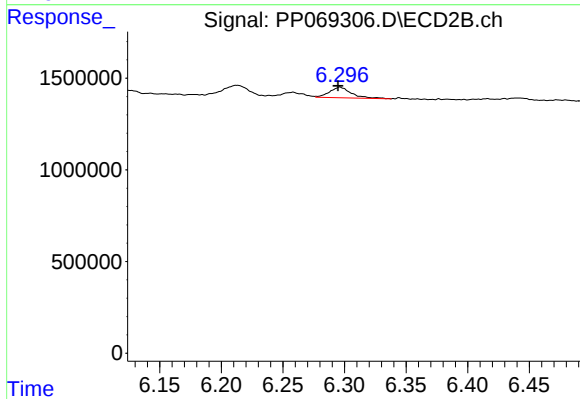

#28 AR-1254-3


R.T.: 6.296 min
Delta R.T.: 0.001 min
Response: 713377
Conc: 9.40 ng/ml

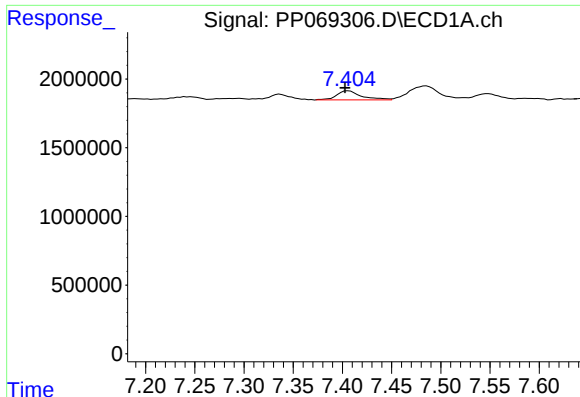

#29 AR-1254-4


R.T.: 7.406 min
Delta R.T.: 0.003 min
Response: 1141771
Conc: 16.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

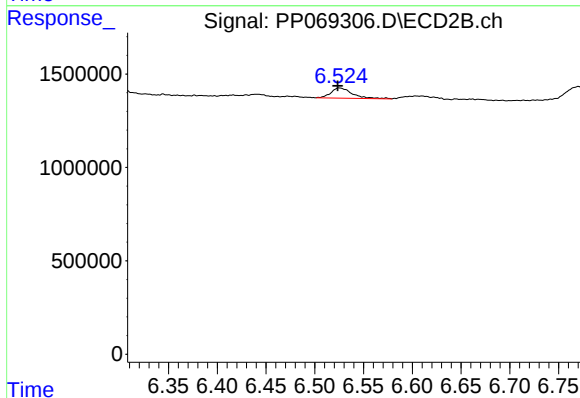


#29 AR-1254-4

R.T.: 6.525 min
Delta R.T.: 0.002 min
Response: 832112
Conc: 16.24 ng/ml

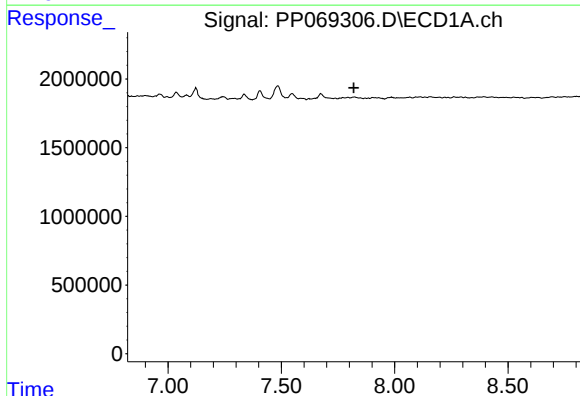


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.820 min
Response: 0
Conc: N.D.

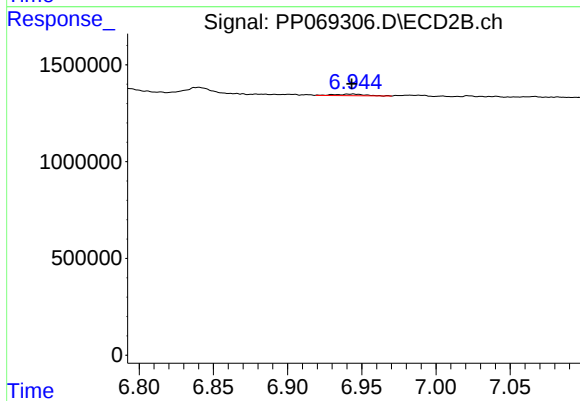

#30 AR-1254-5


R.T.: 6.944 min
Delta R.T.: 0.000 min
Response: 109987
Conc: 1.65 ng/ml

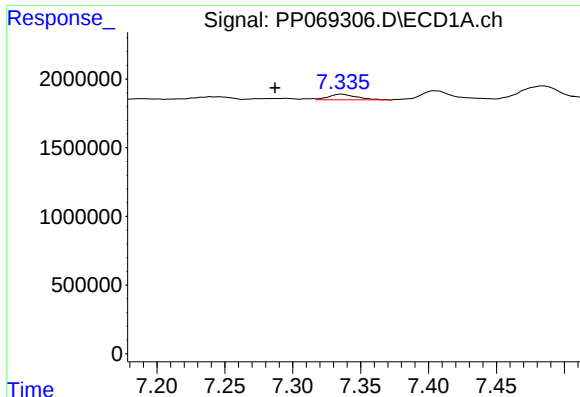

#31 AR-1260-1


R.T.: 7.337 min
Delta R.T.: 0.050 min
Response: 583786
Conc: 9.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

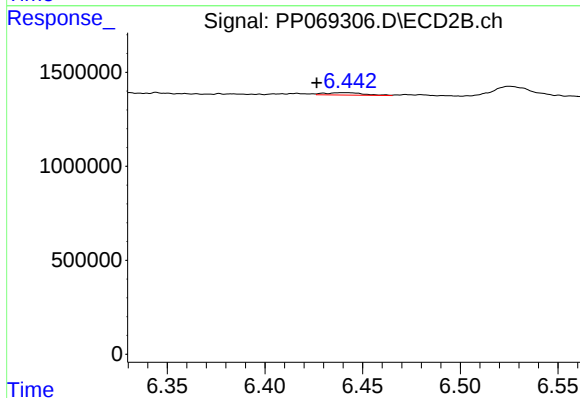


#31 AR-1260-1

R.T.: 6.441 min
Delta R.T.: 0.014 min
Response: 179786
Conc: 3.73 ng/ml

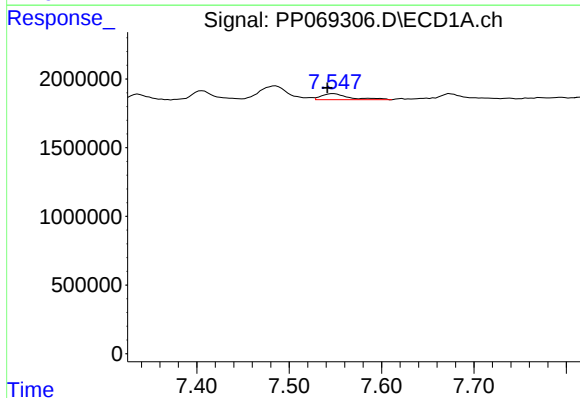


#32 AR-1260-2

R.T.: 7.548 min
Delta R.T.: 0.007 min
Response: 939985
Conc: 12.08 ng/ml

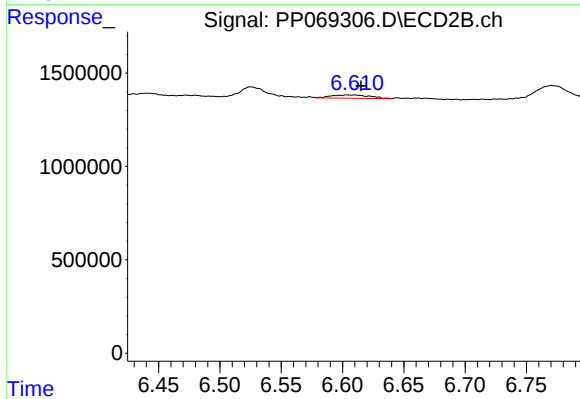

#32 AR-1260-2


R.T.: 6.610 min
Delta R.T.: -0.005 min
Response: 370752
Conc: 6.05 ng/ml

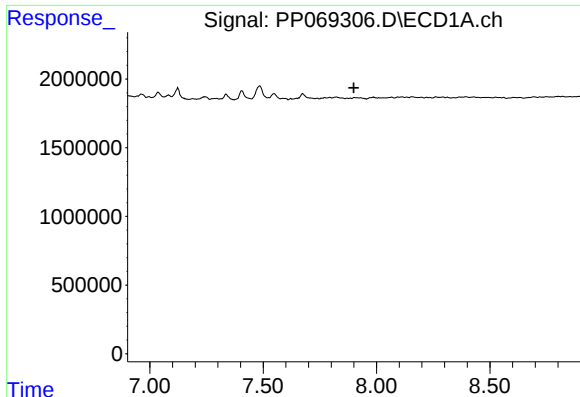

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.900 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

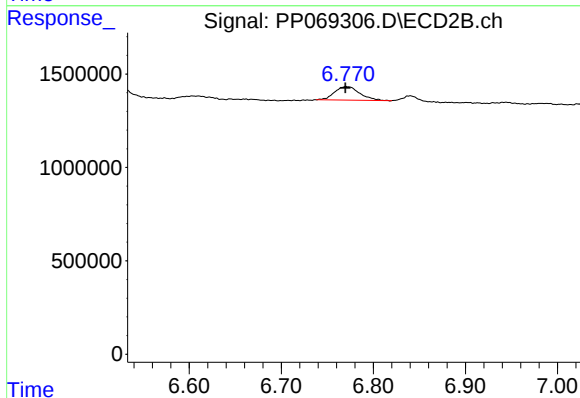


#33 AR-1260-3

R.T.: 6.771 min
Delta R.T.: 0.000 min
Response: 1372426
Conc: 22.81 ng/ml

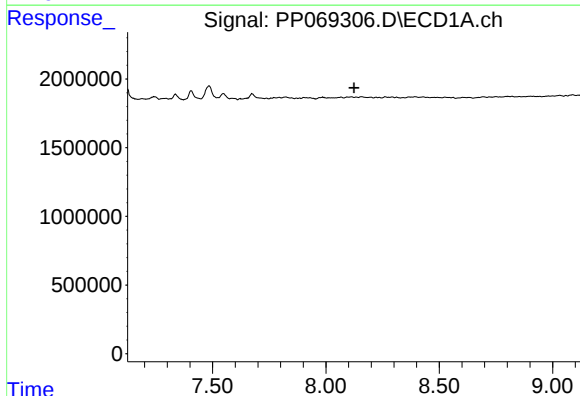


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

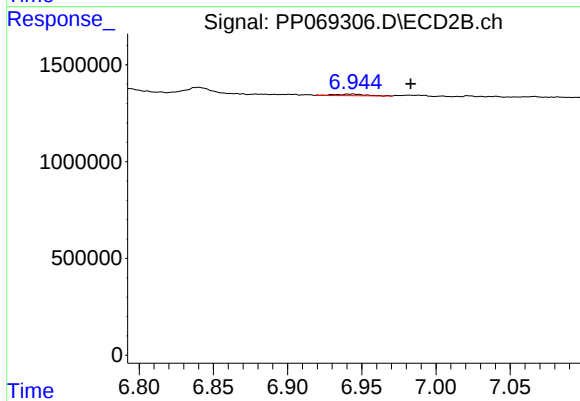

#36 AR-1262-1


R.T.: 6.944 min
Delta R.T.: -0.039 min
Response: 109987
Conc: 1.55 ng/ml

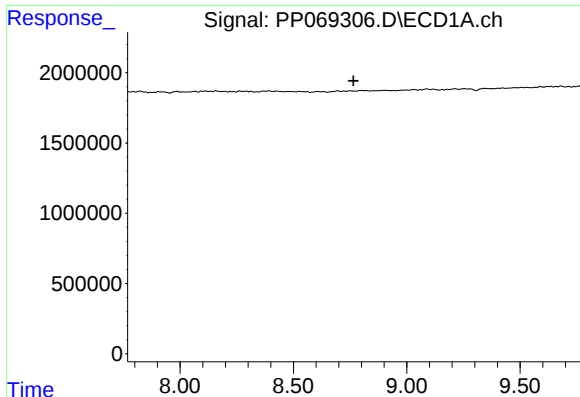

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

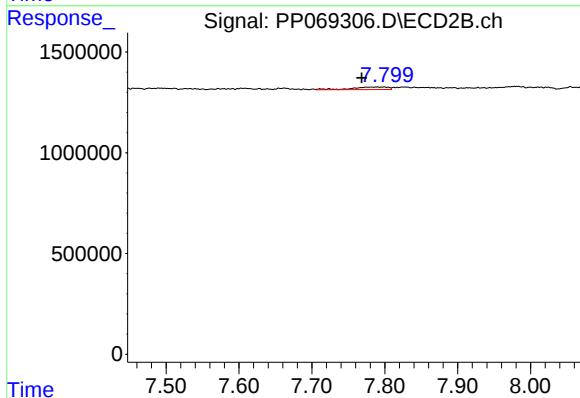


#38 AR-1262-3

R.T.: 7.799 min
Delta R.T.: 0.031 min
Response: 435971
Conc: 8.34 ng/ml

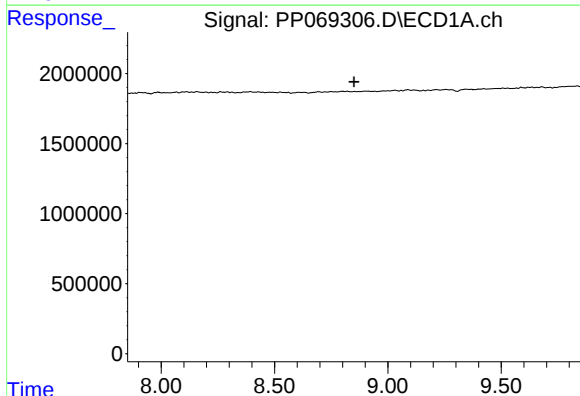


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.852 min
Response: 0
Conc: N.D.

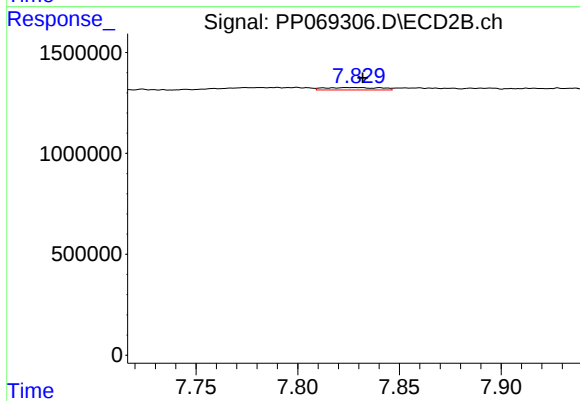

#39 AR-1262-4


R.T.: 7.829 min
Delta R.T.: -0.003 min
Response: 232962
Conc: 2.52 ng/ml

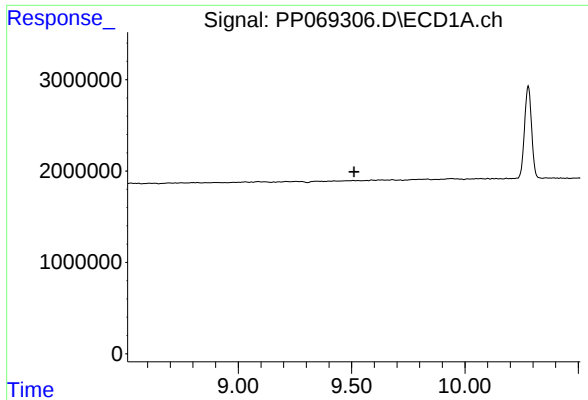

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

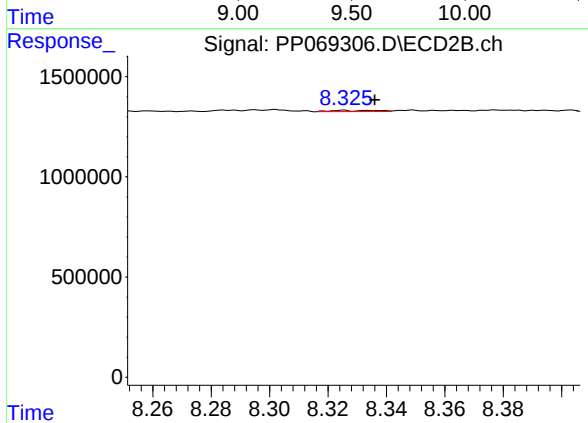


#40 AR-1262-5

R.T.: 8.325 min
Delta R.T.: -0.011 min
Response: 66853
Conc: 1.40 ng/ml

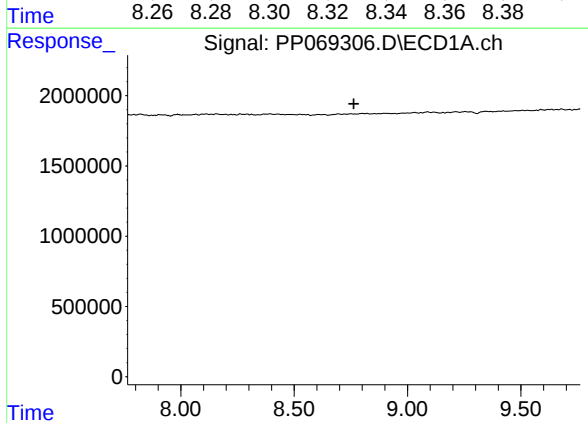


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.763 min
Response: 0
Conc: N.D.

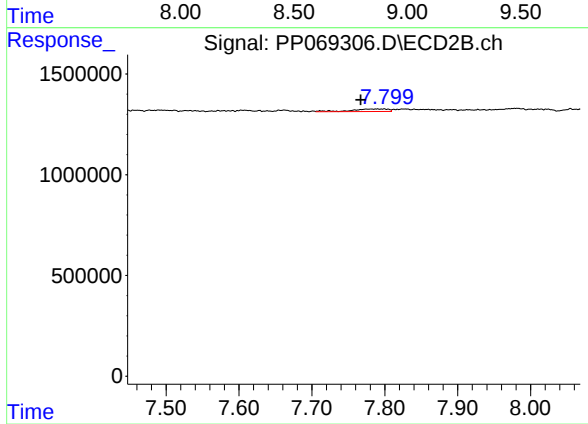

#41 AR-1268-1


R.T.: 7.799 min
Delta R.T.: 0.032 min
Response: 435971
Conc: 3.00 ng/ml

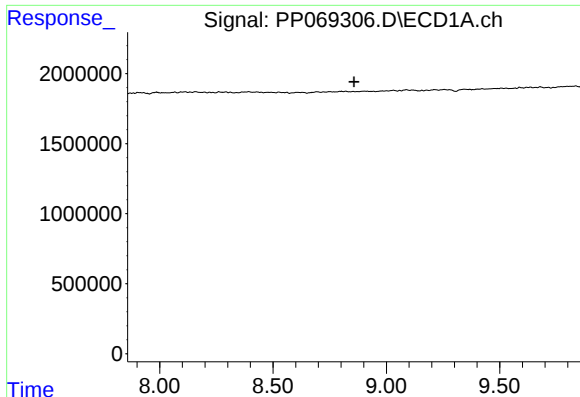

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 8.857 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

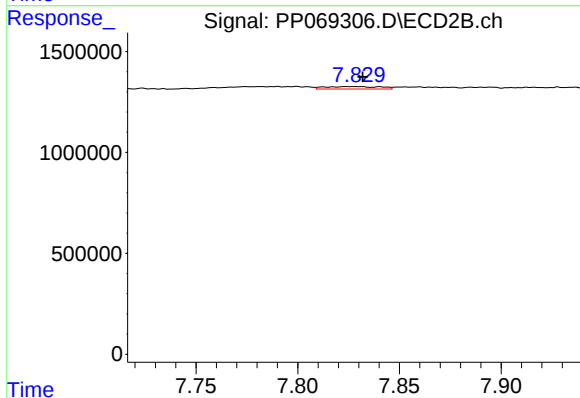


#42 AR-1268-2

R.T.: 7.829 min
Delta R.T.: -0.003 min
Response: 232962
Conc: 1.75 ng/ml

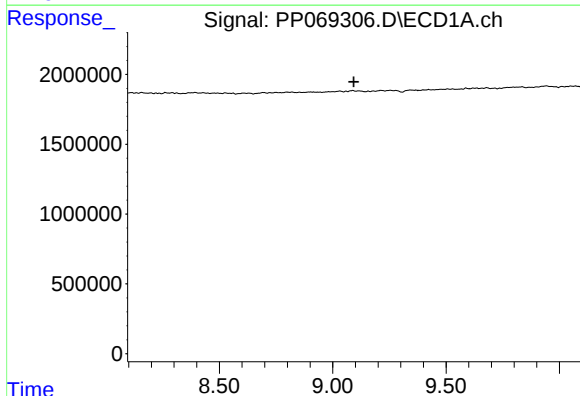


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.093 min
Response: 0
Conc: N.D.

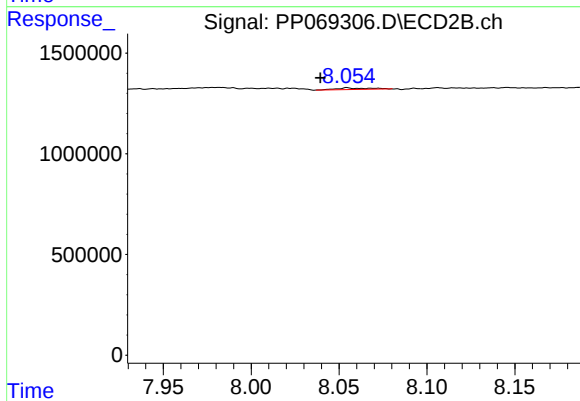

#43 AR-1268-3


R.T.: 8.055 min
Delta R.T.: 0.015 min
Response: 104452
Conc: 0.92 ng/ml

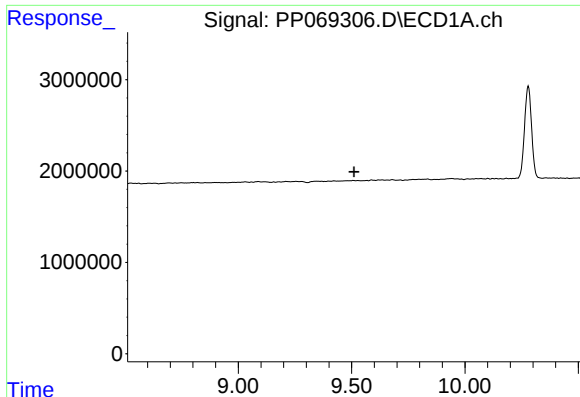

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 9.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

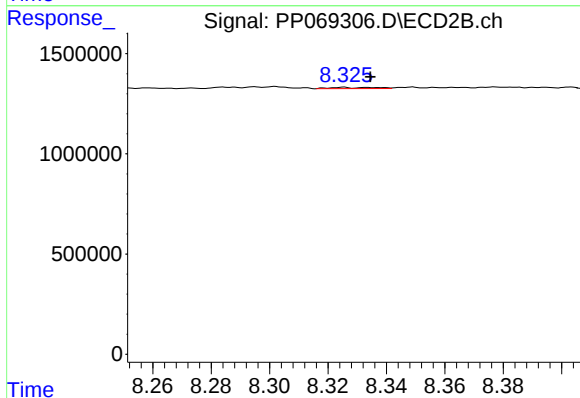


#44 AR-1268-4

R.T.: 8.325 min
Delta R.T.: -0.009 min
Response: 66853
Conc: 1.28 ng/ml

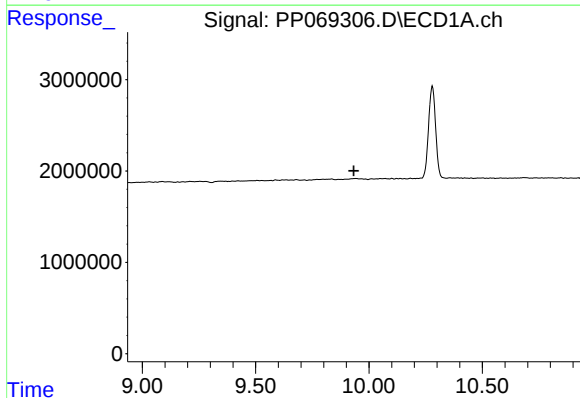

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.933 min
Response: 0
Conc: N.D.

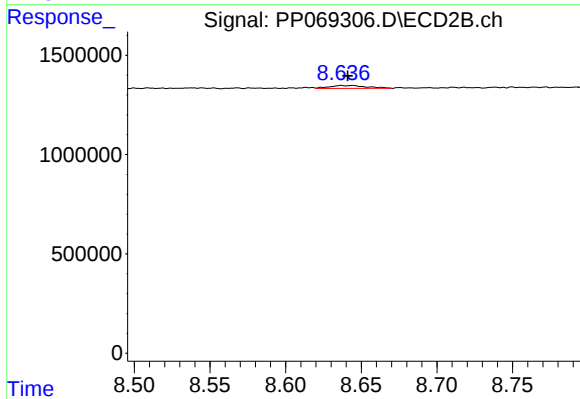

#45 AR-1268-5

R.T.: 8.637 min
Delta R.T.: -0.004 min
Response: 244838
Conc: 0.69 ng/ml