

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
 Data File : PP069307.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2025 11:11
 Operator : YP\AJ
 Sample : Q1168-07
 Misc : AR1254 LOD 25 PPB
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 12:01:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.536	3.841	29367039	19285597	20.515	21.608
2)	SA Decachlor...	10.279	8.913	23107963	25346204	21.144	22.661
Target Compounds							
3)	L1 AR-1016-1	5.625f	0.000	1621194	0	34.990	N.D. #
5)	L1 AR-1016-3	0.000	5.173f	0	582063	N.D.	23.391 #
6)	L1 AR-1016-4	0.000	5.173	0	582063	N.D.	28.820 #
7)	L1 AR-1016-5	6.164	5.387	506081	379411	15.309	14.145
8)	L2 AR-1221-1	4.735	0.000	885845	0	46.576	N.D. #
9)	L2 AR-1221-2	4.840	4.145	488960	808095	35.710	83.452 #
10)	L2 AR-1221-3	4.840f	4.225	488960	79459	11.658	2.724 #
11)	L3 AR-1232-1	4.840f	4.225	488960	79459	14.686	3.384 #
13)	L3 AR-1232-3	0.000	5.173f	0	582063	N.D.	44.956 #
14)	L3 AR-1232-4	0.000	5.213	0	112326	N.D.	10.132 #
15)	L3 AR-1232-5	5.964	5.387	659886	379411	57.570	31.073 #
16)	L4 AR-1242-1	5.625f	0.000	1621194	0	38.873	N.D. #
18)	L4 AR-1242-3	0.000	5.173f	0	582063	N.D.	25.865 #
19)	L4 AR-1242-4	0.000	5.213	0	112326	N.D.	5.205 #
20)	L4 AR-1242-5	6.563f	5.742	706373	1869490	21.678	64.984 #
21)	L5 AR-1248-1	5.625f	0.000	1621194	0	49.977	N.D. #
22)	L5 AR-1248-2	5.964	5.173	659886	582063	15.546	19.360
23)	L5 AR-1248-3	6.164	5.213	506081	112326	10.771	3.625 #
24)	L5 AR-1248-4	6.563	5.387	706373	379411	12.815	10.270
25)	L5 AR-1248-5	6.563f	5.742f	706373	1869490	13.232	50.001 #
26)	L6 AR-1254-1	6.541	5.742	1589954	1869490	27.478	33.956
27)	L6 AR-1254-2	6.757	5.891	2172288	1499872	27.072	31.009
28)	L6 AR-1254-3	7.121	6.297	2505738	2058043	29.728	27.117
29)	L6 AR-1254-4	7.404	6.525	1968912	1705921	28.875	33.286
30)	L6 AR-1254-5	7.820	6.945	1831527	1700488	26.916	25.548
31)	L7 AR-1260-1	7.285	6.428	817553	899332	13.991	18.647 #
32)	L7 AR-1260-2	7.540	6.615	1666038	869527	21.411	14.184 #
33)	L7 AR-1260-3	0.000	6.770	0	1949138	N.D.	32.401 #
34)	L7 AR-1260-4	8.108	7.246	678584	72196	10.285	1.554 #
35)	L7 AR-1260-5	0.000	7.485	0	169178	N.D.	1.522 #
36)	L8 AR-1262-1	8.108	7.014	678584	201803	8.588	2.842 #
37)	L8 AR-1262-2	0.000	7.246	0	72196	N.D.	1.184 #
38)	L8 AR-1262-3	0.000	7.796	0	297882	N.D.	5.696 #
39)	L8 AR-1262-4	0.000	7.828	0	389290	N.D.	4.211 #
40)	L8 AR-1262-5	0.000	8.300f	0	56769	N.D.	1.188 #
41)	L9 AR-1268-1	0.000	7.796	0	297882	N.D.	2.053 #
42)	L9 AR-1268-2	0.000	7.828	0	389290	N.D.	2.931 #
43)	L9 AR-1268-3	0.000	8.063	0	58804	N.D.	0.517 #
44)	L9 AR-1268-4	0.000	8.300	0	56769	N.D.	1.090 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
 Data File : PP069307.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2025 11:11
 Operator : YP\AJ
 Sample : Q1168-07
 Misc : AR1254 LOD 25 PPB
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 12:01:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
45) L9	AR-1268-5	0.000	8.643	0	170545	N.D.	0.479 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
Data File : PP069307.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2025 11:11
Operator : YP\AJ
Sample : Q1168-07
Misc : AR1254 LOD 25 PPB
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 12:01:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

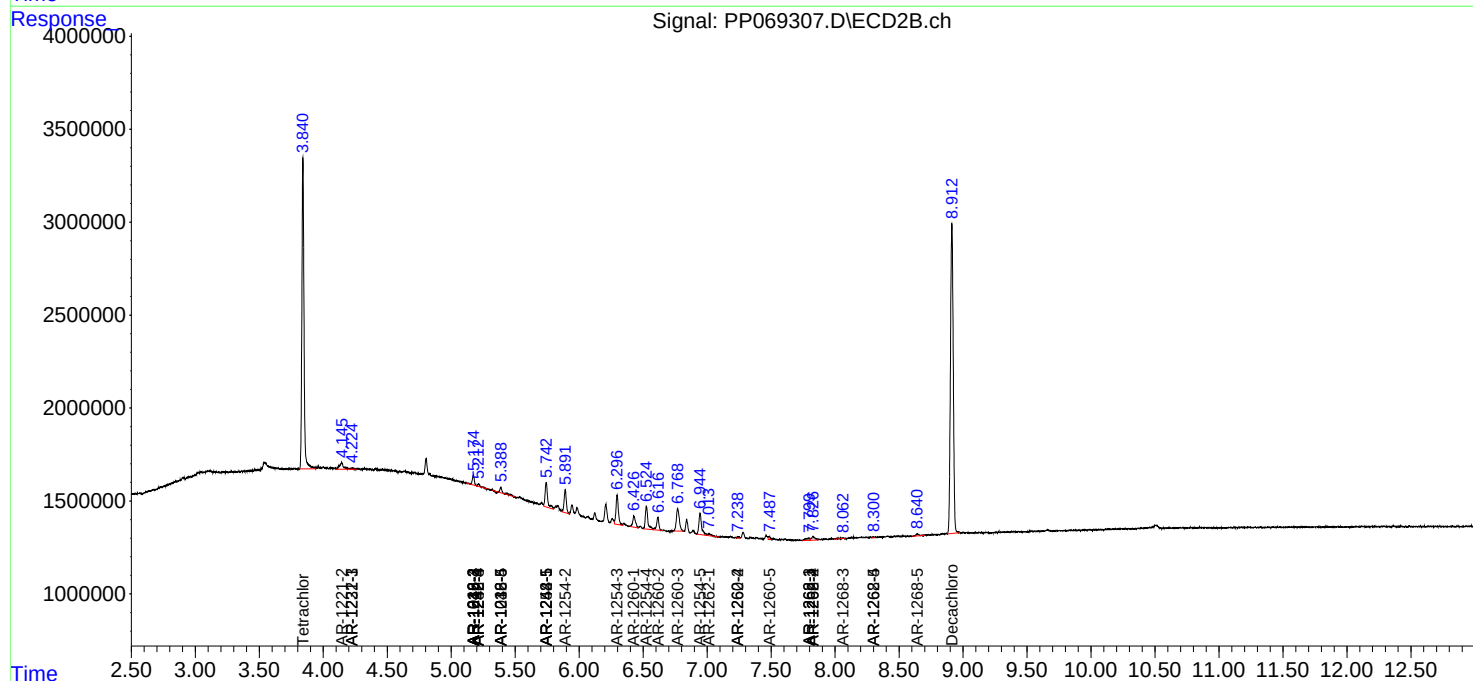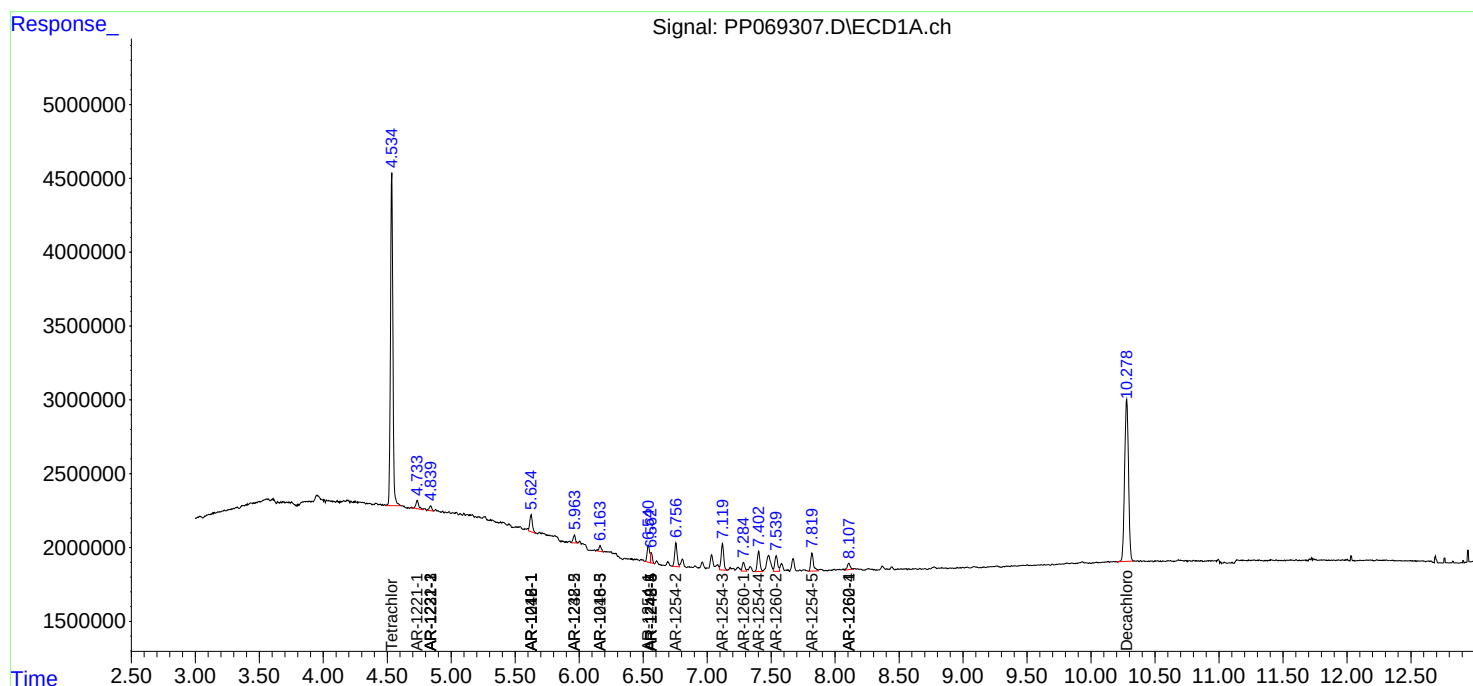


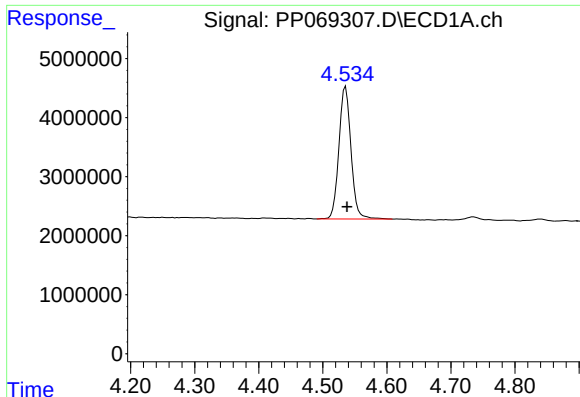

#1 Tetrachloro-m-xylene


R.T.: 4.536 min
Delta R.T.: -0.002 min
Response: 29367039
Conc: 20.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

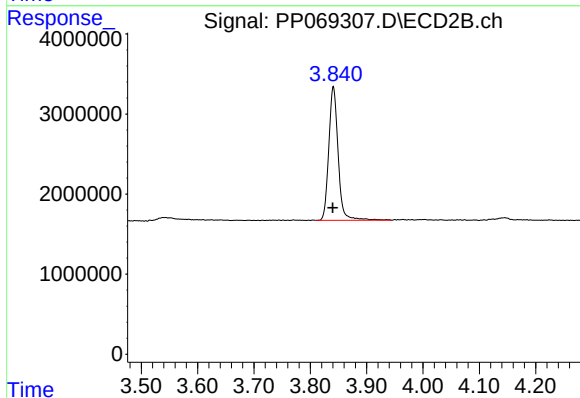


#1 Tetrachloro-m-xylene

R.T.: 3.841 min
Delta R.T.: 0.001 min
Response: 19285597
Conc: 21.61 ng/ml

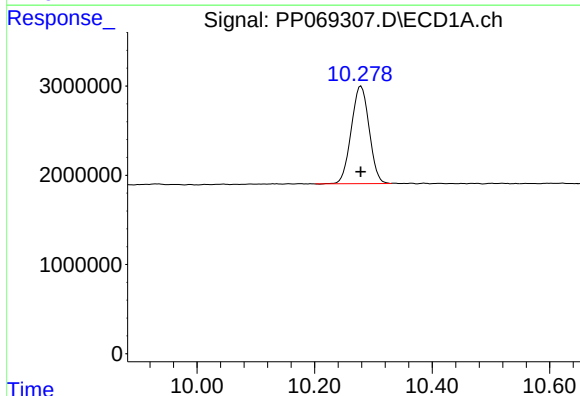


#2 Decachlorobiphenyl

R.T.: 10.279 min
Delta R.T.: 0.000 min
Response: 23107963
Conc: 21.14 ng/ml

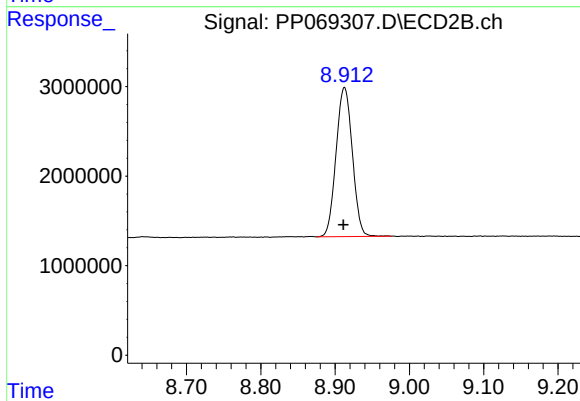

#2 Decachlorobiphenyl


R.T.: 8.913 min
Delta R.T.: 0.001 min
Response: 25346204
Conc: 22.66 ng/ml

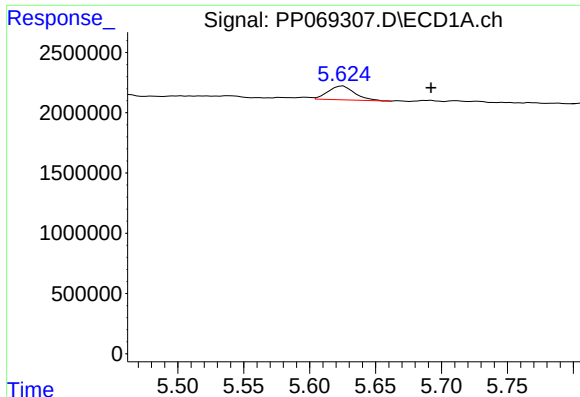

#3 AR-1016-1


R.T.: 5.625 min
Delta R.T.: -0.067 min
Response: 1621194
Conc: 34.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

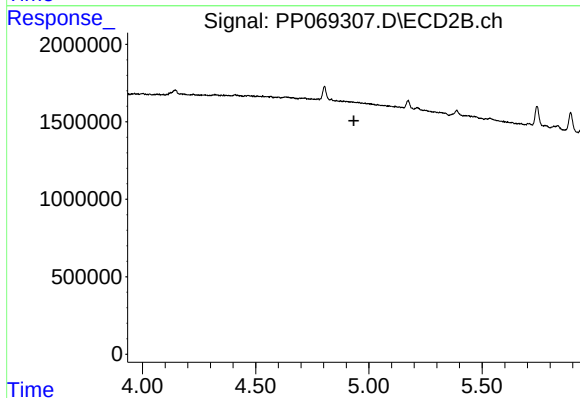


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.934 min
Response: 0
Conc: N.D.

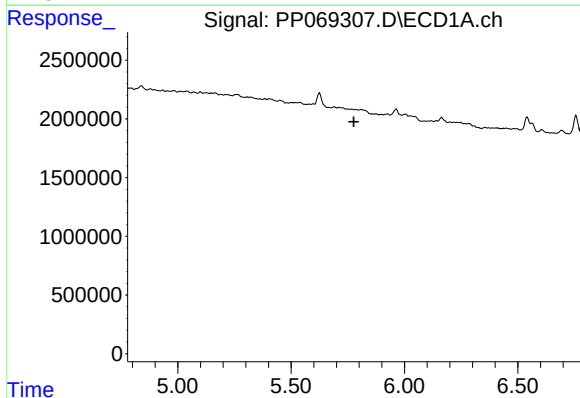


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 5.776 min
Response: 0
Conc: N.D.

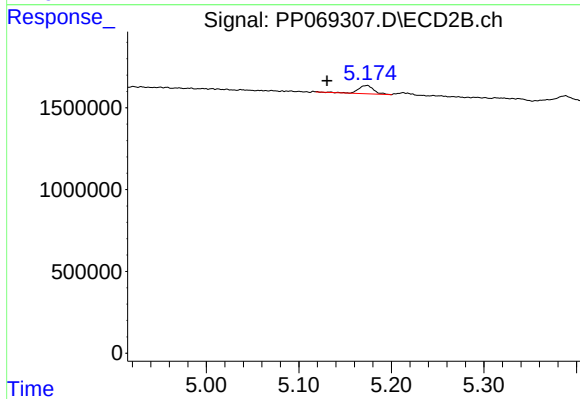

#5 AR-1016-3


R.T.: 5.173 min
Delta R.T.: 0.043 min
Response: 582063
Conc: 23.39 ng/ml

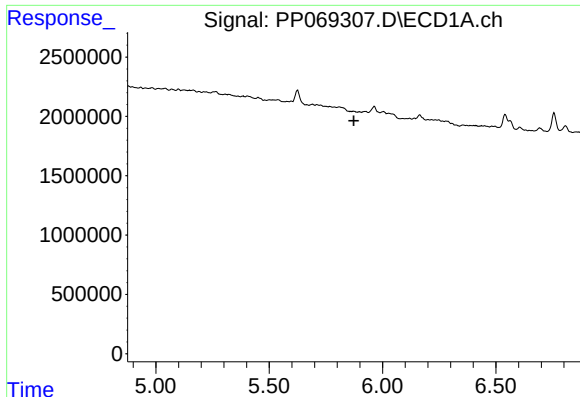

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T.: 5.874 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

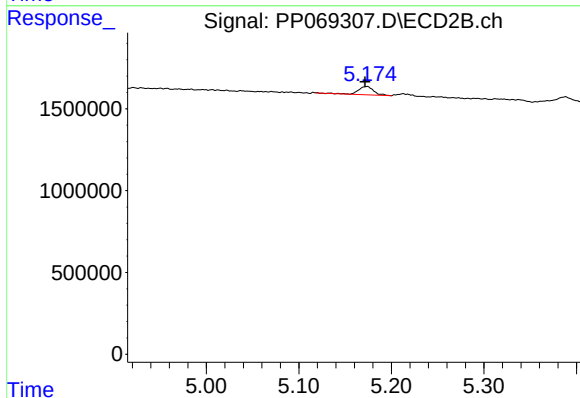


#6 AR-1016-4

R.T.: 5.173 min
Delta R.T.: 0.001 min
Response: 582063
Conc: 28.82 ng/ml

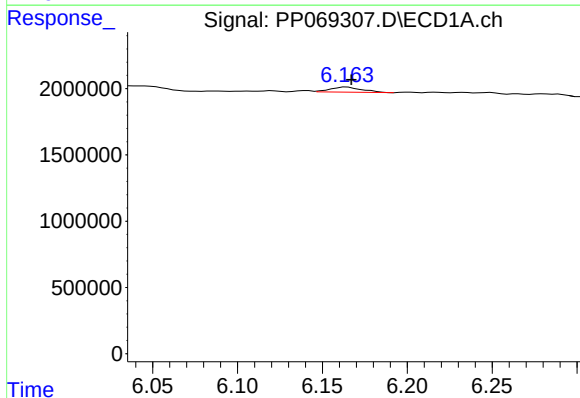


#7 AR-1016-5

R.T.: 6.164 min
Delta R.T.: -0.003 min
Response: 506081
Conc: 15.31 ng/ml

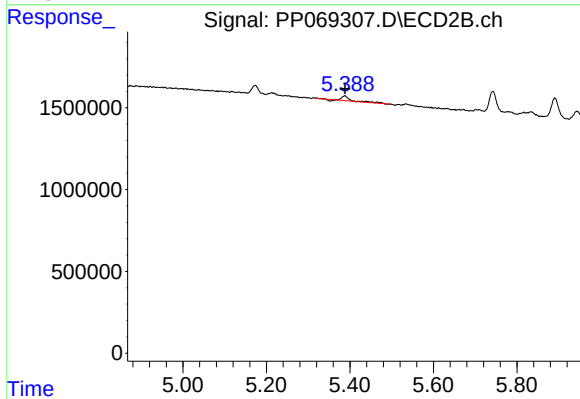

#7 AR-1016-5


R.T.: 5.387 min
Delta R.T.: 0.000 min
Response: 379411
Conc: 14.14 ng/ml

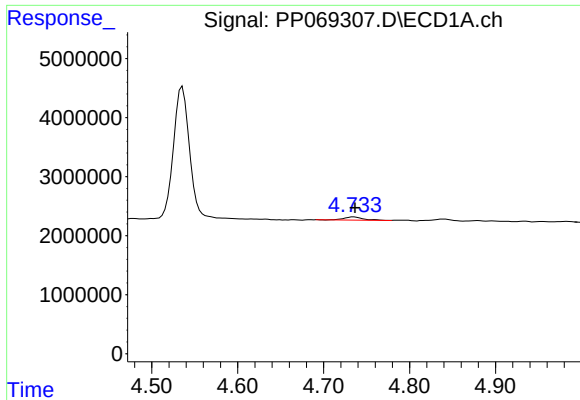

#8 AR-1221-1


R.T.: 4.735 min
Delta R.T.: -0.002 min
Response: 885845
Conc: 46.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

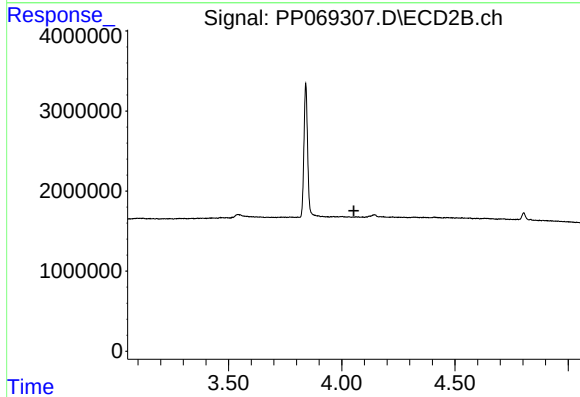


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.054 min
Response: 0
Conc: N.D.

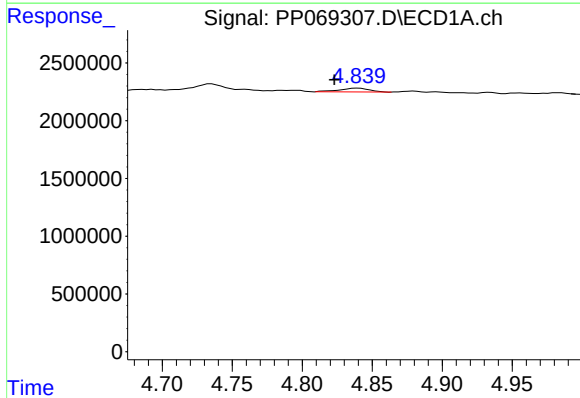


#9 AR-1221-2

R.T.: 4.840 min
Delta R.T.: 0.017 min
Response: 488960
Conc: 35.71 ng/ml

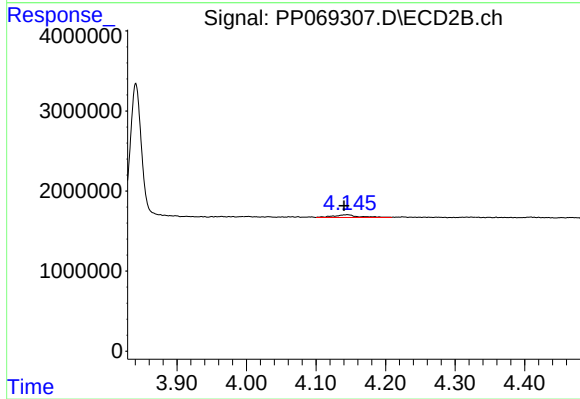

#9 AR-1221-2


R.T.: 4.145 min
Delta R.T.: 0.004 min
Response: 808095
Conc: 83.45 ng/ml

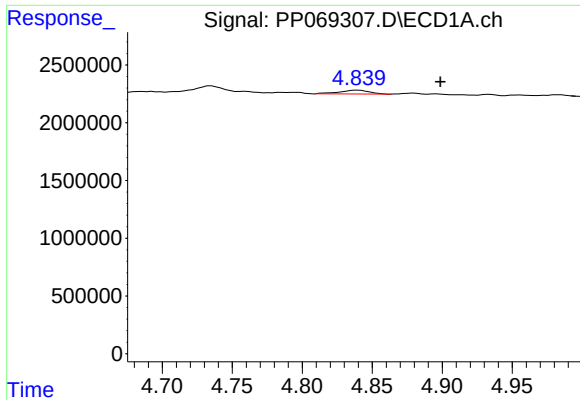

#10 AR-1221-3


R.T.: 4.840 min
Delta R.T.: -0.059 min
Response: 488960
Conc: 11.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

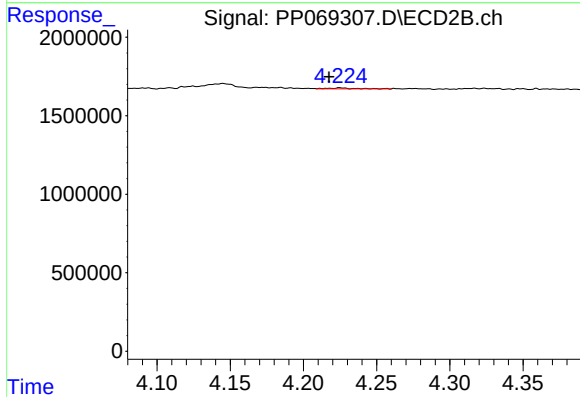


#10 AR-1221-3

R.T.: 4.225 min
Delta R.T.: 0.008 min
Response: 79459
Conc: 2.72 ng/ml

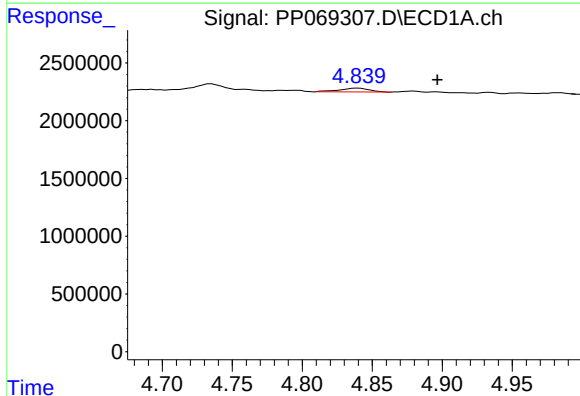


#11 AR-1232-1

R.T.: 4.840 min
Delta R.T.: -0.057 min
Response: 488960
Conc: 14.69 ng/ml

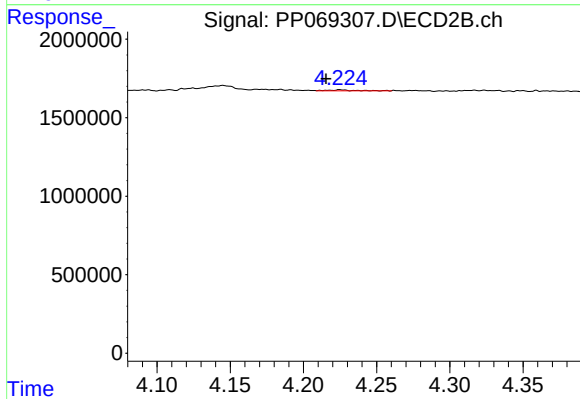

#11 AR-1232-1


R.T.: 4.225 min
Delta R.T.: 0.010 min
Response: 79459
Conc: 3.38 ng/ml

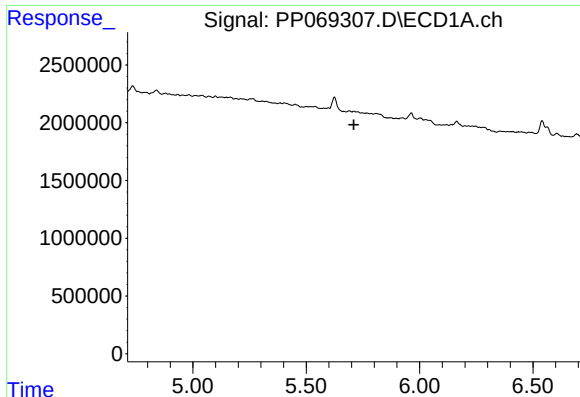

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.710 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

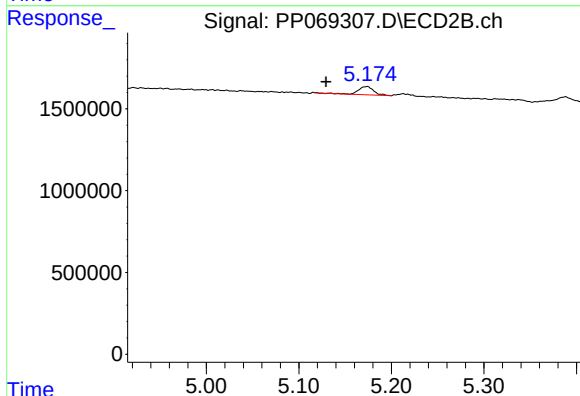


#13 AR-1232-3

R.T.: 5.173 min
Delta R.T.: 0.044 min
Response: 582063
Conc: 44.96 ng/ml

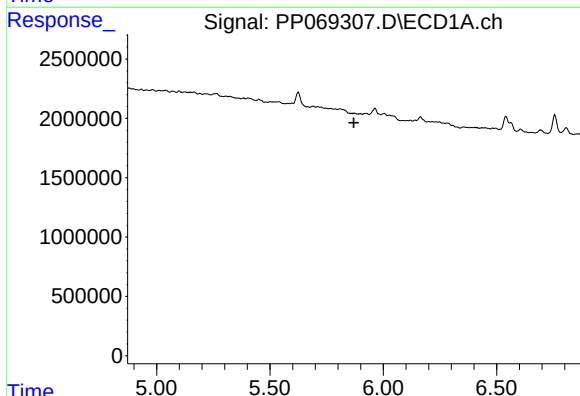


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.870 min
Response: 0
Conc: N.D.

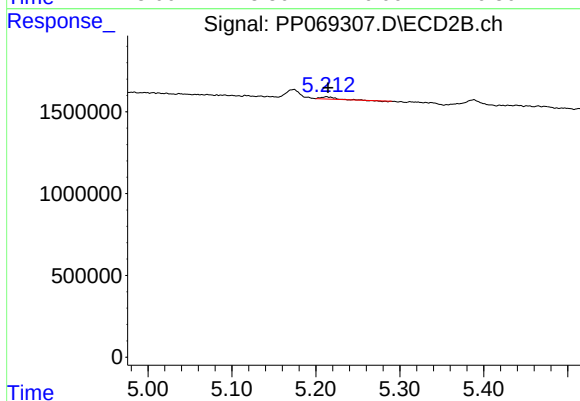

#14 AR-1232-4


R.T.: 5.213 min
Delta R.T.: -0.001 min
Response: 112326
Conc: 10.13 ng/ml

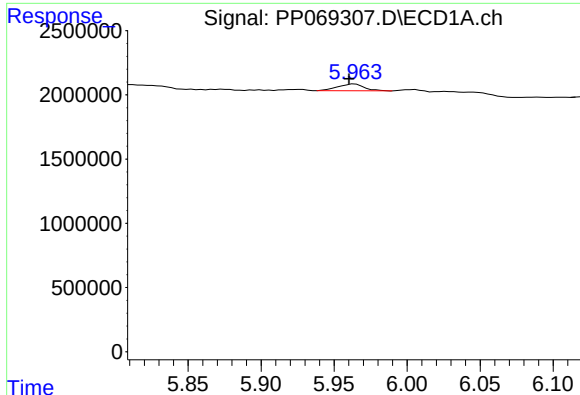

#15 AR-1232-5


R.T.: 5.964 min
Delta R.T.: 0.004 min
Response: 659886
Conc: 57.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

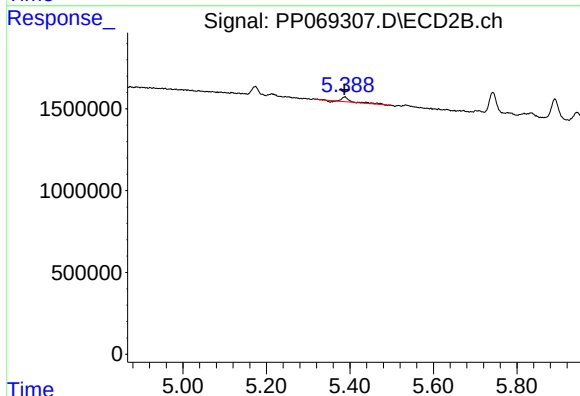


#15 AR-1232-5

R.T.: 5.387 min
Delta R.T.: 0.000 min
Response: 379411
Conc: 31.07 ng/ml

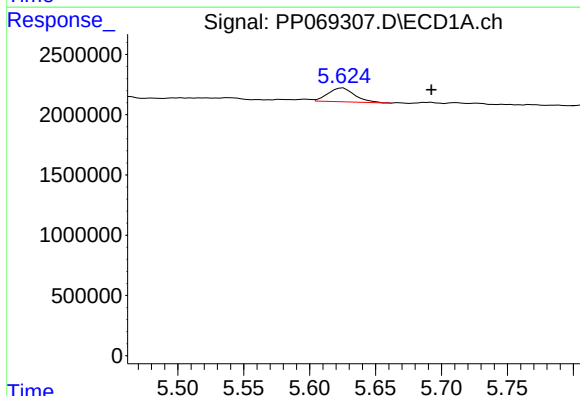


#16 AR-1242-1

R.T.: 5.625 min
Delta R.T.: -0.067 min
Response: 1621194
Conc: 38.87 ng/ml

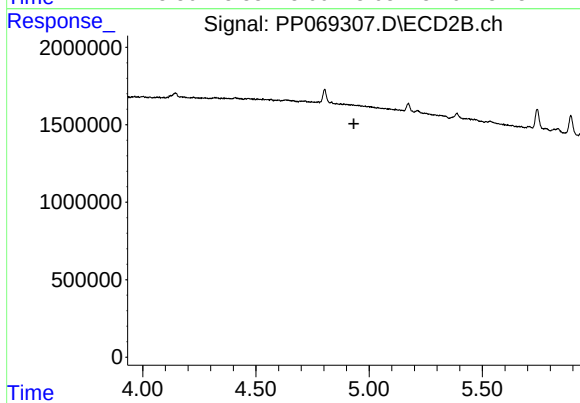

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.933 min
Response: 0
Conc: N.D.

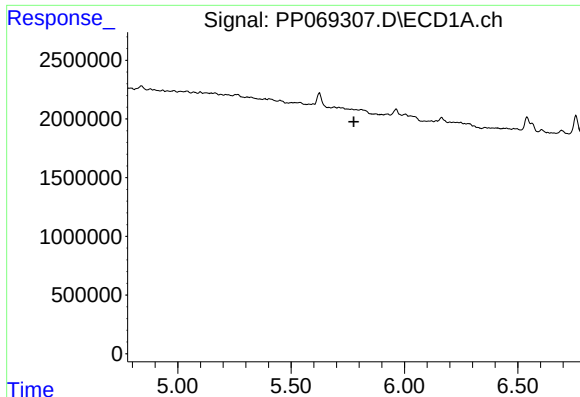

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 5.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

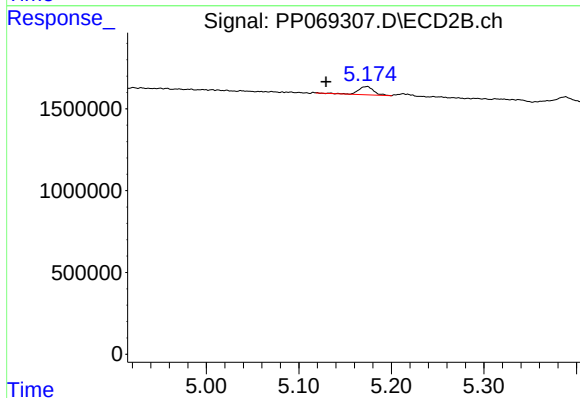


#18 AR-1242-3

R.T.: 5.173 min
Delta R.T.: 0.043 min
Response: 582063
Conc: 25.86 ng/ml

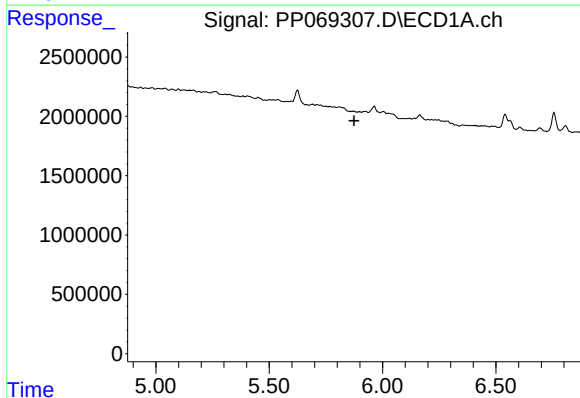


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 5.874 min
Response: 0
Conc: N.D.

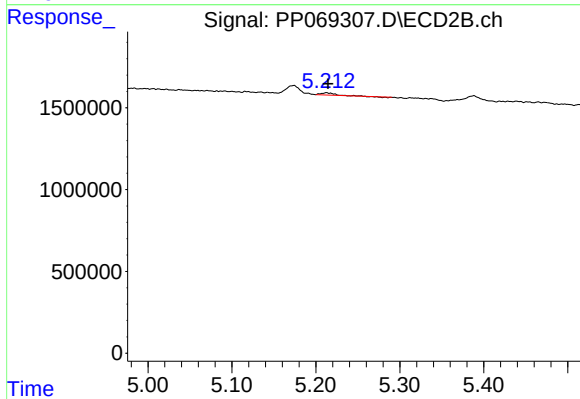

#19 AR-1242-4


R.T.: 5.213 min
Delta R.T.: -0.001 min
Response: 112326
Conc: 5.20 ng/ml

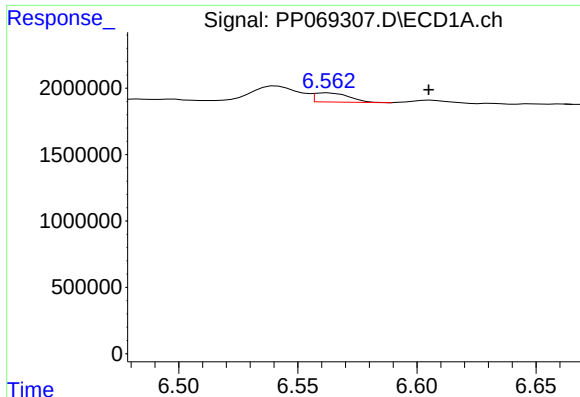

#20 AR-1242-5


R.T.: 6.563 min
Delta R.T.: -0.042 min
Response: 706373
Conc: 21.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

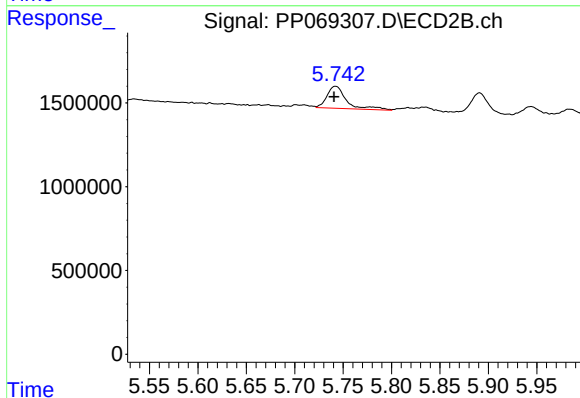


#20 AR-1242-5

R.T.: 5.742 min
Delta R.T.: 0.002 min
Response: 1869490
Conc: 64.98 ng/ml

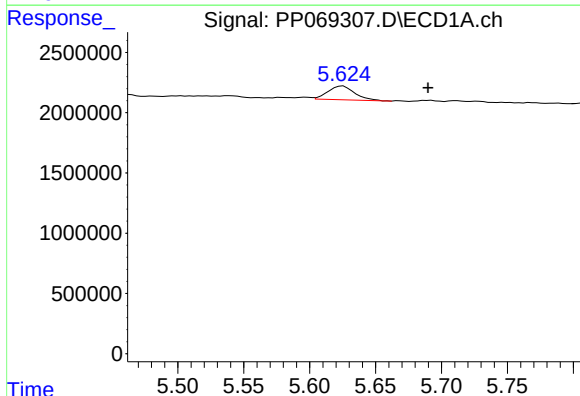


#21 AR-1248-1

R.T.: 5.625 min
Delta R.T.: -0.065 min
Response: 1621194
Conc: 49.98 ng/ml

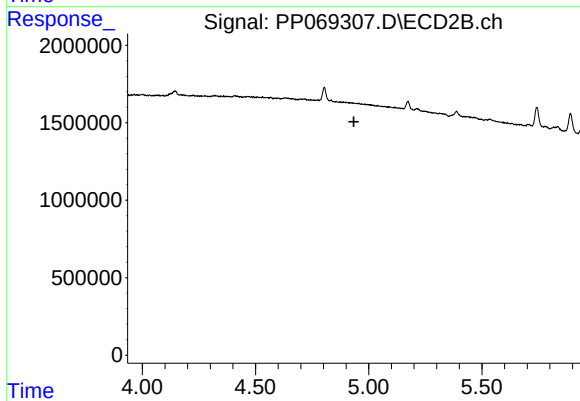

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T. : 4.934 min
Response: 0
Conc: N.D.

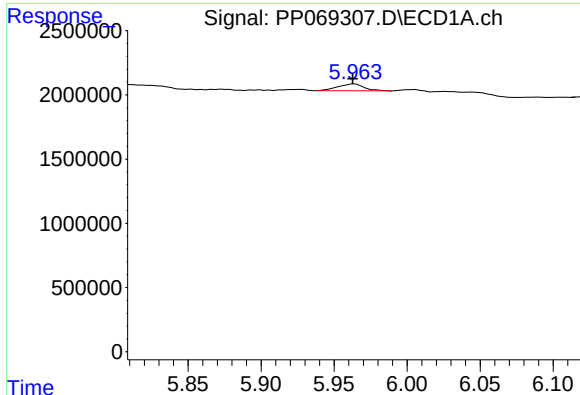

#22 AR-1248-2


R.T.: 5.964 min
Delta R.T.: 0.001 min
Response: 659886
Conc: 15.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

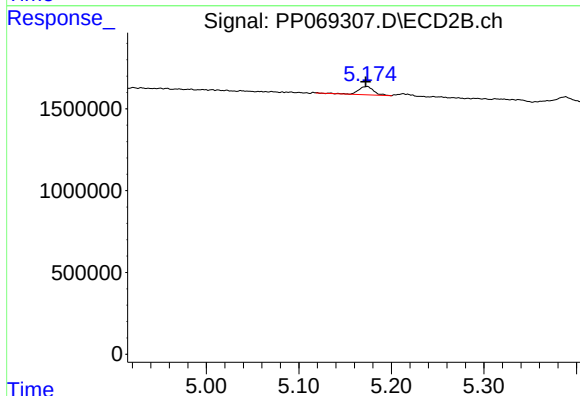


#22 AR-1248-2

R.T.: 5.173 min
Delta R.T.: 0.000 min
Response: 582063
Conc: 19.36 ng/ml

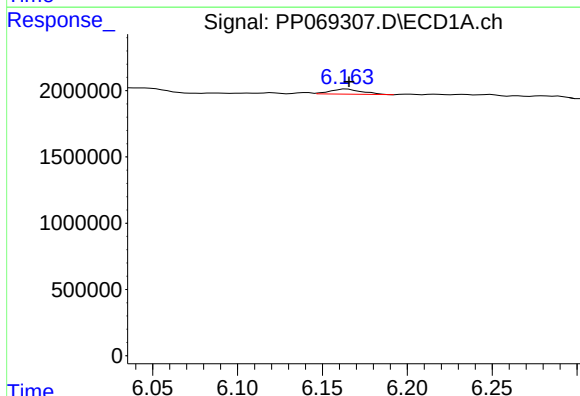


#23 AR-1248-3

R.T.: 6.164 min
Delta R.T.: -0.001 min
Response: 506081
Conc: 10.77 ng/ml

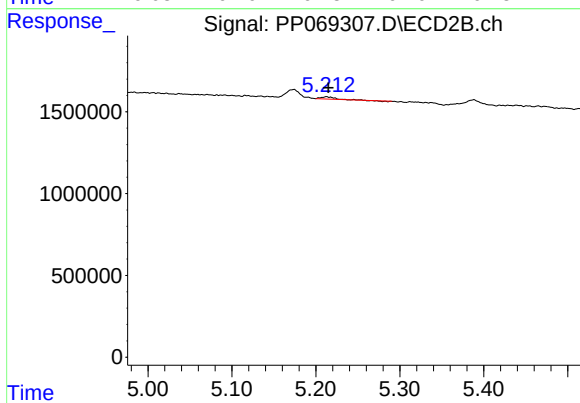

#23 AR-1248-3


R.T.: 5.213 min
Delta R.T.: -0.002 min
Response: 112326
Conc: 3.63 ng/ml

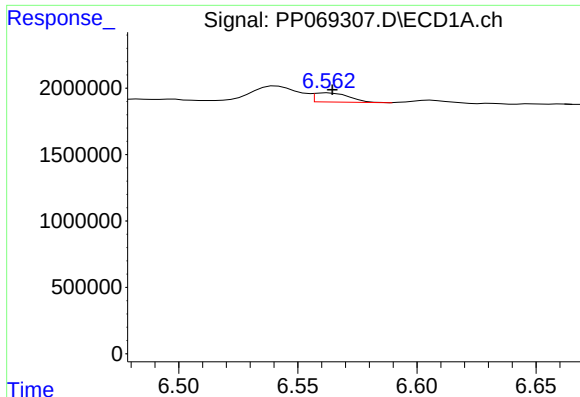

#24 AR-1248-4


R.T.: 6.563 min
Delta R.T.: -0.002 min
Response: 706373
Conc: 12.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

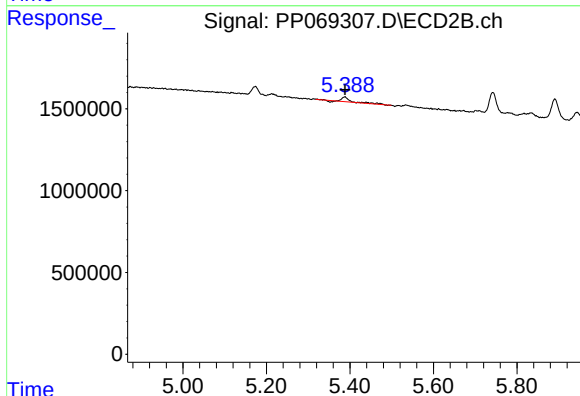


#24 AR-1248-4

R.T.: 5.387 min
Delta R.T.: 0.000 min
Response: 379411
Conc: 10.27 ng/ml

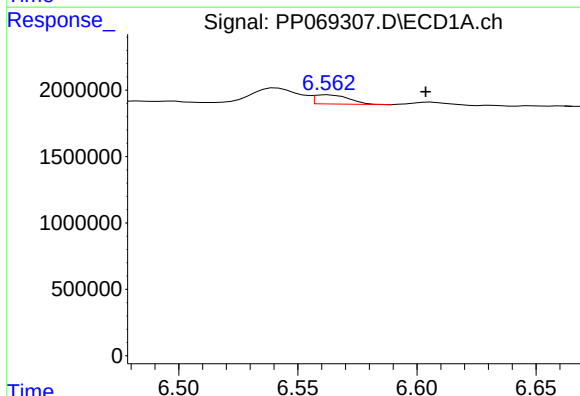


#25 AR-1248-5

R.T.: 6.563 min
Delta R.T.: -0.041 min
Response: 706373
Conc: 13.23 ng/ml

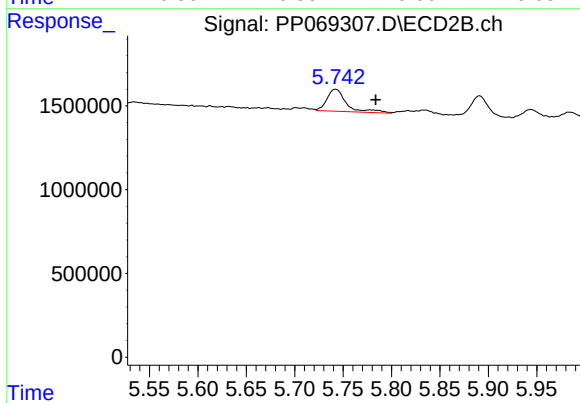

#25 AR-1248-5


R.T.: 5.742 min
Delta R.T.: -0.041 min
Response: 1869490
Conc: 50.00 ng/ml

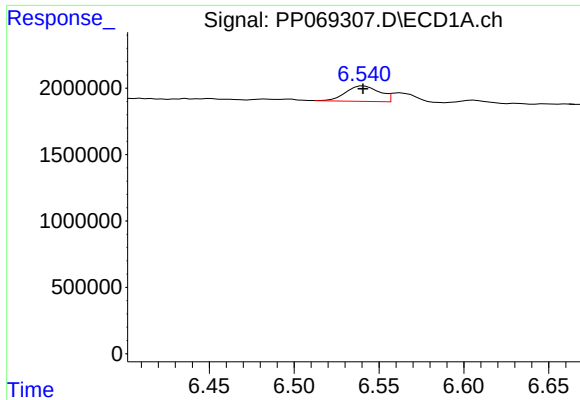

#26 AR-1254-1


R.T.: 6.541 min
Delta R.T.: 0.000 min
Response: 1589954
Conc: 27.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

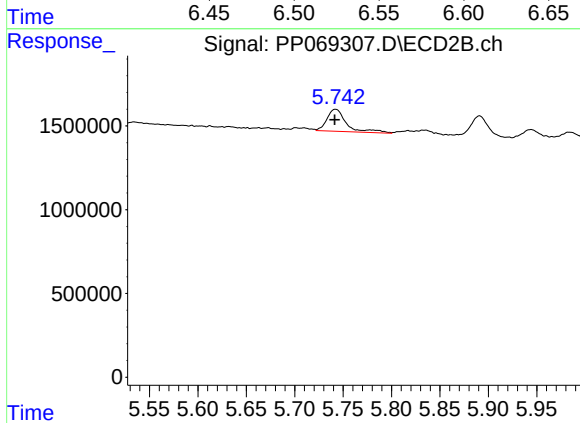


#26 AR-1254-1

R.T.: 5.742 min
Delta R.T.: 0.000 min
Response: 1869490
Conc: 33.96 ng/ml

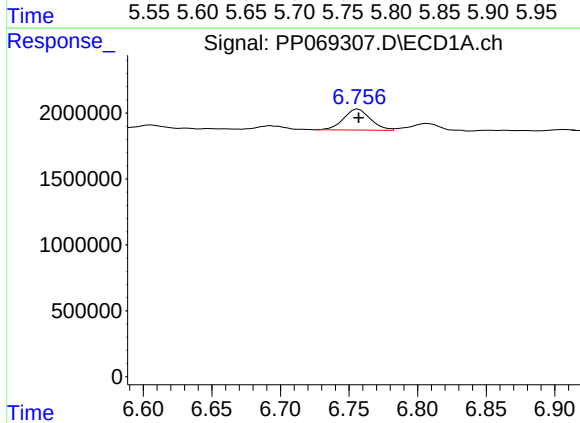


#27 AR-1254-2

R.T.: 6.757 min
Delta R.T.: 0.000 min
Response: 2172288
Conc: 27.07 ng/ml

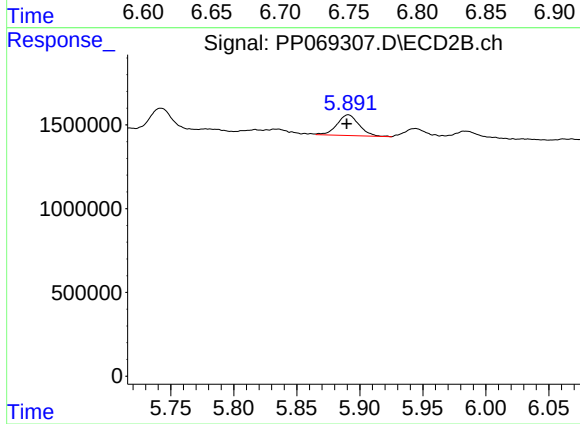

#27 AR-1254-2


R.T.: 5.891 min
Delta R.T.: 0.001 min
Response: 1499872
Conc: 31.01 ng/ml

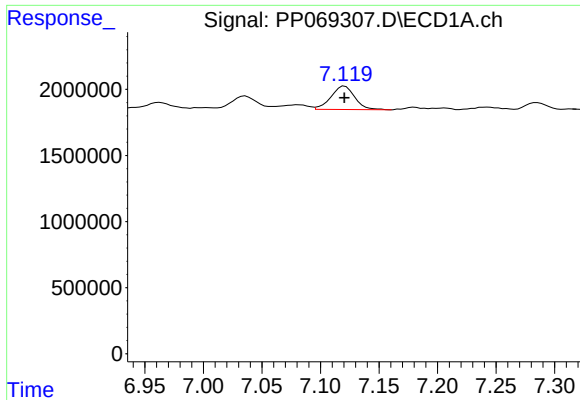

#28 AR-1254-3


R.T.: 7.121 min
Delta R.T.: 0.000 min
Response: 2505738
Conc: 29.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

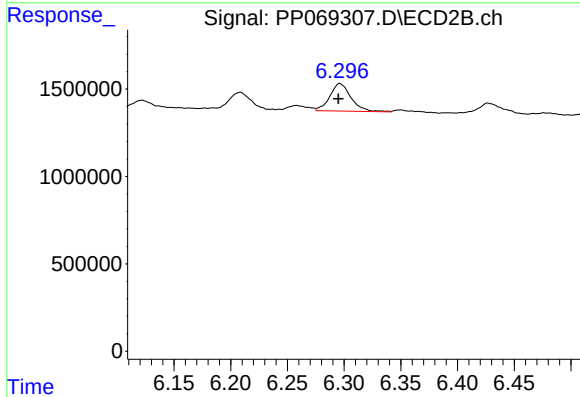


#28 AR-1254-3

R.T.: 6.297 min
Delta R.T.: 0.002 min
Response: 2058043
Conc: 27.12 ng/ml

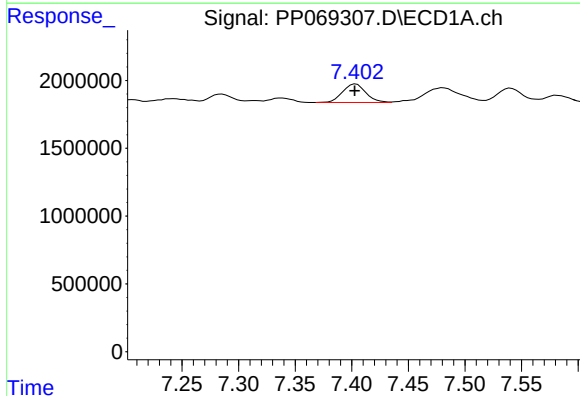


#29 AR-1254-4

R.T.: 7.404 min
Delta R.T.: 0.000 min
Response: 1968912
Conc: 28.87 ng/ml

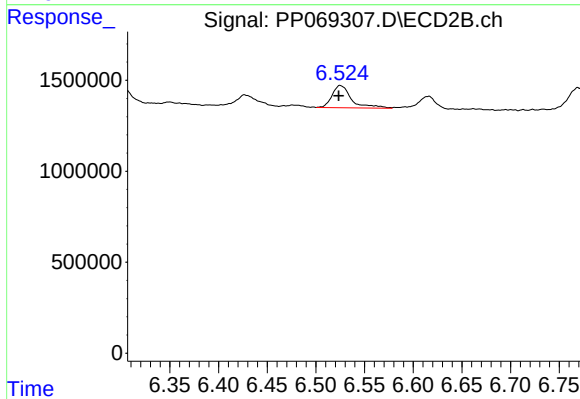

#29 AR-1254-4


R.T.: 6.525 min
Delta R.T.: 0.002 min
Response: 1705921
Conc: 33.29 ng/ml

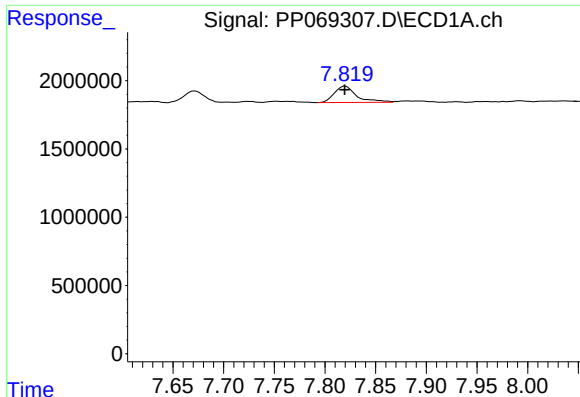

#30 AR-1254-5


R.T.: 7.820 min
Delta R.T.: 0.000 min
Response: 1831527
Conc: 26.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

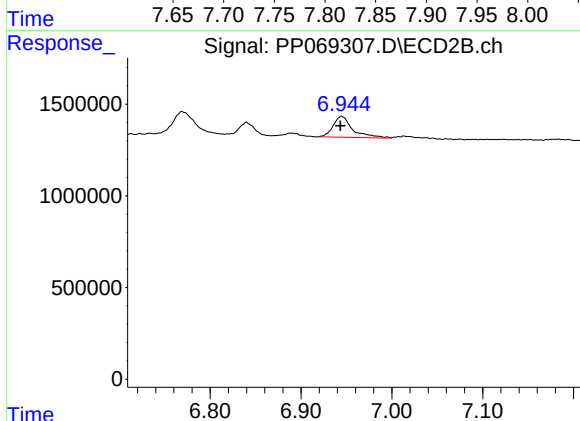


#30 AR-1254-5

R.T.: 6.945 min
Delta R.T.: 0.002 min
Response: 1700488
Conc: 25.55 ng/ml

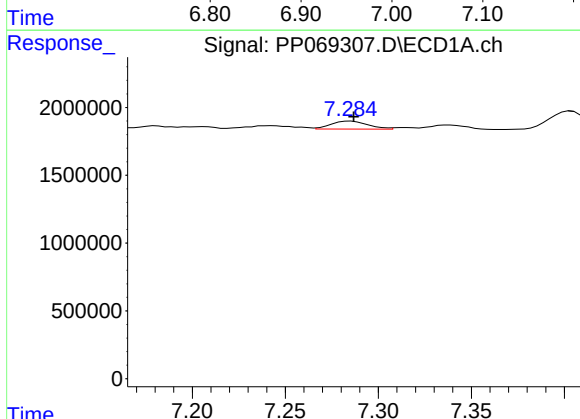


#31 AR-1260-1

R.T.: 7.285 min
Delta R.T.: -0.002 min
Response: 817553
Conc: 13.99 ng/ml

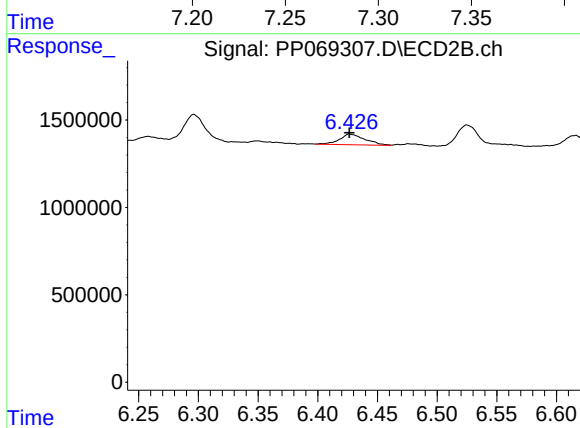

#31 AR-1260-1


R.T.: 6.428 min
Delta R.T.: 0.001 min
Response: 899332
Conc: 18.65 ng/ml

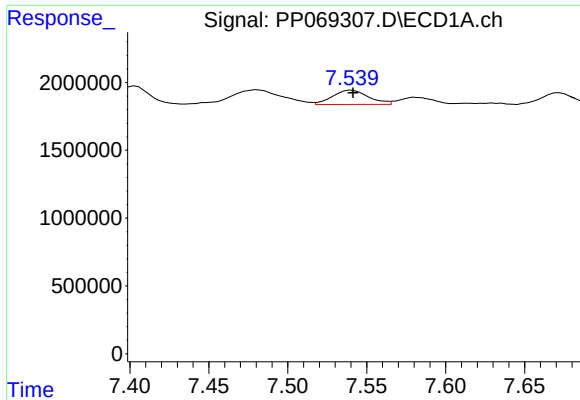

#32 AR-1260-2


R.T.: 7.540 min
Delta R.T.: 0.000 min
Response: 1666038
Conc: 21.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

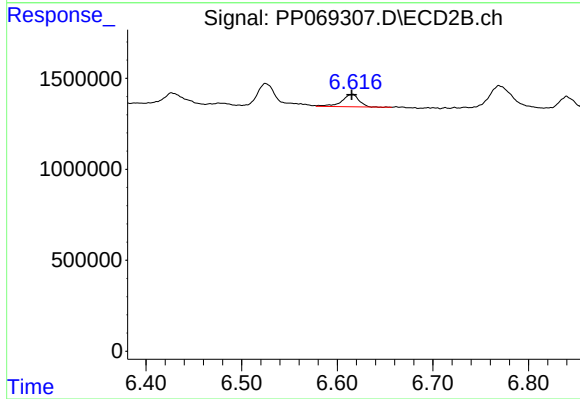


#32 AR-1260-2

R.T.: 6.615 min
Delta R.T.: 0.000 min
Response: 869527
Conc: 14.18 ng/ml

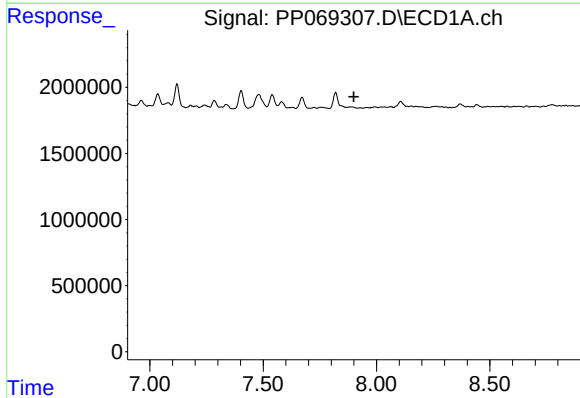


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.900 min
Response: 0
Conc: N.D.

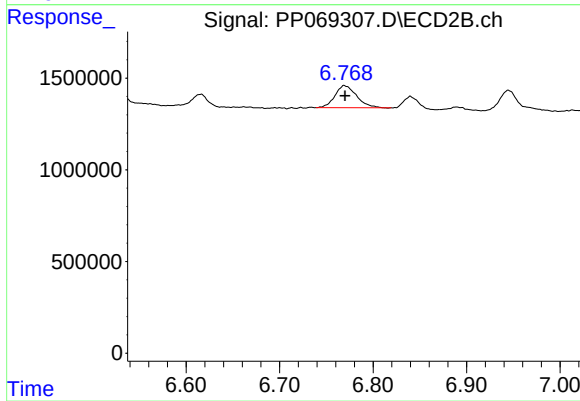

#33 AR-1260-3


R.T.: 6.770 min
Delta R.T.: 0.000 min
Response: 1949138
Conc: 32.40 ng/ml

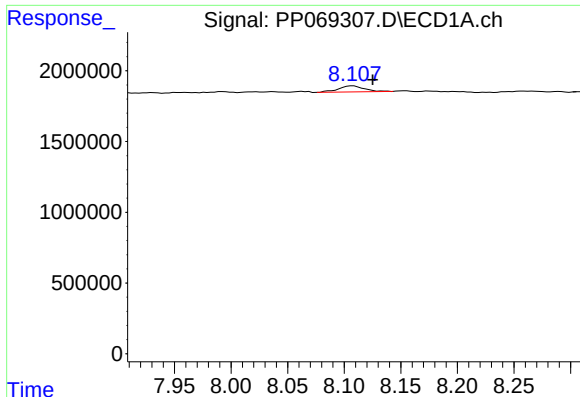

#34 AR-1260-4


R.T.: 8.108 min
Delta R.T.: -0.017 min
Response: 678584
Conc: 10.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

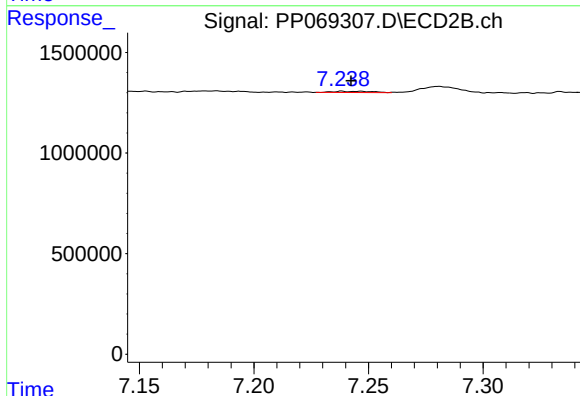


#34 AR-1260-4

R.T.: 7.246 min
Delta R.T.: 0.004 min
Response: 72196
Conc: 1.55 ng/ml

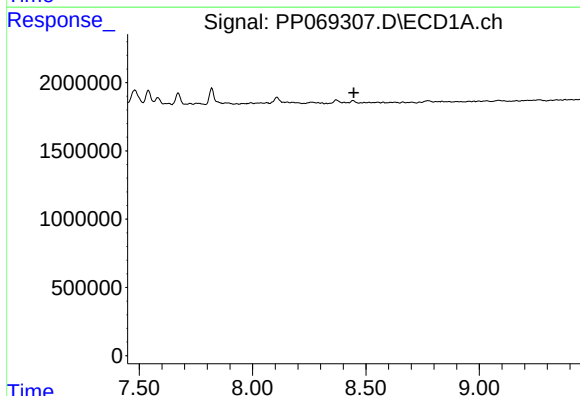


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.447 min
Response: 0
Conc: N.D.

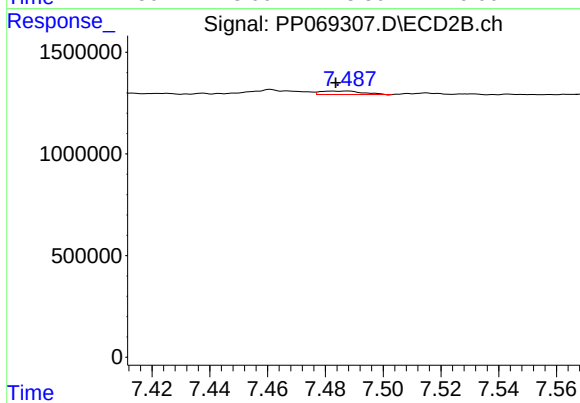

#35 AR-1260-5


R.T.: 7.485 min
Delta R.T.: 0.000 min
Response: 169178
Conc: 1.52 ng/ml

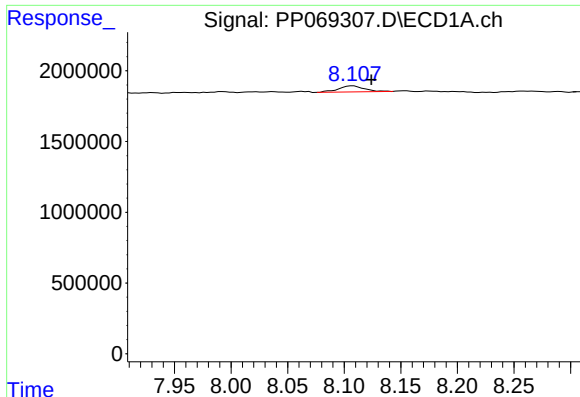

#36 AR-1262-1


R.T.: 8.108 min
Delta R.T.: -0.016 min
Response: 678584
Conc: 8.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

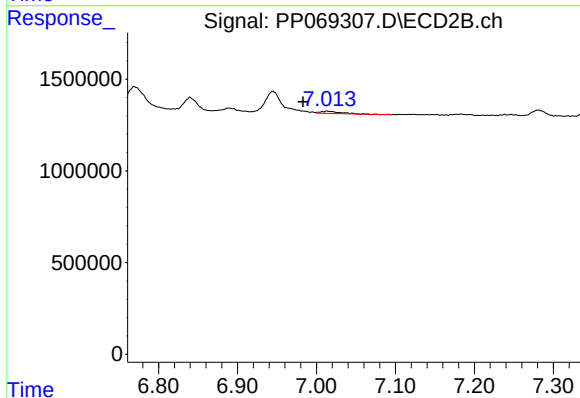


#36 AR-1262-1

R.T.: 7.014 min
Delta R.T.: 0.031 min
Response: 201803
Conc: 2.84 ng/ml

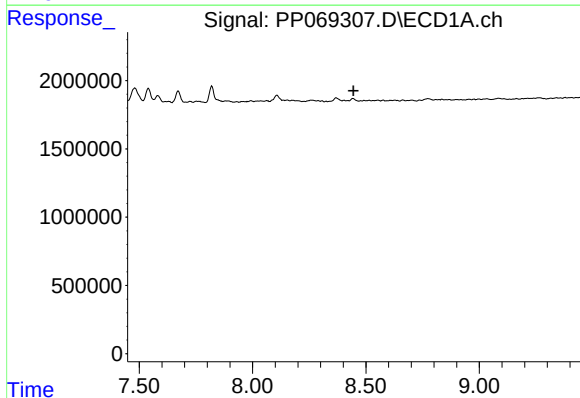


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.446 min
Response: 0
Conc: N.D.

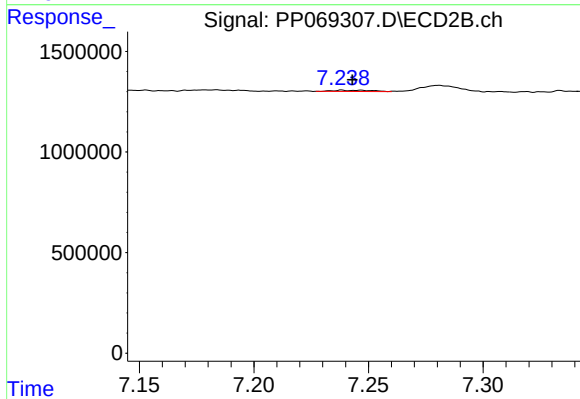

#37 AR-1262-2


R.T.: 7.246 min
Delta R.T.: 0.003 min
Response: 72196
Conc: 1.18 ng/ml

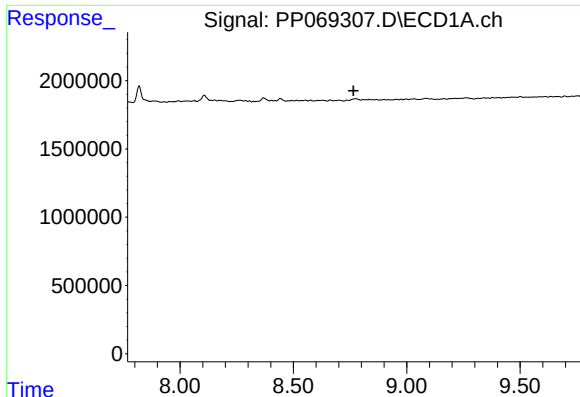

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

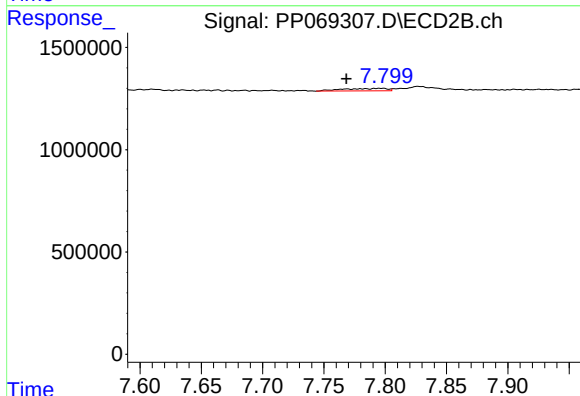


#38 AR-1262-3

R.T.: 7.796 min
Delta R.T.: 0.027 min
Response: 297882
Conc: 5.70 ng/ml

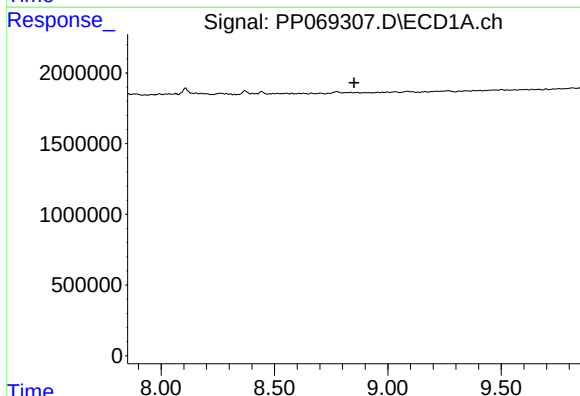


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.852 min
Response: 0
Conc: N.D.

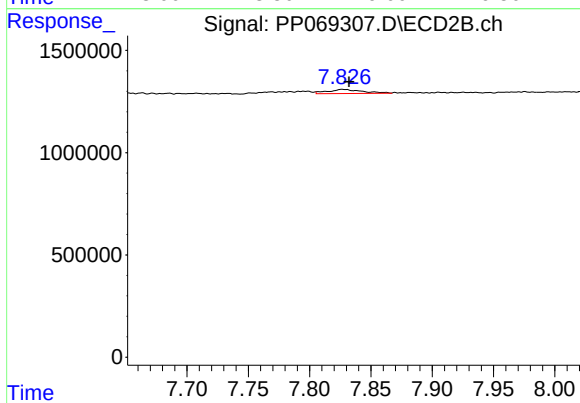

#39 AR-1262-4


R.T.: 7.828 min
Delta R.T.: -0.004 min
Response: 389290
Conc: 4.21 ng/ml

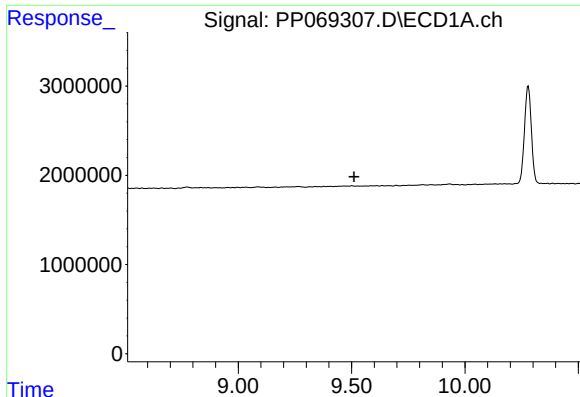

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

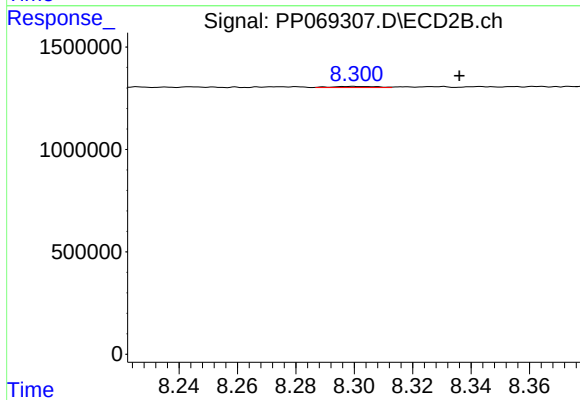


#40 AR-1262-5

R.T.: 8.300 min
Delta R.T.: -0.036 min
Response: 56769
Conc: 1.19 ng/ml

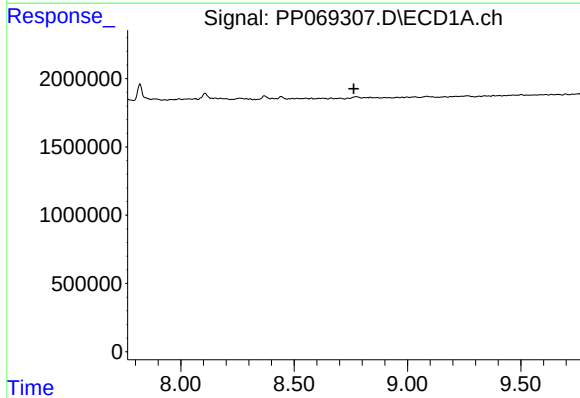


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.763 min
Response: 0
Conc: N.D.

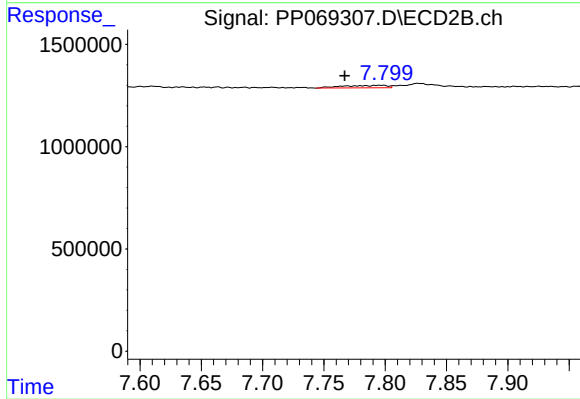

#41 AR-1268-1


R.T.: 7.796 min
Delta R.T.: 0.029 min
Response: 297882
Conc: 2.05 ng/ml

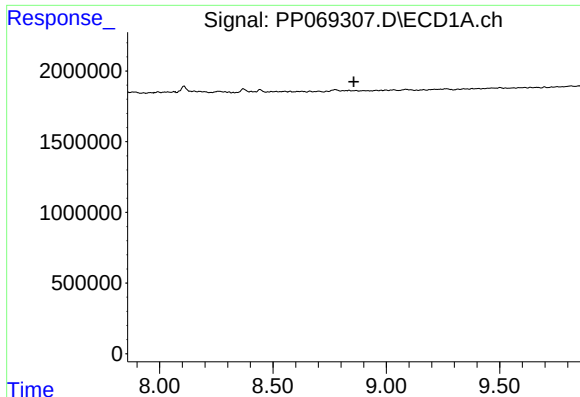

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 8.857 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

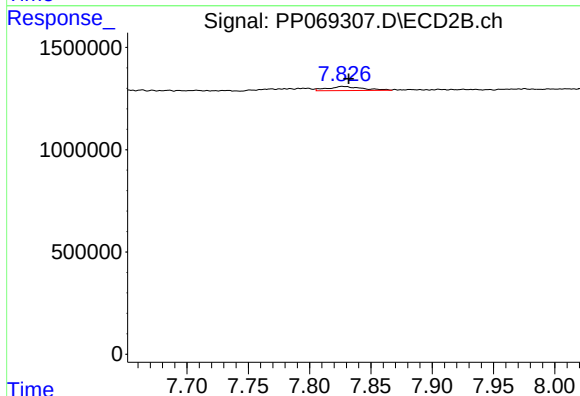


#42 AR-1268-2

R.T.: 7.828 min
Delta R.T.: -0.004 min
Response: 389290
Conc: 2.93 ng/ml

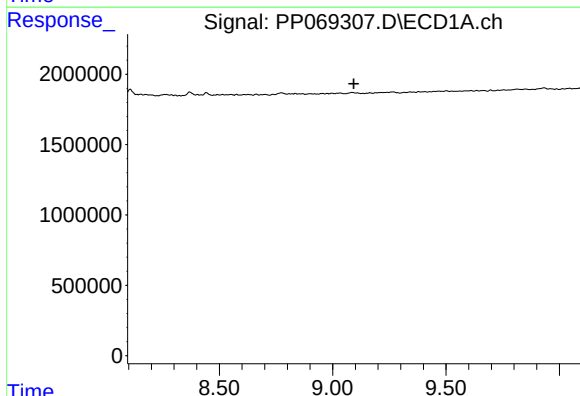


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.093 min
Response: 0
Conc: N.D.

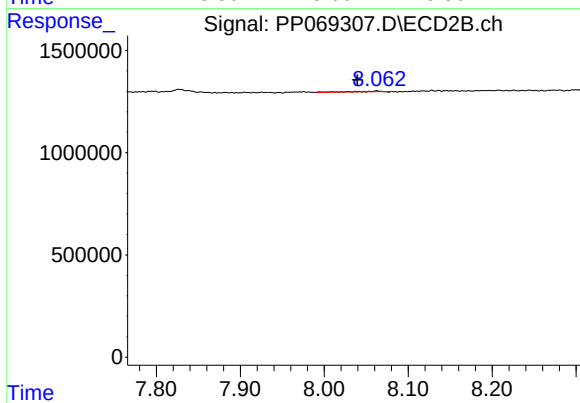

#43 AR-1268-3


R.T.: 8.063 min
Delta R.T.: 0.024 min
Response: 58804
Conc: 0.52 ng/ml

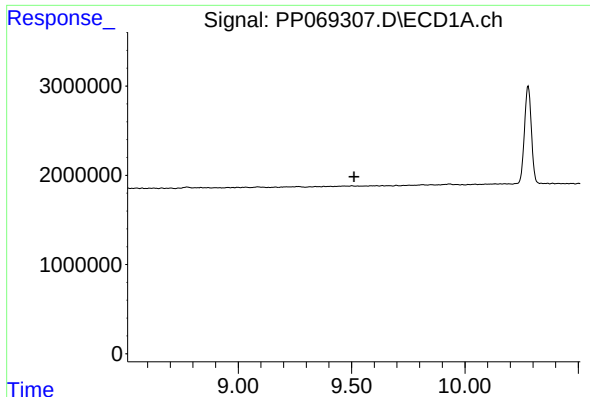

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 9.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

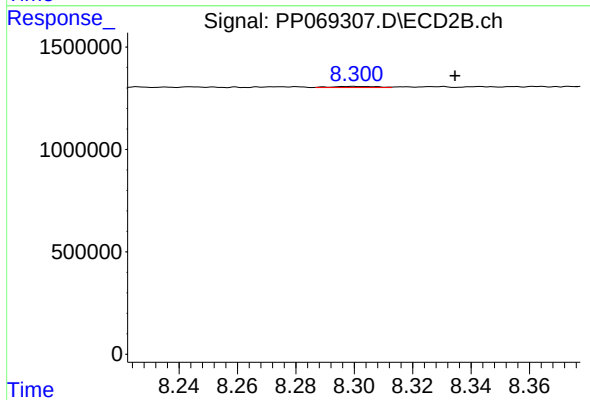


#44 AR-1268-4

R.T.: 8.300 min
Delta R.T.: -0.034 min
Response: 56769
Conc: 1.09 ng/ml

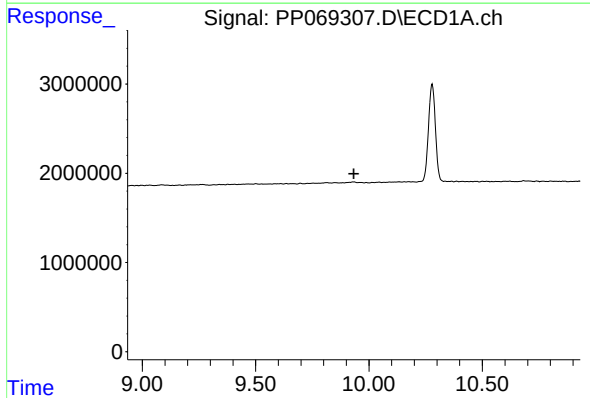

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.933 min
Response: 0
Conc: N.D.

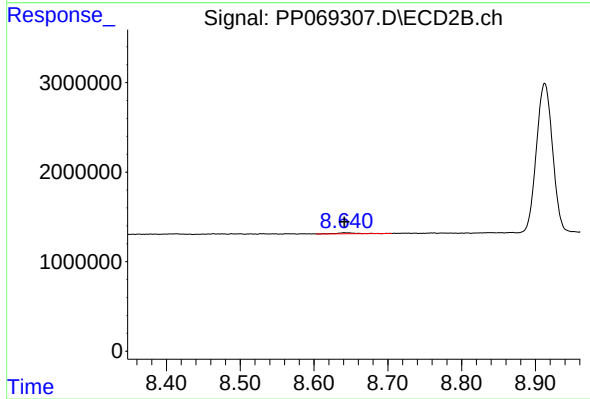

#45 AR-1268-5

R.T.: 8.643 min
Delta R.T.: 0.002 min
Response: 170545
Conc: 0.48 ng/ml