

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
 Data File : PP069323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2025 15:32
 Operator : YP\AJ
 Sample : Q1168-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 00:47:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.537	3.840	28523197	18654649	19.926	20.901
2)	SA Decachlor...	10.279	8.910	22714613	22214767	20.784	19.861
Target Compounds							
3)	L1 AR-1016-1	5.692	4.932	1961442	1361646	42.334	41.749
4)	L1 AR-1016-2	5.713	4.952	2816834	1923991	41.499	42.795
5)	L1 AR-1016-3	5.775	5.130	2416940	1089226	56.740	43.772
6)	L1 AR-1016-4	5.871	5.171	1710613	834480	48.874	41.319
7)	L1 AR-1016-5	6.167	5.387	1594360	1012921	48.228	37.762
8)	L2 AR-1221-1	4.736	4.050	713611	174835	37.520	14.193 #
9)	L2 AR-1221-2	4.840	4.143	677788	558489	49.501	57.675
10)	L2 AR-1221-3	4.899	4.216	1005030	705243	23.962	24.174
11)	L3 AR-1232-1	4.899	4.216	1005030	705243	30.187	30.037
12)	L3 AR-1232-2	5.425	4.952	1172772	1923991	71.764	81.623
13)	L3 AR-1232-3	5.713	5.130	2816834	1089226	81.983	84.128
14)	L3 AR-1232-4	5.871	5.214	1710613	992680	96.014	89.541
15)	L3 AR-1232-5	5.962	5.387	1075699	1012921	93.846	82.956
16)	L4 AR-1242-1	5.692	4.932	1961442	1361646	47.031	47.227
17)	L4 AR-1242-2	5.713	4.952	2816834	1923991	47.750	48.835
18)	L4 AR-1242-3	5.775	5.130	2416940	1089226	65.149	48.401 #
19)	L4 AR-1242-4	5.871	5.214	1710613	992680	52.161	45.995
20)	L4 AR-1242-5	6.541f	5.740	2300672	1145302	70.607	39.811 #
21)	L5 AR-1248-1	5.692	4.932	1961442	1361646	60.465	61.863
22)	L5 AR-1248-2	5.962	5.171	1075699	834480	25.343	27.756
23)	L5 AR-1248-3	6.167	5.214	1594360	992680	33.932	32.038
24)	L5 AR-1248-4	6.541	5.387	2300672	1012921	41.738	27.418 #
25)	L5 AR-1248-5	6.541f	5.740f	2300672	1145302	43.097	30.632 #
26)	L6 AR-1254-1	6.541	5.740	2300672	1145302	39.760	20.803 #
27)	L6 AR-1254-2	6.758	5.889	1052959	961026	13.122	19.869 #
28)	L6 AR-1254-3	7.121	6.311	713975	1804894	8.471	23.781 #
29)	L6 AR-1254-4	7.405	6.526	832071	349663	12.203	6.823 #
30)	L6 AR-1254-5	7.819	6.942	3574576	2509195	52.532	37.698 #
31)	L7 AR-1260-1	7.286	6.426	2479089	2050279	42.424	42.511
32)	L7 AR-1260-2	7.541	6.614	3921836	2683896	50.401	43.780
33)	L7 AR-1260-3	7.899	6.770	2478872	3496522	39.650	58.124 #
34)	L7 AR-1260-4	8.124	7.242	2983873	1866292	45.226	40.163
35)	L7 AR-1260-5	8.446	7.483	5307134	4491989	40.535	40.416
36)	L8 AR-1262-1	8.124	6.981	2983873	2071298	37.762	29.168
37)	L8 AR-1262-2	8.446	7.242	5307134	1866292	34.705	30.605
38)	L8 AR-1262-3	8.771	7.768	3354917	1286790	31.567	24.604
39)	L8 AR-1262-4	8.851	7.830	1080688	3393988	13.212	36.717 #
40)	L8 AR-1262-5	9.512	8.334	1664993	1276008	29.412	26.699
41)	L9 AR-1268-1	8.771	7.768	3354917	1286790	19.000	8.867 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
 Data File : PP069323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2025 15:32
 Operator : YP\AJ
 Sample : Q1168-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 00:47:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.851	7.830	1080688	3393988	6.867	25.554 #
43) L9	AR-1268-3	9.119	8.041	4288713	28981	32.070	0.255 #
44) L9	AR-1268-4	9.512	8.334	1664993	1276008	28.354	24.502
45) L9	AR-1268-5	9.933	8.640	515029	435163	1.352	1.222



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
Data File : PP069323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2025 15:32
Operator : YP\AJ
Sample : Q1168-07
Misc : AR1660 LOD 40 PPB
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 00:47:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

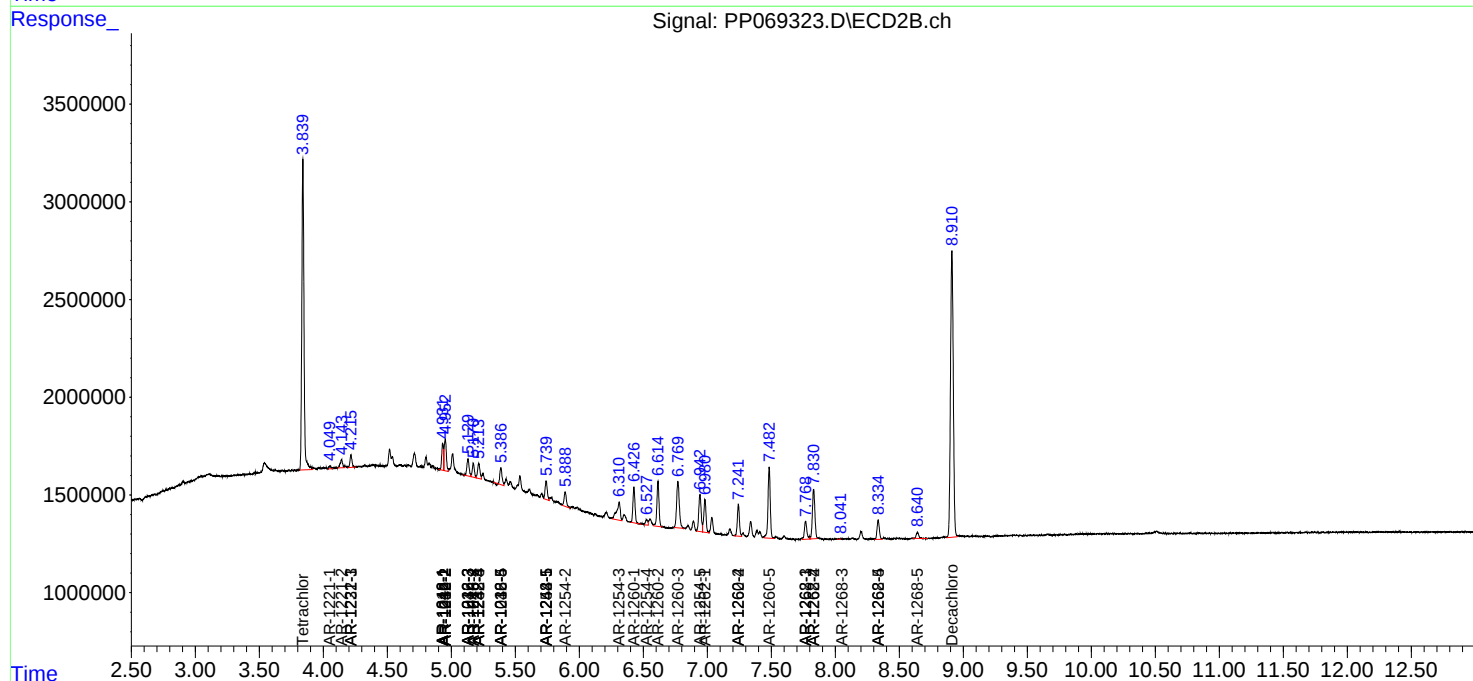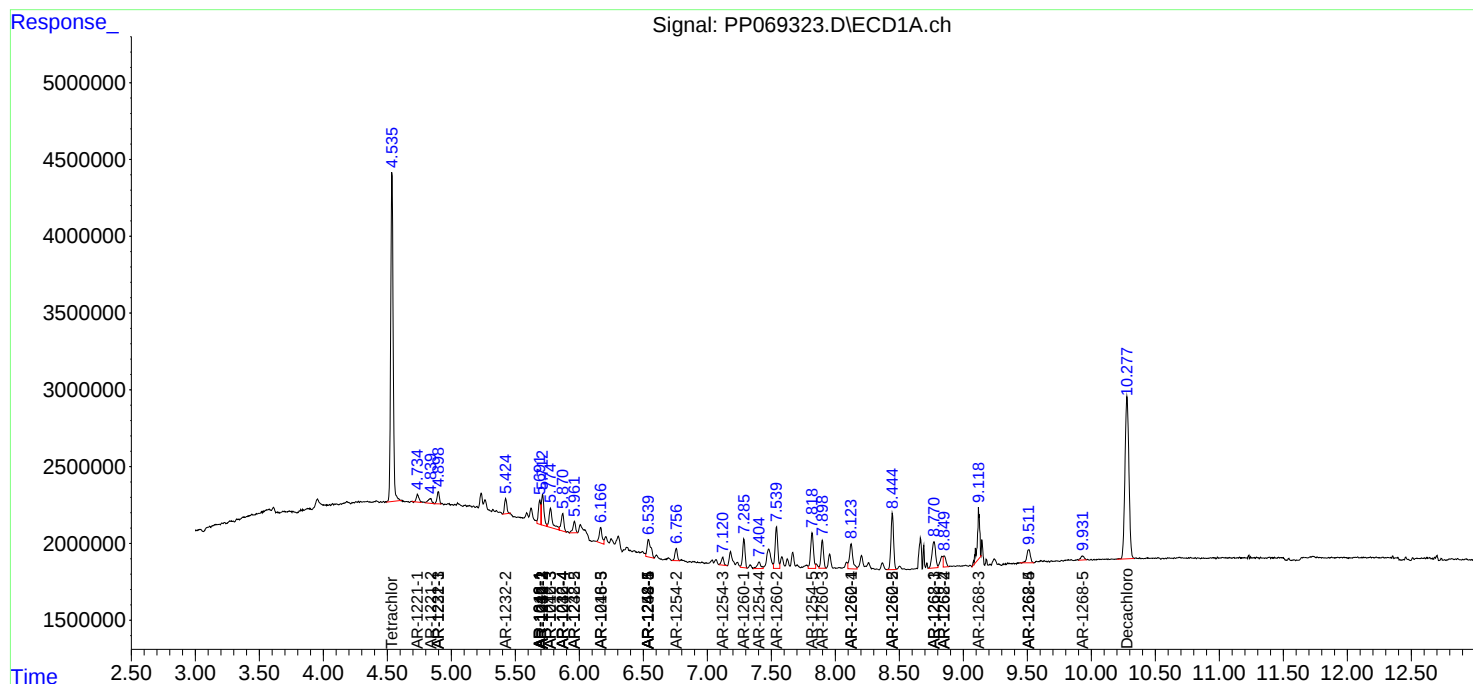


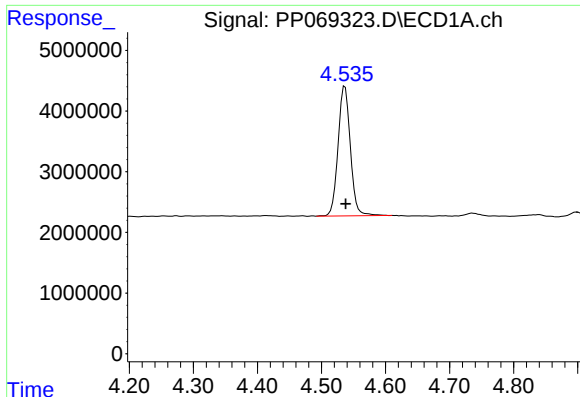

#1 Tetrachloro-m-xylene


R.T.: 4.537 min
Delta R.T.: -0.001 min
Response: 28523197
Conc: 19.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

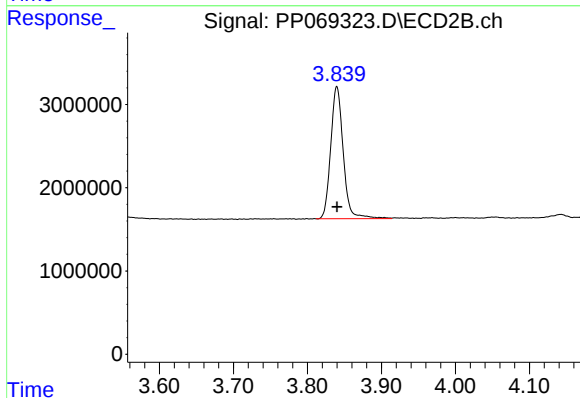


#1 Tetrachloro-m-xylene

R.T.: 3.840 min
Delta R.T.: 0.000 min
Response: 18654649
Conc: 20.90 ng/ml

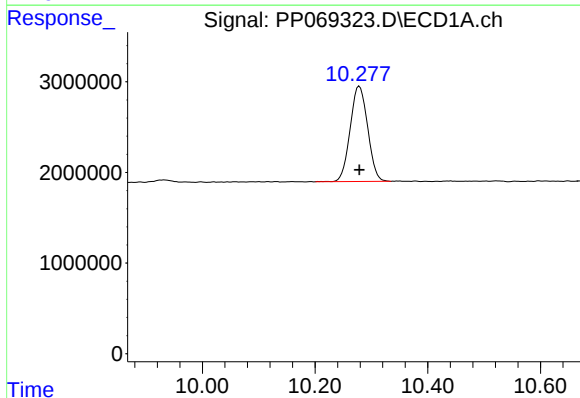


#2 Decachlorobiphenyl

R.T.: 10.279 min
Delta R.T.: 0.000 min
Response: 22714613
Conc: 20.78 ng/ml

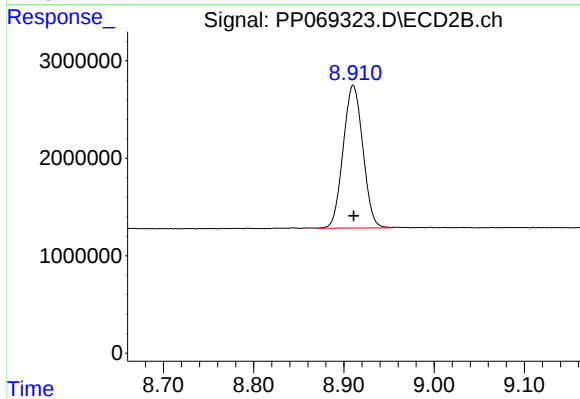

#2 Decachlorobiphenyl


R.T.: 8.910 min
Delta R.T.: 0.000 min
Response: 22214767
Conc: 19.86 ng/ml

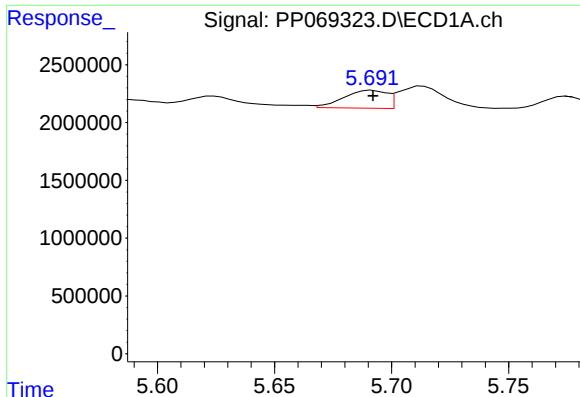

#3 AR-1016-1


R.T.: 5.692 min
Delta R.T.: 0.000 min
Response: 1961442
Conc: 42.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

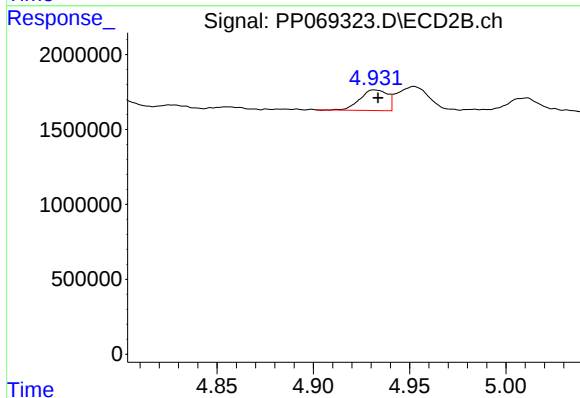


#3 AR-1016-1

R.T.: 4.932 min
Delta R.T.: -0.002 min
Response: 1361646
Conc: 41.75 ng/ml

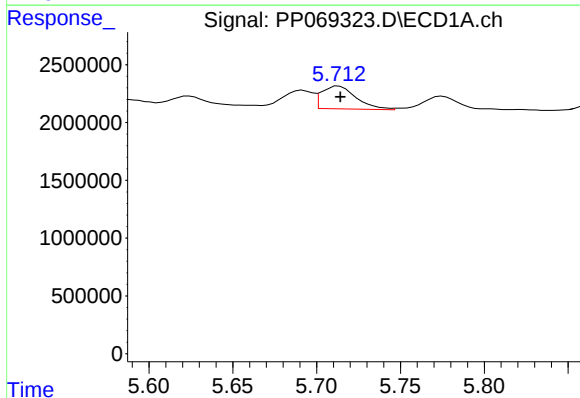


#4 AR-1016-2

R.T.: 5.713 min
Delta R.T.: 0.000 min
Response: 2816834
Conc: 41.50 ng/ml

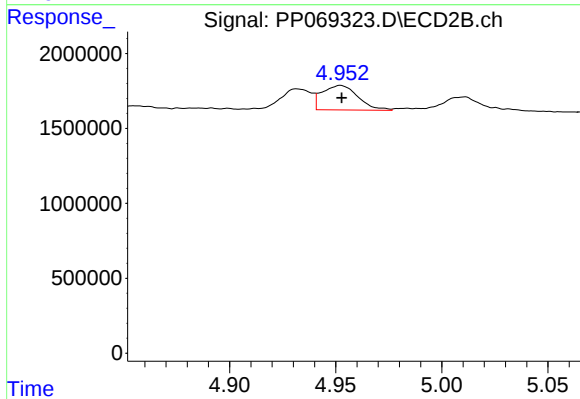

#4 AR-1016-2


R.T.: 4.952 min
Delta R.T.: 0.000 min
Response: 1923991
Conc: 42.79 ng/ml

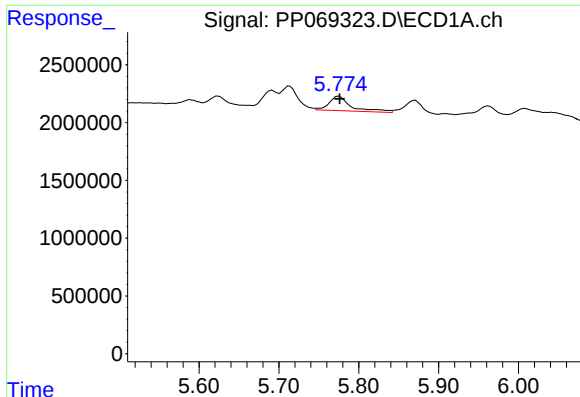

#5 AR-1016-3


R.T.: 5.775 min
Delta R.T.: -0.001 min
Response: 2416940
Conc: 56.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

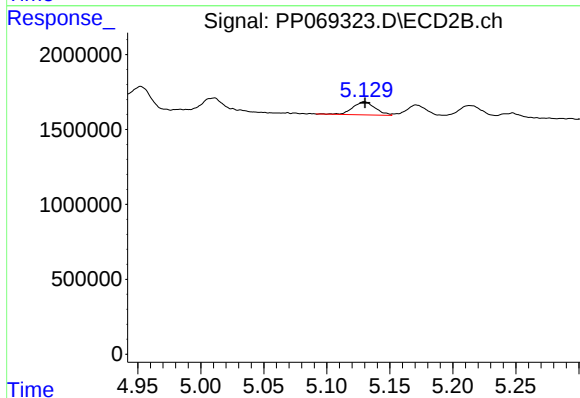


#5 AR-1016-3

R.T.: 5.130 min
Delta R.T.: 0.000 min
Response: 1089226
Conc: 43.77 ng/ml

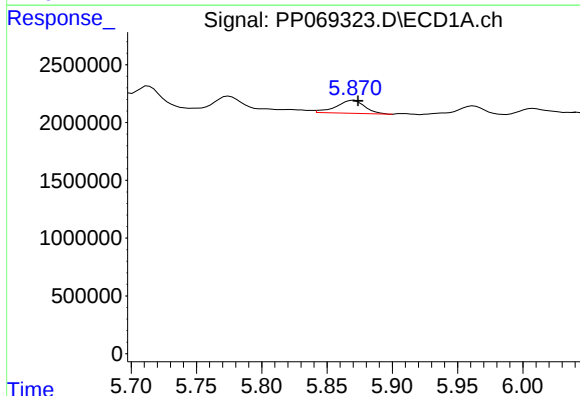


#6 AR-1016-4

R.T.: 5.871 min
Delta R.T.: -0.003 min
Response: 1710613
Conc: 48.87 ng/ml

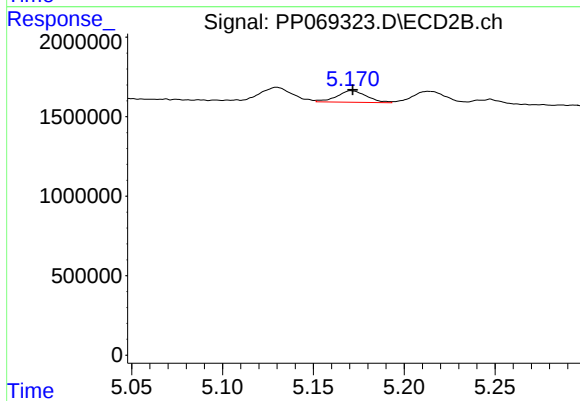

#6 AR-1016-4


R.T.: 5.171 min
Delta R.T.: 0.000 min
Response: 834480
Conc: 41.32 ng/ml

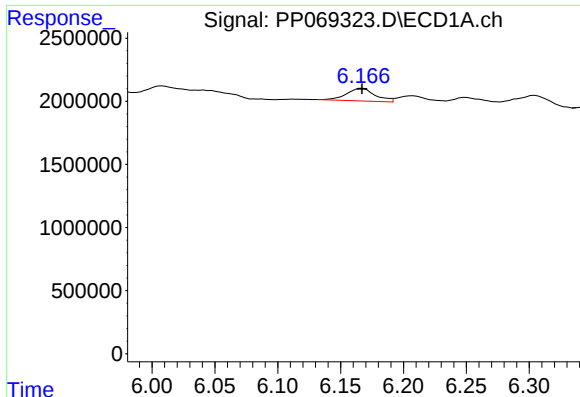

#7 AR-1016-5


R.T.: 6.167 min
Delta R.T.: 0.000 min
Response: 1594360
Conc: 48.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

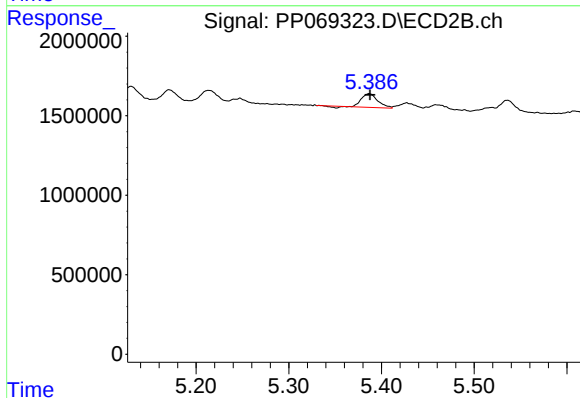


#7 AR-1016-5

R.T.: 5.387 min
Delta R.T.: -0.001 min
Response: 1012921
Conc: 37.76 ng/ml

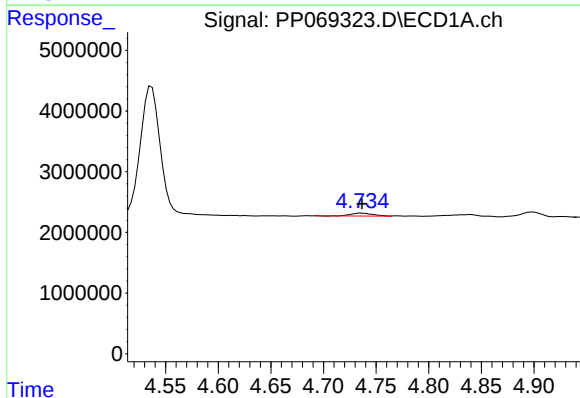


#8 AR-1221-1

R.T.: 4.736 min
Delta R.T.: 0.000 min
Response: 713611
Conc: 37.52 ng/ml

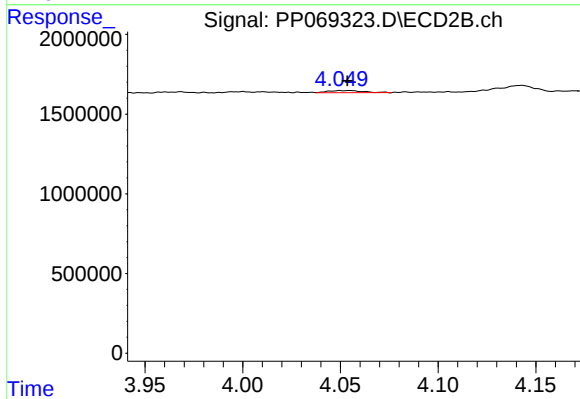

#8 AR-1221-1


R.T.: 4.050 min
Delta R.T.: -0.003 min
Response: 174835
Conc: 14.19 ng/ml

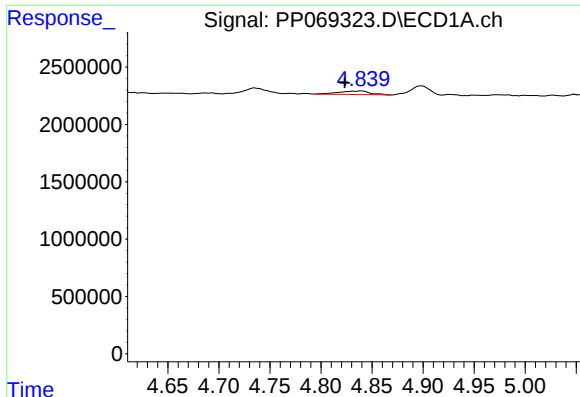

#9 AR-1221-2


R.T.: 4.840 min
Delta R.T.: 0.017 min
Response: 677788
Conc: 49.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

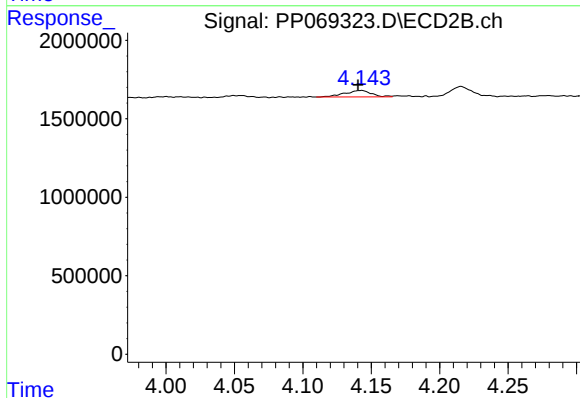


#9 AR-1221-2

R.T.: 4.143 min
Delta R.T.: 0.002 min
Response: 558489
Conc: 57.68 ng/ml

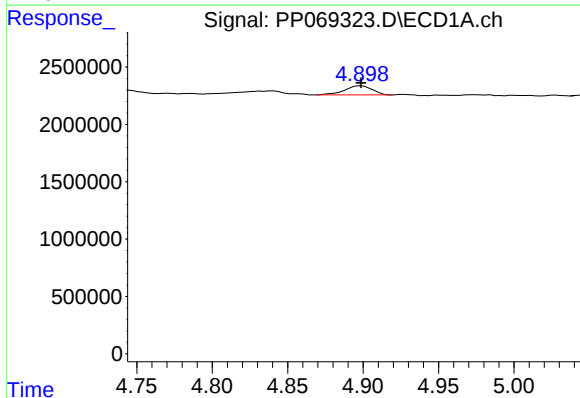


#10 AR-1221-3

R.T.: 4.899 min
Delta R.T.: 0.000 min
Response: 1005030
Conc: 23.96 ng/ml

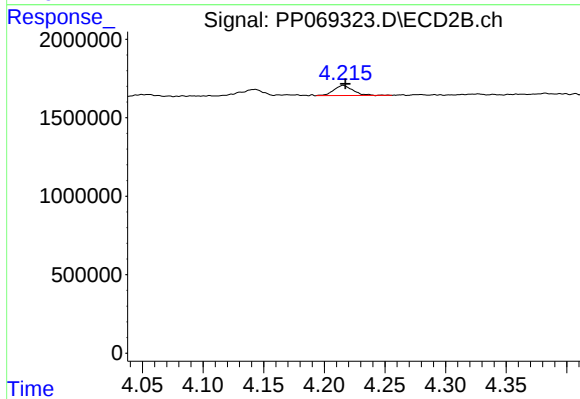

#10 AR-1221-3


R.T.: 4.216 min
Delta R.T.: -0.002 min
Response: 705243
Conc: 24.17 ng/ml

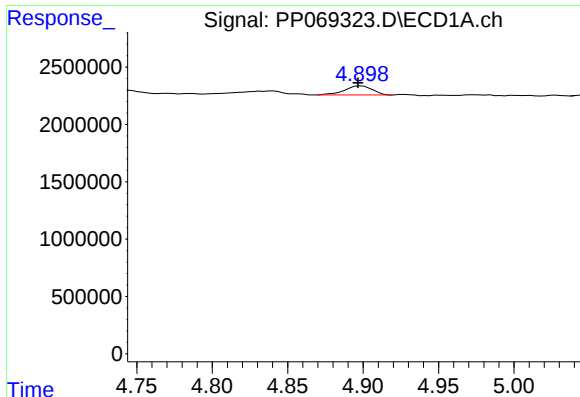

#11 AR-1232-1


R.T.: 4.899 min
Delta R.T.: 0.002 min
Response: 1005030
Conc: 30.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

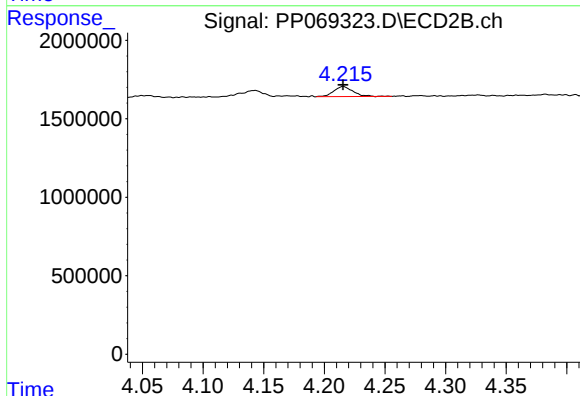


#11 AR-1232-1

R.T.: 4.216 min
Delta R.T.: 0.000 min
Response: 705243
Conc: 30.04 ng/ml

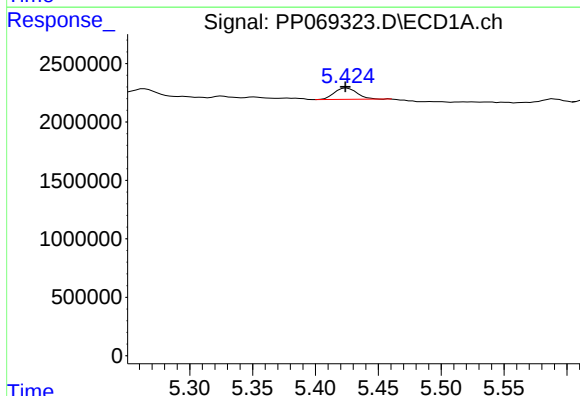


#12 AR-1232-2

R.T.: 5.425 min
Delta R.T.: 0.001 min
Response: 1172772
Conc: 71.76 ng/ml

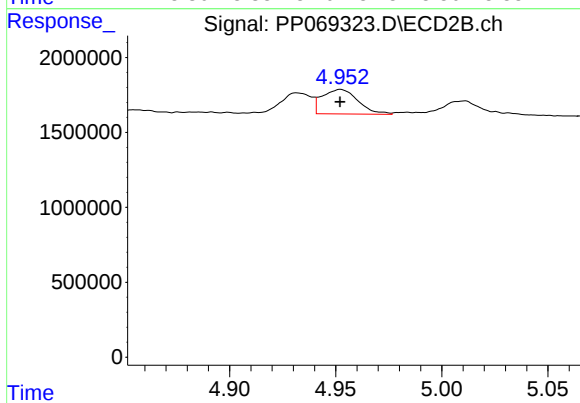

#12 AR-1232-2


R.T.: 4.952 min
Delta R.T.: 0.000 min
Response: 1923991
Conc: 81.62 ng/ml

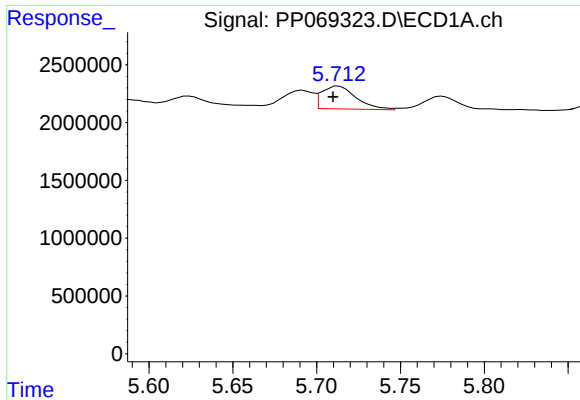

#13 AR-1232-3


R.T.: 5.713 min
Delta R.T.: 0.003 min
Response: 2816834
Conc: 81.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

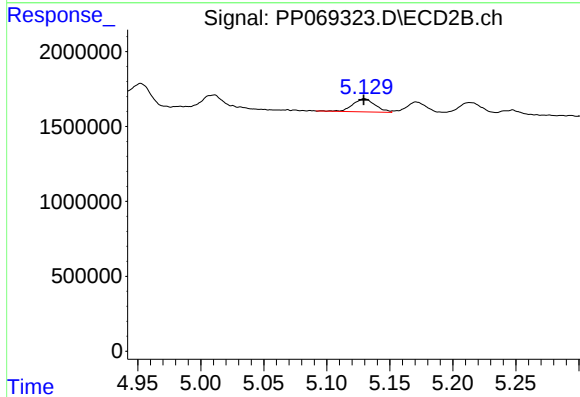


#13 AR-1232-3

R.T.: 5.130 min
Delta R.T.: 0.000 min
Response: 1089226
Conc: 84.13 ng/ml

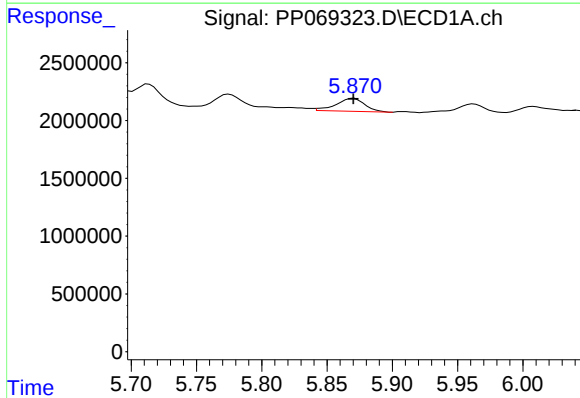


#14 AR-1232-4

R.T.: 5.871 min
Delta R.T.: 0.000 min
Response: 1710613
Conc: 96.01 ng/ml

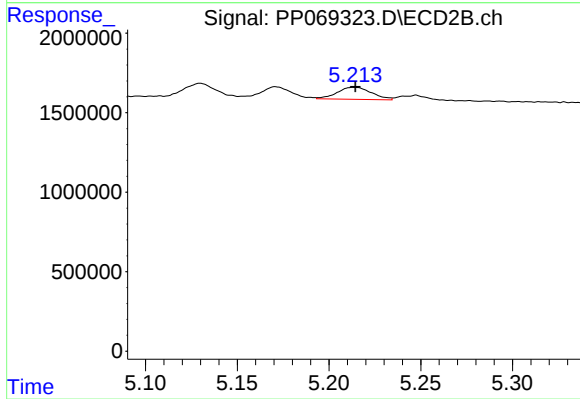

#14 AR-1232-4


R.T.: 5.214 min
Delta R.T.: 0.000 min
Response: 992680
Conc: 89.54 ng/ml

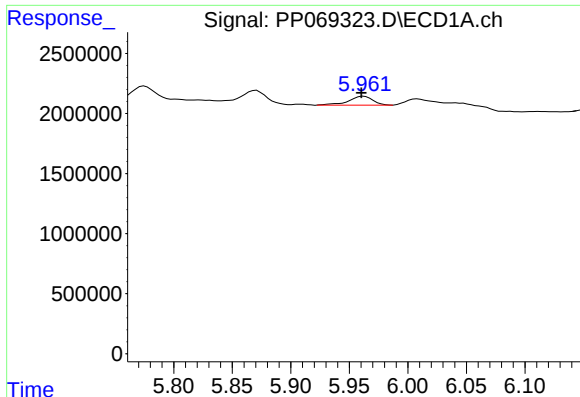

#15 AR-1232-5


R.T.: 5.962 min
Delta R.T.: 0.002 min
Response: 1075699
Conc: 93.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

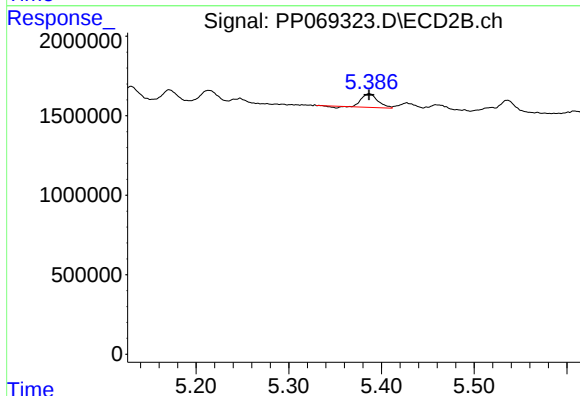


#15 AR-1232-5

R.T.: 5.387 min
Delta R.T.: 0.000 min
Response: 1012921
Conc: 82.96 ng/ml

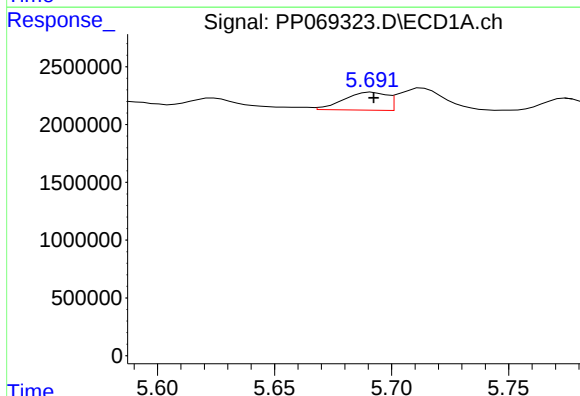


#16 AR-1242-1

R.T.: 5.692 min
Delta R.T.: 0.000 min
Response: 1961442
Conc: 47.03 ng/ml

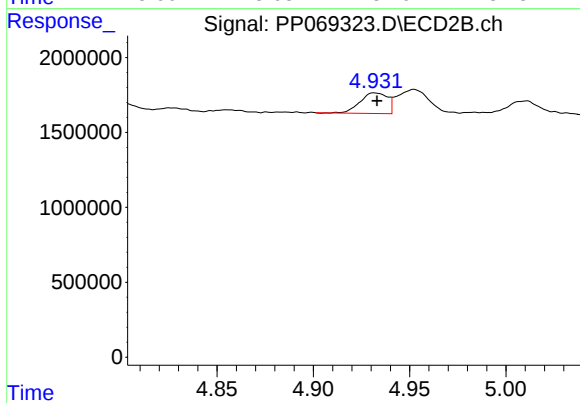

#16 AR-1242-1


R.T.: 4.932 min
Delta R.T.: -0.001 min
Response: 1361646
Conc: 47.23 ng/ml

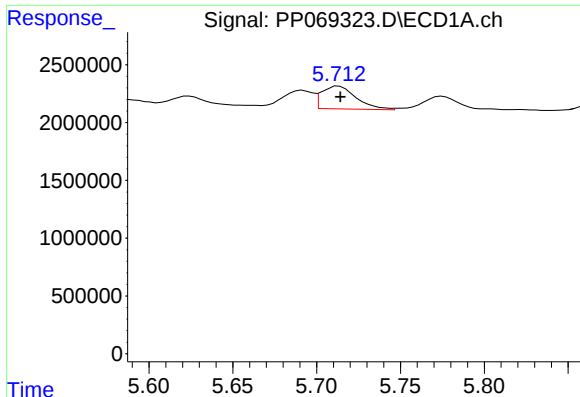

#17 AR-1242-2


R.T.: 5.713 min
Delta R.T.: 0.000 min
Response: 2816834
Conc: 47.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

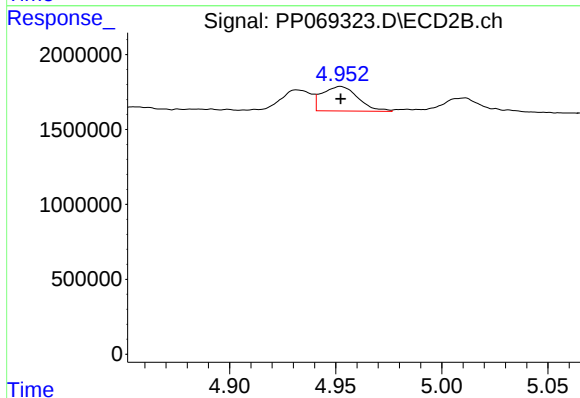


#17 AR-1242-2

R.T.: 4.952 min
Delta R.T.: 0.000 min
Response: 1923991
Conc: 48.84 ng/ml

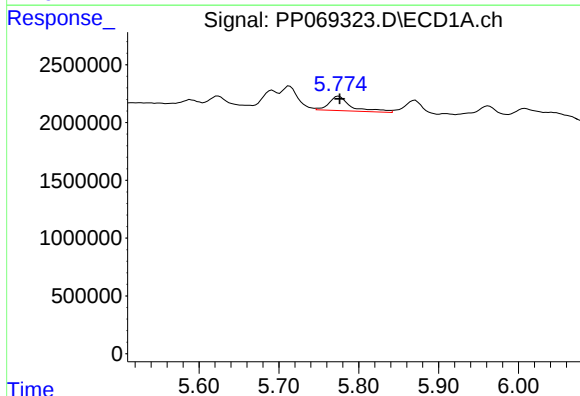


#18 AR-1242-3

R.T.: 5.775 min
Delta R.T.: -0.001 min
Response: 2416940
Conc: 65.15 ng/ml

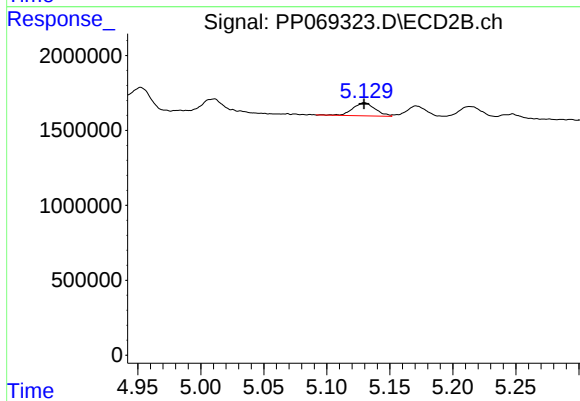

#18 AR-1242-3


R.T.: 5.130 min
Delta R.T.: 0.000 min
Response: 1089226
Conc: 48.40 ng/ml

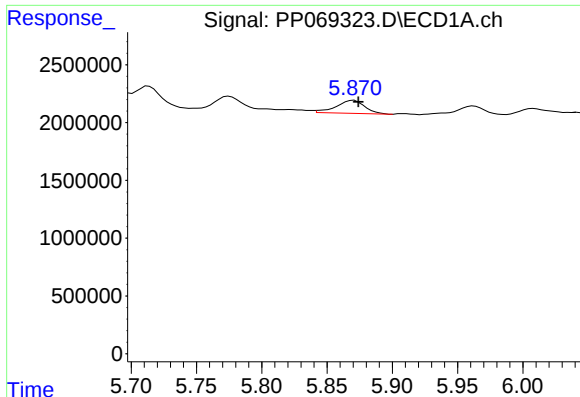

#19 AR-1242-4


R.T.: 5.871 min
Delta R.T.: -0.003 min
Response: 1710613
Conc: 52.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

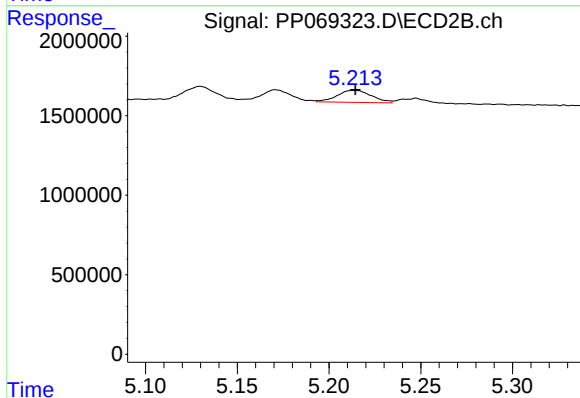


#19 AR-1242-4

R.T.: 5.214 min
Delta R.T.: 0.000 min
Response: 992680
Conc: 46.00 ng/ml

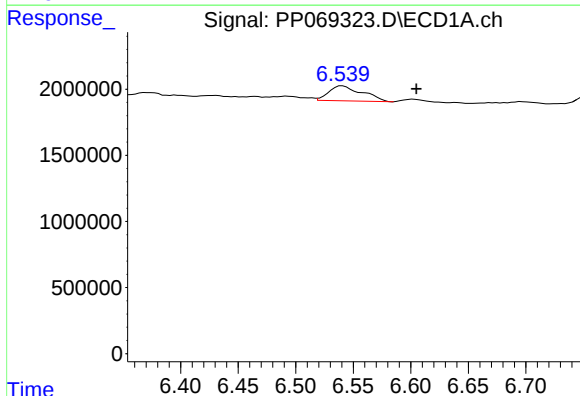


#20 AR-1242-5

R.T.: 6.541 min
Delta R.T.: -0.064 min
Response: 2300672
Conc: 70.61 ng/ml

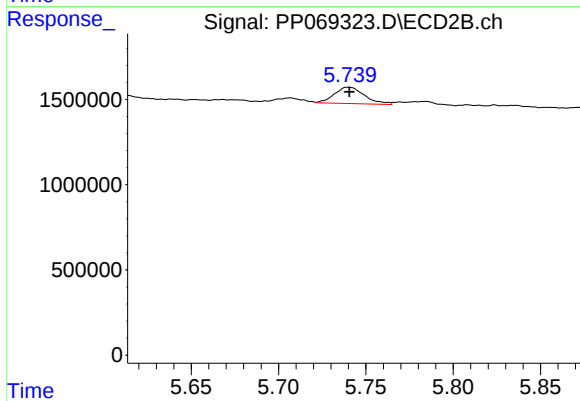

#20 AR-1242-5


R.T.: 5.740 min
Delta R.T.: 0.000 min
Response: 1145302
Conc: 39.81 ng/ml

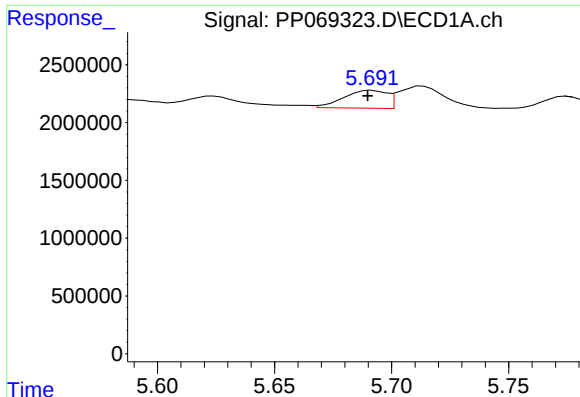

#21 AR-1248-1


R.T.: 5.692 min
Delta R.T.: 0.002 min
Response: 1961442
Conc: 60.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

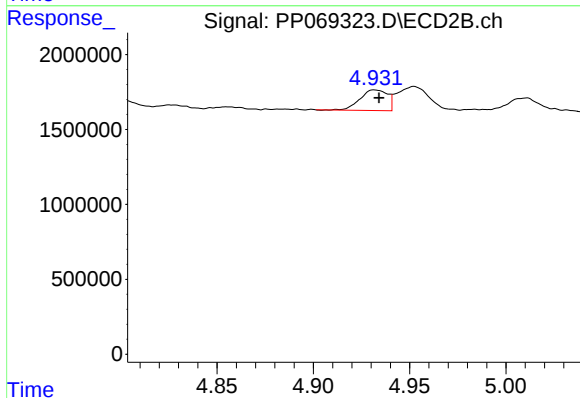


#21 AR-1248-1

R.T.: 4.932 min
Delta R.T.: -0.002 min
Response: 1361646
Conc: 61.86 ng/ml

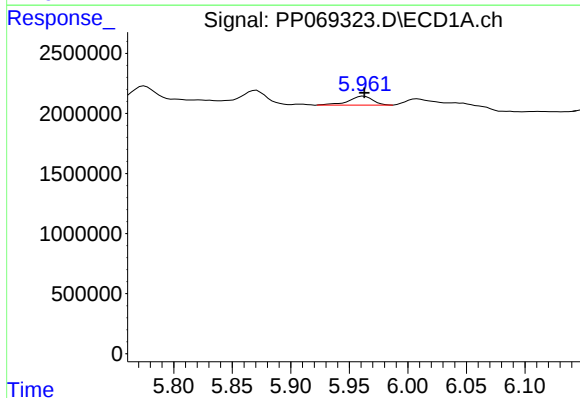


#22 AR-1248-2

R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 1075699
Conc: 25.34 ng/ml

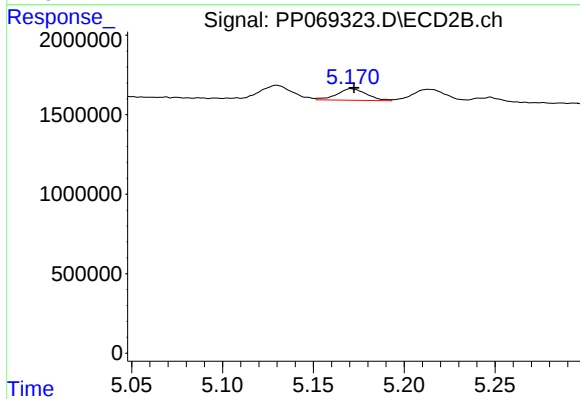

#22 AR-1248-2


R.T.: 5.171 min
Delta R.T.: -0.001 min
Response: 834480
Conc: 27.76 ng/ml

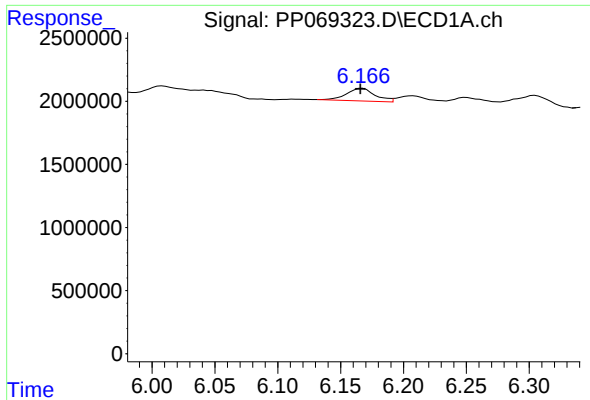

#23 AR-1248-3


R.T.: 6.167 min
Delta R.T.: 0.002 min
Response: 1594360
Conc: 33.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

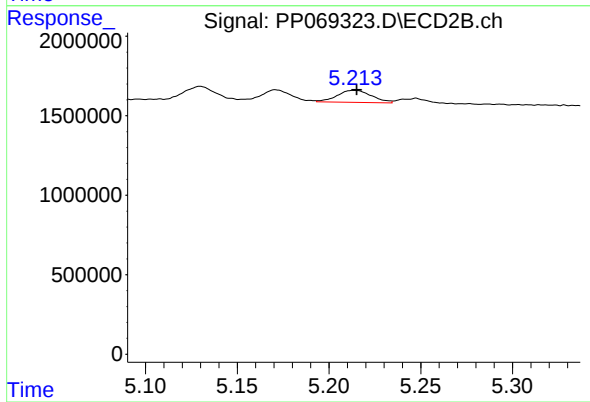


#23 AR-1248-3

R.T.: 5.214 min
Delta R.T.: -0.001 min
Response: 992680
Conc: 32.04 ng/ml

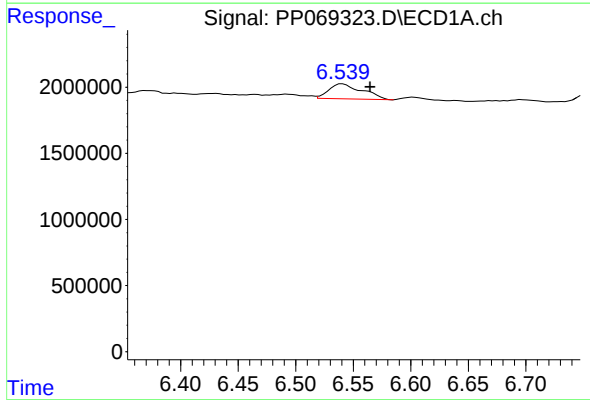


#24 AR-1248-4

R.T.: 6.541 min
Delta R.T.: -0.024 min
Response: 2300672
Conc: 41.74 ng/ml

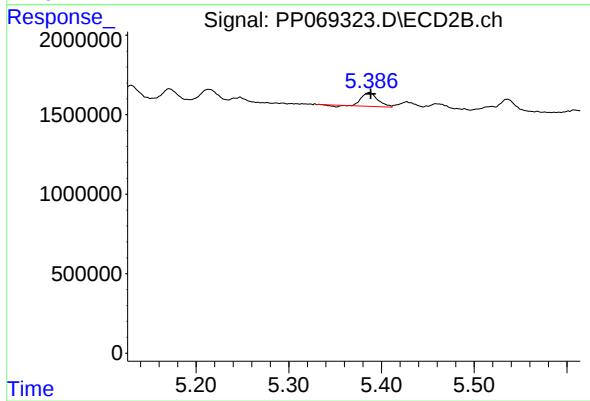

#24 AR-1248-4


R.T.: 5.387 min
Delta R.T.: -0.002 min
Response: 1012921
Conc: 27.42 ng/ml

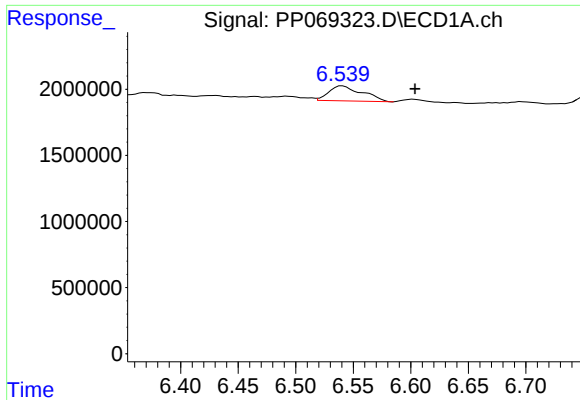

#25 AR-1248-5


R.T.: 6.541 min
Delta R.T.: -0.063 min
Response: 2300672
Conc: 43.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

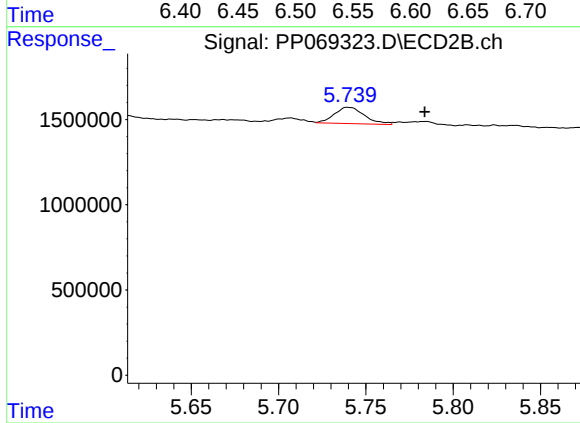


#25 AR-1248-5

R.T.: 5.740 min
Delta R.T.: -0.043 min
Response: 1145302
Conc: 30.63 ng/ml

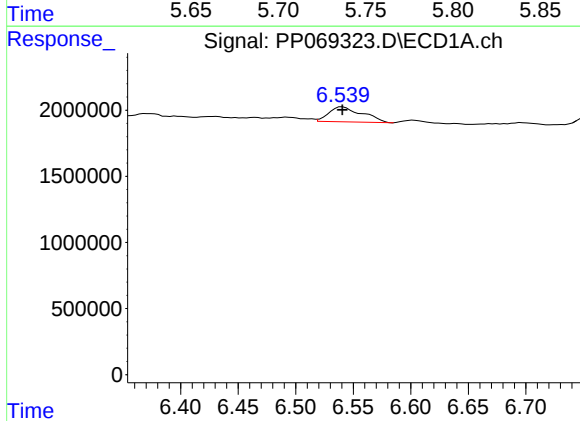


#26 AR-1254-1

R.T.: 6.541 min
Delta R.T.: 0.000 min
Response: 2300672
Conc: 39.76 ng/ml

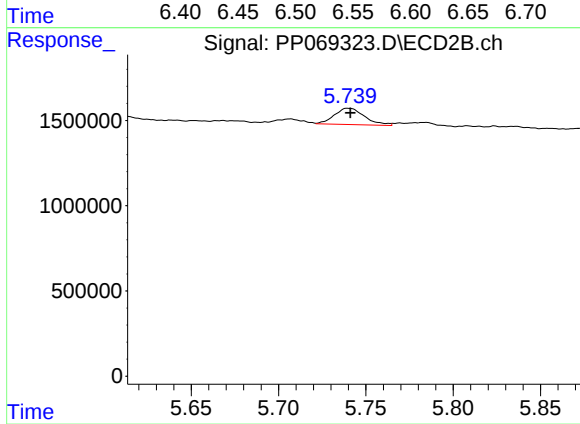

#26 AR-1254-1


R.T.: 5.740 min
Delta R.T.: 0.000 min
Response: 1145302
Conc: 20.80 ng/ml

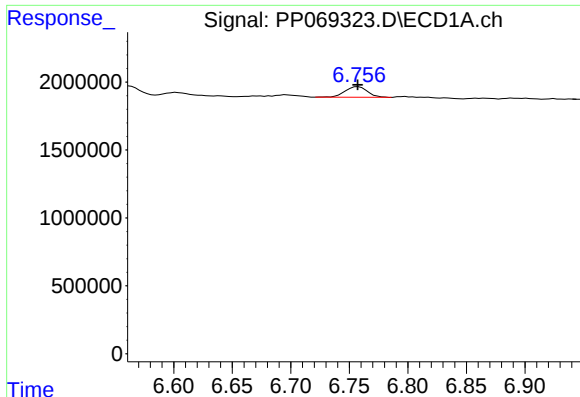

#27 AR-1254-2


R.T.: 6.758 min
Delta R.T.: 0.000 min
Response: 1052959
Conc: 13.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

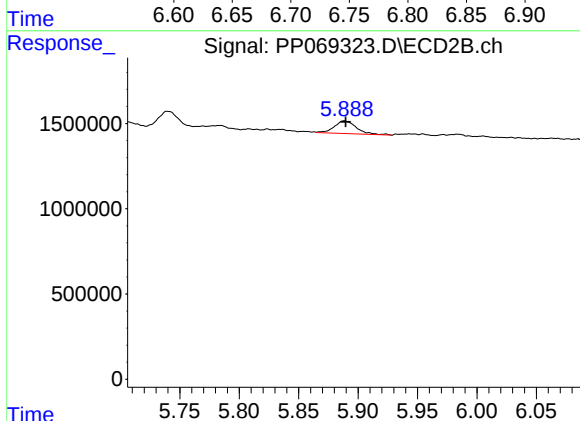


#27 AR-1254-2

R.T.: 5.889 min
Delta R.T.: -0.001 min
Response: 961026
Conc: 19.87 ng/ml

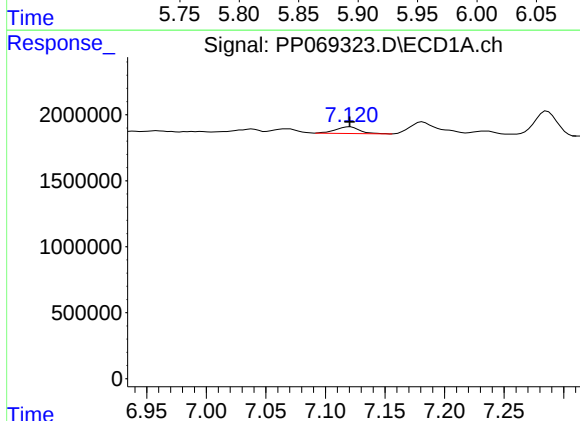


#28 AR-1254-3

R.T.: 7.121 min
Delta R.T.: 0.000 min
Response: 713975
Conc: 8.47 ng/ml

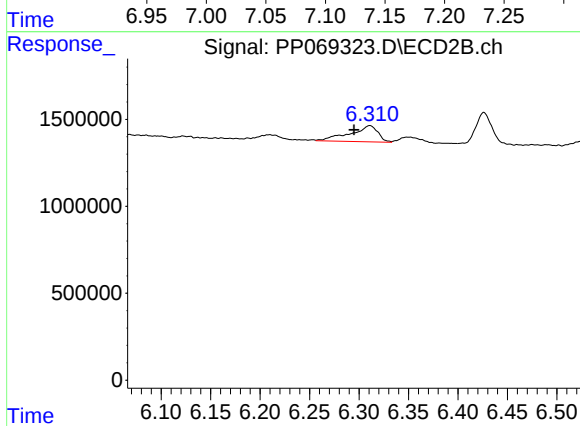

#28 AR-1254-3


R.T.: 6.311 min
Delta R.T.: 0.016 min
Response: 1804894
Conc: 23.78 ng/ml

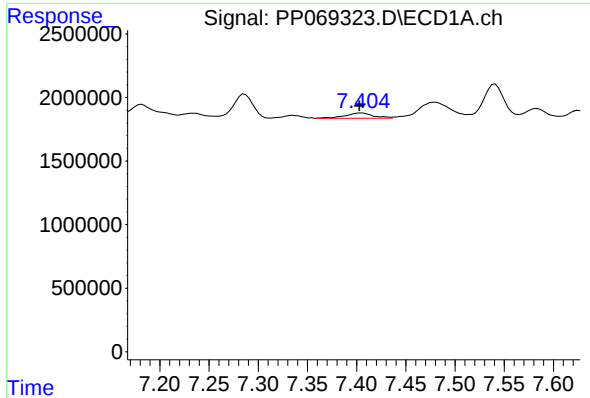

#29 AR-1254-4


R.T.: 7.405 min
Delta R.T.: 0.003 min
Response: 832071
Conc: 12.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

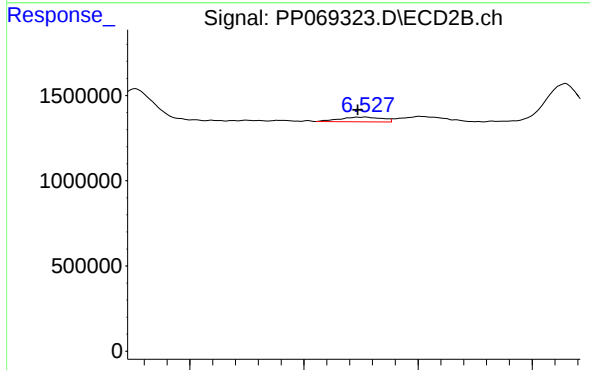


#29 AR-1254-4

R.T.: 6.526 min
Delta R.T.: 0.003 min
Response: 349663
Conc: 6.82 ng/ml

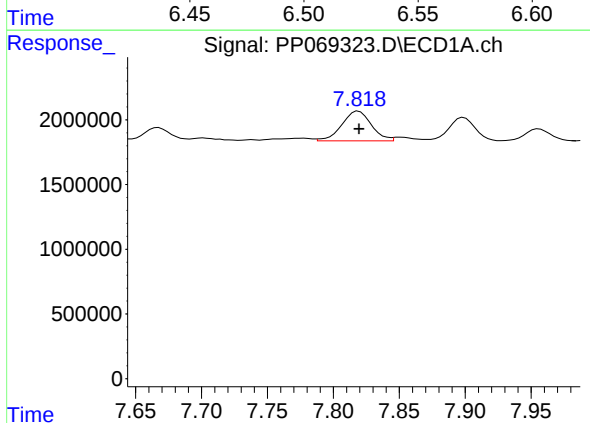


#30 AR-1254-5

R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 3574576
Conc: 52.53 ng/ml

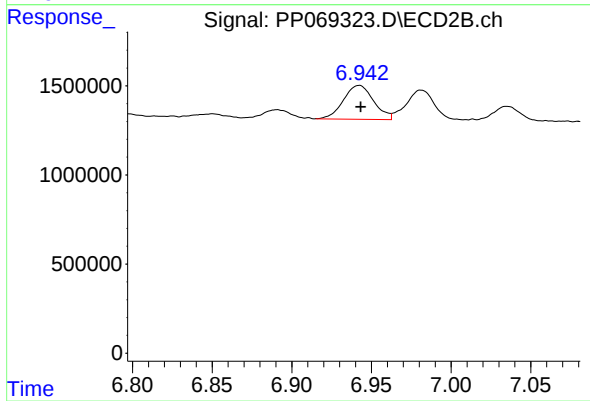

#30 AR-1254-5


R.T.: 6.942 min
Delta R.T.: 0.000 min
Response: 2509195
Conc: 37.70 ng/ml

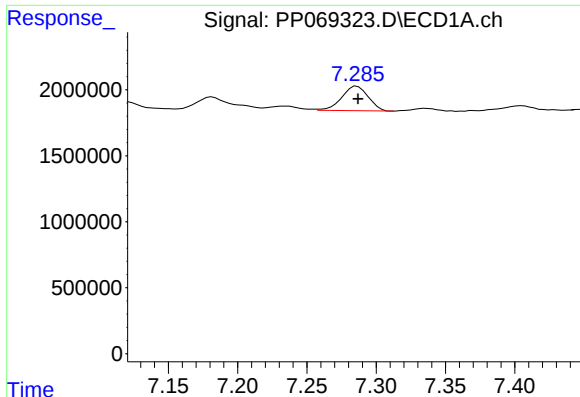

#31 AR-1260-1


R.T.: 7.286 min
Delta R.T.: 0.000 min
Response: 2479089
Conc: 42.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

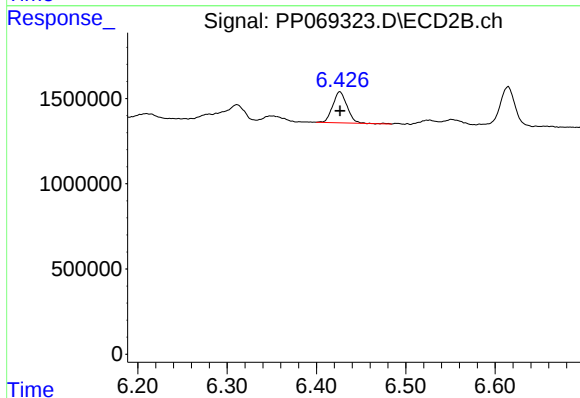


#31 AR-1260-1

R.T.: 6.426 min
Delta R.T.: 0.000 min
Response: 2050279
Conc: 42.51 ng/ml

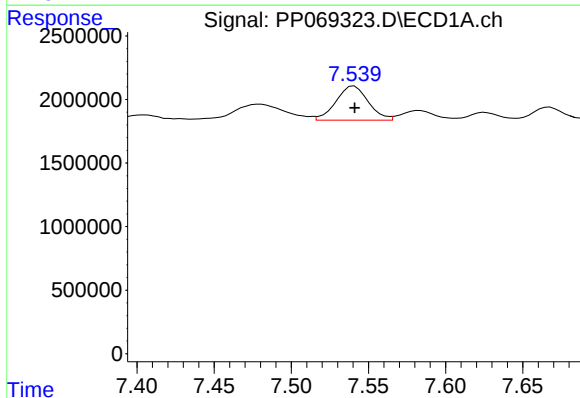


#32 AR-1260-2

R.T.: 7.541 min
Delta R.T.: 0.000 min
Response: 3921836
Conc: 50.40 ng/ml

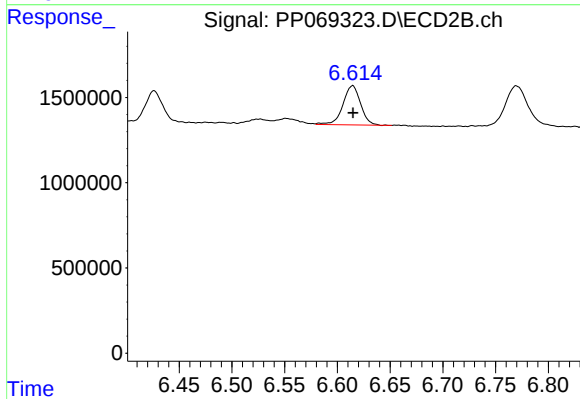

#32 AR-1260-2


R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 2683896
Conc: 43.78 ng/ml

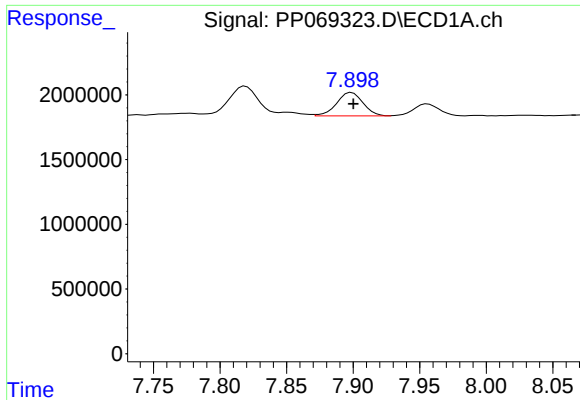

#33 AR-1260-3


R.T.: 7.899 min
Delta R.T.: -0.001 min
Response: 2478872
Conc: 39.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

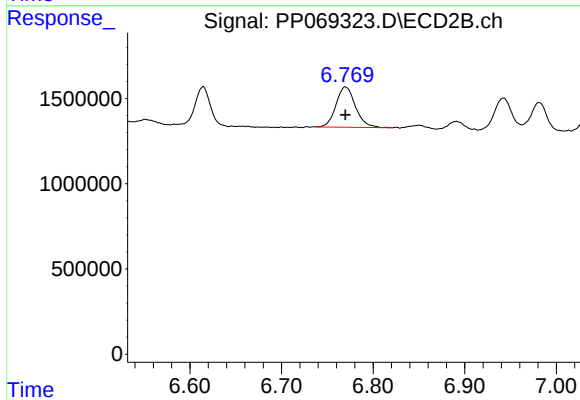


#33 AR-1260-3

R.T.: 6.770 min
Delta R.T.: 0.000 min
Response: 3496522
Conc: 58.12 ng/ml

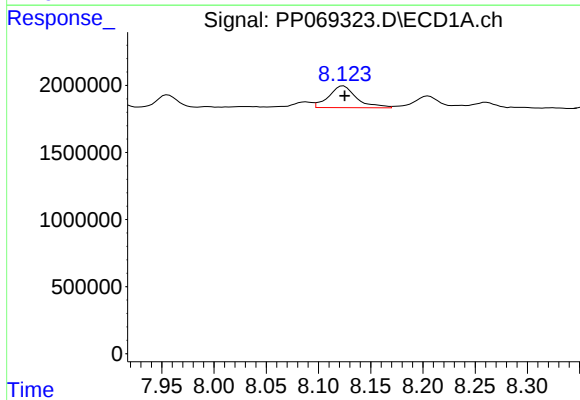


#34 AR-1260-4

R.T.: 8.124 min
Delta R.T.: -0.001 min
Response: 2983873
Conc: 45.23 ng/ml

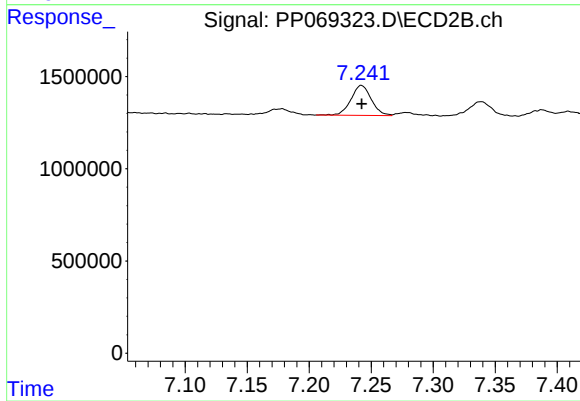

#34 AR-1260-4


R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 1866292
Conc: 40.16 ng/ml

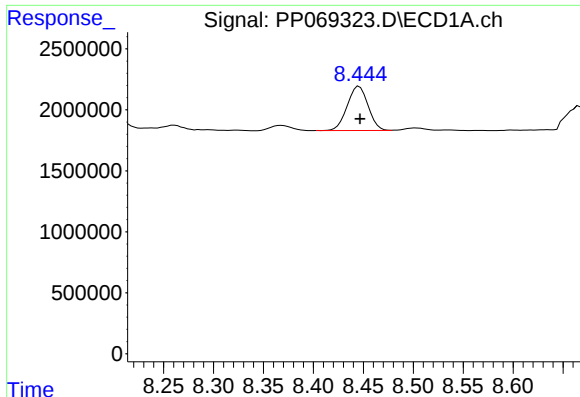

#35 AR-1260-5


R.T.: 8.446 min
Delta R.T.: 0.000 min
Response: 5307134
Conc: 40.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

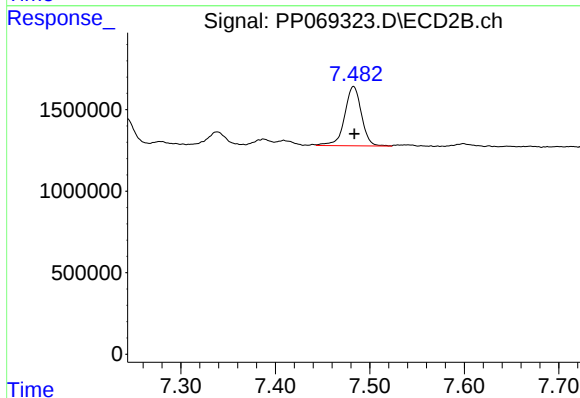


#35 AR-1260-5

R.T.: 7.483 min
Delta R.T.: 0.000 min
Response: 4491989
Conc: 40.42 ng/ml

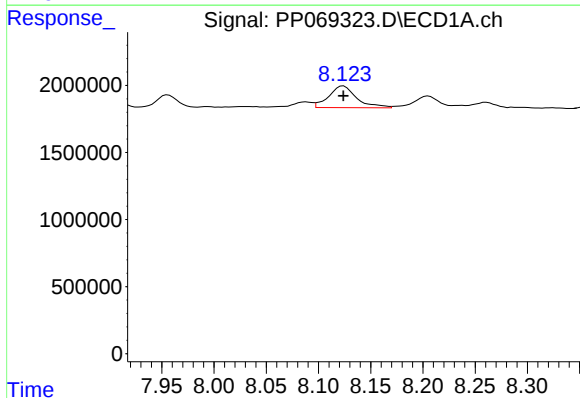


#36 AR-1262-1

R.T.: 8.124 min
Delta R.T.: 0.000 min
Response: 2983873
Conc: 37.76 ng/ml

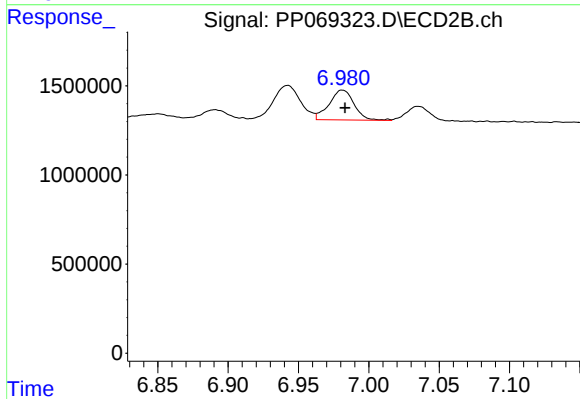

#36 AR-1262-1


R.T.: 6.981 min
Delta R.T.: -0.002 min
Response: 2071298
Conc: 29.17 ng/ml

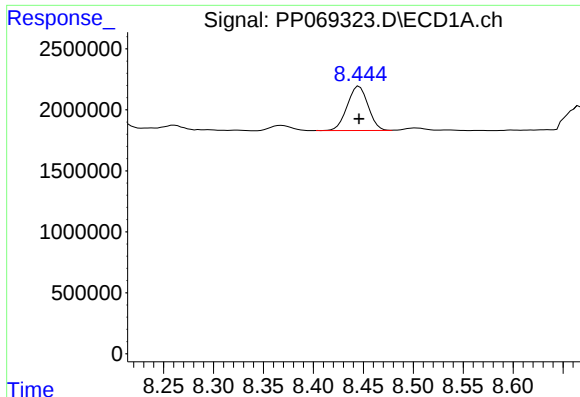

#37 AR-1262-2


R.T.: 8.446 min
Delta R.T.: 0.000 min
Response: 5307134
Conc: 34.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

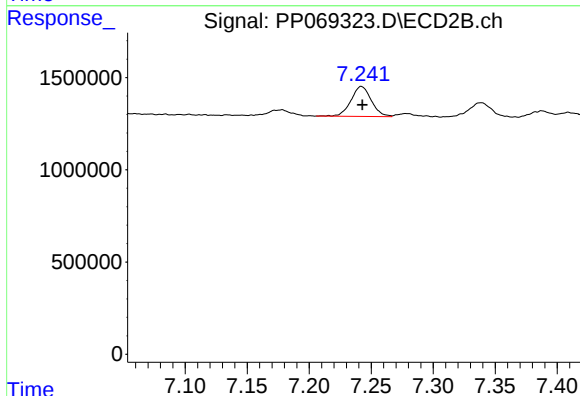


#37 AR-1262-2

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 1866292
Conc: 30.61 ng/ml

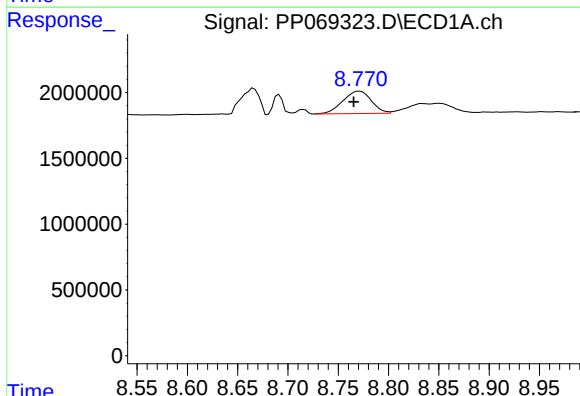


#38 AR-1262-3

R.T.: 8.771 min
Delta R.T.: 0.006 min
Response: 3354917
Conc: 31.57 ng/ml

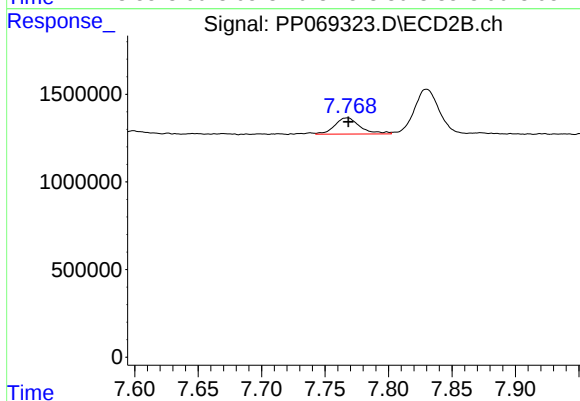

#38 AR-1262-3


R.T.: 7.768 min
Delta R.T.: 0.000 min
Response: 1286790
Conc: 24.60 ng/ml

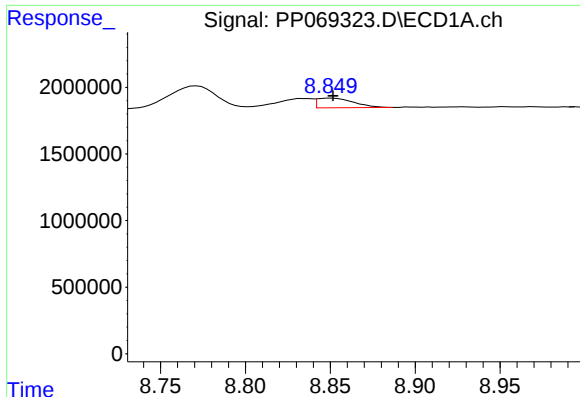

#39 AR-1262-4


R.T.: 8.851 min
Delta R.T.: -0.001 min
Response: 1080688
Conc: 13.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

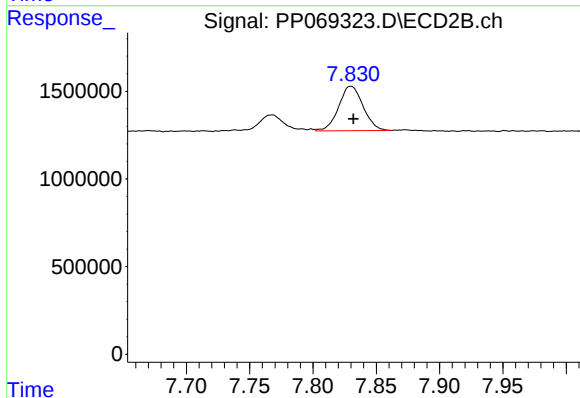


#39 AR-1262-4

R.T.: 7.830 min
Delta R.T.: -0.002 min
Response: 3393988
Conc: 36.72 ng/ml

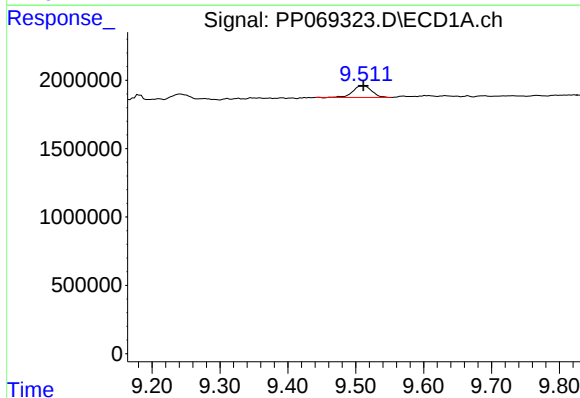


#40 AR-1262-5

R.T.: 9.512 min
Delta R.T.: 0.001 min
Response: 1664993
Conc: 29.41 ng/ml

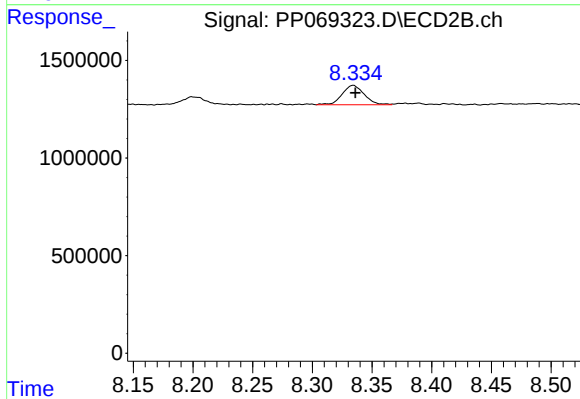

#40 AR-1262-5


R.T.: 8.334 min
Delta R.T.: -0.002 min
Response: 1276008
Conc: 26.70 ng/ml

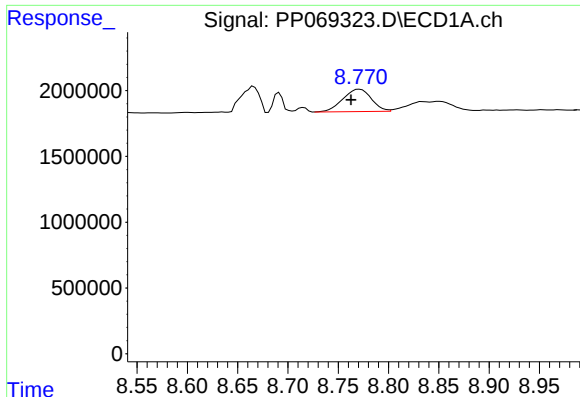

#41 AR-1268-1


R.T.: 8.771 min
Delta R.T.: 0.008 min
Response: 3354917
Conc: 19.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

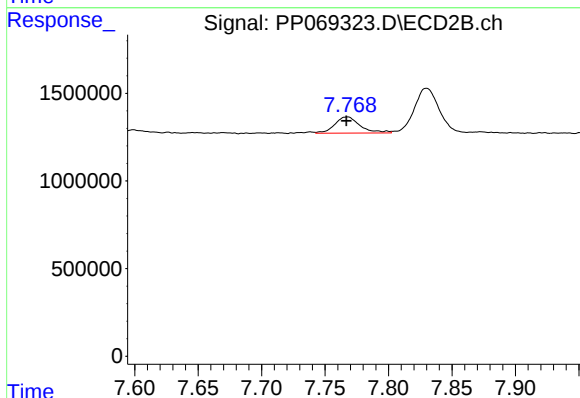


#41 AR-1268-1

R.T.: 7.768 min
Delta R.T.: 0.000 min
Response: 1286790
Conc: 8.87 ng/ml

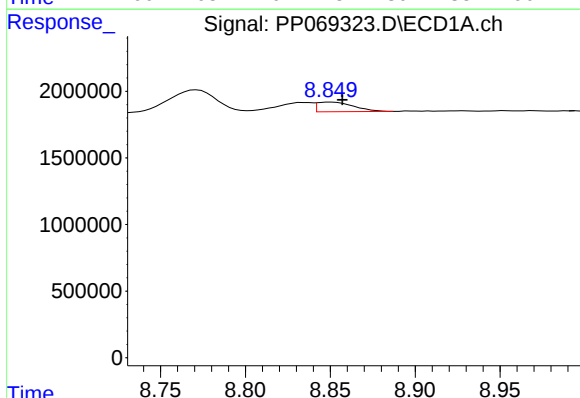


#42 AR-1268-2

R.T.: 8.851 min
Delta R.T.: -0.007 min
Response: 1080688
Conc: 6.87 ng/ml

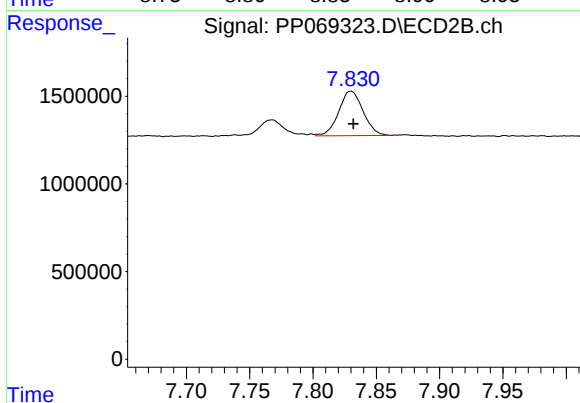

#42 AR-1268-2


R.T.: 7.830 min
Delta R.T.: -0.002 min
Response: 3393988
Conc: 25.55 ng/ml

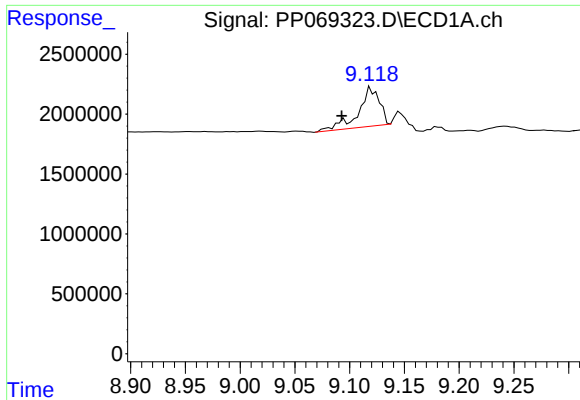

#43 AR-1268-3


R.T.: 9.119 min
Delta R.T.: 0.026 min
Response: 4288713
Conc: 32.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

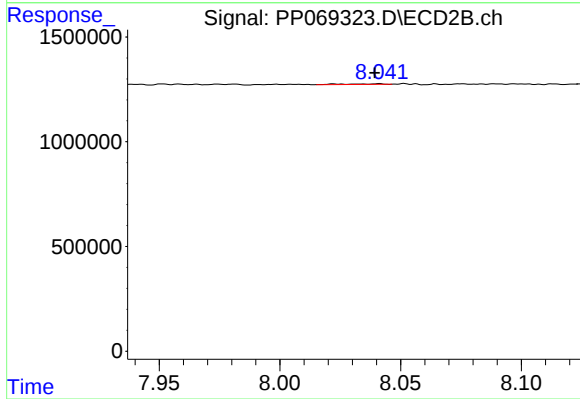


#43 AR-1268-3

R.T.: 8.041 min
Delta R.T.: 0.002 min
Response: 28981
Conc: 0.25 ng/ml

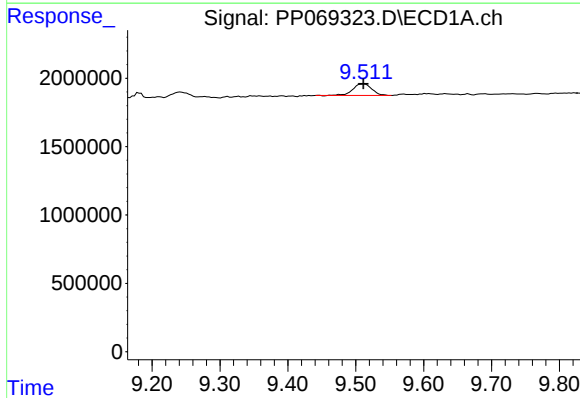


#44 AR-1268-4

R.T.: 9.512 min
Delta R.T.: 0.000 min
Response: 1664993
Conc: 28.35 ng/ml

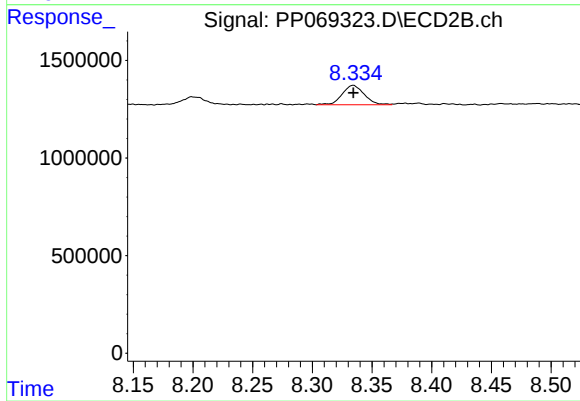

#44 AR-1268-4


R.T.: 8.334 min
Delta R.T.: 0.000 min
Response: 1276008
Conc: 24.50 ng/ml

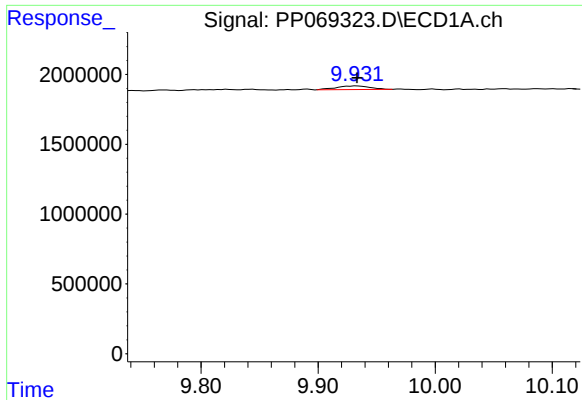

#45 AR-1268-5

R.T.: 9.933 min
Delta R.T.: 0.000 min
Response: 515029
Conc: 1.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

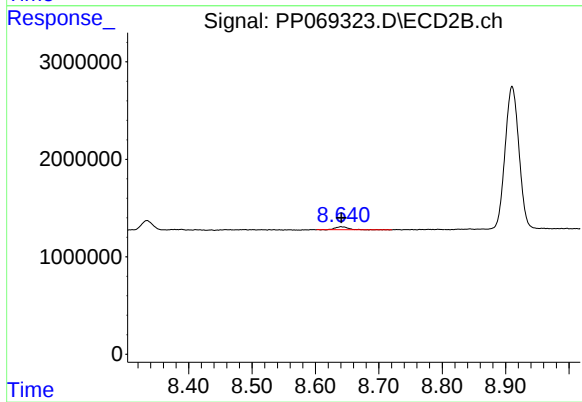

#45 AR-1268-5

R.T.: 8.640 min
Delta R.T.: 0.000 min
Response: 435163
Conc: 1.22 ng/ml