

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
 Data File : PP069327.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2025 16:37
 Operator : YP\AJ
 Sample : Q1168-07
 Misc : AR1248 LOD 40 PPB
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 00:49:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.536	3.841	28596886	18254865	19.977	20.453
2)	SA Decachlor...	10.276	8.909	22962240	23865404	21.010	21.337
Target Compounds							
3)	L1 AR-1016-1	5.690	4.933	1413762	782039	30.513	23.978
4)	L1 AR-1016-2	5.713	4.953	1910703	790661	28.149	17.586 #
5)	L1 AR-1016-3	5.772	5.130	1322650	562442	31.051	22.603 #
6)	L1 AR-1016-4	5.872	5.172	692955	1169387	19.798	57.901 #
7)	L1 AR-1016-5	6.166	5.386	1886237	1665244	57.057	62.081
8)	L2 AR-1221-1	0.000	4.049	0	37936	N.D.	3.080 #
9)	L2 AR-1221-2	4.837	4.145	514881	513366	37.603	53.015 #
10)	L2 AR-1221-3	4.837f	4.215	514881	89502	12.276	3.068 #
11)	L3 AR-1232-1	4.837f	4.215	514881	89502	15.465	3.812 #
12)	L3 AR-1232-2	5.423	4.953	362281	790661	22.169	33.543 #
13)	L3 AR-1232-3	5.713	5.130	1910703	562442	55.610	43.441
14)	L3 AR-1232-4	5.872	5.214	692955	1145852	38.895	103.357 #
15)	L3 AR-1232-5	5.962	5.386	1497118	1665244	130.611	136.380
16)	L4 AR-1242-1	5.690	4.933	1413762	782039	33.899	27.124
17)	L4 AR-1242-2	5.713	4.953	1910703	790661	32.390	20.069 #
18)	L4 AR-1242-3	5.772	5.130	1322650	562442	35.652	24.993 #
19)	L4 AR-1242-4	5.872	5.214	692955	1145852	21.130	53.092 #
20)	L4 AR-1242-5	6.603	5.740	2047530	2112602	62.838	73.435
21)	L5 AR-1248-1	5.690	4.933	1413762	782039	43.582	35.530
22)	L5 AR-1248-2	5.962	5.172	1497118	1169387	35.271	38.896
23)	L5 AR-1248-3	6.166	5.214	1886237	1145852	40.144	36.982
24)	L5 AR-1248-4	6.563	5.386	2277371	1665244	41.316	45.075
25)	L5 AR-1248-5	6.603	5.781	2047530	1561905	38.355	41.774
26)	L6 AR-1254-1	6.538	5.740	2044348	2112602	35.330	38.372
27)	L6 AR-1254-2	6.760	5.888	2235329	731996	27.857	15.134 #
28)	L6 AR-1254-3	7.120	6.295	1423876	1021006	16.893	13.453
29)	L6 AR-1254-4	7.404	6.525	1127388	848133	16.534	16.549
30)	L6 AR-1254-5	0.000	6.943	0	171904	N.D.	2.583 #
31)	L7 AR-1260-1	7.245f	6.412	473565	164809	8.104	3.417 #
32)	L7 AR-1260-2	7.549	6.606	841500	324396	10.814	5.292 #
33)	L7 AR-1260-3	0.000	6.769	0	1365414	N.D.	22.698 #
34)	L7 AR-1260-4	0.000	7.274	0	97072	N.D.	2.089 #
36)	L8 AR-1262-1	0.000	6.943f	0	171904	N.D.	2.421 #
37)	L8 AR-1262-2	0.000	7.274	0	97072	N.D.	1.592 #
38)	L8 AR-1262-3	0.000	7.774	0	218787	N.D.	4.183 #
39)	L8 AR-1262-4	0.000	7.825	0	139312	N.D.	1.507 #
40)	L8 AR-1262-5	0.000	8.390f	0	136667	N.D.	2.860 #
41)	L9 AR-1268-1	0.000	7.774	0	218787	N.D.	1.508 #
42)	L9 AR-1268-2	0.000	7.825	0	139312	N.D.	1.049 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
Data File : PP069327.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2025 16:37
Operator : YP\AJ
Sample : Q1168-07
Misc : AR1248 LOD 40 PPB
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 00:49:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	8.048	0	82976	N.D.	0.730 #
44) L9	AR-1268-4	0.000	8.390f	0	136667	N.D.	2.624 #
45) L9	AR-1268-5	0.000	8.640	0	174303	N.D.	0.489 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
Data File : PP069327.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2025 16:37
Operator : YP\AJ
Sample : Q1168-07
Misc : AR1248 LOD 40 PPB
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 00:49:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

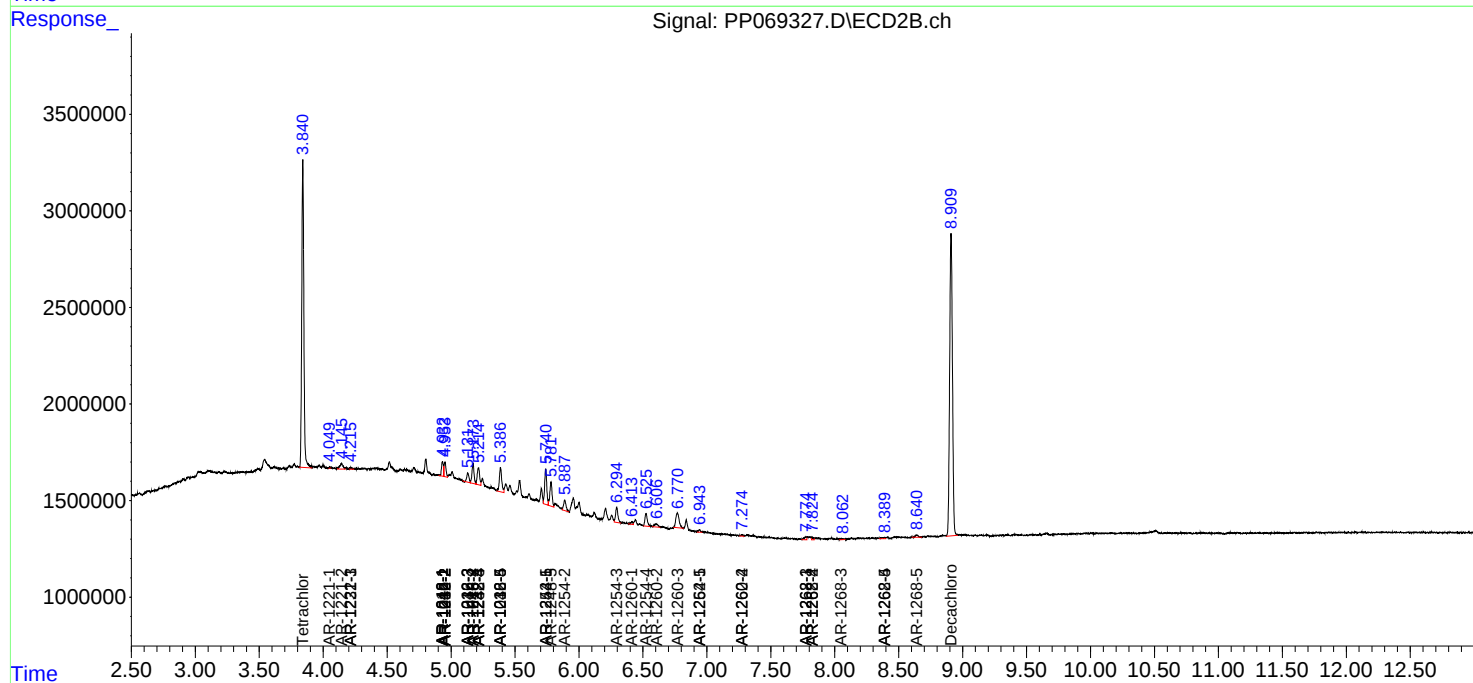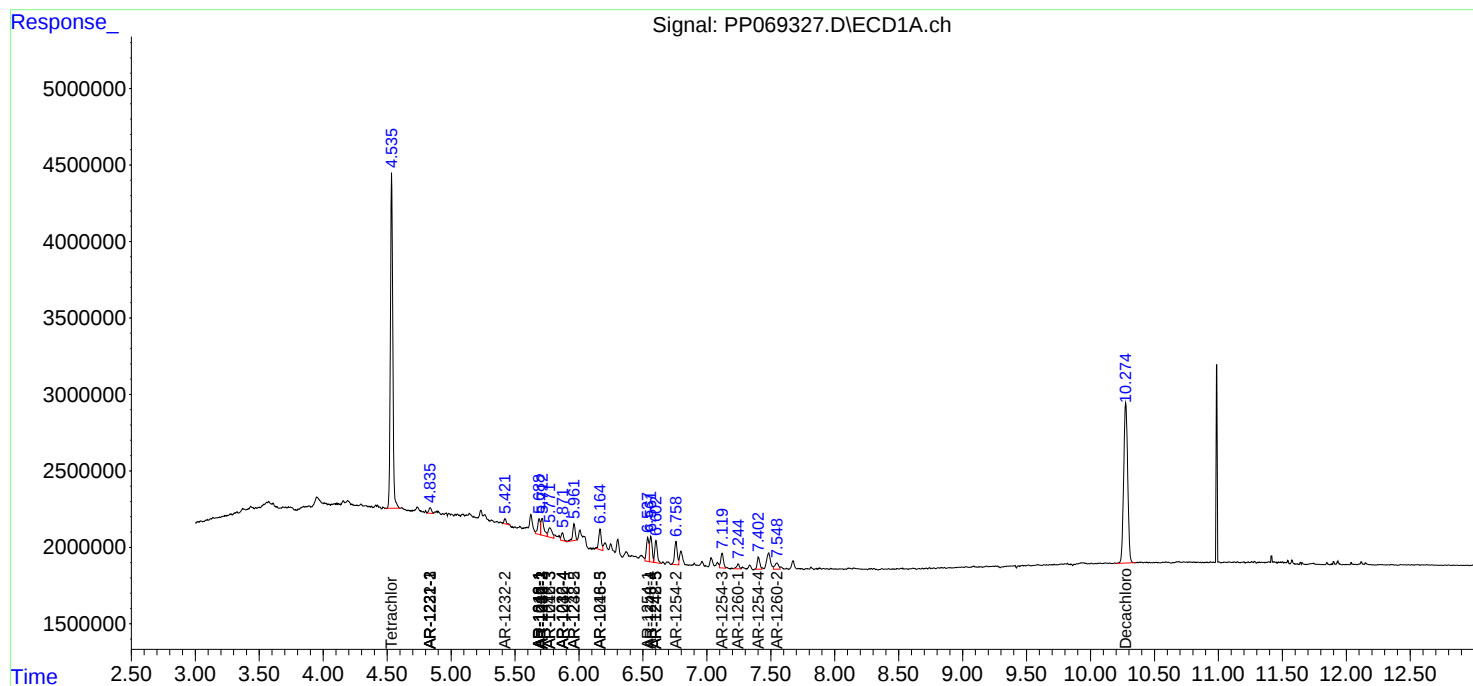


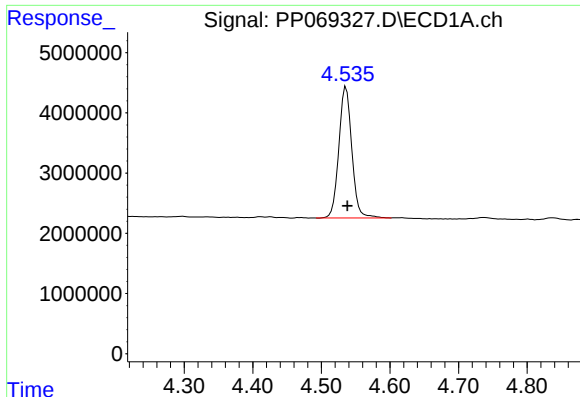

#1 Tetrachloro-m-xylene


R.T.: 4.536 min
Delta R.T.: -0.002 min
Response: 28596886
Conc: 19.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

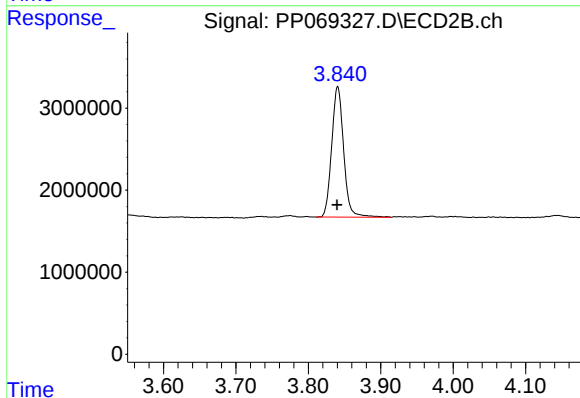


#1 Tetrachloro-m-xylene

R.T.: 3.841 min
Delta R.T.: 0.000 min
Response: 18254865
Conc: 20.45 ng/ml

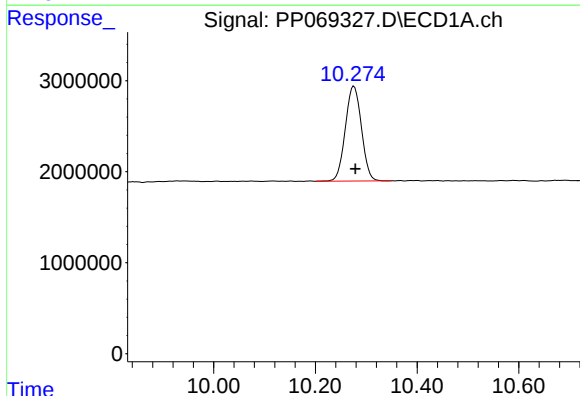


#2 Decachlorobiphenyl

R.T.: 10.276 min
Delta R.T.: -0.003 min
Response: 22962240
Conc: 21.01 ng/ml

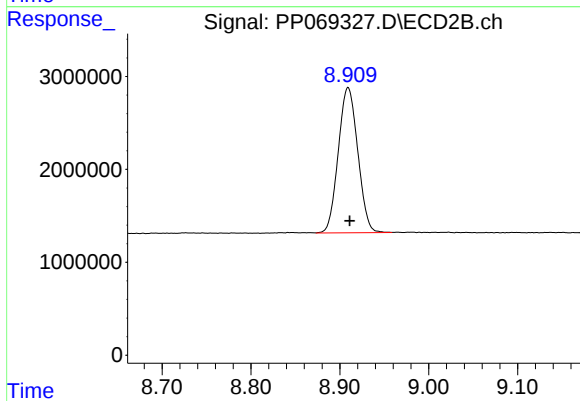

#2 Decachlorobiphenyl


R.T.: 8.909 min
Delta R.T.: -0.002 min
Response: 23865404
Conc: 21.34 ng/ml

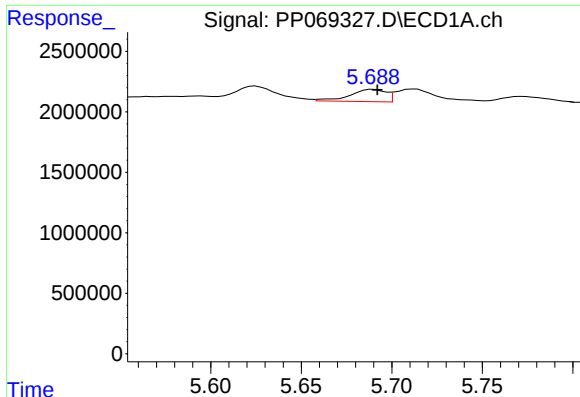

#3 AR-1016-1


R.T.: 5.690 min
Delta R.T.: -0.002 min
Response: 1413762
Conc: 30.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

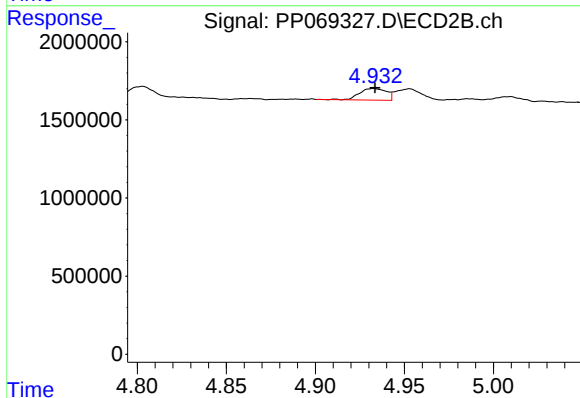


#3 AR-1016-1

R.T.: 4.933 min
Delta R.T.: 0.000 min
Response: 782039
Conc: 23.98 ng/ml

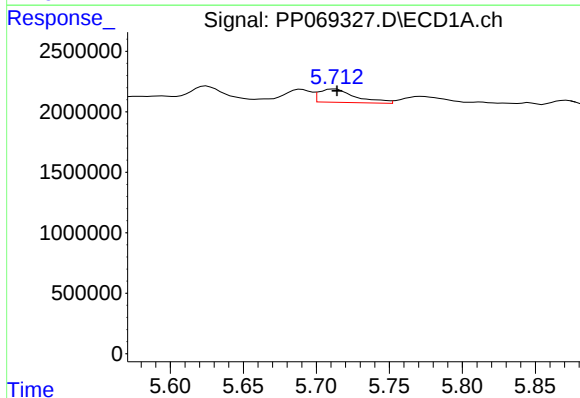


#4 AR-1016-2

R.T.: 5.713 min
Delta R.T.: -0.001 min
Response: 1910703
Conc: 28.15 ng/ml

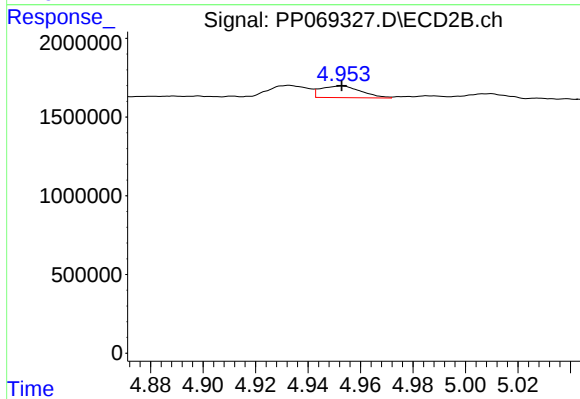

#4 AR-1016-2


R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 790661
Conc: 17.59 ng/ml

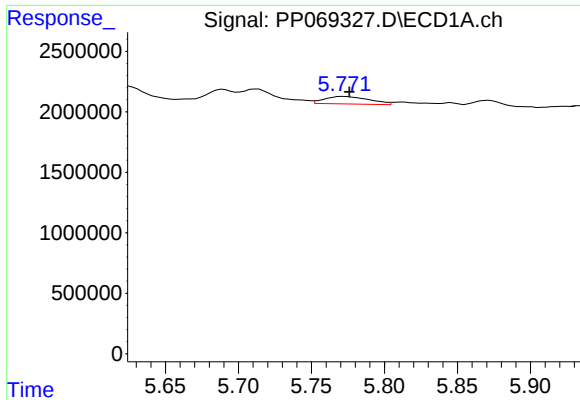

#5 AR-1016-3


R.T.: 5.772 min
Delta R.T.: -0.004 min
Response: 1322650
Conc: 31.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

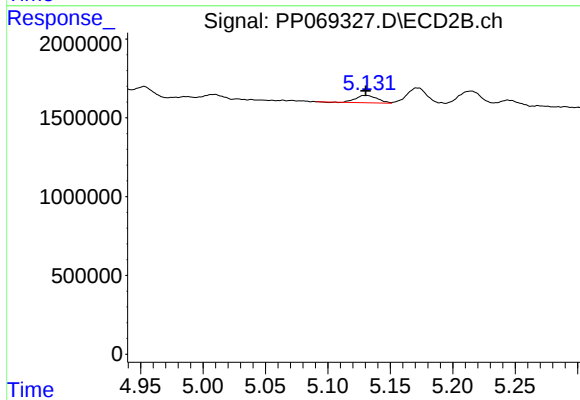


#5 AR-1016-3

R.T.: 5.130 min
Delta R.T.: 0.000 min
Response: 562442
Conc: 22.60 ng/ml

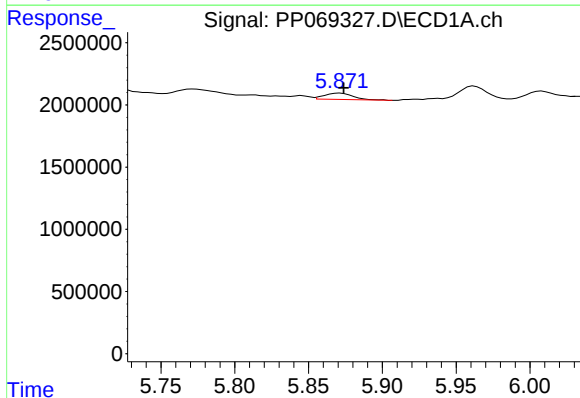


#6 AR-1016-4

R.T.: 5.872 min
Delta R.T.: -0.002 min
Response: 692955
Conc: 19.80 ng/ml

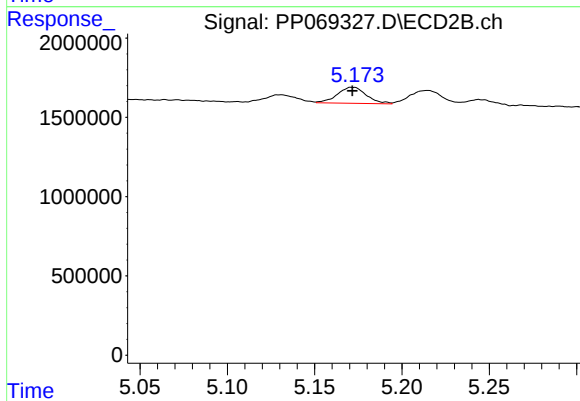

#6 AR-1016-4


R.T.: 5.172 min
Delta R.T.: 0.000 min
Response: 1169387
Conc: 57.90 ng/ml

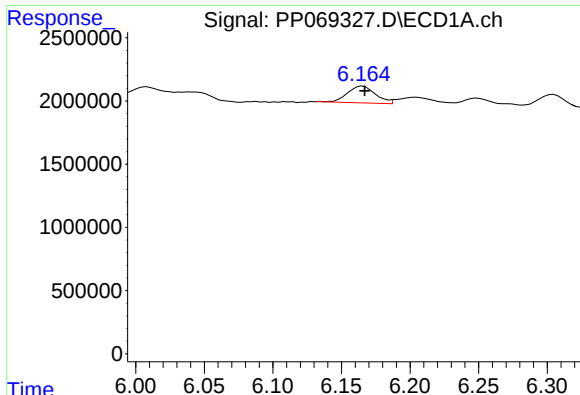

#7 AR-1016-5


R.T.: 6.166 min
Delta R.T.: -0.001 min
Response: 1886237
Conc: 57.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

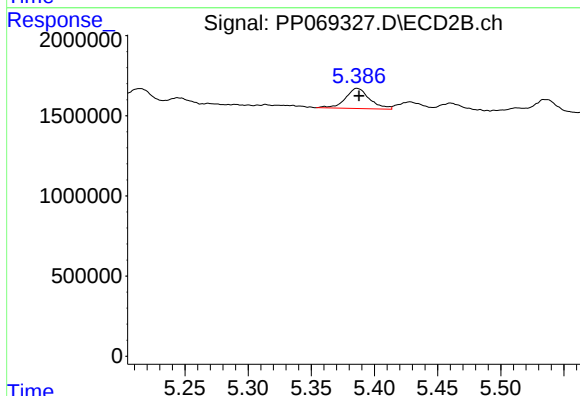


#7 AR-1016-5

R.T.: 5.386 min
Delta R.T.: -0.001 min
Response: 1665244
Conc: 62.08 ng/ml

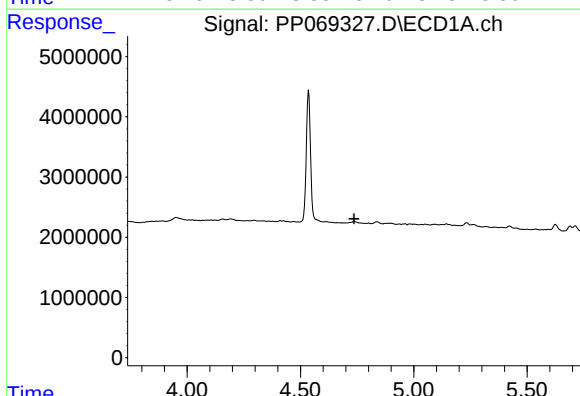


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.737 min
Response: 0
Conc: N.D.

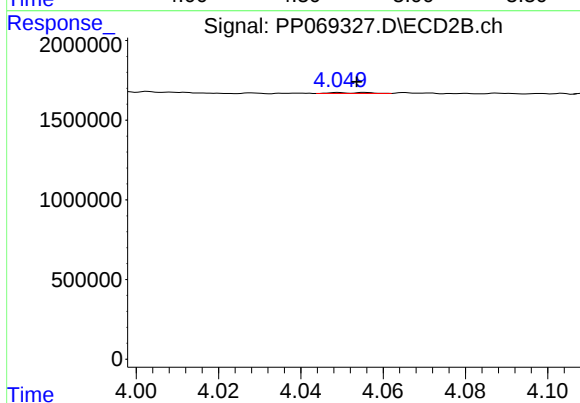

#8 AR-1221-1


R.T.: 4.049 min
Delta R.T.: -0.004 min
Response: 37936
Conc: 3.08 ng/ml

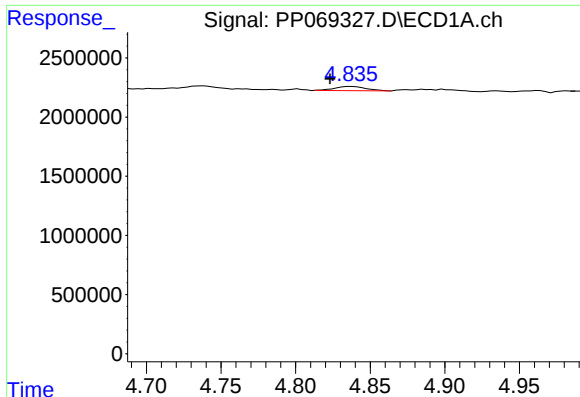

#9 AR-1221-2


R.T.: 4.837 min
Delta R.T.: 0.014 min
Response: 514881
Conc: 37.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

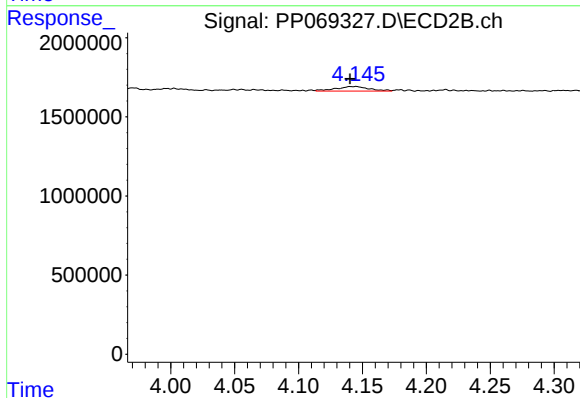


#9 AR-1221-2

R.T.: 4.145 min
Delta R.T.: 0.005 min
Response: 513366
Conc: 53.02 ng/ml

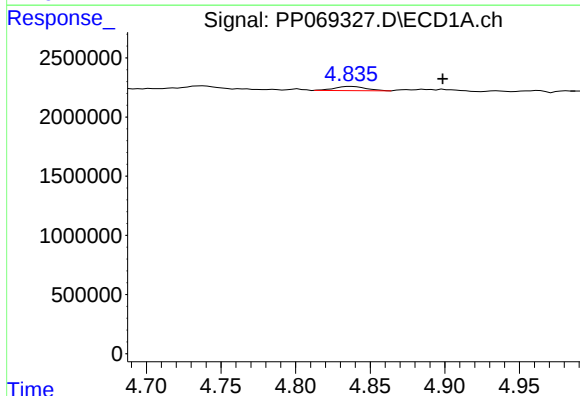


#10 AR-1221-3

R.T.: 4.837 min
Delta R.T.: -0.061 min
Response: 514881
Conc: 12.28 ng/ml

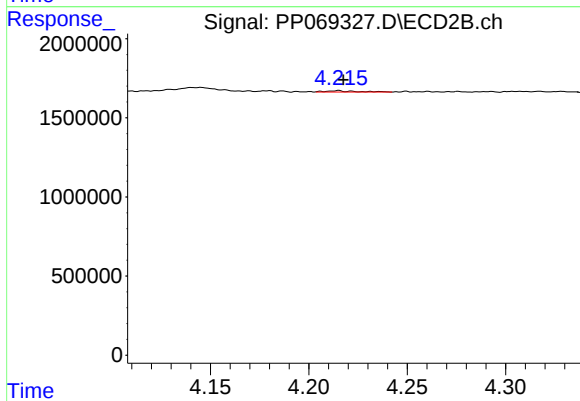

#10 AR-1221-3


R.T.: 4.215 min
Delta R.T.: -0.003 min
Response: 89502
Conc: 3.07 ng/ml

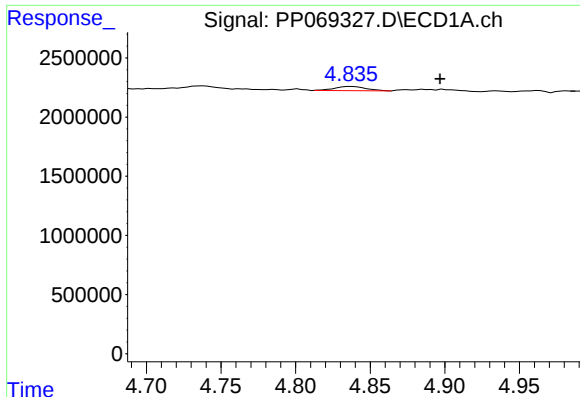

#11 AR-1232-1


R.T.: 4.837 min
Delta R.T.: -0.060 min
Response: 514881
Conc: 15.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

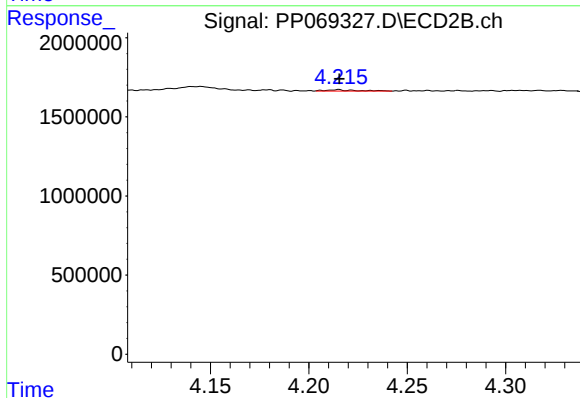


#11 AR-1232-1

R.T.: 4.215 min
Delta R.T.: 0.000 min
Response: 89502
Conc: 3.81 ng/ml

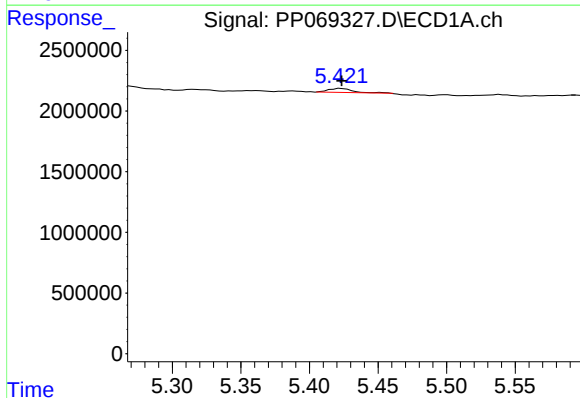


#12 AR-1232-2

R.T.: 5.423 min
Delta R.T.: -0.001 min
Response: 362281
Conc: 22.17 ng/ml

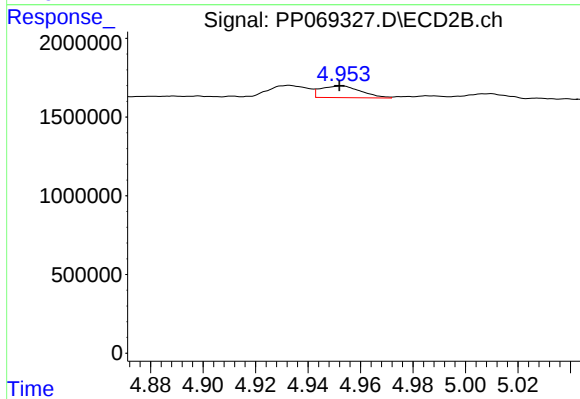

#12 AR-1232-2


R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 790661
Conc: 33.54 ng/ml

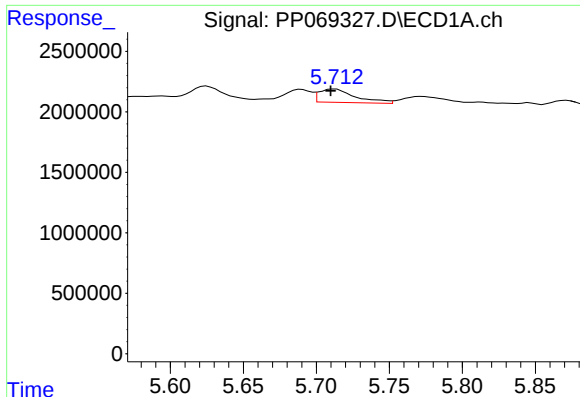

#13 AR-1232-3


R.T.: 5.713 min
Delta R.T.: 0.003 min
Response: 1910703
Conc: 55.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

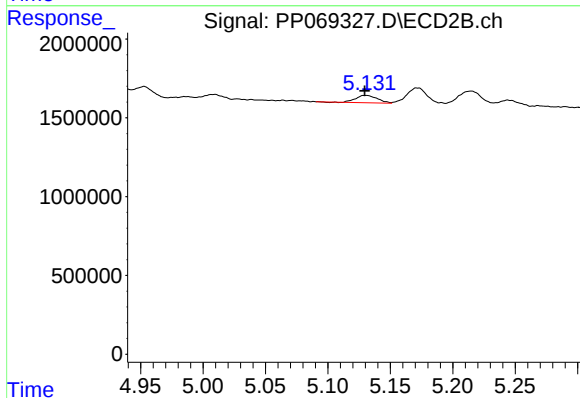


#13 AR-1232-3

R.T.: 5.130 min
Delta R.T.: 0.000 min
Response: 562442
Conc: 43.44 ng/ml

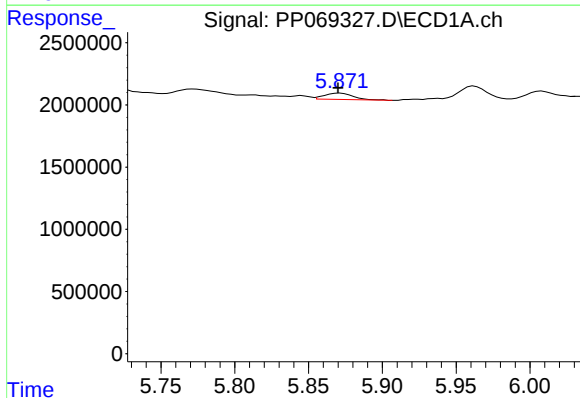


#14 AR-1232-4

R.T.: 5.872 min
Delta R.T.: 0.002 min
Response: 692955
Conc: 38.89 ng/ml

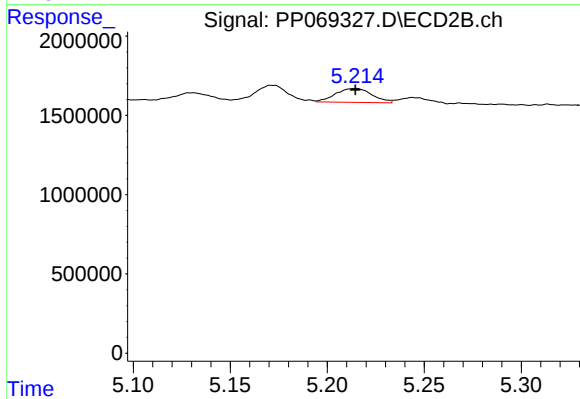

#14 AR-1232-4


R.T.: 5.214 min
Delta R.T.: 0.000 min
Response: 1145852
Conc: 103.36 ng/ml

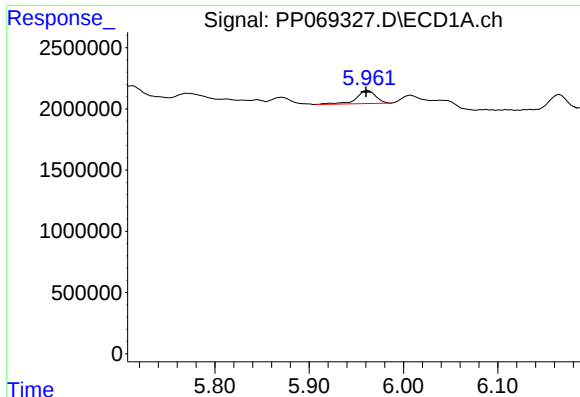

#15 AR-1232-5


R.T.: 5.962 min
Delta R.T.: 0.002 min
Response: 1497118
Conc: 130.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

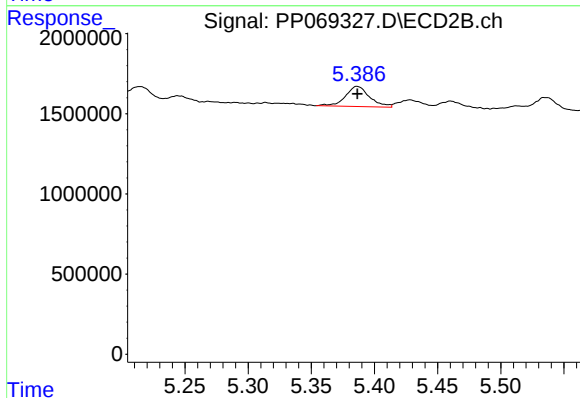


#15 AR-1232-5

R.T.: 5.386 min
Delta R.T.: 0.000 min
Response: 1665244
Conc: 136.38 ng/ml

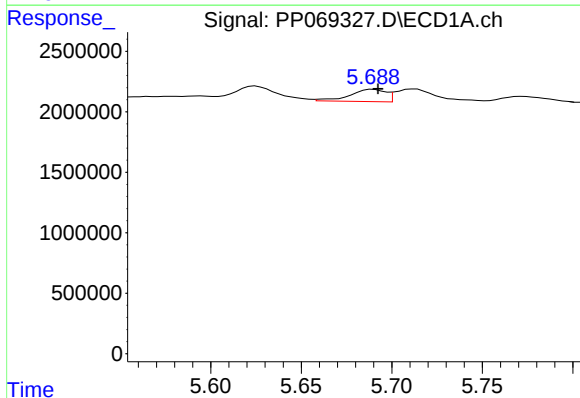


#16 AR-1242-1

R.T.: 5.690 min
Delta R.T.: -0.003 min
Response: 1413762
Conc: 33.90 ng/ml

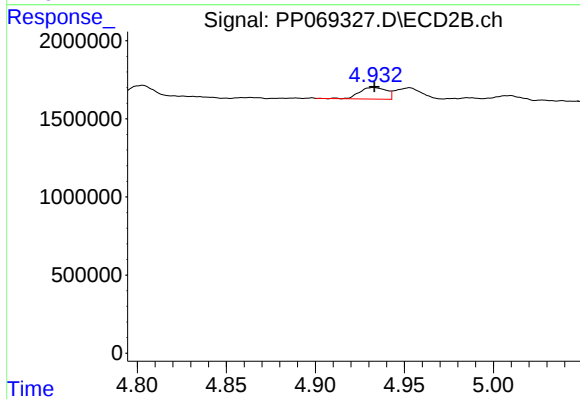

#16 AR-1242-1


R.T.: 4.933 min
Delta R.T.: 0.000 min
Response: 782039
Conc: 27.12 ng/ml

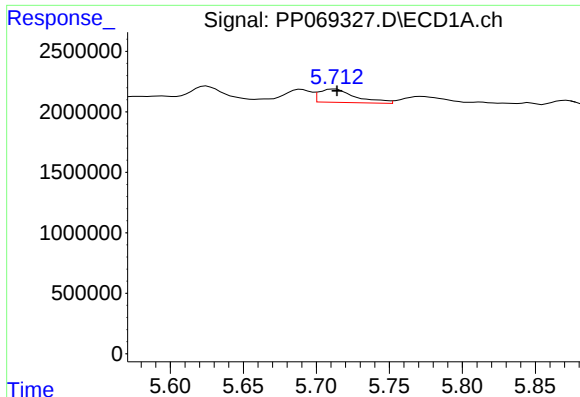

#17 AR-1242-2


R.T.: 5.713 min
Delta R.T.: -0.001 min
Response: 1910703
Conc: 32.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

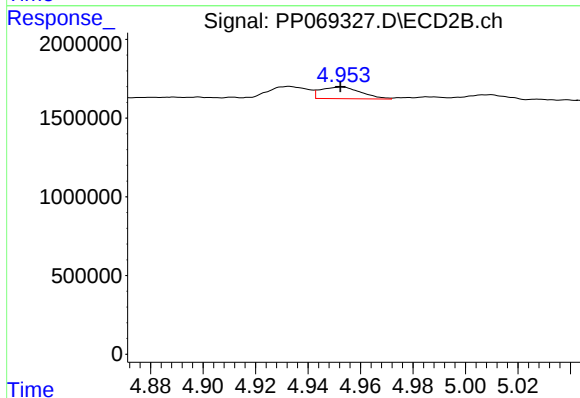


#17 AR-1242-2

R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 790661
Conc: 20.07 ng/ml

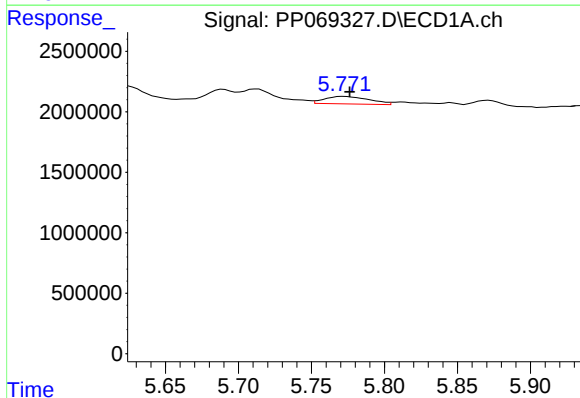


#18 AR-1242-3

R.T.: 5.772 min
Delta R.T.: -0.005 min
Response: 1322650
Conc: 35.65 ng/ml

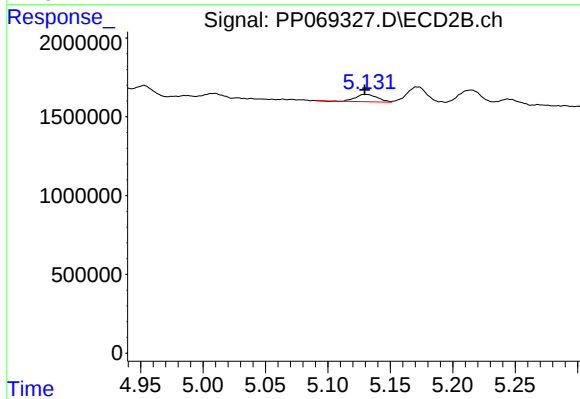

#18 AR-1242-3


R.T.: 5.130 min
Delta R.T.: 0.000 min
Response: 562442
Conc: 24.99 ng/ml

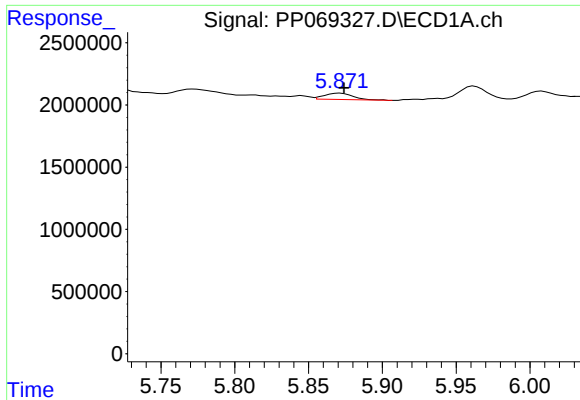

#19 AR-1242-4


R.T.: 5.872 min
Delta R.T.: -0.002 min
Response: 692955
Conc: 21.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

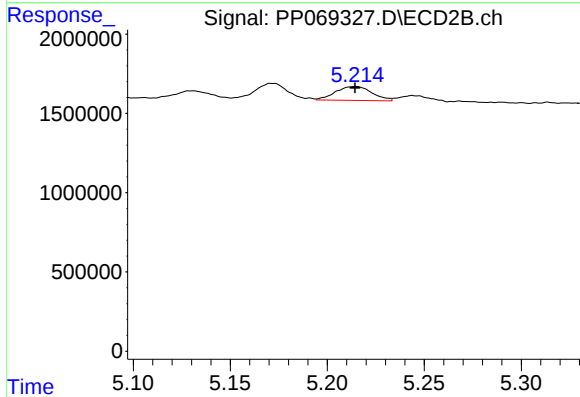


#19 AR-1242-4

R.T.: 5.214 min
Delta R.T.: 0.000 min
Response: 1145852
Conc: 53.09 ng/ml

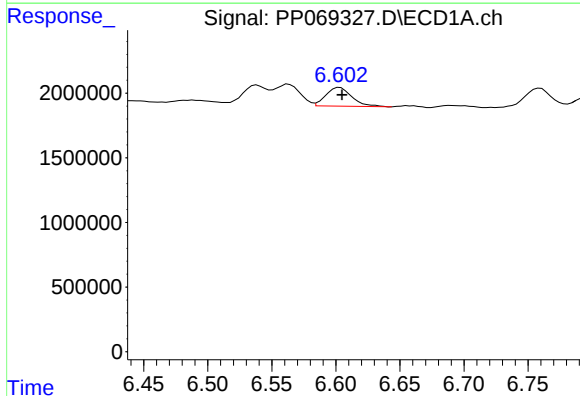


#20 AR-1242-5

R.T.: 6.603 min
Delta R.T.: -0.002 min
Response: 2047530
Conc: 62.84 ng/ml

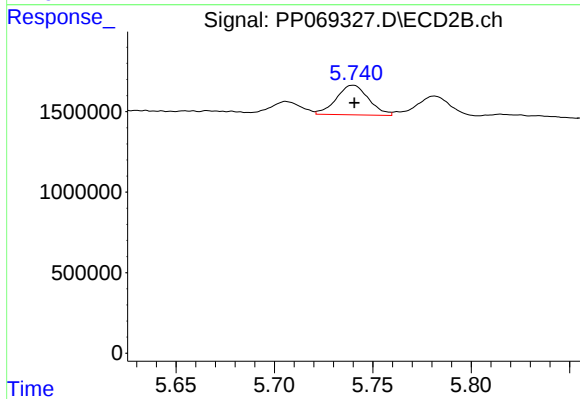

#20 AR-1242-5


R.T.: 5.740 min
Delta R.T.: 0.000 min
Response: 2112602
Conc: 73.43 ng/ml

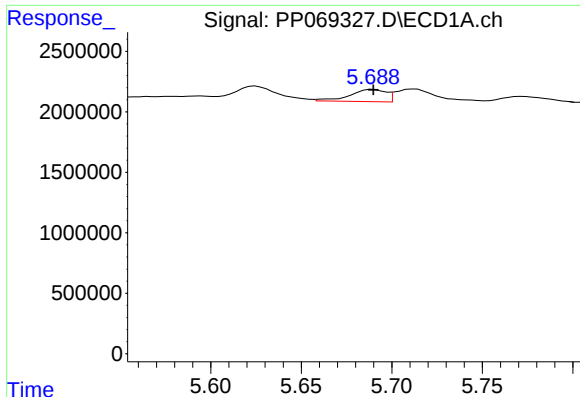

#21 AR-1248-1


R.T.: 5.690 min
Delta R.T.: 0.000 min
Response: 1413762
Conc: 43.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

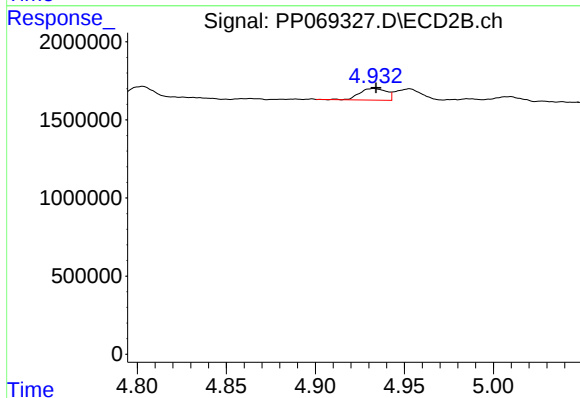


#21 AR-1248-1

R.T.: 4.933 min
Delta R.T.: -0.001 min
Response: 782039
Conc: 35.53 ng/ml

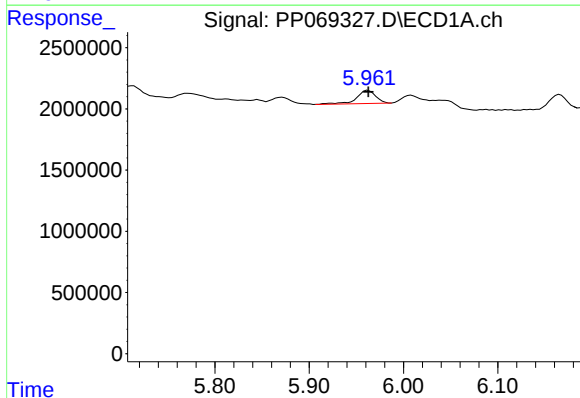


#22 AR-1248-2

R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 1497118
Conc: 35.27 ng/ml

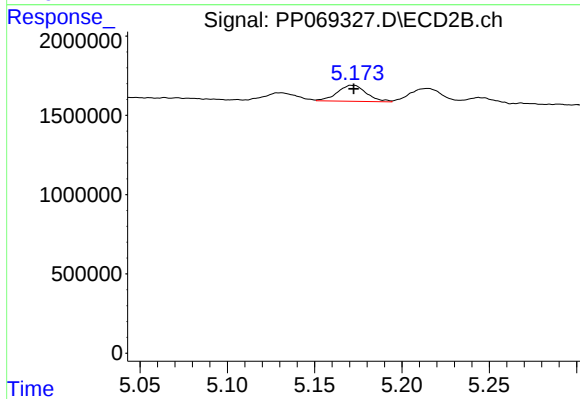

#22 AR-1248-2


R.T.: 5.172 min
Delta R.T.: 0.000 min
Response: 1169387
Conc: 38.90 ng/ml

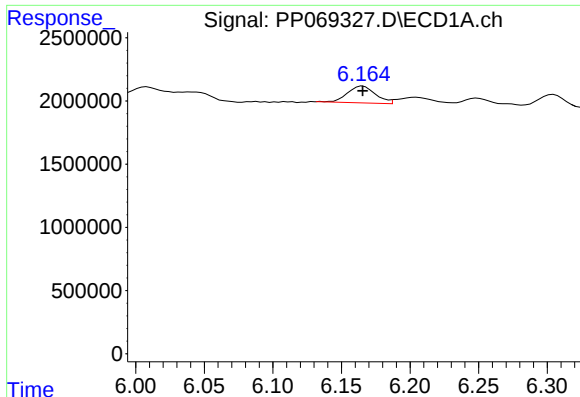

#23 AR-1248-3


R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 1886237
Conc: 40.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

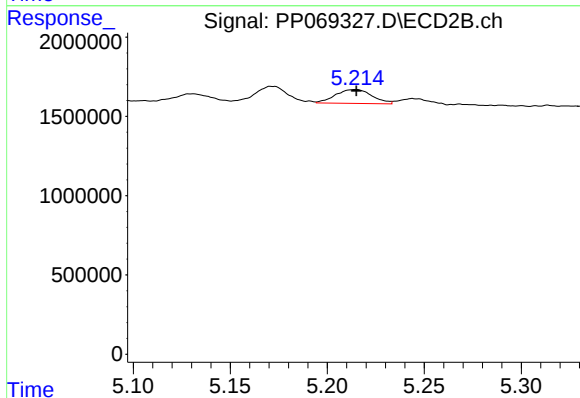


#23 AR-1248-3

R.T.: 5.214 min
Delta R.T.: 0.000 min
Response: 1145852
Conc: 36.98 ng/ml

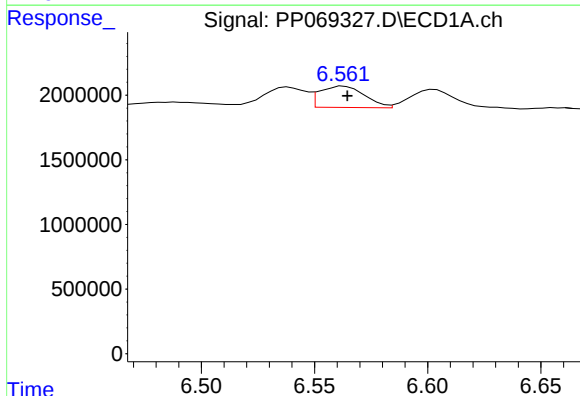


#24 AR-1248-4

R.T.: 6.563 min
Delta R.T.: -0.002 min
Response: 2277371
Conc: 41.32 ng/ml

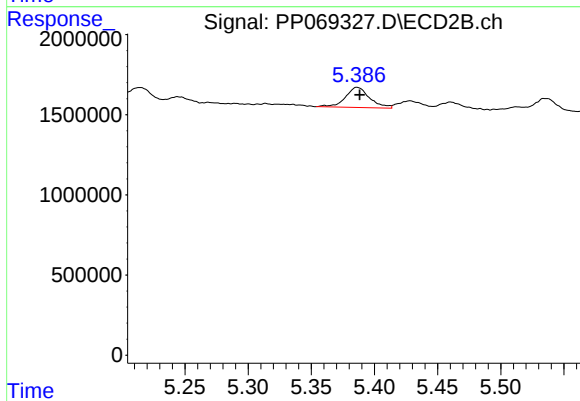

#24 AR-1248-4


R.T.: 5.386 min
Delta R.T.: -0.002 min
Response: 1665244
Conc: 45.08 ng/ml

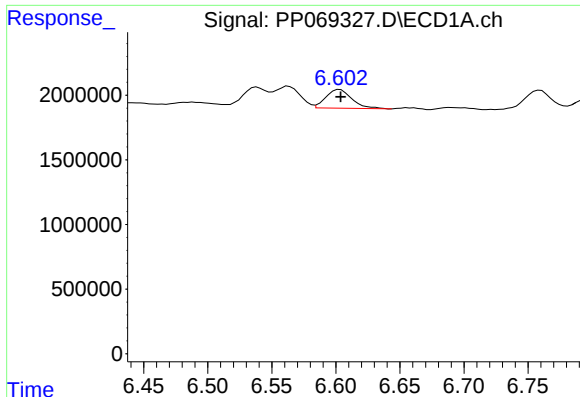

#25 AR-1248-5


R.T.: 6.603 min
Delta R.T.: 0.000 min
Response: 2047530
Conc: 38.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

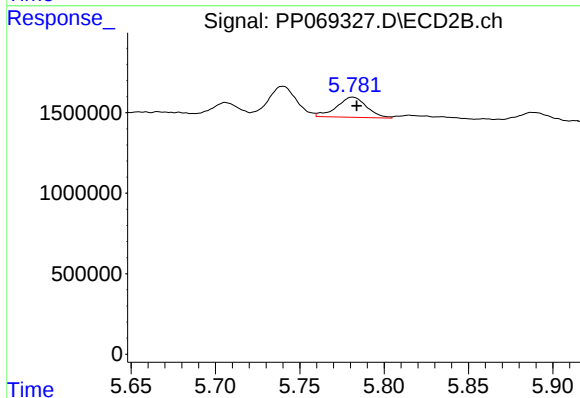


#25 AR-1248-5

R.T.: 5.781 min
Delta R.T.: -0.002 min
Response: 1561905
Conc: 41.77 ng/ml

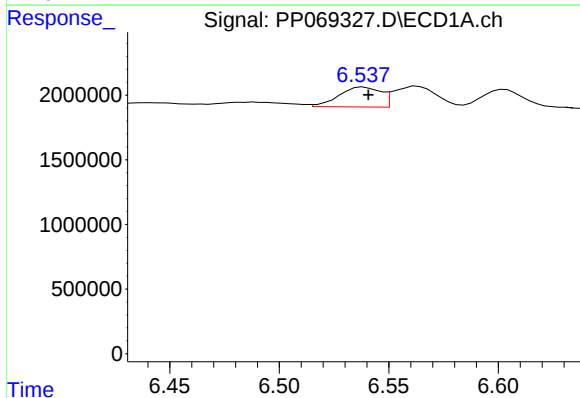


#26 AR-1254-1

R.T.: 6.538 min
Delta R.T.: -0.002 min
Response: 2044348
Conc: 35.33 ng/ml

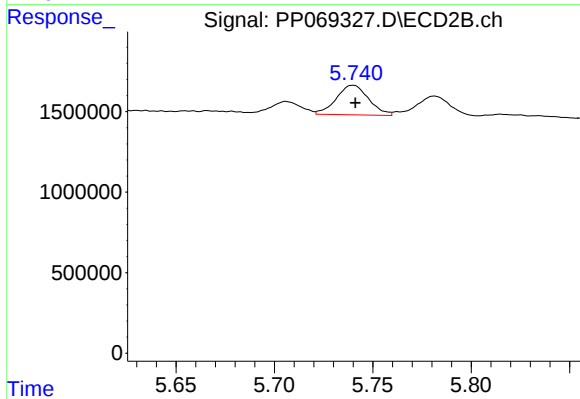

#26 AR-1254-1


R.T.: 5.740 min
Delta R.T.: -0.001 min
Response: 2112602
Conc: 38.37 ng/ml

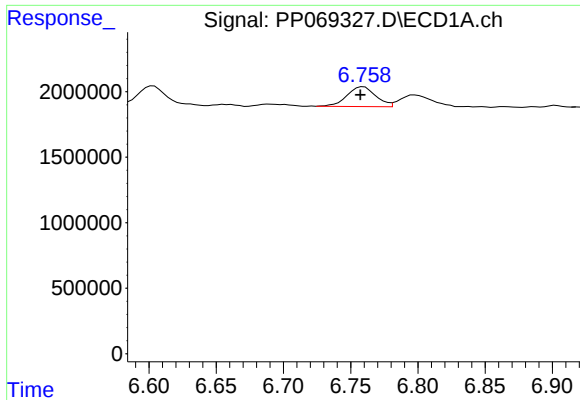

#27 AR-1254-2


R.T.: 6.760 min
Delta R.T.: 0.002 min
Response: 2235329
Conc: 27.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

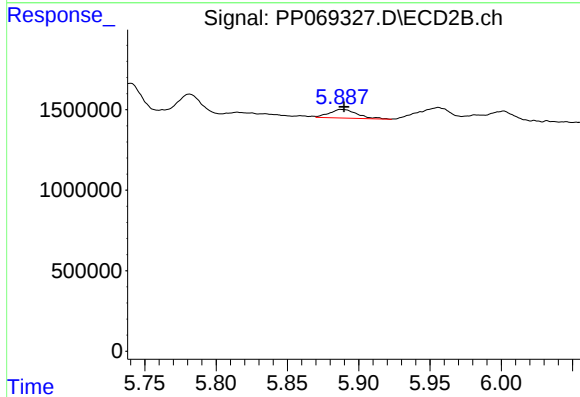


#27 AR-1254-2

R.T.: 5.888 min
Delta R.T.: -0.001 min
Response: 731996
Conc: 15.13 ng/ml

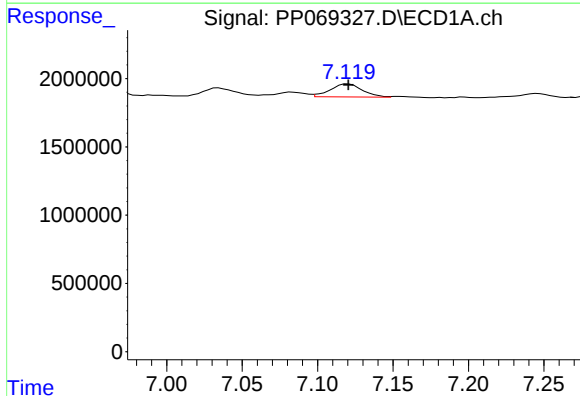


#28 AR-1254-3

R.T.: 7.120 min
Delta R.T.: 0.000 min
Response: 1423876
Conc: 16.89 ng/ml

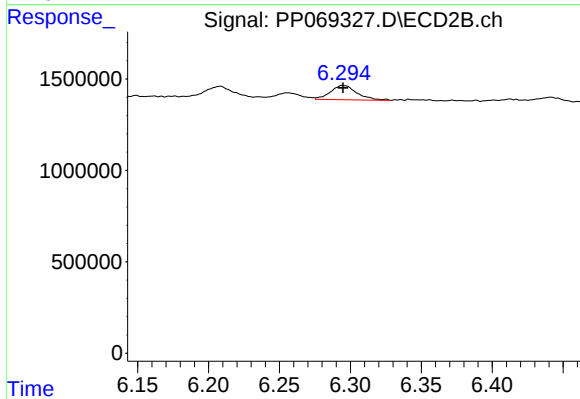

#28 AR-1254-3


R.T.: 6.295 min
Delta R.T.: 0.000 min
Response: 1021006
Conc: 13.45 ng/ml

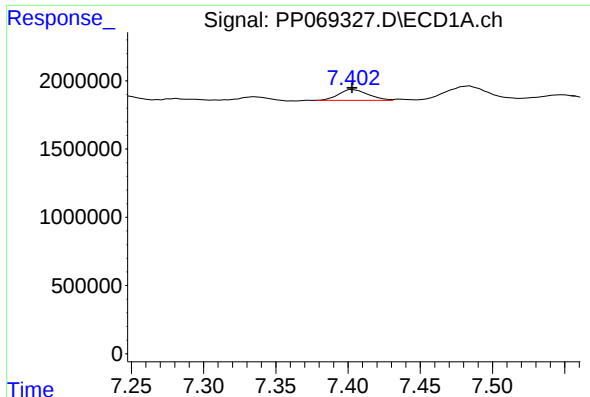

#29 AR-1254-4


R.T.: 7.404 min
Delta R.T.: 0.000 min
Response: 1127388
Conc: 16.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

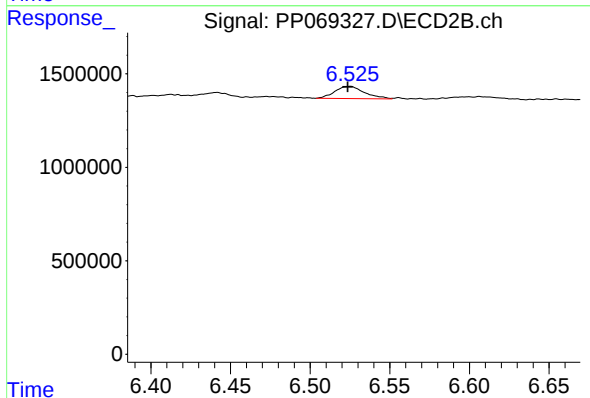


#29 AR-1254-4

R.T.: 6.525 min
Delta R.T.: 0.001 min
Response: 848133
Conc: 16.55 ng/ml

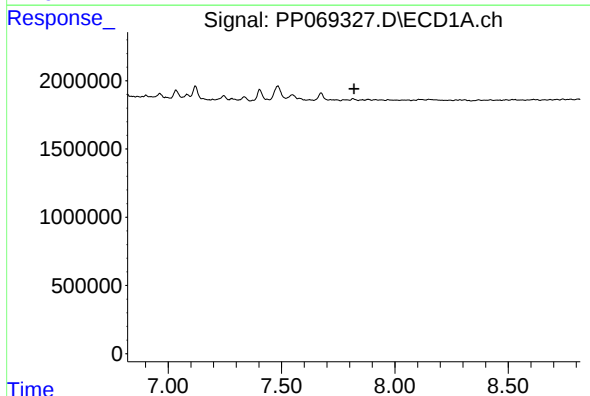


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.820 min
Response: 0
Conc: N.D.

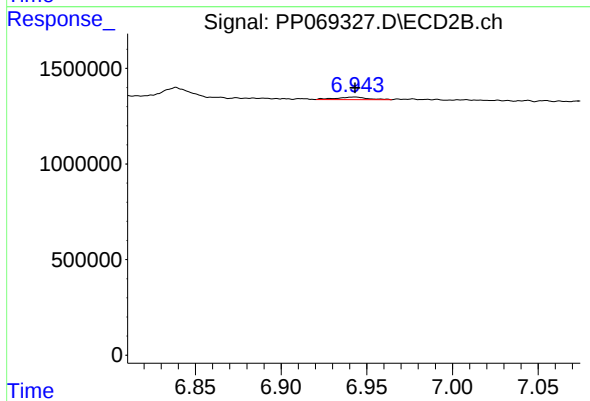

#30 AR-1254-5


R.T.: 6.943 min
Delta R.T.: 0.000 min
Response: 171904
Conc: 2.58 ng/ml

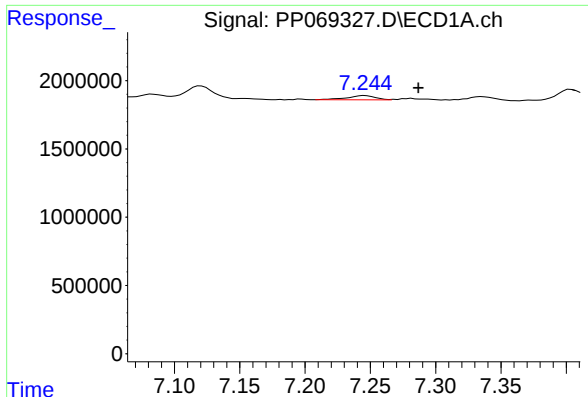

#31 AR-1260-1


R.T.: 7.245 min
Delta R.T.: -0.041 min
Response: 473565
Conc: 8.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

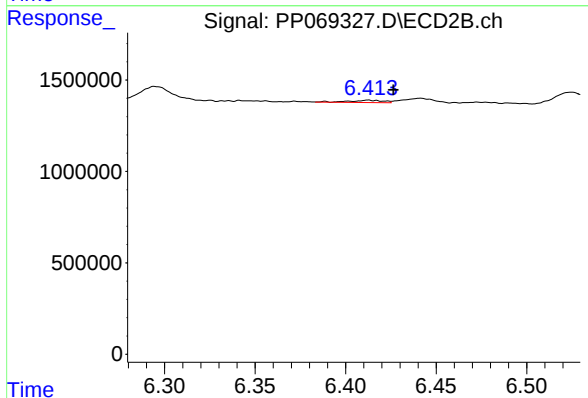


#31 AR-1260-1

R.T.: 6.412 min
Delta R.T.: -0.014 min
Response: 164809
Conc: 3.42 ng/ml

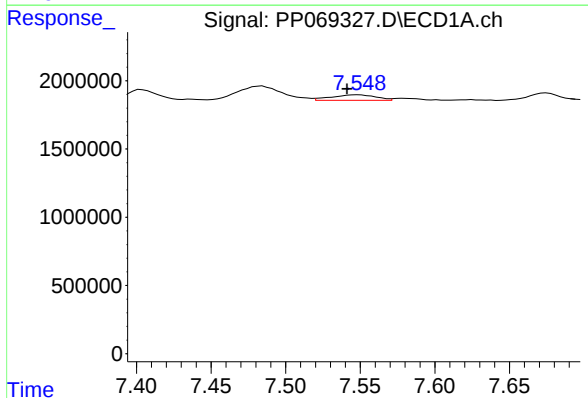


#32 AR-1260-2

R.T.: 7.549 min
Delta R.T.: 0.008 min
Response: 841500
Conc: 10.81 ng/ml

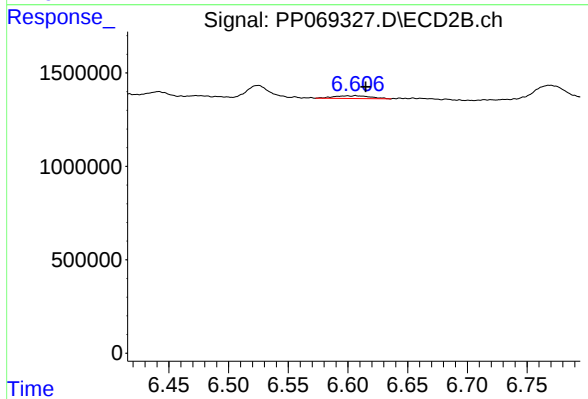

#32 AR-1260-2


R.T.: 6.606 min
Delta R.T.: -0.008 min
Response: 324396
Conc: 5.29 ng/ml

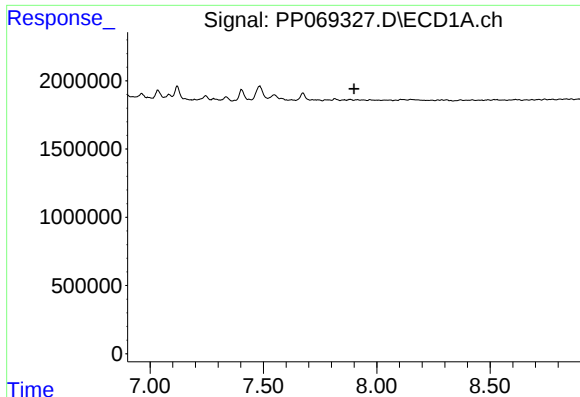

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.900 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

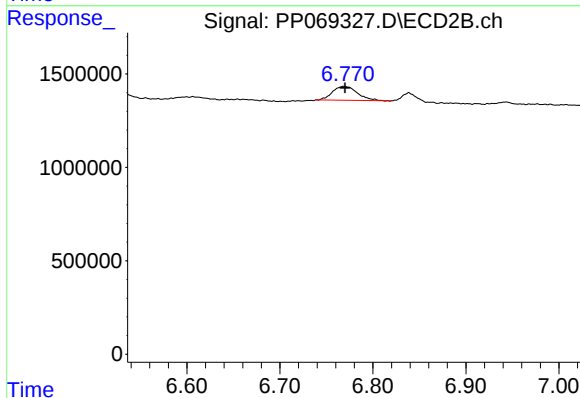


#33 AR-1260-3

R.T.: 6.769 min
Delta R.T.: 0.000 min
Response: 1365414
Conc: 22.70 ng/ml

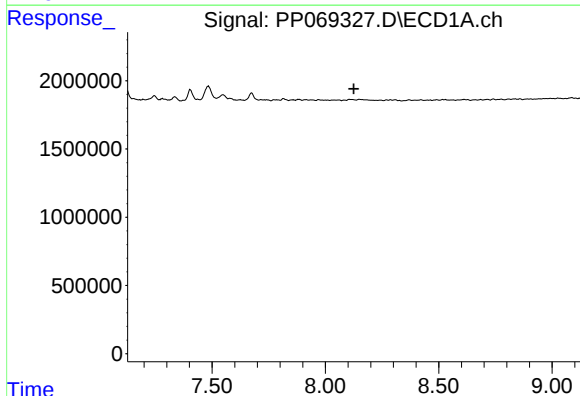


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 8.125 min
Response: 0
Conc: N.D.

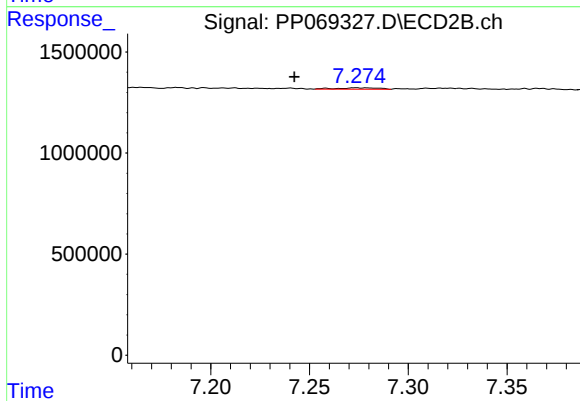

#34 AR-1260-4


R.T.: 7.274 min
Delta R.T.: 0.031 min
Response: 97072
Conc: 2.09 ng/ml

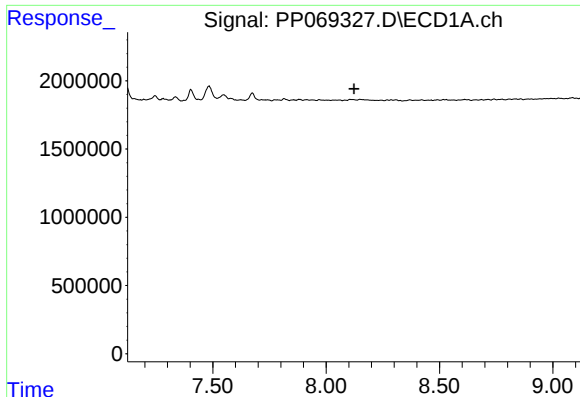

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

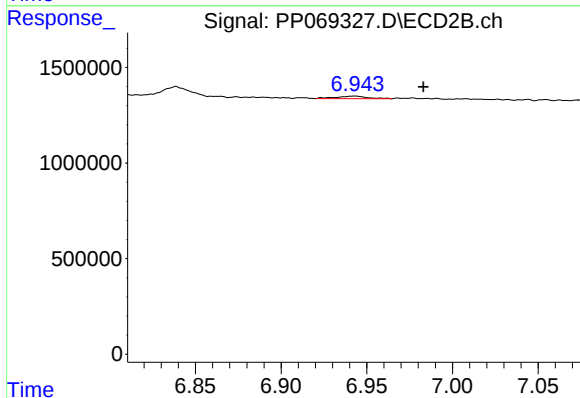


#36 AR-1262-1

R.T.: 6.943 min
Delta R.T.: -0.040 min
Response: 171904
Conc: 2.42 ng/ml

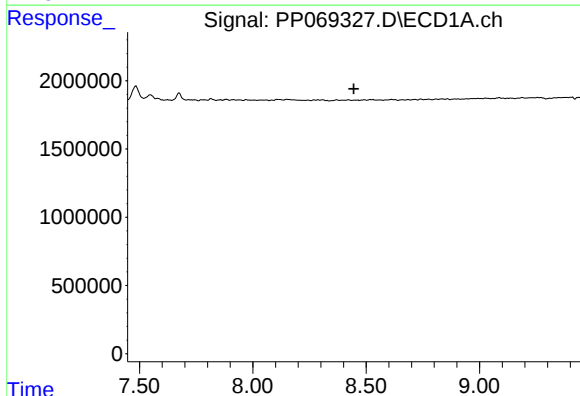


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.446 min
Response: 0
Conc: N.D.

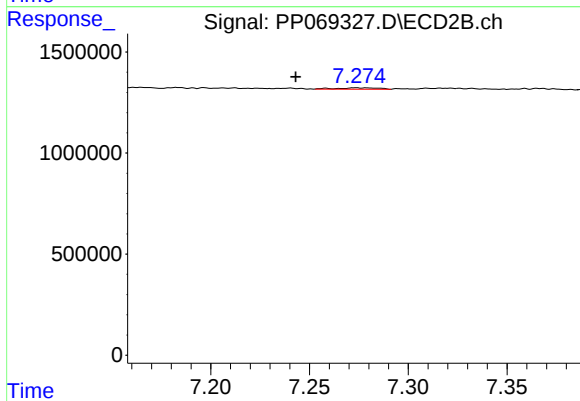

#37 AR-1262-2


R.T.: 7.274 min
Delta R.T.: 0.031 min
Response: 97072
Conc: 1.59 ng/ml

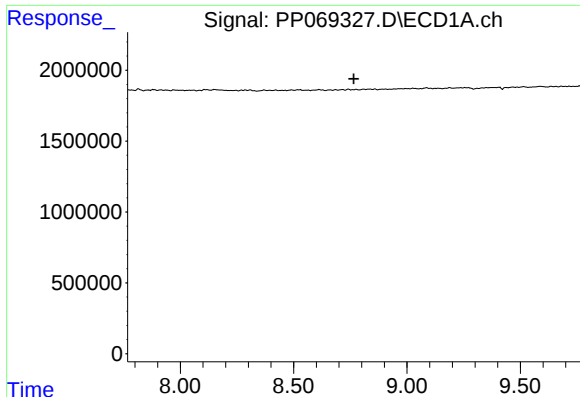

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

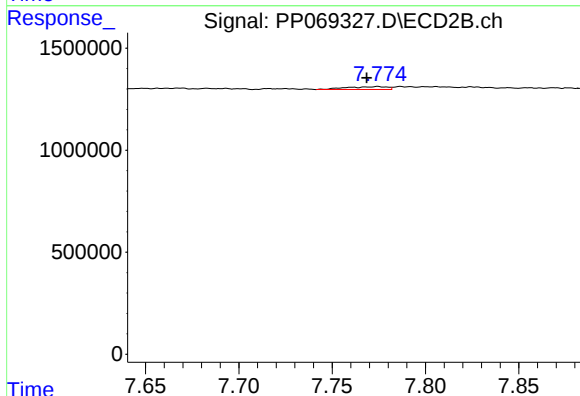


#38 AR-1262-3

R.T.: 7.774 min
Delta R.T.: 0.006 min
Response: 218787
Conc: 4.18 ng/ml

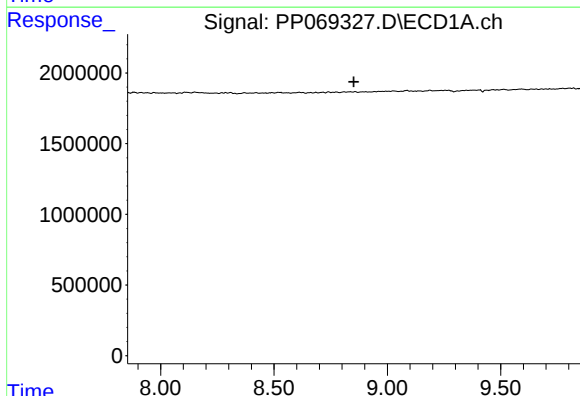


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.852 min
Response: 0
Conc: N.D.

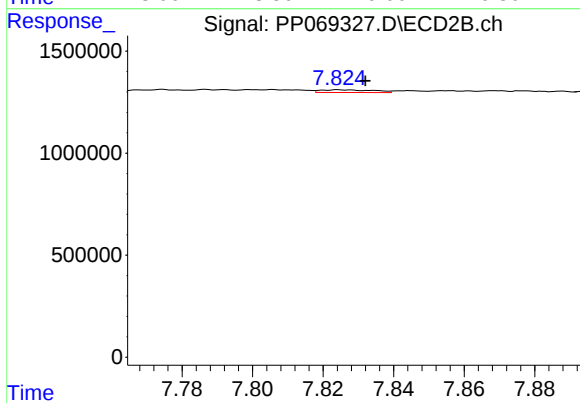

#39 AR-1262-4


R.T.: 7.825 min
Delta R.T.: -0.007 min
Response: 139312
Conc: 1.51 ng/ml

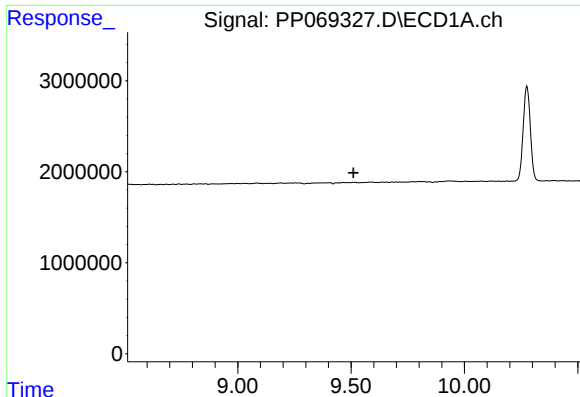

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

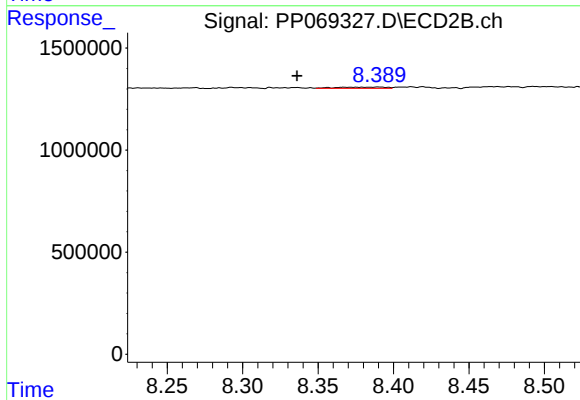


#40 AR-1262-5

R.T.: 8.390 min
Delta R.T.: 0.054 min
Response: 136667
Conc: 2.86 ng/ml

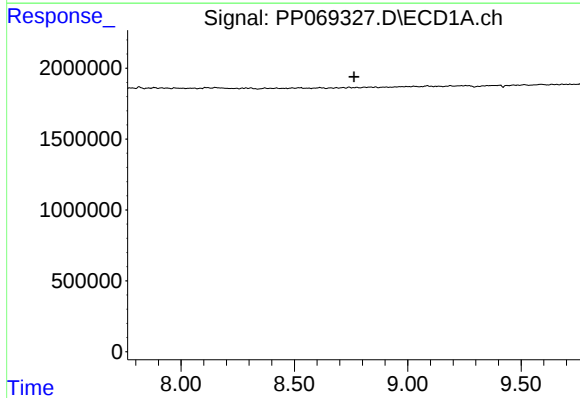


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.763 min
Response: 0
Conc: N.D.

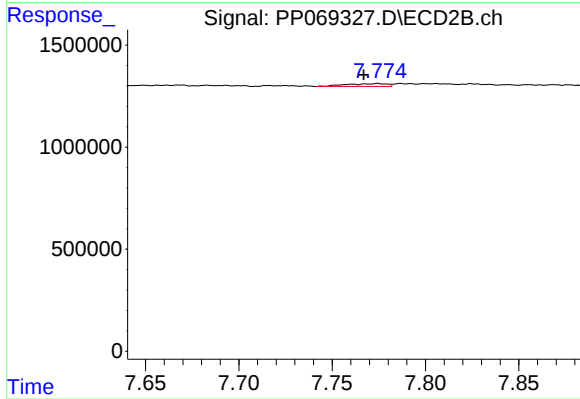

#41 AR-1268-1


R.T.: 7.774 min
Delta R.T.: 0.008 min
Response: 218787
Conc: 1.51 ng/ml

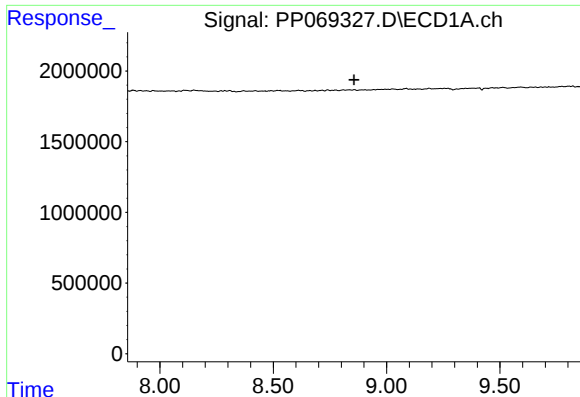

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 8.857 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

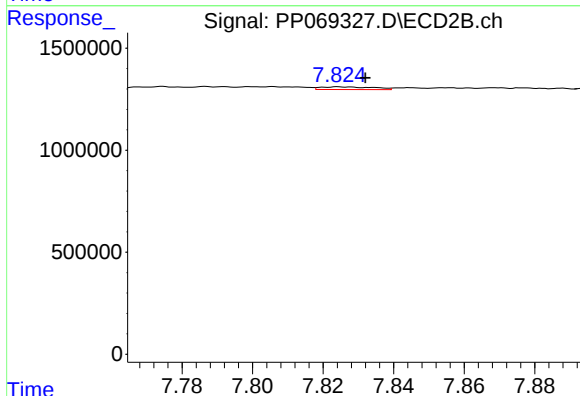


#42 AR-1268-2

R.T.: 7.825 min
Delta R.T.: -0.007 min
Response: 139312
Conc: 1.05 ng/ml

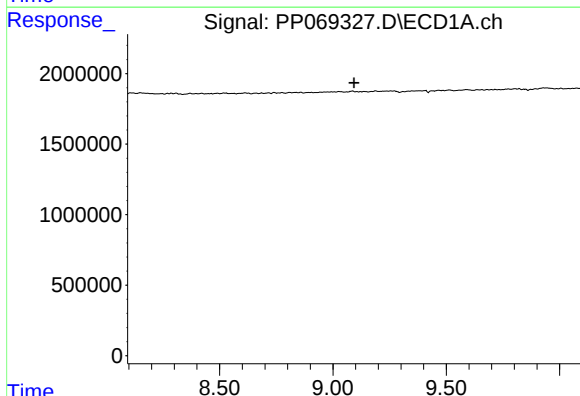


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.093 min
Response: 0
Conc: N.D.

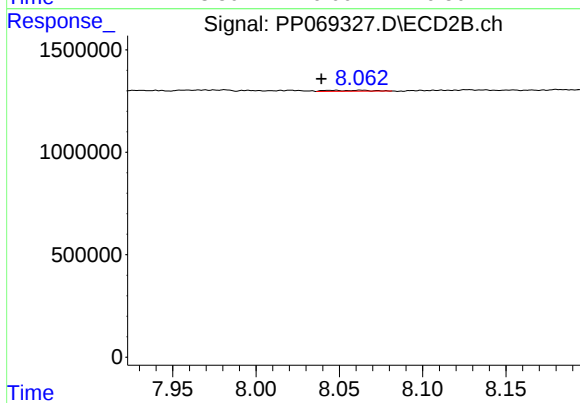

#43 AR-1268-3


R.T.: 8.048 min
Delta R.T.: 0.009 min
Response: 82976
Conc: 0.73 ng/ml

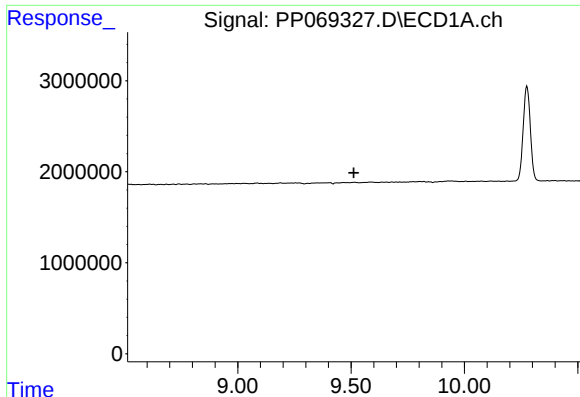

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 9.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

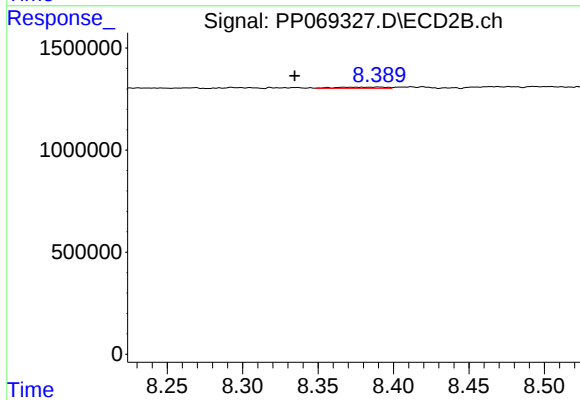


#44 AR-1268-4

R.T.: 8.390 min
Delta R.T.: 0.056 min
Response: 136667
Conc: 2.62 ng/ml

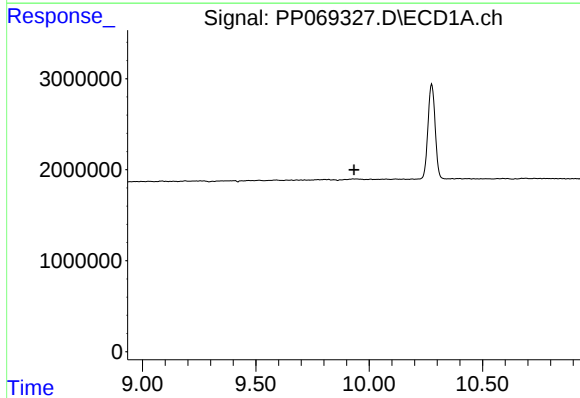

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.933 min
Response: 0
Conc: N.D.

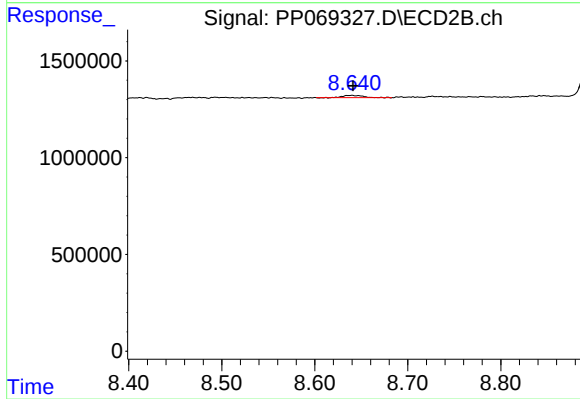

#45 AR-1268-5

R.T.: 8.640 min
Delta R.T.: -0.001 min
Response: 174303
Conc: 0.49 ng/ml