

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
 Data File : PP069328.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2025 16:54
 Operator : YP\AJ
 Sample : Q1168-07
 Misc : AR1254 LOD 40 PPB
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 00:50:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.536	3.840	28322208	18434509	19.785	20.654
2)	SA Decachlor...	10.276	8.909	22662916	23191573	20.737	20.735
Target Compounds							
3)	L1 AR-1016-1	5.624f	4.962	1577430	78171	34.045	2.397 #
4)	L1 AR-1016-2	0.000	4.962	0	78171	N.D.	1.739 #
5)	L1 AR-1016-3	0.000	5.134	0	94601	N.D.	3.802 #
6)	L1 AR-1016-4	0.000	5.171	0	920748	N.D.	45.590 #
7)	L1 AR-1016-5	6.164	5.387	616230	586082	18.641	21.849
8)	L2 AR-1221-1	0.000	3.989f	0	124714	N.D.	10.125 #
9)	L2 AR-1221-2	4.840	4.146	478853	454880	34.972	46.975 #
10)	L2 AR-1221-3	4.840f	4.250	478853	25199	11.417	0.864 #
11)	L3 AR-1232-1	4.840f	4.181	478853	54820	14.383	2.335 #
12)	L3 AR-1232-2	0.000	4.962	0	78171	N.D.	3.316 #
13)	L3 AR-1232-3	0.000	5.134	0	94601	N.D.	7.307 #
14)	L3 AR-1232-4	0.000	5.210	0	334078	N.D.	30.134 #
15)	L3 AR-1232-5	5.962	5.387	1042814	586082	90.977	47.999 #
16)	L4 AR-1242-1	5.624f	4.962	1577430	78171	37.823	2.711 #
17)	L4 AR-1242-2	0.000	4.962	0	78171	N.D.	1.984 #
18)	L4 AR-1242-3	0.000	5.134	0	94601	N.D.	4.204 #
19)	L4 AR-1242-4	0.000	5.210	0	334078	N.D.	15.479 #
20)	L4 AR-1242-5	6.604	5.741	910747	2400880	27.950	83.456 #
21)	L5 AR-1248-1	5.624f	4.962	1577430	78171	48.627	3.552 #
22)	L5 AR-1248-2	5.962	5.171	1042814	920748	24.568	30.626
23)	L5 AR-1248-3	6.164	5.210	616230	334078	13.115	10.782
24)	L5 AR-1248-4	6.563	5.387	1193994	586082	21.661	15.864 #
25)	L5 AR-1248-5	6.604	5.779	910747	285322	17.060	7.631 #
26)	L6 AR-1254-1	6.541	5.741	2737579	2400880	47.311	43.608
27)	L6 AR-1254-2	6.757	5.889	3408653	2140742	42.480	44.259
28)	L6 AR-1254-3	7.120	6.295	3565936	3046702	42.306	40.143
29)	L6 AR-1254-4	7.402	6.523	2802867	2249336	41.105	43.890
30)	L6 AR-1254-5	7.820	6.944	2827862	2521897	41.558	37.889
31)	L7 AR-1260-1	7.285	6.427	1319402	1399866	22.578	29.025 #
32)	L7 AR-1260-2	7.540	6.614	2177805	1295604	27.988	21.134
33)	L7 AR-1260-3	0.000	6.768	0	2383935	N.D.	39.629 #
34)	L7 AR-1260-4	8.106	7.240	987797	153253	14.972	3.298 #
35)	L7 AR-1260-5	0.000	7.484	0	227693	N.D.	2.049 #
36)	L8 AR-1262-1	8.106	7.013	987797	330235	12.501	4.650 #
37)	L8 AR-1262-2	0.000	7.240	0	153253	N.D.	2.513 #
38)	L8 AR-1262-3	0.000	7.772	0	152347	N.D.	2.913 #
39)	L8 AR-1262-4	0.000	7.827	0	388152	N.D.	4.199 #
40)	L8 AR-1262-5	0.000	8.350	0	86744	N.D.	1.815 #
41)	L9 AR-1268-1	0.000	7.772	0	152347	N.D.	1.050 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
Data File : PP069328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2025 16:54
Operator : YP\AJ
Sample : Q1168-07
Misc : AR1254 LOD 40 PPB
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 00:50:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.827	0	388152	N.D.	2.922 #
44) L9	AR-1268-4	0.000	8.350	0	86744	N.D.	1.666 #
45) L9	AR-1268-5	0.000	8.643	0	196730	N.D.	0.552 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
Data File : PP069328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2025 16:54
Operator : YP\AJ
Sample : Q1168-07
Misc : AR1254 LOD 40 PPB
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 00:50:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

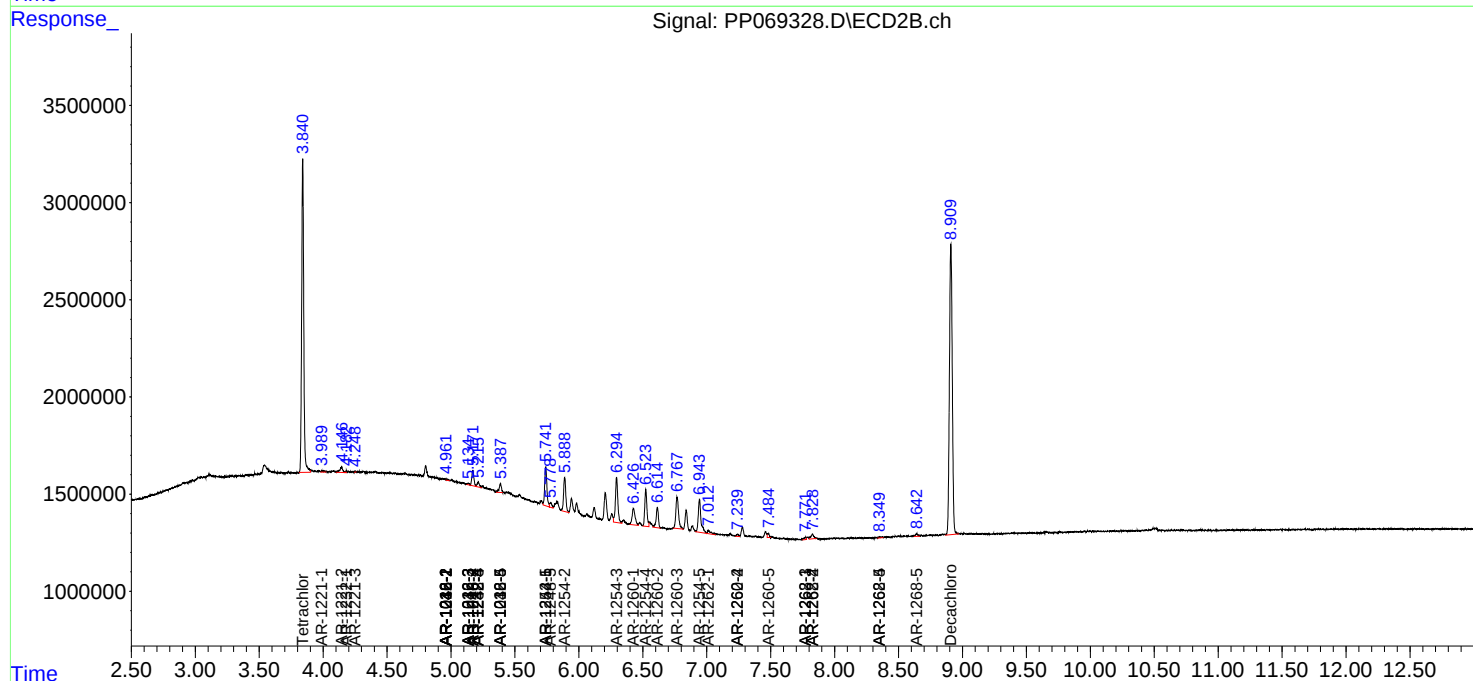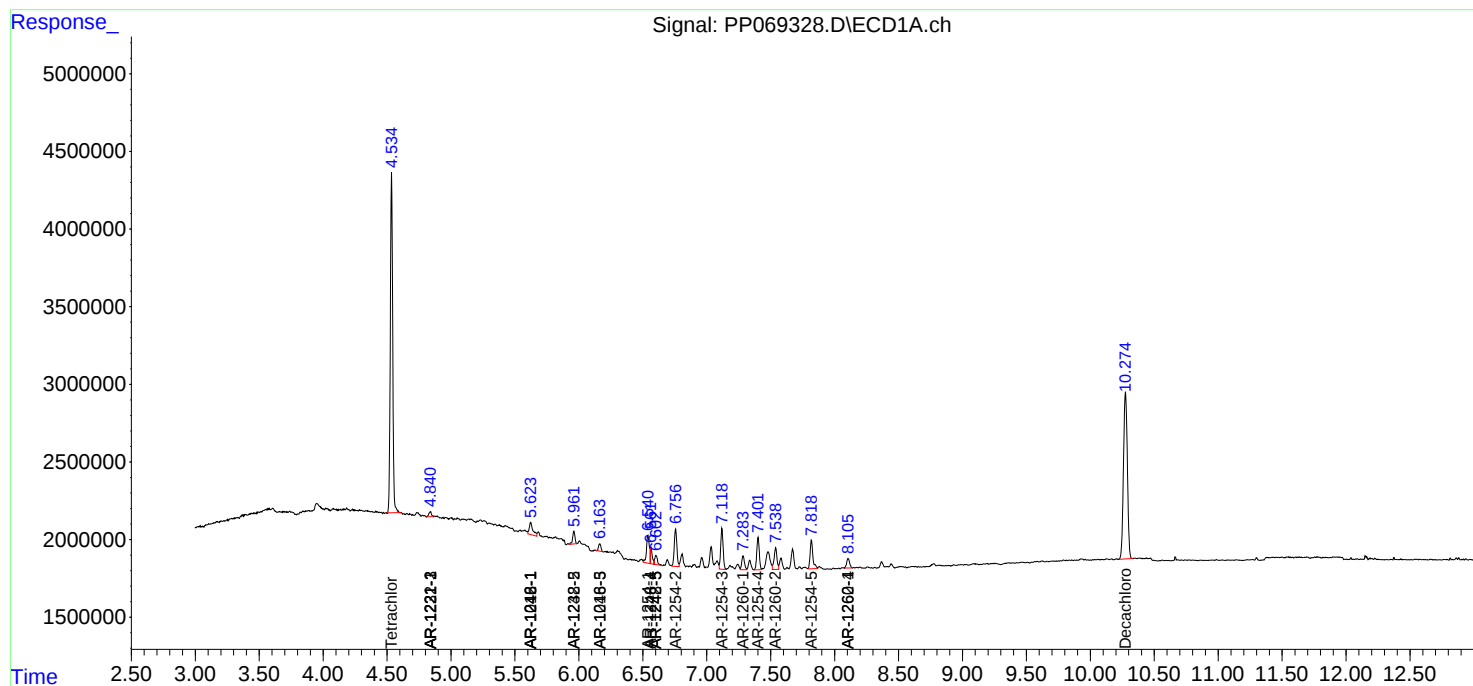


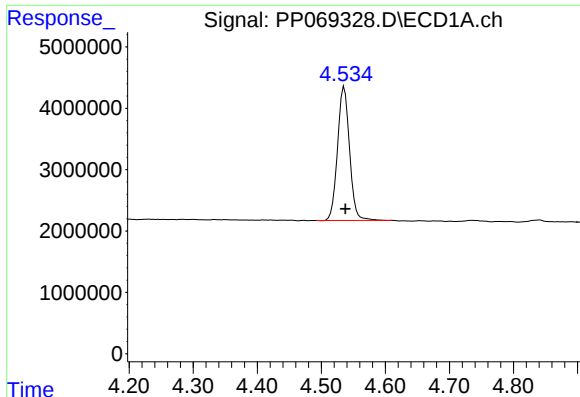

#1 Tetrachloro-m-xylene


R.T.: 4.536 min
Delta R.T.: -0.002 min
Response: 28322208
Conc: 19.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

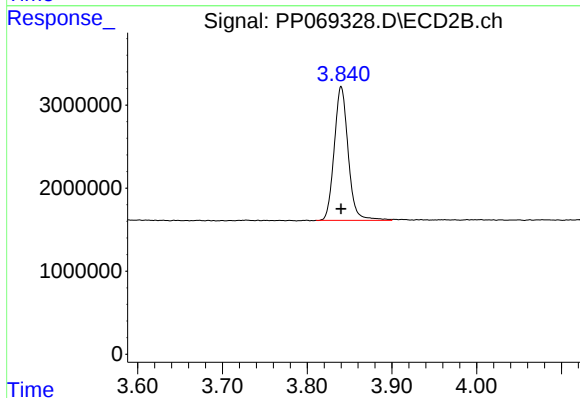


#1 Tetrachloro-m-xylene

R.T.: 3.840 min
Delta R.T.: 0.000 min
Response: 18434509
Conc: 20.65 ng/ml

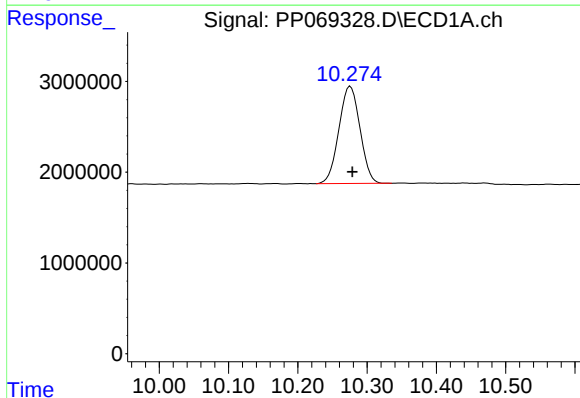


#2 Decachlorobiphenyl

R.T.: 10.276 min
Delta R.T.: -0.003 min
Response: 22662916
Conc: 20.74 ng/ml

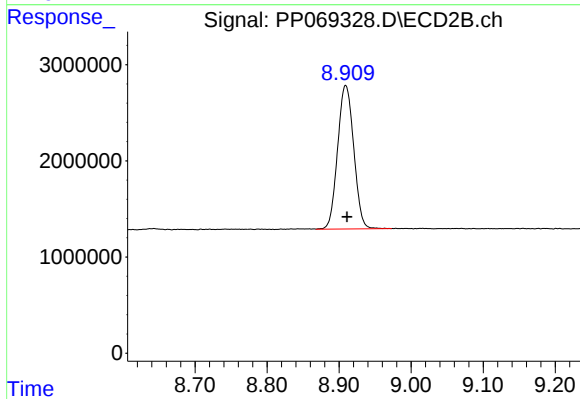

#2 Decachlorobiphenyl


R.T.: 8.909 min
Delta R.T.: -0.002 min
Response: 23191573
Conc: 20.73 ng/ml

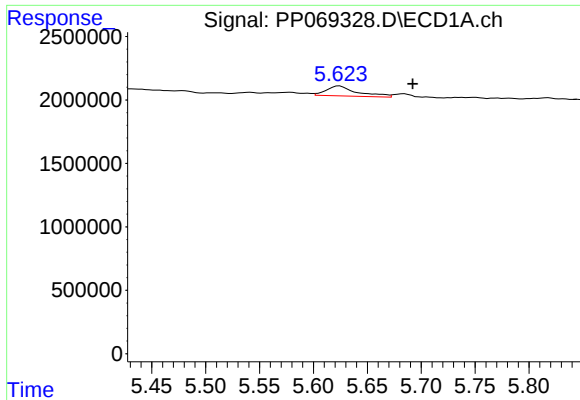

#3 AR-1016-1


R.T.: 5.624 min
Delta R.T.: -0.068 min
Response: 1577430
Conc: 34.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

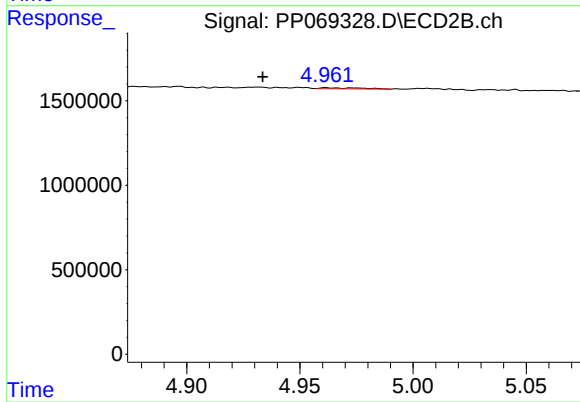


#3 AR-1016-1

R.T.: 4.962 min
Delta R.T.: 0.028 min
Response: 78171
Conc: 2.40 ng/ml

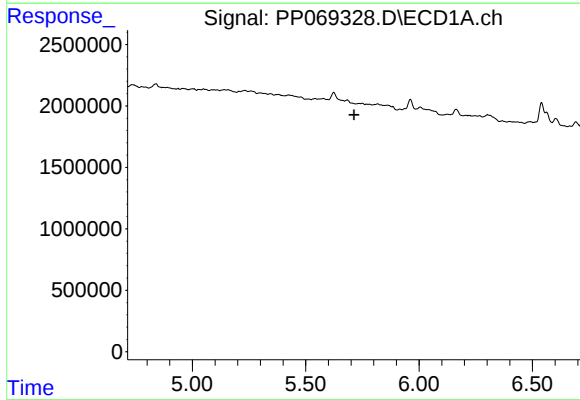


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T. : 5.714 min
Response: 0
Conc: N.D.

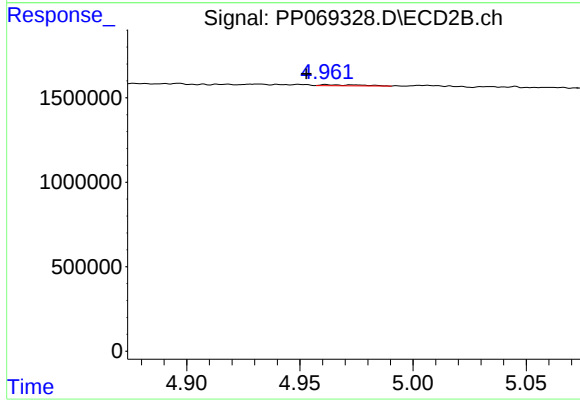

#4 AR-1016-2


R.T.: 4.962 min
Delta R.T.: 0.009 min
Response: 78171
Conc: 1.74 ng/ml

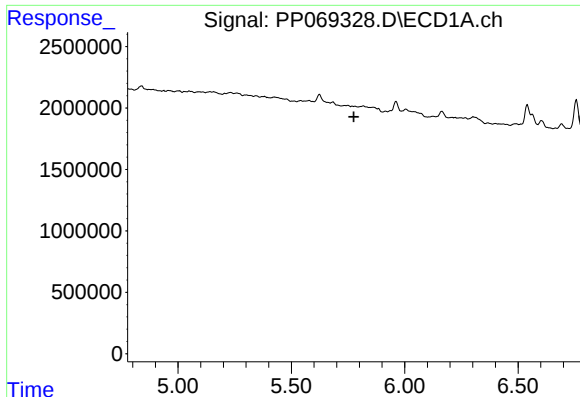

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

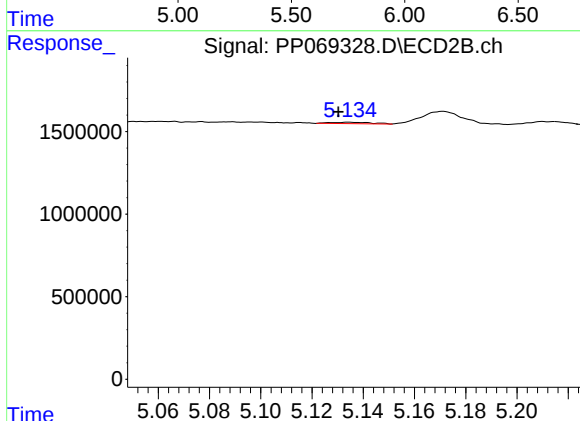


#5 AR-1016-3

R.T.: 5.134 min
Delta R.T.: 0.004 min
Response: 94601
Conc: 3.80 ng/ml

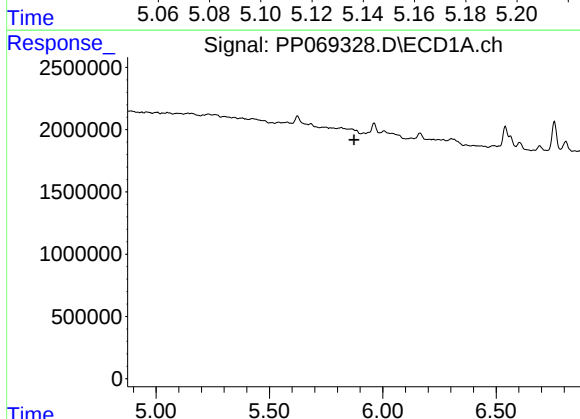


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.874 min
Response: 0
Conc: N.D.

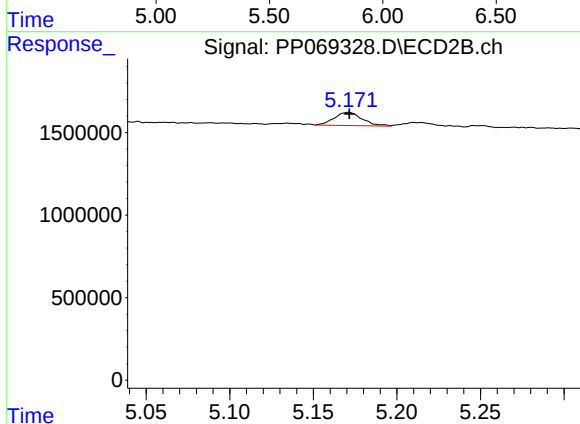

#6 AR-1016-4


R.T.: 5.171 min
Delta R.T.: 0.000 min
Response: 920748
Conc: 45.59 ng/ml

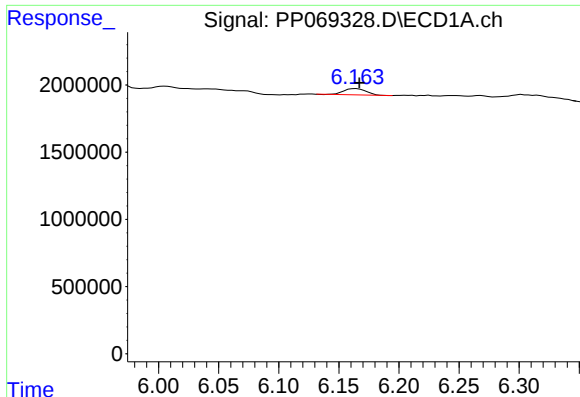

#7 AR-1016-5


R.T.: 6.164 min
Delta R.T.: -0.003 min
Response: 616230
Conc: 18.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

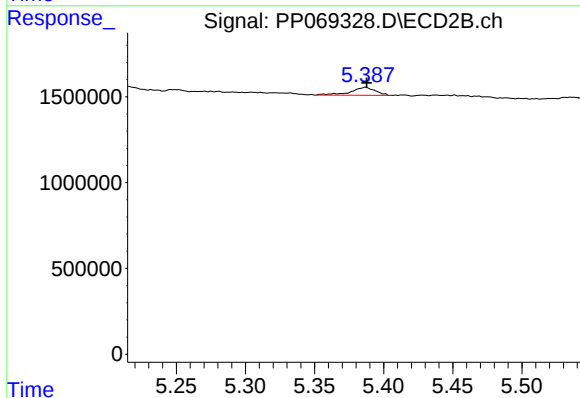


#7 AR-1016-5

R.T.: 5.387 min
Delta R.T.: 0.000 min
Response: 586082
Conc: 21.85 ng/ml

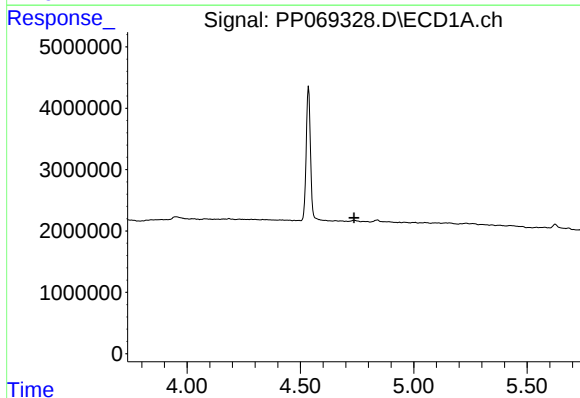


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.737 min
Response: 0
Conc: N.D.

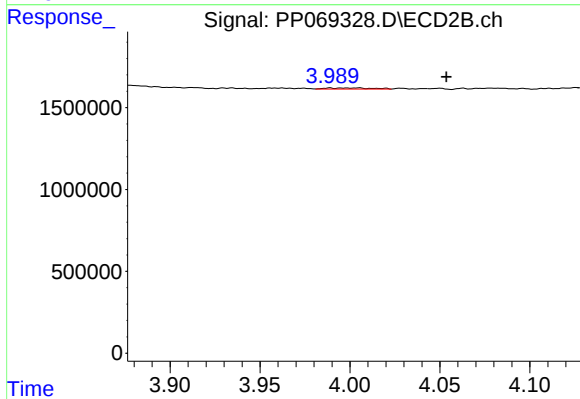

#8 AR-1221-1


R.T.: 3.989 min
Delta R.T.: -0.065 min
Response: 124714
Conc: 10.12 ng/ml

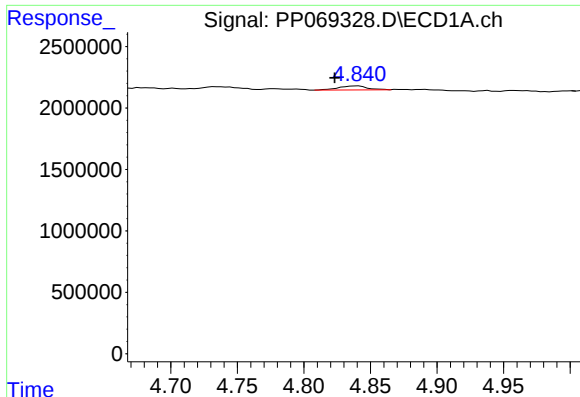

#9 AR-1221-2


R.T.: 4.840 min
Delta R.T.: 0.017 min
Response: 478853
Conc: 34.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

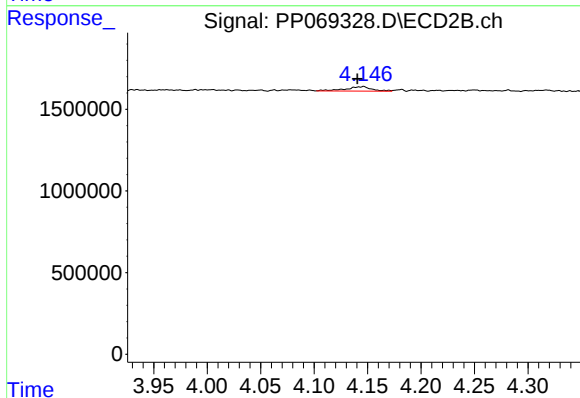


#9 AR-1221-2

R.T.: 4.146 min
Delta R.T.: 0.006 min
Response: 454880
Conc: 46.98 ng/ml

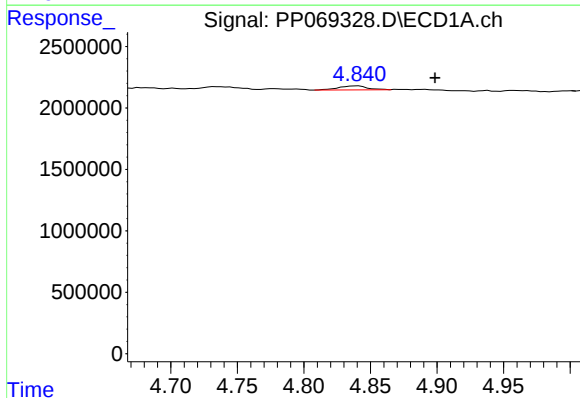


#10 AR-1221-3

R.T.: 4.840 min
Delta R.T.: -0.058 min
Response: 478853
Conc: 11.42 ng/ml

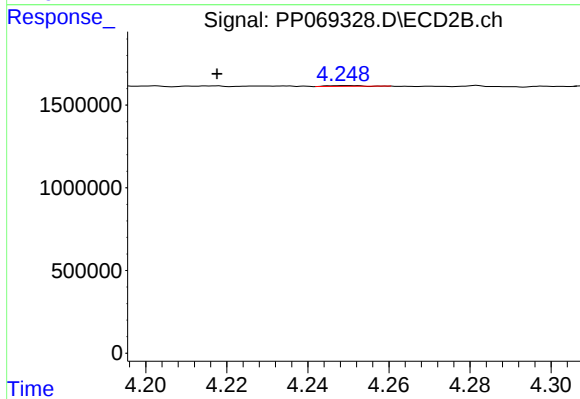

#10 AR-1221-3


R.T.: 4.250 min
Delta R.T.: 0.032 min
Response: 25199
Conc: 0.86 ng/ml

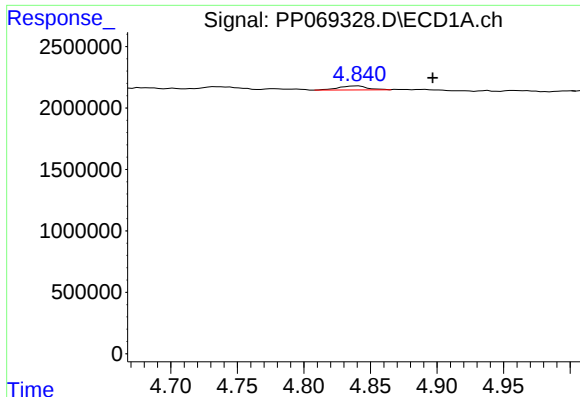

#11 AR-1232-1


R.T.: 4.840 min
Delta R.T.: -0.056 min
Response: 478853
Conc: 14.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

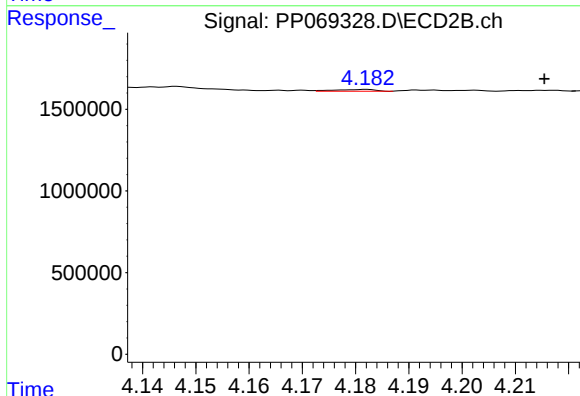


#11 AR-1232-1

R.T.: 4.181 min
Delta R.T.: -0.034 min
Response: 54820
Conc: 2.33 ng/ml

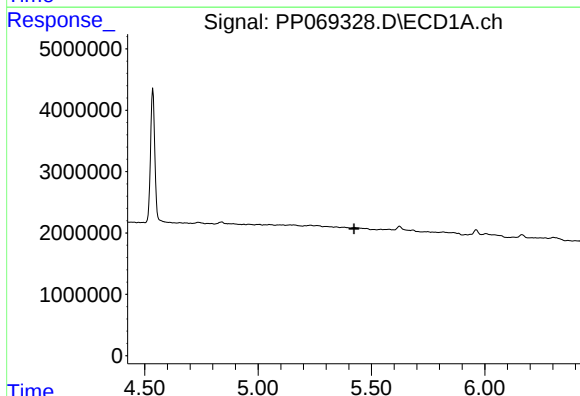


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.424 min
Response: 0
Conc: N.D.

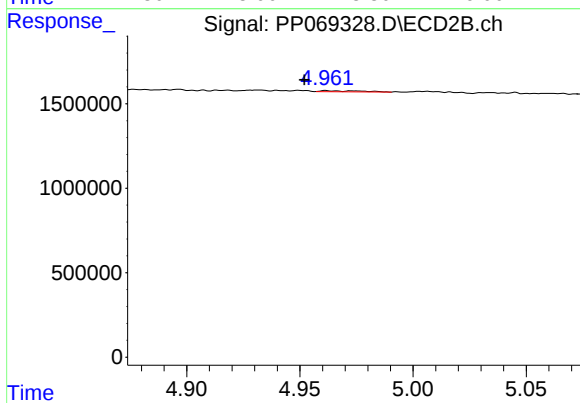

#12 AR-1232-2


R.T.: 4.962 min
Delta R.T.: 0.010 min
Response: 78171
Conc: 3.32 ng/ml

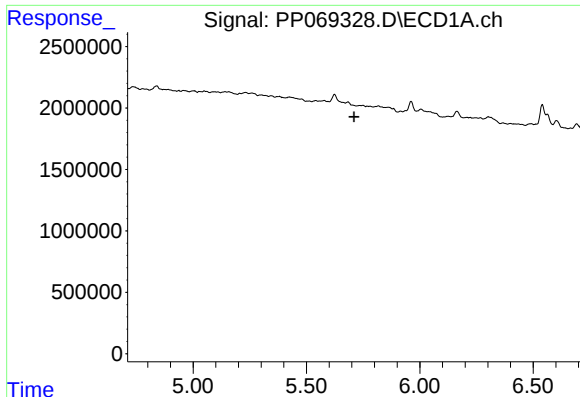

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.710 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

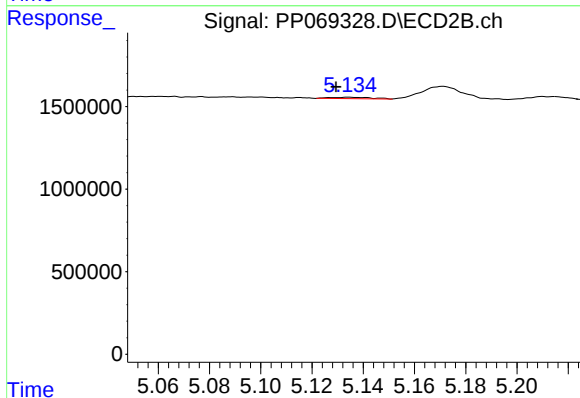


#13 AR-1232-3

R.T.: 5.134 min
Delta R.T.: 0.005 min
Response: 94601
Conc: 7.31 ng/ml

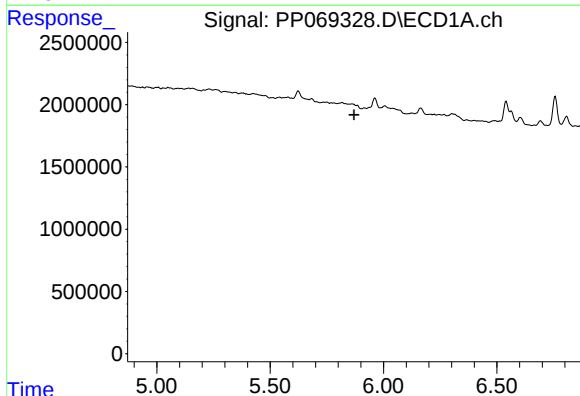


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.870 min
Response: 0
Conc: N.D.

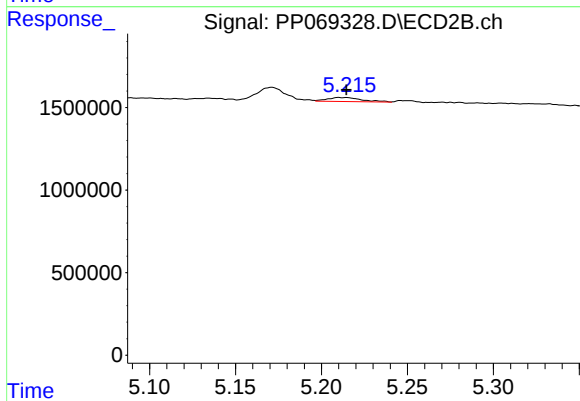

#14 AR-1232-4


R.T.: 5.210 min
Delta R.T.: -0.004 min
Response: 334078
Conc: 30.13 ng/ml

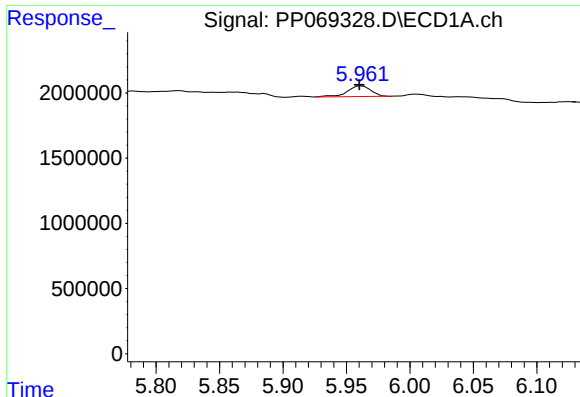

#15 AR-1232-5


R.T.: 5.962 min
Delta R.T.: 0.002 min
Response: 1042814
Conc: 90.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

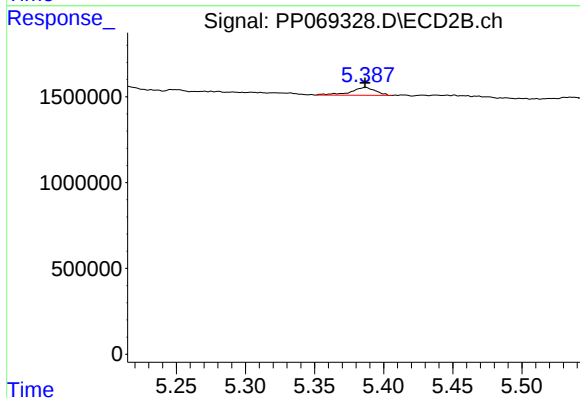


#15 AR-1232-5

R.T.: 5.387 min
Delta R.T.: 0.000 min
Response: 586082
Conc: 48.00 ng/ml

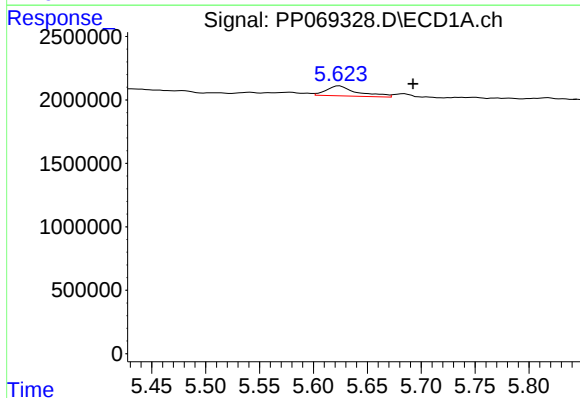


#16 AR-1242-1

R.T.: 5.624 min
Delta R.T.: -0.068 min
Response: 1577430
Conc: 37.82 ng/ml

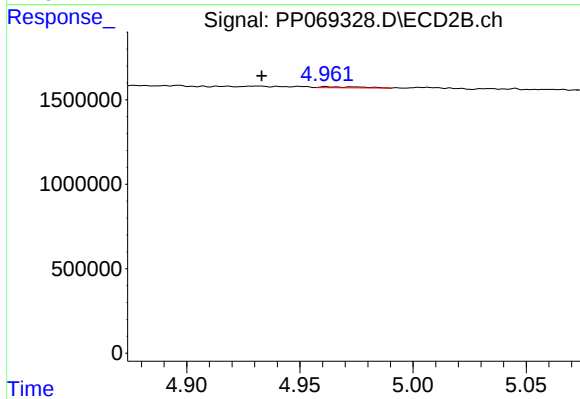

#16 AR-1242-1


R.T.: 4.962 min
Delta R.T.: 0.028 min
Response: 78171
Conc: 2.71 ng/ml

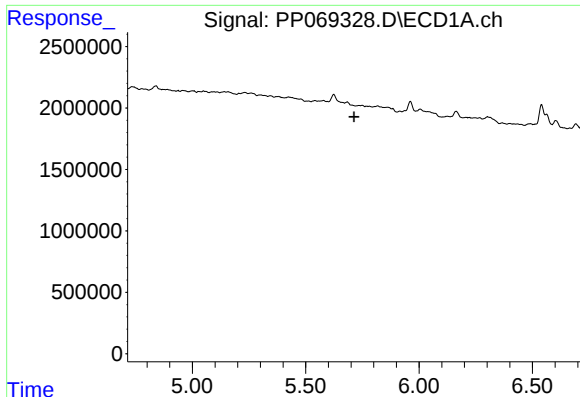

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.714 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

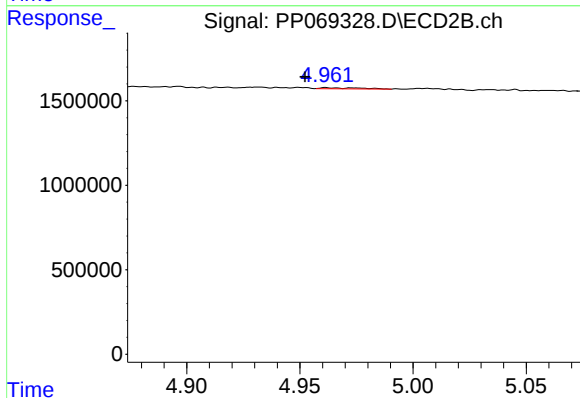


#17 AR-1242-2

R.T.: 4.962 min
Delta R.T.: 0.009 min
Response: 78171
Conc: 1.98 ng/ml

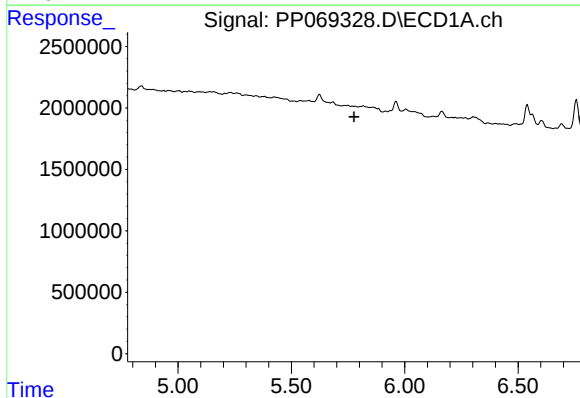


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.776 min
Response: 0
Conc: N.D.

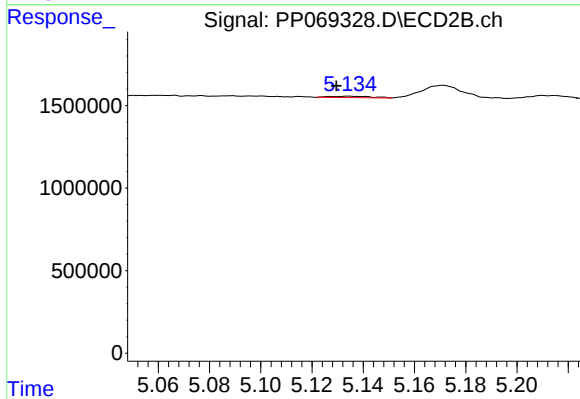

#18 AR-1242-3


R.T.: 5.134 min
Delta R.T.: 0.005 min
Response: 94601
Conc: 4.20 ng/ml

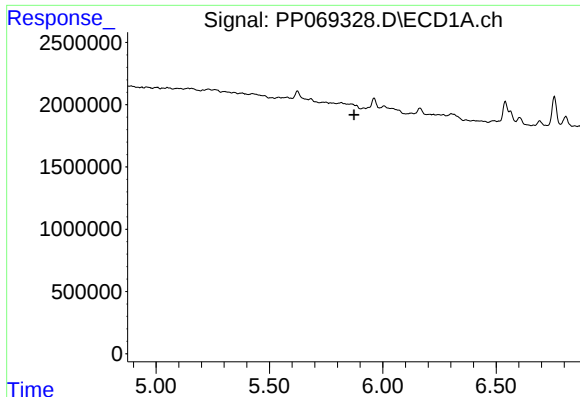

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.874 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

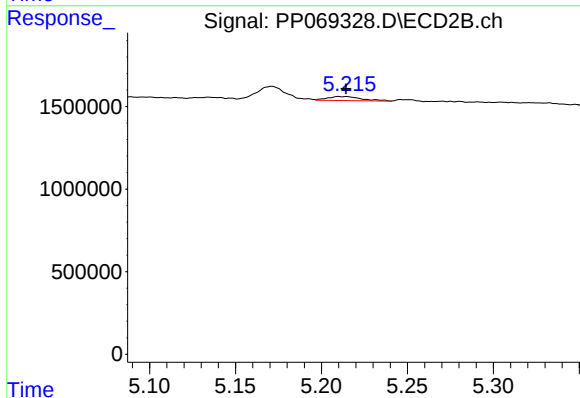


#19 AR-1242-4

R.T.: 5.210 min
Delta R.T.: -0.004 min
Response: 334078
Conc: 15.48 ng/ml

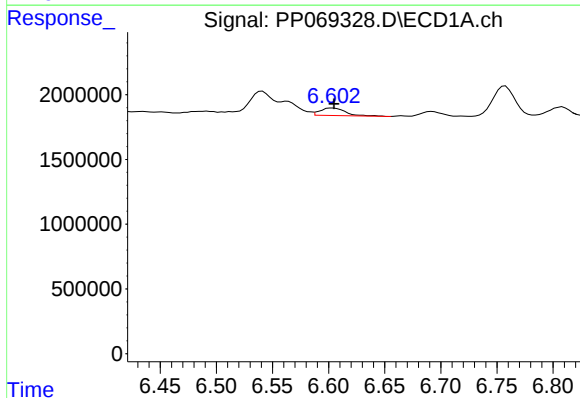


#20 AR-1242-5

R.T.: 6.604 min
Delta R.T.: -0.001 min
Response: 910747
Conc: 27.95 ng/ml

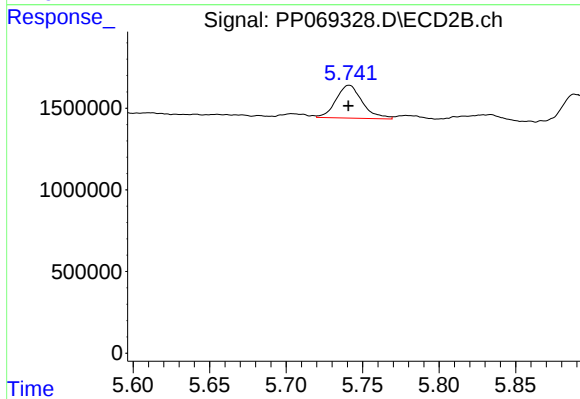

#20 AR-1242-5


R.T.: 5.741 min
Delta R.T.: 0.000 min
Response: 2400880
Conc: 83.46 ng/ml

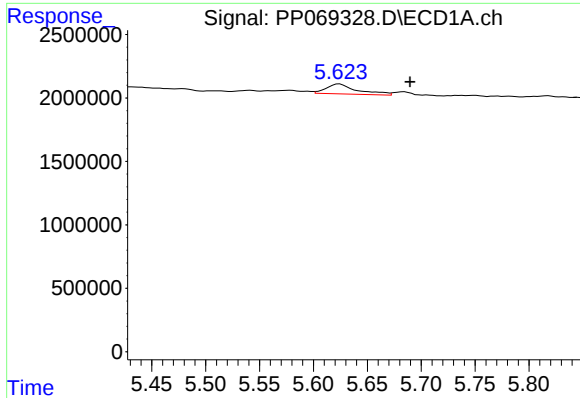

#21 AR-1248-1


R.T.: 5.624 min
Delta R.T.: -0.066 min
Response: 1577430
Conc: 48.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

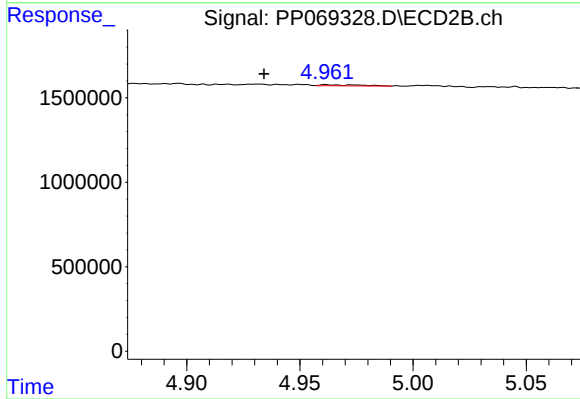


#21 AR-1248-1

R.T.: 4.962 min
Delta R.T.: 0.027 min
Response: 78171
Conc: 3.55 ng/ml

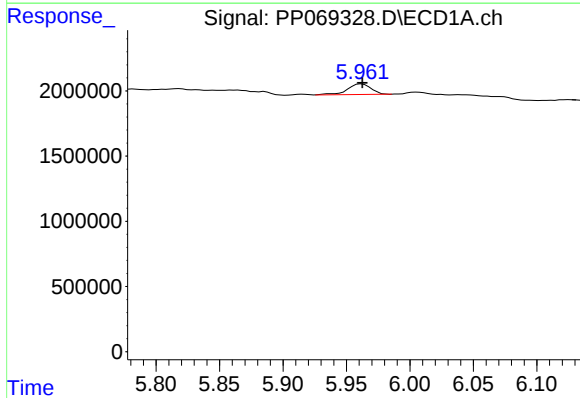


#22 AR-1248-2

R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 1042814
Conc: 24.57 ng/ml

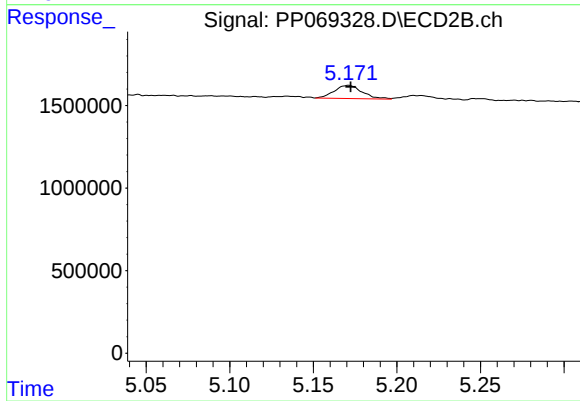

#22 AR-1248-2


R.T.: 5.171 min
Delta R.T.: -0.001 min
Response: 920748
Conc: 30.63 ng/ml

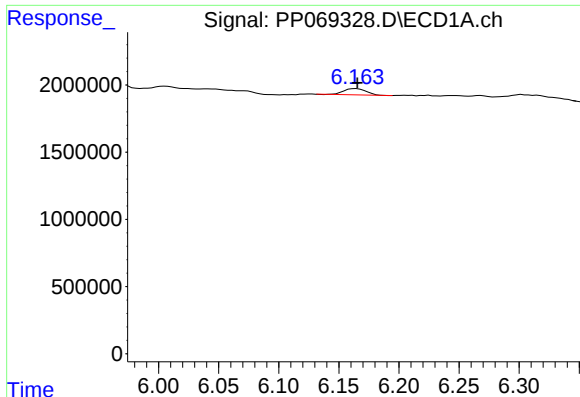

#23 AR-1248-3


R.T.: 6.164 min
Delta R.T.: -0.001 min
Response: 616230
Conc: 13.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

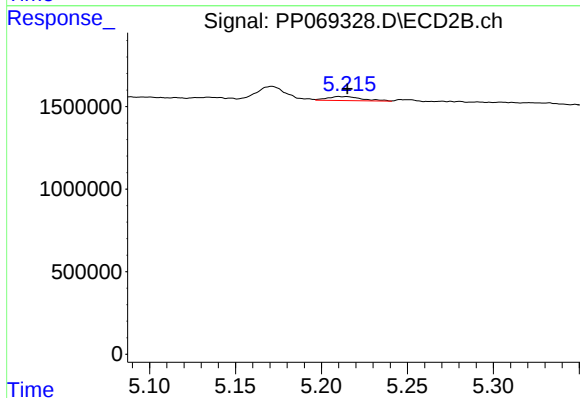


#23 AR-1248-3

R.T.: 5.210 min
Delta R.T.: -0.005 min
Response: 334078
Conc: 10.78 ng/ml

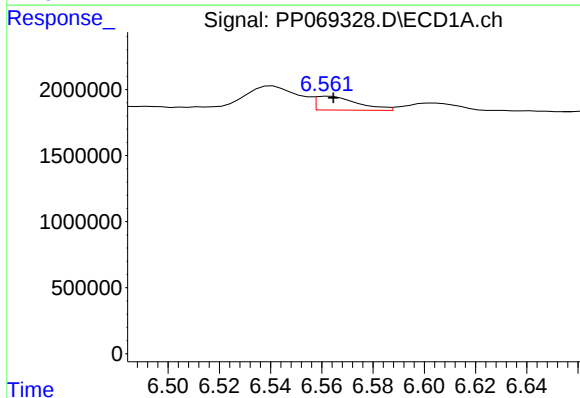


#24 AR-1248-4

R.T.: 6.563 min
Delta R.T.: -0.001 min
Response: 1193994
Conc: 21.66 ng/ml

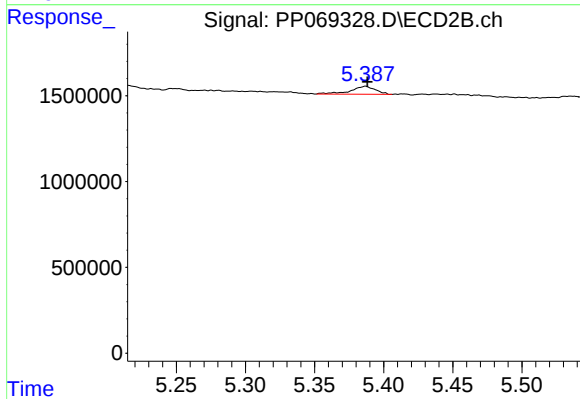

#24 AR-1248-4


R.T.: 5.387 min
Delta R.T.: -0.001 min
Response: 586082
Conc: 15.86 ng/ml

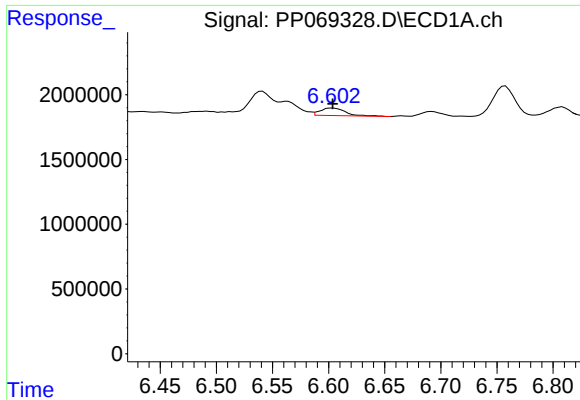

#25 AR-1248-5


R.T.: 6.604 min
Delta R.T.: 0.000 min
Response: 910747
Conc: 17.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

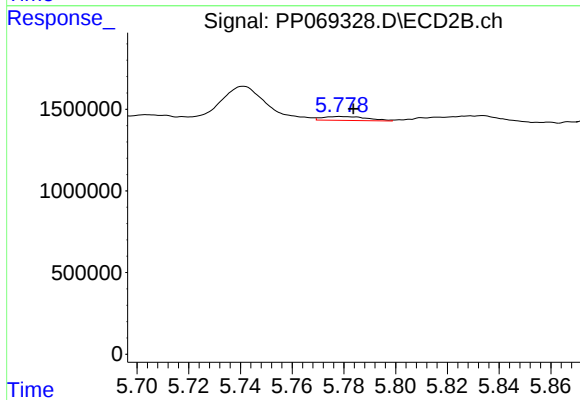


#25 AR-1248-5

R.T.: 5.779 min
Delta R.T.: -0.005 min
Response: 285322
Conc: 7.63 ng/ml

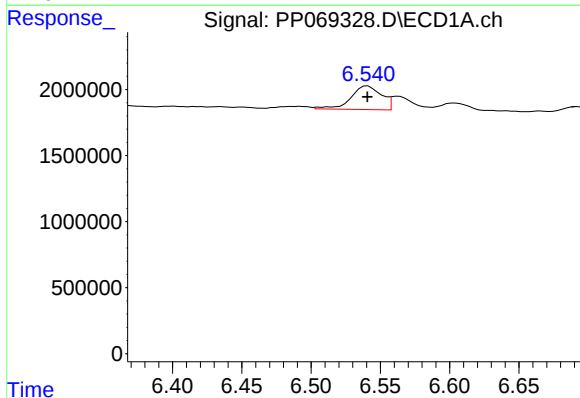


#26 AR-1254-1

R.T.: 6.541 min
Delta R.T.: 0.000 min
Response: 2737579
Conc: 47.31 ng/ml

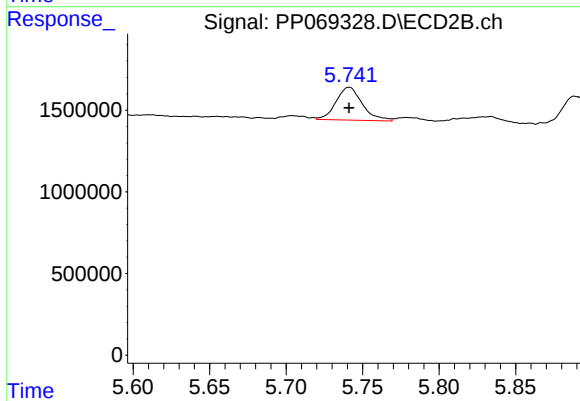

#26 AR-1254-1


R.T.: 5.741 min
Delta R.T.: 0.000 min
Response: 2400880
Conc: 43.61 ng/ml

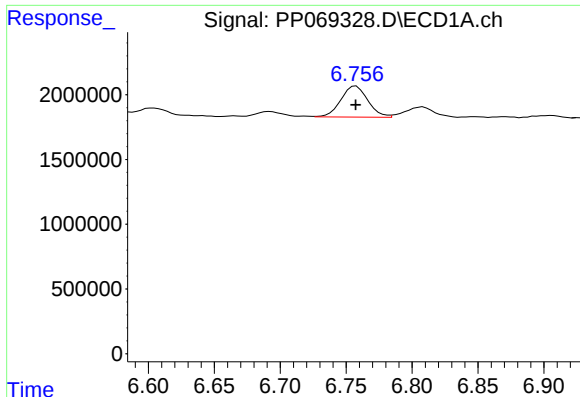

#27 AR-1254-2


R.T.: 6.757 min
Delta R.T.: 0.000 min
Response: 3408653
Conc: 42.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

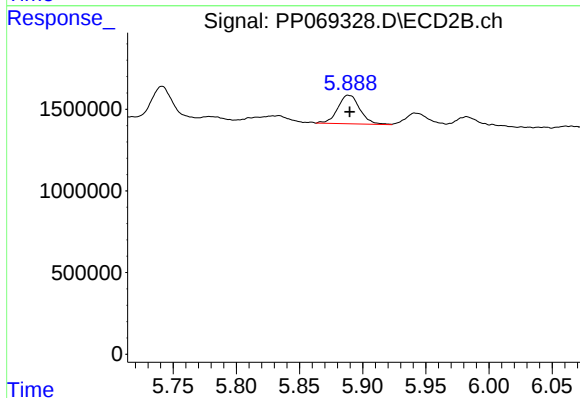


#27 AR-1254-2

R.T.: 5.889 min
Delta R.T.: 0.000 min
Response: 2140742
Conc: 44.26 ng/ml

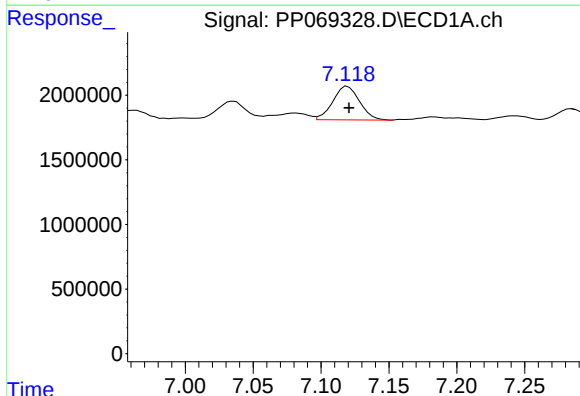


#28 AR-1254-3

R.T.: 7.120 min
Delta R.T.: 0.000 min
Response: 3565936
Conc: 42.31 ng/ml

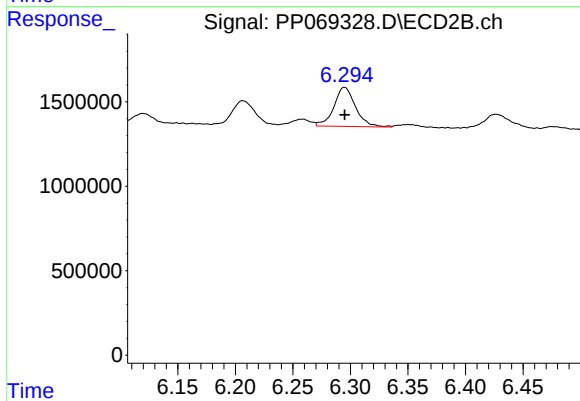

#28 AR-1254-3


R.T.: 6.295 min
Delta R.T.: 0.000 min
Response: 3046702
Conc: 40.14 ng/ml

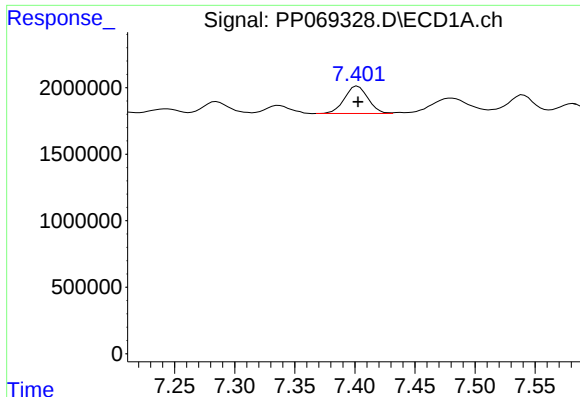

#29 AR-1254-4


R.T.: 7.402 min
Delta R.T.: 0.000 min
Response: 2802867
Conc: 41.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

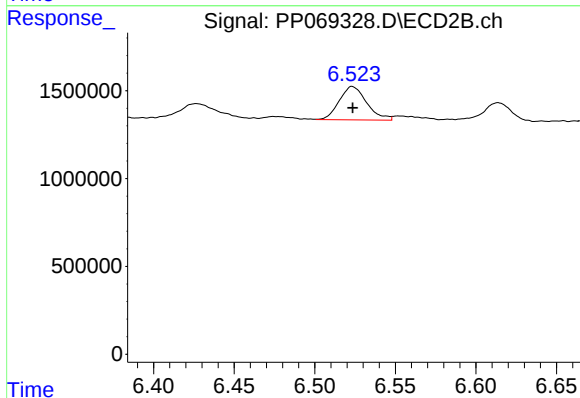


#29 AR-1254-4

R.T.: 6.523 min
Delta R.T.: 0.000 min
Response: 2249336
Conc: 43.89 ng/ml

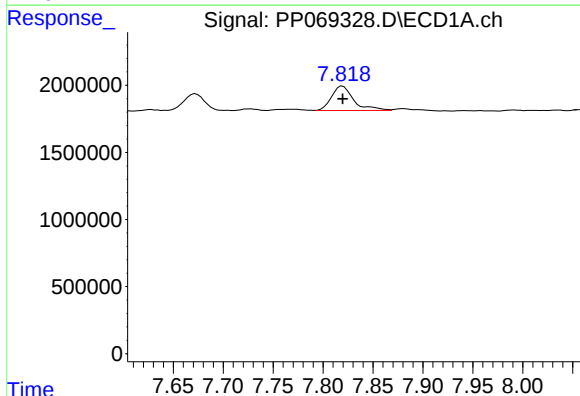


#30 AR-1254-5

R.T.: 7.820 min
Delta R.T.: 0.000 min
Response: 2827862
Conc: 41.56 ng/ml

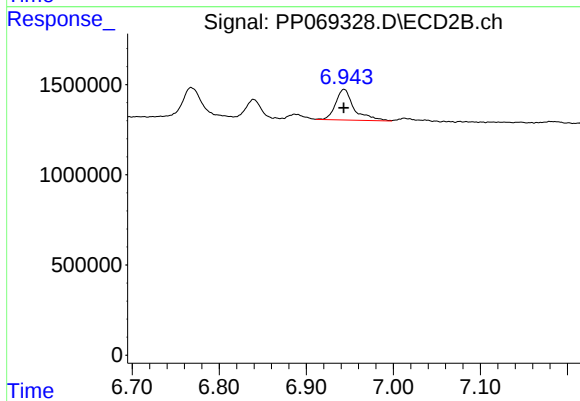

#30 AR-1254-5


R.T.: 6.944 min
Delta R.T.: 0.000 min
Response: 2521897
Conc: 37.89 ng/ml

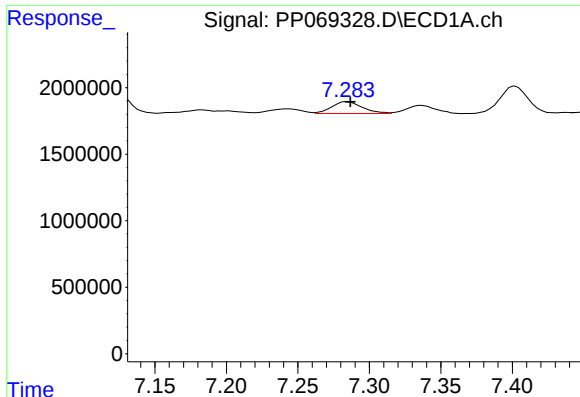

#31 AR-1260-1


R.T.: 7.285 min
Delta R.T.: -0.002 min
Response: 1319402
Conc: 22.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

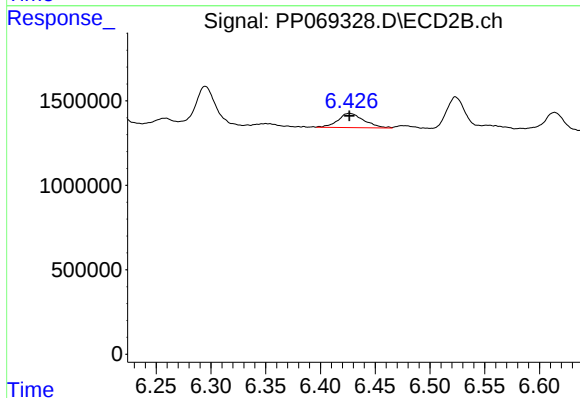


#31 AR-1260-1

R.T.: 6.427 min
Delta R.T.: 0.000 min
Response: 1399866
Conc: 29.03 ng/ml

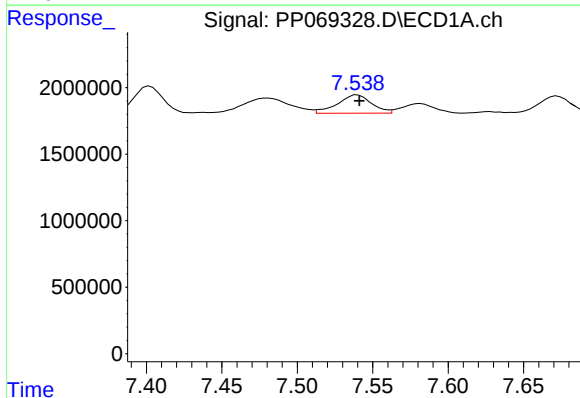


#32 AR-1260-2

R.T.: 7.540 min
Delta R.T.: -0.001 min
Response: 2177805
Conc: 27.99 ng/ml

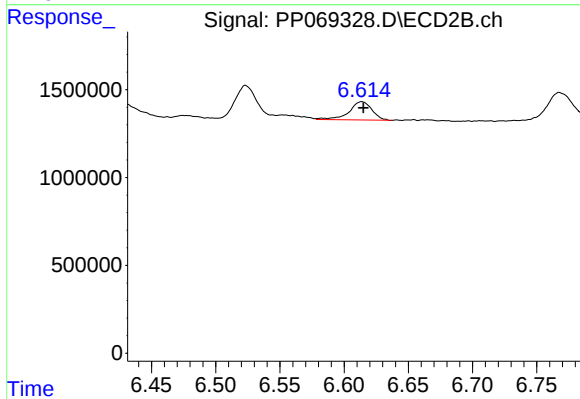

#32 AR-1260-2


R.T.: 6.614 min
Delta R.T.: -0.001 min
Response: 1295604
Conc: 21.13 ng/ml

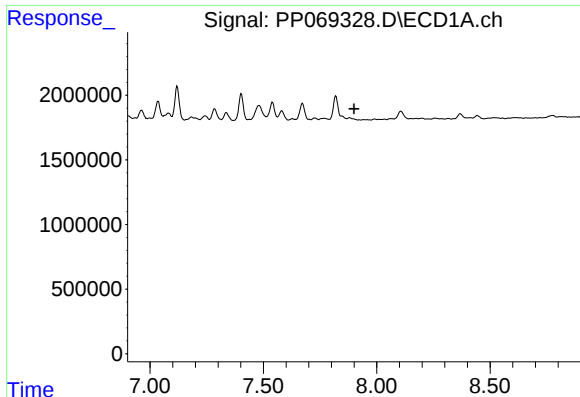

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.900 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

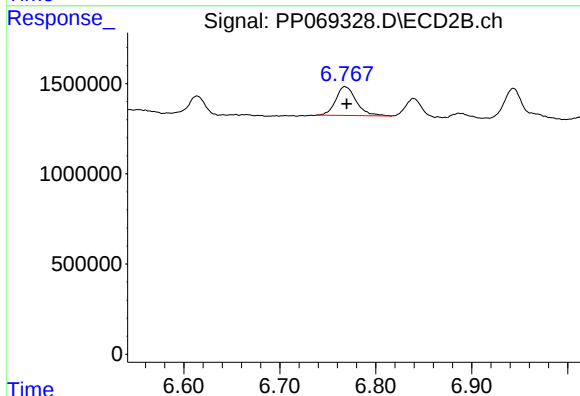


#33 AR-1260-3

R.T.: 6.768 min
Delta R.T.: -0.002 min
Response: 2383935
Conc: 39.63 ng/ml

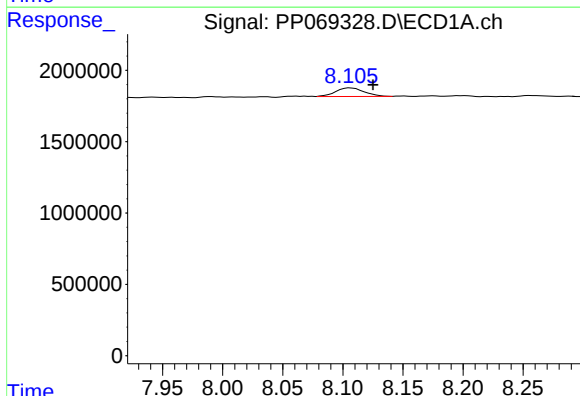


#34 AR-1260-4

R.T.: 8.106 min
Delta R.T.: -0.019 min
Response: 987797
Conc: 14.97 ng/ml

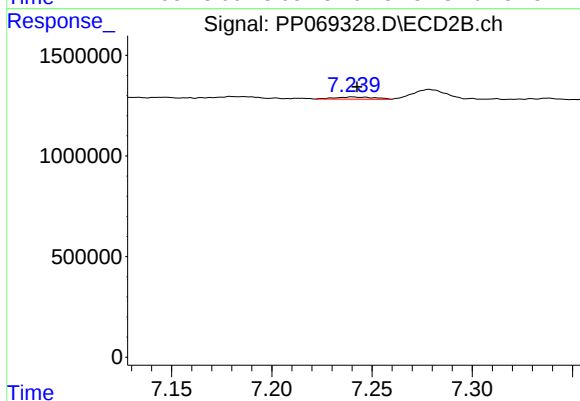

#34 AR-1260-4


R.T.: 7.240 min
Delta R.T.: -0.002 min
Response: 153253
Conc: 3.30 ng/ml

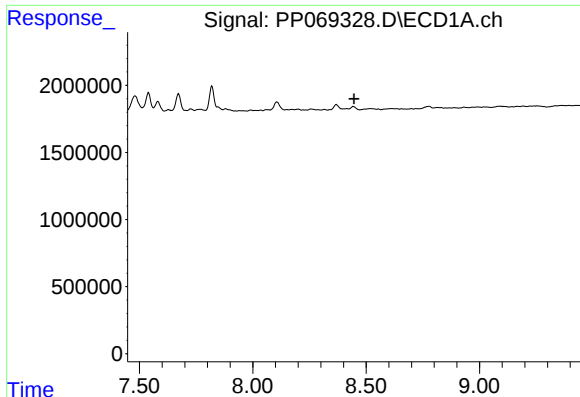

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.447 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

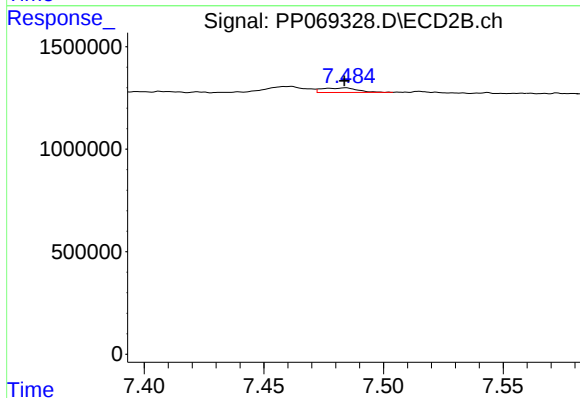


#35 AR-1260-5

R.T.: 7.484 min
Delta R.T.: 0.000 min
Response: 227693
Conc: 2.05 ng/ml

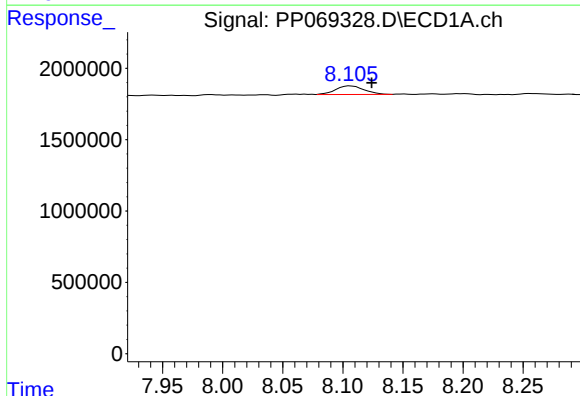


#36 AR-1262-1

R.T.: 8.106 min
Delta R.T.: -0.018 min
Response: 987797
Conc: 12.50 ng/ml

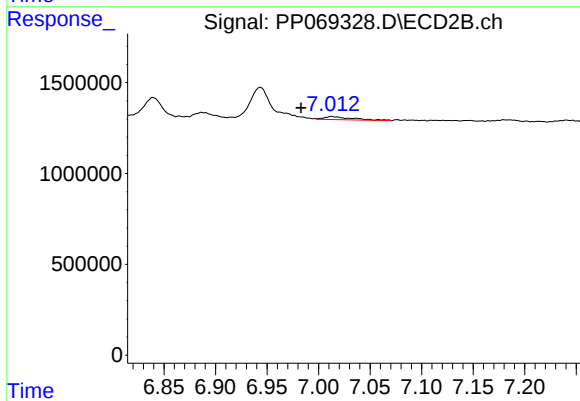

#36 AR-1262-1


R.T.: 7.013 min
Delta R.T.: 0.030 min
Response: 330235
Conc: 4.65 ng/ml

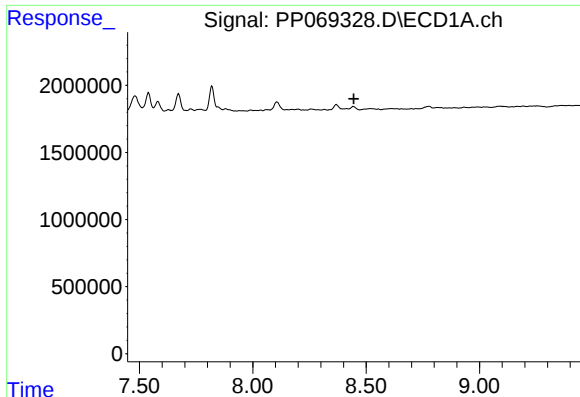

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.446 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

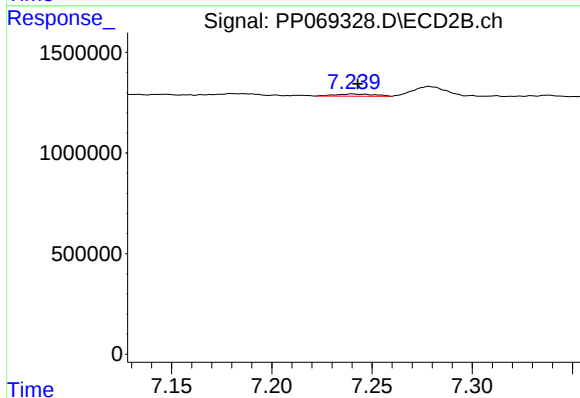


#37 AR-1262-2

R.T.: 7.240 min
Delta R.T.: -0.003 min
Response: 153253
Conc: 2.51 ng/ml

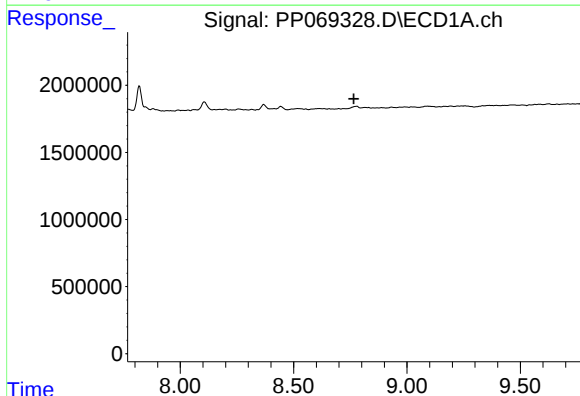


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.766 min
Response: 0
Conc: N.D.

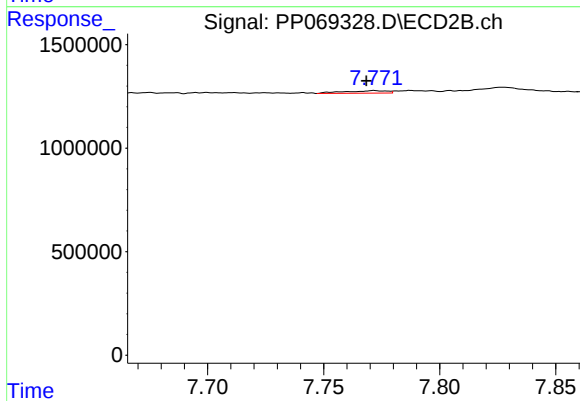

#38 AR-1262-3


R.T.: 7.772 min
Delta R.T.: 0.003 min
Response: 152347
Conc: 2.91 ng/ml

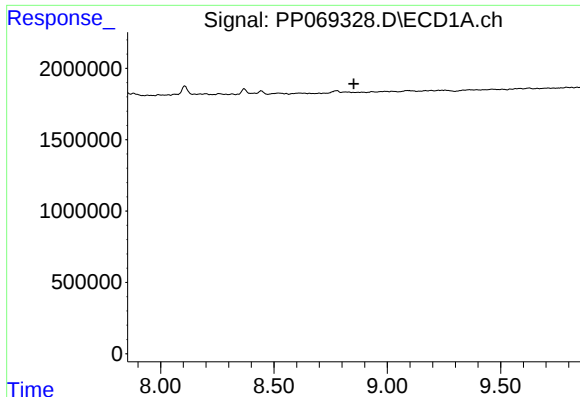

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.852 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

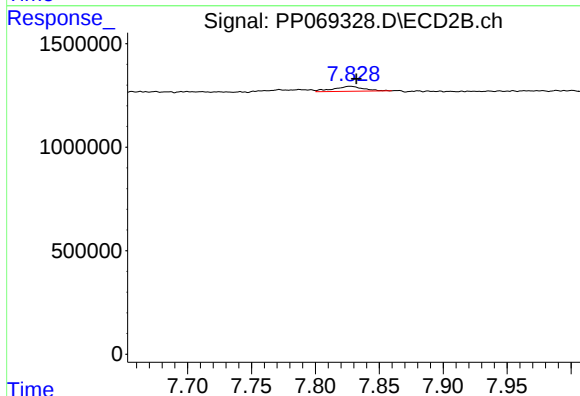


#39 AR-1262-4

R.T.: 7.827 min
Delta R.T.: -0.005 min
Response: 388152
Conc: 4.20 ng/ml

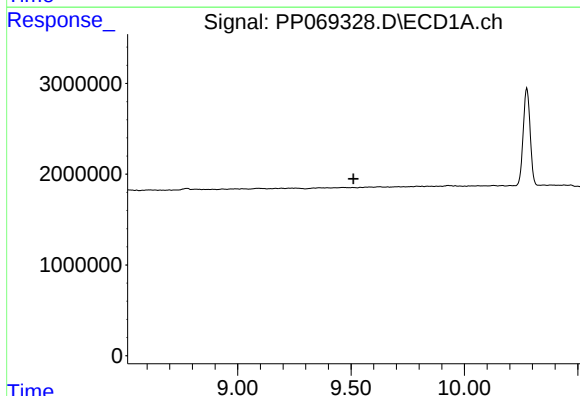


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.511 min
Response: 0
Conc: N.D.

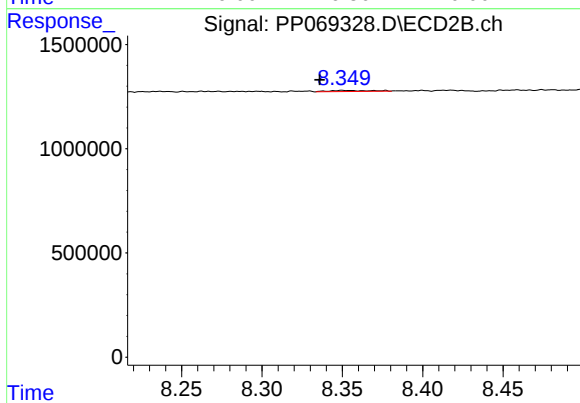

#40 AR-1262-5


R.T.: 8.350 min
Delta R.T.: 0.014 min
Response: 86744
Conc: 1.82 ng/ml

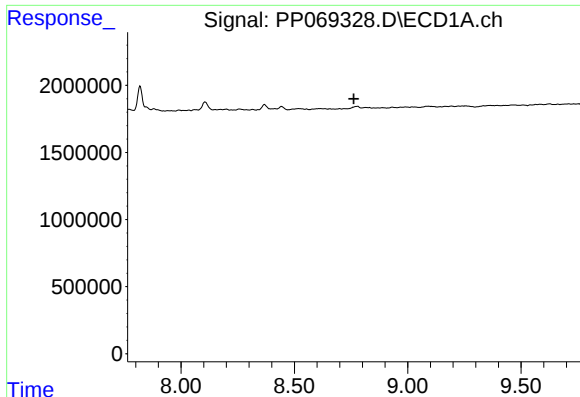

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

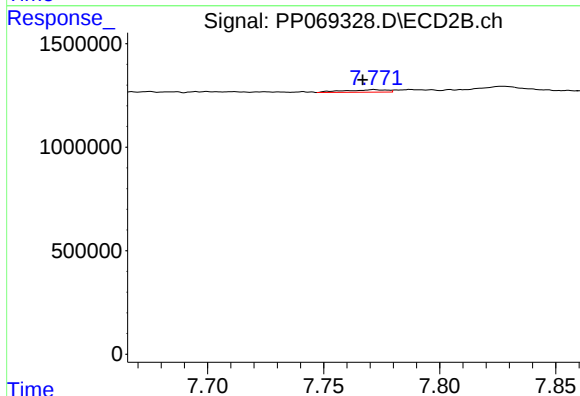


#41 AR-1268-1

R.T.: 7.772 min
Delta R.T.: 0.005 min
Response: 152347
Conc: 1.05 ng/ml

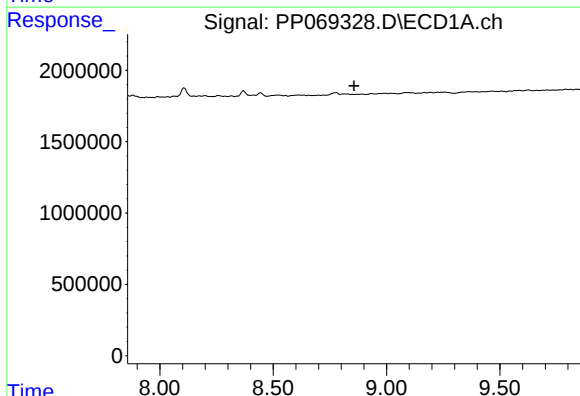


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.857 min
Response: 0
Conc: N.D.

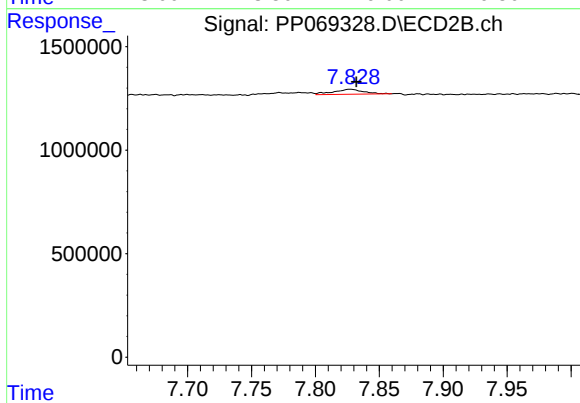

#42 AR-1268-2


R.T.: 7.827 min
Delta R.T.: -0.005 min
Response: 388152
Conc: 2.92 ng/ml

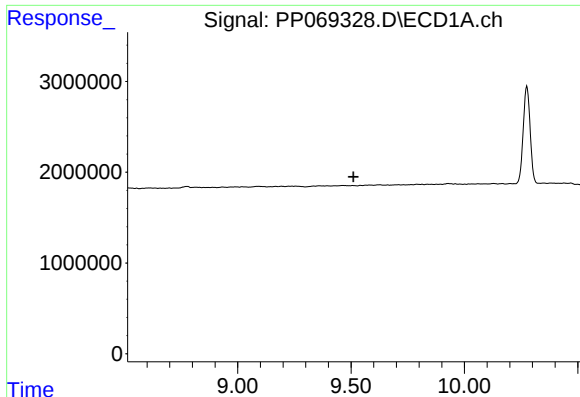

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 9.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

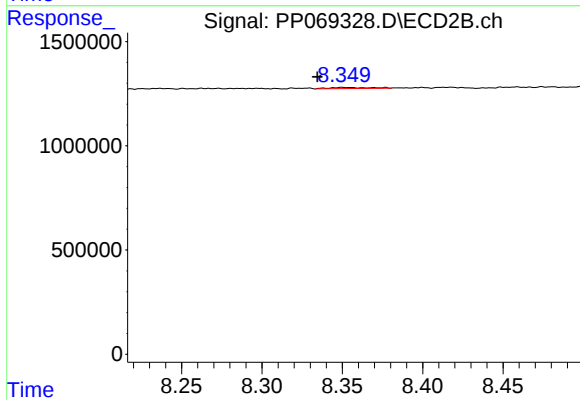


#44 AR-1268-4

R.T.: 8.350 min
Delta R.T.: 0.015 min
Response: 86744
Conc: 1.67 ng/ml

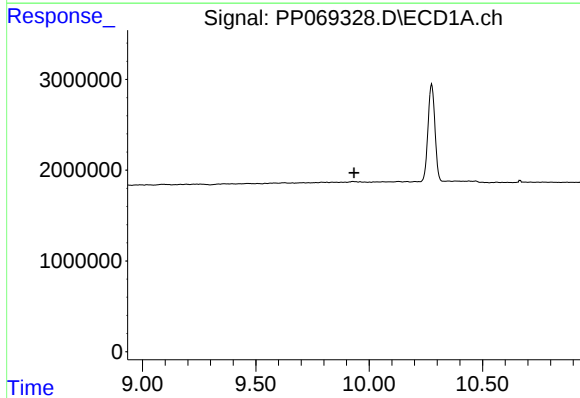

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.933 min
Response: 0
Conc: N.D.

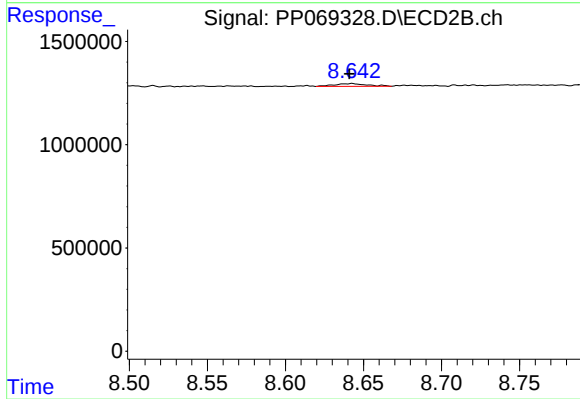

#45 AR-1268-5

R.T.: 8.643 min
Delta R.T.: 0.002 min
Response: 196730
Conc: 0.55 ng/ml