

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
 Data File : PP069365.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2025 02:56
 Operator : YP\AJ
 Sample : Q1168-09
 Misc : AR1660 MDL 25 PPB
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT1-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:21:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.535	3.838	28126591	18094524	19.649	20.273
2)	SA Decachlor...	10.272	8.905	23011778	21967047	21.056	19.640
Target Compounds							
3)	L1 AR-1016-1	5.688	4.931	1477726	842259	31.894	25.824
4)	L1 AR-1016-2	5.709	4.949	2096722	1120760	30.890	24.929
5)	L1 AR-1016-3	5.772	5.127	1484166	630289	34.842	25.329 #
6)	L1 AR-1016-4	5.871	5.168	1047227	477711	29.920	23.653
7)	L1 AR-1016-5	6.162	5.384	742377	616334	22.456	22.977
8)	L2 AR-1221-1	4.736	4.053	952228	93267	50.066	7.572 #
9)	L2 AR-1221-2	4.838	4.141	593827	620689	43.369	64.098 #
10)	L2 AR-1221-3	4.898	4.213	934092	444160	22.270	15.224 #
11)	L3 AR-1232-1	4.898	4.213	934092	444160	28.056	18.917 #
12)	L3 AR-1232-2	5.424	4.949	993078	1120760	60.768	47.547
13)	L3 AR-1232-3	5.709	5.127	2096722	630289	61.024	48.681
14)	L3 AR-1232-4	5.871	5.212	1047227	629310	58.779	56.765
15)	L3 AR-1232-5	5.959	5.384	1052387	616334	91.812	50.476 #
16)	L4 AR-1242-1	5.688	4.931	1477726	842259	35.433	29.213
17)	L4 AR-1242-2	5.709	4.949	2096722	1120760	35.543	28.447
18)	L4 AR-1242-3	5.772	5.127	1484166	630289	40.006	28.008 #
19)	L4 AR-1242-4	5.871	5.212	1047227	629310	31.933	29.159
20)	L4 AR-1242-5	6.537f	5.739	1506581	770023	46.236	26.766 #
21)	L5 AR-1248-1	5.688	4.931	1477726	842259	45.554	38.266
22)	L5 AR-1248-2	5.959	5.168	1052387	477711	24.793	15.889 #
23)	L5 AR-1248-3	6.162	5.212	742377	629310	15.800	20.311 #
24)	L5 AR-1248-4	6.537	5.384	1506581	616334	27.332	16.683 #
25)	L5 AR-1248-5	6.537f	5.775	1506581	211329	28.222	5.652 #
26)	L6 AR-1254-1	6.537	5.739	1506581	770023	26.037	13.986 #
27)	L6 AR-1254-2	6.756	5.887	795391	543194	9.912	11.230
28)	L6 AR-1254-3	7.113	6.308	764841	853533	9.074	11.246
29)	L6 AR-1254-4	7.402	6.519	671654	393413	9.850	7.676
30)	L6 AR-1254-5	7.815	6.940	2366079	1448145	34.772	21.757 #
31)	L7 AR-1260-1	7.282	6.423	1393754	1245436	23.851	25.823
32)	L7 AR-1260-2	7.537	6.611	2681653	1597941	34.463	26.066
33)	L7 AR-1260-3	7.896	6.766	1652718	2293790	26.435	38.130 #
34)	L7 AR-1260-4	8.120	7.239	1829668	1037223	27.732	22.321
35)	L7 AR-1260-5	8.441	7.478	3399993	2620706	25.969	23.579
36)	L8 AR-1262-1	8.120	6.979	1829668	1150555	23.155	16.202 #
37)	L8 AR-1262-2	8.441	7.239	3399993	1037223	22.233	17.009
38)	L8 AR-1262-3	8.765	7.763	2202277	810608	20.721	15.499 #
39)	L8 AR-1262-4	8.843	7.826	1522410	2088744	18.613	22.597
40)	L8 AR-1262-5	9.505	8.330	1080936	802197	19.094	16.785
41)	L9 AR-1268-1	8.765	7.763	2202277	810608	12.472	5.586 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
 Data File : PP069365.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2025 02:56
 Operator : YP\AJ
 Sample : Q1168-09
 Misc : AR1660 MDL 25 PPB
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT1-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:21:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.843	7.826	1522410	2088744	9.674	15.727 #
43) L9	AR-1268-3	0.000	8.063	0	20557	N.D.	0.181 #
44) L9	AR-1268-4	9.505	8.330	1080936	802197	18.408	15.404
45) L9	AR-1268-5	0.000	8.637	0	361486	N.D.	1.015 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
Data File : PP069365.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2025 02:56
Operator : YP\AJ
Sample : Q1168-09
Misc : AR1660 MDL 25 PPB
ALS Vial : 59 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:21:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

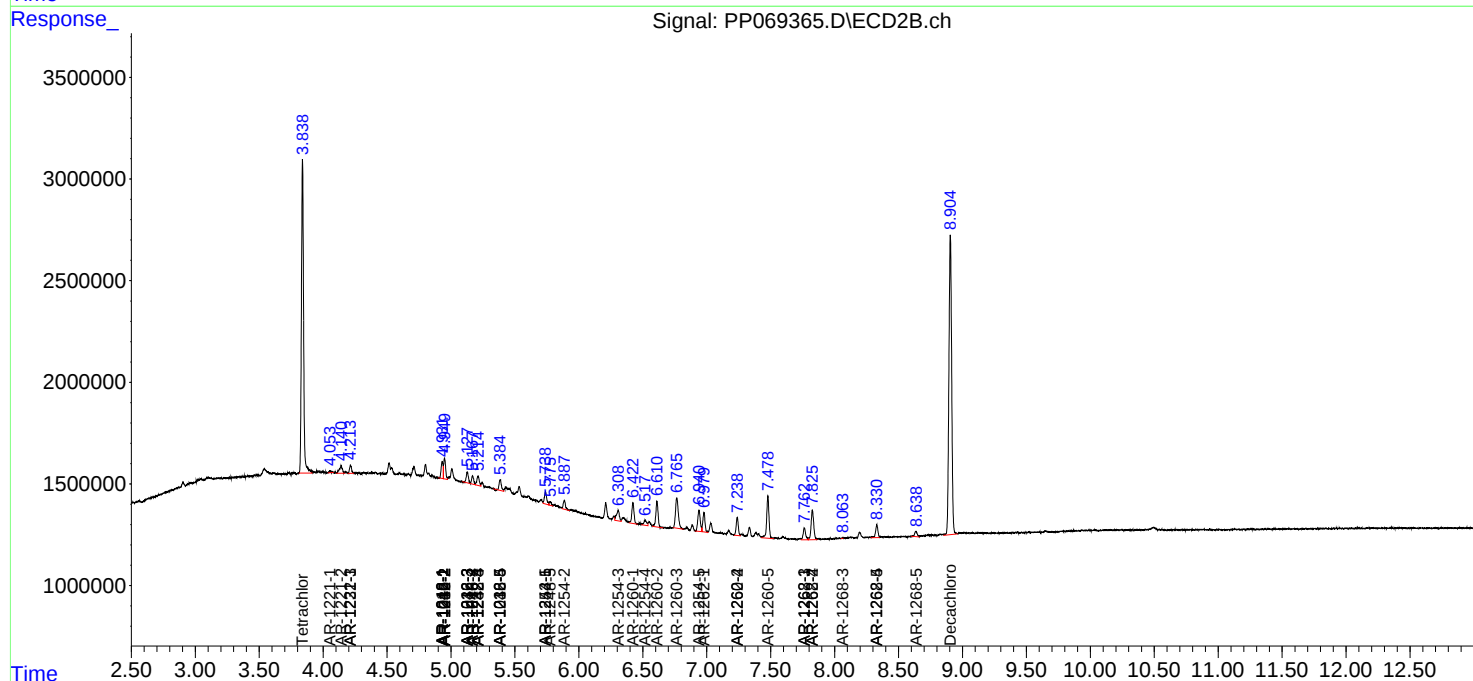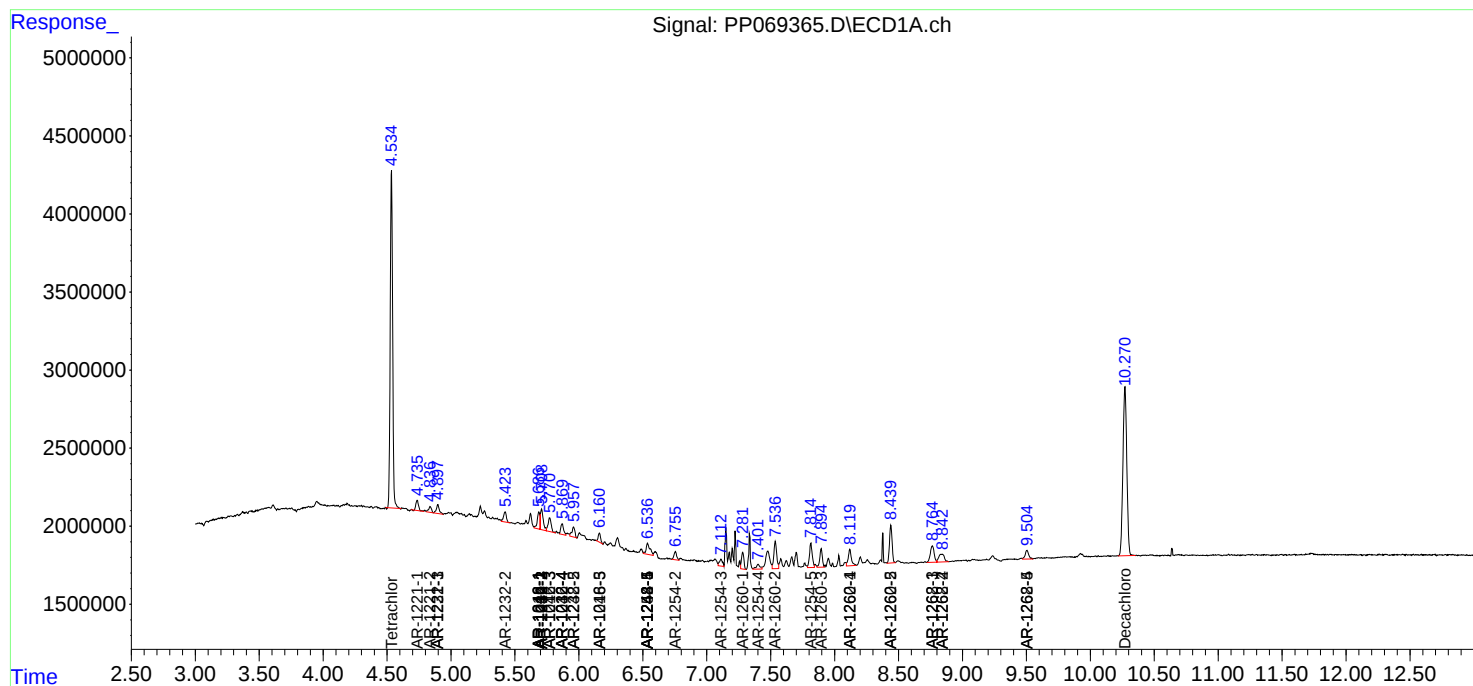


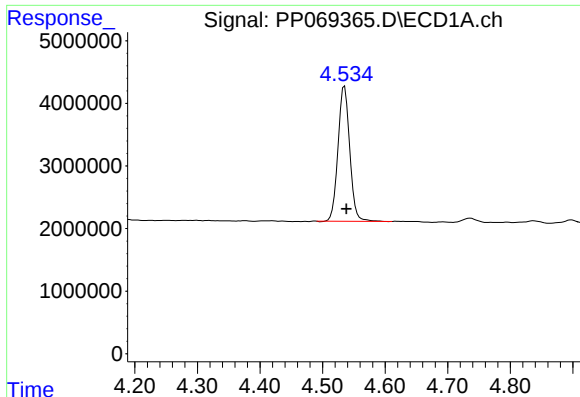

#1 Tetrachloro-m-xylene


R.T.: 4.535 min
Delta R.T.: -0.003 min
Response: 28126591
Conc: 19.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

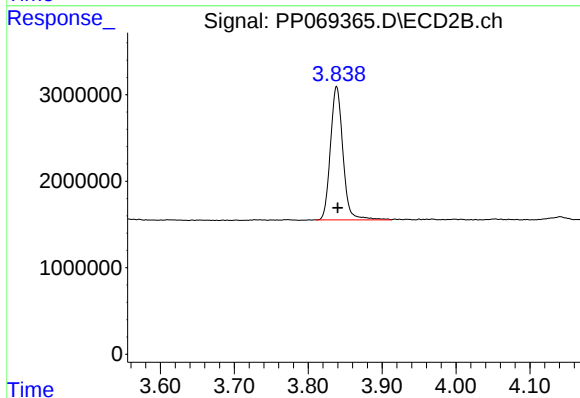


#1 Tetrachloro-m-xylene

R.T.: 3.838 min
Delta R.T.: -0.002 min
Response: 18094524
Conc: 20.27 ng/ml

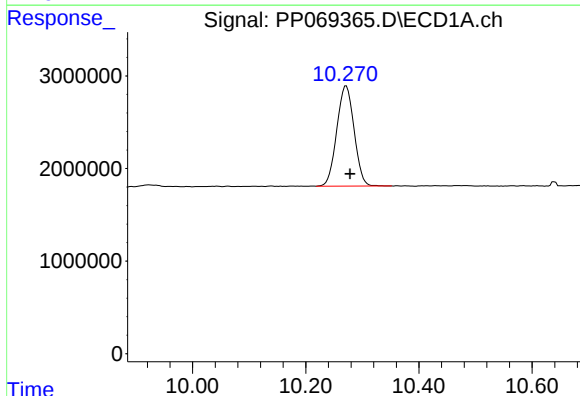


#2 Decachlorobiphenyl

R.T.: 10.272 min
Delta R.T.: -0.007 min
Response: 23011778
Conc: 21.06 ng/ml

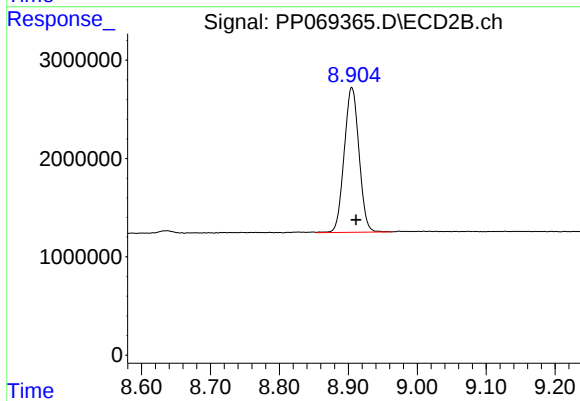

#2 Decachlorobiphenyl


R.T.: 8.905 min
Delta R.T.: -0.006 min
Response: 21967047
Conc: 19.64 ng/ml

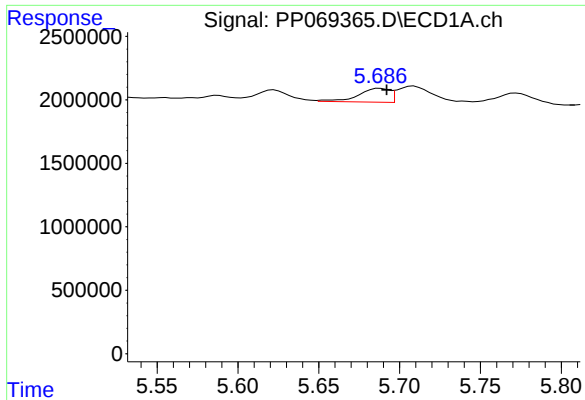

#3 AR-1016-1


R.T.: 5.688 min
Delta R.T.: -0.004 min
Response: 1477726
Conc: 31.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

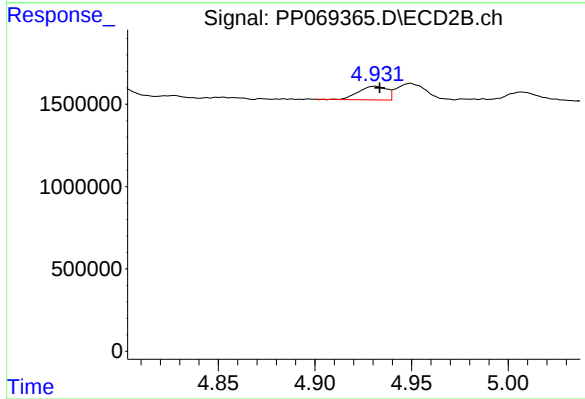


#3 AR-1016-1

R.T.: 4.931 min
Delta R.T.: -0.003 min
Response: 842259
Conc: 25.82 ng/ml

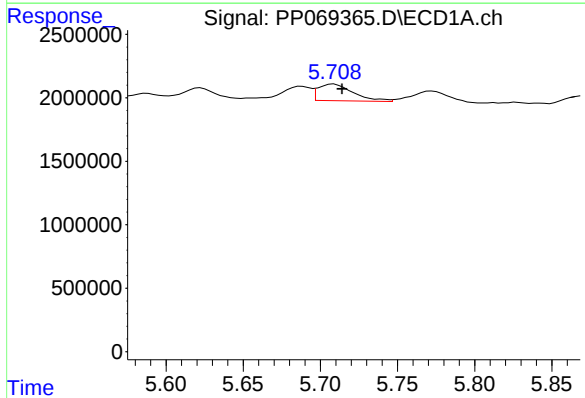


#4 AR-1016-2

R.T.: 5.709 min
Delta R.T.: -0.005 min
Response: 2096722
Conc: 30.89 ng/ml

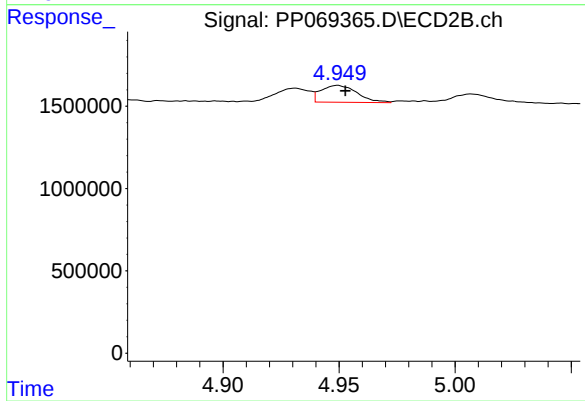

#4 AR-1016-2


R.T.: 4.949 min
Delta R.T.: -0.003 min
Response: 1120760
Conc: 24.93 ng/ml

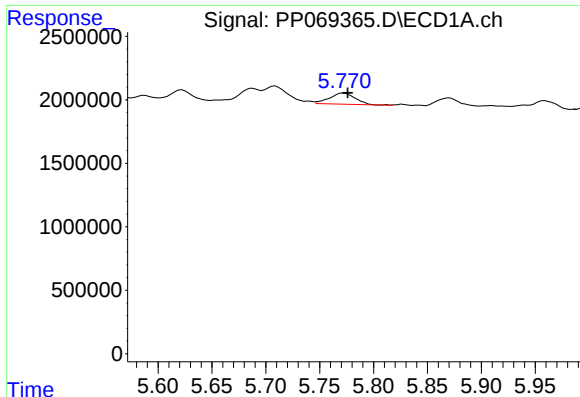

#5 AR-1016-3


R.T.: 5.772 min
Delta R.T.: -0.004 min
Response: 1484166
Conc: 34.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

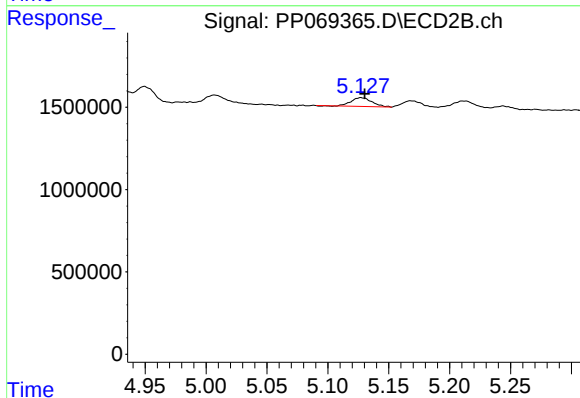


#5 AR-1016-3

R.T.: 5.127 min
Delta R.T.: -0.003 min
Response: 630289
Conc: 25.33 ng/ml

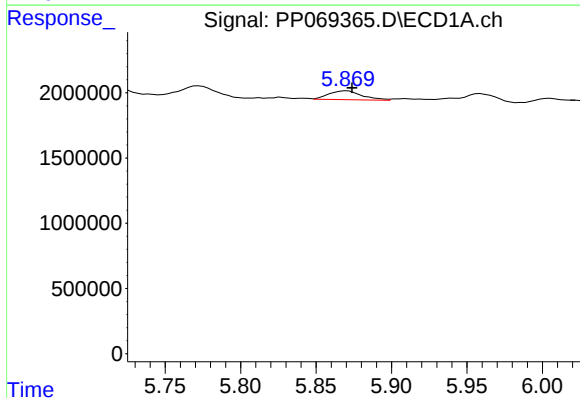


#6 AR-1016-4

R.T.: 5.871 min
Delta R.T.: -0.003 min
Response: 1047227
Conc: 29.92 ng/ml

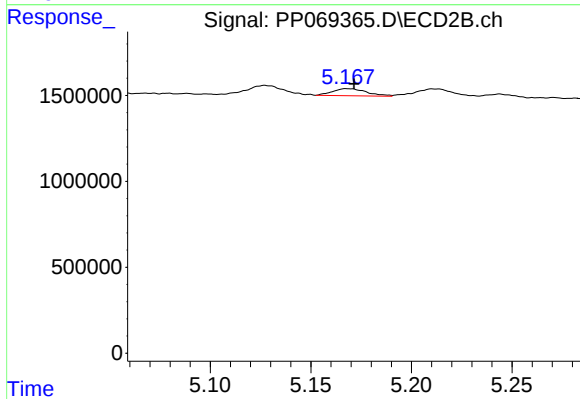

#6 AR-1016-4


R.T.: 5.168 min
Delta R.T.: -0.003 min
Response: 477711
Conc: 23.65 ng/ml

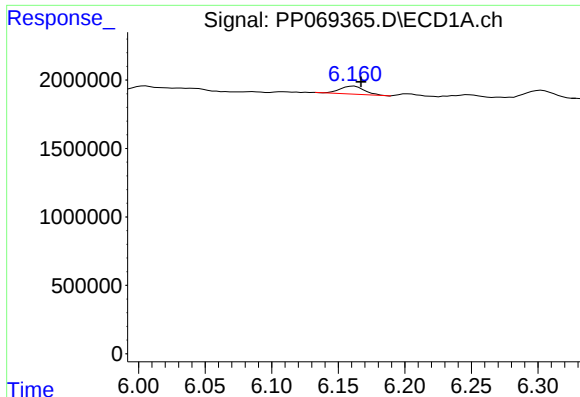

#7 AR-1016-5


R.T.: 6.162 min
Delta R.T.: -0.005 min
Response: 742377
Conc: 22.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

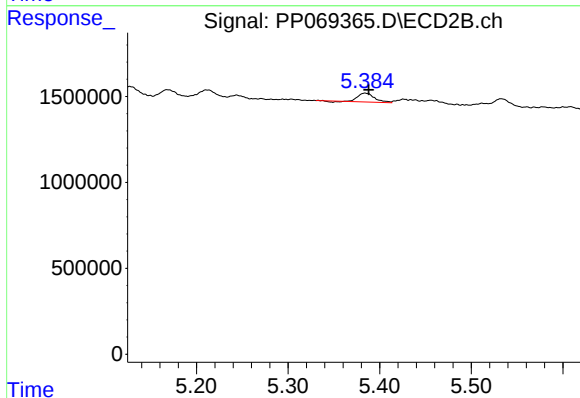


#7 AR-1016-5

R.T.: 5.384 min
Delta R.T.: -0.004 min
Response: 616334
Conc: 22.98 ng/ml

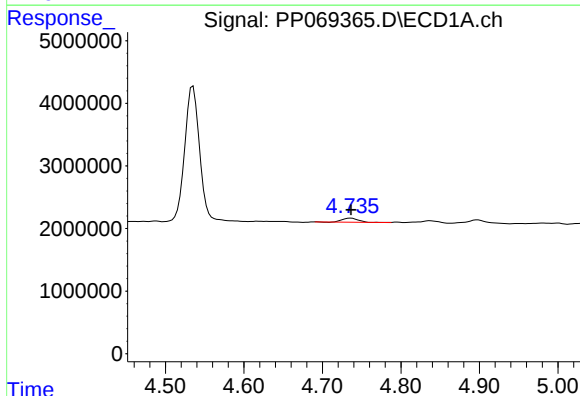


#8 AR-1221-1

R.T.: 4.736 min
Delta R.T.: 0.000 min
Response: 952228
Conc: 50.07 ng/ml

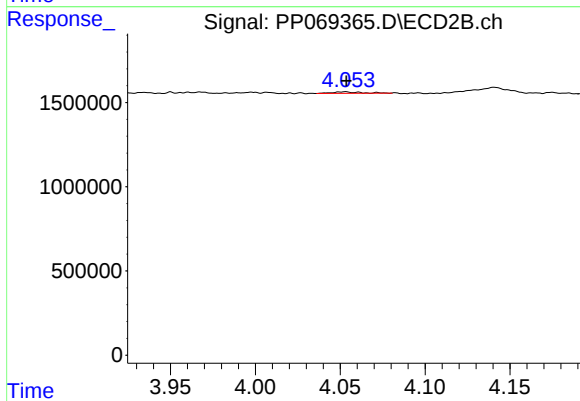

#8 AR-1221-1


R.T.: 4.053 min
Delta R.T.: 0.000 min
Response: 93267
Conc: 7.57 ng/ml

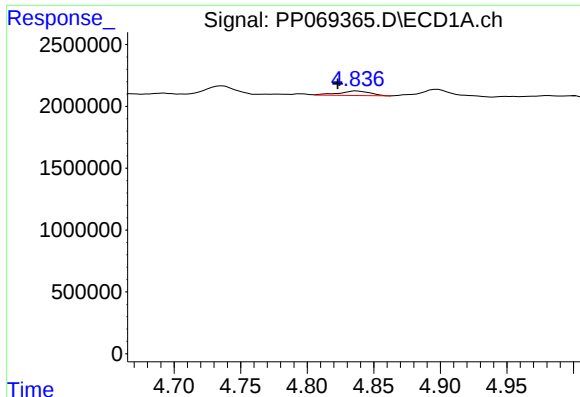

#9 AR-1221-2


R.T.: 4.838 min
Delta R.T.: 0.014 min
Response: 593827
Conc: 43.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

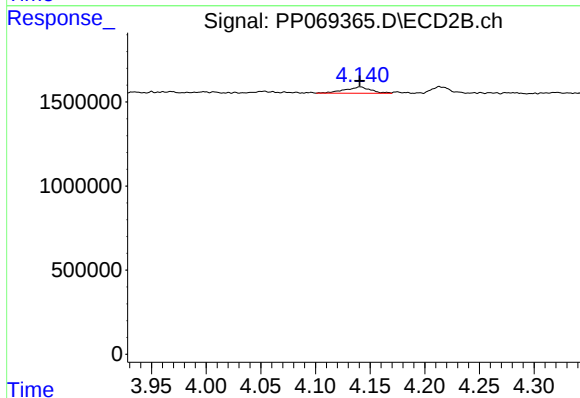


#9 AR-1221-2

R.T.: 4.141 min
Delta R.T.: 0.000 min
Response: 620689
Conc: 64.10 ng/ml

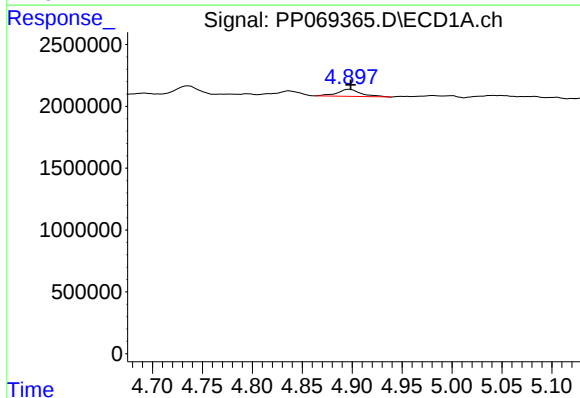


#10 AR-1221-3

R.T.: 4.898 min
Delta R.T.: 0.000 min
Response: 934092
Conc: 22.27 ng/ml

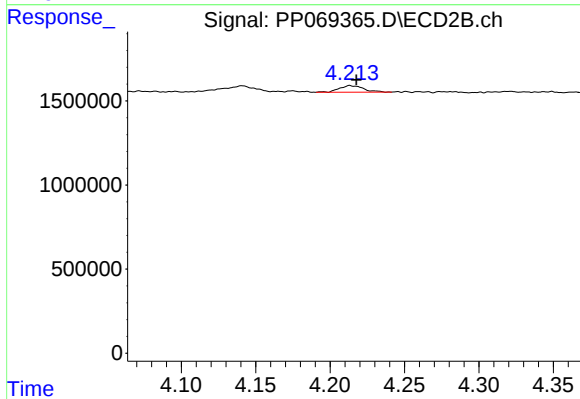

#10 AR-1221-3


R.T.: 4.213 min
Delta R.T.: -0.004 min
Response: 444160
Conc: 15.22 ng/ml

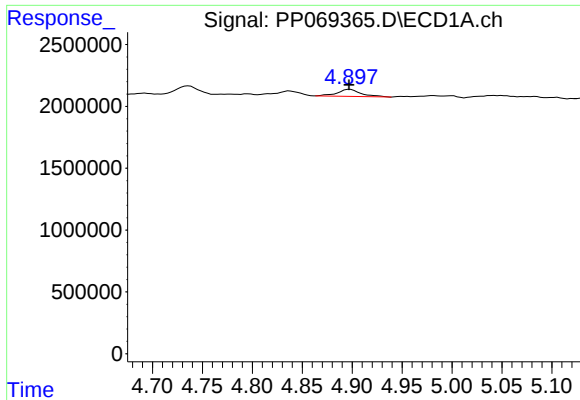

#11 AR-1232-1


R.T.: 4.898 min
Delta R.T.: 0.001 min
Response: 934092
Conc: 28.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

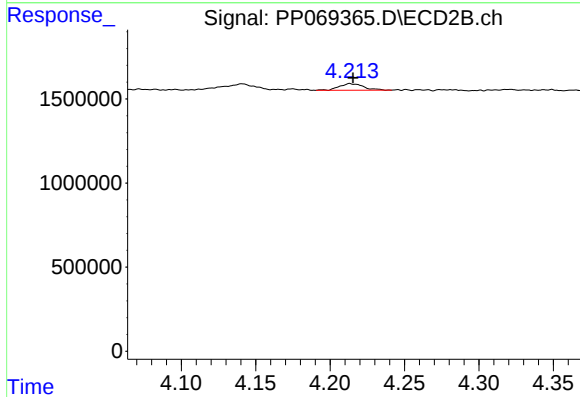


#11 AR-1232-1

R.T.: 4.213 min
Delta R.T.: -0.002 min
Response: 444160
Conc: 18.92 ng/ml

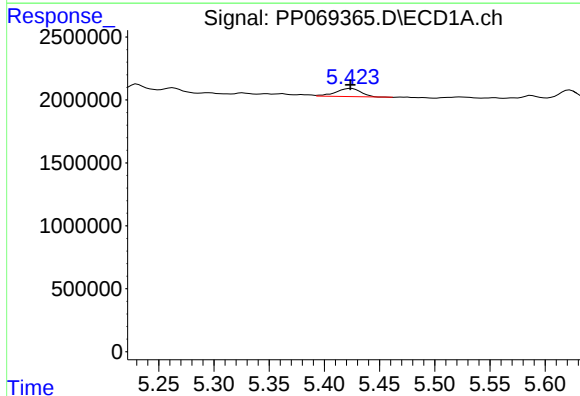


#12 AR-1232-2

R.T.: 5.424 min
Delta R.T.: 0.000 min
Response: 993078
Conc: 60.77 ng/ml

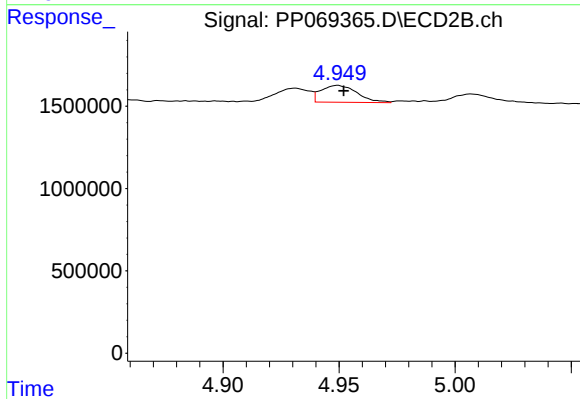

#12 AR-1232-2


R.T.: 4.949 min
Delta R.T.: -0.003 min
Response: 1120760
Conc: 47.55 ng/ml

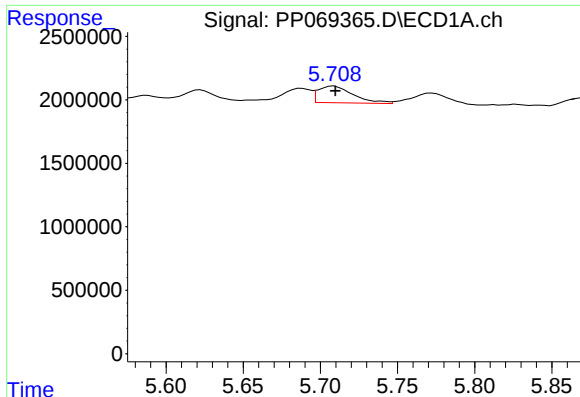

#13 AR-1232-3


R.T.: 5.709 min
Delta R.T.: 0.000 min
Response: 2096722
Conc: 61.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

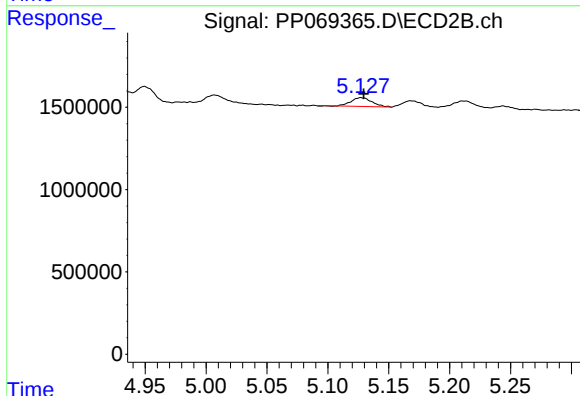


#13 AR-1232-3

R.T.: 5.127 min
Delta R.T.: -0.002 min
Response: 630289
Conc: 48.68 ng/ml

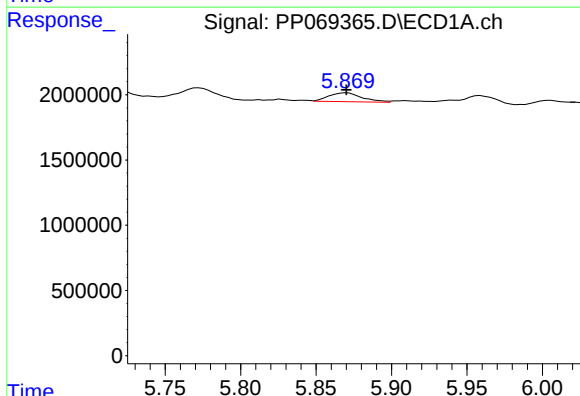


#14 AR-1232-4

R.T.: 5.871 min
Delta R.T.: 0.000 min
Response: 1047227
Conc: 58.78 ng/ml

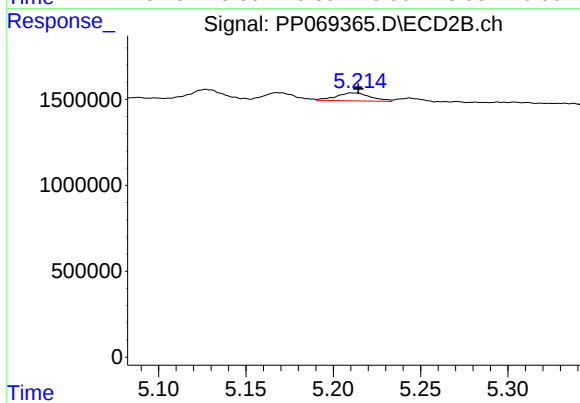

#14 AR-1232-4


R.T.: 5.212 min
Delta R.T.: -0.003 min
Response: 629310
Conc: 56.76 ng/ml

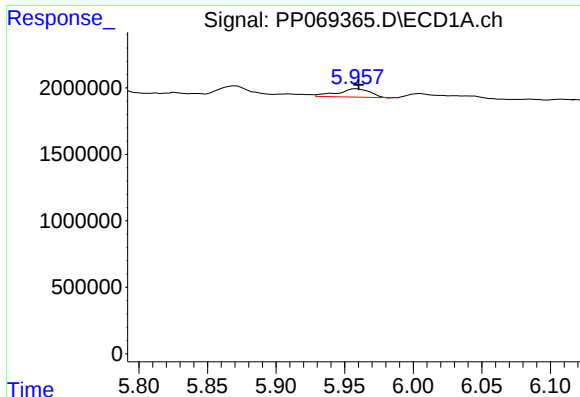

#15 AR-1232-5


R.T.: 5.959 min
Delta R.T.: -0.001 min
Response: 1052387
Conc: 91.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

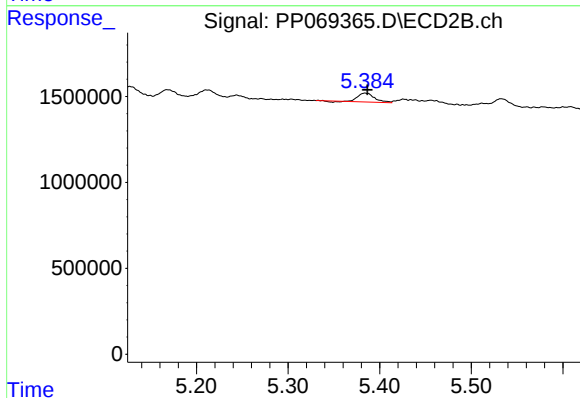


#15 AR-1232-5

R.T.: 5.384 min
Delta R.T.: -0.002 min
Response: 616334
Conc: 50.48 ng/ml

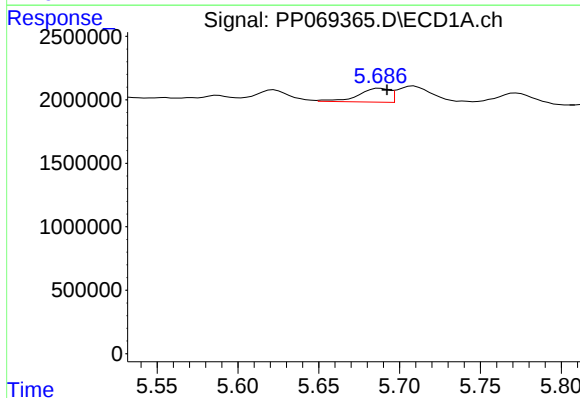


#16 AR-1242-1

R.T.: 5.688 min
Delta R.T.: -0.004 min
Response: 1477726
Conc: 35.43 ng/ml

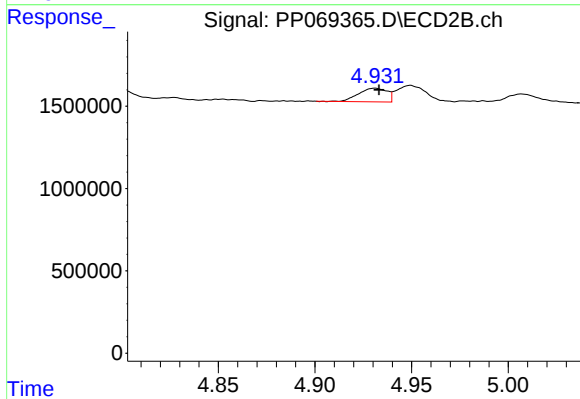

#16 AR-1242-1


R.T.: 4.931 min
Delta R.T.: -0.002 min
Response: 842259
Conc: 29.21 ng/ml

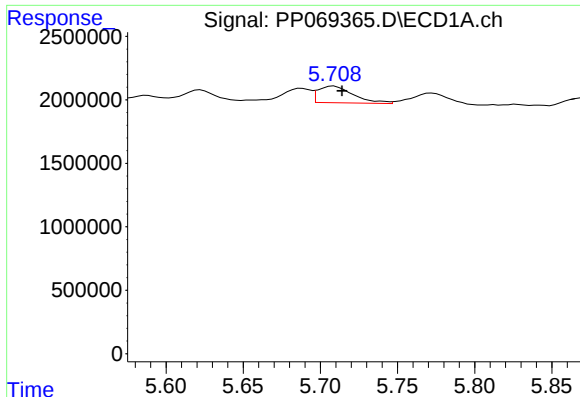

#17 AR-1242-2


R.T.: 5.709 min
Delta R.T.: -0.005 min
Response: 2096722
Conc: 35.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

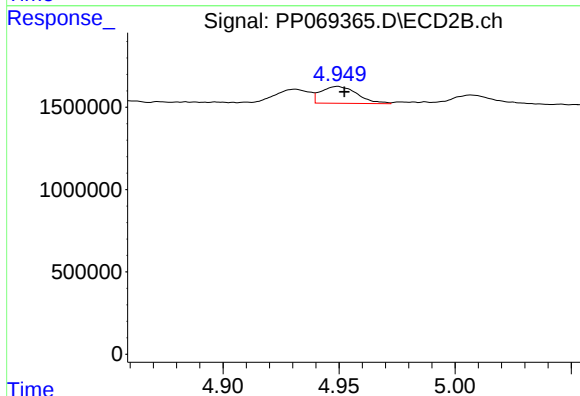


#17 AR-1242-2

R.T.: 4.949 min
Delta R.T.: -0.003 min
Response: 1120760
Conc: 28.45 ng/ml

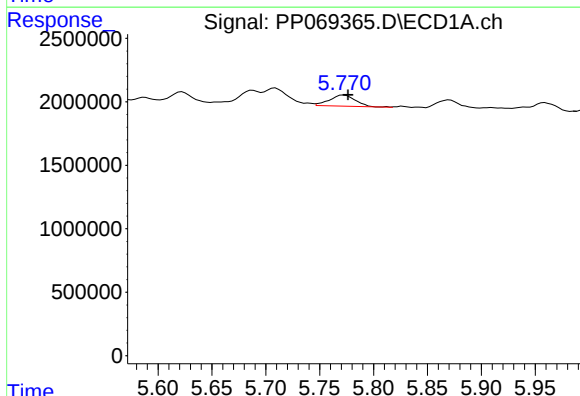


#18 AR-1242-3

R.T.: 5.772 min
Delta R.T.: -0.004 min
Response: 1484166
Conc: 40.01 ng/ml

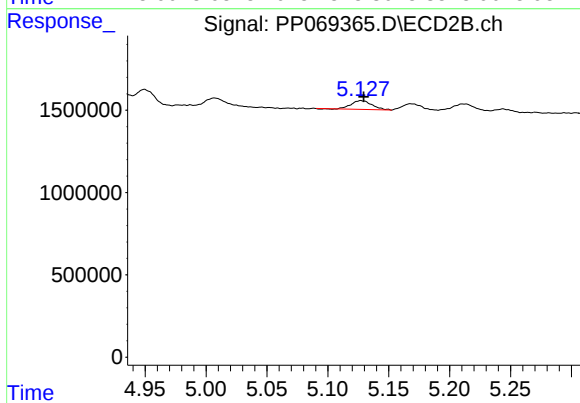

#18 AR-1242-3


R.T.: 5.127 min
Delta R.T.: -0.002 min
Response: 630289
Conc: 28.01 ng/ml

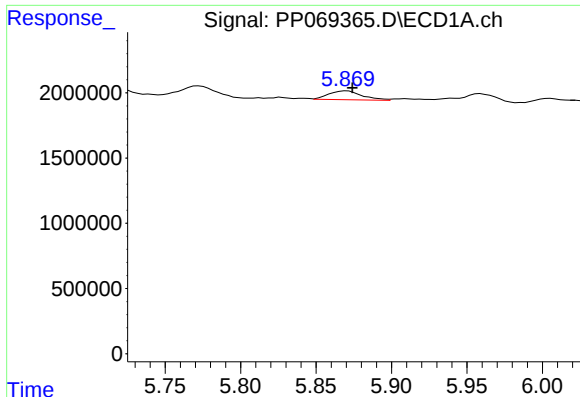

#19 AR-1242-4


R.T.: 5.871 min
Delta R.T.: -0.004 min
Response: 1047227
Conc: 31.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

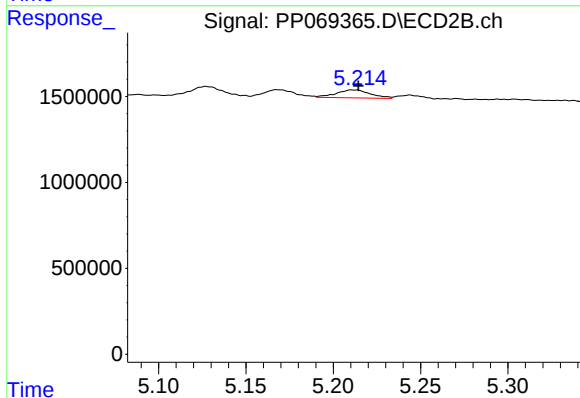


#19 AR-1242-4

R.T.: 5.212 min
Delta R.T.: -0.003 min
Response: 629310
Conc: 29.16 ng/ml

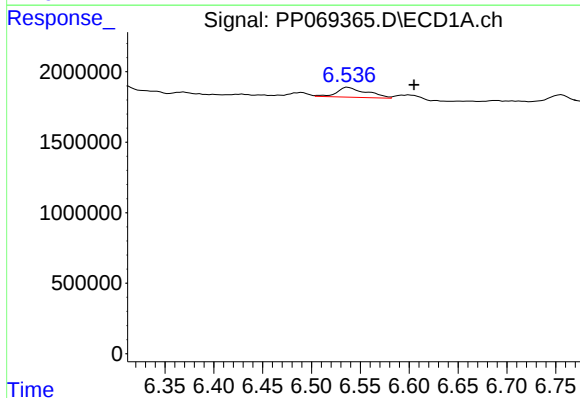


#20 AR-1242-5

R.T.: 6.537 min
Delta R.T.: -0.068 min
Response: 1506581
Conc: 46.24 ng/ml

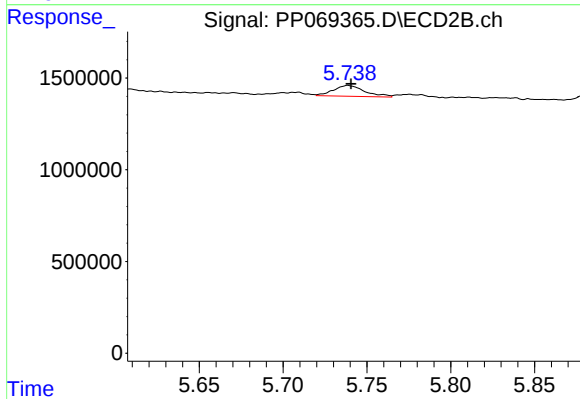

#20 AR-1242-5


R.T.: 5.739 min
Delta R.T.: -0.002 min
Response: 770023
Conc: 26.77 ng/ml

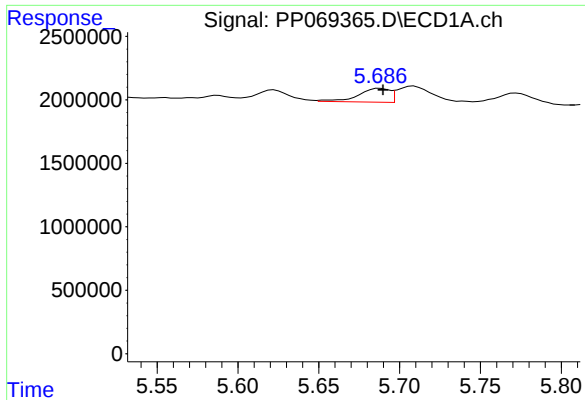

#21 AR-1248-1


R.T.: 5.688 min
Delta R.T.: -0.002 min
Response: 1477726
Conc: 45.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

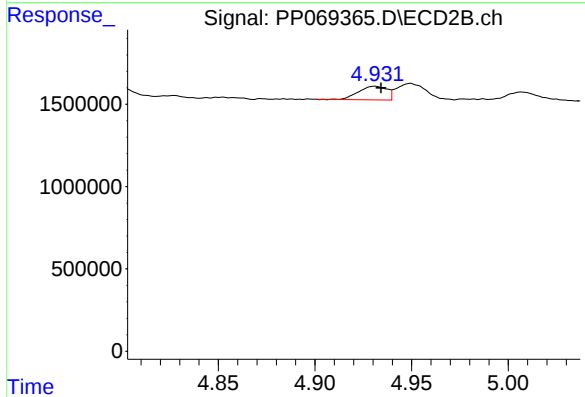


#21 AR-1248-1

R.T.: 4.931 min
Delta R.T.: -0.003 min
Response: 842259
Conc: 38.27 ng/ml

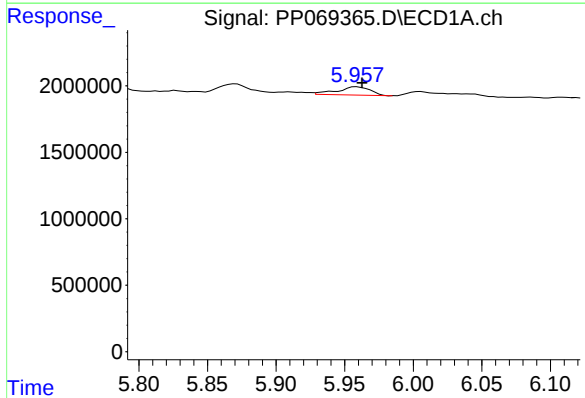


#22 AR-1248-2

R.T.: 5.959 min
Delta R.T.: -0.004 min
Response: 1052387
Conc: 24.79 ng/ml

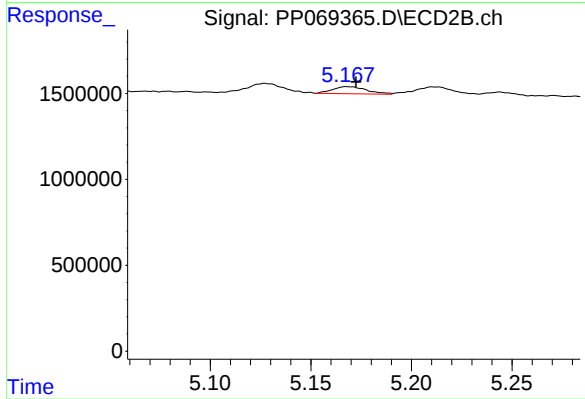

#22 AR-1248-2


R.T.: 5.168 min
Delta R.T.: -0.004 min
Response: 477711
Conc: 15.89 ng/ml

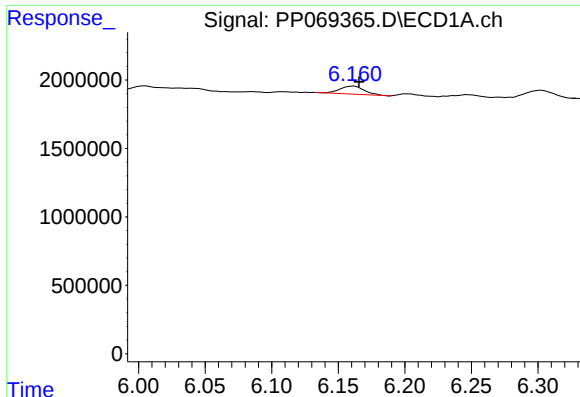

#23 AR-1248-3


R.T.: 6.162 min
Delta R.T.: -0.004 min
Response: 742377
Conc: 15.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

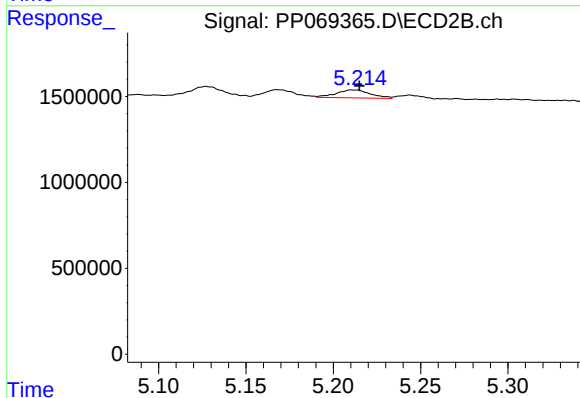


#23 AR-1248-3

R.T.: 5.212 min
Delta R.T.: -0.004 min
Response: 629310
Conc: 20.31 ng/ml

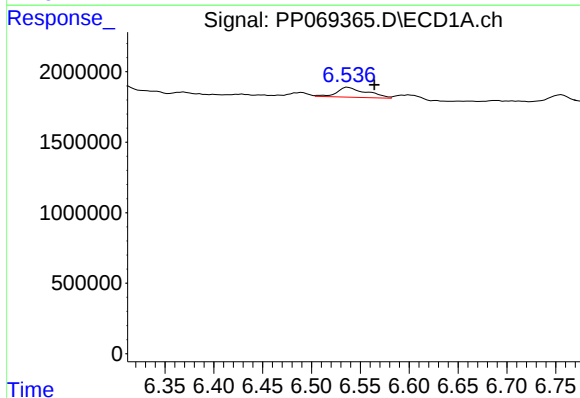


#24 AR-1248-4

R.T.: 6.537 min
Delta R.T.: -0.027 min
Response: 1506581
Conc: 27.33 ng/ml

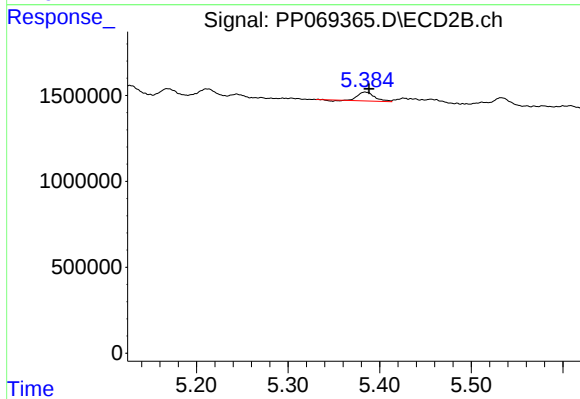

#24 AR-1248-4


R.T.: 5.384 min
Delta R.T.: -0.004 min
Response: 616334
Conc: 16.68 ng/ml

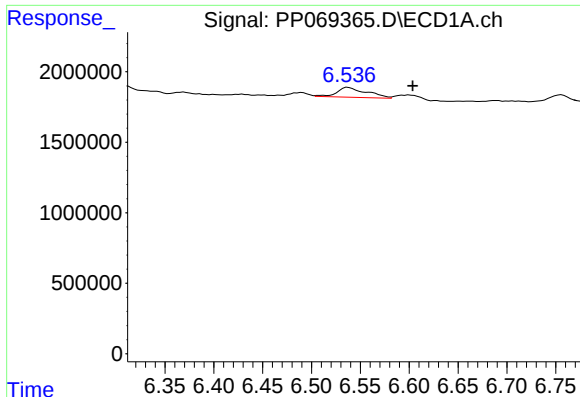

#25 AR-1248-5


R.T.: 6.537 min
Delta R.T.: -0.066 min
Response: 1506581
Conc: 28.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

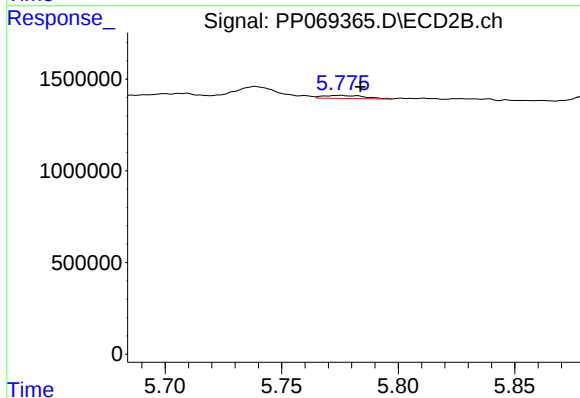


#25 AR-1248-5

R.T.: 5.775 min
Delta R.T.: -0.008 min
Response: 211329
Conc: 5.65 ng/ml

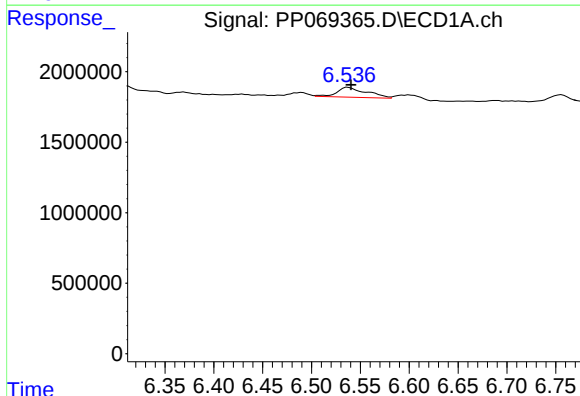


#26 AR-1254-1

R.T.: 6.537 min
Delta R.T.: -0.003 min
Response: 1506581
Conc: 26.04 ng/ml

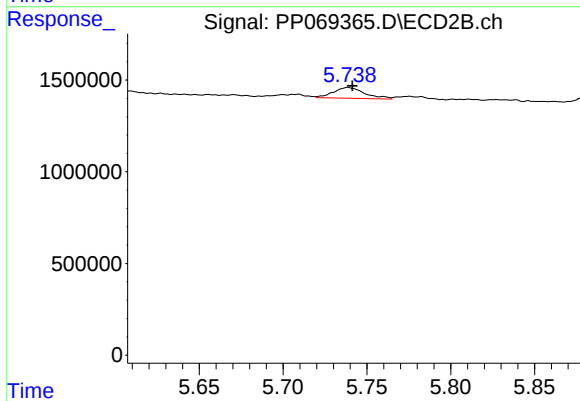

#26 AR-1254-1


R.T.: 5.739 min
Delta R.T.: -0.002 min
Response: 770023
Conc: 13.99 ng/ml

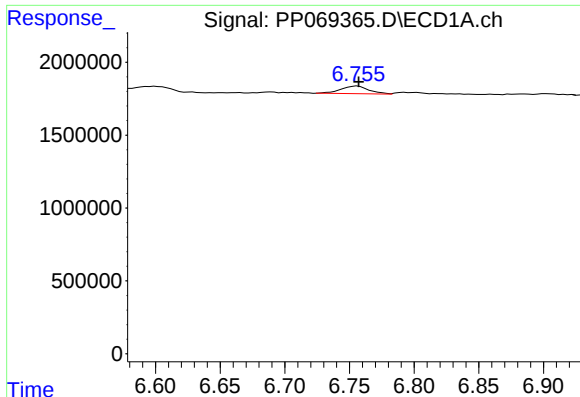

#27 AR-1254-2


R.T.: 6.756 min
Delta R.T.: -0.001 min
Response: 795391
Conc: 9.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

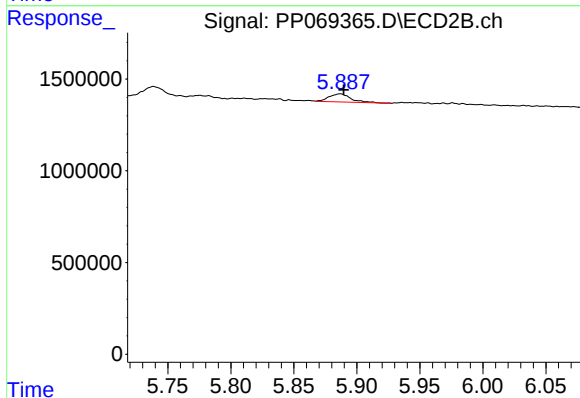


#27 AR-1254-2

R.T.: 5.887 min
Delta R.T.: -0.003 min
Response: 543194
Conc: 11.23 ng/ml

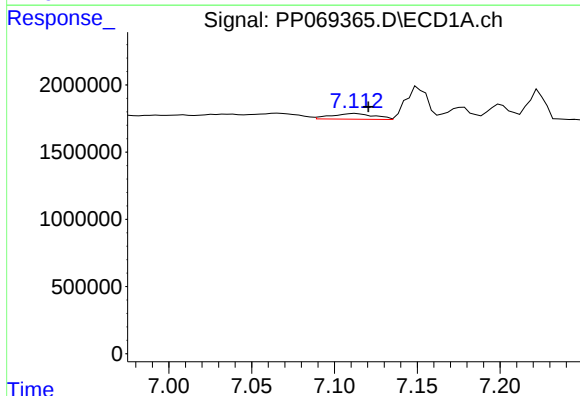


#28 AR-1254-3

R.T.: 7.113 min
Delta R.T.: -0.008 min
Response: 764841
Conc: 9.07 ng/ml

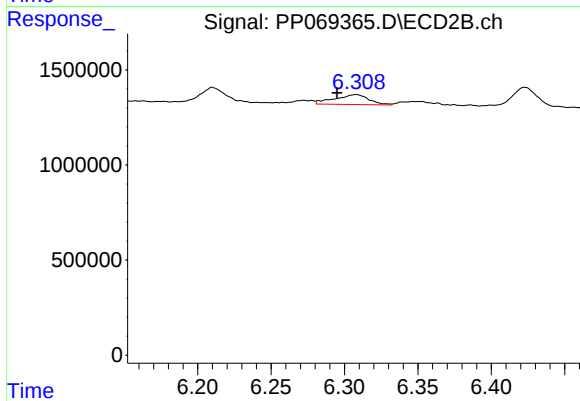

#28 AR-1254-3


R.T.: 6.308 min
Delta R.T.: 0.013 min
Response: 853533
Conc: 11.25 ng/ml

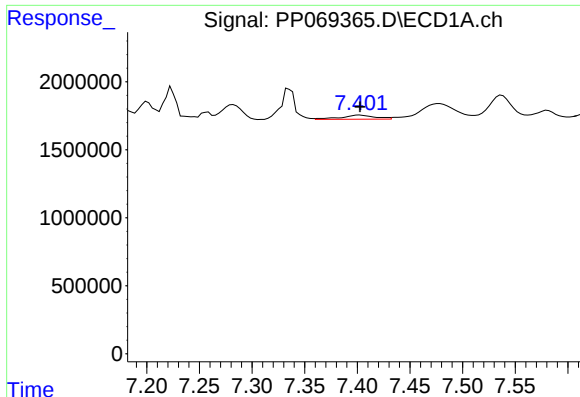

#29 AR-1254-4


R.T.: 7.402 min
Delta R.T.: 0.000 min
Response: 671654
Conc: 9.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

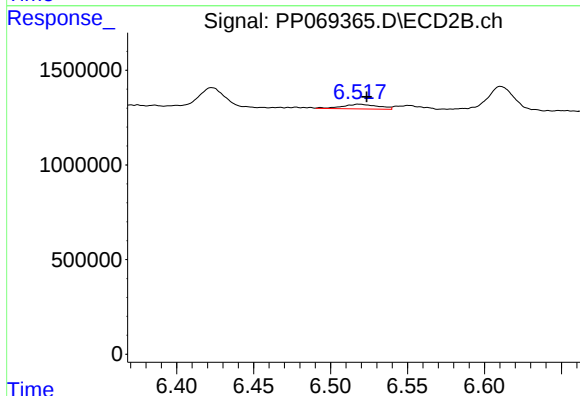


#29 AR-1254-4

R.T.: 6.519 min
Delta R.T.: -0.005 min
Response: 393413
Conc: 7.68 ng/ml

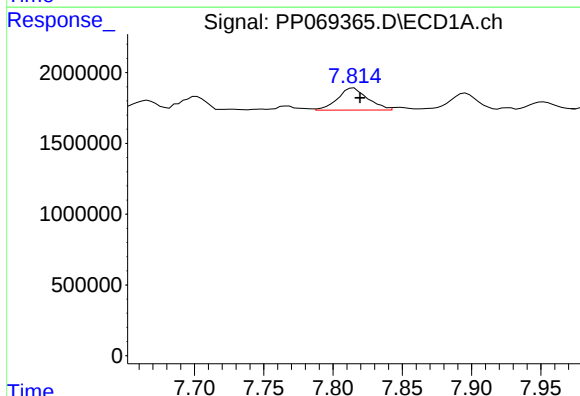


#30 AR-1254-5

R.T.: 7.815 min
Delta R.T.: -0.005 min
Response: 2366079
Conc: 34.77 ng/ml

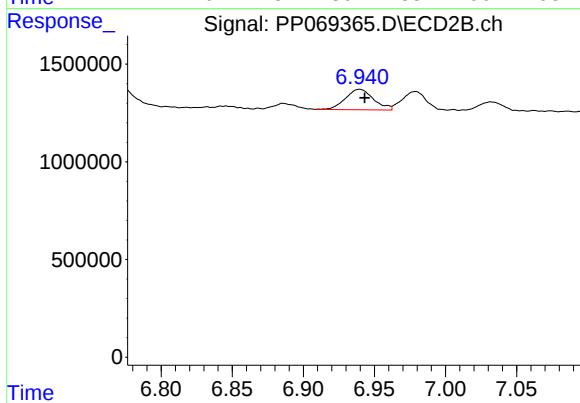

#30 AR-1254-5


R.T.: 6.940 min
Delta R.T.: -0.004 min
Response: 1448145
Conc: 21.76 ng/ml

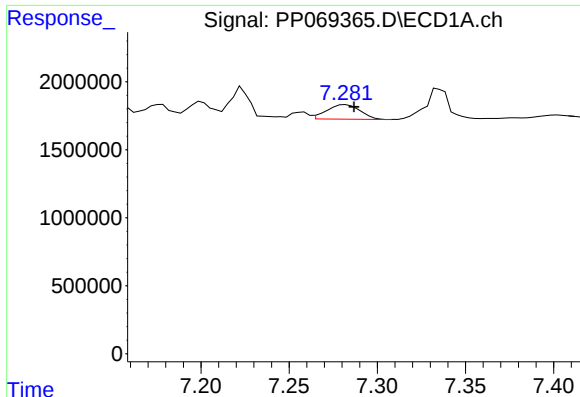

#31 AR-1260-1


R.T.: 7.282 min
Delta R.T.: -0.005 min
Response: 1393754
Conc: 23.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

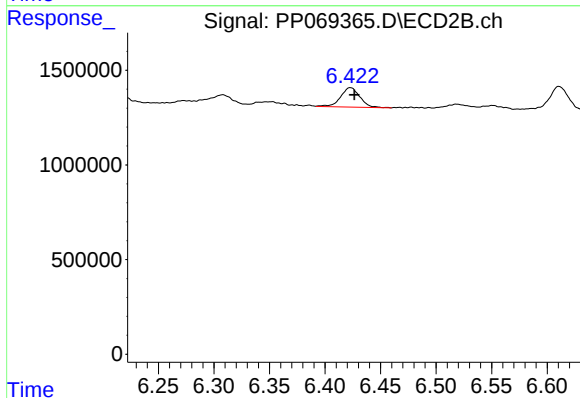


#31 AR-1260-1

R.T.: 6.423 min
Delta R.T.: -0.004 min
Response: 1245436
Conc: 25.82 ng/ml

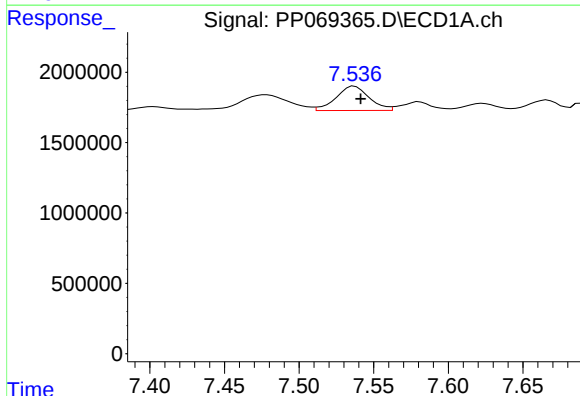


#32 AR-1260-2

R.T.: 7.537 min
Delta R.T.: -0.004 min
Response: 2681653
Conc: 34.46 ng/ml

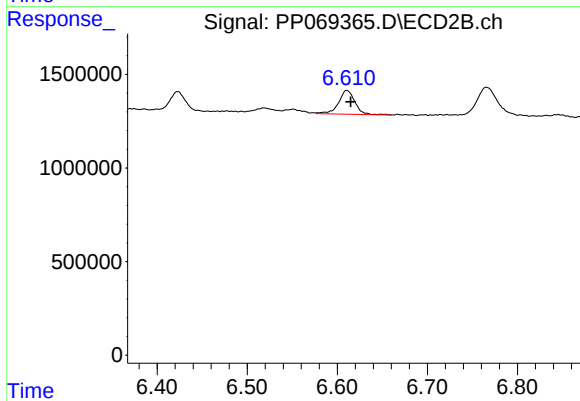

#32 AR-1260-2


R.T.: 6.611 min
Delta R.T.: -0.004 min
Response: 1597941
Conc: 26.07 ng/ml

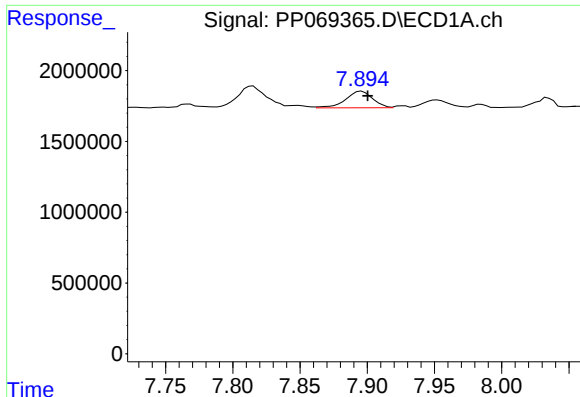

#33 AR-1260-3


R.T.: 7.896 min
Delta R.T.: -0.004 min
Response: 1652718
Conc: 26.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

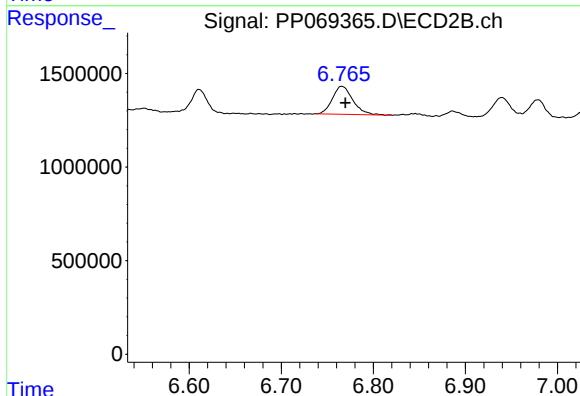


#33 AR-1260-3

R.T.: 6.766 min
Delta R.T.: -0.004 min
Response: 2293790
Conc: 38.13 ng/ml

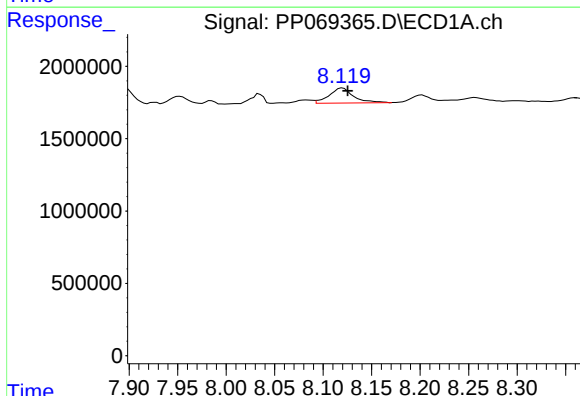


#34 AR-1260-4

R.T.: 8.120 min
Delta R.T.: -0.005 min
Response: 1829668
Conc: 27.73 ng/ml

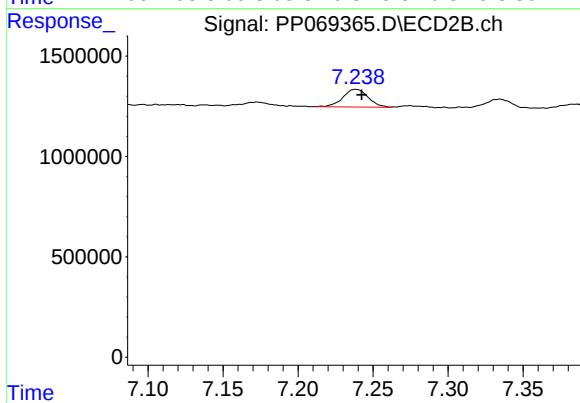

#34 AR-1260-4


R.T.: 7.239 min
Delta R.T.: -0.004 min
Response: 1037223
Conc: 22.32 ng/ml

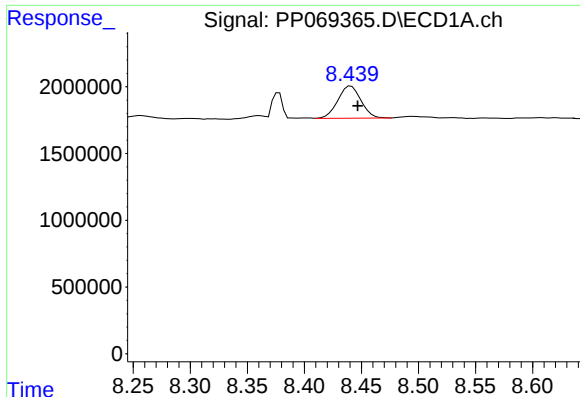

#35 AR-1260-5


R.T.: 8.441 min
Delta R.T.: -0.006 min
Response: 3399993
Conc: 25.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

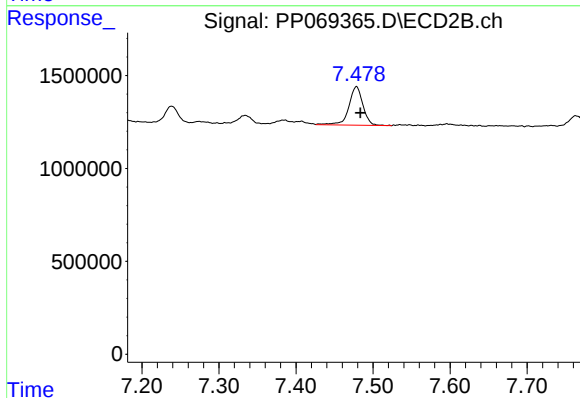


#35 AR-1260-5

R.T.: 7.478 min
Delta R.T.: -0.005 min
Response: 2620706
Conc: 23.58 ng/ml

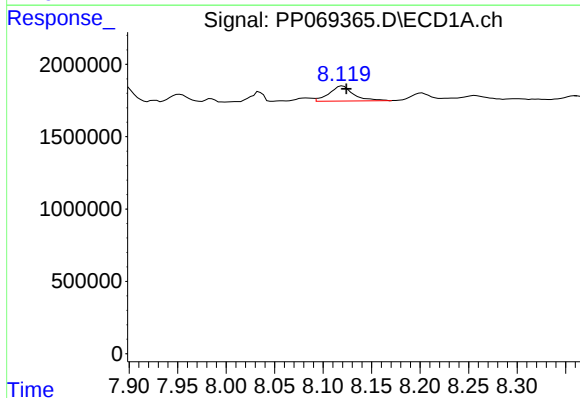


#36 AR-1262-1

R.T.: 8.120 min
Delta R.T.: -0.004 min
Response: 1829668
Conc: 23.16 ng/ml

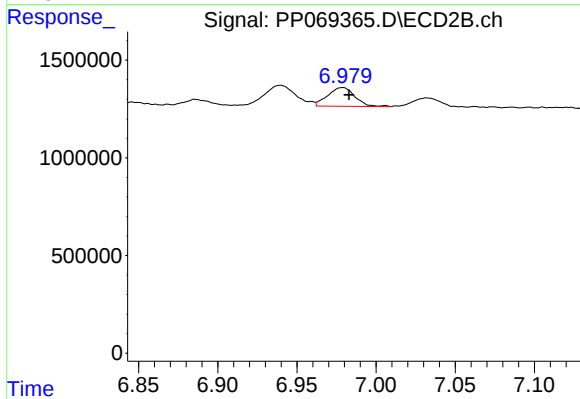

#36 AR-1262-1


R.T.: 6.979 min
Delta R.T.: -0.004 min
Response: 1150555
Conc: 16.20 ng/ml

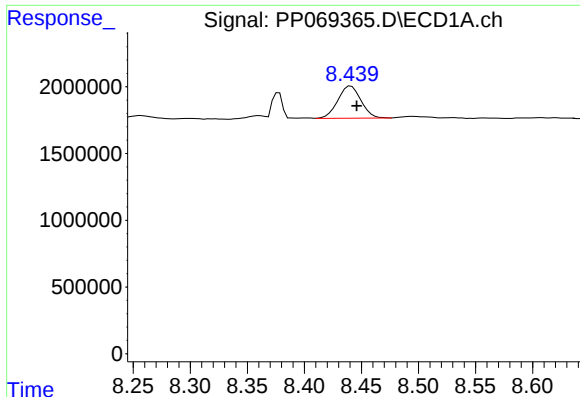

#37 AR-1262-2


R.T.: 8.441 min
Delta R.T.: -0.005 min
Response: 3399993
Conc: 22.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

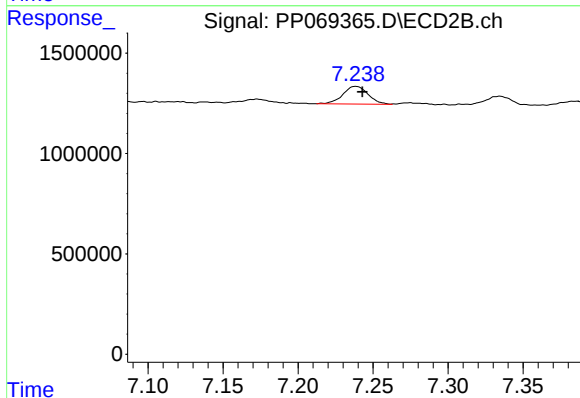


#37 AR-1262-2

R.T.: 7.239 min
Delta R.T.: -0.004 min
Response: 1037223
Conc: 17.01 ng/ml

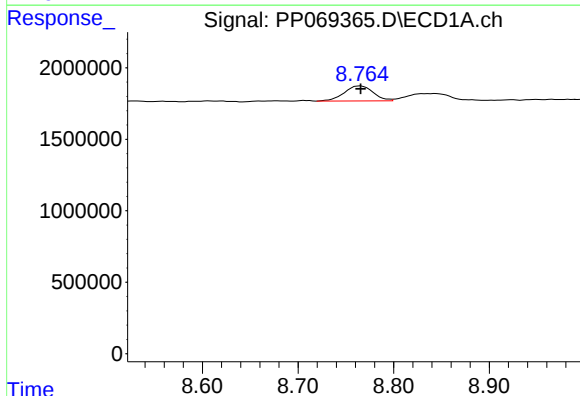


#38 AR-1262-3

R.T.: 8.765 min
Delta R.T.: 0.000 min
Response: 2202277
Conc: 20.72 ng/ml

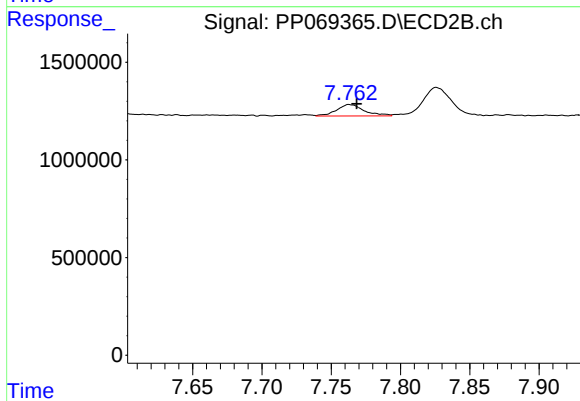

#38 AR-1262-3


R.T.: 7.763 min
Delta R.T.: -0.005 min
Response: 810608
Conc: 15.50 ng/ml

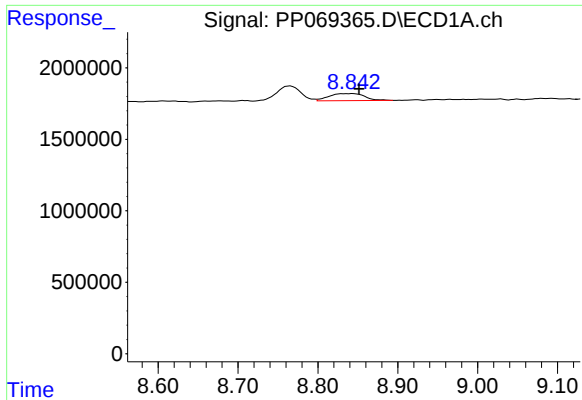

#39 AR-1262-4


R.T.: 8.843 min
Delta R.T.: -0.008 min
Response: 1522410
Conc: 18.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

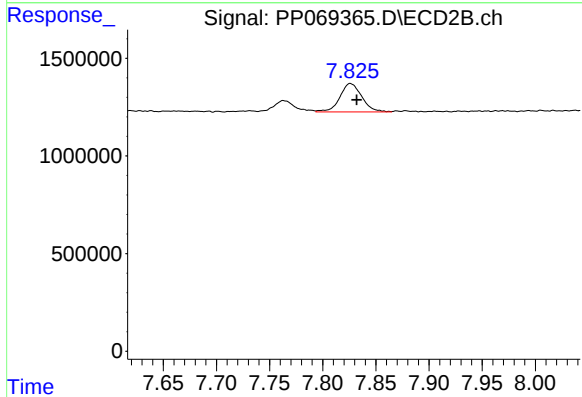


#39 AR-1262-4

R.T.: 7.826 min
Delta R.T.: -0.006 min
Response: 2088744
Conc: 22.60 ng/ml

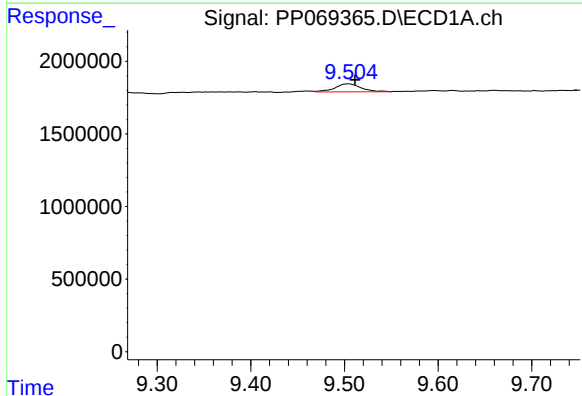


#40 AR-1262-5

R.T.: 9.505 min
Delta R.T.: -0.006 min
Response: 1080936
Conc: 19.09 ng/ml

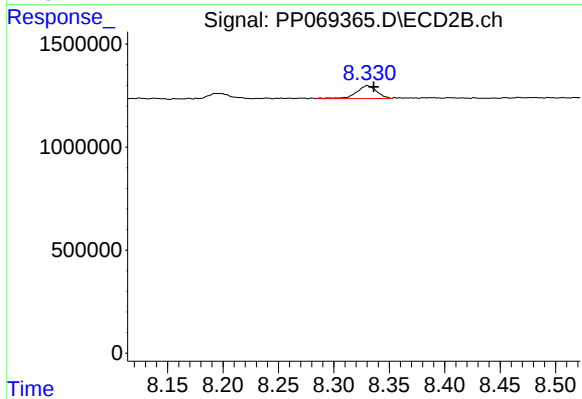

#40 AR-1262-5


R.T.: 8.330 min
Delta R.T.: -0.006 min
Response: 802197
Conc: 16.79 ng/ml

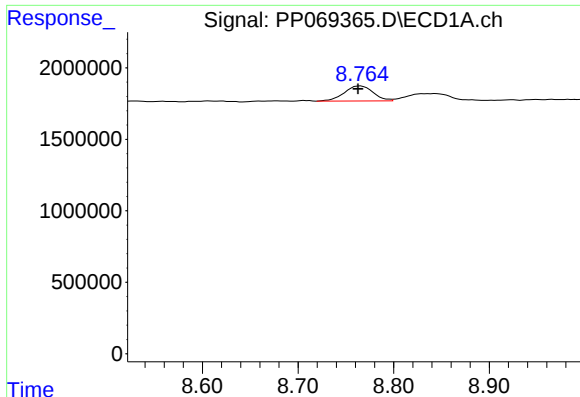

#41 AR-1268-1


R.T.: 8.765 min
Delta R.T.: 0.002 min
Response: 2202277
Conc: 12.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

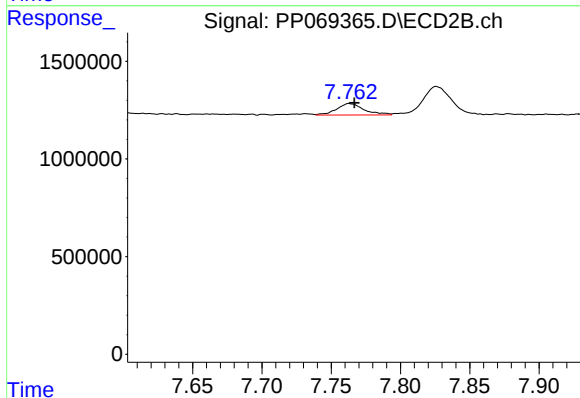


#41 AR-1268-1

R.T.: 7.763 min
Delta R.T.: -0.004 min
Response: 810608
Conc: 5.59 ng/ml

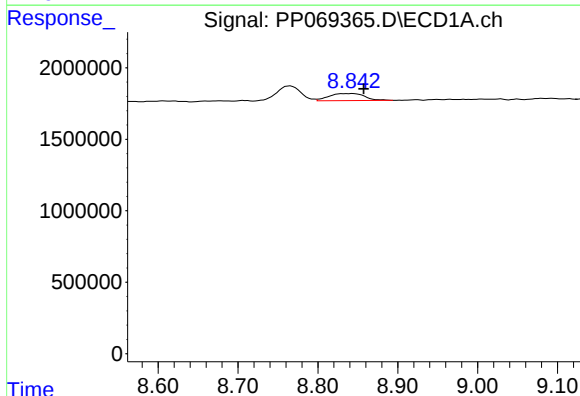


#42 AR-1268-2

R.T.: 8.843 min
Delta R.T.: -0.014 min
Response: 1522410
Conc: 9.67 ng/ml

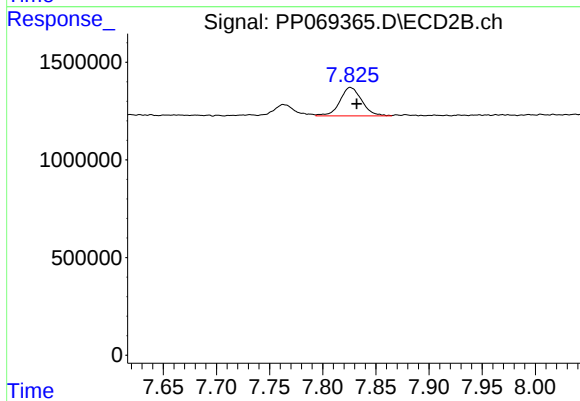

#42 AR-1268-2


R.T.: 7.826 min
Delta R.T.: -0.006 min
Response: 2088744
Conc: 15.73 ng/ml

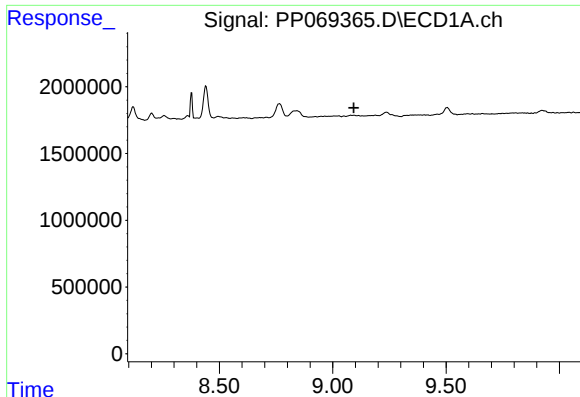

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.093 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

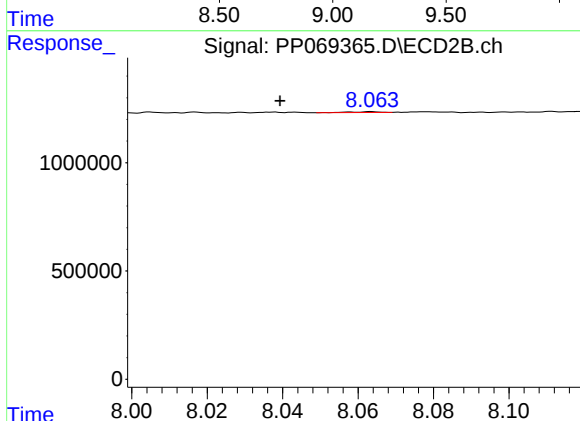


#43 AR-1268-3

R.T.: 8.063 min
Delta R.T.: 0.024 min
Response: 20557
Conc: 0.18 ng/ml

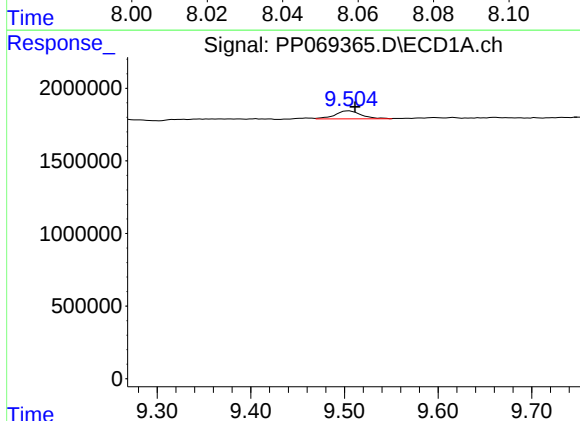


#44 AR-1268-4

R.T.: 9.505 min
Delta R.T.: -0.006 min
Response: 1080936
Conc: 18.41 ng/ml

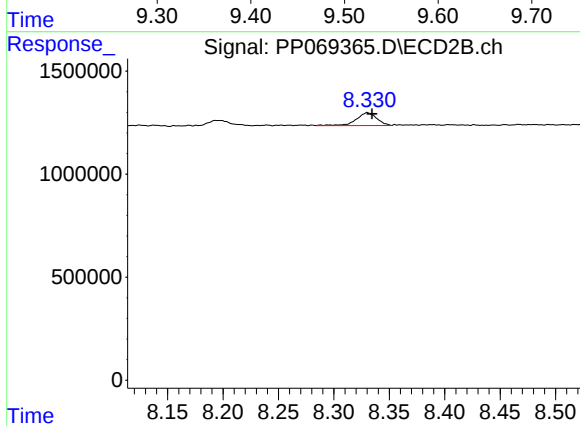

#44 AR-1268-4


R.T.: 8.330 min
Delta R.T.: -0.004 min
Response: 802197
Conc: 15.40 ng/ml

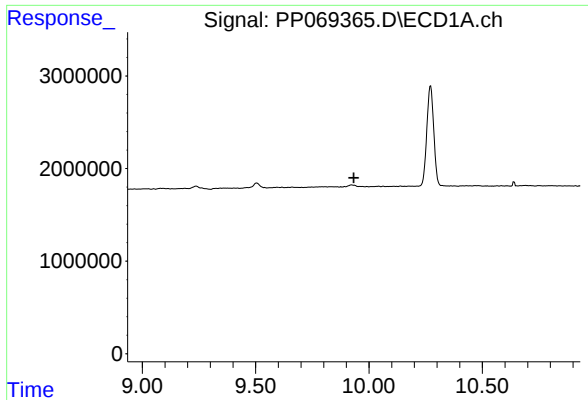

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.933 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

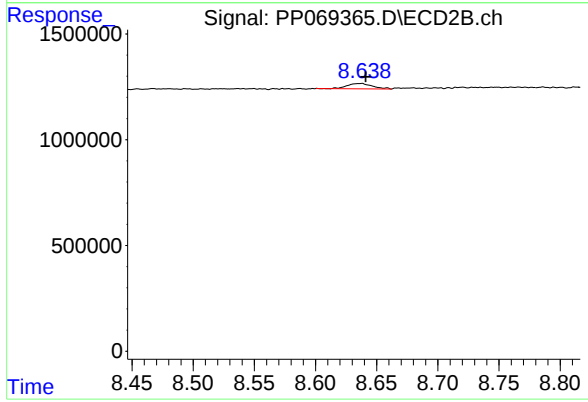

#45 AR-1268-5

R.T.: 8.637 min
Delta R.T.: -0.004 min
Response: 361486
Conc: 1.01 ng/ml