

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
 Data File : PP069370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2025 04:18
 Operator : YP\AJ
 Sample : Q1168-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT1-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 05:34:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.535	3.841	29664378	18879441	20.723	21.153
2)	SA Decachlor...	10.271	8.906	23922943	23834750	21.889	21.310
Target Compounds							
3)	L1 AR-1016-1	5.624f	4.987f	2043515	99326	44.105	3.045 #
4)	L1 AR-1016-2	0.000	4.987	0	99326	N.D.	2.209 #
5)	L1 AR-1016-3	0.000	5.170f	0	593237	N.D.	23.840 #
6)	L1 AR-1016-4	0.000	5.170	0	593237	N.D.	29.374 #
7)	L1 AR-1016-5	6.163	5.387	445548	528091	13.478	19.687 #
8)	L2 AR-1221-1	4.737	4.054	705200	48664	37.078	3.951 #
9)	L2 AR-1221-2	4.838	4.143	417421	746939	30.485	77.136 #
10)	L2 AR-1221-3	4.838f	4.216	417421	47722	9.952	1.636 #
11)	L3 AR-1232-1	4.838f	4.216	417421	47722	12.538	2.032 #
12)	L3 AR-1232-2	0.000	4.987f	0	99326	N.D.	4.214 #
13)	L3 AR-1232-3	0.000	5.170f	0	593237	N.D.	45.820 #
14)	L3 AR-1232-4	0.000	5.214	0	152912	N.D.	13.793 #
15)	L3 AR-1232-5	5.960	5.387	677478	528091	59.104	43.250 #
16)	L4 AR-1242-1	5.624f	4.987f	2043515	99326	48.999	3.445 #
17)	L4 AR-1242-2	0.000	4.987	0	99326	N.D.	2.521 #
18)	L4 AR-1242-3	0.000	5.170f	0	593237	N.D.	26.361 #
19)	L4 AR-1242-4	0.000	5.214	0	152912	N.D.	7.085 #
20)	L4 AR-1242-5	6.562f	5.740	735853	1649476	22.583	57.336 #
21)	L5 AR-1248-1	5.624f	4.987f	2043515	99326	62.996	4.513 #
22)	L5 AR-1248-2	5.960	5.170	677478	593237	15.961	19.732
23)	L5 AR-1248-3	6.163	5.214	445548	152912	9.482	4.935 #
24)	L5 AR-1248-4	6.562	5.387	735853	528091	13.350	14.294
25)	L5 AR-1248-5	6.562f	5.814	735853	148195	13.784	3.964 #
26)	L6 AR-1254-1	6.539	5.740	1610372	1649476	27.830	29.960
27)	L6 AR-1254-2	6.755	5.887	2500902	1406754	31.167	29.084
28)	L6 AR-1254-3	7.118	6.293	2574523	1990888	30.544	26.232
29)	L6 AR-1254-4	7.401	6.521	1919032	1474177	28.143	28.765
30)	L6 AR-1254-5	7.817	6.940	1822529	1704260	26.784	25.605
31)	L7 AR-1260-1	7.284	6.424	906814	925169	15.518	19.183
32)	L7 AR-1260-2	7.537	6.612	1560692	893605	20.057	14.577 #
33)	L7 AR-1260-3	0.000	6.766	0	1845680	N.D.	30.681 #
34)	L7 AR-1260-4	8.104	7.233	688995	101287	10.443	2.180 #
35)	L7 AR-1260-5	0.000	7.481	0	269701	N.D.	2.427 #
36)	L8 AR-1262-1	8.104	7.010	688995	309816	8.719	4.363 #
37)	L8 AR-1262-2	0.000	7.233	0	101287	N.D.	1.661 #
38)	L8 AR-1262-3	0.000	7.772	0	350949	N.D.	6.710 #
39)	L8 AR-1262-4	0.000	7.828	0	401500	N.D.	4.344 #
40)	L8 AR-1262-5	0.000	8.406f	0	199503	N.D.	4.174 #
41)	L9 AR-1268-1	0.000	7.772	0	350949	N.D.	2.418 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
Data File : PP069370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2025 04:18
Operator : YP\AJ
Sample : Q1168-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 64 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 05:34:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	0.000	7.828	0	401500	N.D.	3.023 #
45)	L9 AR-1268-5	0.000	8.639	0	130065	N.D.	0.365 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
Data File : PP069370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2025 04:18
Operator : YP\AJ
Sample : Q1168-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 64 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 05:34:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

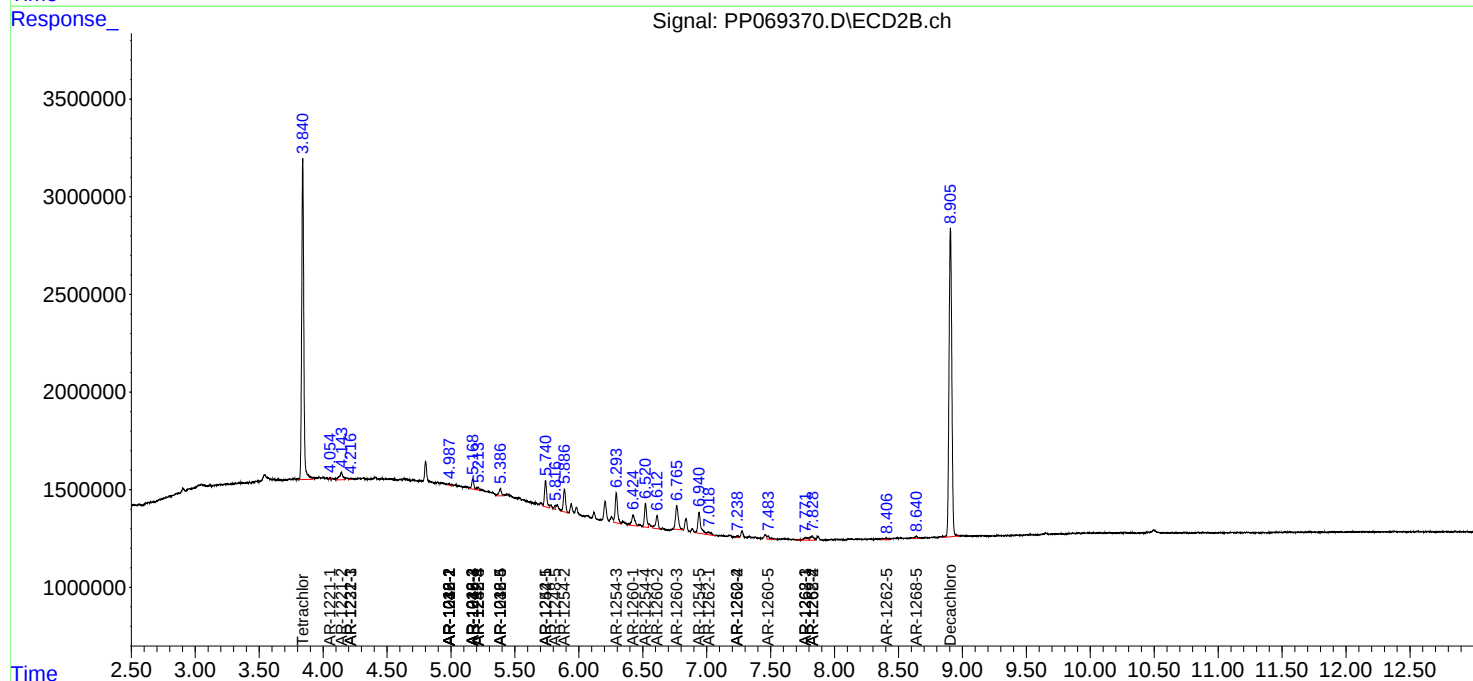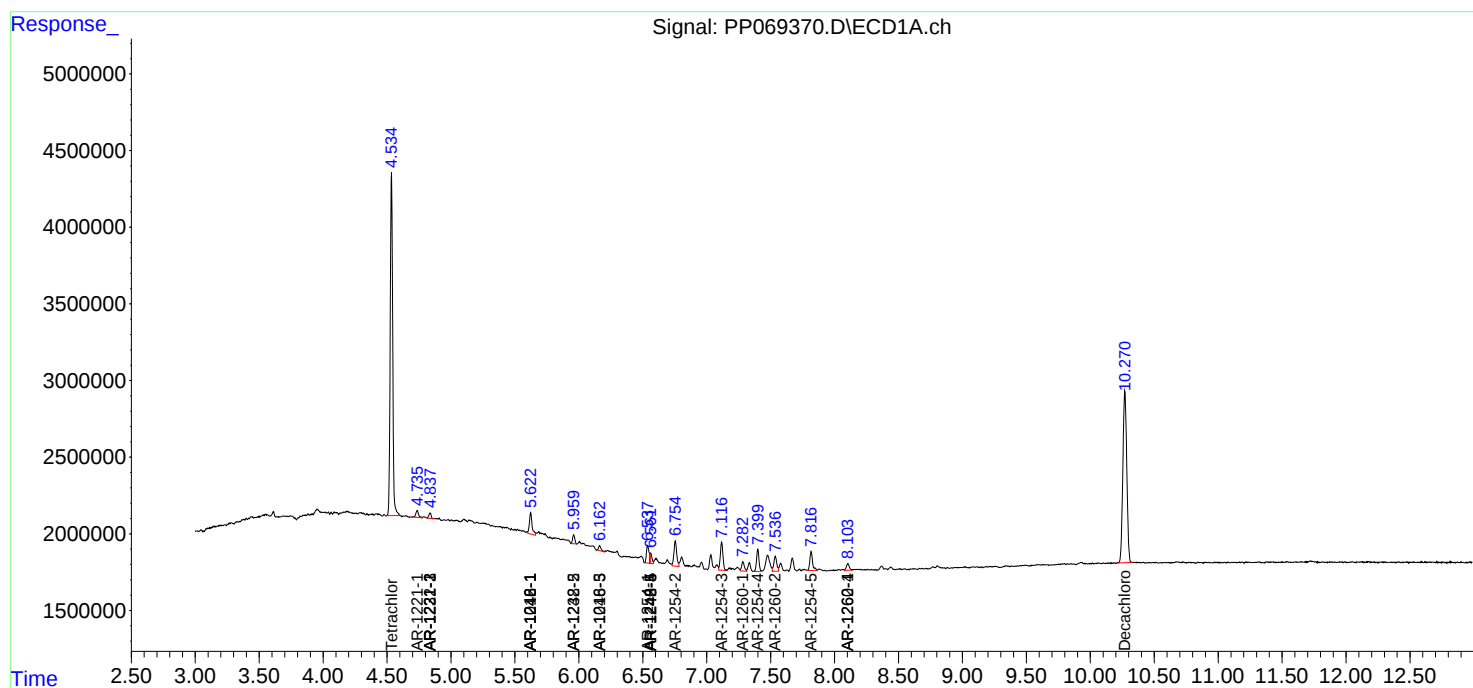


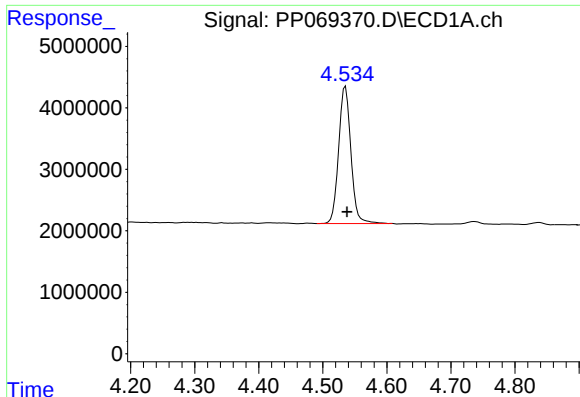

#1 Tetrachloro-m-xylene


R.T.: 4.535 min
Delta R.T.: -0.003 min
Response: 29664378
Conc: 20.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

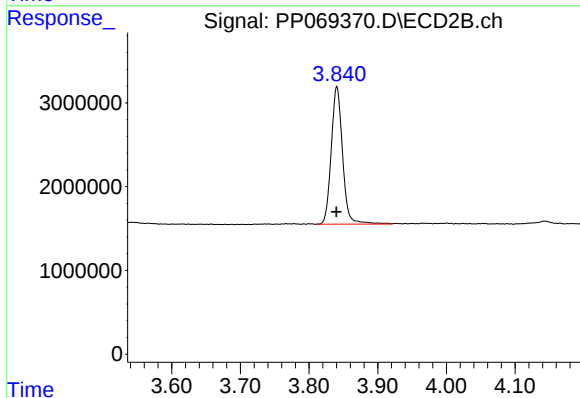


#1 Tetrachloro-m-xylene

R.T.: 3.841 min
Delta R.T.: 0.000 min
Response: 18879441
Conc: 21.15 ng/ml

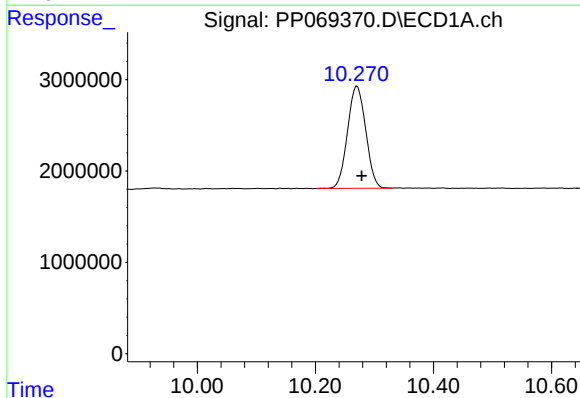


#2 Decachlorobiphenyl

R.T.: 10.271 min
Delta R.T.: -0.008 min
Response: 23922943
Conc: 21.89 ng/ml

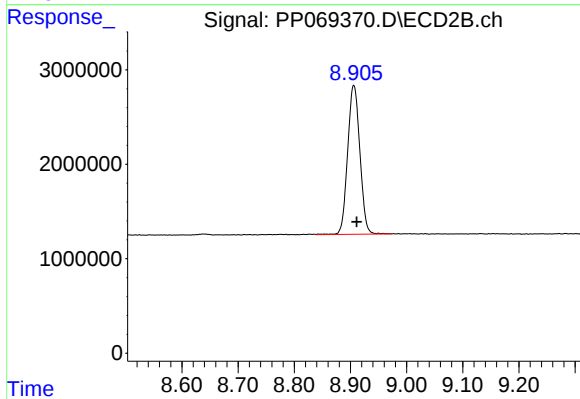

#2 Decachlorobiphenyl


R.T.: 8.906 min
Delta R.T.: -0.005 min
Response: 23834750
Conc: 21.31 ng/ml

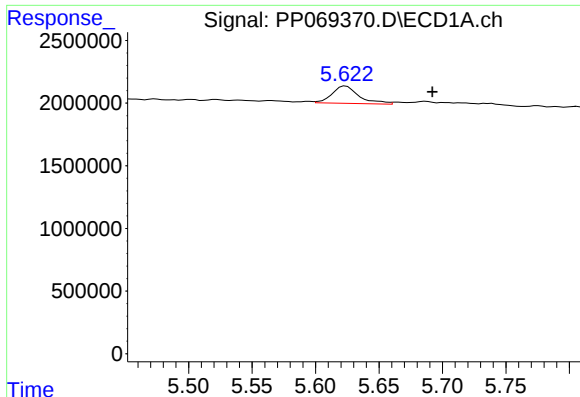

#3 AR-1016-1


R.T.: 5.624 min
Delta R.T.: -0.068 min
Response: 2043515
Conc: 44.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

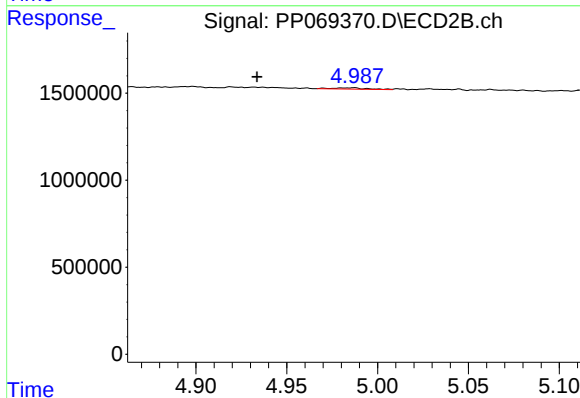


#3 AR-1016-1

R.T.: 4.987 min
Delta R.T.: 0.053 min
Response: 99326
Conc: 3.05 ng/ml

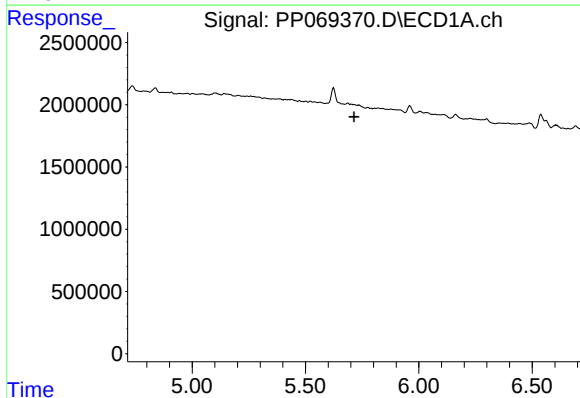


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T. : 5.714 min
Response: 0
Conc: N.D.

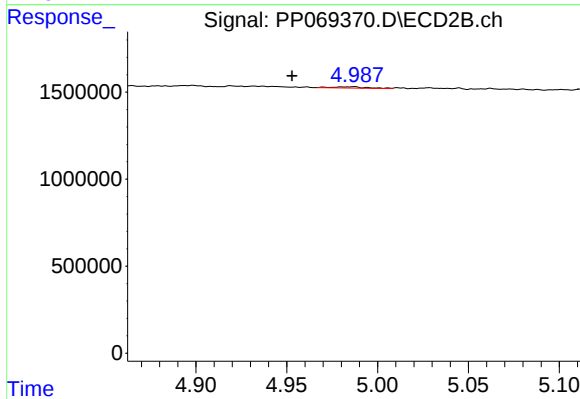

#4 AR-1016-2


R.T.: 4.987 min
Delta R.T.: 0.034 min
Response: 99326
Conc: 2.21 ng/ml

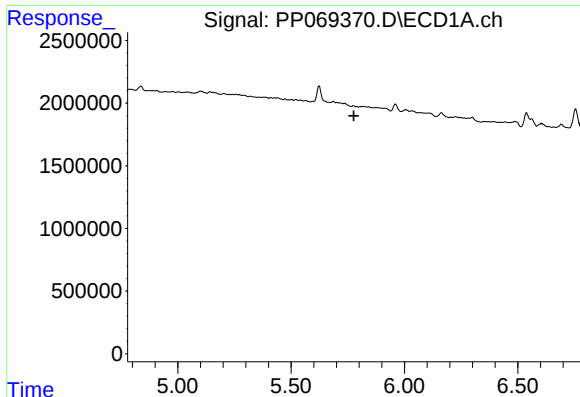

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

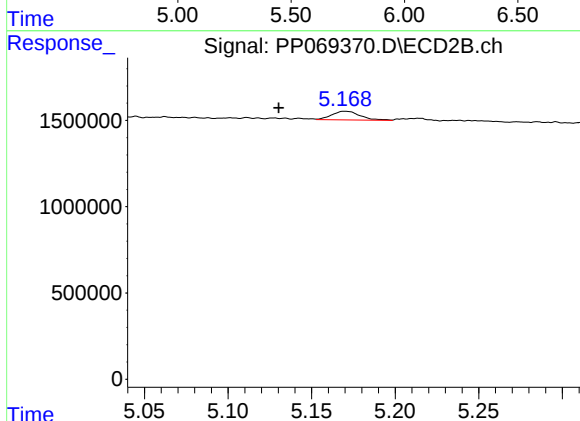


#5 AR-1016-3

R.T.: 5.170 min
Delta R.T.: 0.040 min
Response: 593237
Conc: 23.84 ng/ml

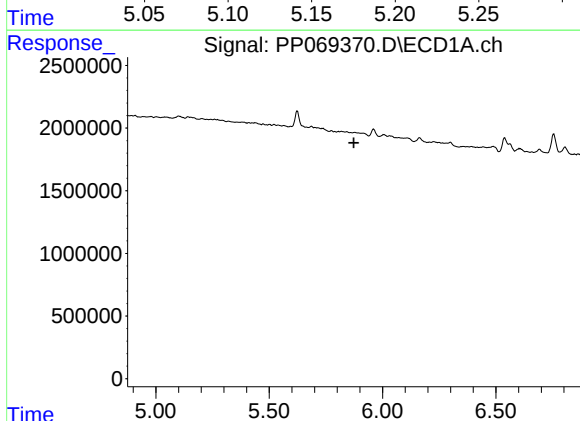


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.874 min
Response: 0
Conc: N.D.

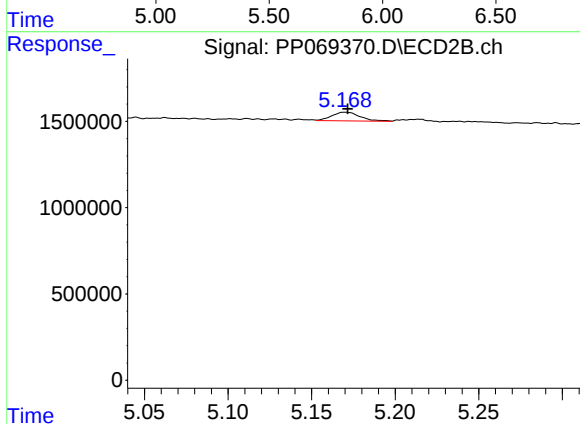

#6 AR-1016-4


R.T.: 5.170 min
Delta R.T.: -0.001 min
Response: 593237
Conc: 29.37 ng/ml

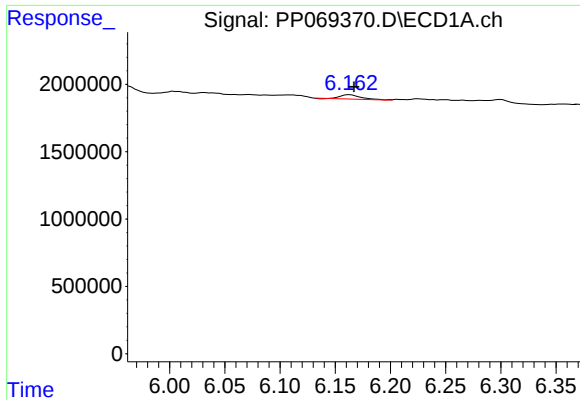

#7 AR-1016-5


R.T.: 6.163 min
Delta R.T.: -0.004 min
Response: 445548
Conc: 13.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

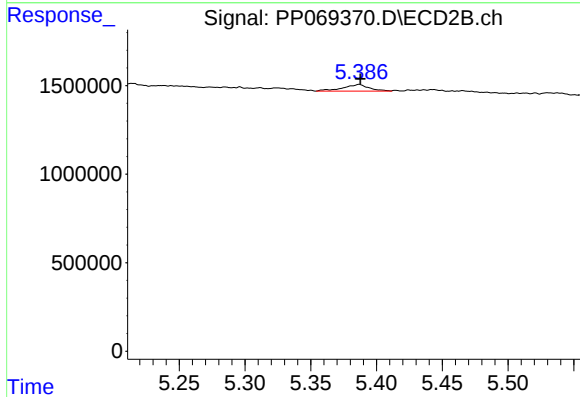


#7 AR-1016-5

R.T.: 5.387 min
Delta R.T.: 0.000 min
Response: 528091
Conc: 19.69 ng/ml

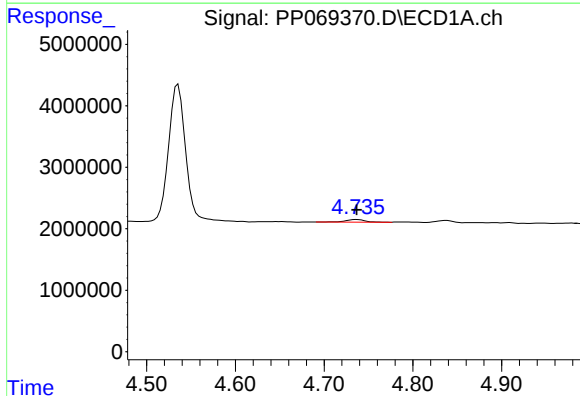


#8 AR-1221-1

R.T.: 4.737 min
Delta R.T.: 0.000 min
Response: 705200
Conc: 37.08 ng/ml

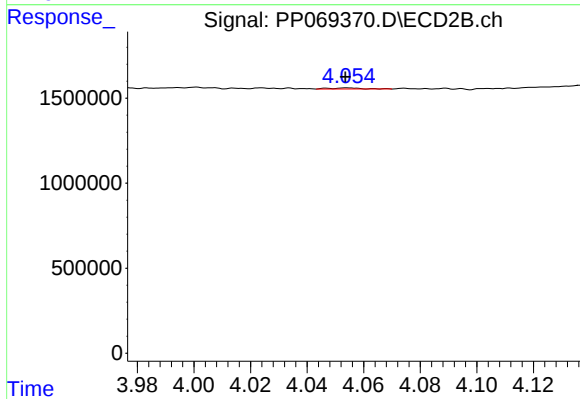

#8 AR-1221-1


R.T.: 4.054 min
Delta R.T.: 0.000 min
Response: 48664
Conc: 3.95 ng/ml

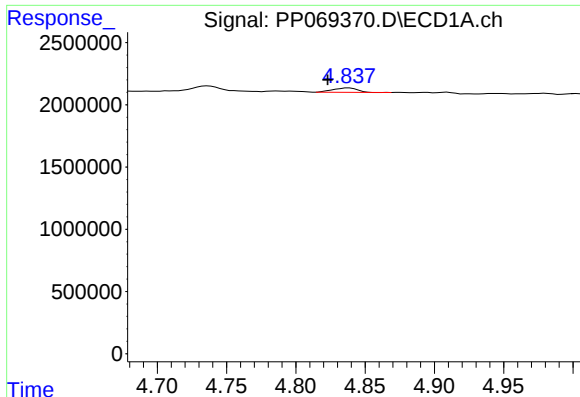

#9 AR-1221-2


R.T.: 4.838 min
Delta R.T.: 0.015 min
Response: 417421
Conc: 30.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

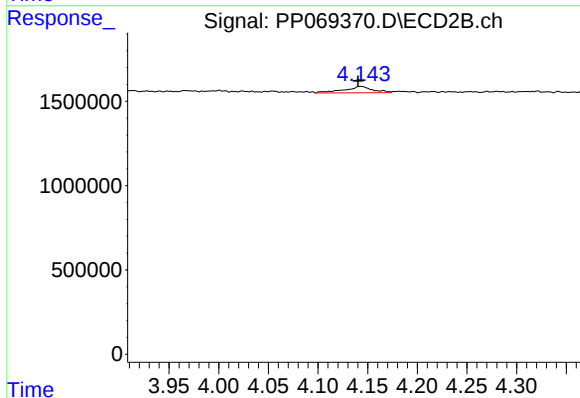


#9 AR-1221-2

R.T.: 4.143 min
Delta R.T.: 0.003 min
Response: 746939
Conc: 77.14 ng/ml

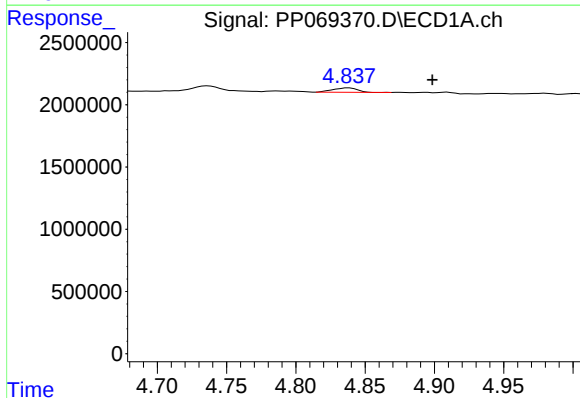


#10 AR-1221-3

R.T.: 4.838 min
Delta R.T.: -0.060 min
Response: 417421
Conc: 9.95 ng/ml

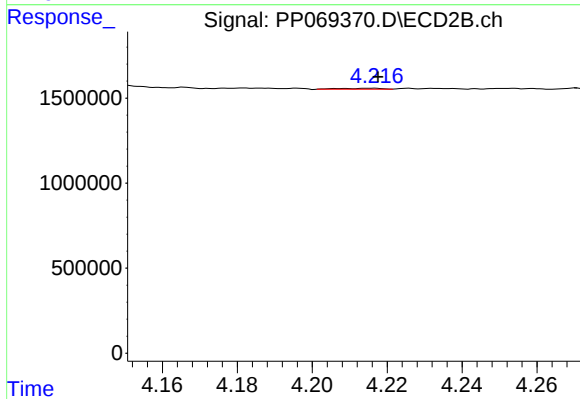

#10 AR-1221-3


R.T.: 4.216 min
Delta R.T.: -0.002 min
Response: 47722
Conc: 1.64 ng/ml

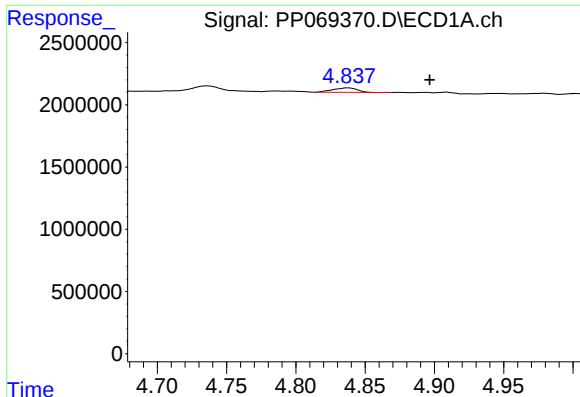

#11 AR-1232-1


R.T.: 4.838 min
Delta R.T.: -0.059 min
Response: 417421
Conc: 12.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

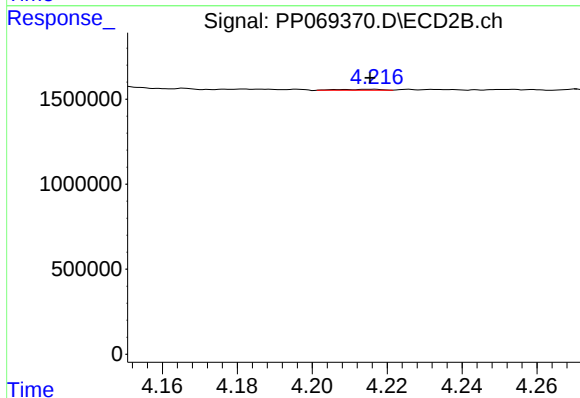


#11 AR-1232-1

R.T.: 4.216 min
Delta R.T.: 0.000 min
Response: 47722
Conc: 2.03 ng/ml

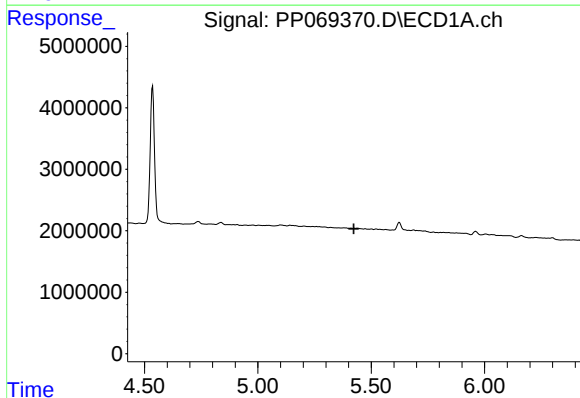


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.424 min
Response: 0
Conc: N.D.

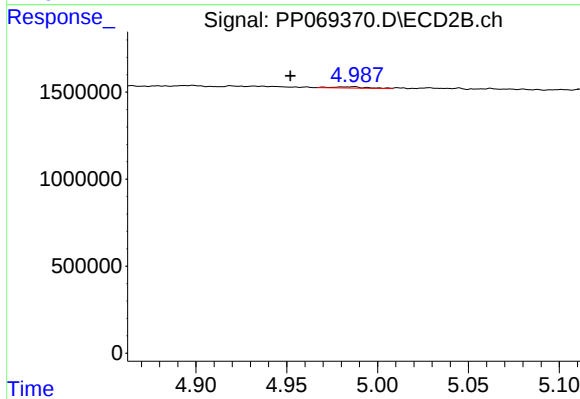

#12 AR-1232-2


R.T.: 4.987 min
Delta R.T.: 0.035 min
Response: 99326
Conc: 4.21 ng/ml

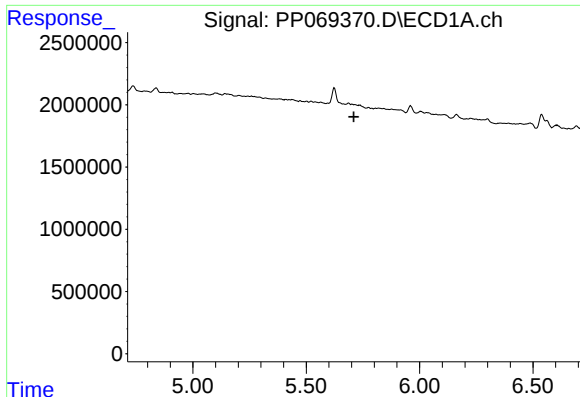

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.710 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

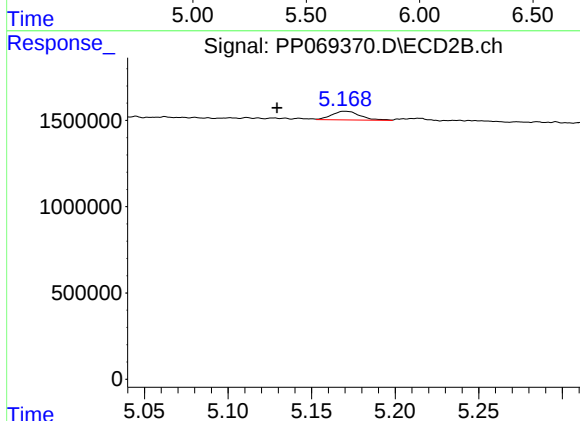


#13 AR-1232-3

R.T.: 5.170 min
Delta R.T.: 0.041 min
Response: 593237
Conc: 45.82 ng/ml

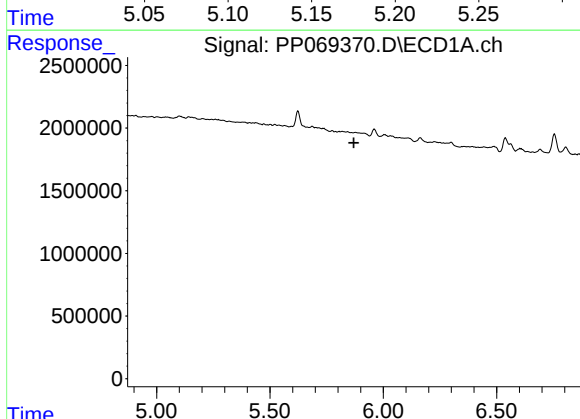


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.870 min
Response: 0
Conc: N.D.

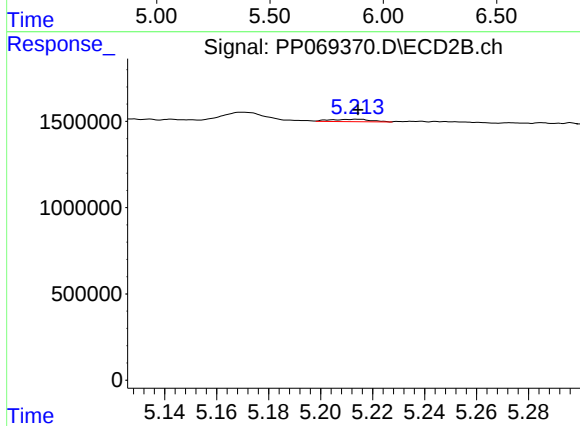

#14 AR-1232-4


R.T.: 5.214 min
Delta R.T.: 0.000 min
Response: 152912
Conc: 13.79 ng/ml

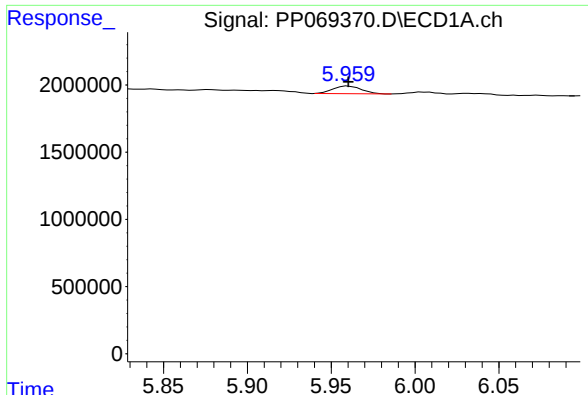

#15 AR-1232-5


R.T.: 5.960 min
Delta R.T.: 0.000 min
Response: 677478
Conc: 59.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

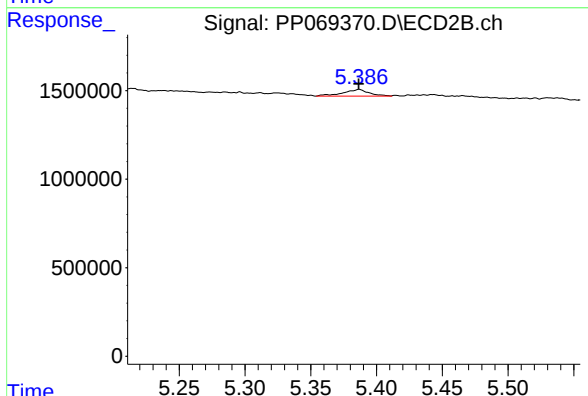


#15 AR-1232-5

R.T.: 5.387 min
Delta R.T.: 0.000 min
Response: 528091
Conc: 43.25 ng/ml

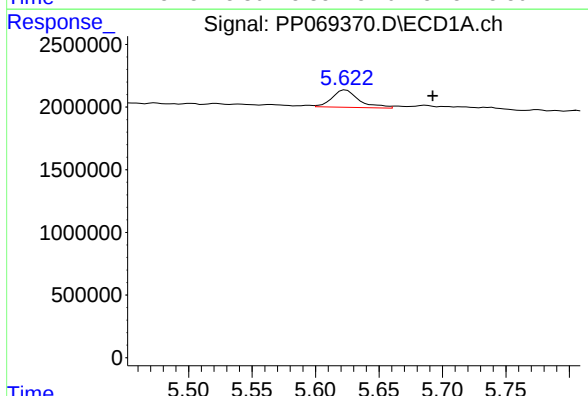


#16 AR-1242-1

R.T.: 5.624 min
Delta R.T.: -0.069 min
Response: 2043515
Conc: 49.00 ng/ml

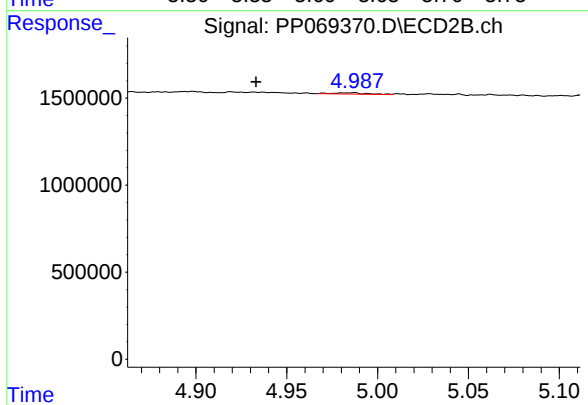

#16 AR-1242-1


R.T.: 4.987 min
Delta R.T.: 0.054 min
Response: 99326
Conc: 3.44 ng/ml

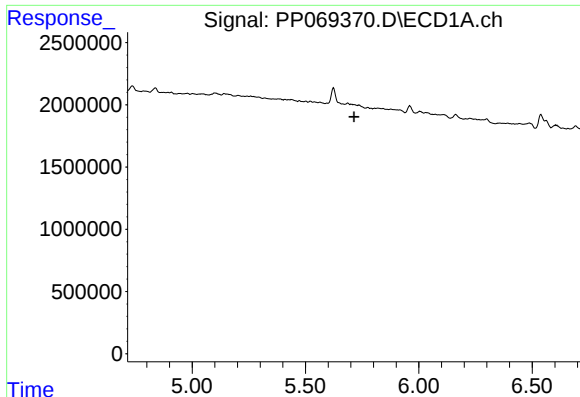

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.714 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

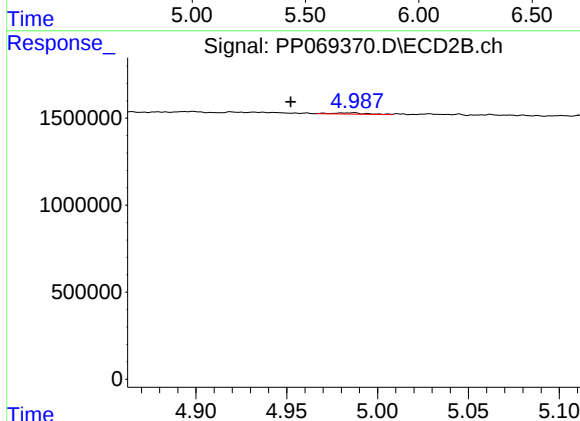


#17 AR-1242-2

R.T.: 4.987 min
Delta R.T.: 0.035 min
Response: 99326
Conc: 2.52 ng/ml

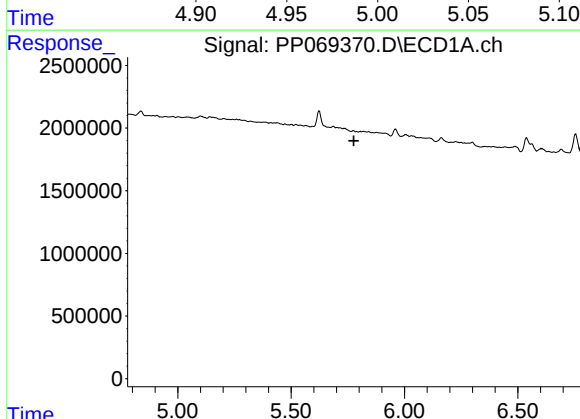


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.776 min
Response: 0
Conc: N.D.

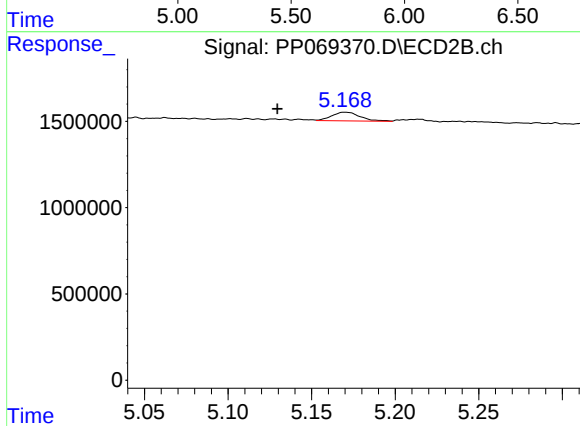

#18 AR-1242-3


R.T.: 5.170 min
Delta R.T.: 0.041 min
Response: 593237
Conc: 26.36 ng/ml

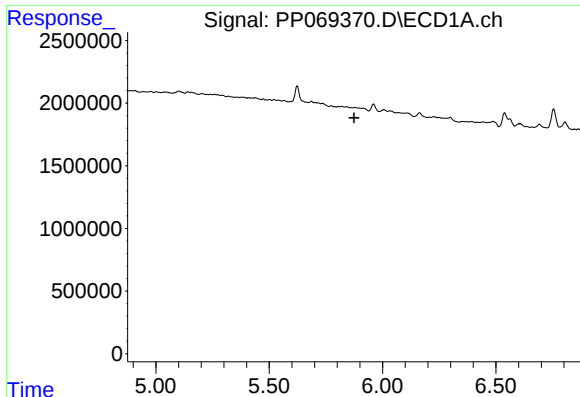

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.874 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

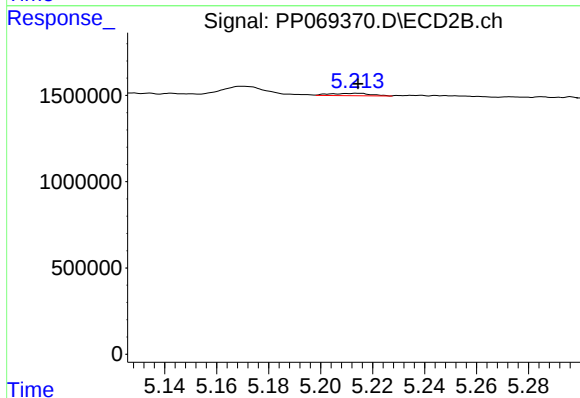


#19 AR-1242-4

R.T.: 5.214 min
Delta R.T.: 0.000 min
Response: 152912
Conc: 7.09 ng/ml

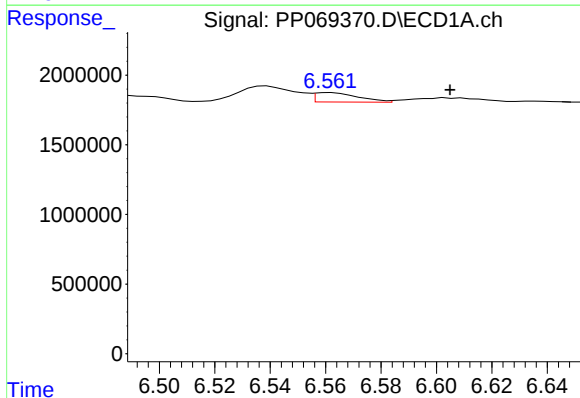


#20 AR-1242-5

R.T.: 6.562 min
Delta R.T.: -0.043 min
Response: 735853
Conc: 22.58 ng/ml

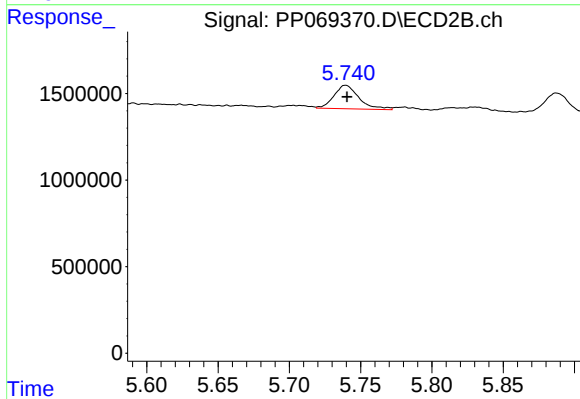

#20 AR-1242-5


R.T.: 5.740 min
Delta R.T.: -0.001 min
Response: 1649476
Conc: 57.34 ng/ml

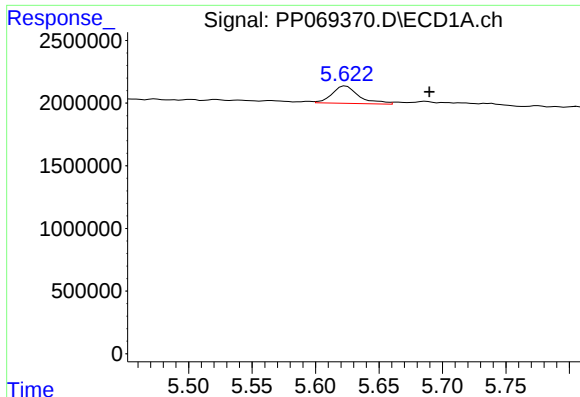

#21 AR-1248-1


R.T.: 5.624 min
Delta R.T.: -0.066 min
Response: 2043515
Conc: 63.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

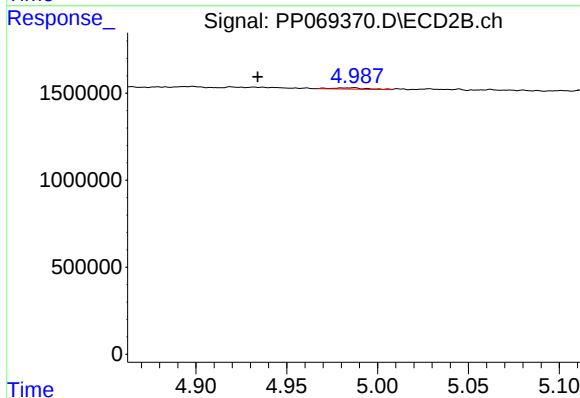


#21 AR-1248-1

R.T.: 4.987 min
Delta R.T.: 0.053 min
Response: 99326
Conc: 4.51 ng/ml

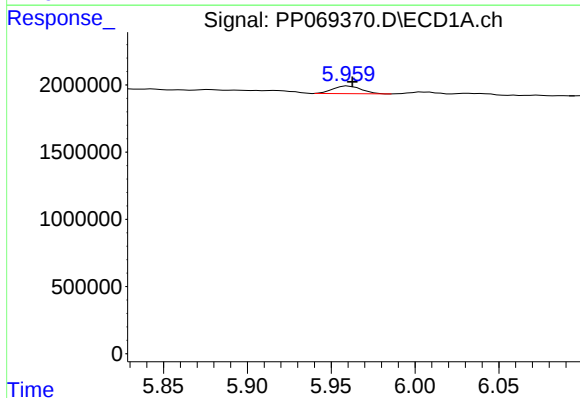


#22 AR-1248-2

R.T.: 5.960 min
Delta R.T.: -0.002 min
Response: 677478
Conc: 15.96 ng/ml

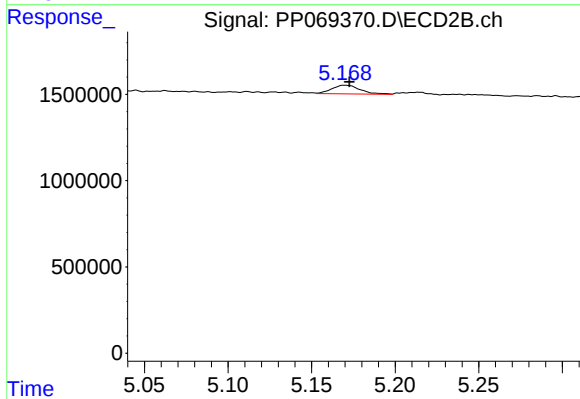

#22 AR-1248-2


R.T.: 5.170 min
Delta R.T.: -0.002 min
Response: 593237
Conc: 19.73 ng/ml

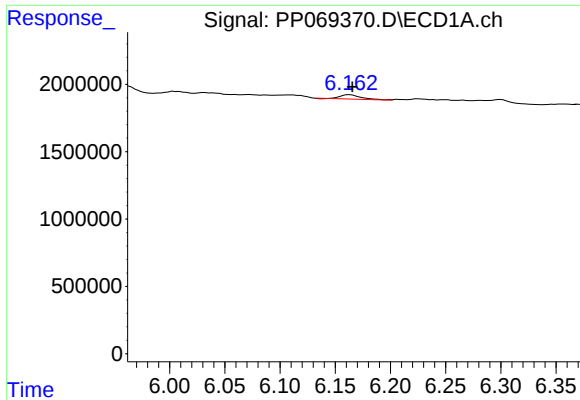

#23 AR-1248-3


R.T.: 6.163 min
Delta R.T.: -0.002 min
Response: 445548
Conc: 9.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

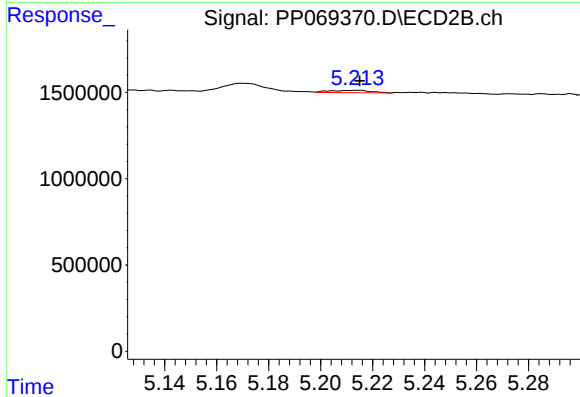


#23 AR-1248-3

R.T.: 5.214 min
Delta R.T.: 0.000 min
Response: 152912
Conc: 4.94 ng/ml

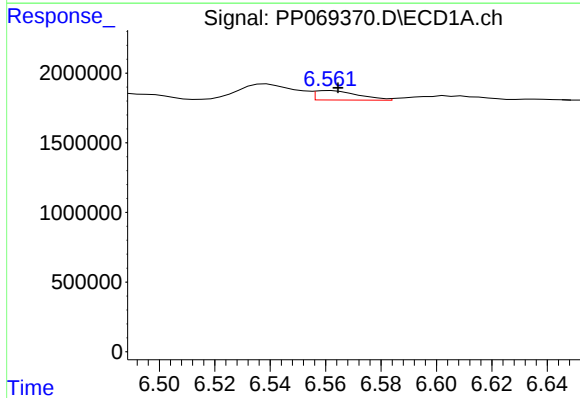


#24 AR-1248-4

R.T.: 6.562 min
Delta R.T.: -0.003 min
Response: 735853
Conc: 13.35 ng/ml

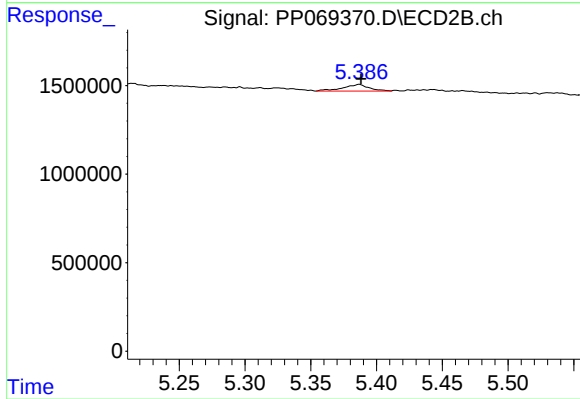

#24 AR-1248-4


R.T.: 5.387 min
Delta R.T.: -0.001 min
Response: 528091
Conc: 14.29 ng/ml

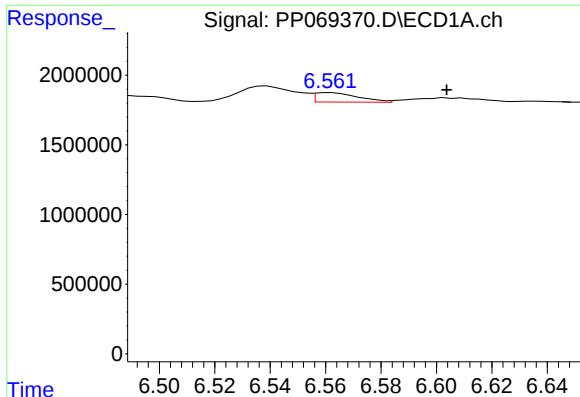

#25 AR-1248-5


R.T.: 6.562 min
Delta R.T.: -0.042 min
Response: 735853
Conc: 13.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

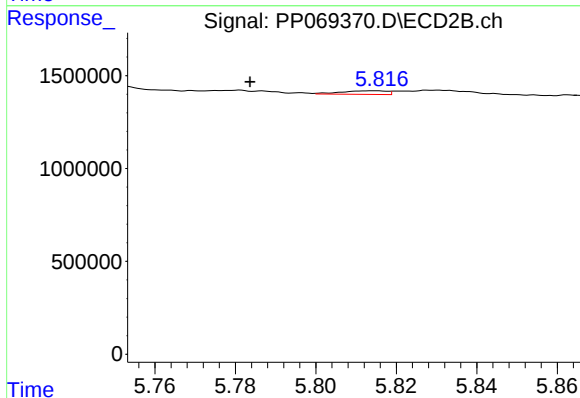


#25 AR-1248-5

R.T.: 5.814 min
Delta R.T.: 0.030 min
Response: 148195
Conc: 3.96 ng/ml

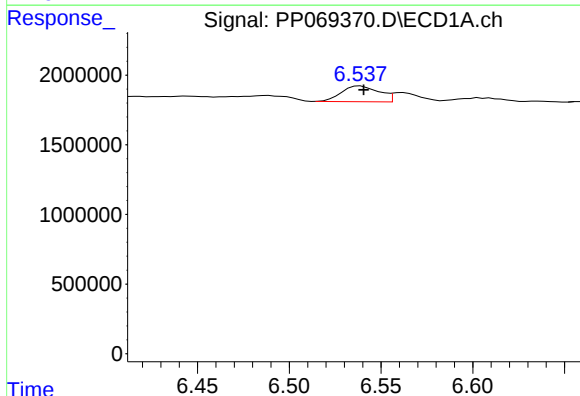


#26 AR-1254-1

R.T.: 6.539 min
Delta R.T.: -0.002 min
Response: 1610372
Conc: 27.83 ng/ml

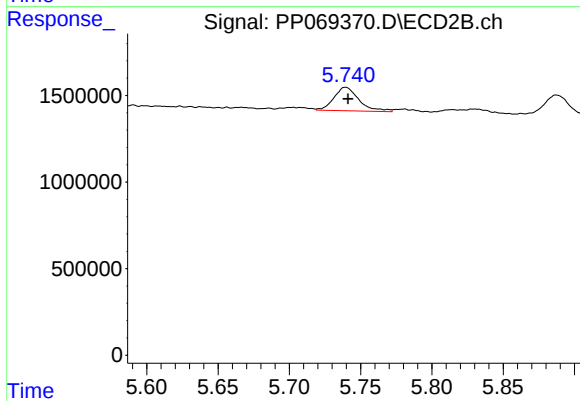

#26 AR-1254-1


R.T.: 5.740 min
Delta R.T.: -0.002 min
Response: 1649476
Conc: 29.96 ng/ml

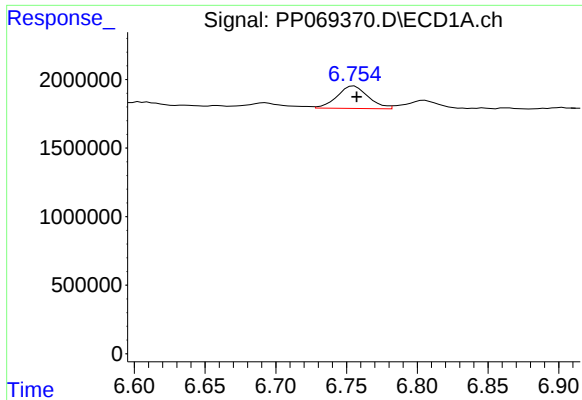

#27 AR-1254-2


R.T.: 6.755 min
Delta R.T.: -0.002 min
Response: 2500902
Conc: 31.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

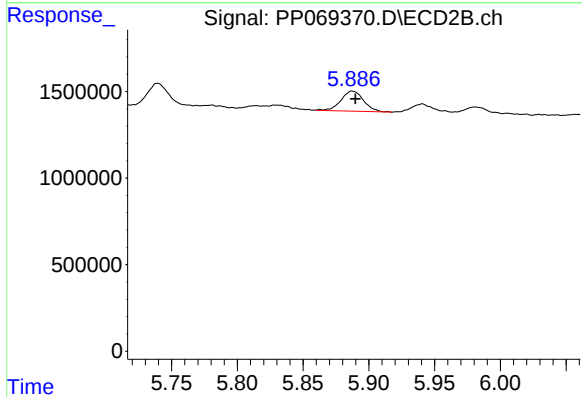


#27 AR-1254-2

R.T.: 5.887 min
Delta R.T.: -0.002 min
Response: 1406754
Conc: 29.08 ng/ml

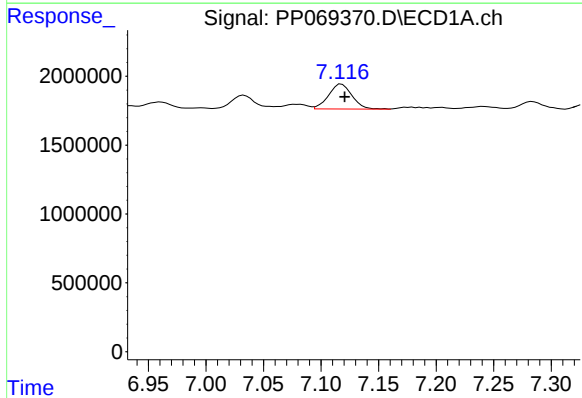


#28 AR-1254-3

R.T.: 7.118 min
Delta R.T.: -0.003 min
Response: 2574523
Conc: 30.54 ng/ml

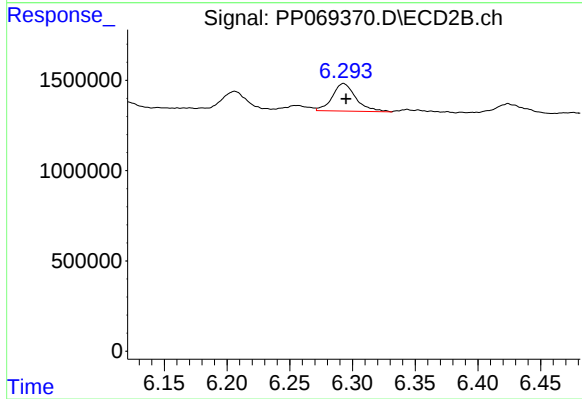

#28 AR-1254-3


R.T.: 6.293 min
Delta R.T.: -0.002 min
Response: 1990888
Conc: 26.23 ng/ml

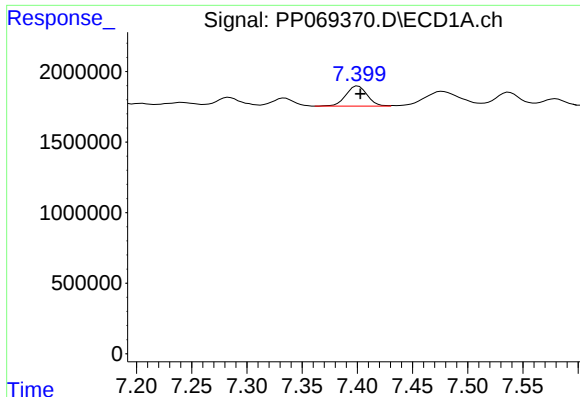

#29 AR-1254-4


R.T.: 7.401 min
Delta R.T.: -0.002 min
Response: 1919032
Conc: 28.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

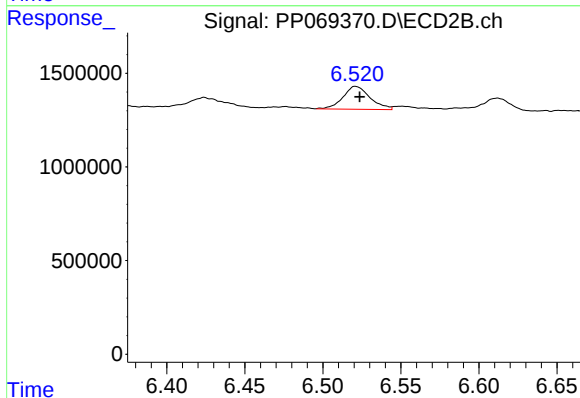


#29 AR-1254-4

R.T.: 6.521 min
Delta R.T.: -0.002 min
Response: 1474177
Conc: 28.76 ng/ml

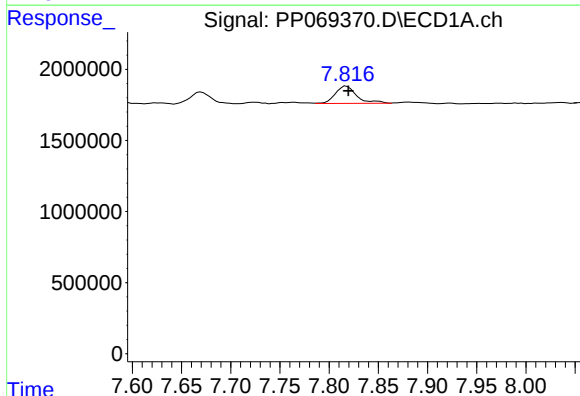


#30 AR-1254-5

R.T.: 7.817 min
Delta R.T.: -0.002 min
Response: 1822529
Conc: 26.78 ng/ml

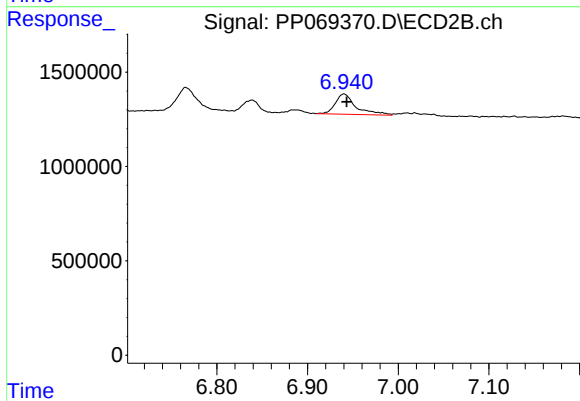

#30 AR-1254-5


R.T.: 6.940 min
Delta R.T.: -0.003 min
Response: 1704260
Conc: 25.60 ng/ml

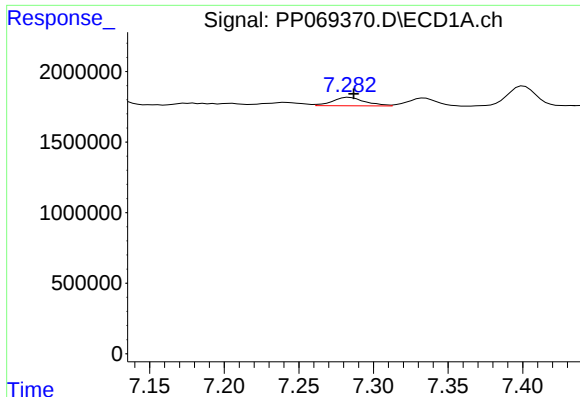

#31 AR-1260-1


R.T.: 7.284 min
Delta R.T.: -0.003 min
Response: 906814
Conc: 15.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

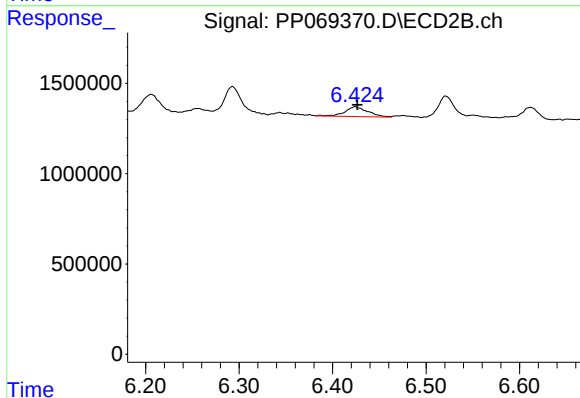


#31 AR-1260-1

R.T.: 6.424 min
Delta R.T.: -0.002 min
Response: 925169
Conc: 19.18 ng/ml

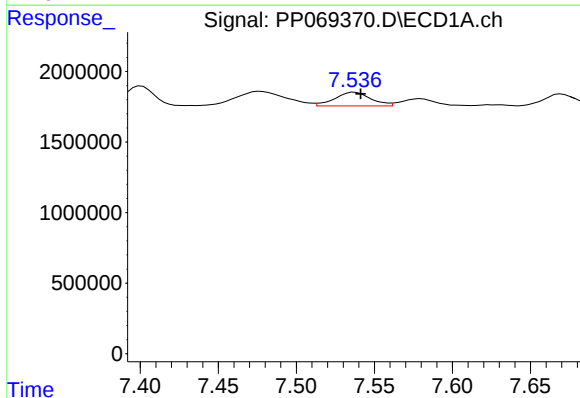


#32 AR-1260-2

R.T.: 7.537 min
Delta R.T.: -0.004 min
Response: 1560692
Conc: 20.06 ng/ml

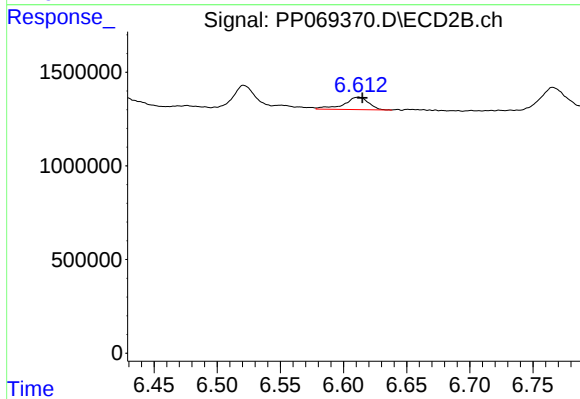

#32 AR-1260-2


R.T.: 6.612 min
Delta R.T.: -0.003 min
Response: 893605
Conc: 14.58 ng/ml

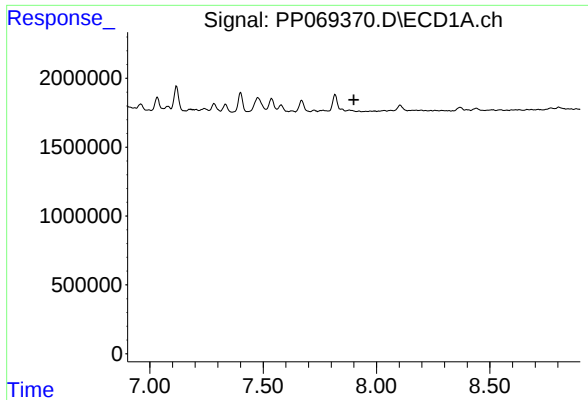

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.900 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

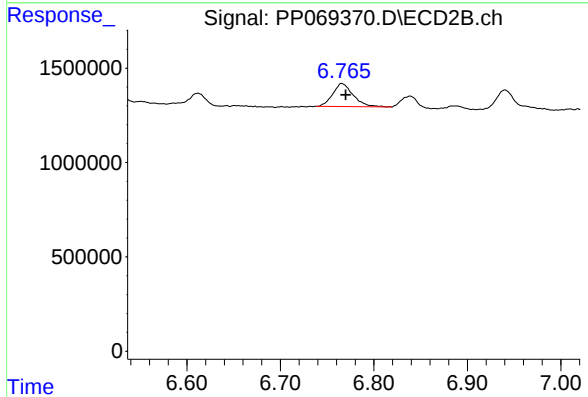


#33 AR-1260-3

R.T.: 6.766 min
Delta R.T.: -0.004 min
Response: 1845680
Conc: 30.68 ng/ml

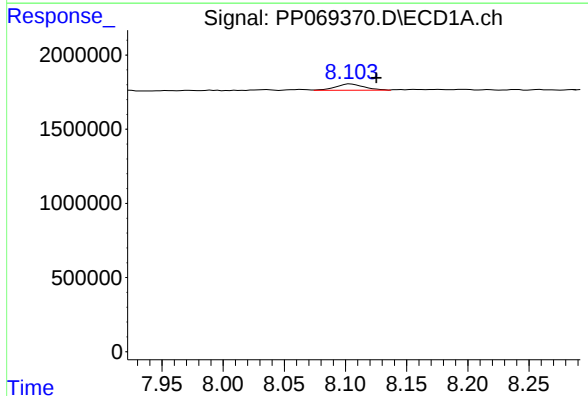


#34 AR-1260-4

R.T.: 8.104 min
Delta R.T.: -0.021 min
Response: 688995
Conc: 10.44 ng/ml

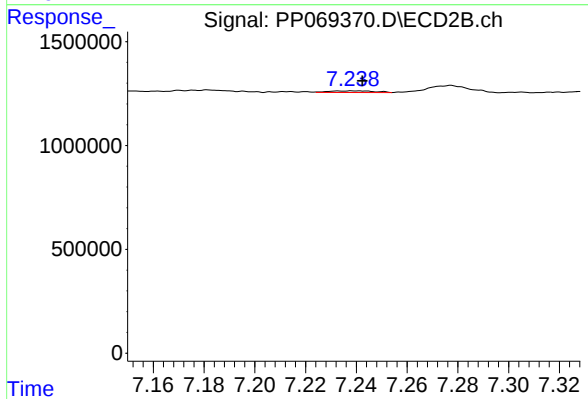

#34 AR-1260-4


R.T.: 7.233 min
Delta R.T.: -0.009 min
Response: 101287
Conc: 2.18 ng/ml

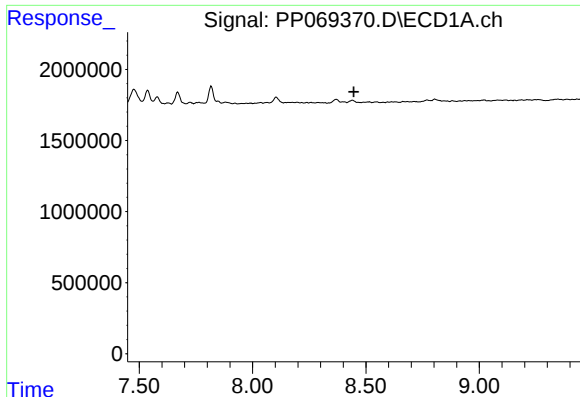

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.447 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

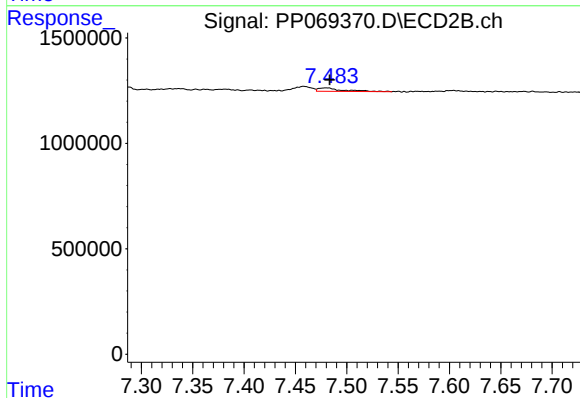


#35 AR-1260-5

R.T.: 7.481 min
Delta R.T.: -0.003 min
Response: 269701
Conc: 2.43 ng/ml

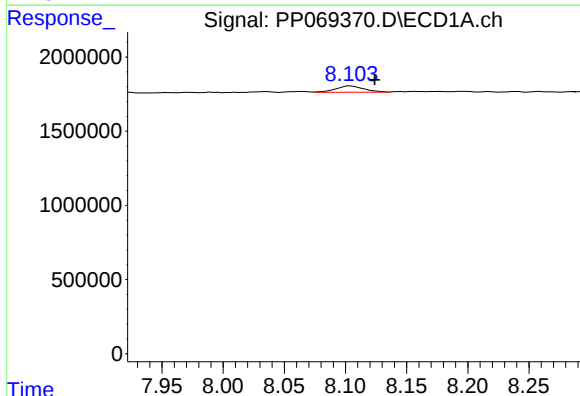


#36 AR-1262-1

R.T.: 8.104 min
Delta R.T.: -0.020 min
Response: 688995
Conc: 8.72 ng/ml

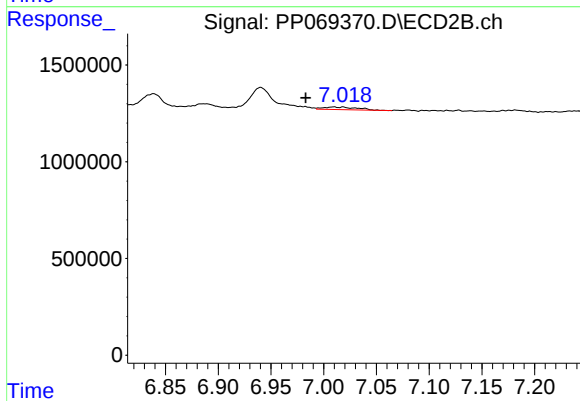

#36 AR-1262-1


R.T.: 7.010 min
Delta R.T.: 0.027 min
Response: 309816
Conc: 4.36 ng/ml

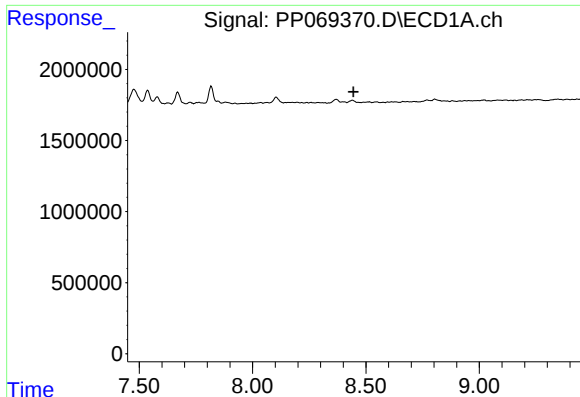

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.446 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

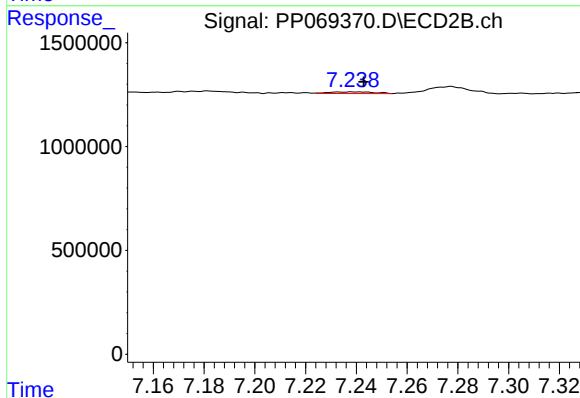


#37 AR-1262-2

R.T.: 7.233 min
Delta R.T.: -0.010 min
Response: 101287
Conc: 1.66 ng/ml

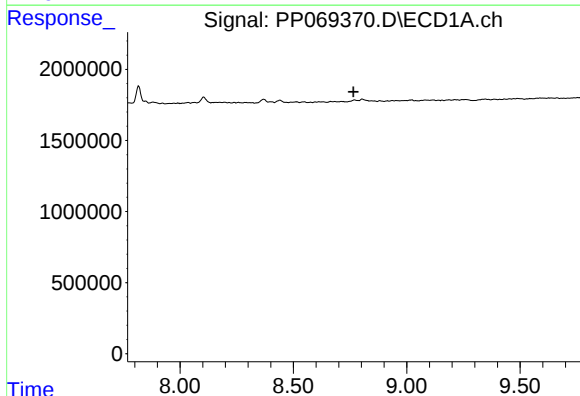


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.766 min
Response: 0
Conc: N.D.

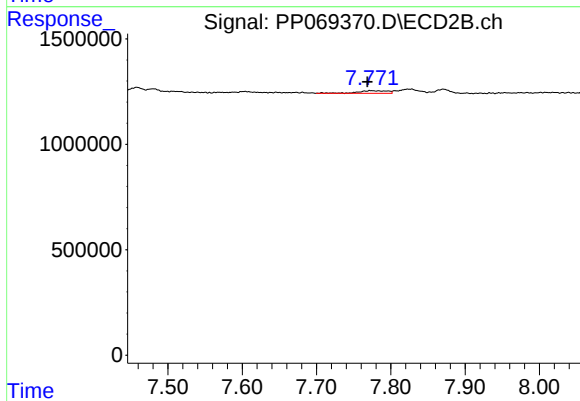

#38 AR-1262-3


R.T.: 7.772 min
Delta R.T.: 0.004 min
Response: 350949
Conc: 6.71 ng/ml

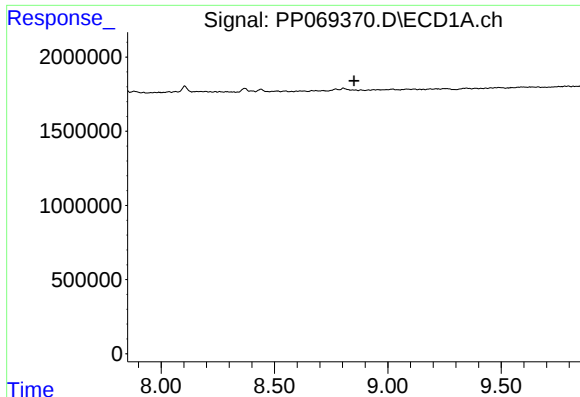

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.852 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

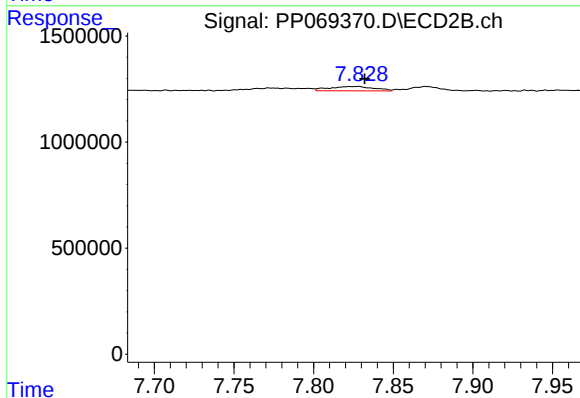


#39 AR-1262-4

R.T.: 7.828 min
Delta R.T.: -0.004 min
Response: 401500
Conc: 4.34 ng/ml

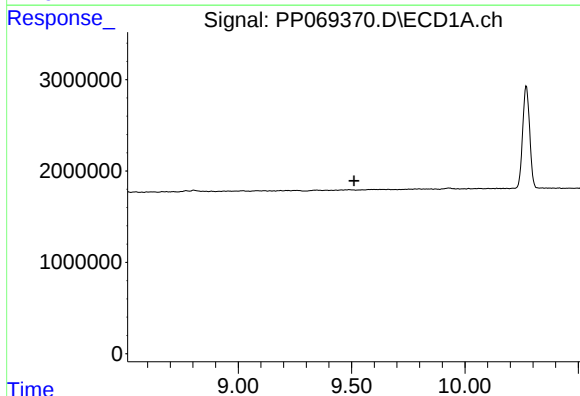


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.511 min
Response: 0
Conc: N.D.

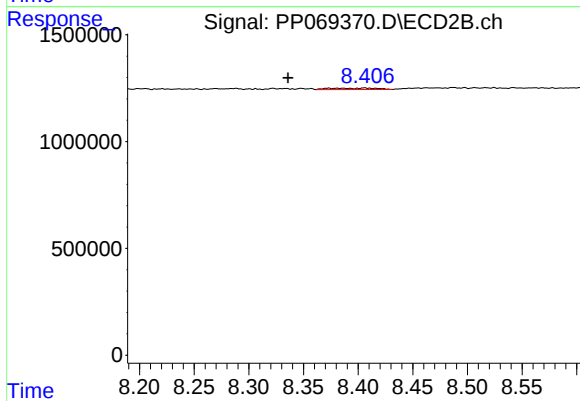

#40 AR-1262-5


R.T.: 8.406 min
Delta R.T.: 0.070 min
Response: 199503
Conc: 4.17 ng/ml

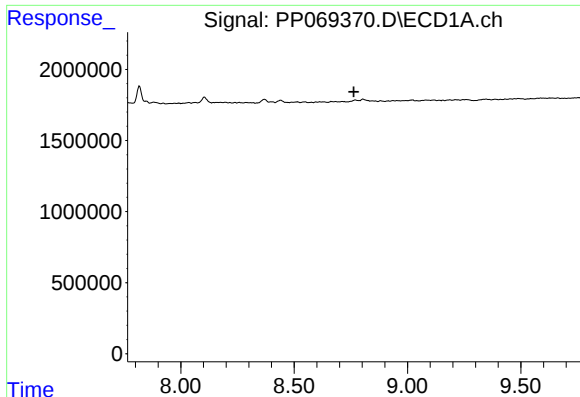

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

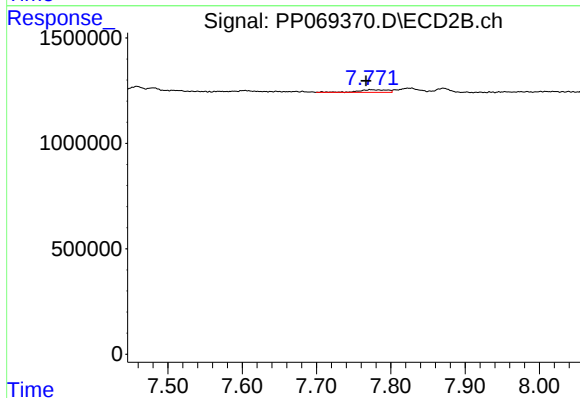


#41 AR-1268-1

R.T.: 7.772 min
Delta R.T.: 0.006 min
Response: 350949
Conc: 2.42 ng/ml

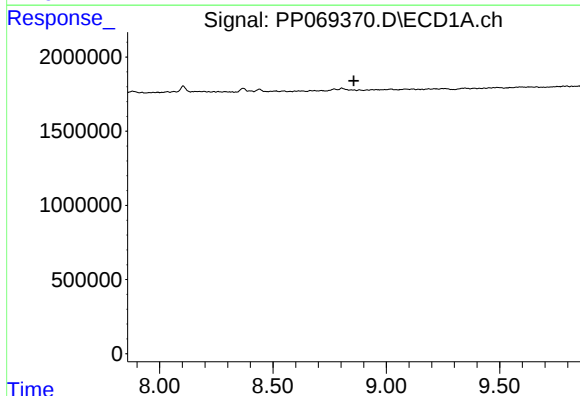


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.857 min
Response: 0
Conc: N.D.

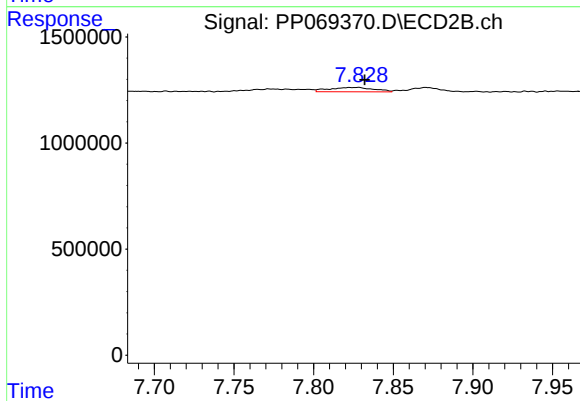

#42 AR-1268-2


R.T.: 7.828 min
Delta R.T.: -0.004 min
Response: 401500
Conc: 3.02 ng/ml

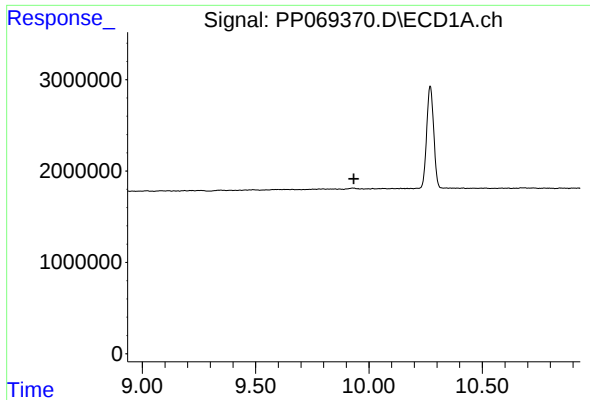

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.933 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

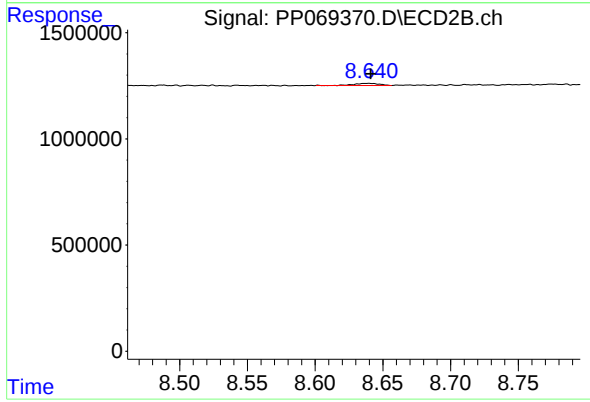

#45 AR-1268-5

R.T.: 8.639 min
Delta R.T.: -0.002 min
Response: 130065
Conc: 0.37 ng/ml