

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
 Data File : PP069332.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2025 17:59
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/31/2025
 Supervised By :Ankita Jodhani 01/31/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 00:52:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.536	3.841	39027156	24448386	27.263	27.392m
2) SA Decachlor...	10.276	8.911	29960876	32094137	27.414	28.694

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
Data File : PP069332.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2025 17:59
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/31/2025
Supervised By :Ankita Jodhani 01/31/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 00:52:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

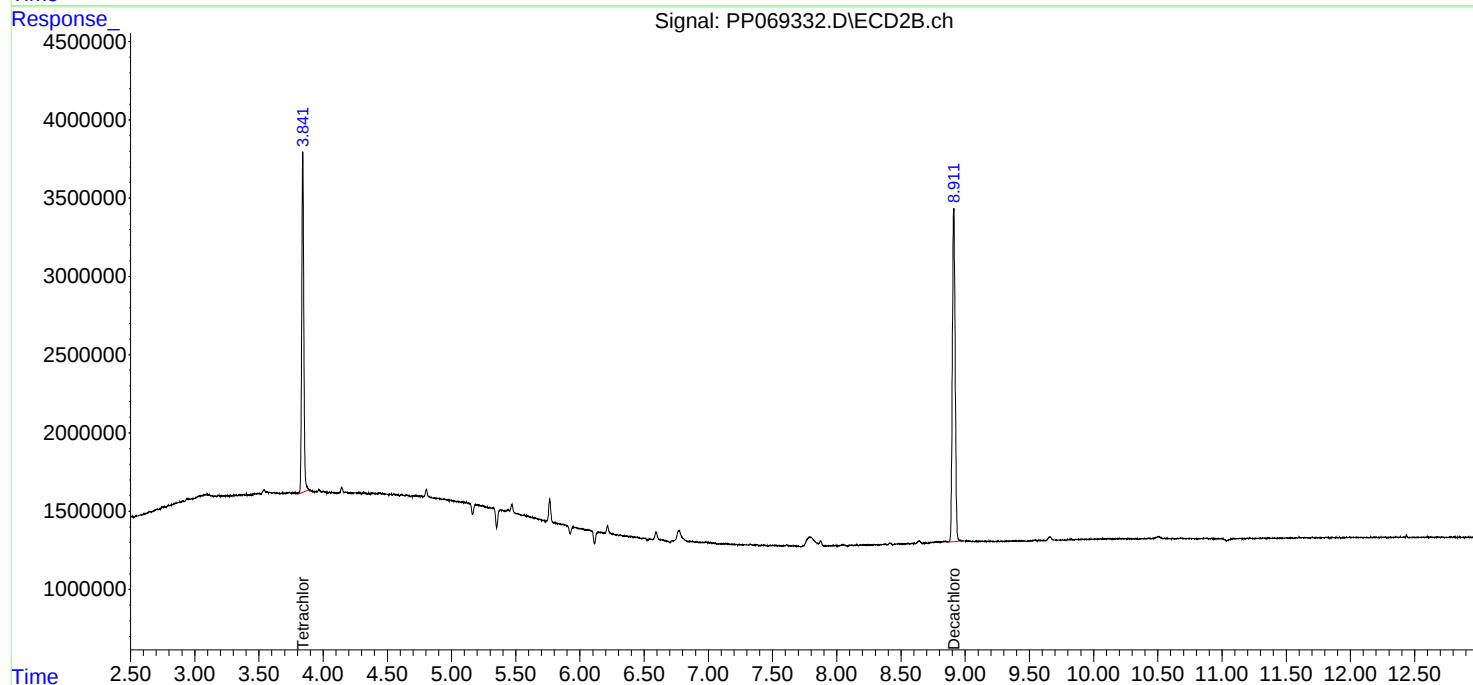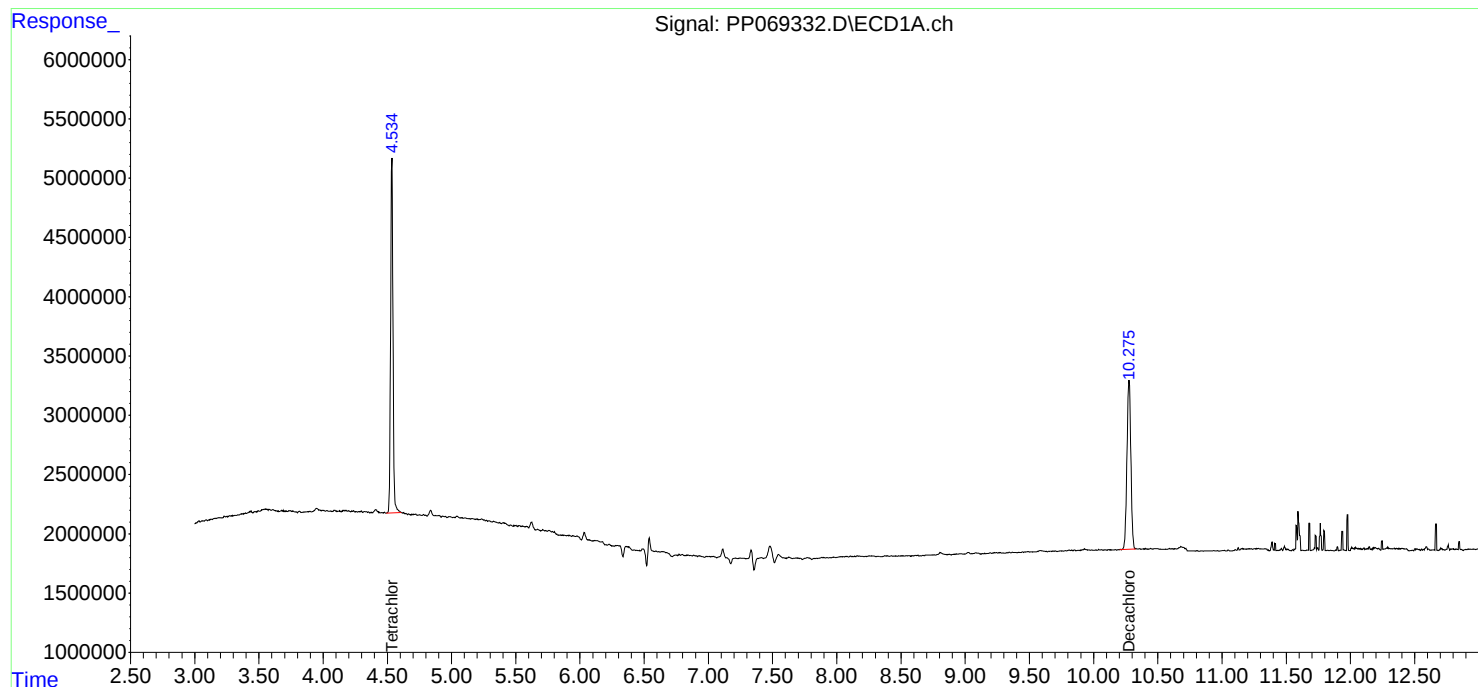

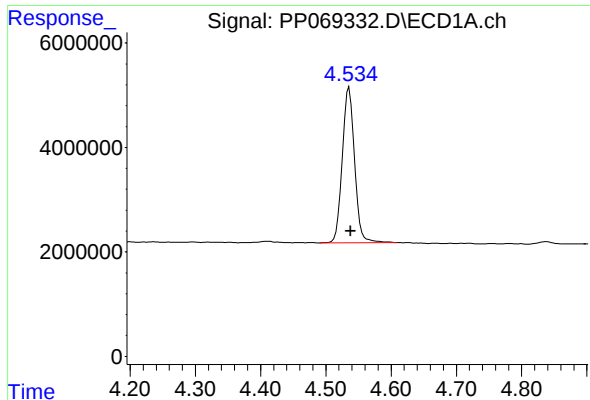


#1 Tetrachloro-m-xylene

R.T.: 4.536 min
Delta R.T.: -0.002 min
Response: 39027156
Conc: 27.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/31/2025
Supervised By :Ankita Jodhani 01/31/2025

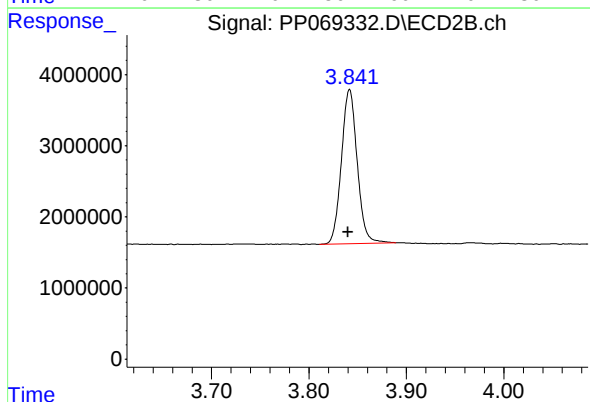


#1 Tetrachloro-m-xylene

R.T.: 3.841 min
Delta R.T.: 0.001 min
Response: 24448386
Conc: 27.39 ng/ml

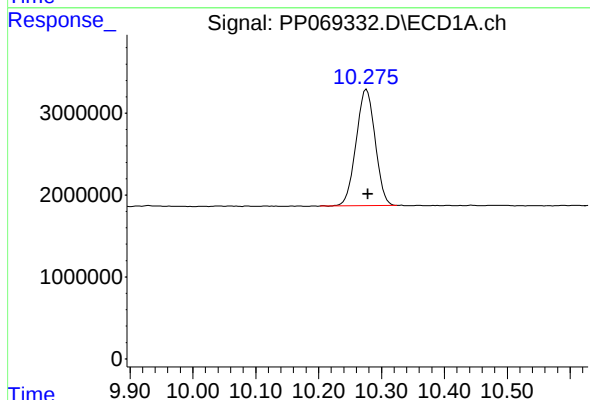

#2 Decachlorobiphenyl

R.T.: 10.276 min
Delta R.T.: -0.002 min
Response: 29960876
Conc: 27.41 ng/ml

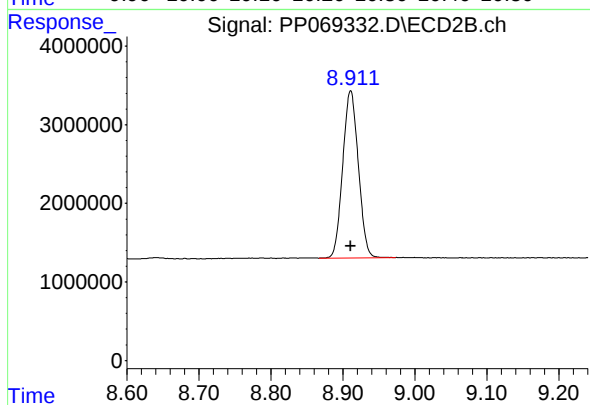

#2 Decachlorobiphenyl

R.T.: 8.911 min
Delta R.T.: 0.000 min
Response: 32094137
Conc: 28.69 ng/ml