

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
 Data File : PP069372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2025 04:50
 Operator : YP\AJ
 Sample : Q1168-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT1-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 05:35:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.534	3.839	29552176	18772179	20.644	21.032
2) SA Decachlor...	10.269	8.905	24911221	28353328	22.794	25.350
Target Compounds						
41) L9 AR-1268-1	8.756	7.763	4303093	4099683	24.369	28.250
42) L9 AR-1268-2	8.849	7.828	3783911	3750974	24.044	28.242
43) L9 AR-1268-3	9.083	8.036	3225818	2903047	24.122	25.524
44) L9 AR-1268-4	9.502	8.330	1374127	1353290	23.401	25.986
45) L9 AR-1268-5	9.924	8.635	9511764	9753144	24.972	27.383



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012925\
Data File : PP069372.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2025 04:50
Operator : YP\AJ
Sample : Q1168-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 66 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 05:35:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

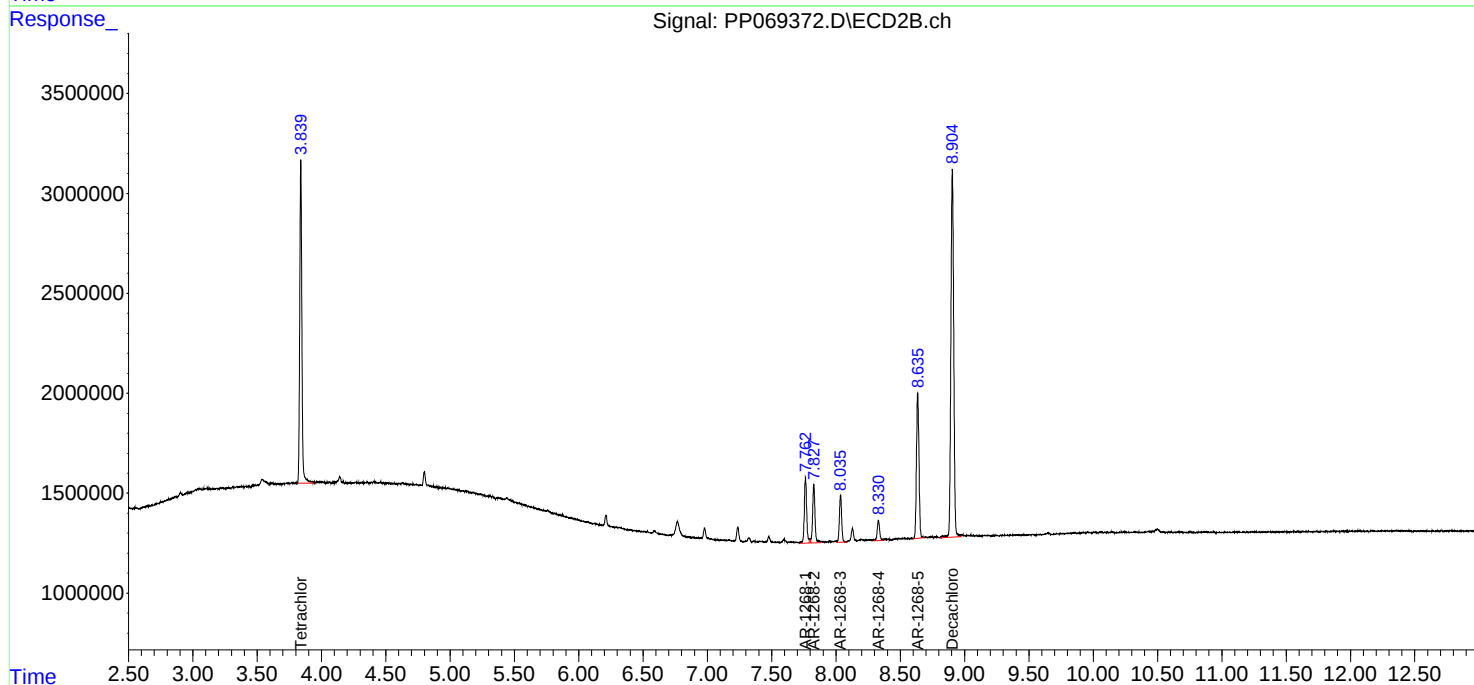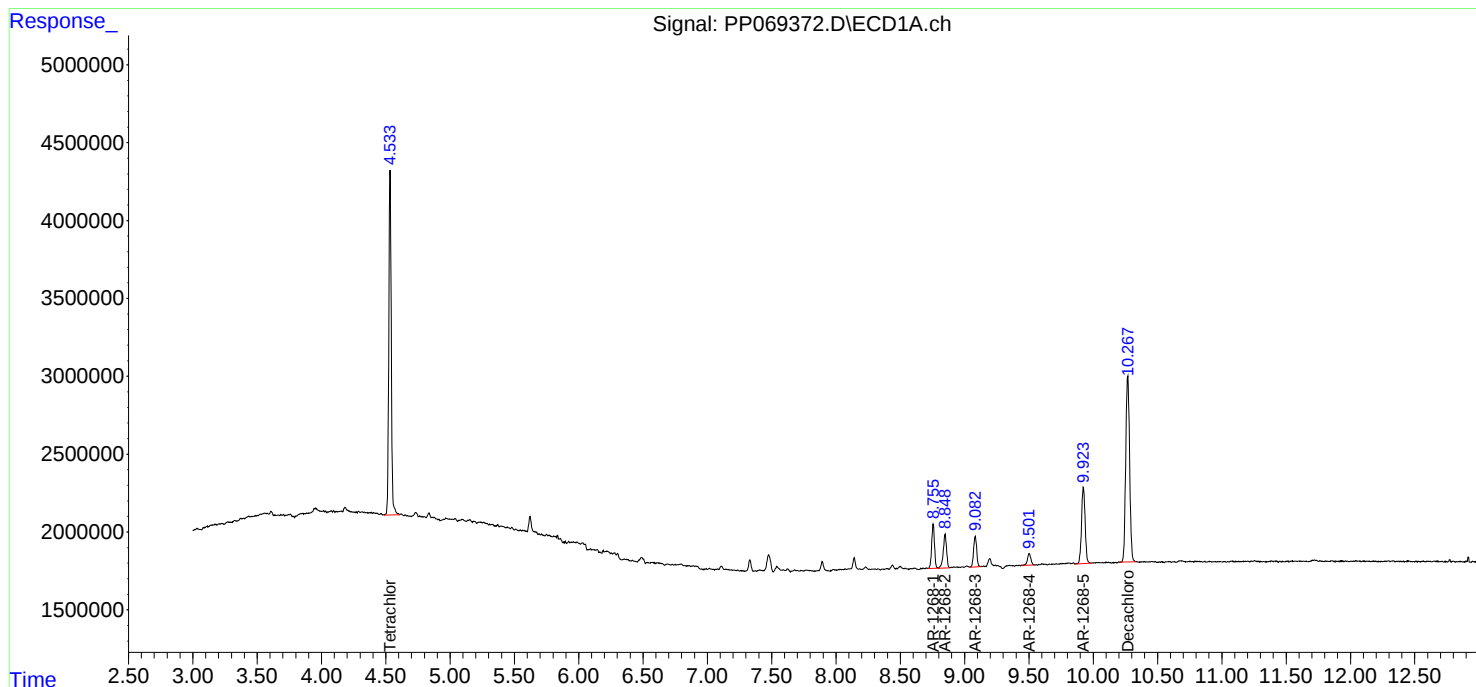


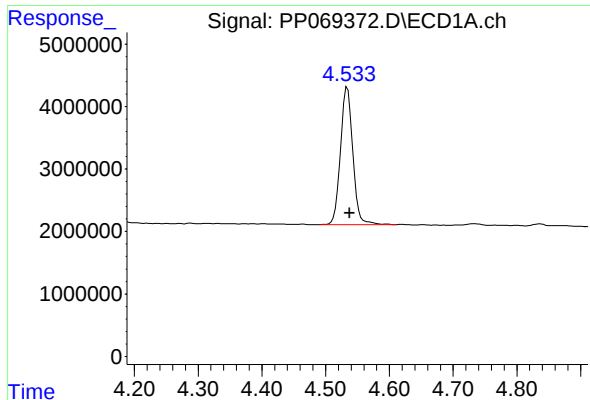

#1 Tetrachloro-m-xylene


R.T.: 4.534 min
Delta R.T.: -0.004 min
Response: 29552176
Conc: 20.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

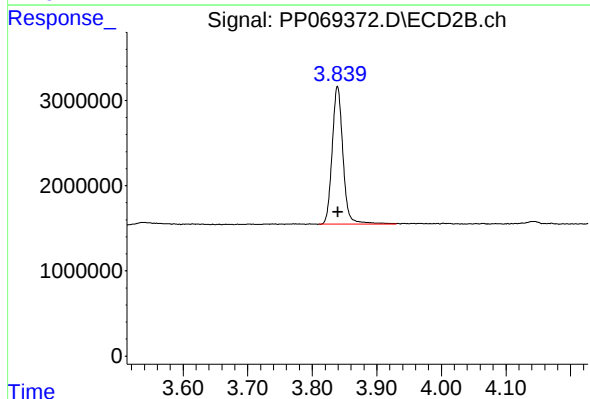


#1 Tetrachloro-m-xylene

R.T.: 3.839 min
Delta R.T.: 0.000 min
Response: 18772179
Conc: 21.03 ng/ml

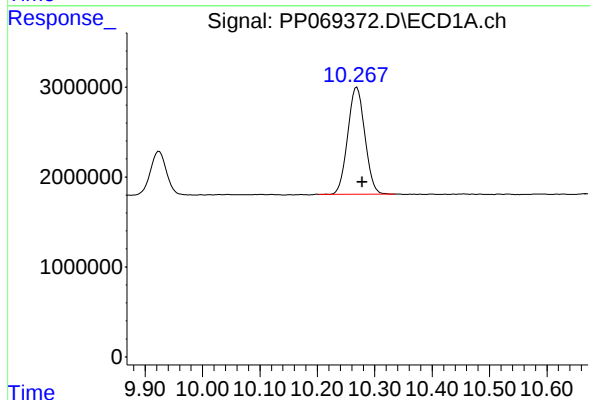


#2 Decachlorobiphenyl

R.T.: 10.269 min
Delta R.T.: -0.010 min
Response: 24911221
Conc: 22.79 ng/ml

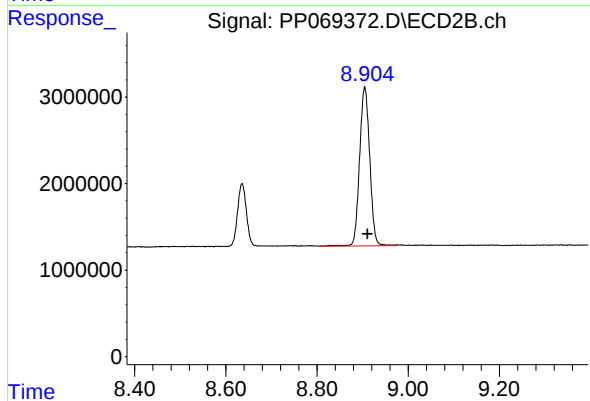

#2 Decachlorobiphenyl


R.T.: 8.905 min
Delta R.T.: -0.006 min
Response: 28353328
Conc: 25.35 ng/ml

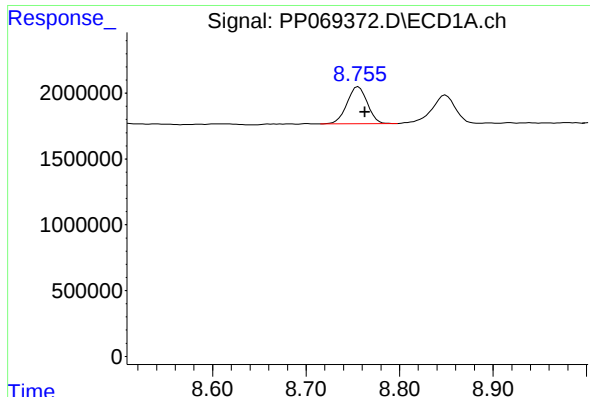

#41 AR-1268-1


R.T.: 8.756 min
Delta R.T.: -0.007 min
Response: 4303093
Conc: 24.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

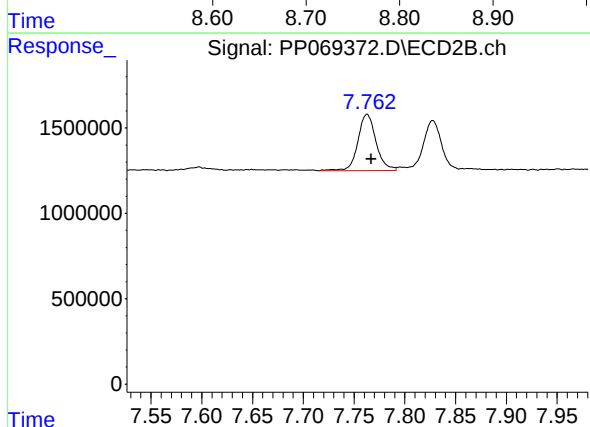


#41 AR-1268-1

R.T.: 7.763 min
Delta R.T.: -0.004 min
Response: 4099683
Conc: 28.25 ng/ml

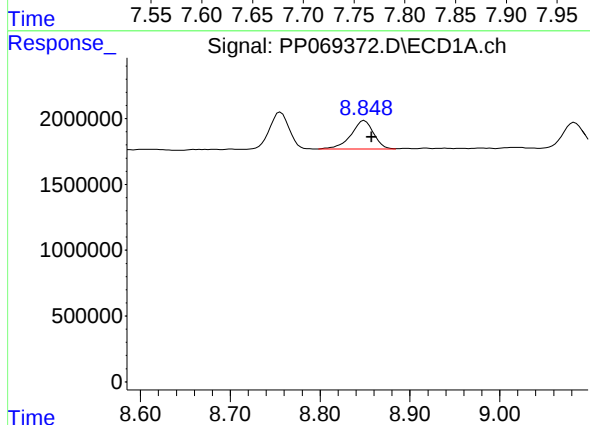


#42 AR-1268-2

R.T.: 8.849 min
Delta R.T.: -0.008 min
Response: 3783911
Conc: 24.04 ng/ml

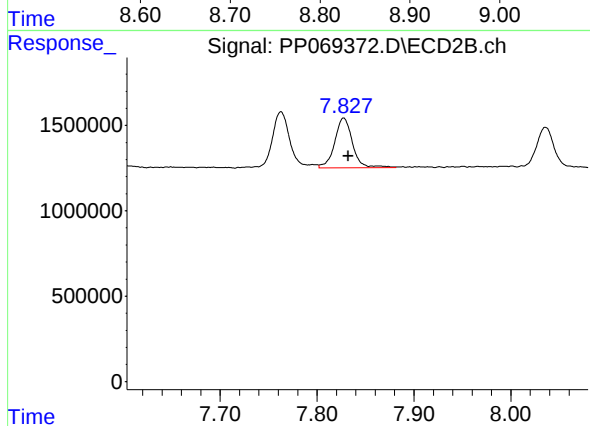

#42 AR-1268-2


R.T.: 7.828 min
Delta R.T.: -0.004 min
Response: 3750974
Conc: 28.24 ng/ml

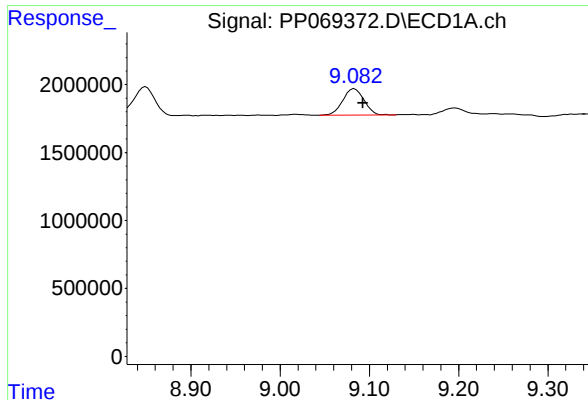

#43 AR-1268-3


R.T.: 9.083 min
Delta R.T.: -0.010 min
Response: 3225818
Conc: 24.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

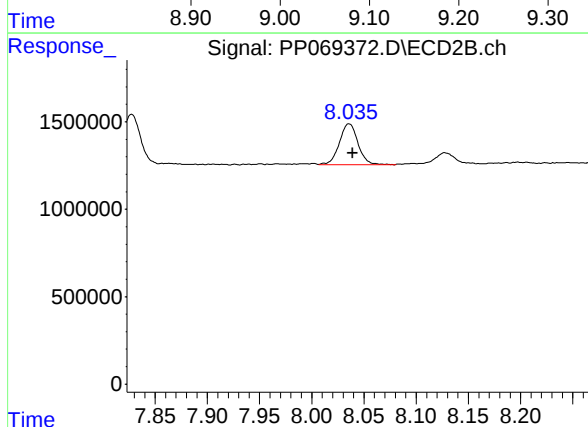


#43 AR-1268-3

R.T.: 8.036 min
Delta R.T.: -0.003 min
Response: 2903047
Conc: 25.52 ng/ml

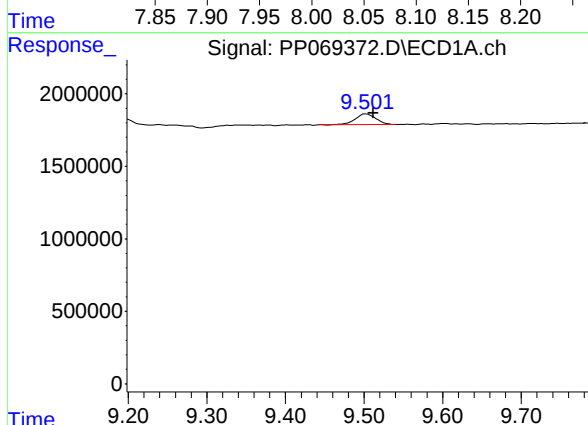


#44 AR-1268-4

R.T.: 9.502 min
Delta R.T.: -0.009 min
Response: 1374127
Conc: 23.40 ng/ml

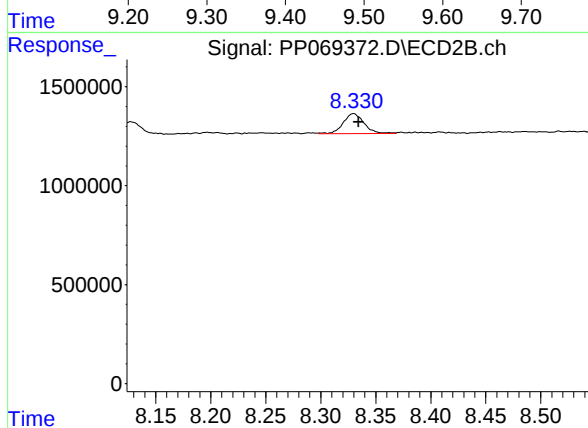

#44 AR-1268-4


R.T.: 8.330 min
Delta R.T.: -0.005 min
Response: 1353290
Conc: 25.99 ng/ml

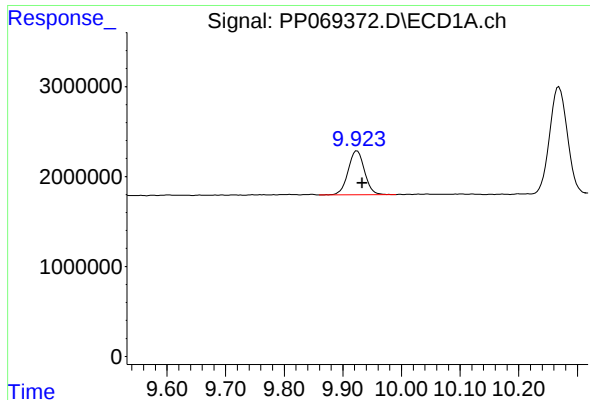

#45 AR-1268-5

R.T.: 9.924 min
Delta R.T.: -0.009 min
Response: 9511764
Conc: 24.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2025

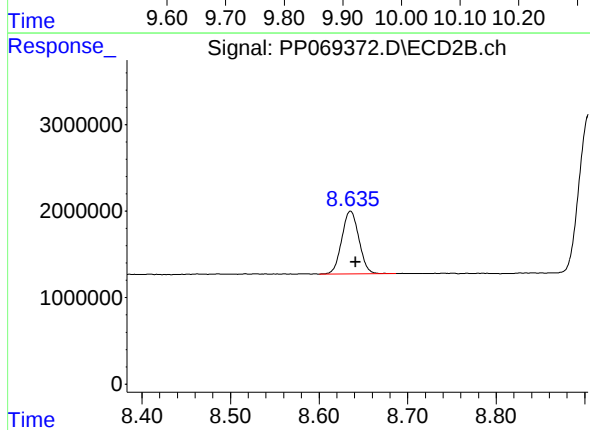

#45 AR-1268-5

R.T.: 8.635 min
Delta R.T.: -0.006 min
Response: 9753144
Conc: 27.38 ng/ml