

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP013023\
 Data File : PP055067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2023 15:31
 Operator : YP\AJ
 Sample : 01345-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RBR200007

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/31/2023
 Supervised By :Ankita Jodhani 01/31/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 17:14:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 03:37:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.352	3.606f	25142987	23906964	14.461	15.925m
2) SA Decachlor...	10.089	8.595	35669591	27686806	20.598m	20.500m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP013023\
Data File : PP055067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2023 15:31
Operator : YP\AJ
Sample : 01345-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
RBR200007


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/31/2023
Supervised By :Ankita Jodhani 01/31/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 17:14:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 03:37:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

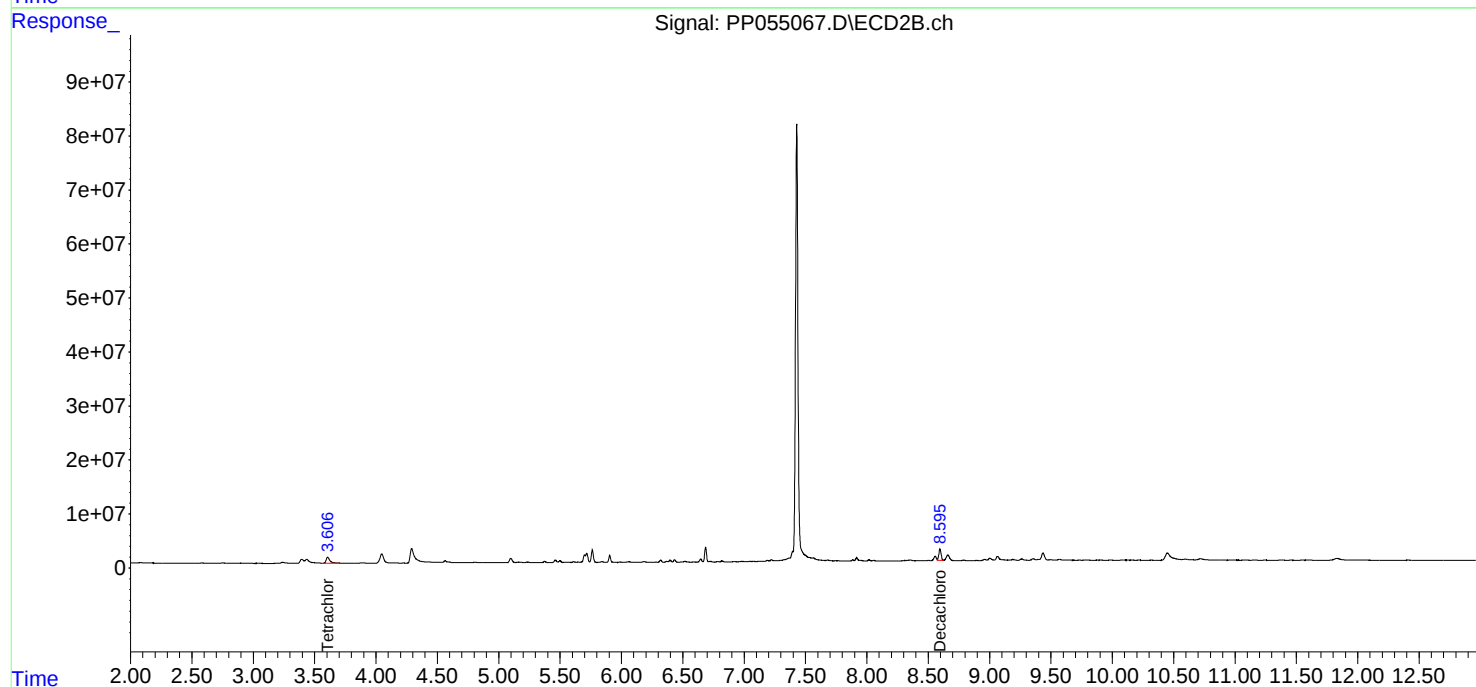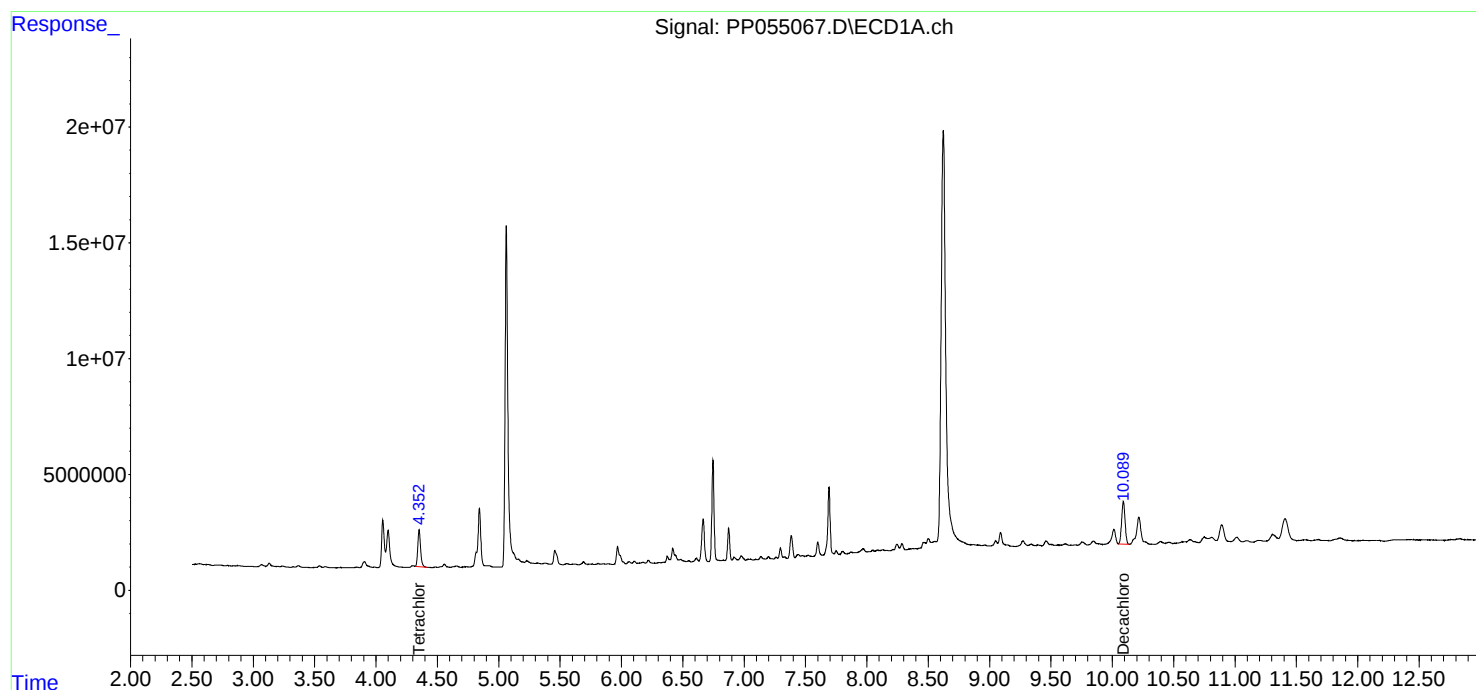

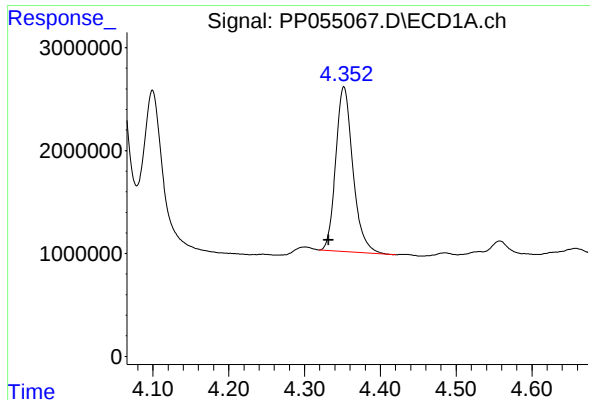


#1 Tetrachloro-m-xylene

R.T.: 4.352 min
Delta R.T.: 0.020 min
Response: 25142987
Conc: 14.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
RBR200007


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/31/2023
Supervised By :Ankita Jodhani 01/31/2023

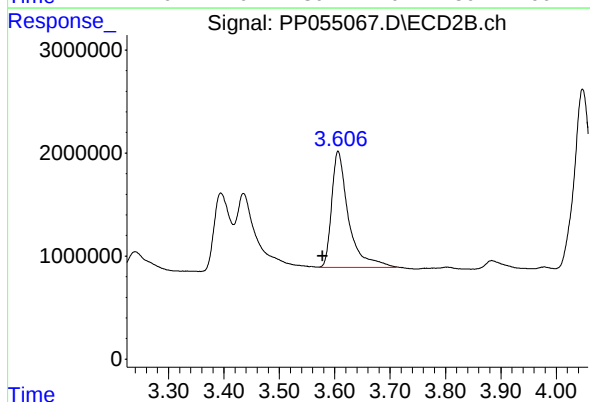


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: 0.027 min
Response: 23906964
Conc: 15.93 ng/ml m

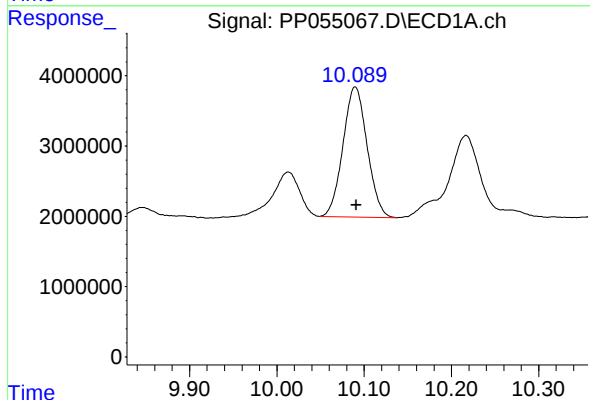

#2 Decachlorobiphenyl

R.T.: 10.089 min
Delta R.T.: -0.002 min
Response: 35669591
Conc: 20.60 ng/ml m

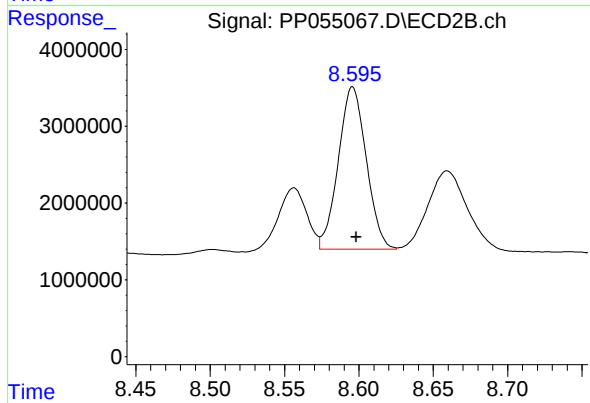

#2 Decachlorobiphenyl

R.T.: 8.595 min
Delta R.T.: -0.003 min
Response: 27686806
Conc: 20.50 ng/ml m