

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP013023\
 Data File : PP055116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2023 05:58
 Operator : YP\AJ
 Sample : 01344-05 10X
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DBA3342-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/31/2023
 Supervised By :Ankita Jodhani 01/31/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 06:15:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 03:37:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.328	3.575	2963034	2754025	1.704m	1.835
2) SA Decachlor...	10.083	8.588	3806372	2944768	2.198	2.180

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP013023\
Data File : PP055116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2023 05:58
Operator : YP\AJ
Sample : 01344-05 10X
Misc :
ALS Vial : 53 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
DBA3342-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/31/2023
Supervised By :Ankita Jodhani 01/31/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 06:15:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 03:37:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

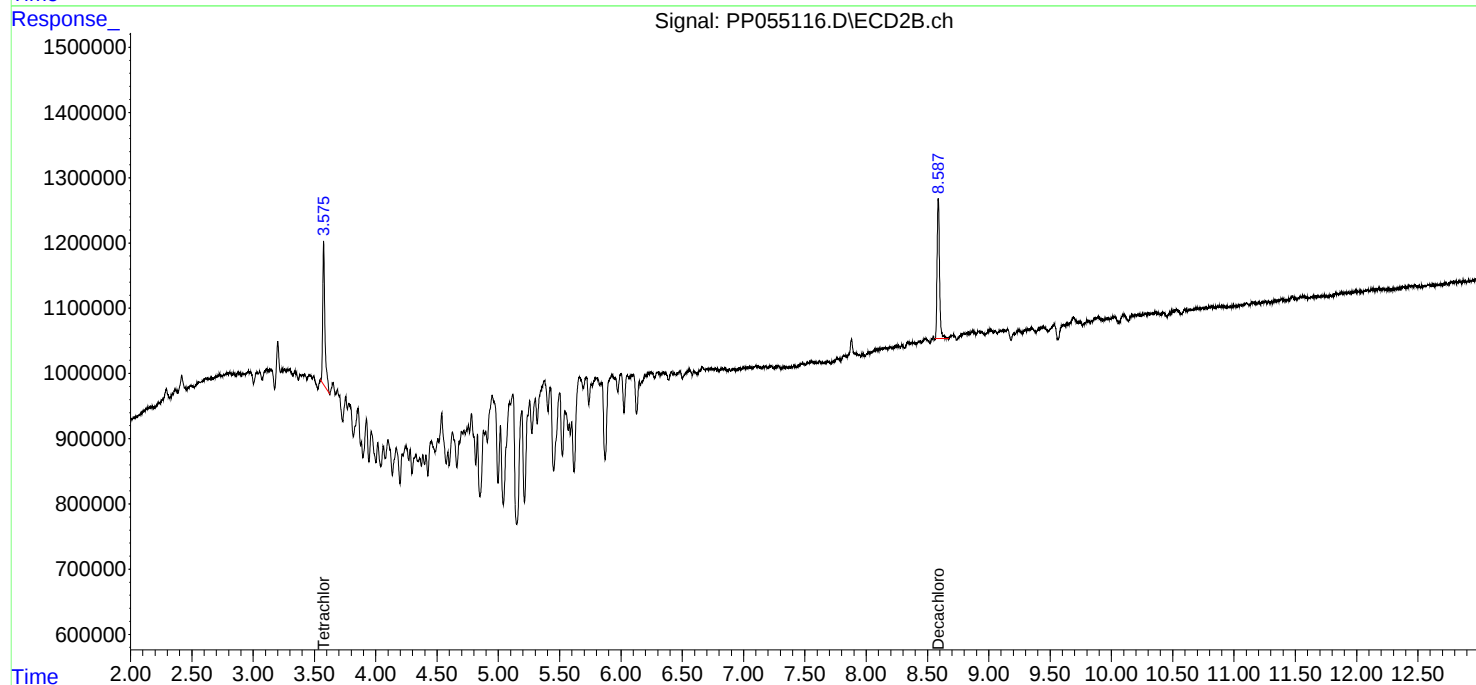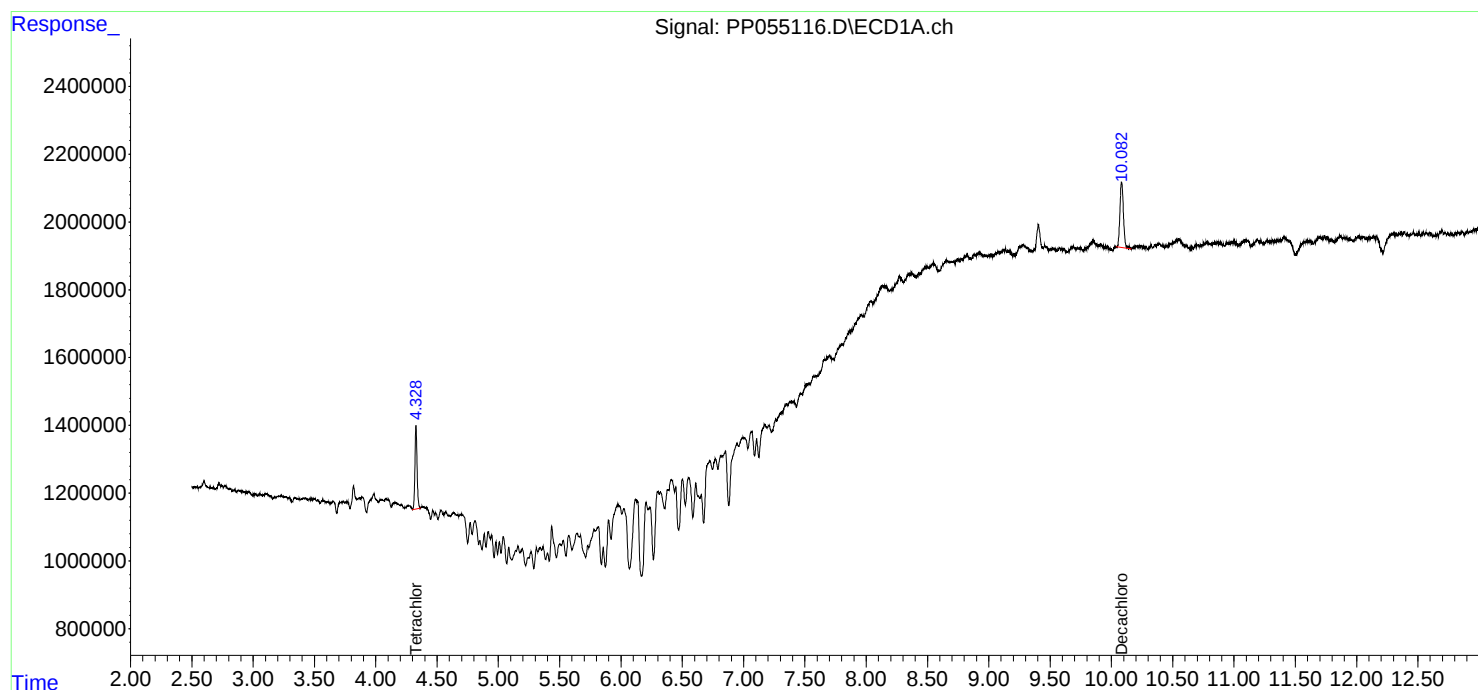

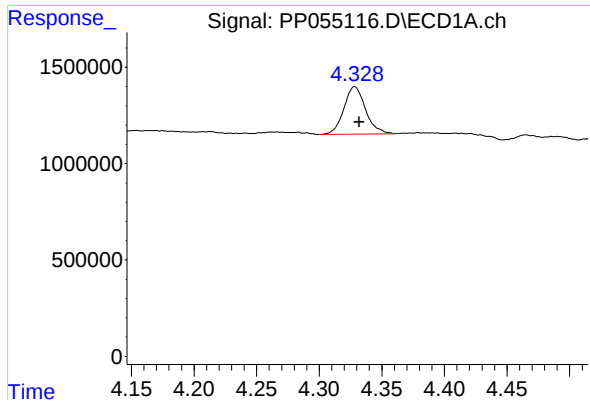


#1 Tetrachloro-m-xylene

R.T.: 4.328 min
Delta R.T.: -0.004 min
Response: 2963034
Conc: 1.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
DBA3342-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/31/2023
Supervised By :Ankita Jodhani 01/31/2023

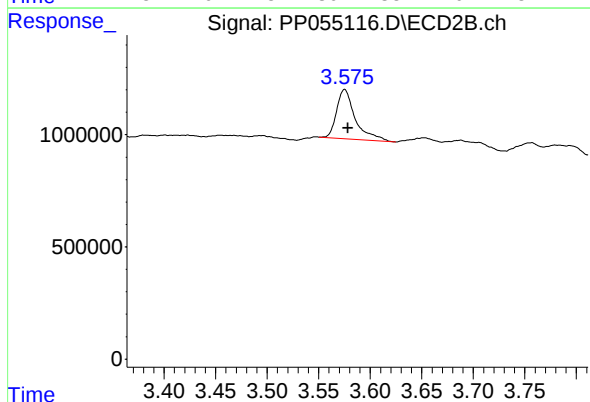


#1 Tetrachloro-m-xylene

R.T.: 3.575 min
Delta R.T.: -0.003 min
Response: 2754025
Conc: 1.83 ng/ml

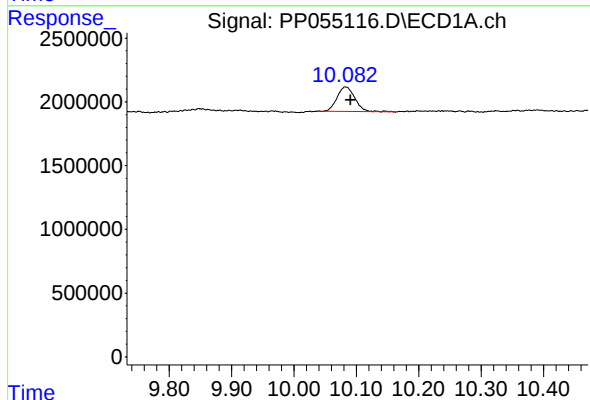

#2 Decachlorobiphenyl

R.T.: 10.083 min
Delta R.T.: -0.008 min
Response: 3806372
Conc: 2.20 ng/ml

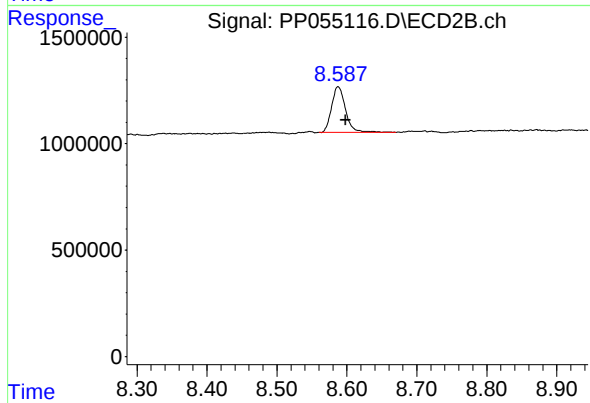

#2 Decachlorobiphenyl

R.T.: 8.588 min
Delta R.T.: -0.010 min
Response: 2944768
Conc: 2.18 ng/ml