

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP013119\
 Data File : PP029054.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jan 2019 23:22
 Operator : EI\MA
 Sample : K1282-08
 Misc : hexane
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 06:24:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012819.M
 Quant Title : 8080.M
 QLast Update : Mon Jan 28 11:24:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.019	12.165	66005136	88772676	260.688	215.569
Target Compounds							
1) T	Dalapon	0.000	2.959	0	241.9E6	N.D.	418.717 #
7) T	MCPA	12.994	12.998	34857138	1448687	62.326	0.976 #
8) T	DICHLORPROP	0.000	13.596	0	33537746	N.D.	87.699 #
10) T	Pentachlo...	14.278	0.000	19388043	0	2.881	N.D. #
12) T	2,4,5-T	0.000	15.905	0	20362874	N.D.	9.328 #
14) T	DINOSEB	17.742	0.000	3793319	0	1.657	N.D. #
15) T	Picloram	0.000	18.287	0	4113296	N.D.	1.196 #
16) T	DCPA	18.143	0.000	20970738	0	6.082	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP013119\
Data File : PP029054.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jan 2019 23:22
Operator : EI\MA
Sample : K1282-08
Misc : hexane
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 06:24:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012819.M
Quant Title : 8080.M
QLast Update : Mon Jan 28 11:24:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

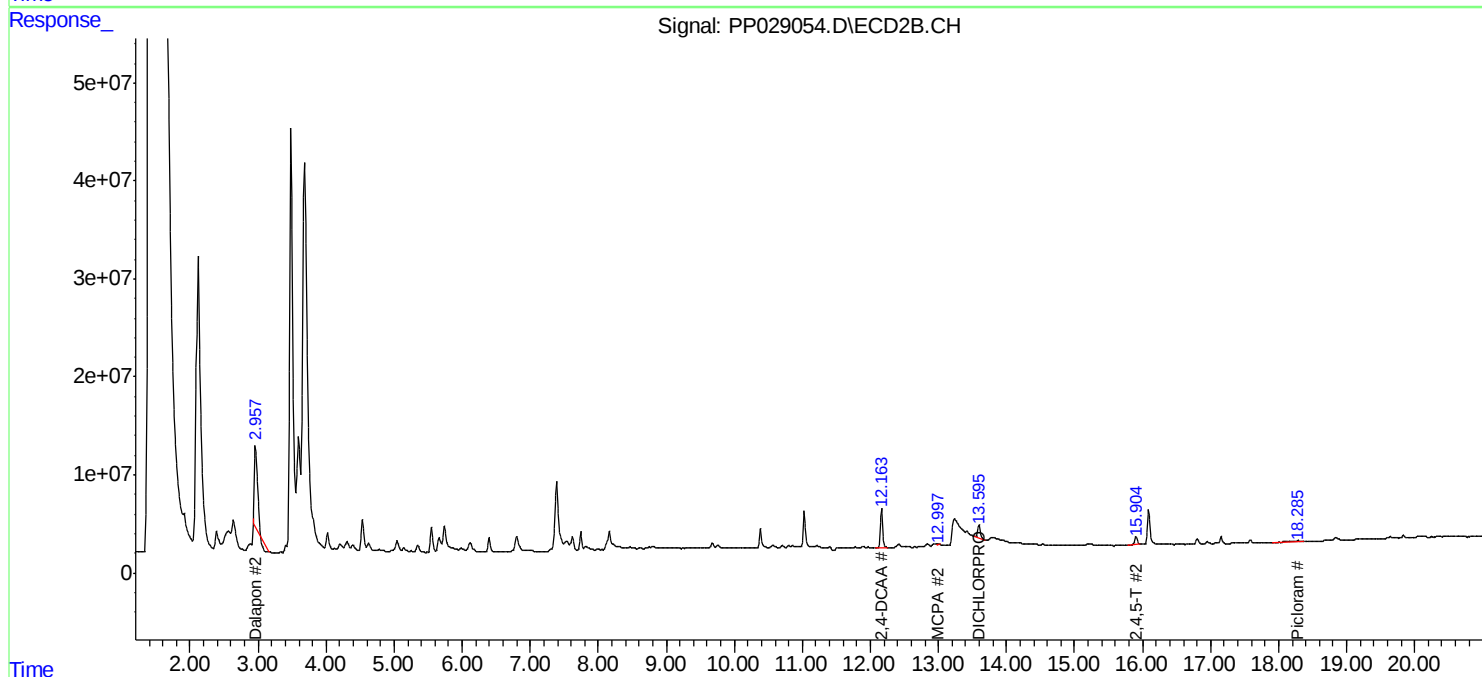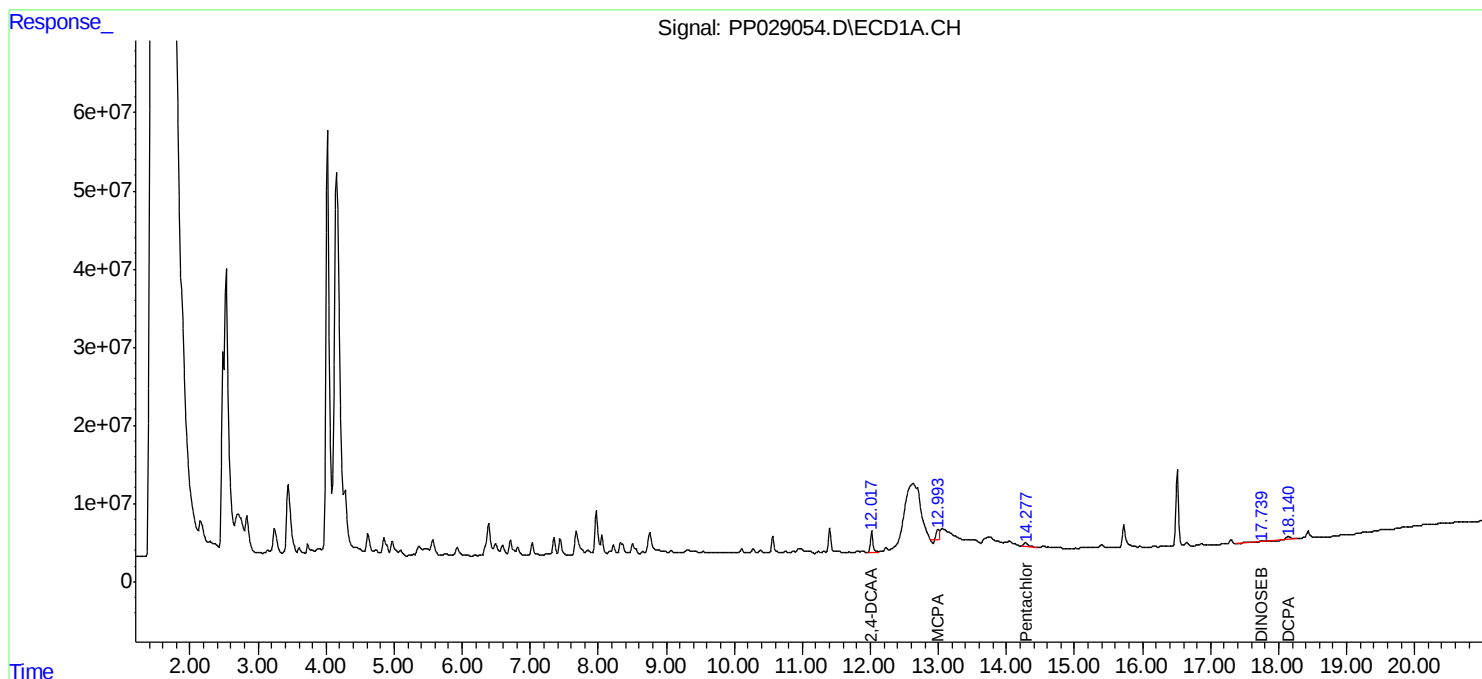


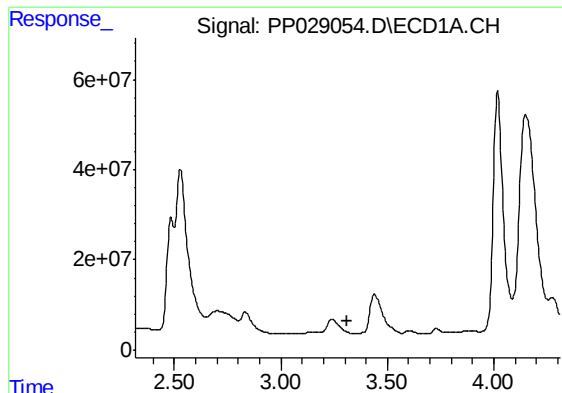

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP-2

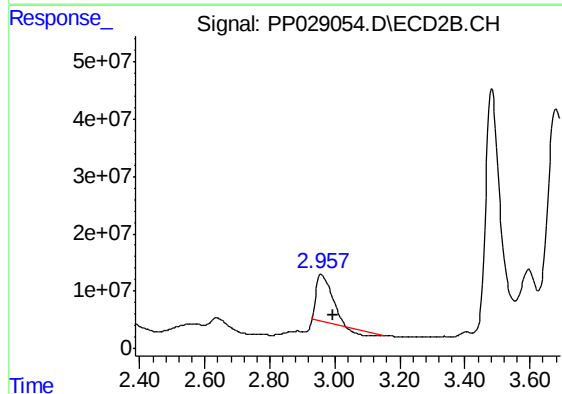


#1 Dalapon

R.T.: 2.959 min
Delta R.T.: -0.034 min
Response: 241914709
Conc: 418.72 ng/ml

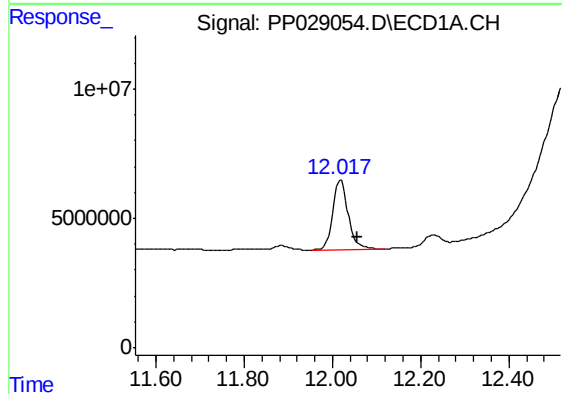


#4 2,4-DCAA

R.T.: 12.019 min
Delta R.T.: -0.039 min
Response: 66005136
Conc: 260.69 ng/ml

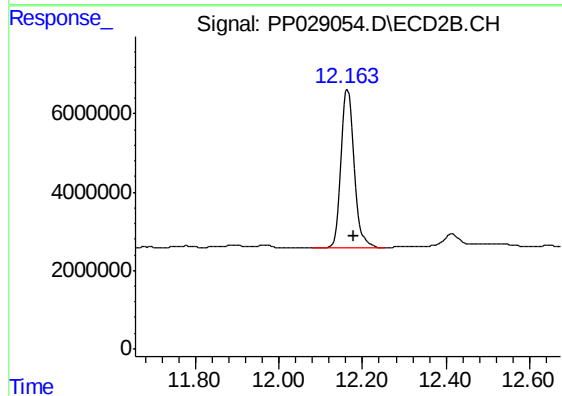

#4 2,4-DCAA


R.T.: 12.165 min
Delta R.T.: -0.013 min
Response: 88772676
Conc: 215.57 ng/ml

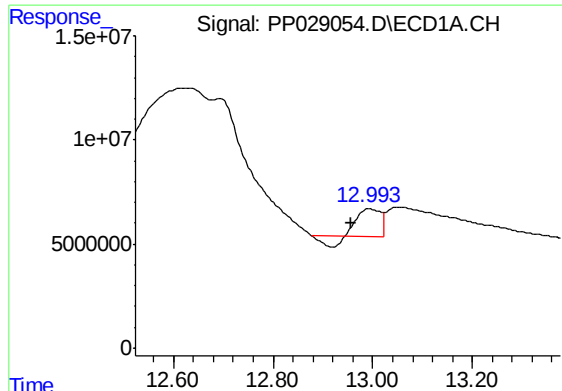

#7 MCPA


R.T.: 12.994 min
Delta R.T.: 0.037 min
Response: 34857138
Conc: 62.33 ug/ml

Instrument :
ECD_P
ClientSampleId :
TP-2

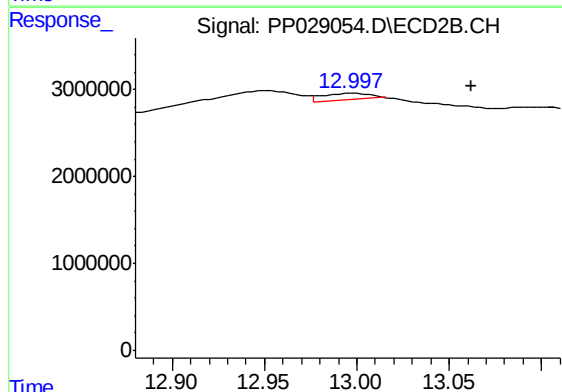


#7 MCPA

R.T.: 12.998 min
Delta R.T.: -0.064 min
Response: 1448687
Conc: 0.98 ug/ml

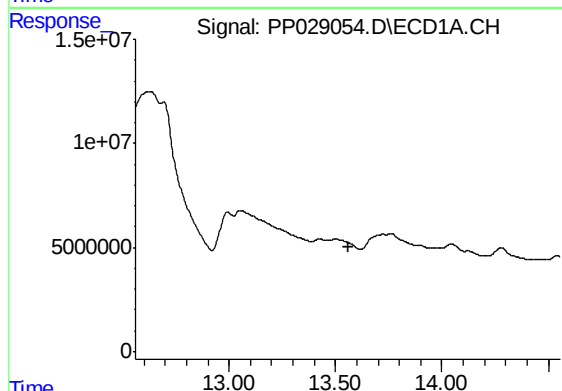


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.559 min
Response: 0
Conc: N.D.

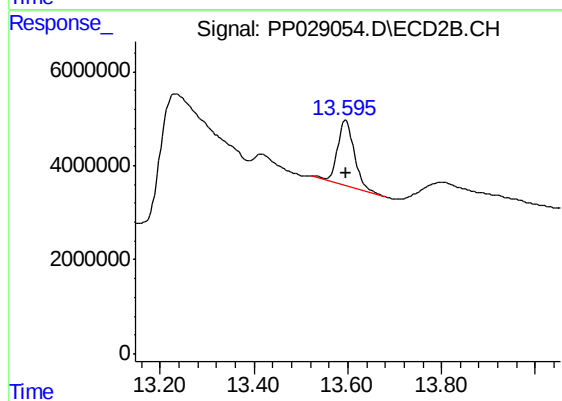

#8 DICHLORPROP


R.T.: 13.596 min
Delta R.T.: 0.000 min
Response: 33537746
Conc: 87.70 ng/ml

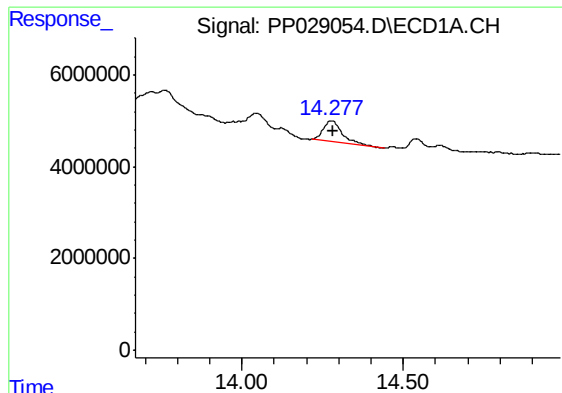

#10 Pentachlorophenol


R.T.: 14.278 min
Delta R.T.: -0.004 min
Response: 19388043
Conc: 2.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-2

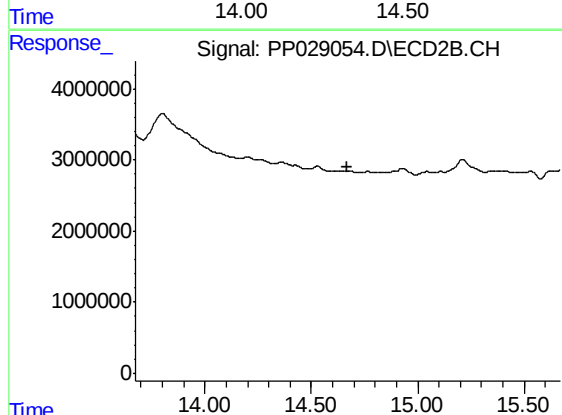


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 14.672 min
Response: 0
Conc: N.D.

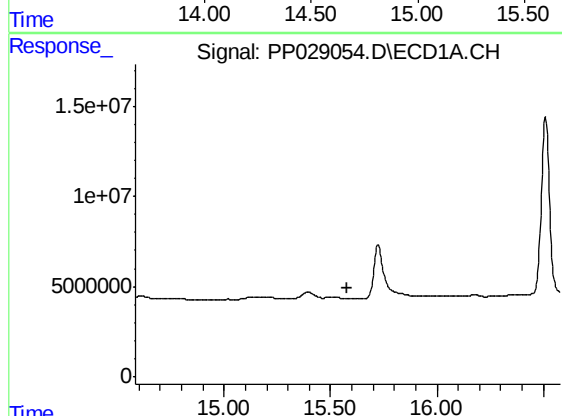


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 15.581 min
Response: 0
Conc: N.D.

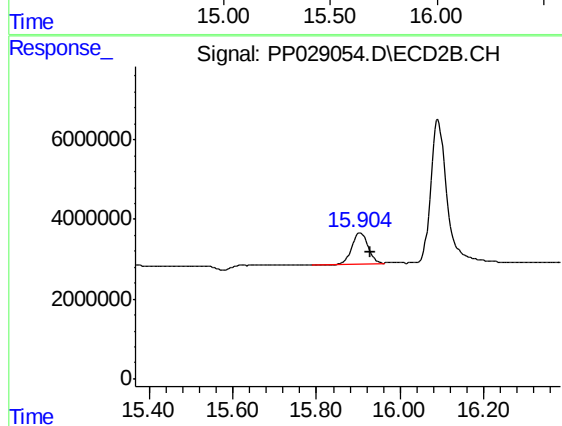

#12 2,4,5-T


R.T.: 15.905 min
Delta R.T.: -0.025 min
Response: 20362874
Conc: 9.33 ng/ml

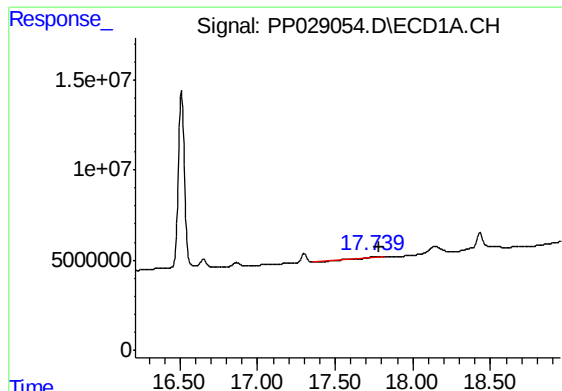

#14 DINOSEB


R.T.: 17.742 min
Delta R.T.: -0.042 min
Response: 3793319
Conc: 1.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-2

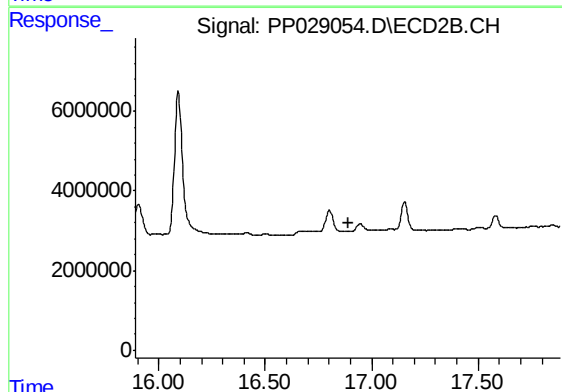


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.889 min
Response: 0
Conc: N.D.

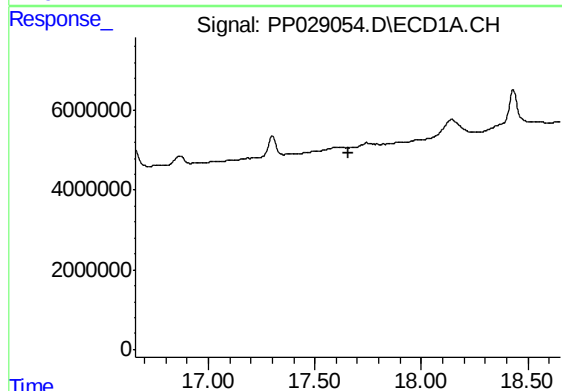


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.657 min
Response: 0
Conc: N.D.

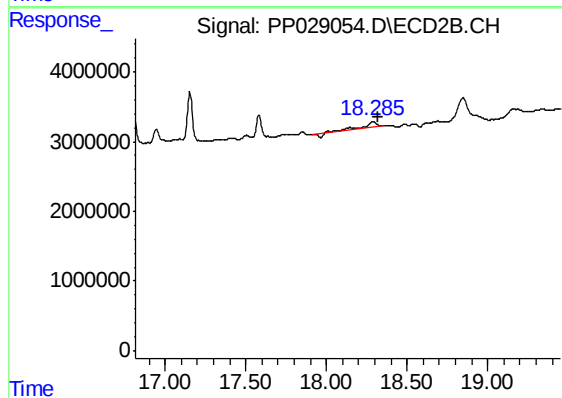

#15 Picloram


R.T.: 18.287 min
Delta R.T.: -0.029 min
Response: 4113296
Conc: 1.20 ng/ml

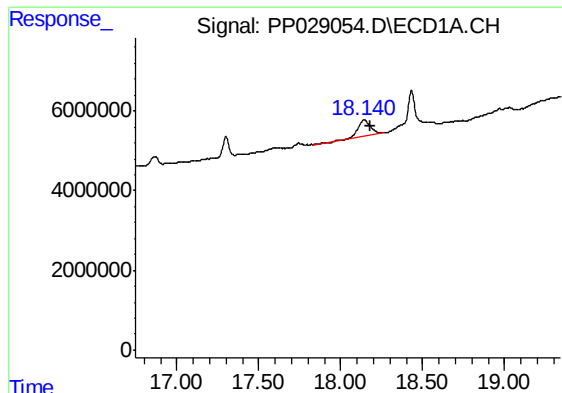

#16 DCPA

R.T.: 18.143 min
Delta R.T.: -0.034 min
Response: 20970738
Conc: 6.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-2

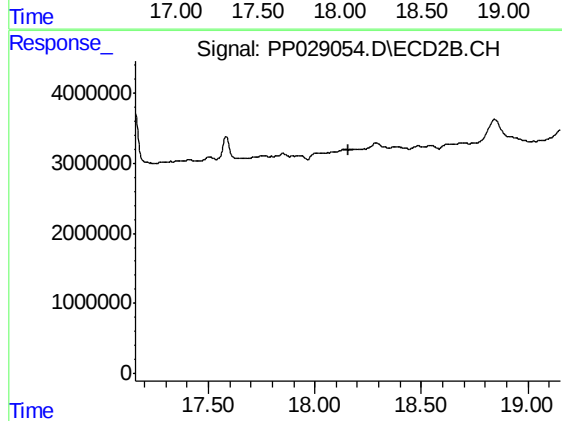

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.157 min
Response: 0
Conc: N.D.