

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP013122\
 Data File : PP043361.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Jan 2022 17:00
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 00:23:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 25 03:09:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.863	4.030	508078	519541	22.104	23.316
2)	SA Decachlor...	10.778	9.354	322307	462257	22.756	24.795
Target Compounds							
20)	L4 AR-1242-5	0.000	6.196f	0	10897	N.D.	17.043 #
25)	L5 AR-1248-5	0.000	6.196f	0	10897	N.D.	12.335 #
26)	L6 AR-1254-1	0.000	6.196f	0	10897	N.D.	7.684 #
30)	L6 AR-1254-5	8.419	0.000	8988	0	11.127	N.D. #
33)	L7 AR-1260-3	8.512f	0.000	3110	0	4.715	N.D. #
35)	L7 AR-1260-5	9.041	0.000	1859	0	1.408	N.D. #
36)	L8 AR-1262-1	8.512f	0.000	3110	0	3.130	N.D. #
37)	L8 AR-1262-2	9.041	0.000	1859	0	1.209	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP013122\
Data File : PP043361.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jan 2022 17:00
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 00:23:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

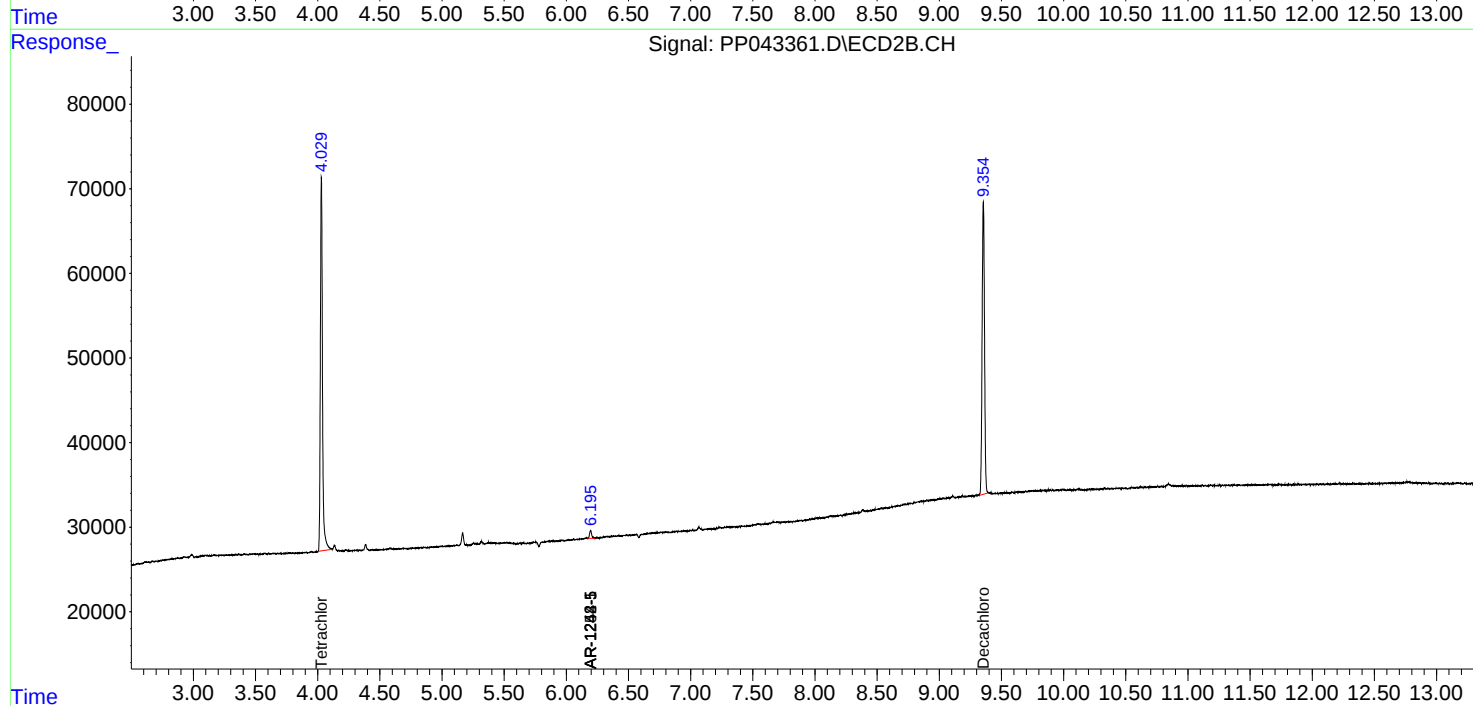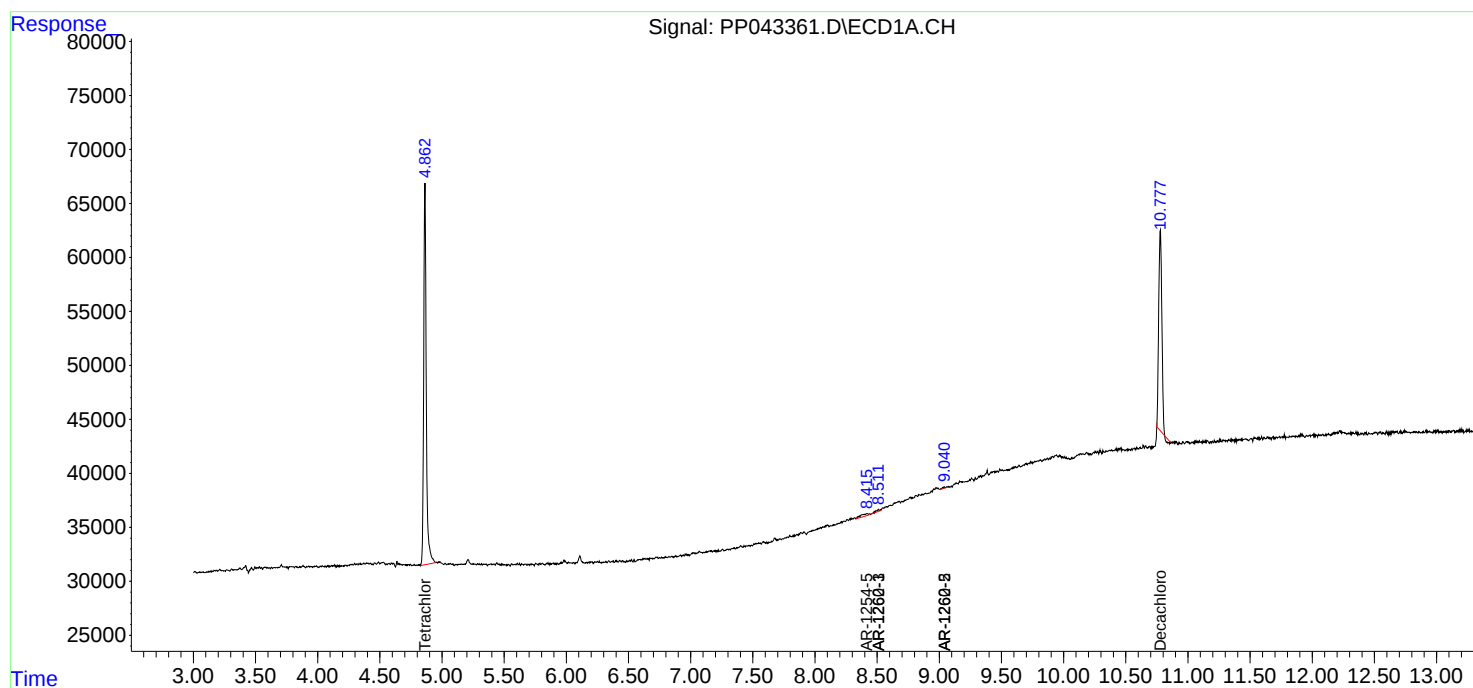


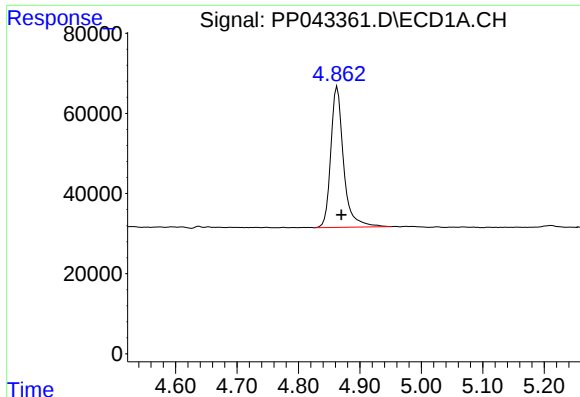

#1 Tetrachloro-m-xylene


R.T.: 4.863 min
Delta R.T.: -0.007 min
Response: 508078
Conc: 22.10 ng/ml

Instrument :
ECD_P
ClientSampleId :

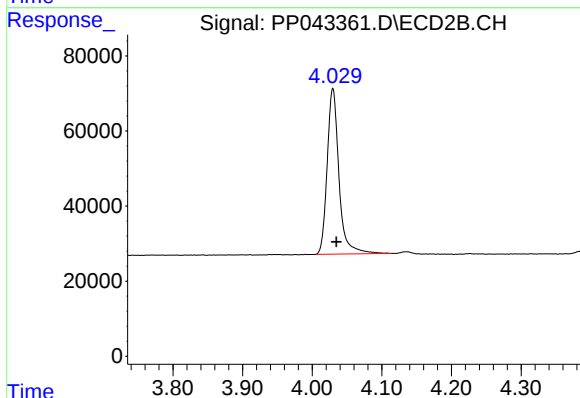


#1 Tetrachloro-m-xylene

R.T.: 4.030 min
Delta R.T.: -0.005 min
Response: 519541
Conc: 23.32 ng/ml

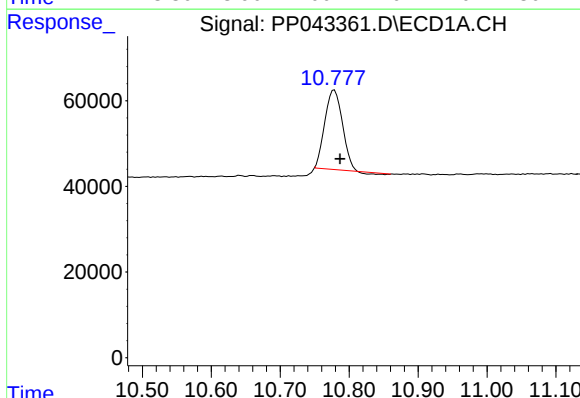


#2 Decachlorobiphenyl

R.T.: 10.778 min
Delta R.T.: -0.009 min
Response: 322307
Conc: 22.76 ng/ml

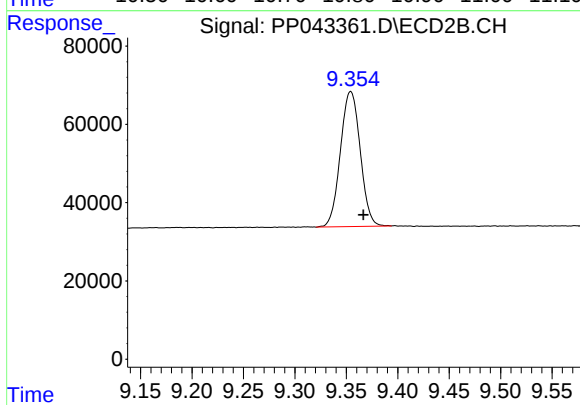

#2 Decachlorobiphenyl


R.T.: 9.354 min
Delta R.T.: -0.012 min
Response: 462257
Conc: 24.80 ng/ml

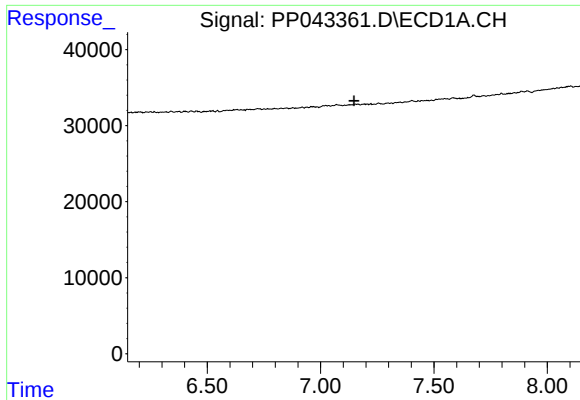

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.148 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

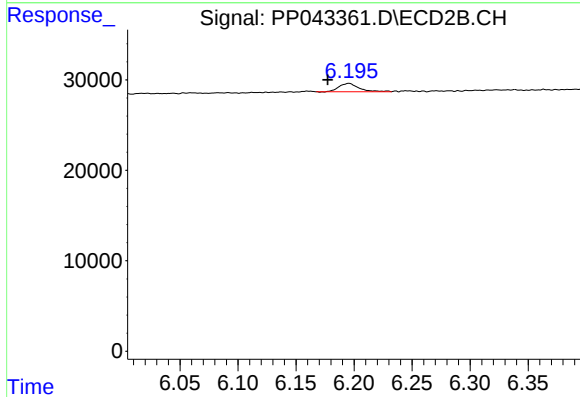


#20 AR-1242-5

R.T.: 6.196 min
Delta R.T.: 0.018 min
Response: 10897
Conc: 17.04 ng/ml

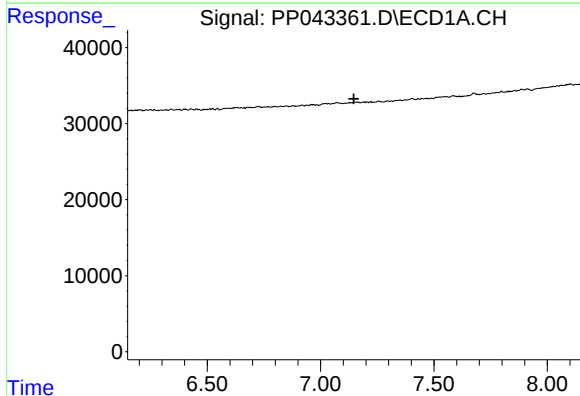


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 7.147 min
Response: 0
Conc: N.D.

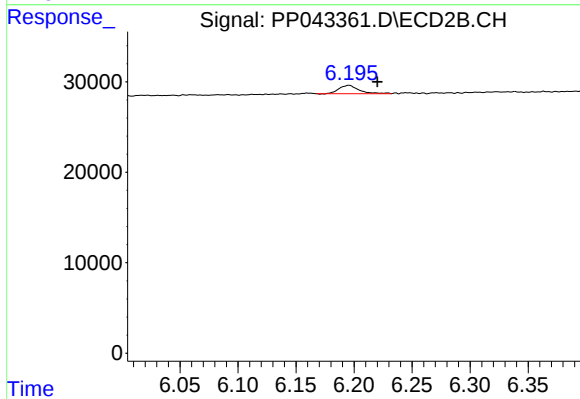

#25 AR-1248-5


R.T.: 6.196 min
Delta R.T.: -0.025 min
Response: 10897
Conc: 12.33 ng/ml

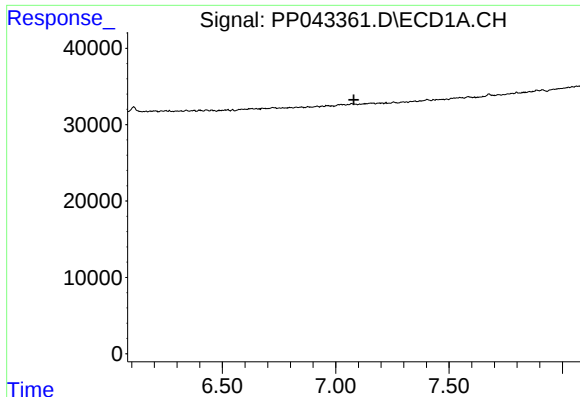

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 7.080 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

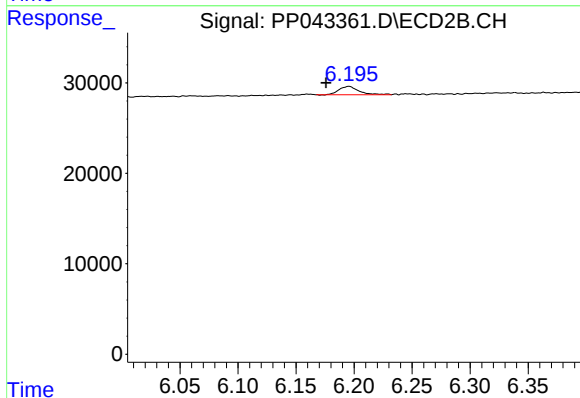


#26 AR-1254-1

R.T.: 6.196 min
Delta R.T.: 0.020 min
Response: 10897
Conc: 7.68 ng/ml

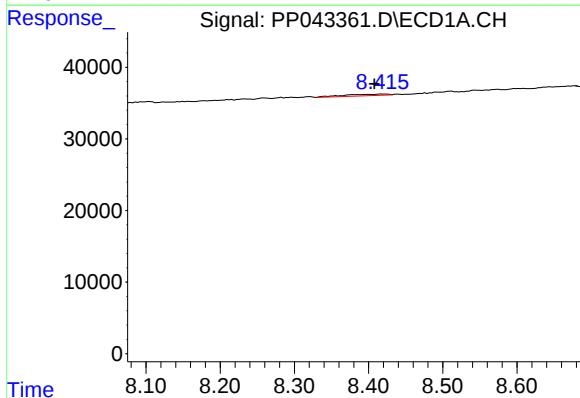


#30 AR-1254-5

R.T.: 8.419 min
Delta R.T.: 0.011 min
Response: 8988
Conc: 11.13 ng/ml

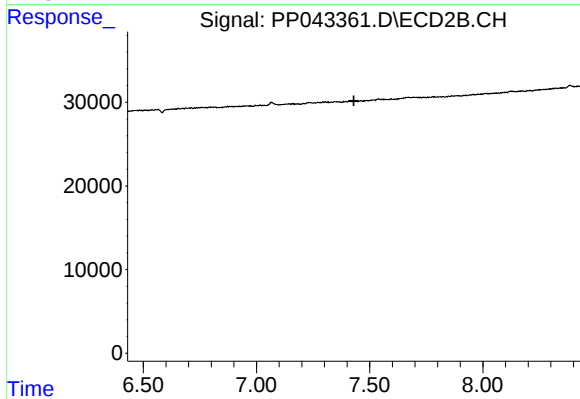

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

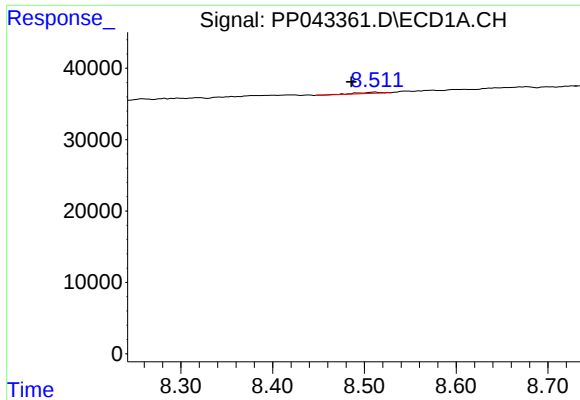

#33 AR-1260-3


R.T.: 8.512 min
Delta R.T.: 0.026 min
Response: 3110
Conc: 4.71 ng/ml

Instrument :
ECD_P
ClientSampleId :

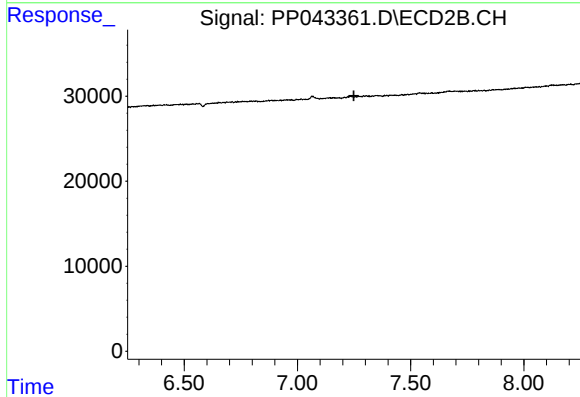


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.250 min
Response: 0
Conc: N.D.

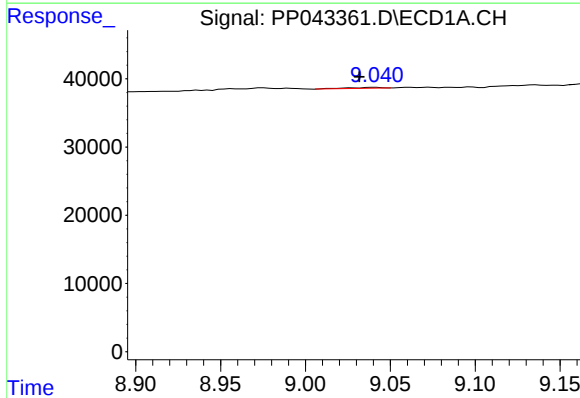


#35 AR-1260-5

R.T.: 9.041 min
Delta R.T.: 0.009 min
Response: 1859
Conc: 1.41 ng/ml

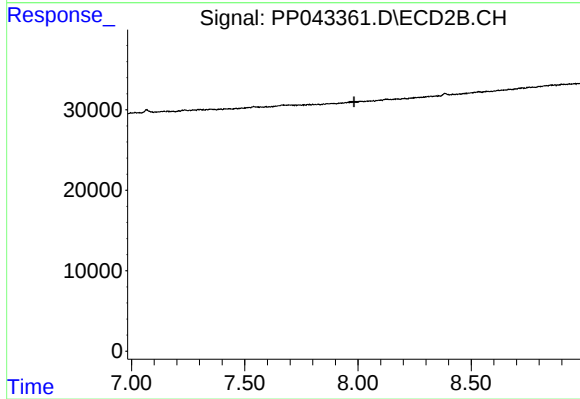

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.982 min
Response: 0
Conc: N.D.

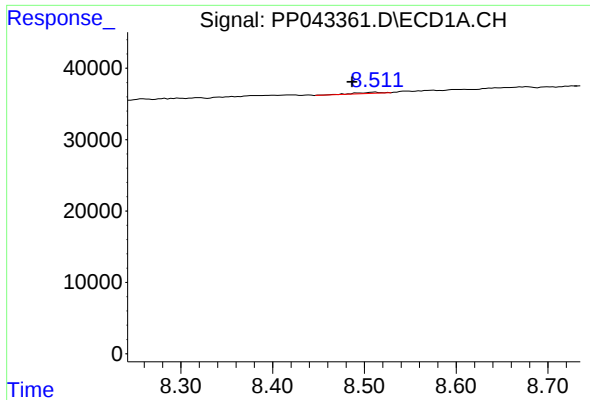

#36 AR-1262-1


R.T.: 8.512 min
Delta R.T.: 0.026 min
Response: 3110
Conc: 3.13 ng/ml

Instrument :
ECD_P
ClientSampleId :

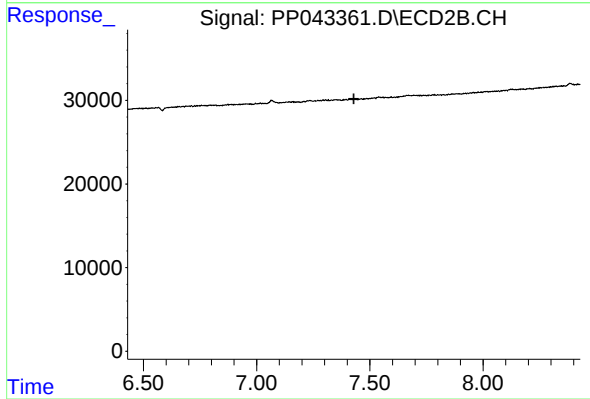


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.429 min
Response: 0
Conc: N.D.

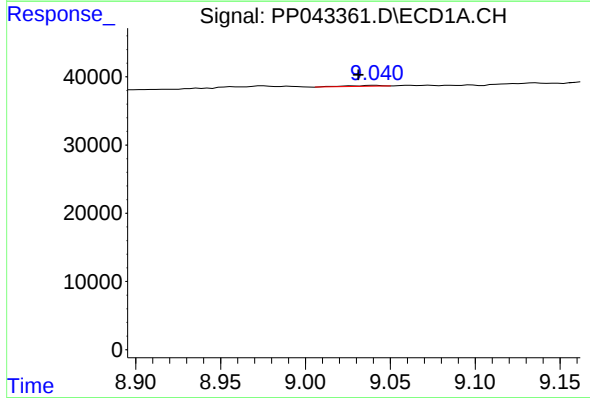

#37 AR-1262-2

R.T.: 9.041 min
Delta R.T.: 0.010 min
Response: 1859
Conc: 1.21 ng/ml

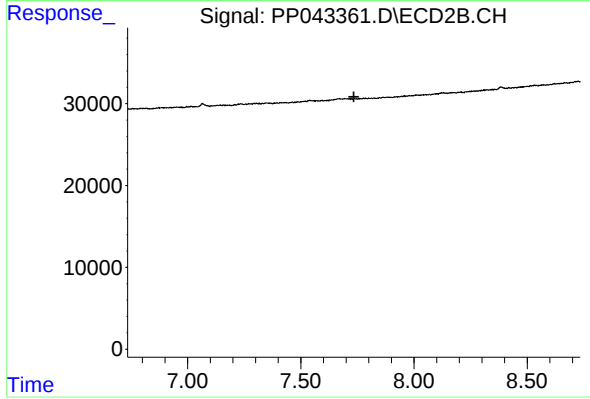

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.735 min
Response: 0
Conc: N.D.