

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP013122\
 Data File : PP043368.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Jan 2022 18:56
 Operator : AJ\MA
 Sample : N1335-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 00:28:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 25 03:09:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.864	4.030	498695	492005	21.696	22.081
2)	SA Decachlor...	10.778	9.354	322058	430613	22.739	23.098
Target Compounds							
8)	L2 AR-1221-1	5.104	0.000	26008	0	104.146	N.D. #
9)	L2 AR-1221-2	5.210	4.384	3344	14717	17.437	61.198 #
10)	L2 AR-1221-3	0.000	4.486	0	482	N.D.	0.672 #
11)	L3 AR-1232-1	0.000	4.486	0	482	N.D.	0.821 #
14)	L3 AR-1232-4	0.000	5.631f	0	6512	N.D.	26.979 #
19)	L4 AR-1242-4	0.000	5.631f	0	6512	N.D.	13.027 #
23)	L5 AR-1248-3	0.000	5.631f	0	6512	N.D.	8.529 #
32)	L7 AR-1260-2	8.101f	0.000	13684	0	16.073	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP013122\
Data File : PP043368.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jan 2022 18:56
Operator : AJ\MA
Sample : N1335-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 00:28:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

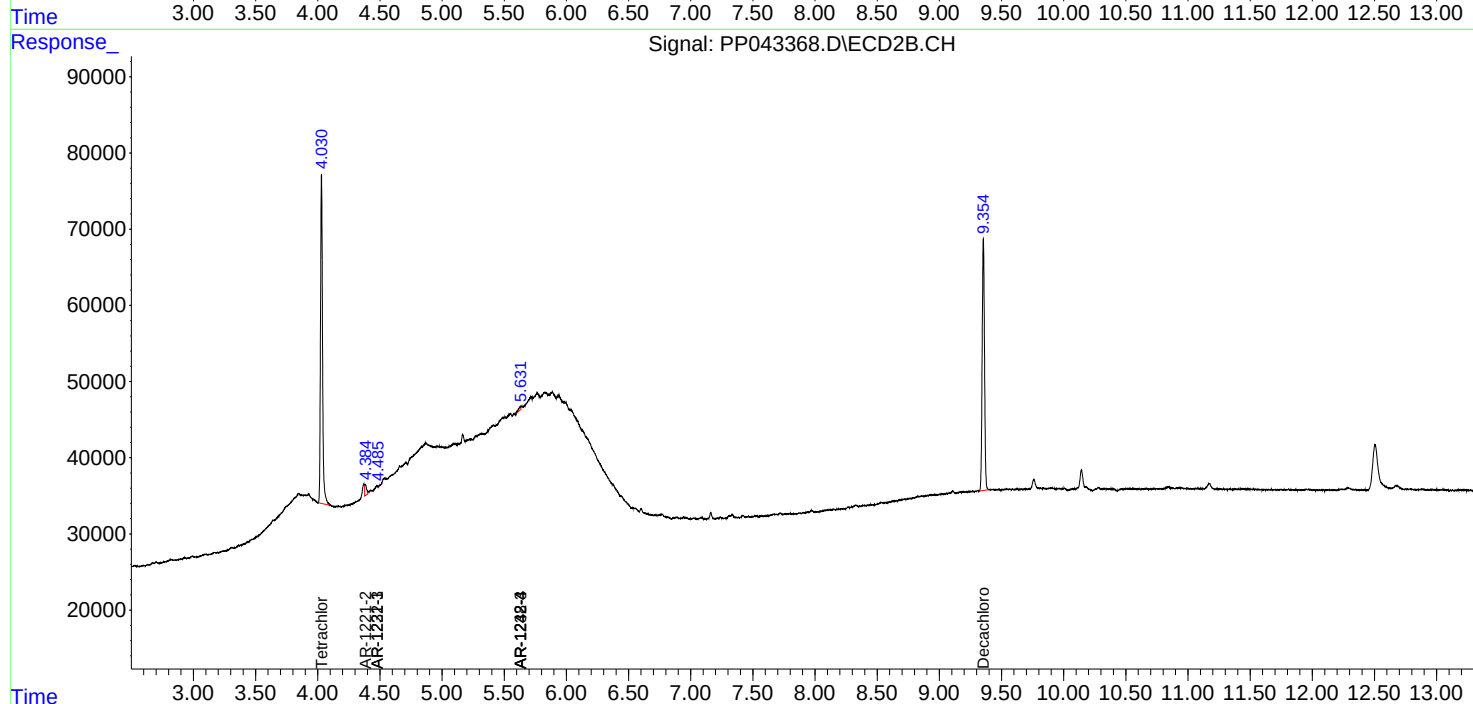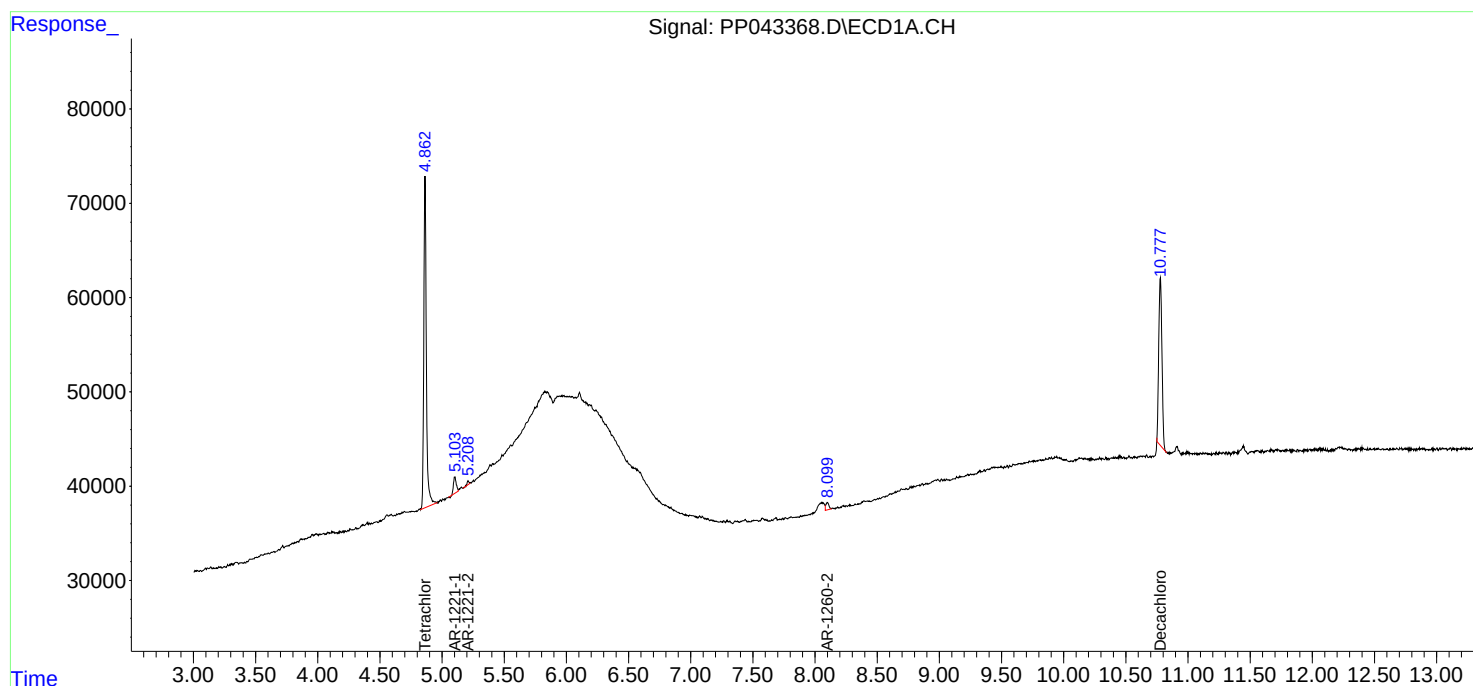


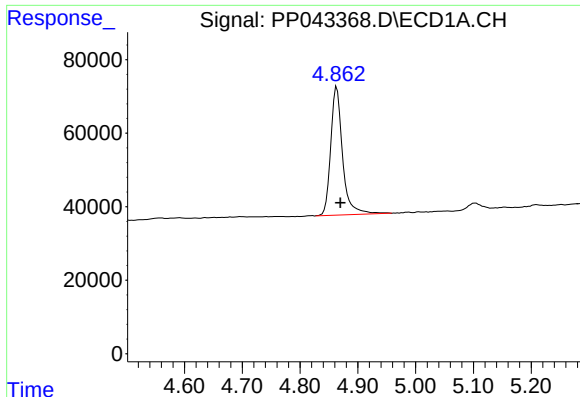

#1 Tetrachloro-m-xylene


R.T.: 4.864 min
Delta R.T.: -0.006 min
Response: 498695
Conc: 21.70 ng/ml

Instrument :
ECD_P
ClientSampleId :

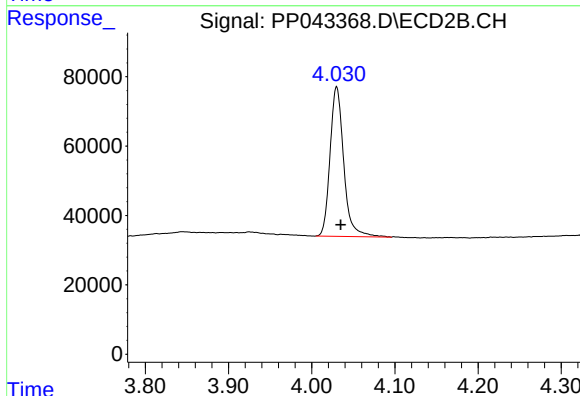


#1 Tetrachloro-m-xylene

R.T.: 4.030 min
Delta R.T.: -0.005 min
Response: 492005
Conc: 22.08 ng/ml

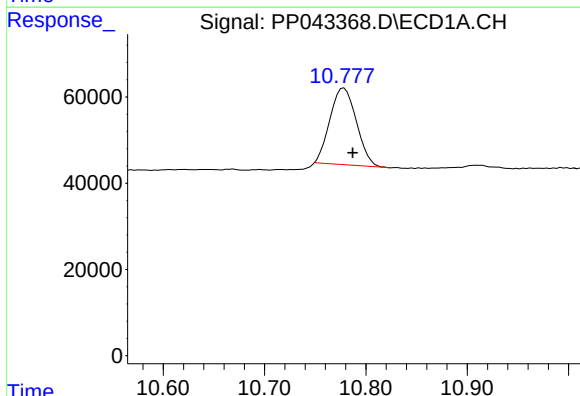


#2 Decachlorobiphenyl

R.T.: 10.778 min
Delta R.T.: -0.009 min
Response: 322058
Conc: 22.74 ng/ml

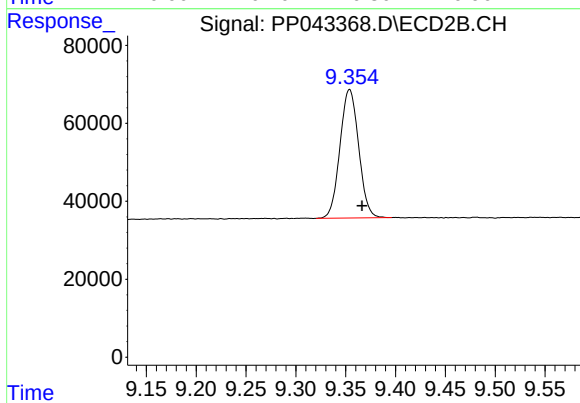

#2 Decachlorobiphenyl


R.T.: 9.354 min
Delta R.T.: -0.012 min
Response: 430613
Conc: 23.10 ng/ml

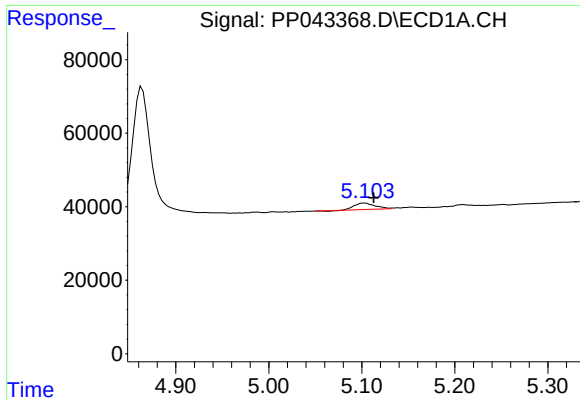

#8 AR-1221-1


R.T.: 5.104 min
Delta R.T.: -0.009 min
Response: 26008
Conc: 104.15 ng/ml

Instrument :
ECD_P
ClientSampleId :

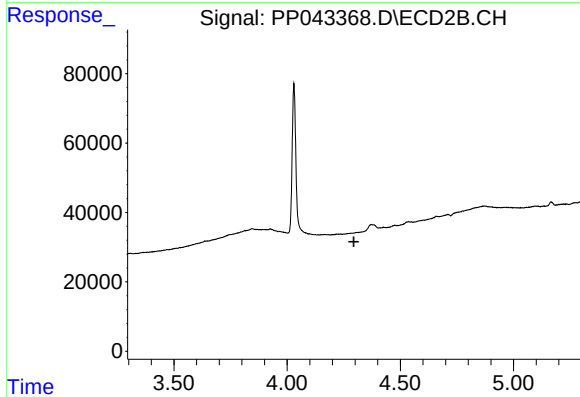


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.295 min
Response: 0
Conc: N.D.

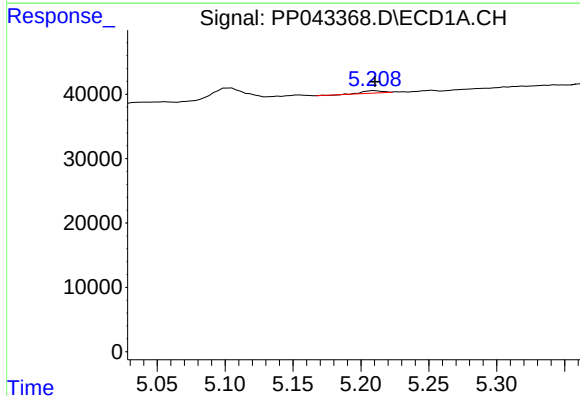


#9 AR-1221-2

R.T.: 5.210 min
Delta R.T.: 0.000 min
Response: 3344
Conc: 17.44 ng/ml

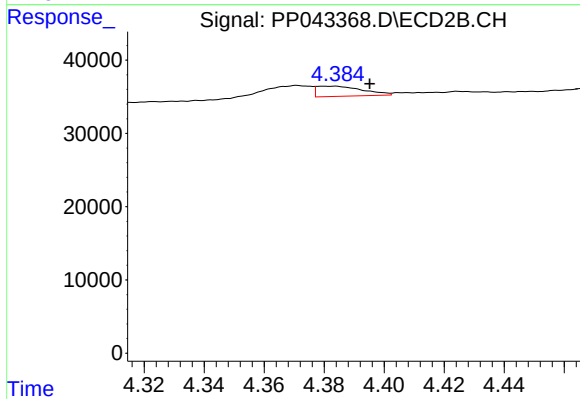

#9 AR-1221-2


R.T.: 4.384 min
Delta R.T.: -0.011 min
Response: 14717
Conc: 61.20 ng/ml

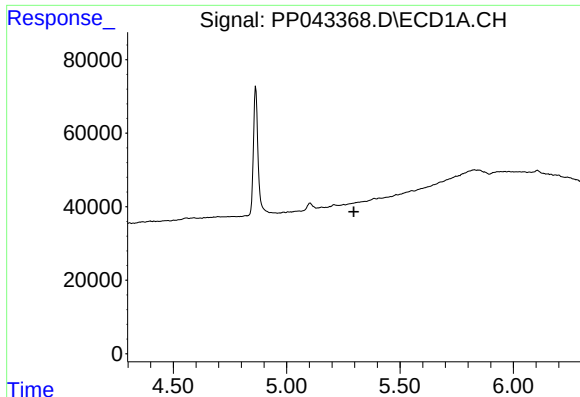

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 5.296 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

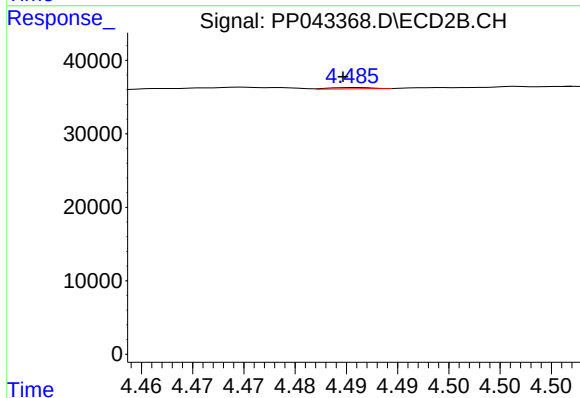


#10 AR-1221-3

R.T.: 4.486 min
Delta R.T.: 0.001 min
Response: 482
Conc: 0.67 ng/ml

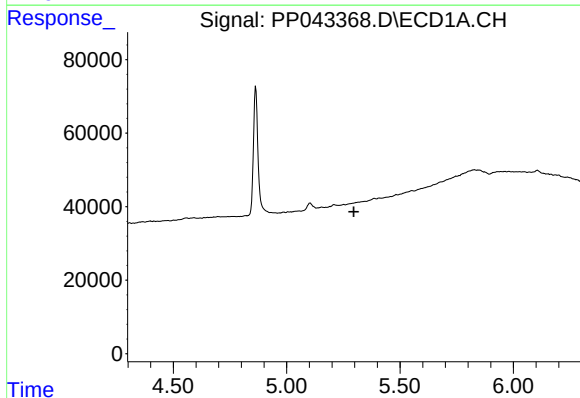


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.296 min
Response: 0
Conc: N.D.

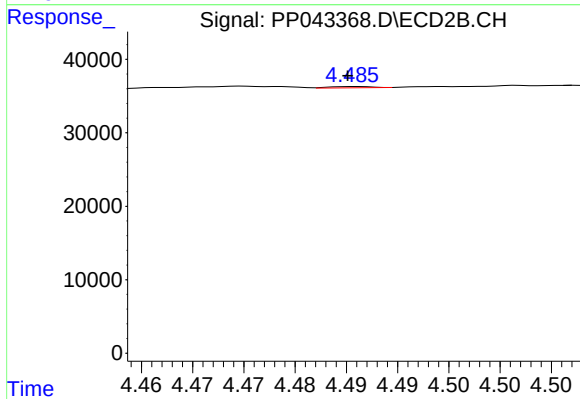

#11 AR-1232-1


R.T.: 4.486 min
Delta R.T.: 0.000 min
Response: 482
Conc: 0.82 ng/ml

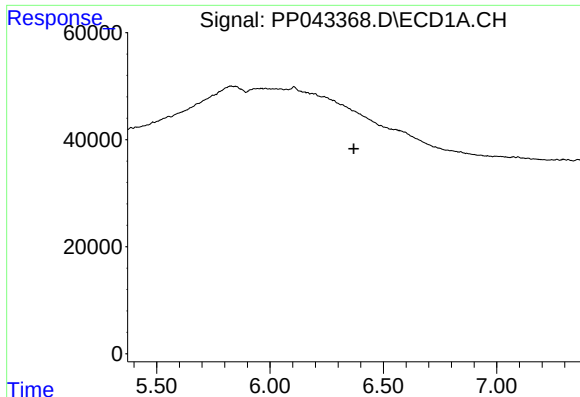

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T.: 6.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

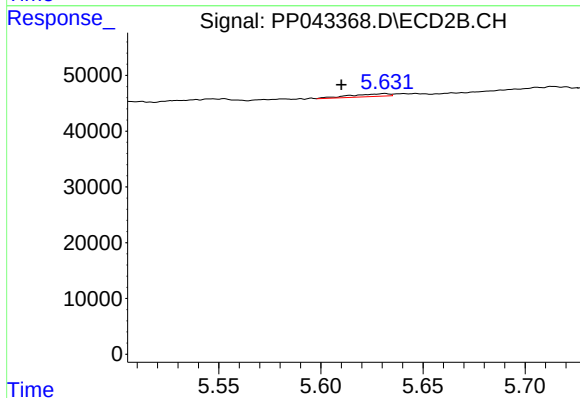


#14 AR-1232-4

R.T.: 5.631 min
Delta R.T.: 0.021 min
Response: 6512
Conc: 26.98 ng/ml

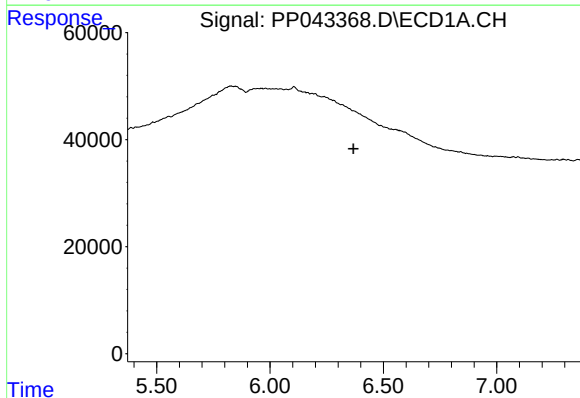


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 6.368 min
Response: 0
Conc: N.D.

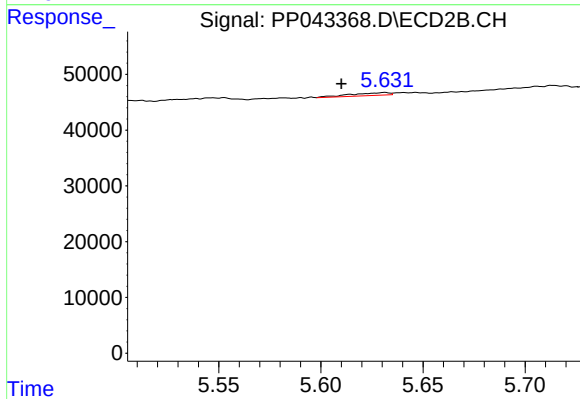

#19 AR-1242-4


R.T.: 5.631 min
Delta R.T.: 0.021 min
Response: 6512
Conc: 13.03 ng/ml

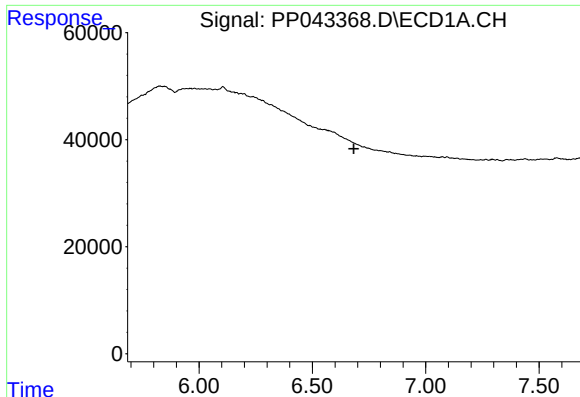

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 6.683 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

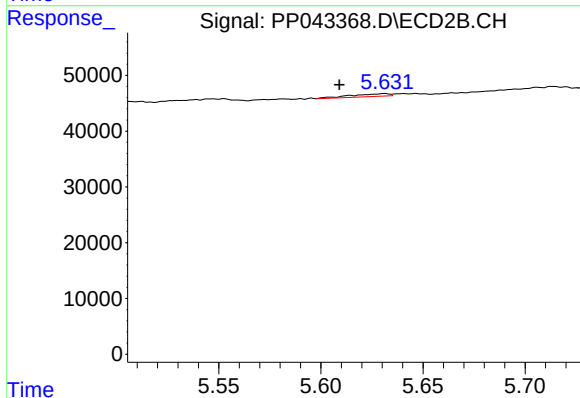


#23 AR-1248-3

R.T.: 5.631 min
Delta R.T.: 0.022 min
Response: 6512
Conc: 8.53 ng/ml

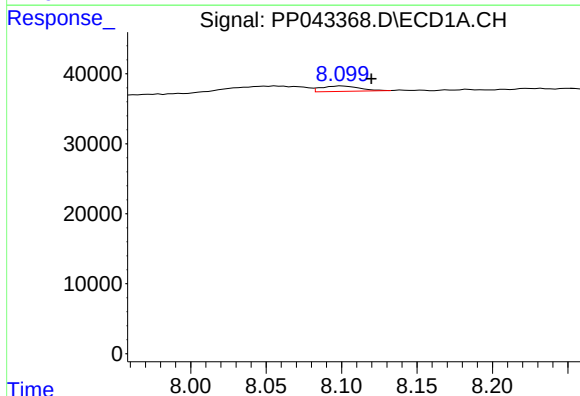

#32 AR-1260-2

R.T.: 8.101 min
Delta R.T.: -0.019 min
Response: 13684
Conc: 16.07 ng/ml

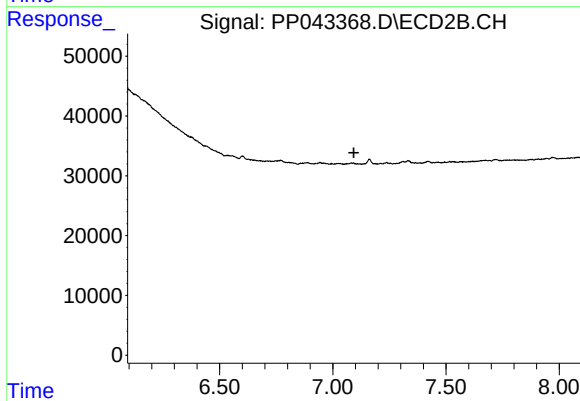

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.093 min
Response: 0
Conc: N.D.