

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP013122\
 Data File : PP043378.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Jan 2022 22:23
 Operator : AJ\MA
 Sample : N1332-02 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 00:35:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 25 03:09:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.864	4.030	47486	47296	2.066	2.123
2)	SA Decachlor...	10.781	9.353	31909	46540	2.253	2.496
Target Compounds							
10)	L2 AR-1221-3	0.000	4.479	0	10551	N.D.	14.703 #
11)	L3 AR-1232-1	0.000	4.479	0	10551	N.D.	17.953 #
29)	L6 AR-1254-4	7.961f	0.000	29912	0	42.435	N.D. #
30)	L6 AR-1254-5	8.402	7.427	6681	1140	8.271	0.738 #
32)	L7 AR-1260-2	8.094f	0.000	11964	0	14.052	N.D. #
35)	L7 AR-1260-5	0.000	7.963f	0	14429	N.D.	6.521 #
36)	L8 AR-1262-1	0.000	7.427	0	1140	N.D.	1.362 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP013122\
Data File : PP043378.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jan 2022 22:23
Operator : AJ\MA
Sample : N1332-02 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 00:35:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

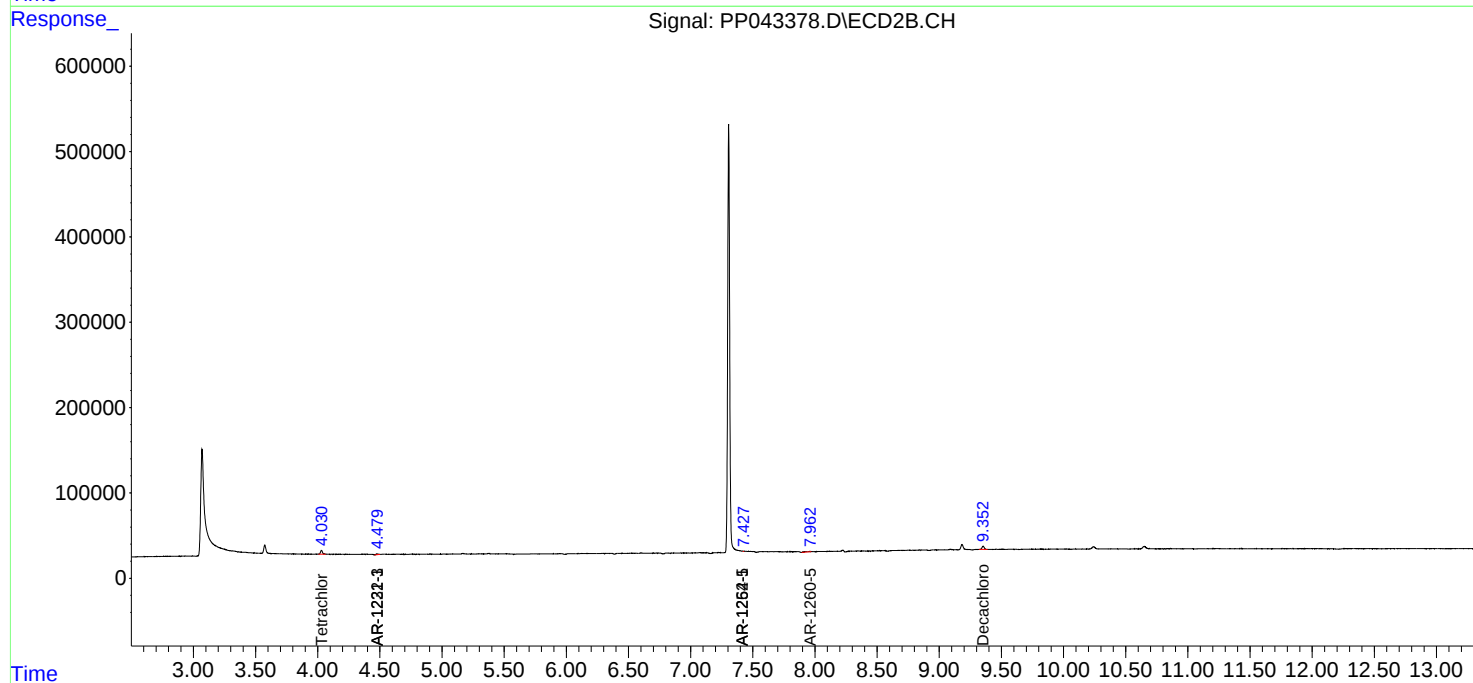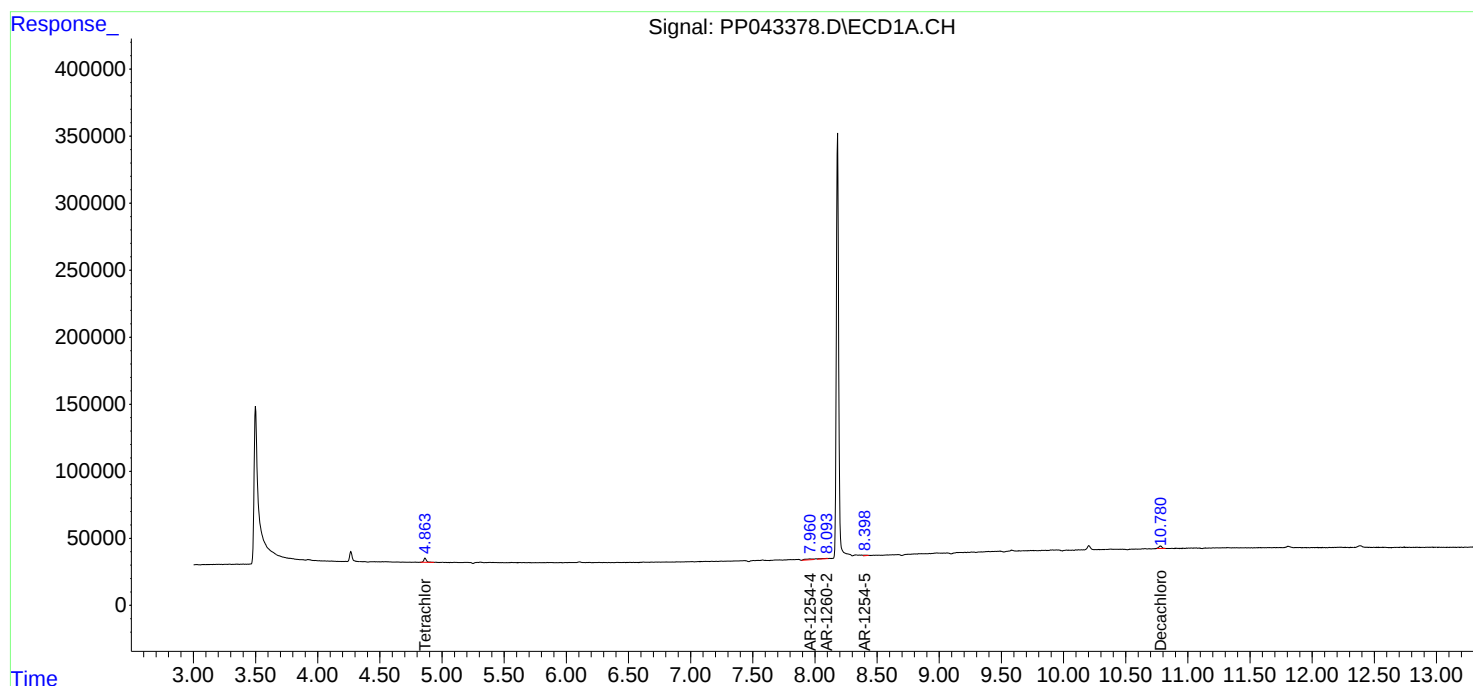


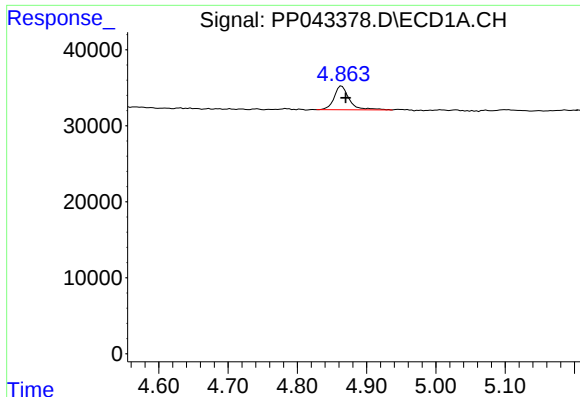

#1 Tetrachloro-m-xylene


R.T.: 4.864 min
Delta R.T.: -0.006 min
Response: 47486
Conc: 2.07 ng/ml

Instrument :
ECD_P
ClientSampleId :

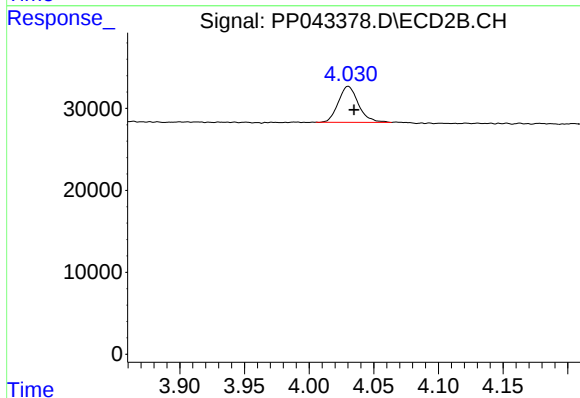


#1 Tetrachloro-m-xylene

R.T.: 4.030 min
Delta R.T.: -0.005 min
Response: 47296
Conc: 2.12 ng/ml

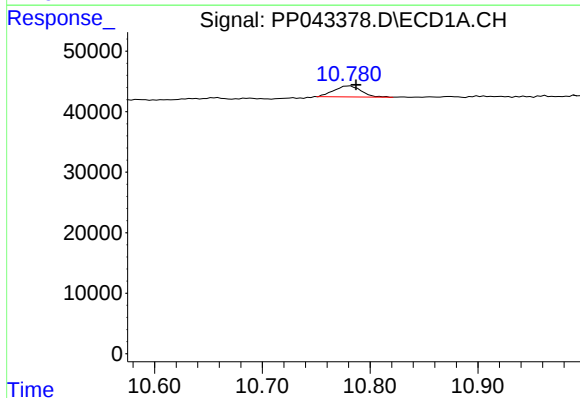


#2 Decachlorobiphenyl

R.T.: 10.781 min
Delta R.T.: -0.006 min
Response: 31909
Conc: 2.25 ng/ml

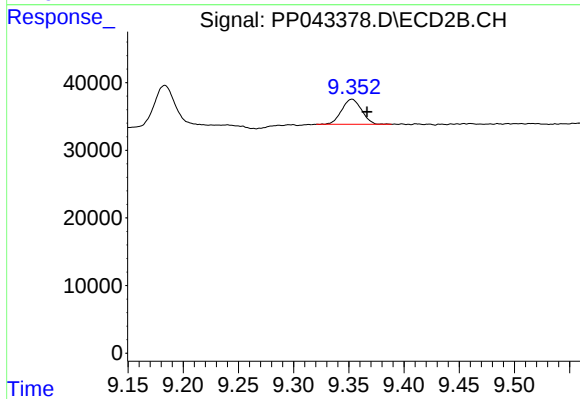

#2 Decachlorobiphenyl


R.T.: 9.353 min
Delta R.T.: -0.014 min
Response: 46540
Conc: 2.50 ng/ml

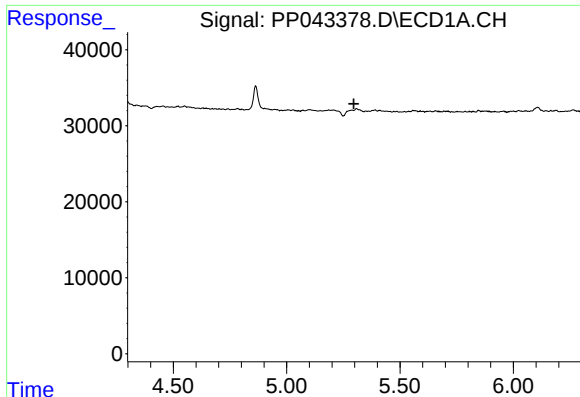

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 5.296 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

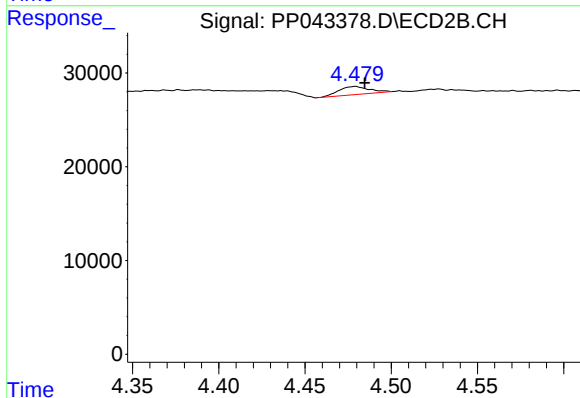


#10 AR-1221-3

R.T.: 4.479 min
Delta R.T.: -0.005 min
Response: 10551
Conc: 14.70 ng/ml

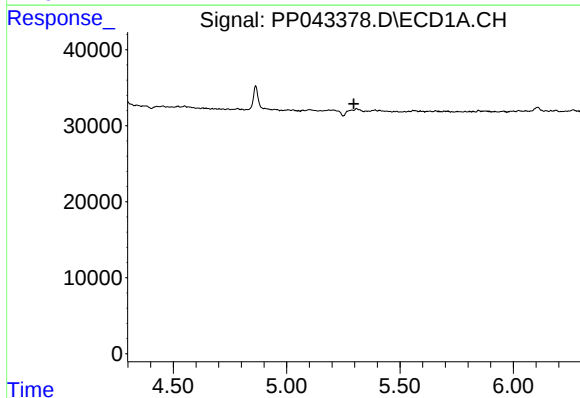


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.296 min
Response: 0
Conc: N.D.

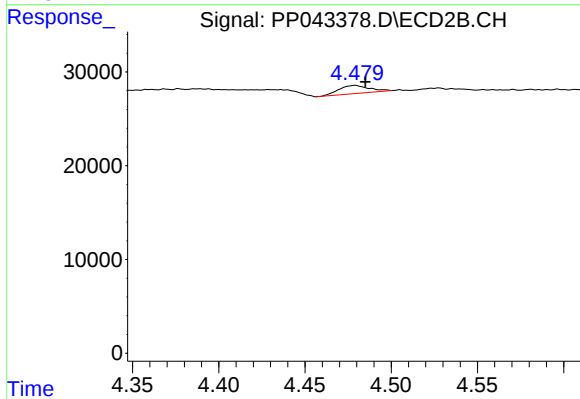

#11 AR-1232-1


R.T.: 4.479 min
Delta R.T.: -0.006 min
Response: 10551
Conc: 17.95 ng/ml

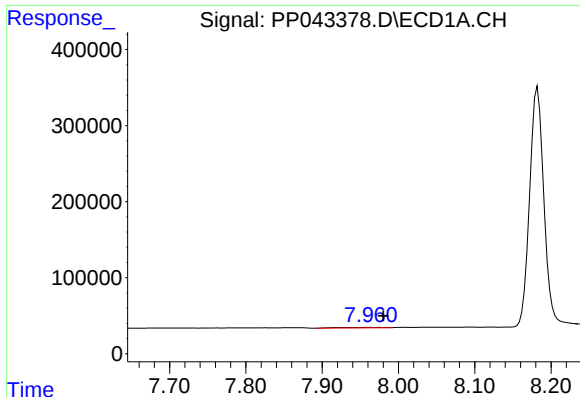

#29 AR-1254-4


R.T.: 7.961 min
Delta R.T.: -0.019 min
Response: 29912
Conc: 42.43 ng/ml

Instrument :
ECD_P
ClientSampleId :

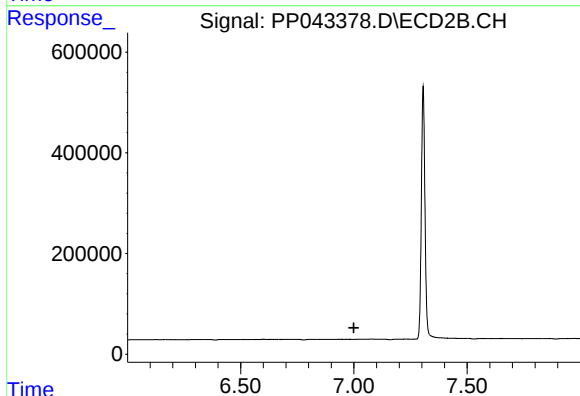


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.000 min
Response: 0
Conc: N.D.

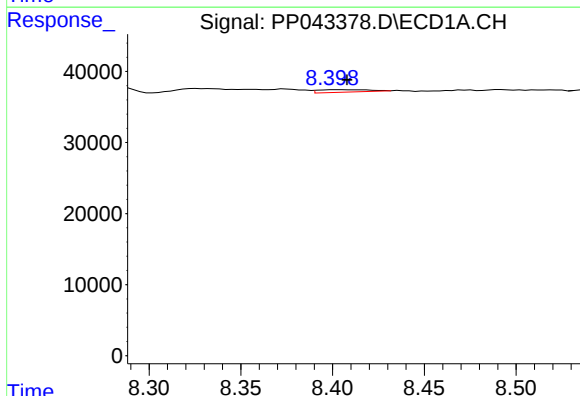


#30 AR-1254-5

R.T.: 8.402 min
Delta R.T.: -0.006 min
Response: 6681
Conc: 8.27 ng/ml

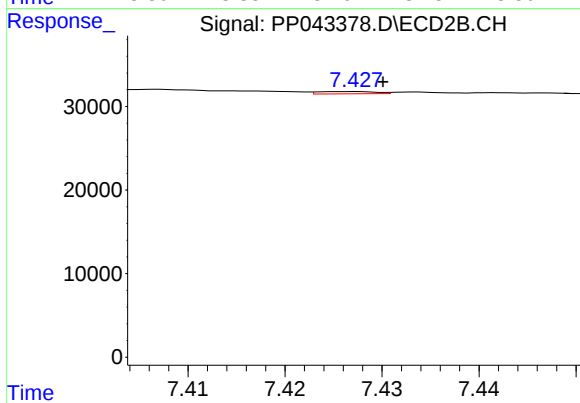

#30 AR-1254-5


R.T.: 7.427 min
Delta R.T.: -0.003 min
Response: 1140
Conc: 0.74 ng/ml

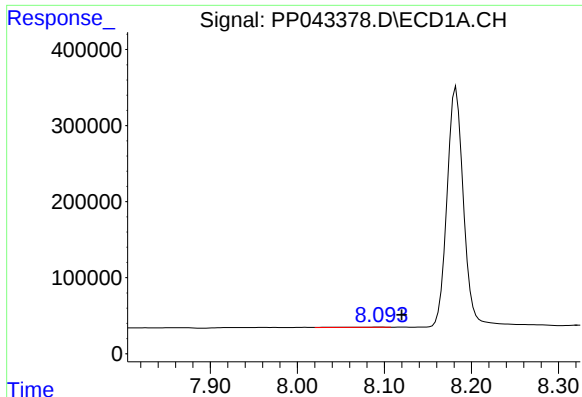

#32 AR-1260-2


R.T.: 8.094 min
Delta R.T.: -0.026 min
Response: 11964
Conc: 14.05 ng/ml

Instrument :
ECD_P
ClientSampleId :

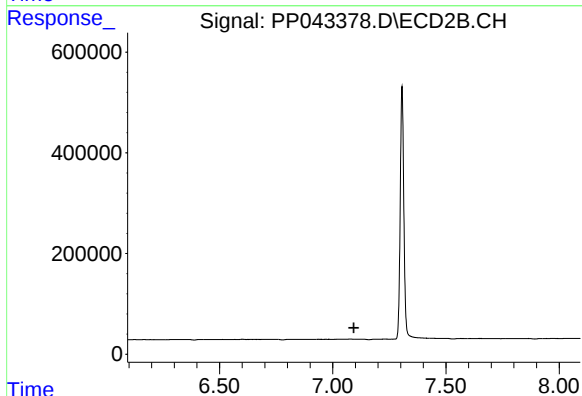


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.093 min
Response: 0
Conc: N.D.

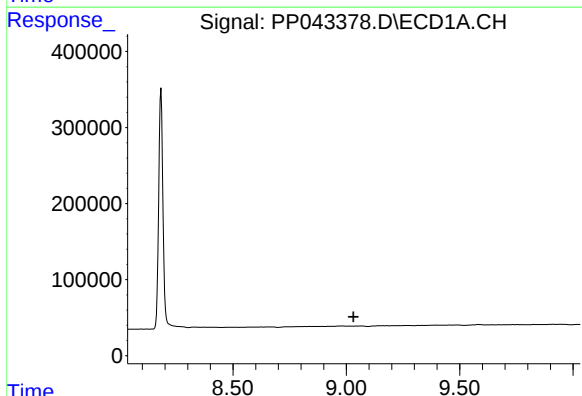


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 9.032 min
Response: 0
Conc: N.D.

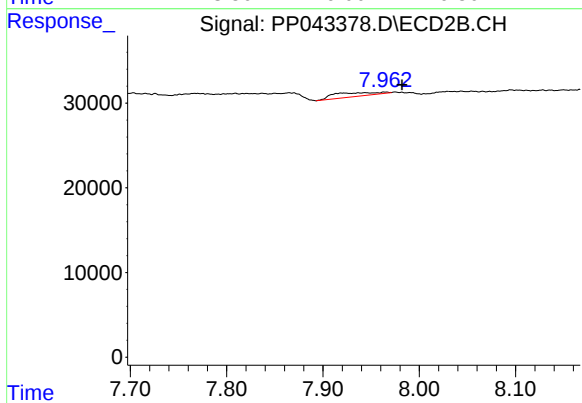

#35 AR-1260-5


R.T.: 7.963 min
Delta R.T.: -0.019 min
Response: 14429
Conc: 6.52 ng/ml

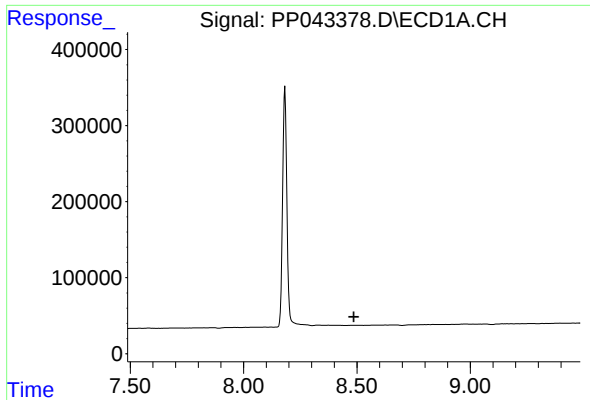

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 8.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

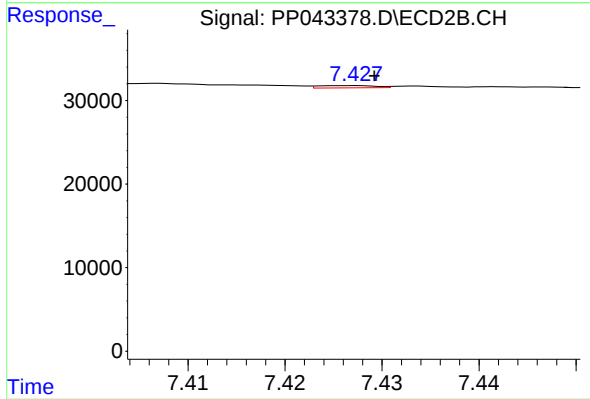

#36 AR-1262-1

R.T.: 7.427 min
Delta R.T.: -0.002 min
Response: 1140
Conc: 1.36 ng/ml