

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP013123\
 Data File : PP055141.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2023 13:35
 Operator : YP\AJ
 Sample : PB150573BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB150573BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/01/2023
 Supervised By :Ankita Jodhani 02/01/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 20:39:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 03:37:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.329	3.576	32821690	27757793	18.877	18.490
2) SA Decachlor...	10.083	8.587	37323697	31381077	21.554	23.236m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP013123\
Data File : PP055141.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2023 13:35
Operator : YP\AJ
Sample : PB150573BL
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB150573BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/01/2023
Supervised By :Ankita Jodhani 02/01/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 20:39:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 03:37:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

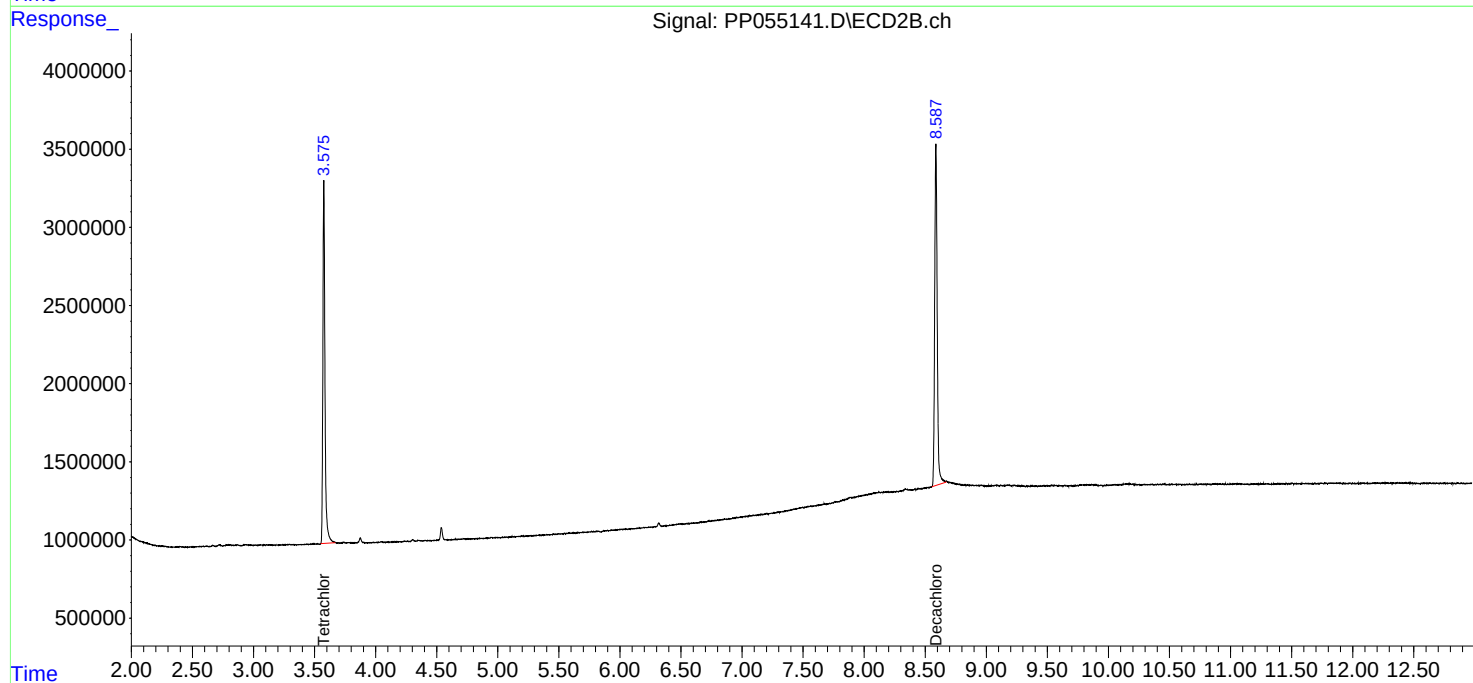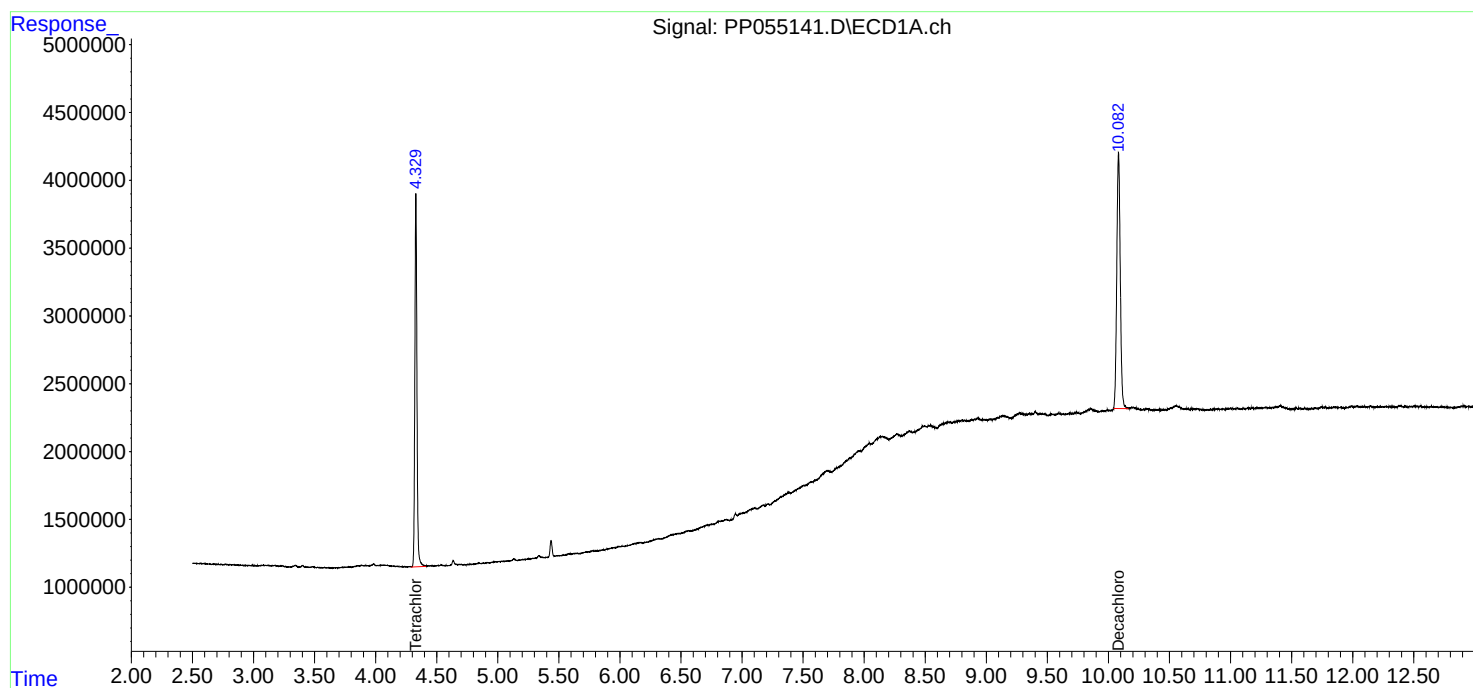

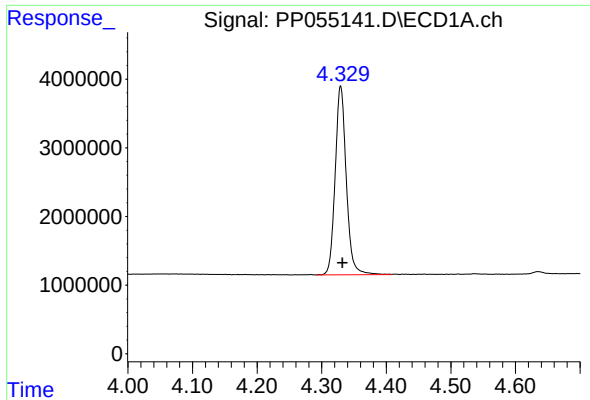


#1 Tetrachloro-m-xylene

R.T.: 4.329 min
Delta R.T.: -0.003 min
Response: 32821690
Conc: 18.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB150573BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/01/2023
Supervised By :Ankita Jodhani 02/01/2023

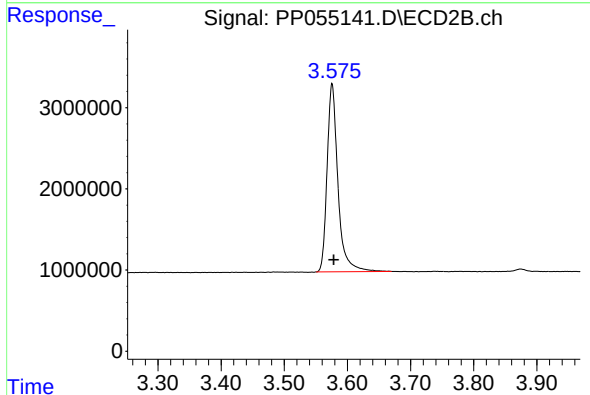


#1 Tetrachloro-m-xylene

R.T.: 3.576 min
Delta R.T.: -0.003 min
Response: 27757793
Conc: 18.49 ng/ml

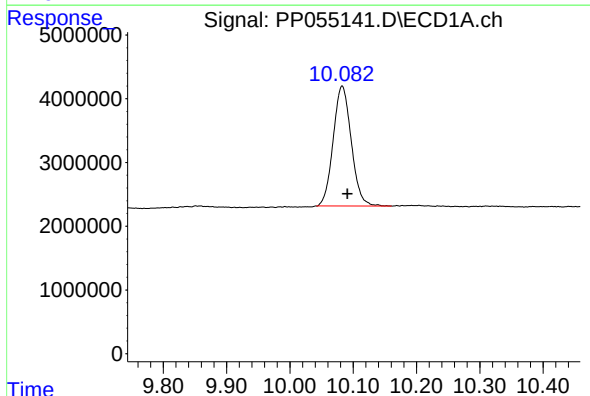

#2 Decachlorobiphenyl

R.T.: 10.083 min
Delta R.T.: -0.008 min
Response: 37323697
Conc: 21.55 ng/ml

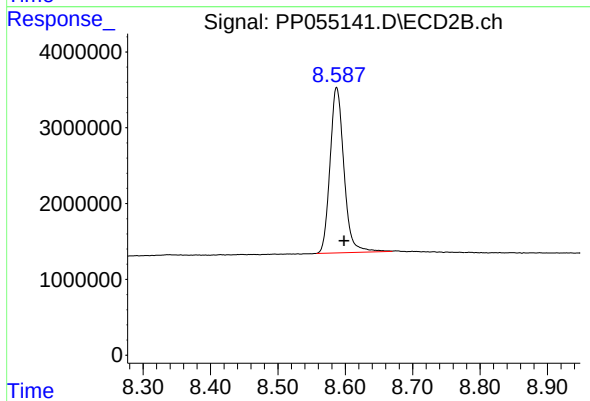

#2 Decachlorobiphenyl

R.T.: 8.587 min
Delta R.T.: -0.011 min
Response: 31381077
Conc: 23.24 ng/ml m