

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020122\
 Data File : PP043405.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Feb 2022 15:20
 Operator : AJ\MA
 Sample : N1338-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 00:13:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 25 03:09:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.862	4.028	469516	471972	20.426	21.182
2)	SA Decachlor...	10.773	9.351	353415	412844	24.953	22.145

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020122\
Data File : PP043405.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Feb 2022 15:20
Operator : AJ\MA
Sample : N1338-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 00:13:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

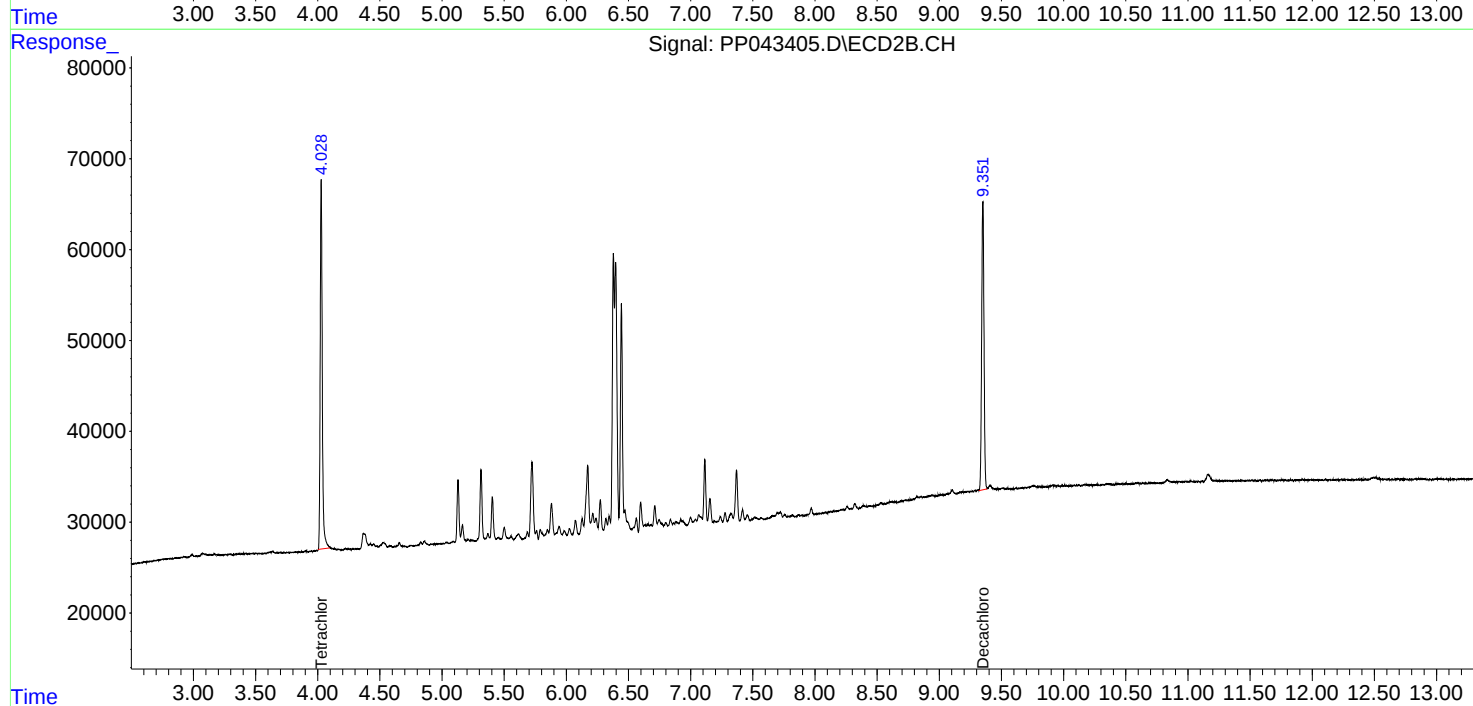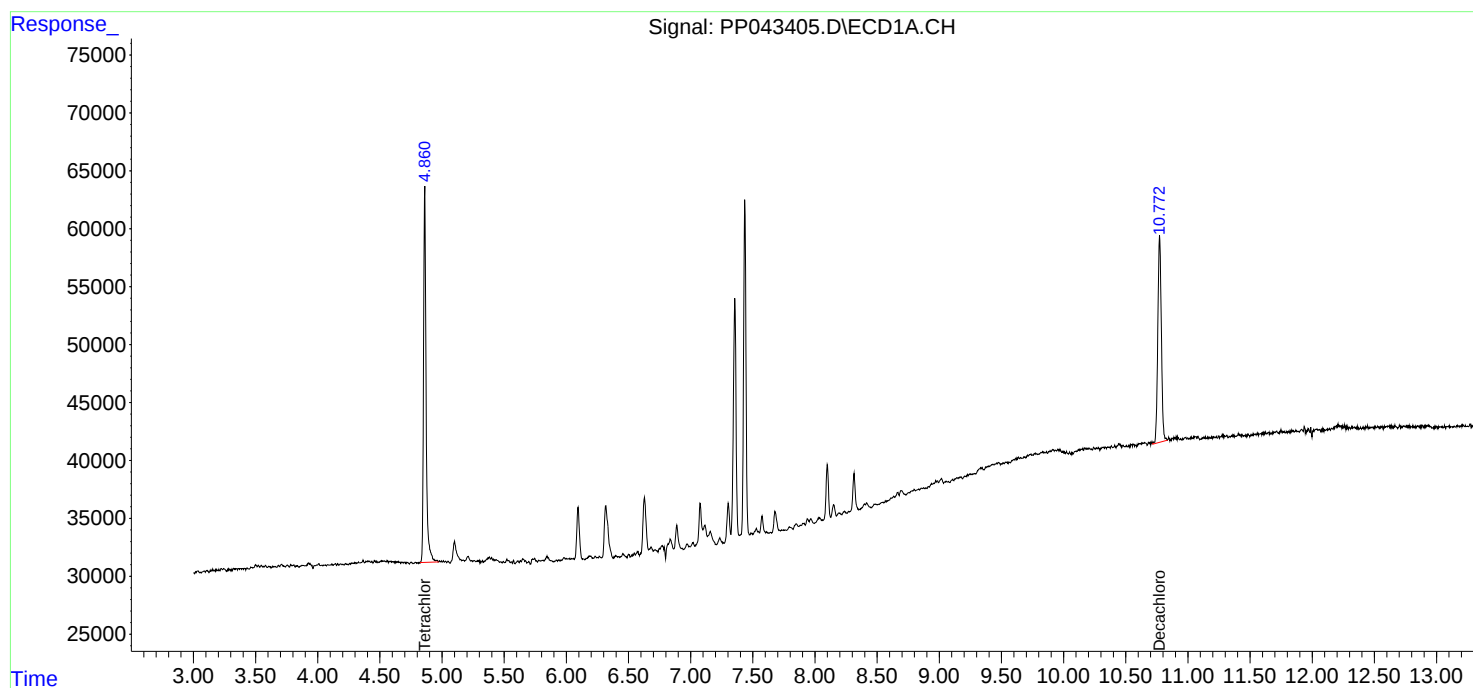


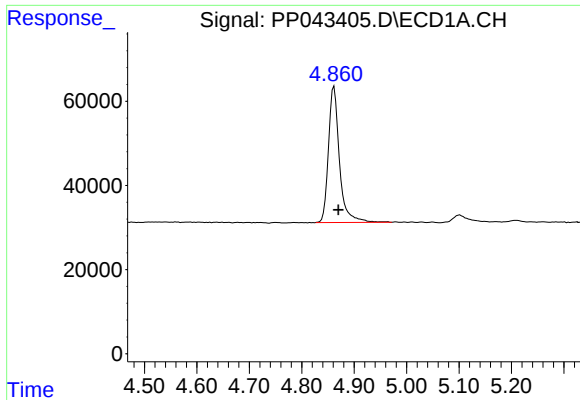

#1 Tetrachloro-m-xylene


R.T.: 4.862 min
Delta R.T.: -0.008 min
Response: 469516
Conc: 20.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
HP-1

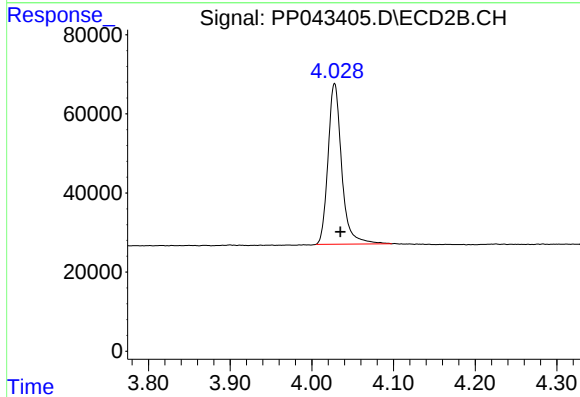


#1 Tetrachloro-m-xylene

R.T.: 4.028 min
Delta R.T.: -0.007 min
Response: 471972
Conc: 21.18 ng/ml

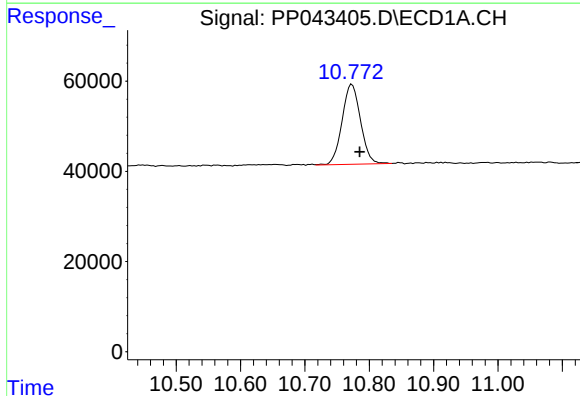

#2 Decachlorobiphenyl

R.T.: 10.773 min
Delta R.T.: -0.012 min
Response: 353415
Conc: 24.95 ng/ml

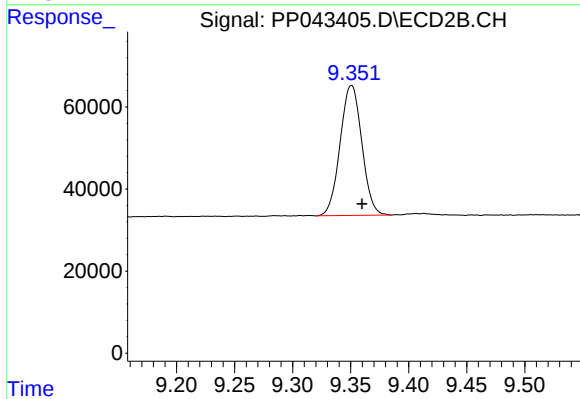

#2 Decachlorobiphenyl

R.T.: 9.351 min
Delta R.T.: -0.009 min
Response: 412844
Conc: 22.14 ng/ml