

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020122\
Data File : PP043423.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Feb 2022 21:13
Operator : AJ\MA
Sample : N1342-21
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
31538

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 00:22:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.863	4.029	193951	917647	8.438	41.183 #
2) SA Decachlor...	10.776	9.352	411904	488753	29.082	26.216

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020122\
Data File : PP043423.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Feb 2022 21:13
Operator : AJ\MA
Sample : N1342-21
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
31538

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 00:22:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

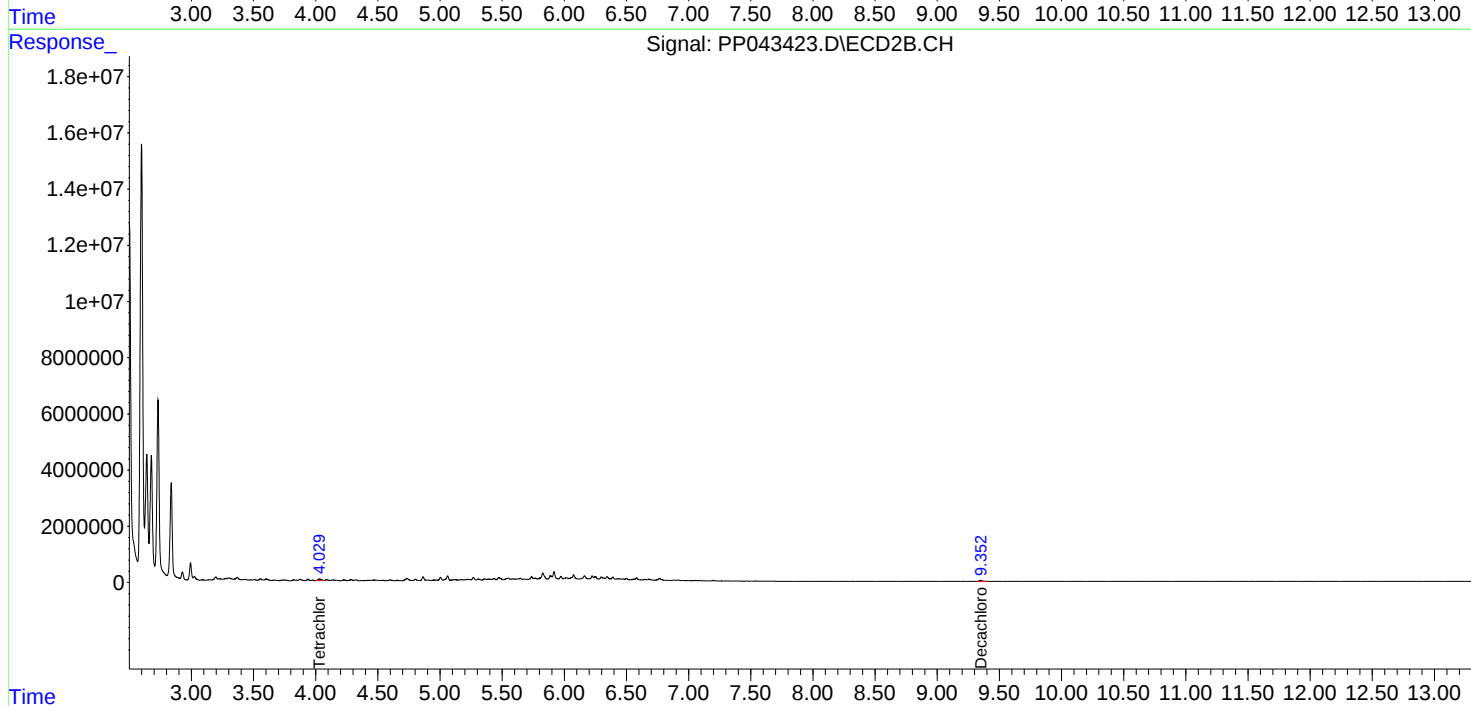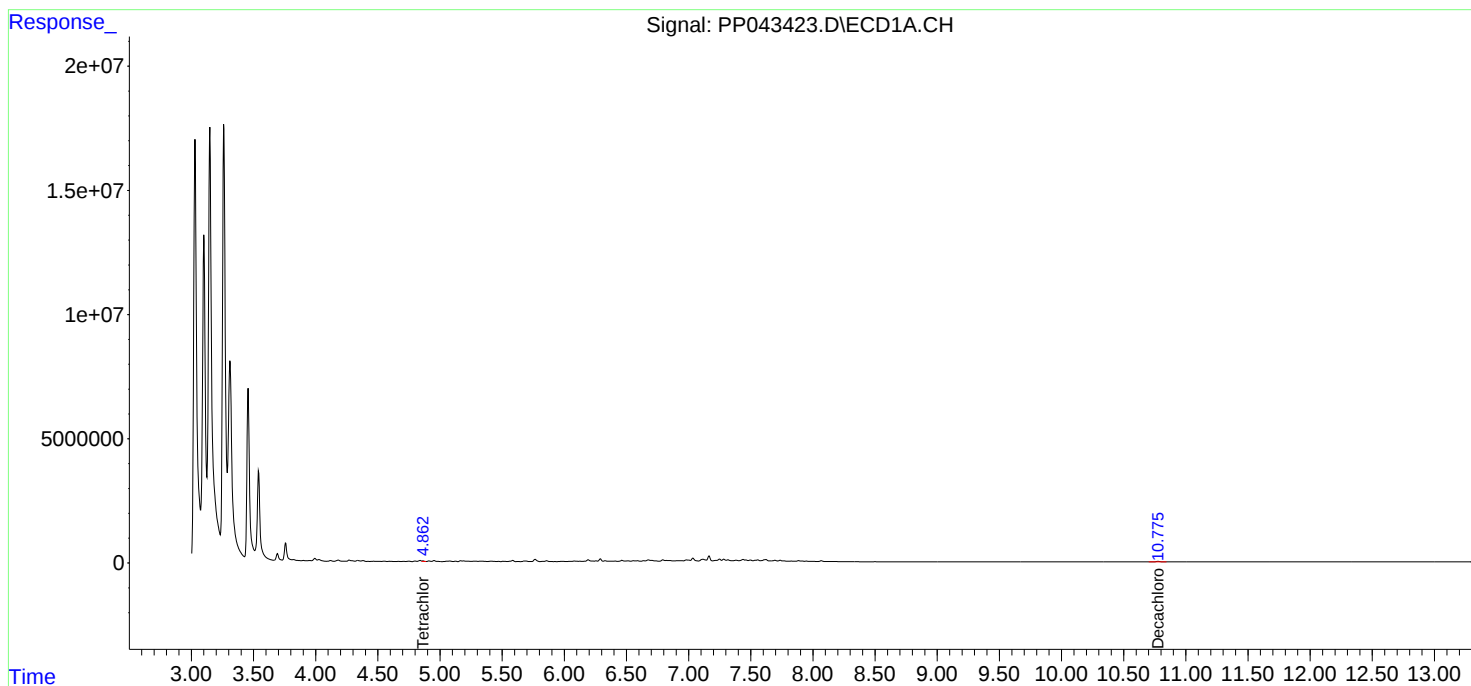


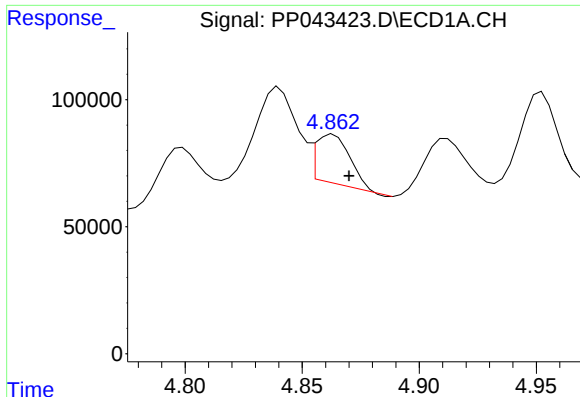

#1 Tetrachloro-m-xylene


R.T.: 4.863 min
Delta R.T.: -0.007 min
Response: 193951
Conc: 8.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
31538

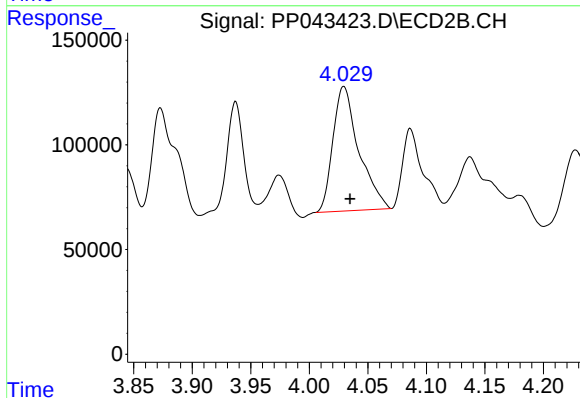


#1 Tetrachloro-m-xylene

R.T.: 4.029 min
Delta R.T.: -0.005 min
Response: 917647
Conc: 41.18 ng/ml

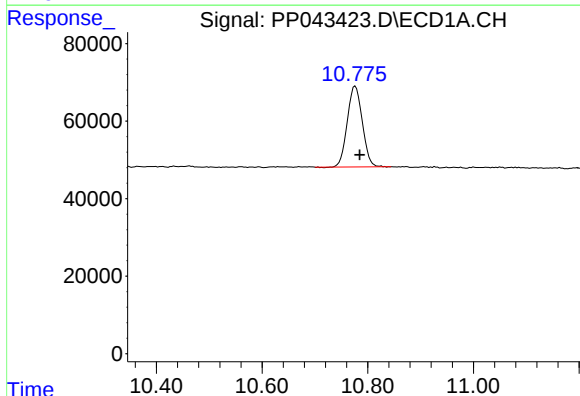

#2 Decachlorobiphenyl

R.T.: 10.776 min
Delta R.T.: -0.009 min
Response: 411904
Conc: 29.08 ng/ml

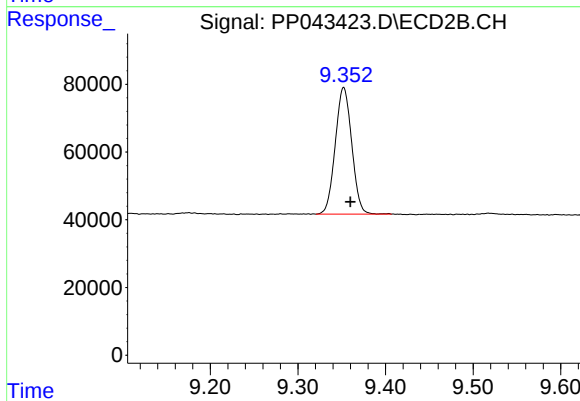

#2 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: -0.008 min
Response: 488753
Conc: 26.22 ng/ml