

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020124\
 Data File : PP063203.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2024 23:16
 Operator : YP\AJ
 Sample : P1187-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 01:43:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 01 16:28:12 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.491	3.647	51972417	50932486	21.728	21.428
2)	SA Decachlor...	10.363	8.703	53655652	57351376	23.859	23.153
Target Compounds							
3)	L1 AR-1016-1	5.673	4.742	3445719	3104364	45.790	43.393
4)	L1 AR-1016-2	5.696	4.761	4823757	4327336	44.413	42.130
5)	L1 AR-1016-3	5.758	4.938	3202678	2365653	46.409	42.779
6)	L1 AR-1016-4	5.858	4.981	2323520	2303166	41.489	46.541
7)	L1 AR-1016-5	6.155	5.196	2692543	2885570	44.096	45.871
9)	L2 AR-1221-2	4.800	3.950	1301232	1002431	60.991	50.751
10)	L2 AR-1221-3	4.866	4.026	1904387	1759558	30.915	28.900
11)	L3 AR-1232-1	4.866	4.026	1904387	1759558	35.868	32.738
12)	L3 AR-1232-2	5.403	4.761	2682762	4327336	88.680	90.303
13)	L3 AR-1232-3	5.696	4.938	4823757	2365653	94.654	91.072
14)	L3 AR-1232-4	5.858	5.023	2323520	2724572	88.432	104.521
15)	L3 AR-1232-5	5.950	5.196	2355944	2885570	102.190	105.834
16)	L4 AR-1242-1	5.673	4.742	3445719	3104364	60.516	57.126
17)	L4 AR-1242-2	5.696	4.761	4823757	4327336	58.837	55.563
18)	L4 AR-1242-3	5.758	4.938	3202678	2365653	61.028	55.824
19)	L4 AR-1242-4	5.858	5.023	2323520	2724572	54.112	58.339
20)	L4 AR-1242-5	6.603	5.551	768037	2810343	17.222	54.303 #
21)	L5 AR-1248-1	5.673	4.742	3445719	3104364	77.694	74.933
22)	L5 AR-1248-2	5.950	4.981	2355944	2303166	32.793	34.812
23)	L5 AR-1248-3	6.155	5.023	2692543	2724572	34.650	38.893
24)	L5 AR-1248-4	6.562	5.196	849015	2885570	11.393	36.111 #
25)	L5 AR-1248-5	6.603	5.591	768037	577708	9.873	8.420
26)	L6 AR-1254-1	6.536	5.551	2459265	2810343	27.504	23.174
27)	L6 AR-1254-2	6.757	5.699	2112501	1933392	16.094	17.818
28)	L6 AR-1254-3	7.126	6.123f	1879558	4017892	14.057	23.437 #
29)	L6 AR-1254-4	7.414	0.000	987831	0	12.505	N.D. #
30)	L6 AR-1254-5	7.835	6.756	6610929	6487331	66.726	45.661 #
31)	L7 AR-1260-1	7.292	6.238	6563146	6088992	53.925	45.937
32)	L7 AR-1260-2	7.551	6.426	6639165	6751472	52.204	45.710
33)	L7 AR-1260-3	7.914	6.581	5044937	6703407	48.804	46.237
34)	L7 AR-1260-4	8.143	7.057	5630547	5432942	47.955	44.570
35)	L7 AR-1260-5	8.473	7.300	8930473	10517288	45.506	42.331
36)	L8 AR-1262-1	7.972	6.850	2443900	2344309	38.610	33.038
37)	L8 AR-1262-2	8.473	7.057	8930473	5432942	38.753	33.159
38)	L8 AR-1262-3	8.809	7.587	5773712	2414696	34.945	19.965 #
39)	L8 AR-1262-4	8.872f	7.650	4060429	7728736	30.063	36.675
40)	L8 AR-1262-5	9.573	8.148	1897051	2266588	26.030	27.763
41)	L9 AR-1268-1	8.809	7.587	5773712	2414696	19.826	7.507 #
42)	L9 AR-1268-2	8.872f	7.650	4060429	7728736	16.083	25.863 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020124\
Data File : PP063203.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2024 23:16
Operator : YP\AJ
Sample : P1187-07
Misc : AR1660 LOD 40 PPB
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 01:43:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 01 16:28:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44)	L9 AR-1268-4	9.573	8.148	1897051	2266588	24.530	25.819
45)	L9 AR-1268-5	10.006	8.442	923954	1064896	1.266	1.264



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020124\
Data File : PP063203.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2024 23:16
Operator : YP\AJ
Sample : P1187-07
Misc : AR1660 LOD 40 PPB
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 01:43:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 01 16:28:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

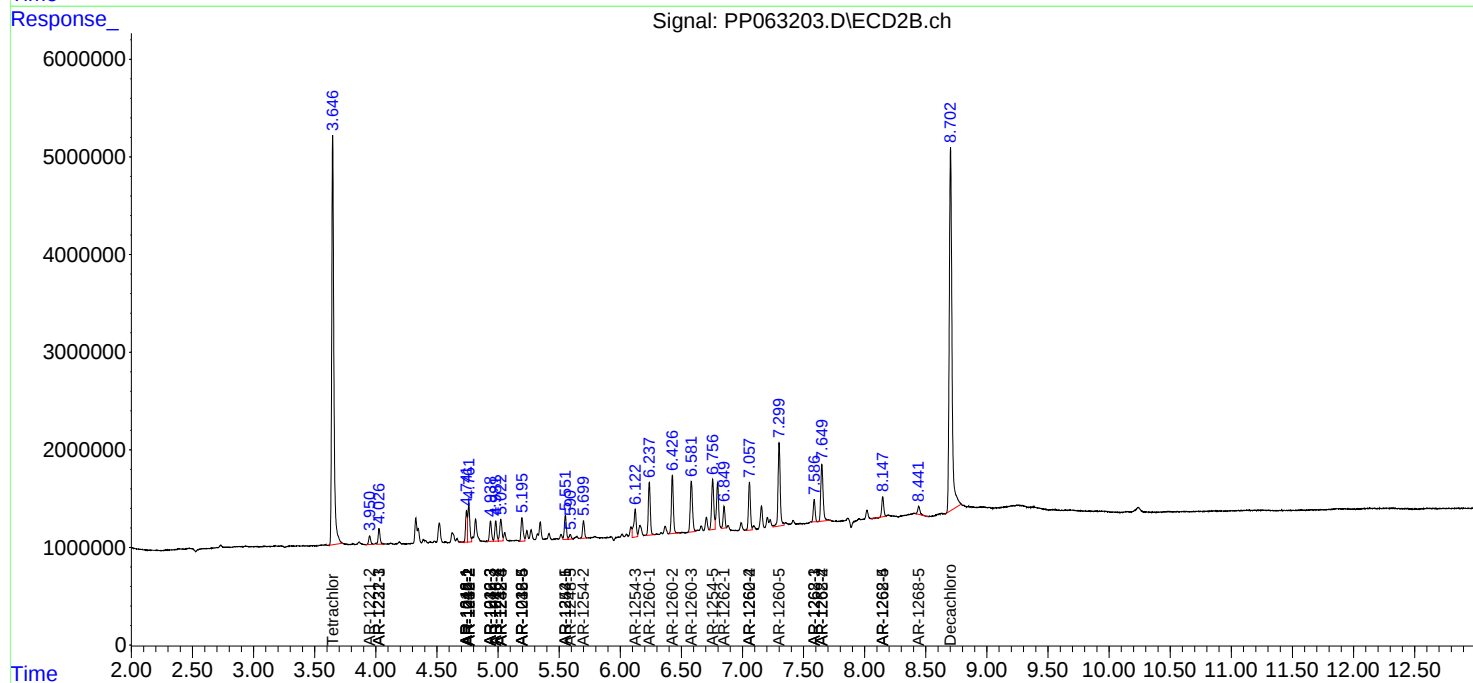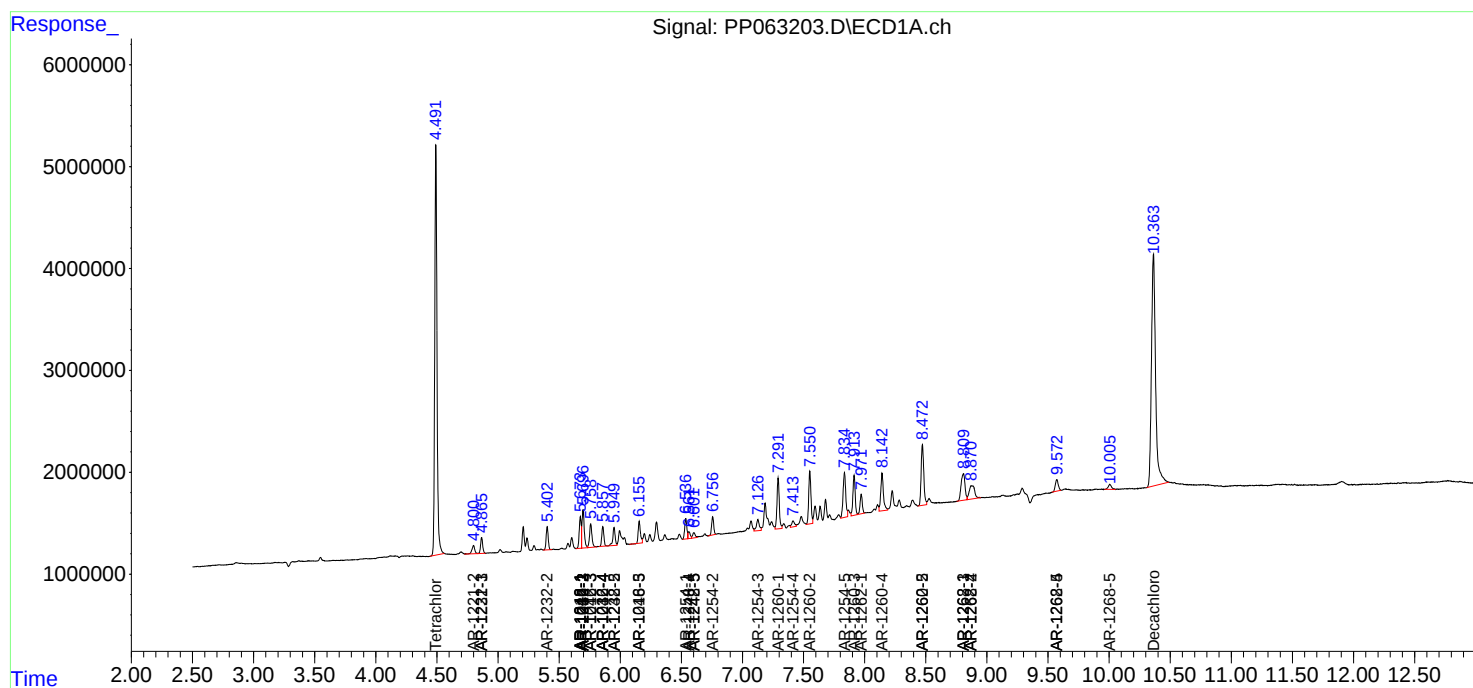


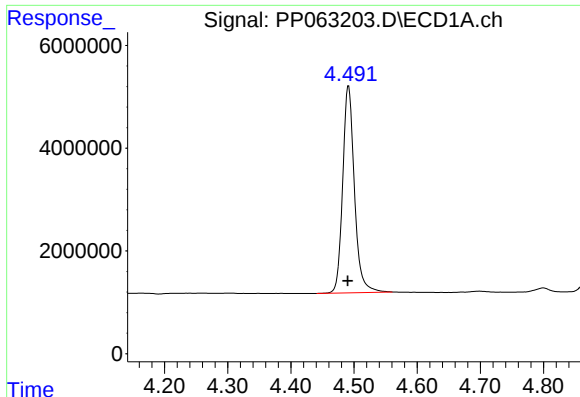

#1 Tetrachloro-m-xylene


R.T.: 4.491 min
Delta R.T.: 0.001 min
Response: 51972417
Conc: 21.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

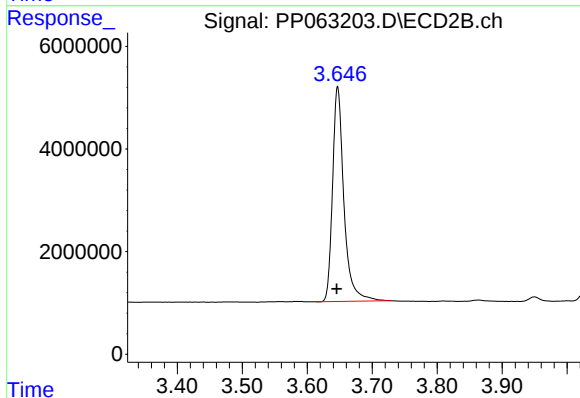


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: 0.001 min
Response: 50932486
Conc: 21.43 ng/ml

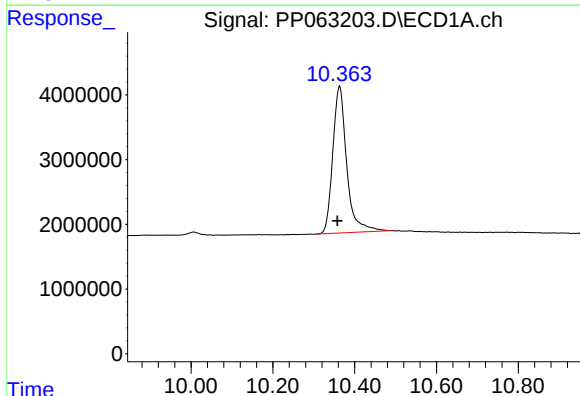


#2 Decachlorobiphenyl

R.T.: 10.363 min
Delta R.T.: 0.005 min
Response: 53655652
Conc: 23.86 ng/ml

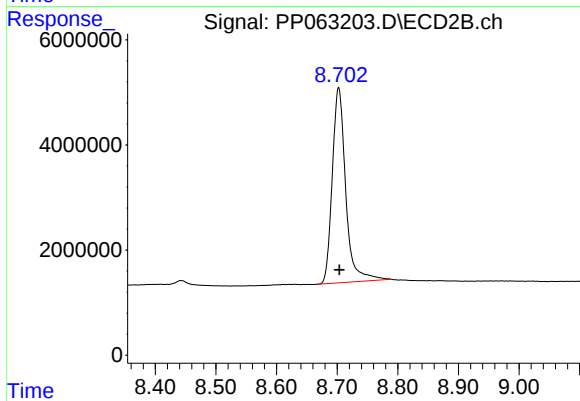

#2 Decachlorobiphenyl


R.T.: 8.703 min
Delta R.T.: -0.001 min
Response: 57351376
Conc: 23.15 ng/ml

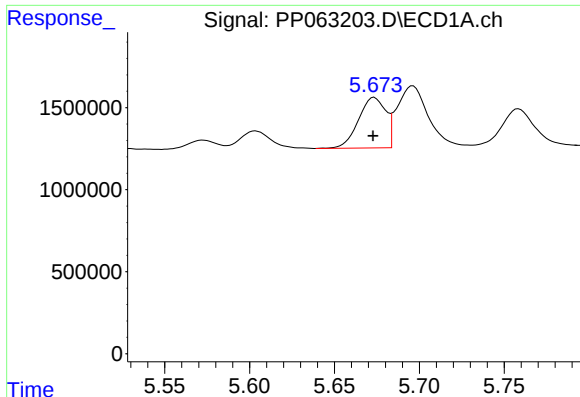

#3 AR-1016-1


R.T.: 5.673 min
Delta R.T.: 0.000 min
Response: 3445719
Conc: 45.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

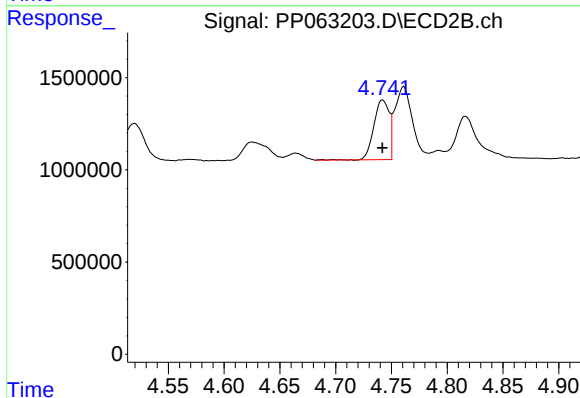


#3 AR-1016-1

R.T.: 4.742 min
Delta R.T.: 0.000 min
Response: 3104364
Conc: 43.39 ng/ml

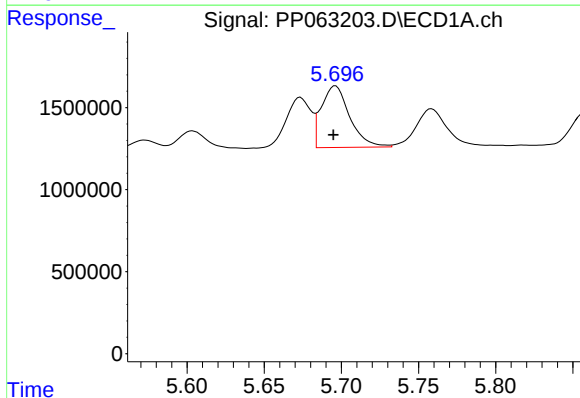


#4 AR-1016-2

R.T.: 5.696 min
Delta R.T.: 0.001 min
Response: 4823757
Conc: 44.41 ng/ml

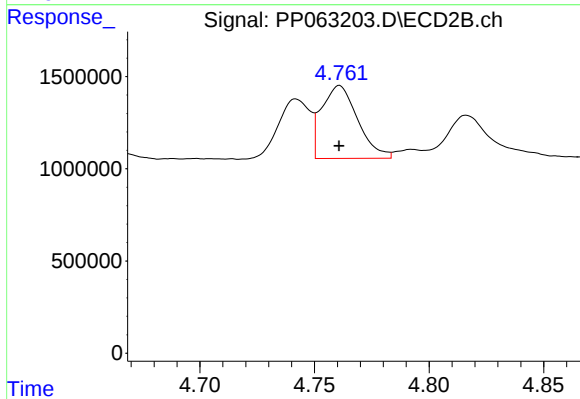

#4 AR-1016-2


R.T.: 4.761 min
Delta R.T.: 0.000 min
Response: 4327336
Conc: 42.13 ng/ml

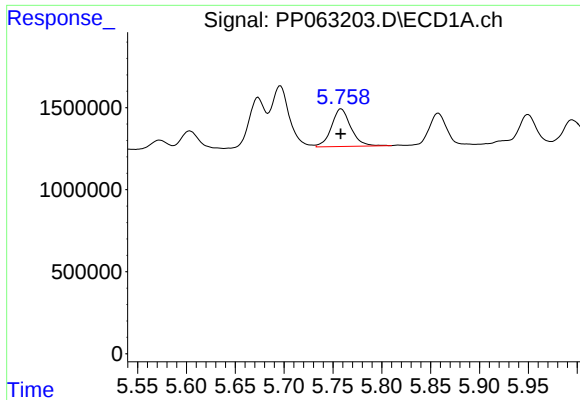

#5 AR-1016-3


R.T.: 5.758 min
Delta R.T.: 0.000 min
Response: 3202678
Conc: 46.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

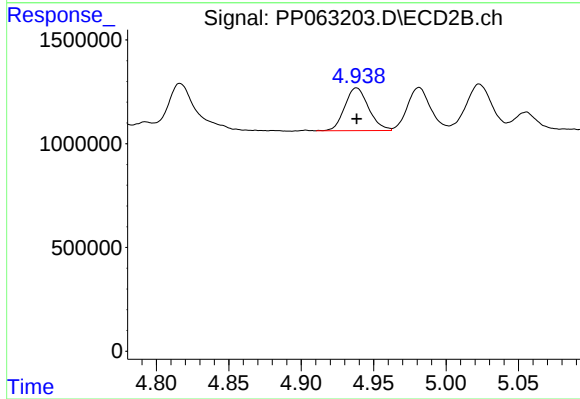


#5 AR-1016-3

R.T.: 4.938 min
Delta R.T.: 0.000 min
Response: 2365653
Conc: 42.78 ng/ml

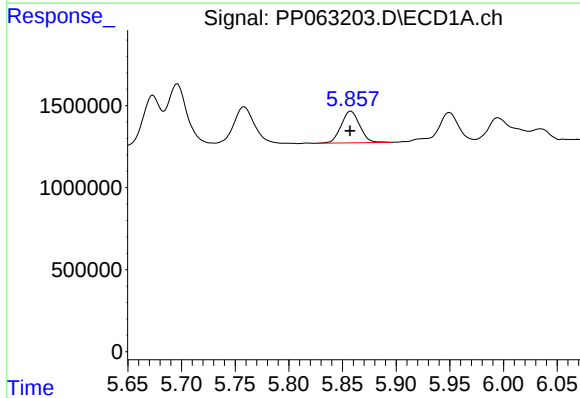


#6 AR-1016-4

R.T.: 5.858 min
Delta R.T.: 0.000 min
Response: 2323520
Conc: 41.49 ng/ml

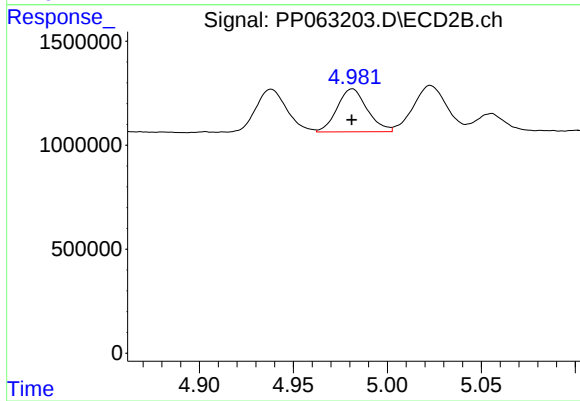

#6 AR-1016-4


R.T.: 4.981 min
Delta R.T.: 0.000 min
Response: 2303166
Conc: 46.54 ng/ml

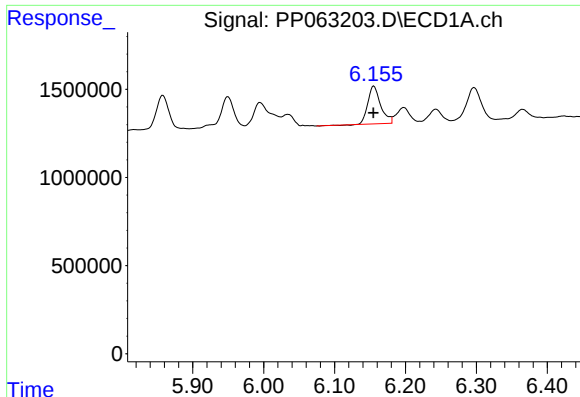

#7 AR-1016-5


R.T.: 6.155 min
Delta R.T.: 0.000 min
Response: 2692543
Conc: 44.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

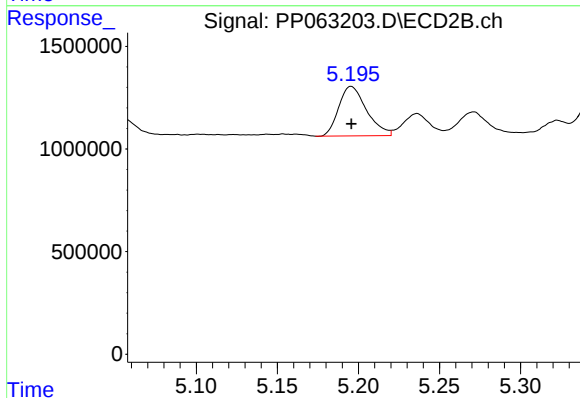


#7 AR-1016-5

R.T.: 5.196 min
Delta R.T.: 0.000 min
Response: 2885570
Conc: 45.87 ng/ml

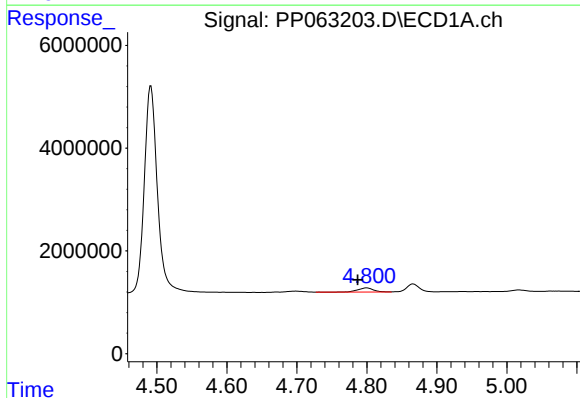


#9 AR-1221-2

R.T.: 4.800 min
Delta R.T.: 0.013 min
Response: 1301232
Conc: 60.99 ng/ml

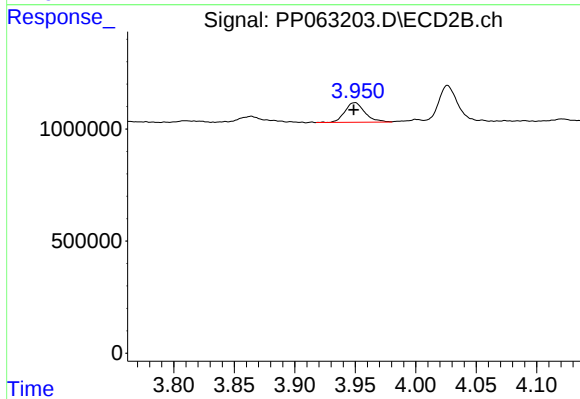

#9 AR-1221-2


R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 1002431
Conc: 50.75 ng/ml

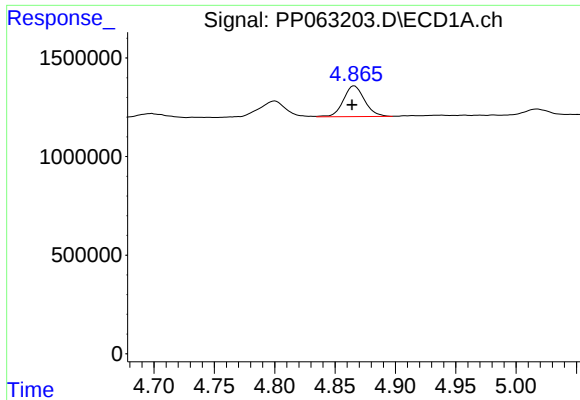

#10 AR-1221-3


R.T.: 4.866 min
Delta R.T.: 0.002 min
Response: 1904387
Conc: 30.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

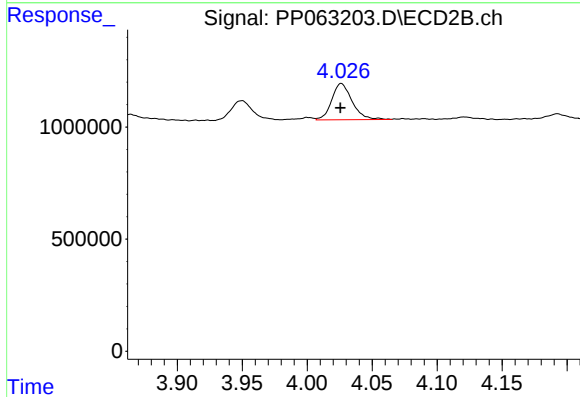


#10 AR-1221-3

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 1759558
Conc: 28.90 ng/ml

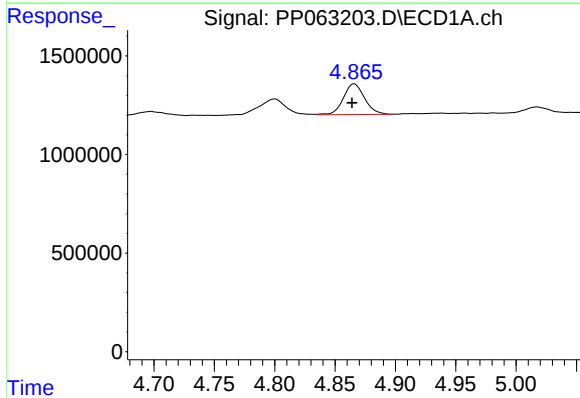


#11 AR-1232-1

R.T.: 4.866 min
Delta R.T.: 0.002 min
Response: 1904387
Conc: 35.87 ng/ml

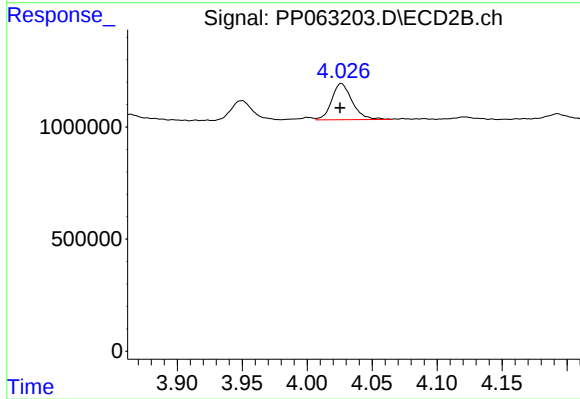

#11 AR-1232-1


R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 1759558
Conc: 32.74 ng/ml

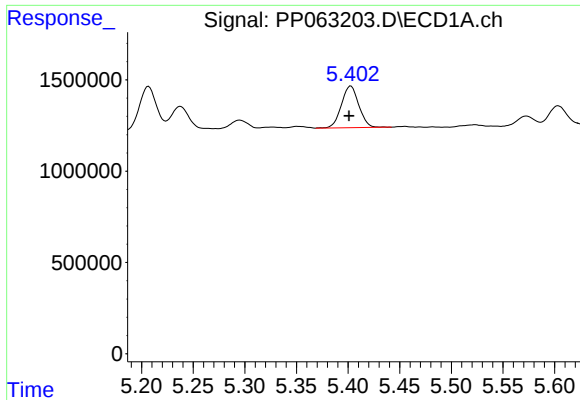

#12 AR-1232-2


R.T.: 5.403 min
Delta R.T.: 0.002 min
Response: 2682762
Conc: 88.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

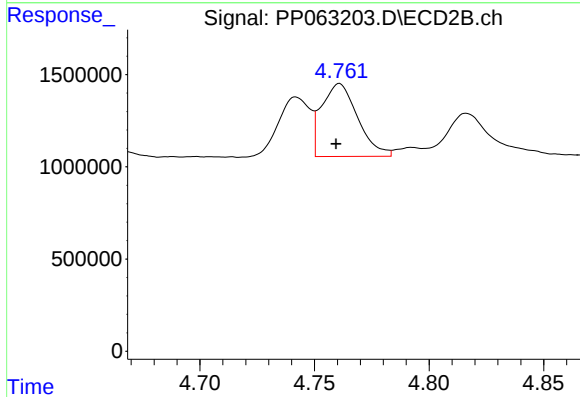


#12 AR-1232-2

R.T.: 4.761 min
Delta R.T.: 0.001 min
Response: 4327336
Conc: 90.30 ng/ml

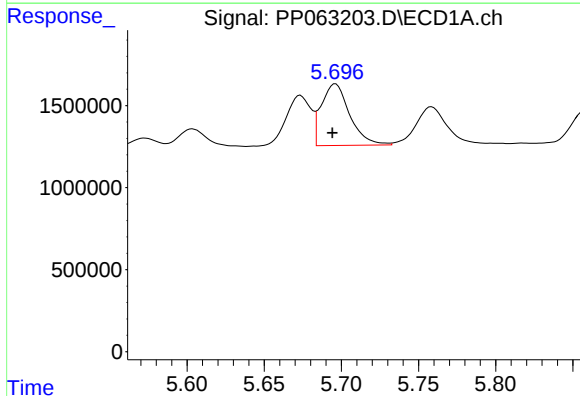


#13 AR-1232-3

R.T.: 5.696 min
Delta R.T.: 0.002 min
Response: 4823757
Conc: 94.65 ng/ml

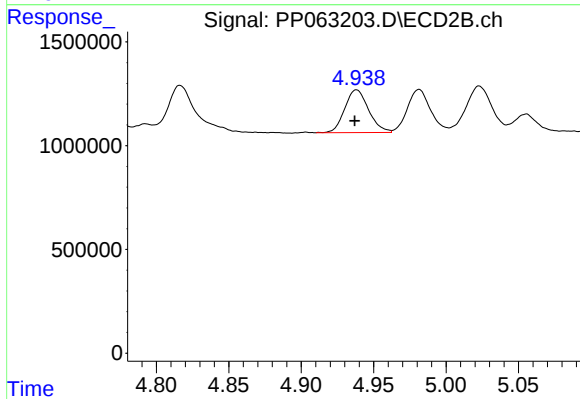

#13 AR-1232-3


R.T.: 4.938 min
Delta R.T.: 0.001 min
Response: 2365653
Conc: 91.07 ng/ml

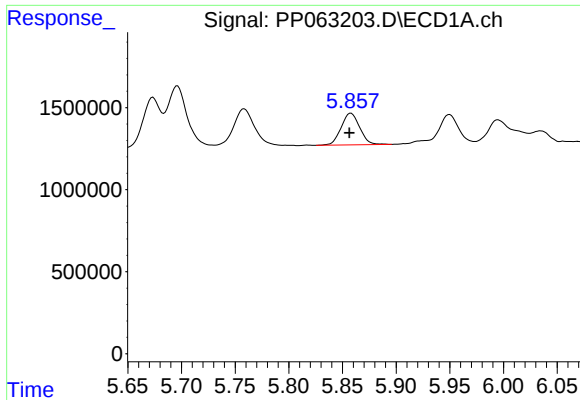

#14 AR-1232-4


R.T.: 5.858 min
Delta R.T.: 0.001 min
Response: 2323520
Conc: 88.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

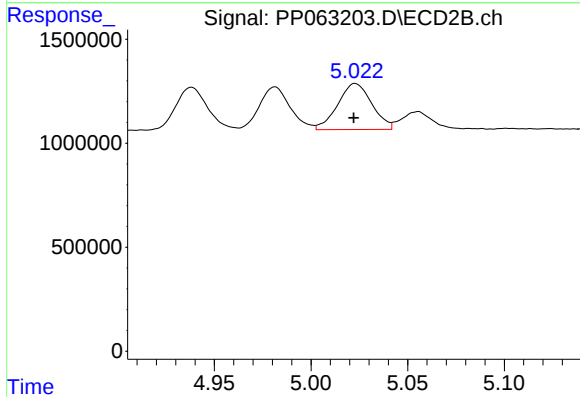


#14 AR-1232-4

R.T.: 5.023 min
Delta R.T.: 0.000 min
Response: 2724572
Conc: 104.52 ng/ml

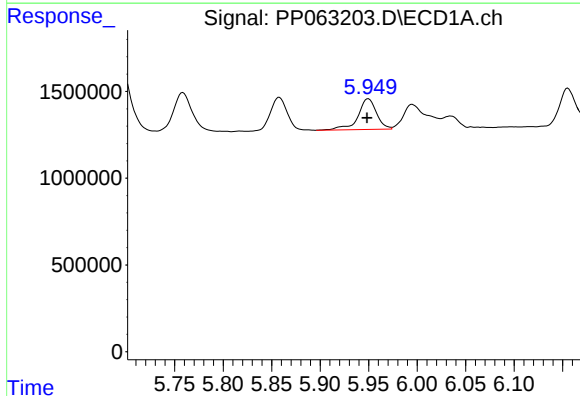


#15 AR-1232-5

R.T.: 5.950 min
Delta R.T.: 0.001 min
Response: 2355944
Conc: 102.19 ng/ml

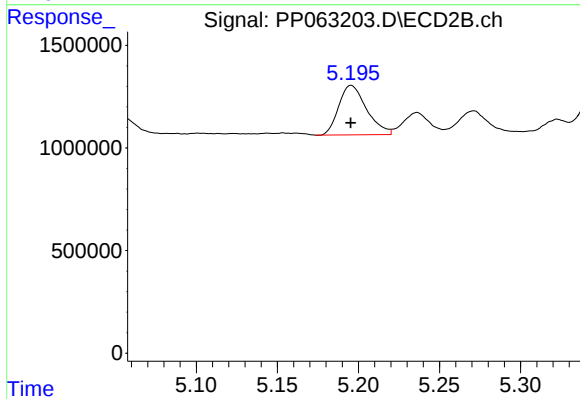

#15 AR-1232-5


R.T.: 5.196 min
Delta R.T.: 0.000 min
Response: 2885570
Conc: 105.83 ng/ml

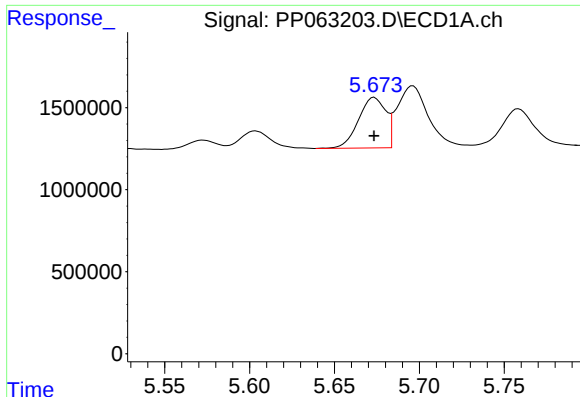

#16 AR-1242-1


R.T.: 5.673 min
Delta R.T.: 0.000 min
Response: 3445719
Conc: 60.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

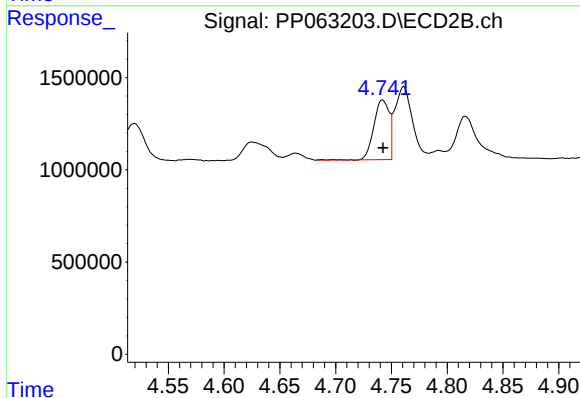


#16 AR-1242-1

R.T.: 4.742 min
Delta R.T.: 0.000 min
Response: 3104364
Conc: 57.13 ng/ml

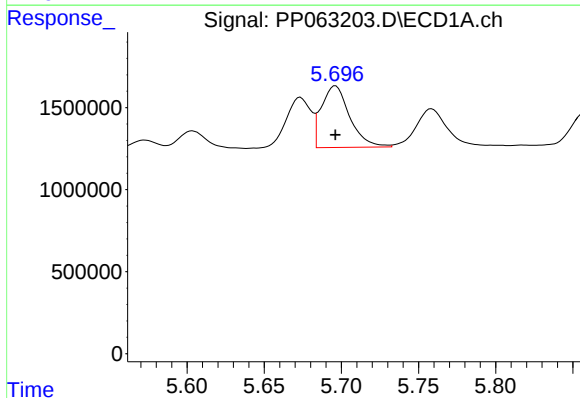


#17 AR-1242-2

R.T.: 5.696 min
Delta R.T.: 0.000 min
Response: 4823757
Conc: 58.84 ng/ml

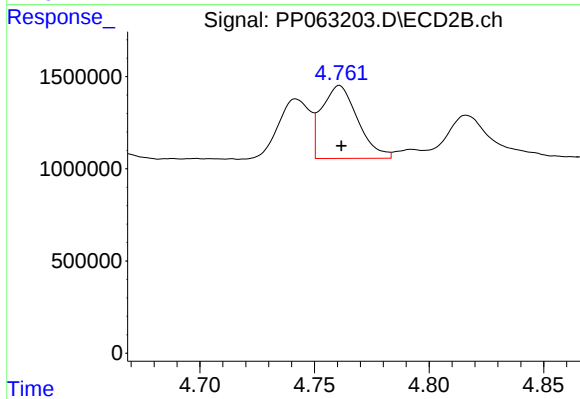

#17 AR-1242-2


R.T.: 4.761 min
Delta R.T.: 0.000 min
Response: 4327336
Conc: 55.56 ng/ml

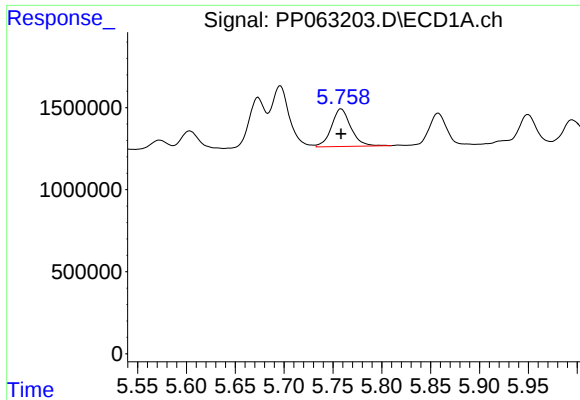

#18 AR-1242-3


R.T.: 5.758 min
Delta R.T.: 0.000 min
Response: 3202678
Conc: 61.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

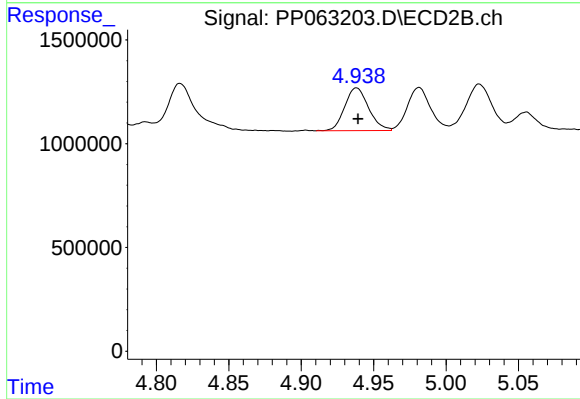


#18 AR-1242-3

R.T.: 4.938 min
Delta R.T.: -0.001 min
Response: 2365653
Conc: 55.82 ng/ml

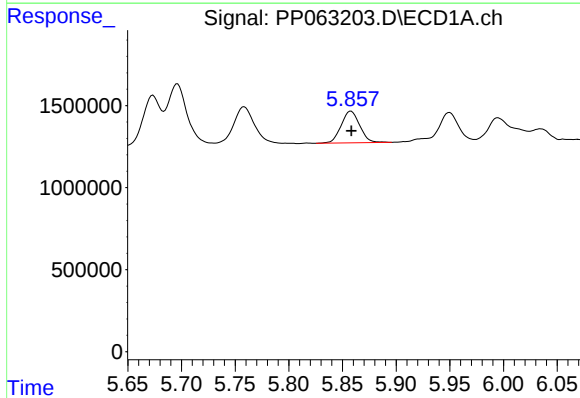


#19 AR-1242-4

R.T.: 5.858 min
Delta R.T.: 0.000 min
Response: 2323520
Conc: 54.11 ng/ml

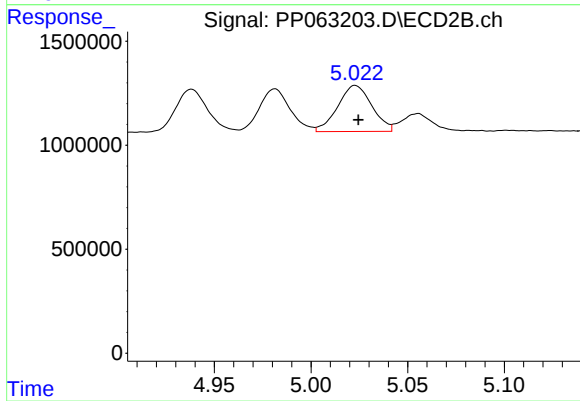

#19 AR-1242-4


R.T.: 5.023 min
Delta R.T.: -0.002 min
Response: 2724572
Conc: 58.34 ng/ml

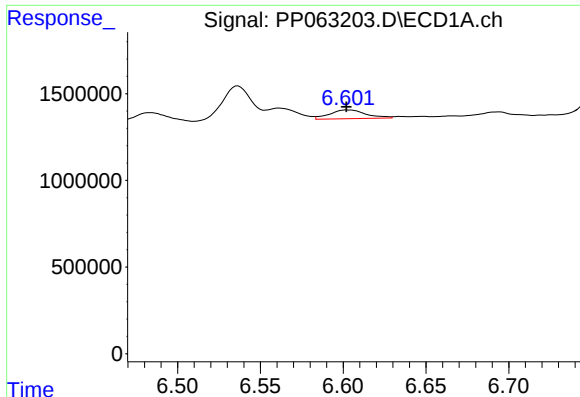

#20 AR-1242-5


R.T.: 6.603 min
Delta R.T.: 0.000 min
Response: 768037
Conc: 17.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

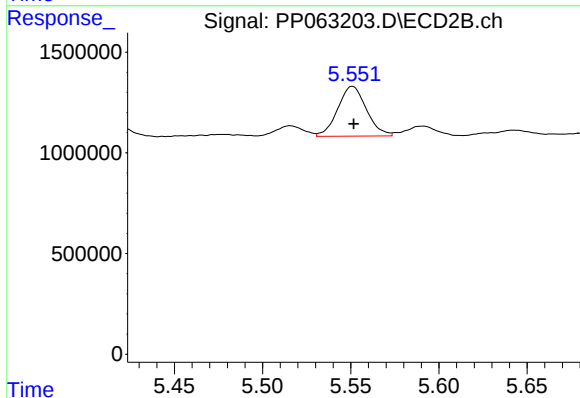


#20 AR-1242-5

R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 2810343
Conc: 54.30 ng/ml

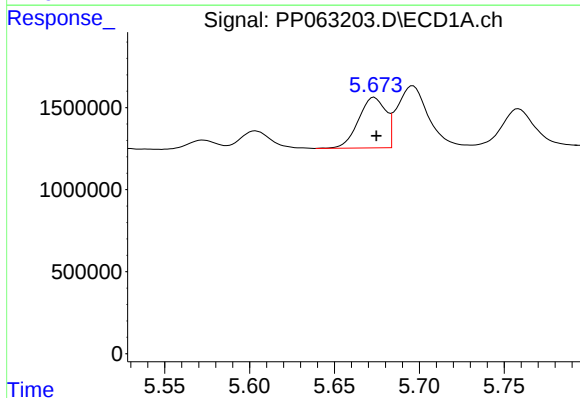


#21 AR-1248-1

R.T.: 5.673 min
Delta R.T.: -0.001 min
Response: 3445719
Conc: 77.69 ng/ml

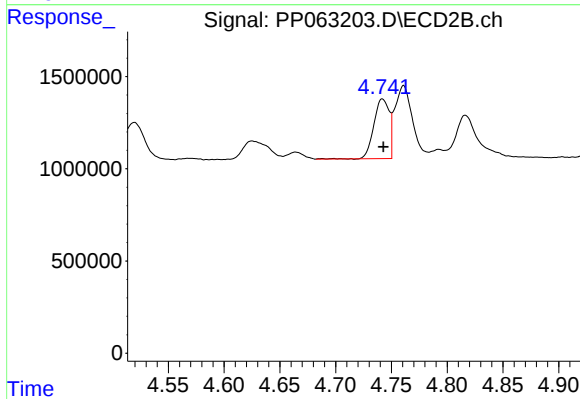

#21 AR-1248-1


R.T.: 4.742 min
Delta R.T.: 0.000 min
Response: 3104364
Conc: 74.93 ng/ml

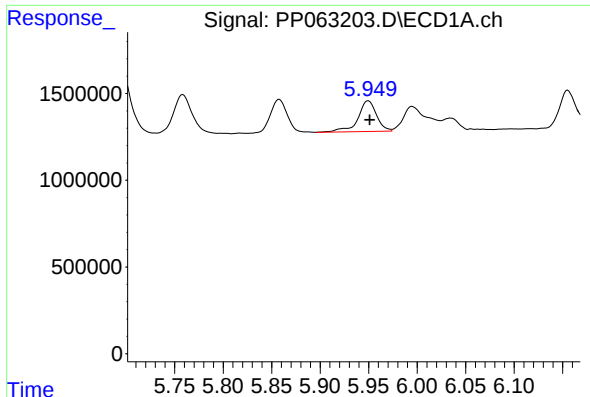

#22 AR-1248-2


R.T.: 5.950 min
Delta R.T.: -0.002 min
Response: 2355944
Conc: 32.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

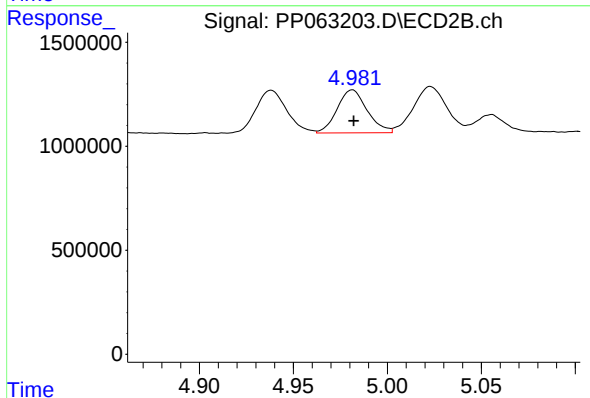


#22 AR-1248-2

R.T.: 4.981 min
Delta R.T.: 0.000 min
Response: 2303166
Conc: 34.81 ng/ml

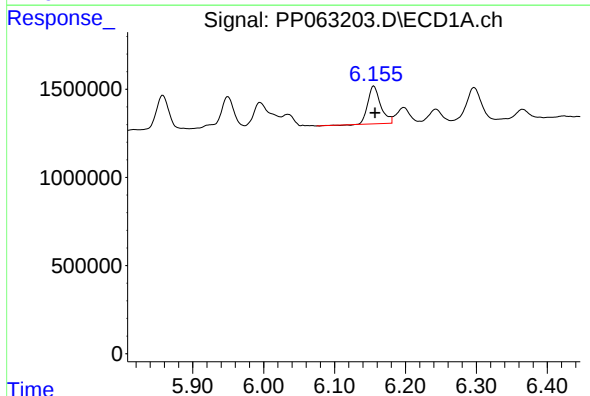


#23 AR-1248-3

R.T.: 6.155 min
Delta R.T.: -0.002 min
Response: 2692543
Conc: 34.65 ng/ml

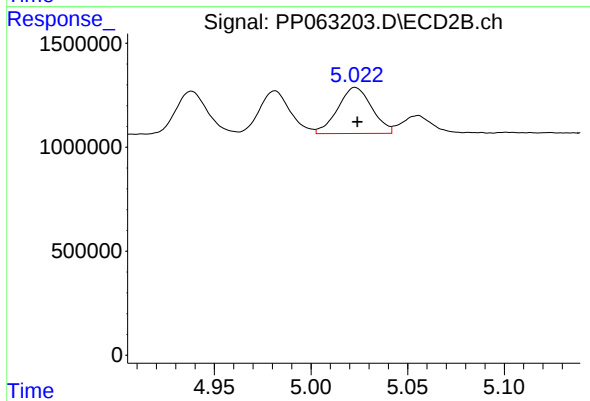

#23 AR-1248-3


R.T.: 5.023 min
Delta R.T.: -0.001 min
Response: 2724572
Conc: 38.89 ng/ml

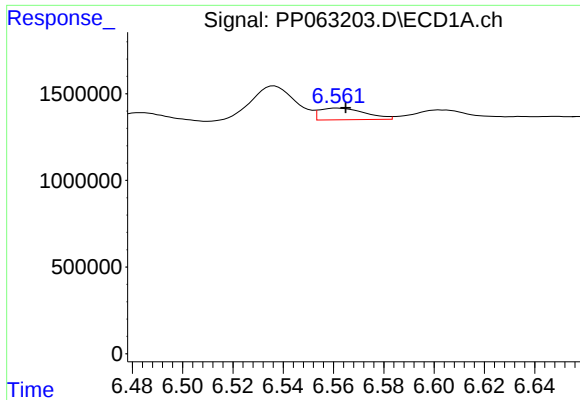

#24 AR-1248-4


R.T.: 6.562 min
Delta R.T.: -0.003 min
Response: 849015
Conc: 11.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

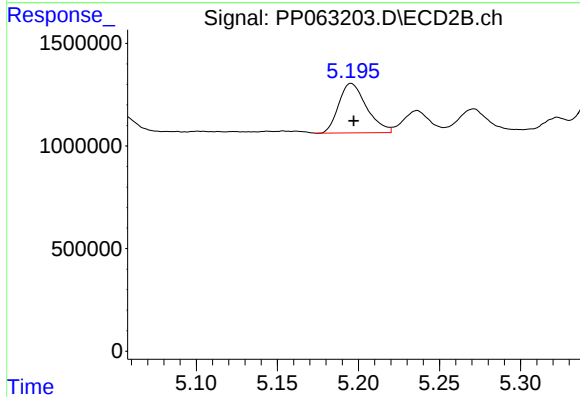


#24 AR-1248-4

R.T.: 5.196 min
Delta R.T.: -0.002 min
Response: 2885570
Conc: 36.11 ng/ml

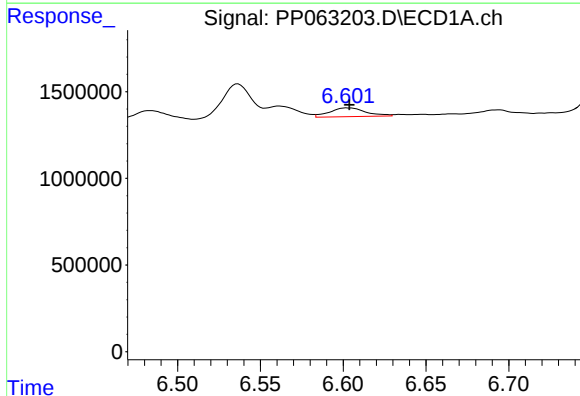


#25 AR-1248-5

R.T.: 6.603 min
Delta R.T.: -0.001 min
Response: 768037
Conc: 9.87 ng/ml

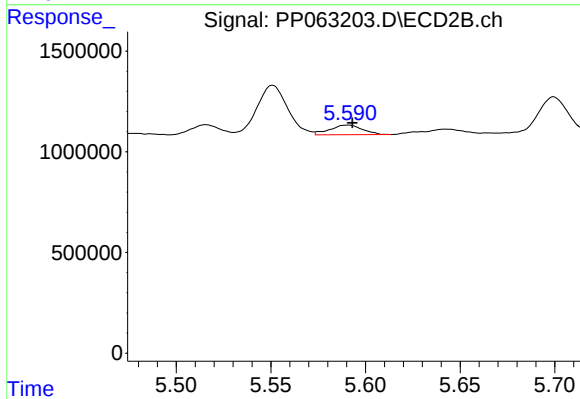

#25 AR-1248-5


R.T.: 5.591 min
Delta R.T.: -0.002 min
Response: 577708
Conc: 8.42 ng/ml

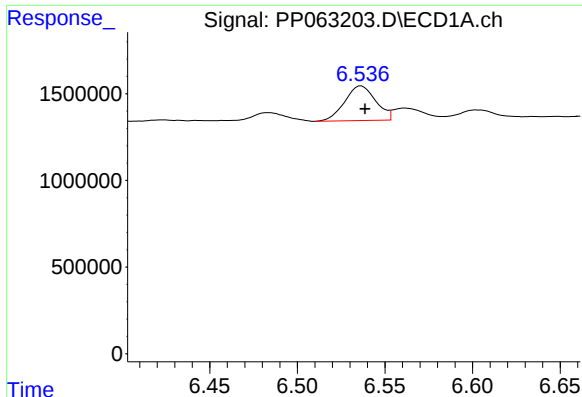

#26 AR-1254-1


R.T.: 6.536 min
Delta R.T.: -0.002 min
Response: 2459265
Conc: 27.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

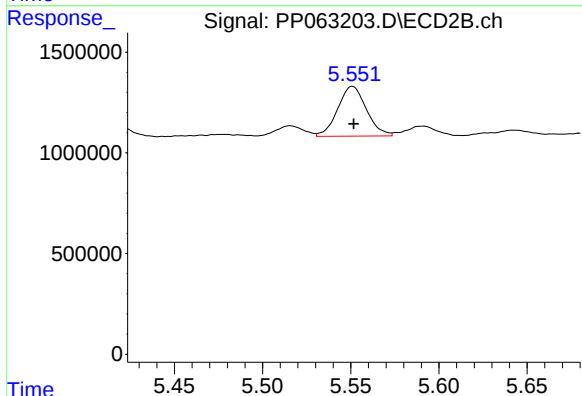


#26 AR-1254-1

R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 2810343
Conc: 23.17 ng/ml

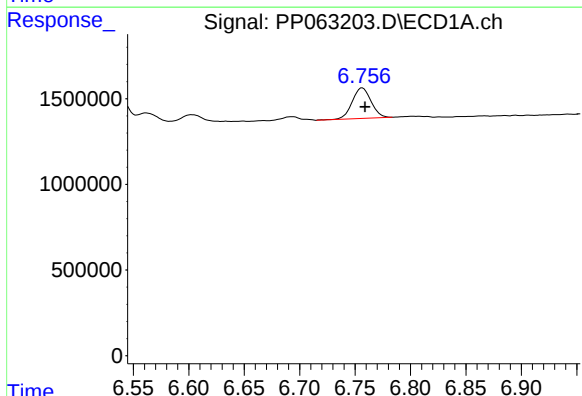


#27 AR-1254-2

R.T.: 6.757 min
Delta R.T.: -0.002 min
Response: 2112501
Conc: 16.09 ng/ml

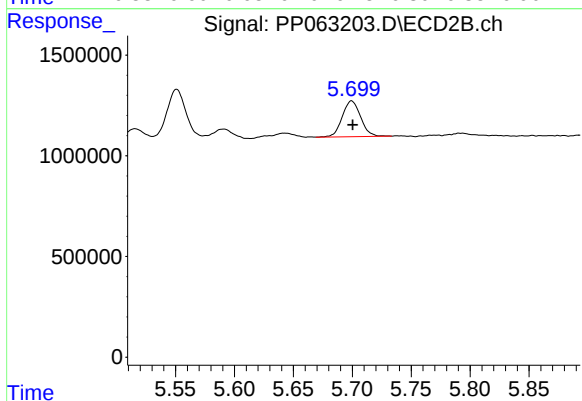

#27 AR-1254-2


R.T.: 5.699 min
Delta R.T.: 0.000 min
Response: 1933392
Conc: 17.82 ng/ml

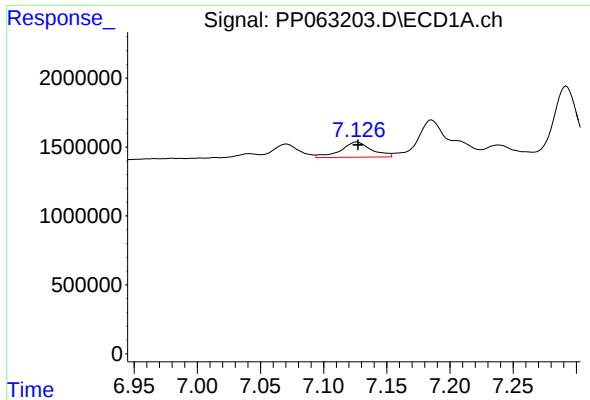

#28 AR-1254-3


R.T.: 7.126 min
Delta R.T.: 0.000 min
Response: 1879558
Conc: 14.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

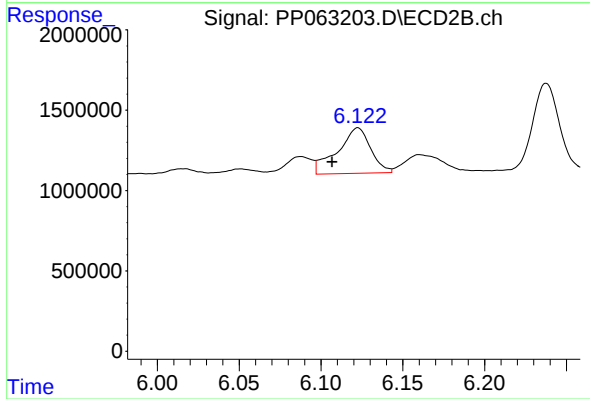


#28 AR-1254-3

R.T.: 6.123 min
Delta R.T.: 0.016 min
Response: 4017892
Conc: 23.44 ng/ml

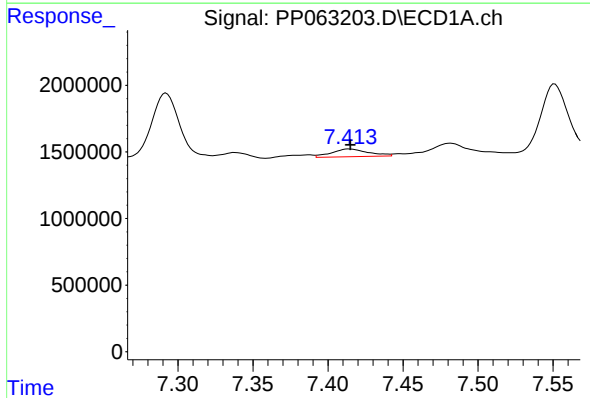


#29 AR-1254-4

R.T.: 7.414 min
Delta R.T.: -0.001 min
Response: 987831
Conc: 12.51 ng/ml

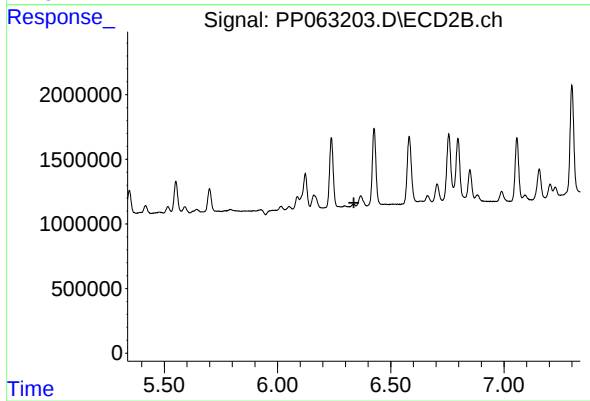

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.337 min
Response: 0
Conc: N.D.

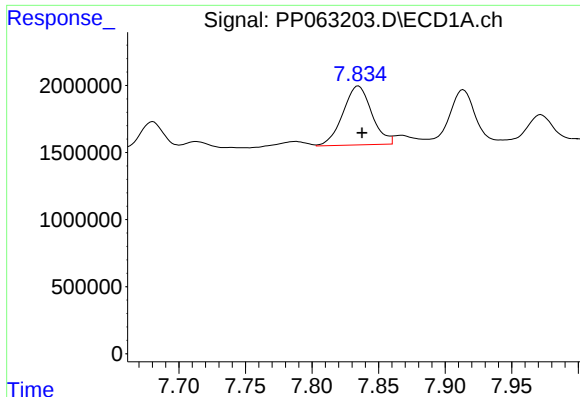

#30 AR-1254-5


R.T.: 7.835 min
Delta R.T.: -0.003 min
Response: 6610929
Conc: 66.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

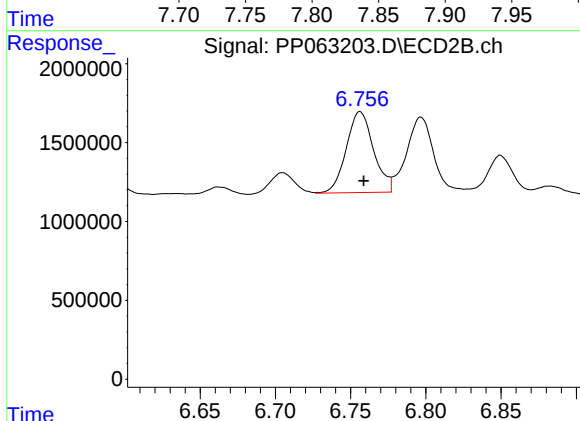


#30 AR-1254-5

R.T.: 6.756 min
Delta R.T.: -0.002 min
Response: 6487331
Conc: 45.66 ng/ml

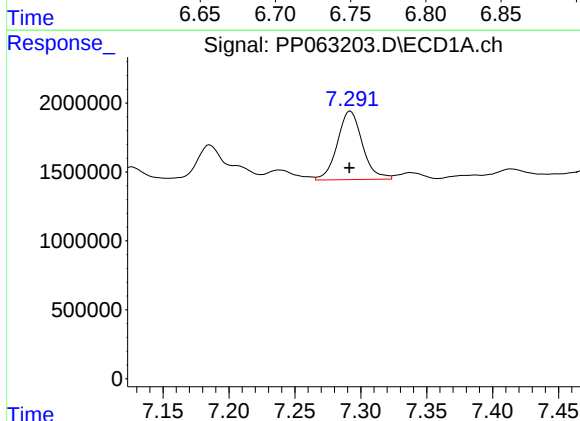


#31 AR-1260-1

R.T.: 7.292 min
Delta R.T.: 0.000 min
Response: 6563146
Conc: 53.93 ng/ml

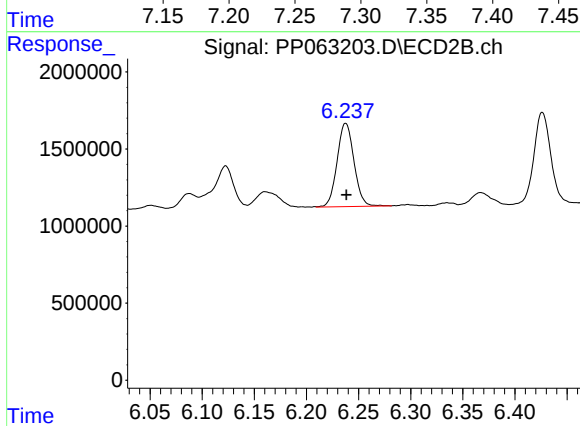

#31 AR-1260-1


R.T.: 6.238 min
Delta R.T.: 0.000 min
Response: 6088992
Conc: 45.94 ng/ml

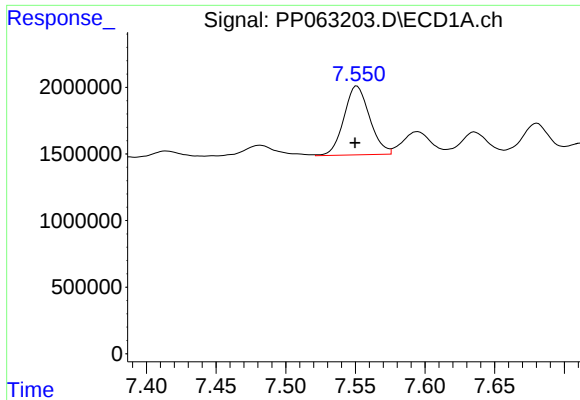

#32 AR-1260-2


R.T.: 7.551 min
Delta R.T.: 0.001 min
Response: 6639165
Conc: 52.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

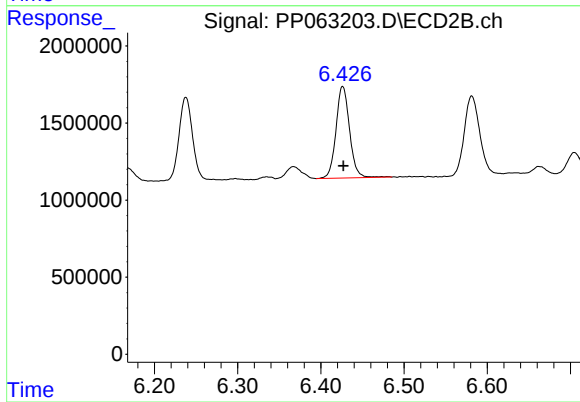


#32 AR-1260-2

R.T.: 6.426 min
Delta R.T.: 0.000 min
Response: 6751472
Conc: 45.71 ng/ml

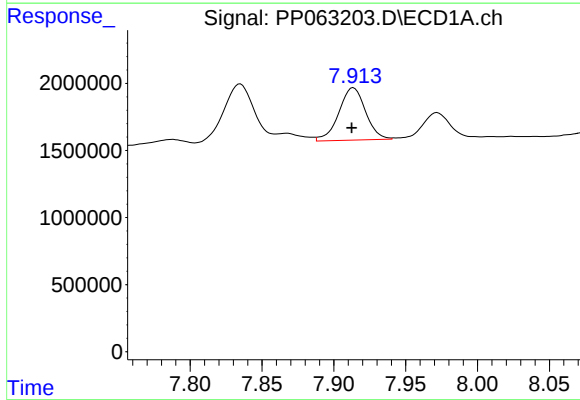


#33 AR-1260-3

R.T.: 7.914 min
Delta R.T.: 0.001 min
Response: 5044937
Conc: 48.80 ng/ml

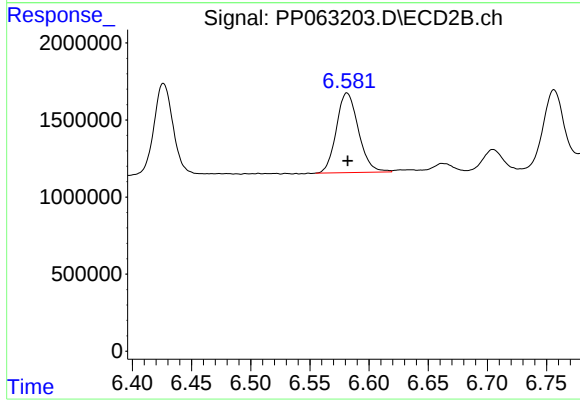

#33 AR-1260-3


R.T.: 6.581 min
Delta R.T.: 0.000 min
Response: 6703407
Conc: 46.24 ng/ml

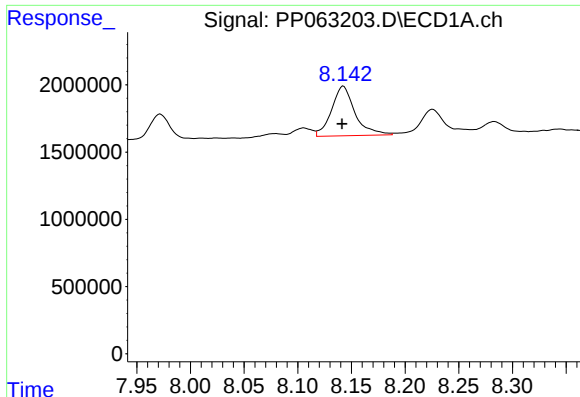

#34 AR-1260-4


R.T.: 8.143 min
Delta R.T.: 0.001 min
Response: 5630547
Conc: 47.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

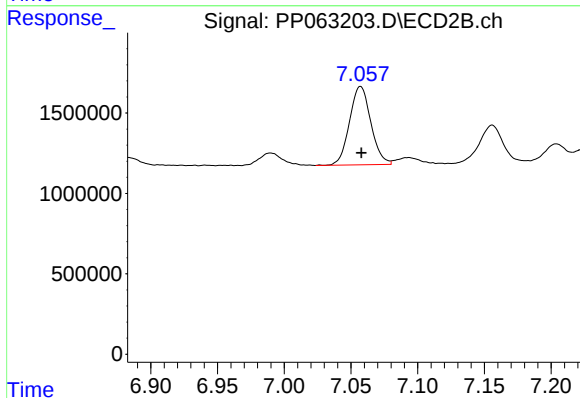


#34 AR-1260-4

R.T.: 7.057 min
Delta R.T.: 0.000 min
Response: 5432942
Conc: 44.57 ng/ml

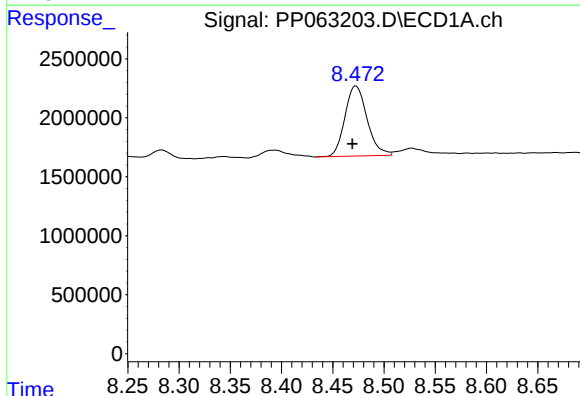


#35 AR-1260-5

R.T.: 8.473 min
Delta R.T.: 0.003 min
Response: 8930473
Conc: 45.51 ng/ml

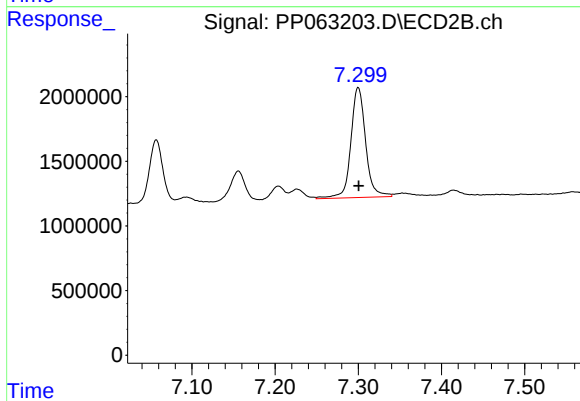

#35 AR-1260-5


R.T.: 7.300 min
Delta R.T.: 0.000 min
Response: 10517288
Conc: 42.33 ng/ml

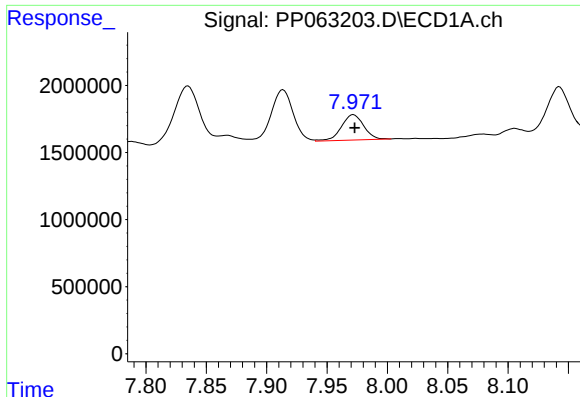

#36 AR-1262-1


R.T.: 7.972 min
Delta R.T.: 0.000 min
Response: 2443900
Conc: 38.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

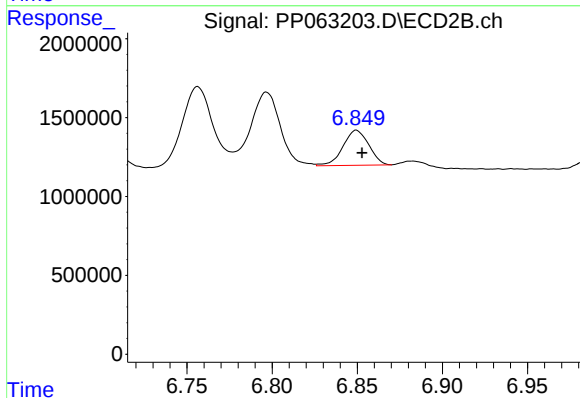


#36 AR-1262-1

R.T.: 6.850 min
Delta R.T.: -0.003 min
Response: 2344309
Conc: 33.04 ng/ml

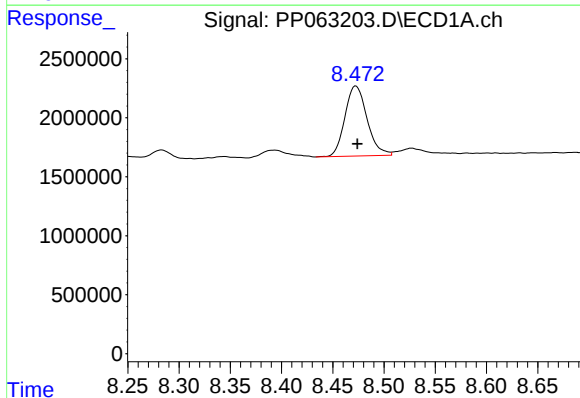


#37 AR-1262-2

R.T.: 8.473 min
Delta R.T.: -0.002 min
Response: 8930473
Conc: 38.75 ng/ml

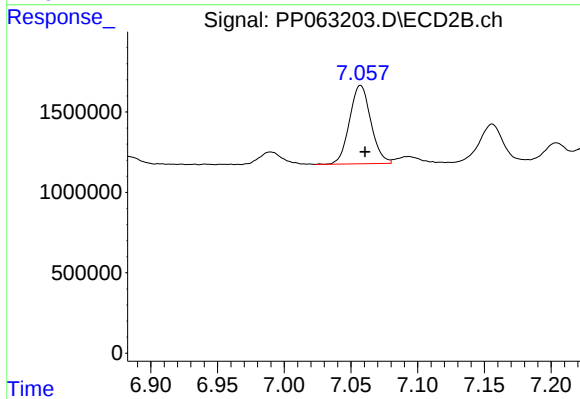

#37 AR-1262-2


R.T.: 7.057 min
Delta R.T.: -0.003 min
Response: 5432942
Conc: 33.16 ng/ml

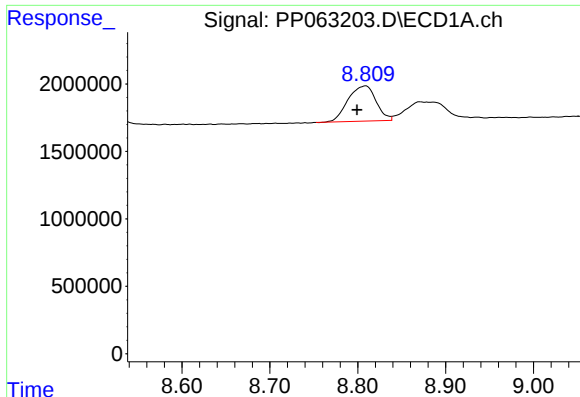

#38 AR-1262-3


R.T.: 8.809 min
Delta R.T.: 0.010 min
Response: 5773712
Conc: 34.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

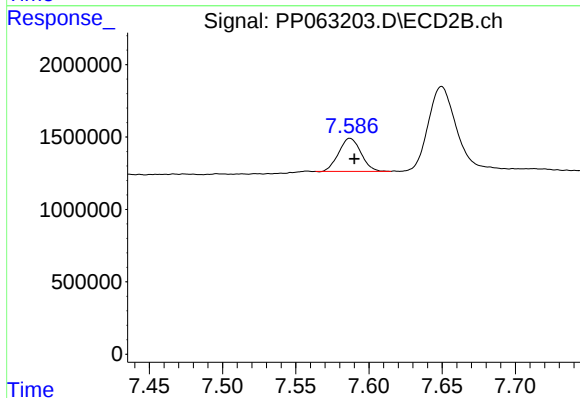


#38 AR-1262-3

R.T.: 7.587 min
Delta R.T.: -0.003 min
Response: 2414696
Conc: 19.97 ng/ml

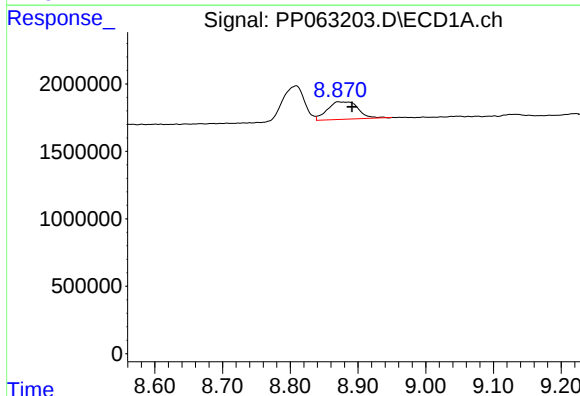


#39 AR-1262-4

R.T.: 8.872 min
Delta R.T.: -0.019 min
Response: 4060429
Conc: 30.06 ng/ml

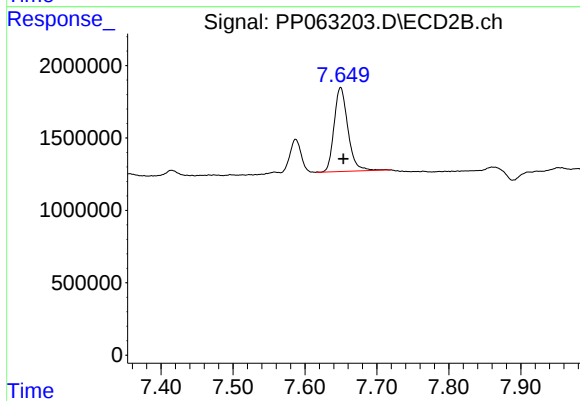

#39 AR-1262-4


R.T.: 7.650 min
Delta R.T.: -0.004 min
Response: 7728736
Conc: 36.67 ng/ml

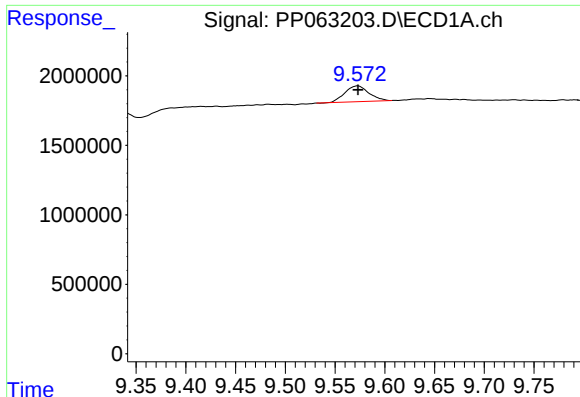

#40 AR-1262-5


R.T.: 9.573 min
Delta R.T.: 0.000 min
Response: 1897051
Conc: 26.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

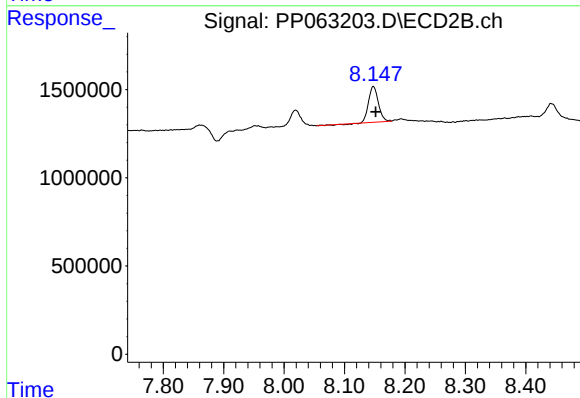


#40 AR-1262-5

R.T.: 8.148 min
Delta R.T.: -0.004 min
Response: 2266588
Conc: 27.76 ng/ml

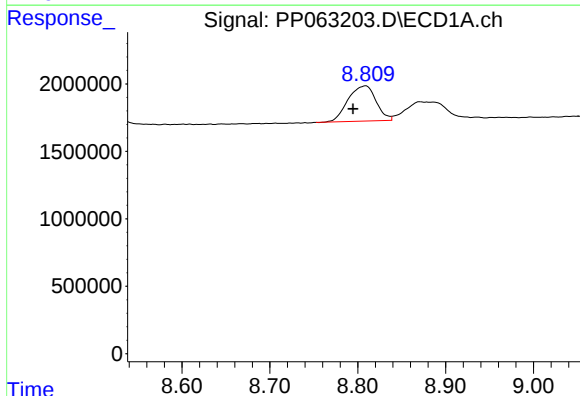


#41 AR-1268-1

R.T.: 8.809 min
Delta R.T.: 0.015 min
Response: 5773712
Conc: 19.83 ng/ml

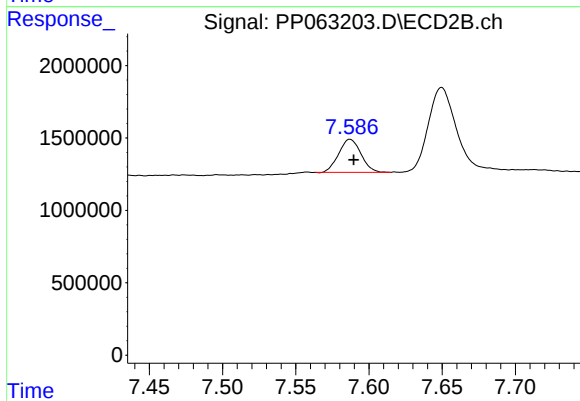

#41 AR-1268-1


R.T.: 7.587 min
Delta R.T.: -0.003 min
Response: 2414696
Conc: 7.51 ng/ml

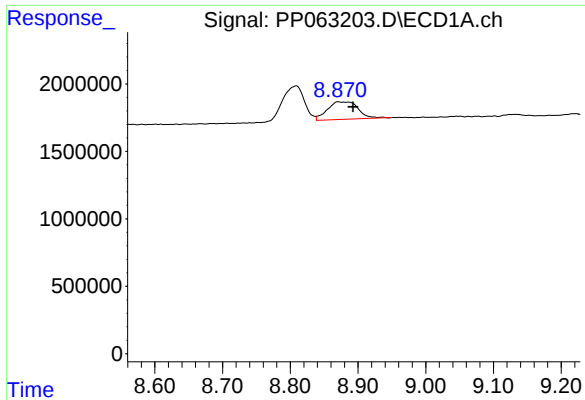

#42 AR-1268-2


R.T.: 8.872 min
Delta R.T.: -0.021 min
Response: 4060429
Conc: 16.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

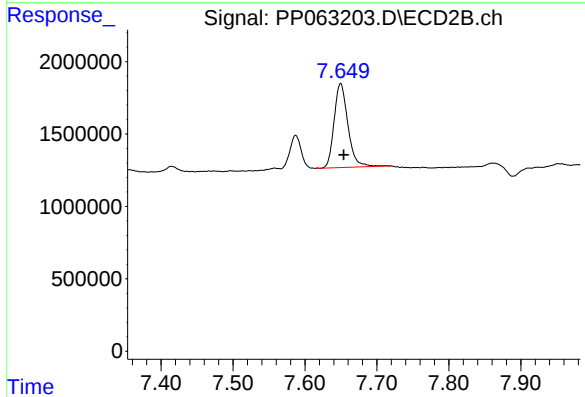


#42 AR-1268-2

R.T.: 7.650 min
Delta R.T.: -0.004 min
Response: 7728736
Conc: 25.86 ng/ml

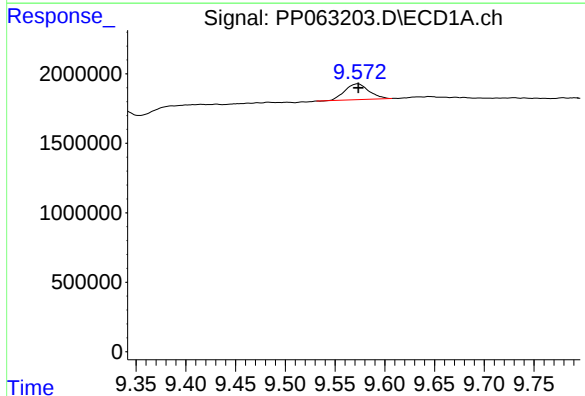


#44 AR-1268-4

R.T.: 9.573 min
Delta R.T.: 0.000 min
Response: 1897051
Conc: 24.53 ng/ml

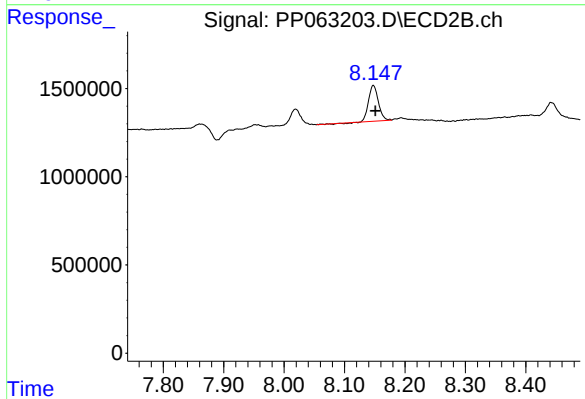

#44 AR-1268-4


R.T.: 8.148 min
Delta R.T.: -0.003 min
Response: 2266588
Conc: 25.82 ng/ml

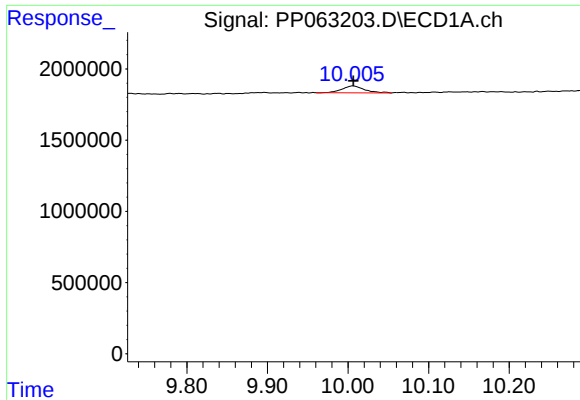

#45 AR-1268-5

R.T.: 10.006 min
Delta R.T.: 0.000 min
Response: 923954
Conc: 1.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

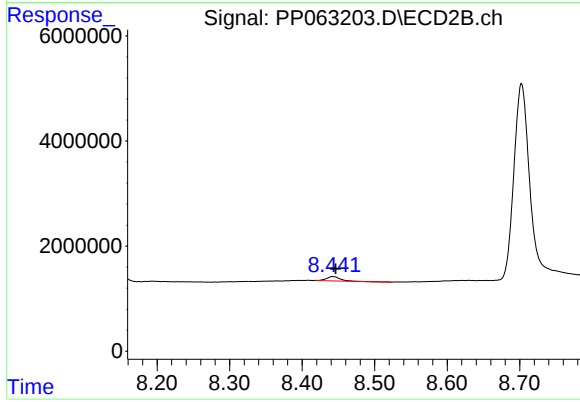

#45 AR-1268-5

R.T.: 8.442 min
Delta R.T.: -0.004 min
Response: 1064896
Conc: 1.26 ng/ml