

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020124\
 Data File : PP063245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Feb 2024 10:38
 Operator : YP\AJ
 Sample : P1187-09
 Misc : AR1660 MDL 25 PPB
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 01:41:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 02 09:02:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.491	3.646	42181901	41301921	17.635	17.376
2)	SA Decachlor...	10.362	8.696	44493507	47778409	19.785	19.288
Target Compounds							
3)	L1 AR-1016-1	5.673	4.741	1621195	1552969	21.544	21.708
4)	L1 AR-1016-2	5.696	4.759	2272863	2083910	20.927	20.289
5)	L1 AR-1016-3	5.759	4.936	1523318	1153278	22.074	20.855
6)	L1 AR-1016-4	5.858	4.979	1111189	1125525	19.841	22.744
7)	L1 AR-1016-5	6.156	5.193	1416434	1469589	23.197	23.362
9)	L2 AR-1221-2	4.801	3.948	960902	683750	45.039	34.617
10)	L2 AR-1221-3	4.866	4.025	892459	885303	14.488	14.541
11)	L3 AR-1232-1	4.866	4.025	892459	885303	16.809	16.472
12)	L3 AR-1232-2	5.403	4.759	1262847	2083910	41.744	43.487
13)	L3 AR-1232-3	5.696	4.936	2272863	1153278	44.599	44.398
14)	L3 AR-1232-4	5.858	5.021	1111189	1340998	42.291	51.444
15)	L3 AR-1232-5	5.950	5.193	1079971	1469589	46.844	53.900
16)	L4 AR-1242-1	5.673	4.741	1621195	1552969	28.472	28.578
17)	L4 AR-1242-2	5.696	4.759	2272863	2083910	27.723	26.757
18)	L4 AR-1242-3	5.759	4.936	1523318	1153278	29.027	27.215
19)	L4 AR-1242-4	5.858	5.021	1111189	1340998	25.878	28.713
20)	L4 AR-1242-5	6.603	5.548	383866	1209033	8.607	23.362 #
21)	L5 AR-1248-1	5.673	4.741	1621195	1552969	36.554	37.486
22)	L5 AR-1248-2	5.950	4.979	1079971	1125525	15.032	17.012
23)	L5 AR-1248-3	6.156	5.021	1416434	1340998	18.228	19.142
24)	L5 AR-1248-4	6.561	5.193	419648	1469589	5.631	18.391 #
25)	L5 AR-1248-5	6.603	0.000	383866	0	4.934	N.D. #
26)	L6 AR-1254-1	6.536	5.548	1225980	1209033	13.711	9.970 #
27)	L6 AR-1254-2	6.757	5.696	1094380	953772	8.337	8.790
28)	L6 AR-1254-3	7.125	6.119	1049923	1876583	7.853	10.946 #
29)	L6 AR-1254-4	7.414	6.362f	595767	493664	7.542	6.067
30)	L6 AR-1254-5	7.835	6.752	3278381	3235201	33.090	22.771 #
31)	L7 AR-1260-1	7.292	6.234	2841579	2996352	23.347	22.605
32)	L7 AR-1260-2	7.551	6.422	3248644	3445185	25.544	23.325
33)	L7 AR-1260-3	7.913	6.577	2576542	3030888	24.925	20.906
34)	L7 AR-1260-4	8.143	7.052	2897241	2387025	24.676	19.582
35)	L7 AR-1260-5	8.472	7.294	4394803	5420507	22.394	21.817
36)	L8 AR-1262-1	7.971	6.844	1450089	1403755	22.910	19.783
37)	L8 AR-1262-2	8.472	7.052	4394803	2387025	19.071	14.569
38)	L8 AR-1262-3	8.809	7.581	2860775	1127960	17.315	9.326 #
39)	L8 AR-1262-4	8.886	7.644	1960004	4034928	14.512	19.147 #
40)	L8 AR-1262-5	9.573	8.142	964654	1091258	13.236	13.367
41)	L9 AR-1268-1	8.809	7.581	2860775	1127960	9.823	3.507 #
42)	L9 AR-1268-2	8.886	7.644	1960004	4034928	7.764	13.502 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020124\
 Data File : PP063245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Feb 2024 10:38
 Operator : YP\AJ
 Sample : P1187-09
 Misc : AR1660 MDL 25 PPB
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 01:41:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 02 09:02:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	9.573	8.142	964654	1091258	12.474	12.431
45) L9	AR-1268-5	0.000	8.436	0	691001	N.D.	0.820 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020124\
Data File : PP063245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Feb 2024 10:38
Operator : YP\AJ
Sample : P1187-09
Misc : AR1660 MDL 25 PPB
ALS Vial : 76 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 01:41:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 02 09:02:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

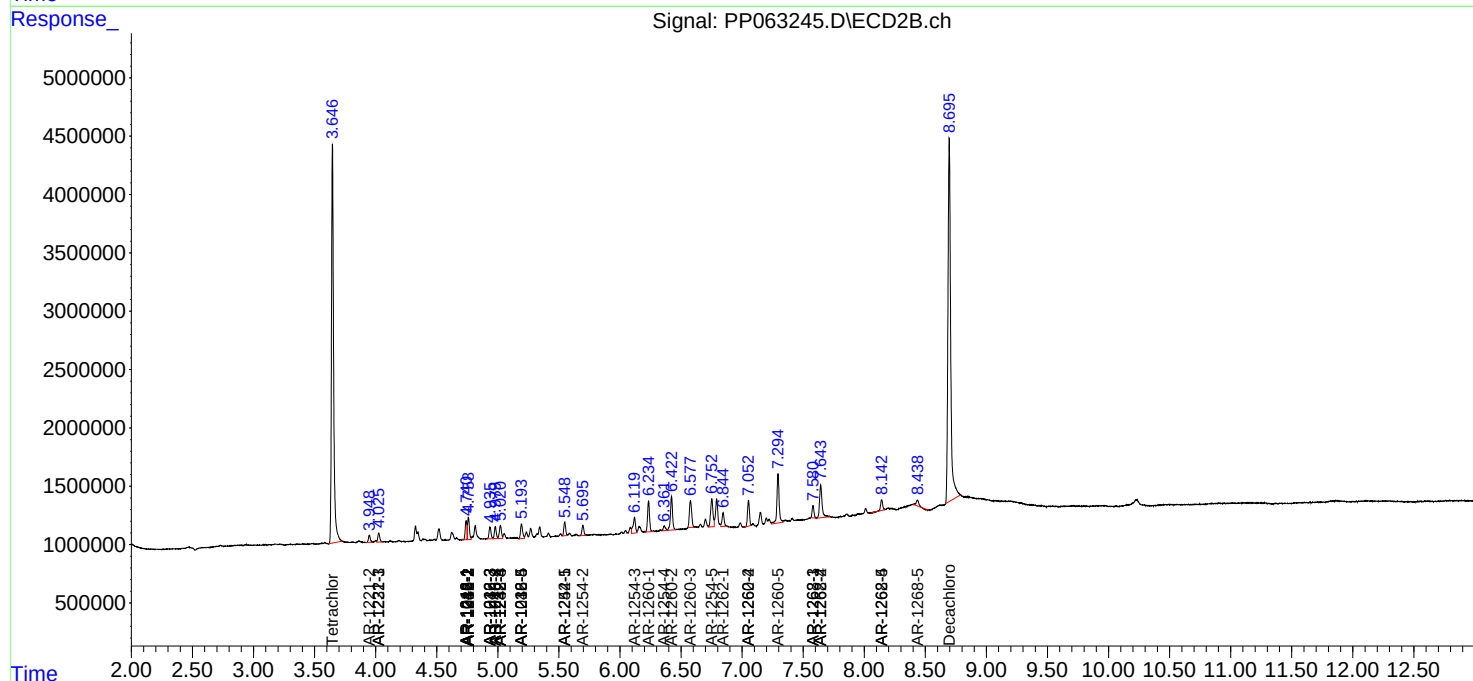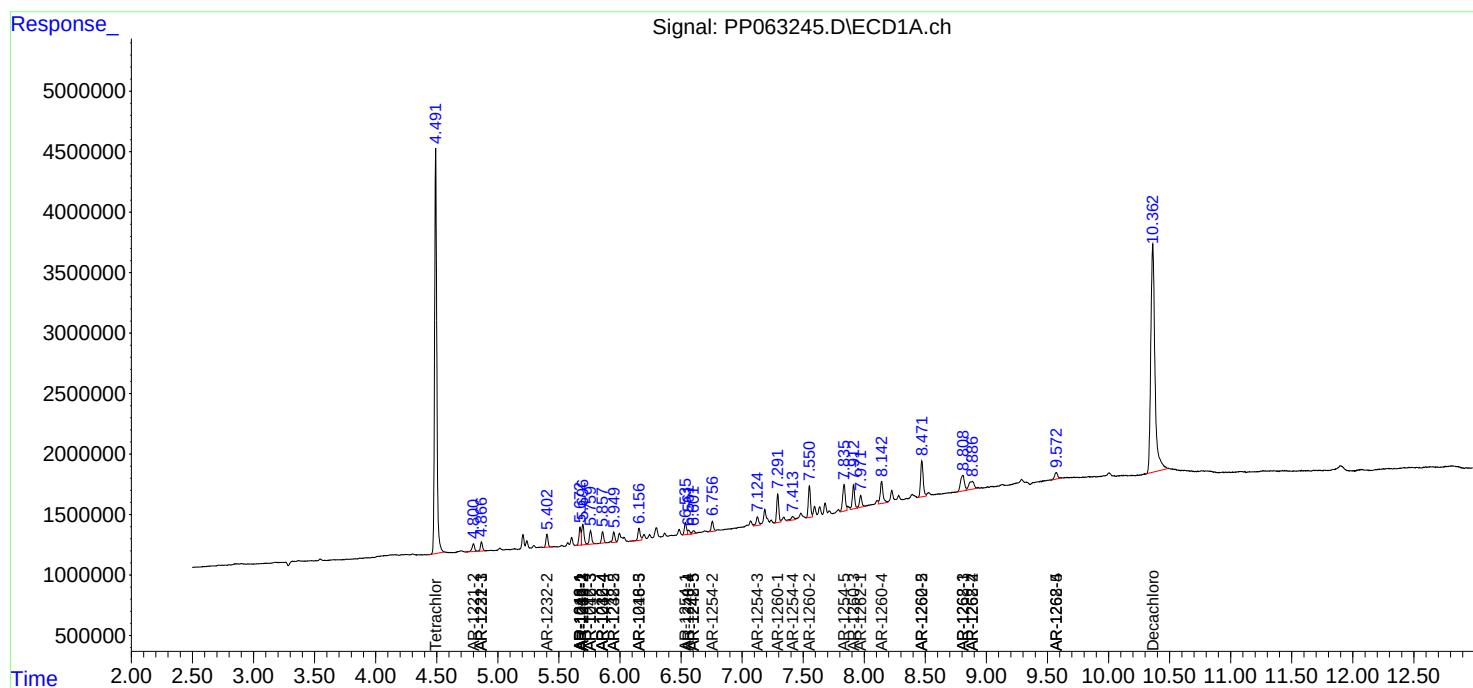


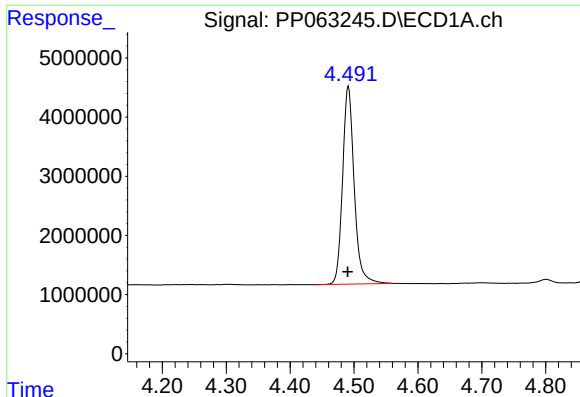

#1 Tetrachloro-m-xylene


R.T.: 4.491 min
Delta R.T.: 0.001 min
Response: 42181901
Conc: 17.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

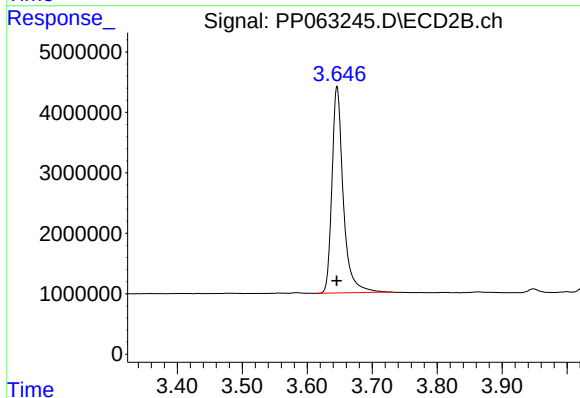


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 41301921
Conc: 17.38 ng/ml

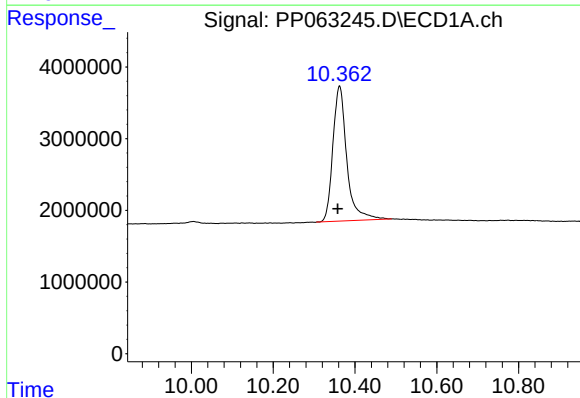


#2 Decachlorobiphenyl

R.T.: 10.362 min
Delta R.T.: 0.004 min
Response: 44493507
Conc: 19.79 ng/ml

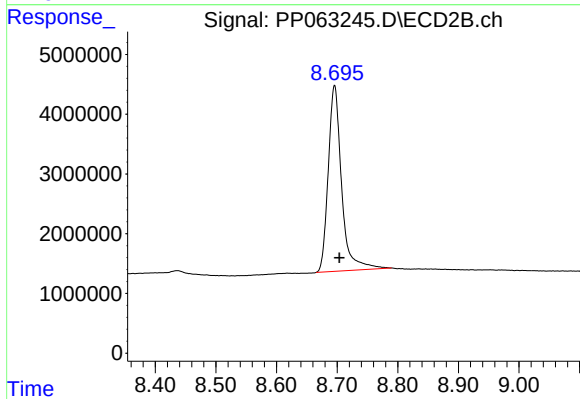

#2 Decachlorobiphenyl


R.T.: 8.696 min
Delta R.T.: -0.008 min
Response: 47778409
Conc: 19.29 ng/ml

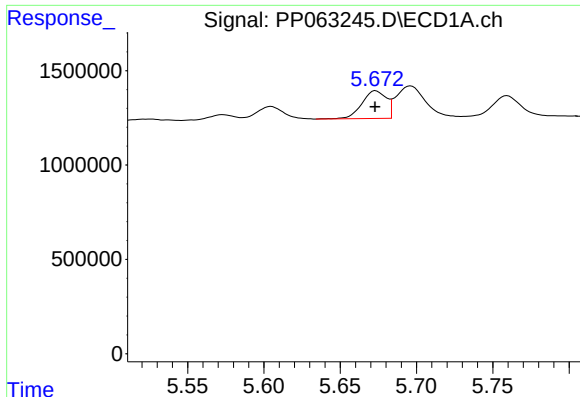

#3 AR-1016-1


R.T.: 5.673 min
Delta R.T.: 0.000 min
Response: 1621195
Conc: 21.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

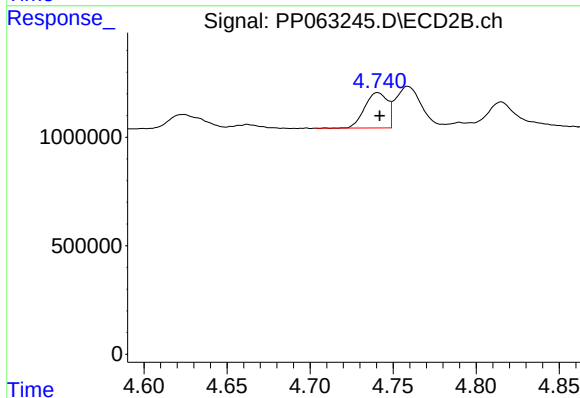


#3 AR-1016-1

R.T.: 4.741 min
Delta R.T.: -0.001 min
Response: 1552969
Conc: 21.71 ng/ml

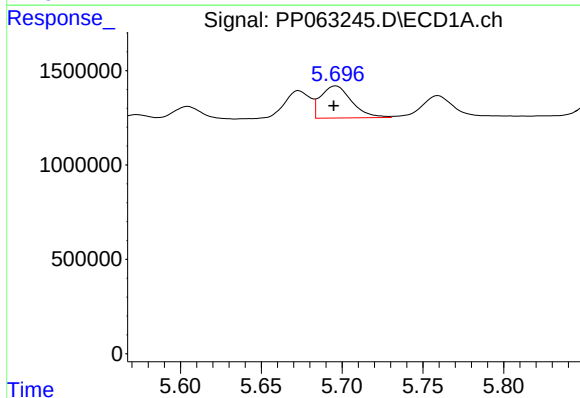


#4 AR-1016-2

R.T.: 5.696 min
Delta R.T.: 0.002 min
Response: 2272863
Conc: 20.93 ng/ml

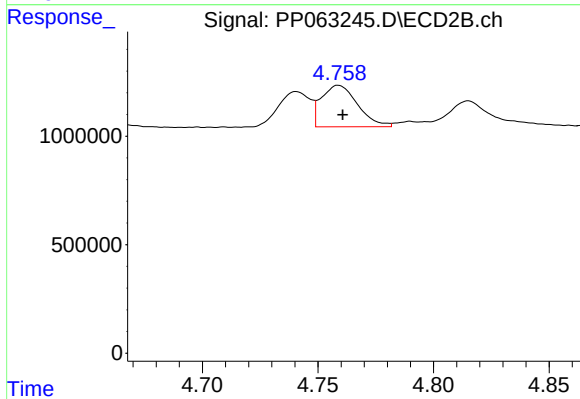

#4 AR-1016-2


R.T.: 4.759 min
Delta R.T.: -0.002 min
Response: 2083910
Conc: 20.29 ng/ml

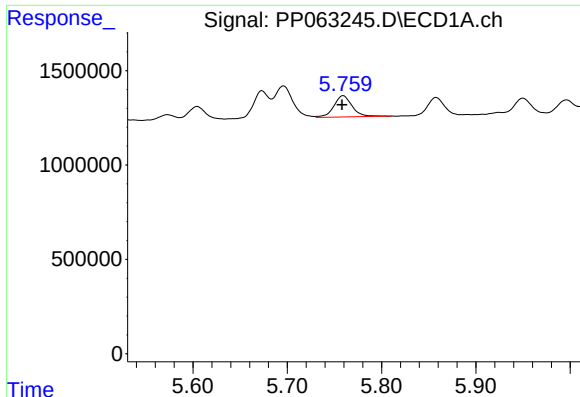

#5 AR-1016-3


R.T.: 5.759 min
Delta R.T.: 0.001 min
Response: 1523318
Conc: 22.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

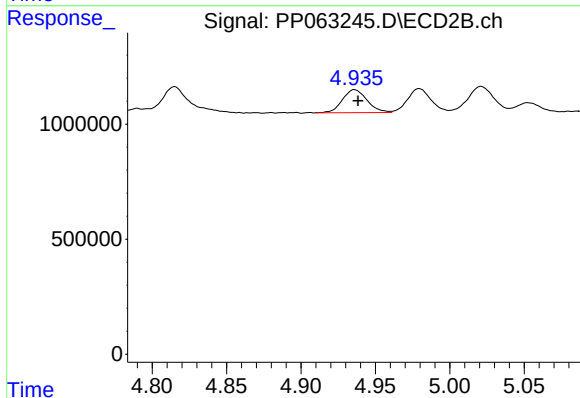


#5 AR-1016-3

R.T.: 4.936 min
Delta R.T.: -0.002 min
Response: 1153278
Conc: 20.86 ng/ml

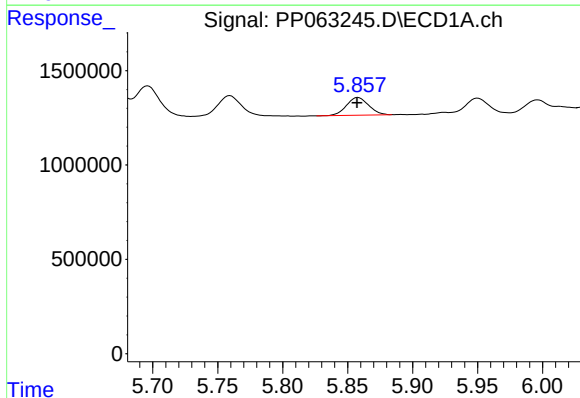


#6 AR-1016-4

R.T.: 5.858 min
Delta R.T.: 0.000 min
Response: 1111189
Conc: 19.84 ng/ml

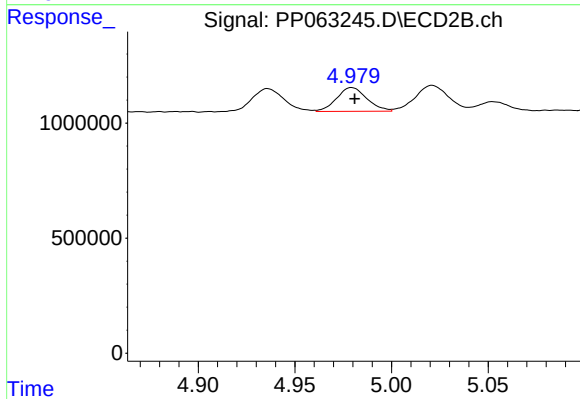

#6 AR-1016-4


R.T.: 4.979 min
Delta R.T.: -0.002 min
Response: 1125525
Conc: 22.74 ng/ml

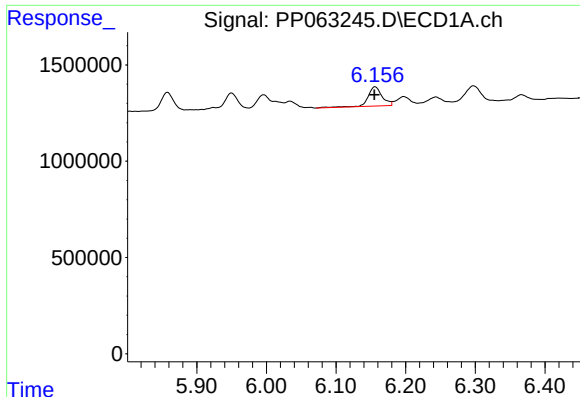

#7 AR-1016-5


R.T.: 6.156 min
Delta R.T.: 0.001 min
Response: 1416434
Conc: 23.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

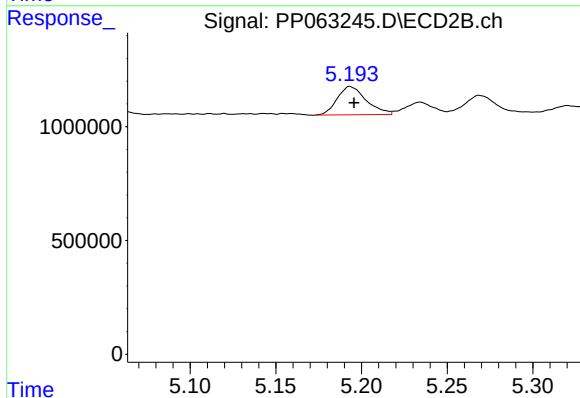


#7 AR-1016-5

R.T.: 5.193 min
Delta R.T.: -0.002 min
Response: 1469589
Conc: 23.36 ng/ml

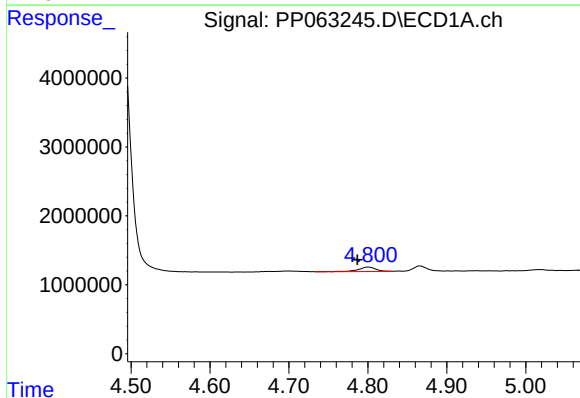


#9 AR-1221-2

R.T.: 4.801 min
Delta R.T.: 0.014 min
Response: 960902
Conc: 45.04 ng/ml

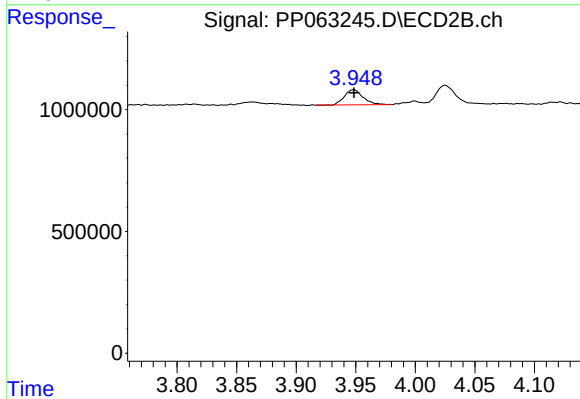

#9 AR-1221-2


R.T.: 3.948 min
Delta R.T.: 0.000 min
Response: 683750
Conc: 34.62 ng/ml

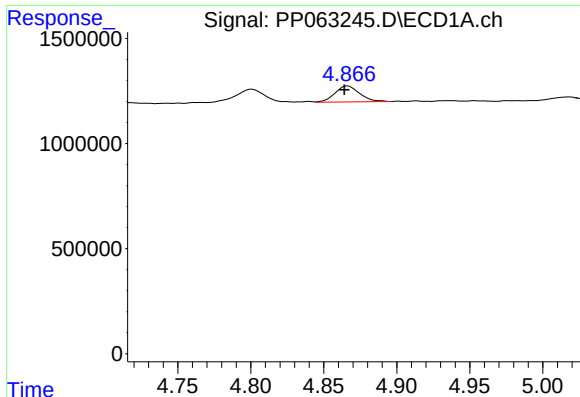

#10 AR-1221-3


R.T.: 4.866 min
Delta R.T.: 0.002 min
Response: 892459
Conc: 14.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

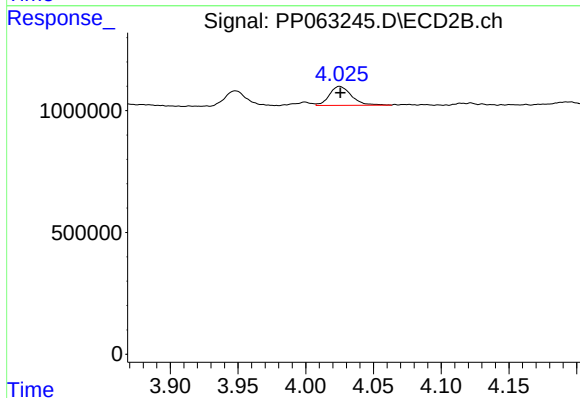


#10 AR-1221-3

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 885303
Conc: 14.54 ng/ml

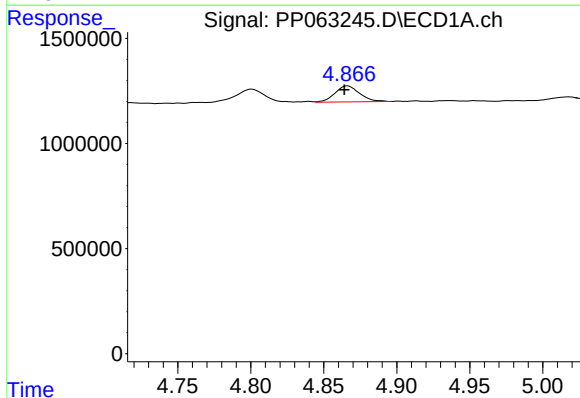


#11 AR-1232-1

R.T.: 4.866 min
Delta R.T.: 0.002 min
Response: 892459
Conc: 16.81 ng/ml

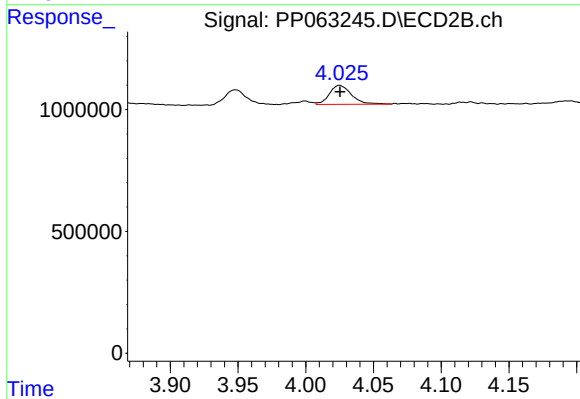

#11 AR-1232-1


R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 885303
Conc: 16.47 ng/ml

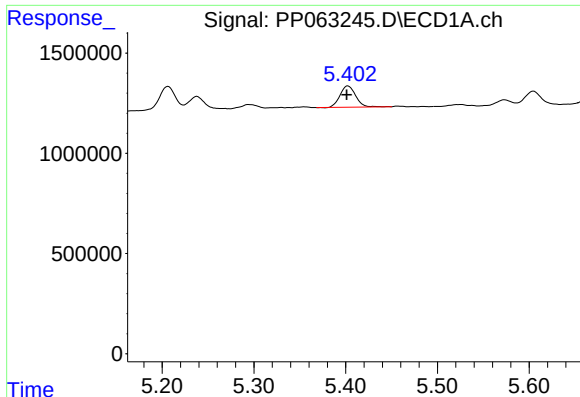

#12 AR-1232-2


R.T.: 5.403 min
Delta R.T.: 0.001 min
Response: 1262847
Conc: 41.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

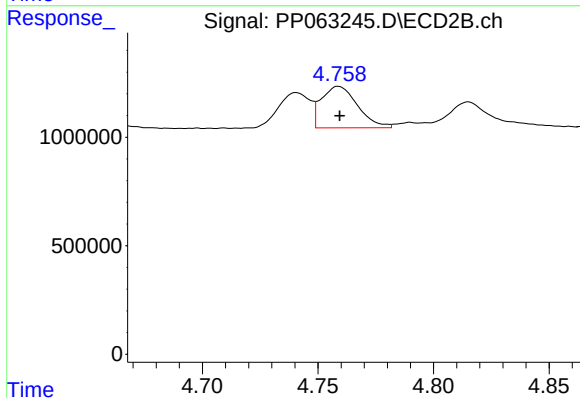


#12 AR-1232-2

R.T.: 4.759 min
Delta R.T.: 0.000 min
Response: 2083910
Conc: 43.49 ng/ml

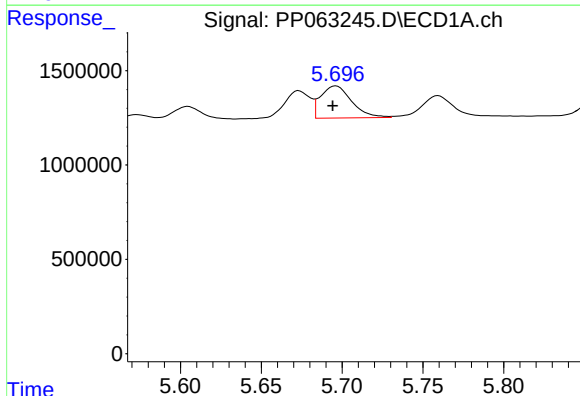


#13 AR-1232-3

R.T.: 5.696 min
Delta R.T.: 0.002 min
Response: 2272863
Conc: 44.60 ng/ml

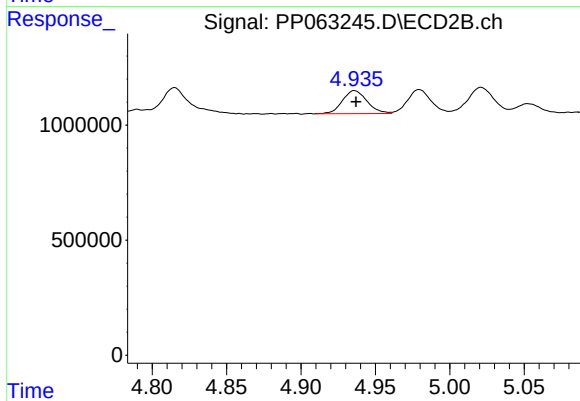

#13 AR-1232-3


R.T.: 4.936 min
Delta R.T.: -0.001 min
Response: 1153278
Conc: 44.40 ng/ml

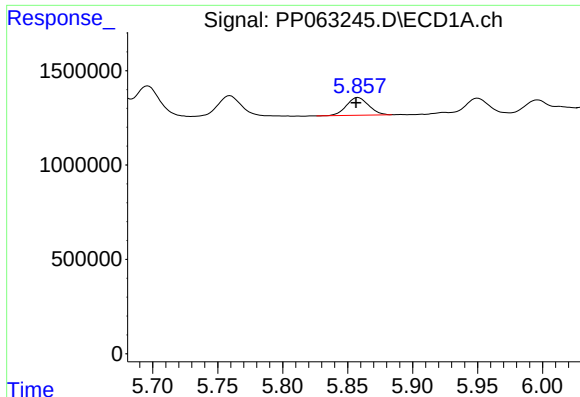

#14 AR-1232-4


R.T.: 5.858 min
Delta R.T.: 0.002 min
Response: 1111189
Conc: 42.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

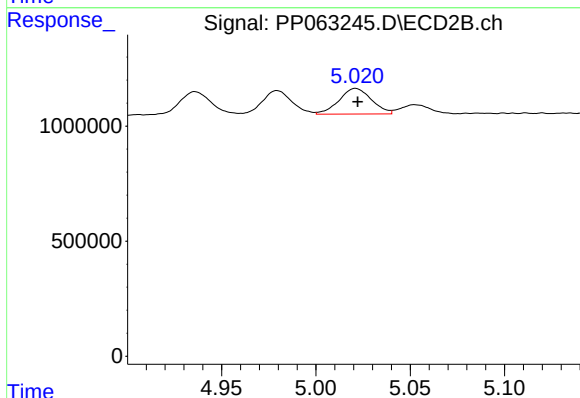


#14 AR-1232-4

R.T.: 5.021 min
Delta R.T.: -0.001 min
Response: 1340998
Conc: 51.44 ng/ml

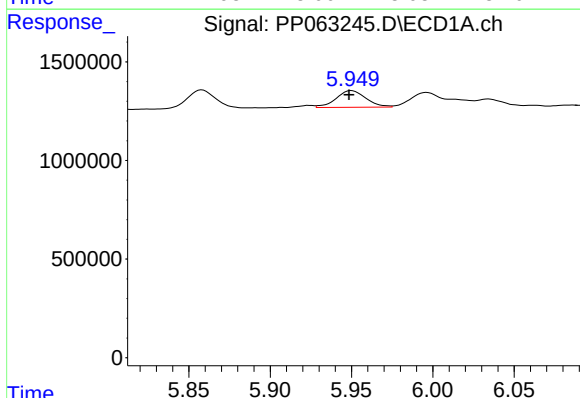


#15 AR-1232-5

R.T.: 5.950 min
Delta R.T.: 0.002 min
Response: 1079971
Conc: 46.84 ng/ml

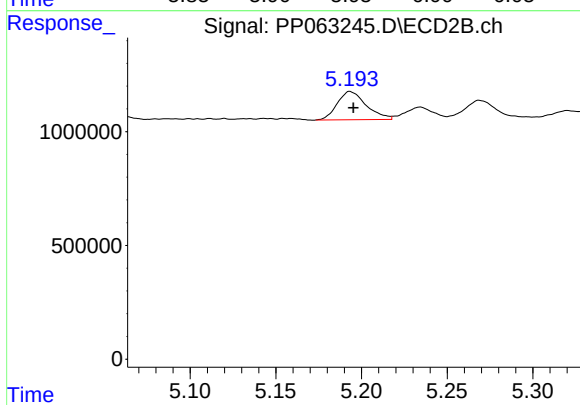

#15 AR-1232-5


R.T.: 5.193 min
Delta R.T.: -0.002 min
Response: 1469589
Conc: 53.90 ng/ml

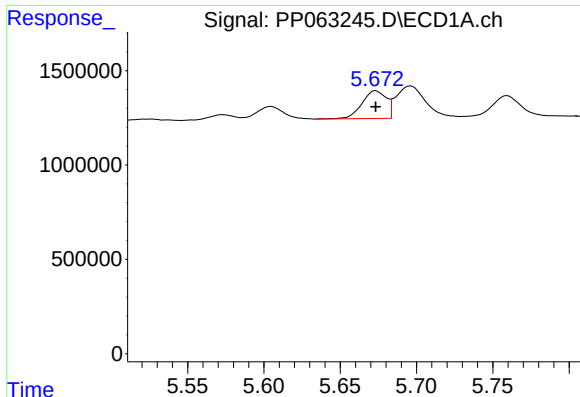

#16 AR-1242-1


R.T.: 5.673 min
Delta R.T.: 0.000 min
Response: 1621195
Conc: 28.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

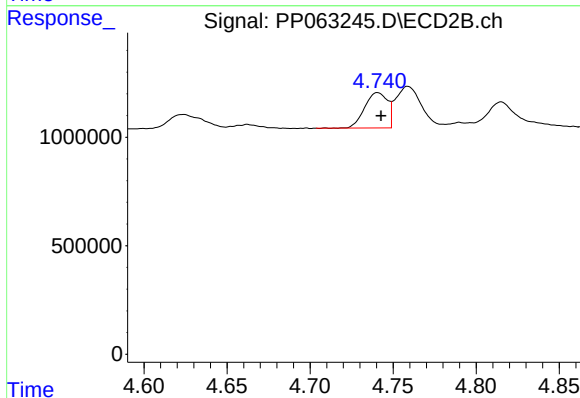


#16 AR-1242-1

R.T.: 4.741 min
Delta R.T.: -0.002 min
Response: 1552969
Conc: 28.58 ng/ml

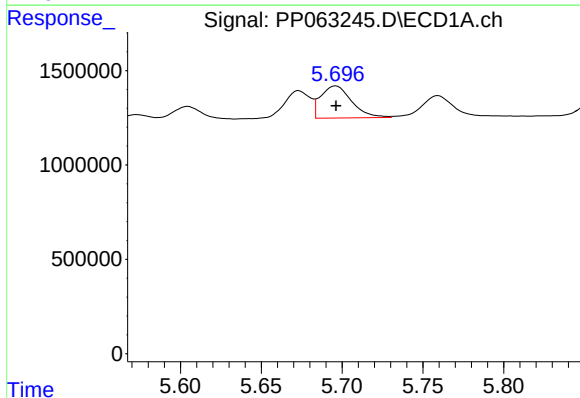


#17 AR-1242-2

R.T.: 5.696 min
Delta R.T.: 0.000 min
Response: 2272863
Conc: 27.72 ng/ml

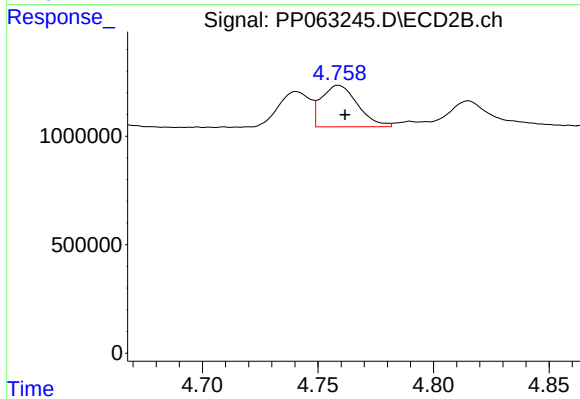

#17 AR-1242-2


R.T.: 4.759 min
Delta R.T.: -0.003 min
Response: 2083910
Conc: 26.76 ng/ml

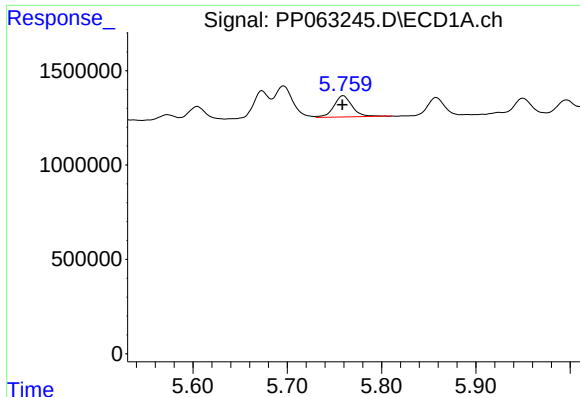

#18 AR-1242-3


R.T.: 5.759 min
Delta R.T.: 0.001 min
Response: 1523318
Conc: 29.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

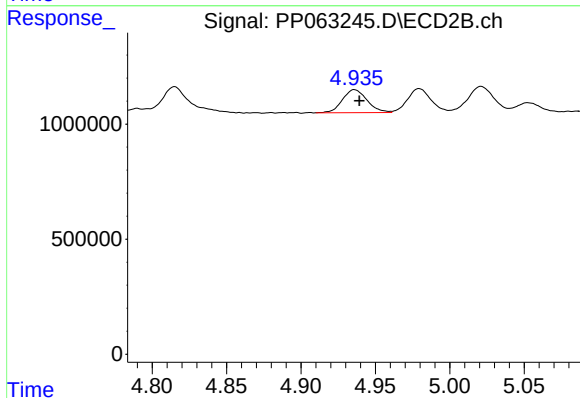


#18 AR-1242-3

R.T.: 4.936 min
Delta R.T.: -0.003 min
Response: 1153278
Conc: 27.21 ng/ml

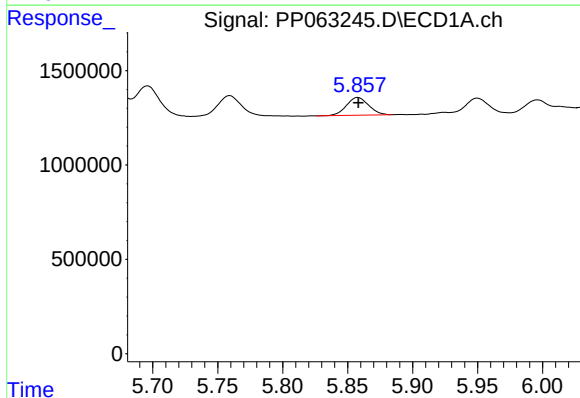


#19 AR-1242-4

R.T.: 5.858 min
Delta R.T.: 0.000 min
Response: 1111189
Conc: 25.88 ng/ml

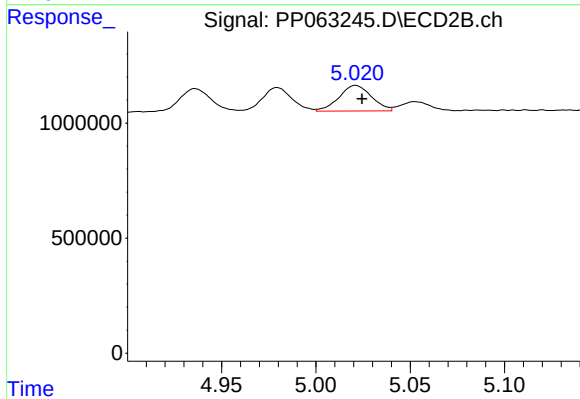

#19 AR-1242-4


R.T.: 5.021 min
Delta R.T.: -0.003 min
Response: 1340998
Conc: 28.71 ng/ml

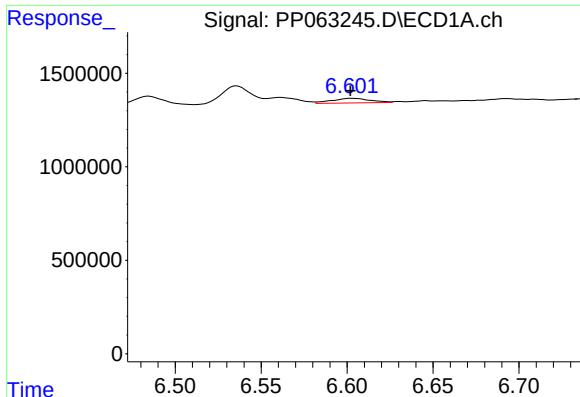

#20 AR-1242-5


R.T.: 6.603 min
Delta R.T.: 0.000 min
Response: 383866
Conc: 8.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

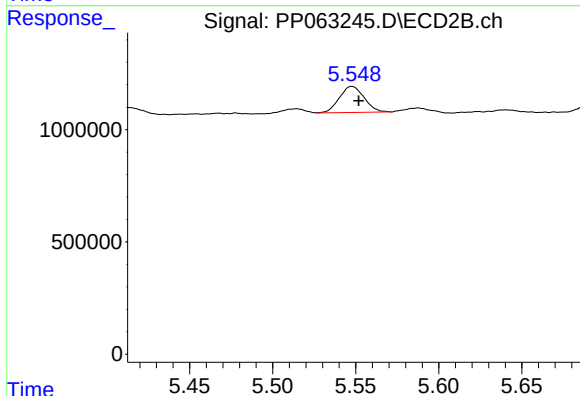


#20 AR-1242-5

R.T.: 5.548 min
Delta R.T.: -0.004 min
Response: 1209033
Conc: 23.36 ng/ml

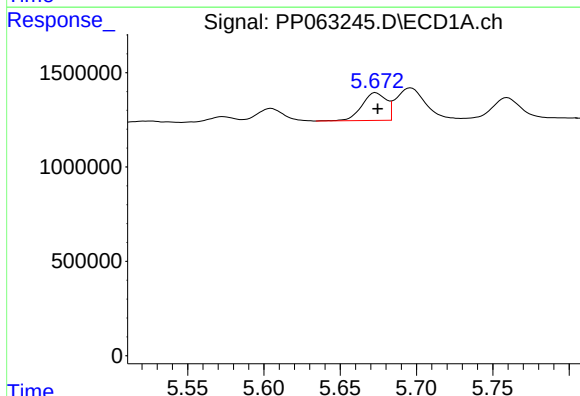


#21 AR-1248-1

R.T.: 5.673 min
Delta R.T.: -0.001 min
Response: 1621195
Conc: 36.55 ng/ml

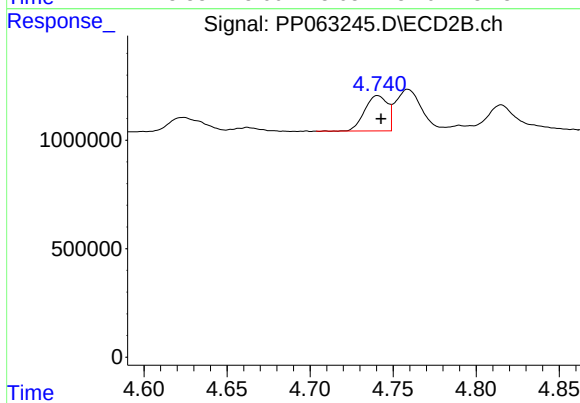

#21 AR-1248-1


R.T.: 4.741 min
Delta R.T.: -0.002 min
Response: 1552969
Conc: 37.49 ng/ml

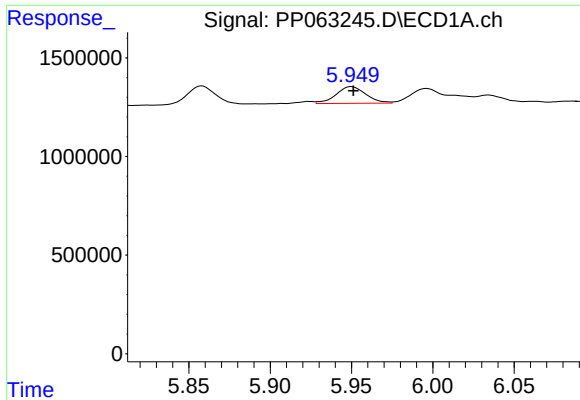

#22 AR-1248-2


R.T.: 5.950 min
Delta R.T.: -0.001 min
Response: 1079971
Conc: 15.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

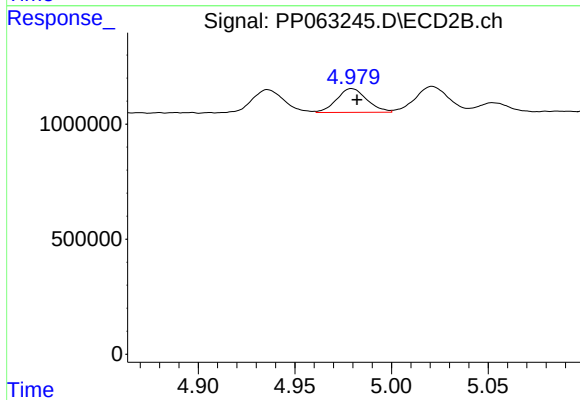


#22 AR-1248-2

R.T.: 4.979 min
Delta R.T.: -0.003 min
Response: 1125525
Conc: 17.01 ng/ml

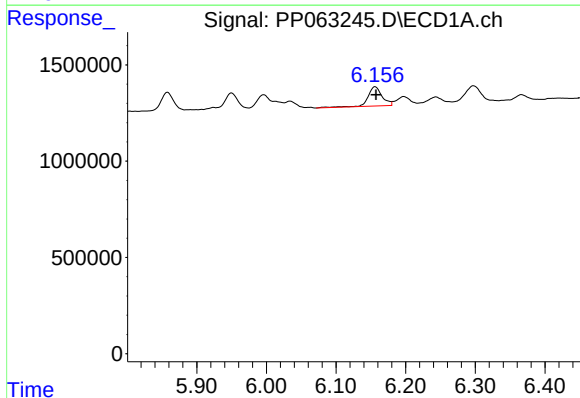


#23 AR-1248-3

R.T.: 6.156 min
Delta R.T.: -0.001 min
Response: 1416434
Conc: 18.23 ng/ml

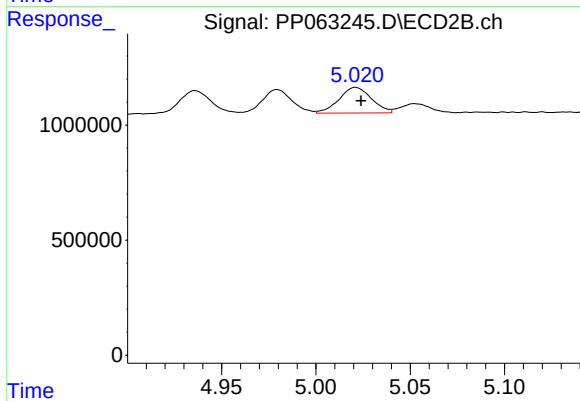

#23 AR-1248-3


R.T.: 5.021 min
Delta R.T.: -0.003 min
Response: 1340998
Conc: 19.14 ng/ml

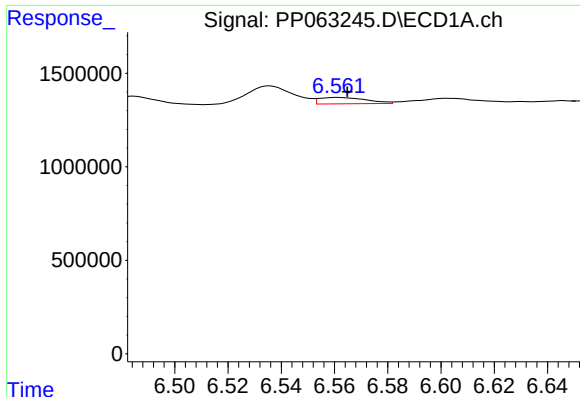

#24 AR-1248-4


R.T.: 6.561 min
Delta R.T.: -0.003 min
Response: 419648
Conc: 5.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

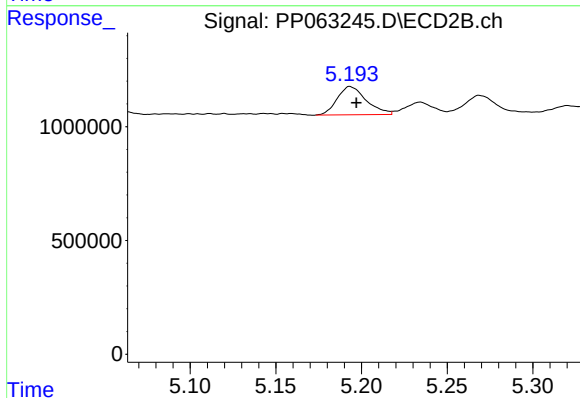


#24 AR-1248-4

R.T.: 5.193 min
Delta R.T.: -0.004 min
Response: 1469589
Conc: 18.39 ng/ml

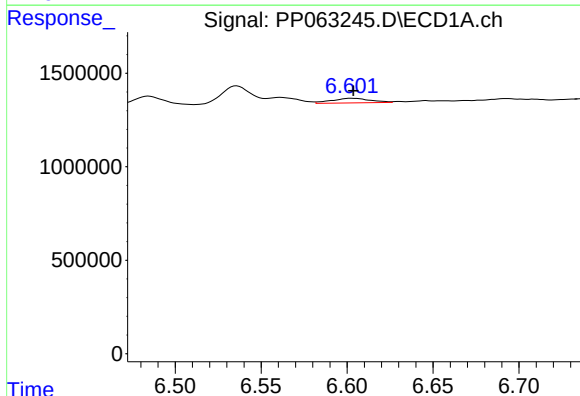


#25 AR-1248-5

R.T.: 6.603 min
Delta R.T.: -0.001 min
Response: 383866
Conc: 4.93 ng/ml

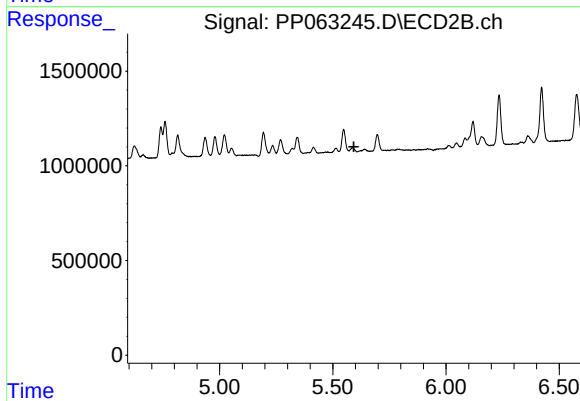

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 5.593 min
Response: 0
Conc: N.D.

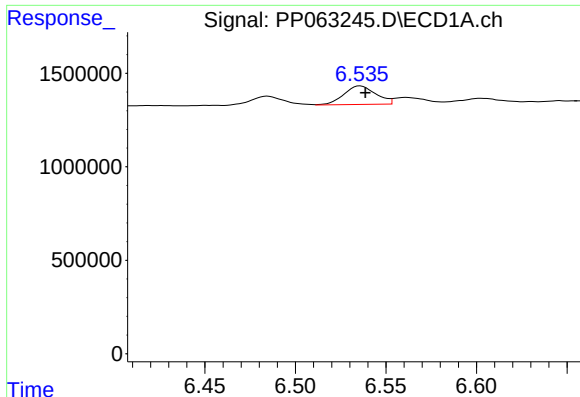

#26 AR-1254-1


R.T.: 6.536 min
Delta R.T.: -0.003 min
Response: 1225980
Conc: 13.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

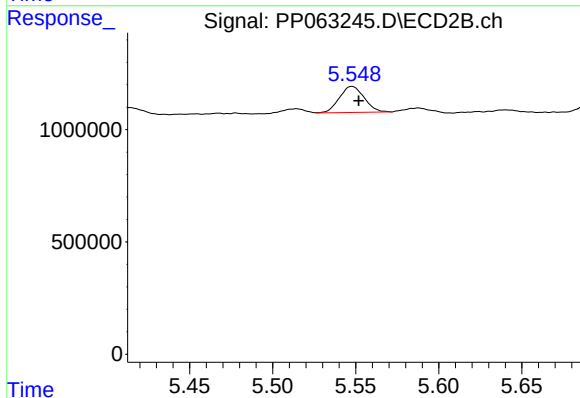


#26 AR-1254-1

R.T.: 5.548 min
Delta R.T.: -0.004 min
Response: 1209033
Conc: 9.97 ng/ml

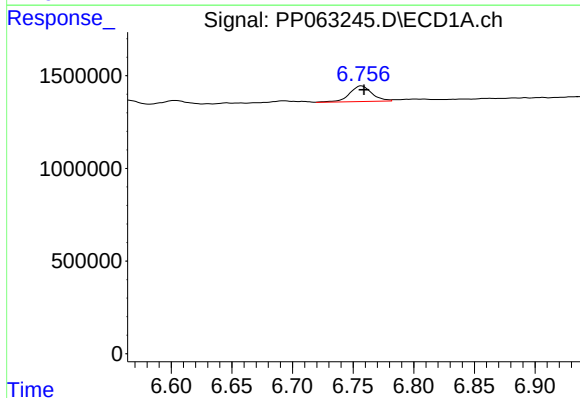


#27 AR-1254-2

R.T.: 6.757 min
Delta R.T.: -0.002 min
Response: 1094380
Conc: 8.34 ng/ml

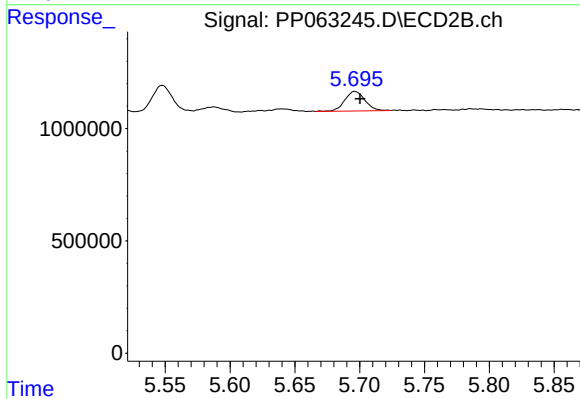

#27 AR-1254-2


R.T.: 5.696 min
Delta R.T.: -0.004 min
Response: 953772
Conc: 8.79 ng/ml

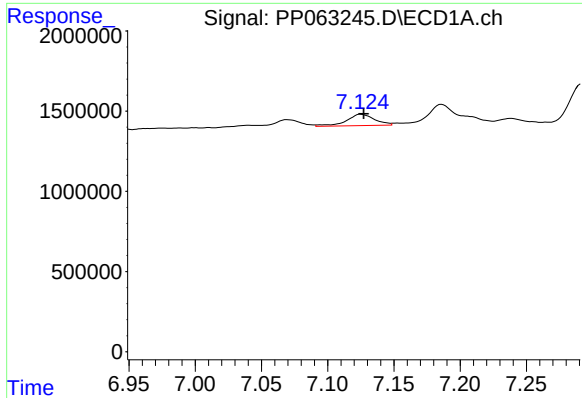

#28 AR-1254-3


R.T.: 7.125 min
Delta R.T.: -0.002 min
Response: 1049923
Conc: 7.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

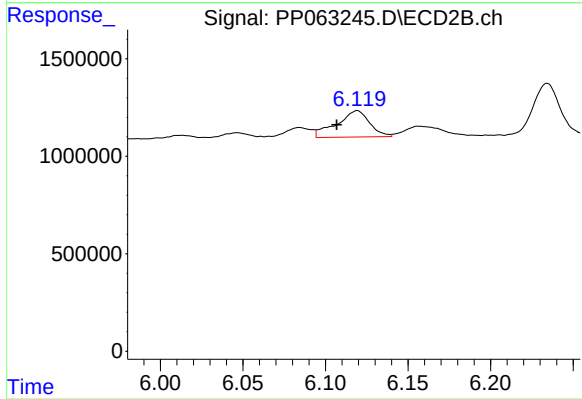


#28 AR-1254-3

R.T.: 6.119 min
Delta R.T.: 0.012 min
Response: 1876583
Conc: 10.95 ng/ml

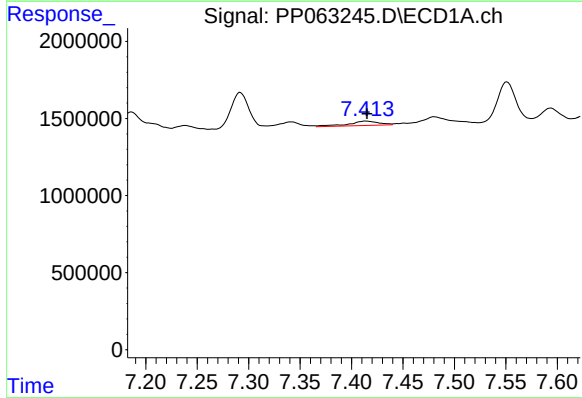


#29 AR-1254-4

R.T.: 7.414 min
Delta R.T.: -0.001 min
Response: 595767
Conc: 7.54 ng/ml

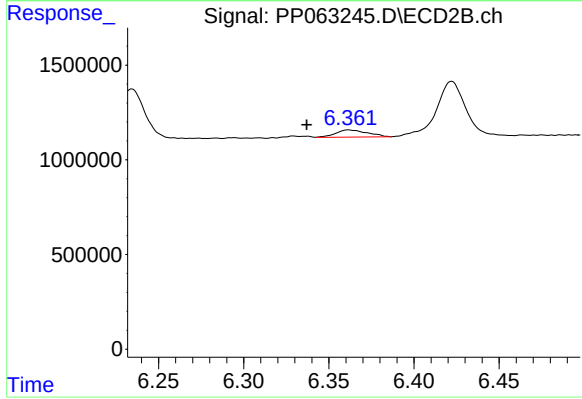

#29 AR-1254-4


R.T.: 6.362 min
Delta R.T.: 0.025 min
Response: 493664
Conc: 6.07 ng/ml

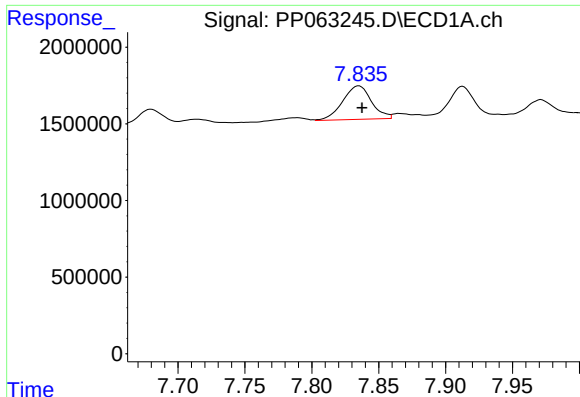

#30 AR-1254-5


R.T.: 7.835 min
Delta R.T.: -0.002 min
Response: 3278381
Conc: 33.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

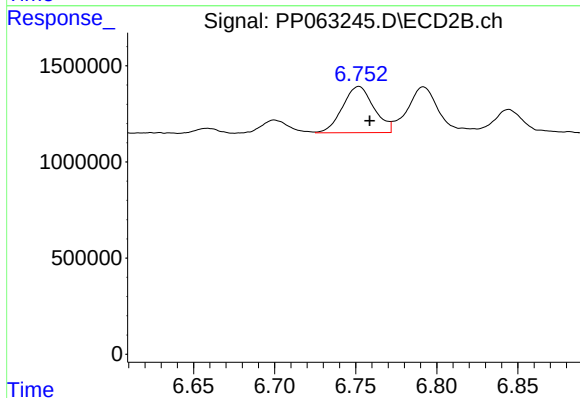


#30 AR-1254-5

R.T.: 6.752 min
Delta R.T.: -0.007 min
Response: 3235201
Conc: 22.77 ng/ml

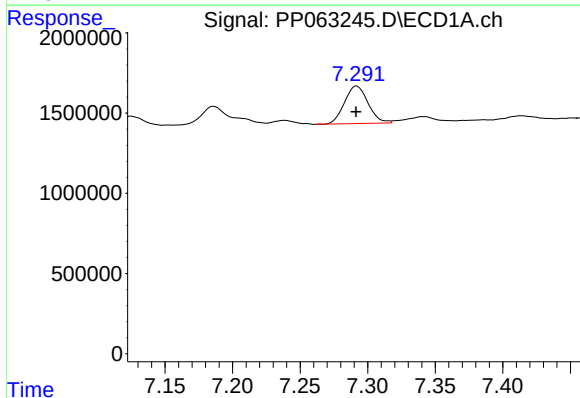


#31 AR-1260-1

R.T.: 7.292 min
Delta R.T.: 0.000 min
Response: 2841579
Conc: 23.35 ng/ml

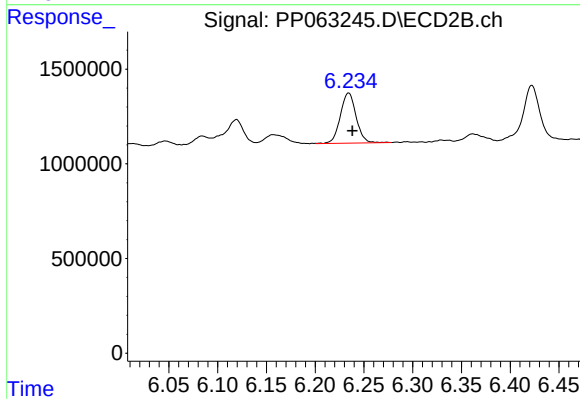

#31 AR-1260-1


R.T.: 6.234 min
Delta R.T.: -0.004 min
Response: 2996352
Conc: 22.61 ng/ml

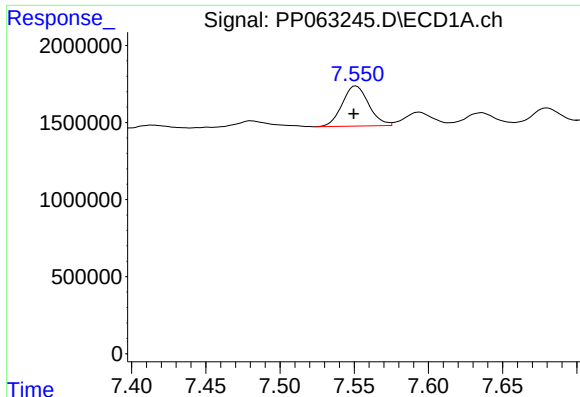

#32 AR-1260-2


R.T.: 7.551 min
Delta R.T.: 0.001 min
Response: 3248644
Conc: 25.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

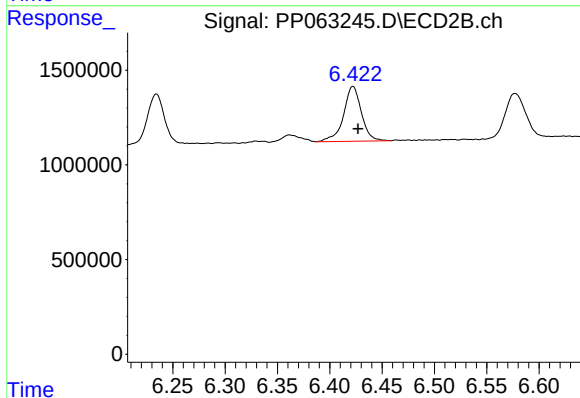


#32 AR-1260-2

R.T.: 6.422 min
Delta R.T.: -0.005 min
Response: 3445185
Conc: 23.33 ng/ml

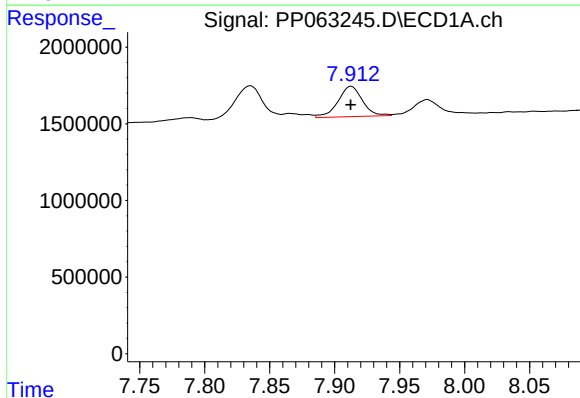


#33 AR-1260-3

R.T.: 7.913 min
Delta R.T.: 0.000 min
Response: 2576542
Conc: 24.92 ng/ml

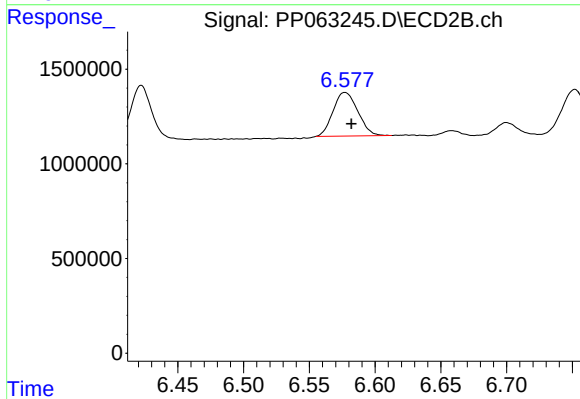

#33 AR-1260-3


R.T.: 6.577 min
Delta R.T.: -0.005 min
Response: 3030888
Conc: 20.91 ng/ml

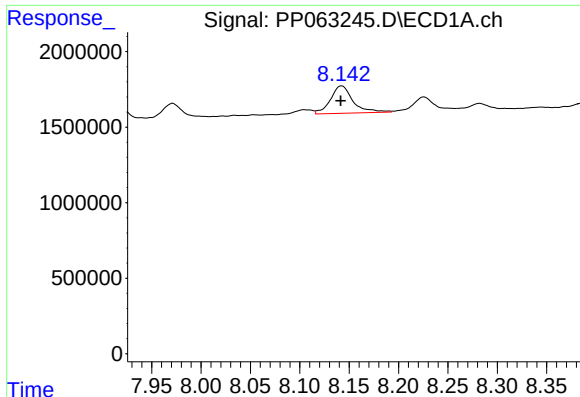

#34 AR-1260-4


R.T.: 8.143 min
Delta R.T.: 0.001 min
Response: 2897241
Conc: 24.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

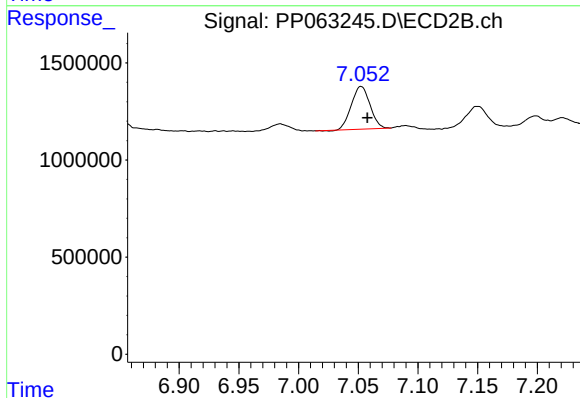


#34 AR-1260-4

R.T.: 7.052 min
Delta R.T.: -0.005 min
Response: 2387025
Conc: 19.58 ng/ml

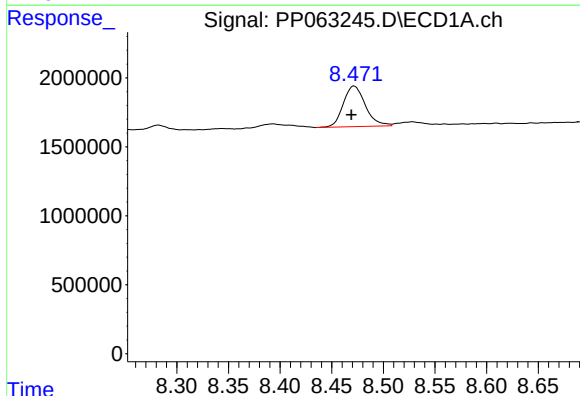


#35 AR-1260-5

R.T.: 8.472 min
Delta R.T.: 0.003 min
Response: 4394803
Conc: 22.39 ng/ml

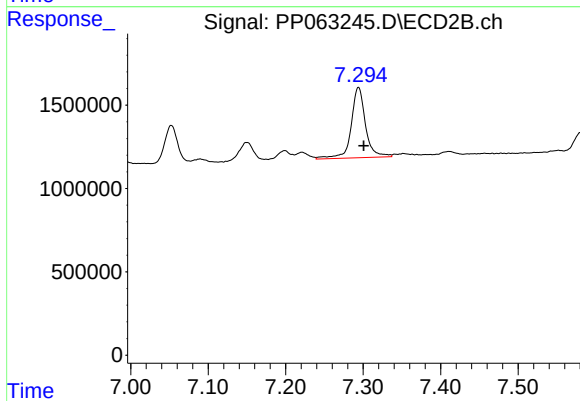

#35 AR-1260-5


R.T.: 7.294 min
Delta R.T.: -0.007 min
Response: 5420507
Conc: 21.82 ng/ml

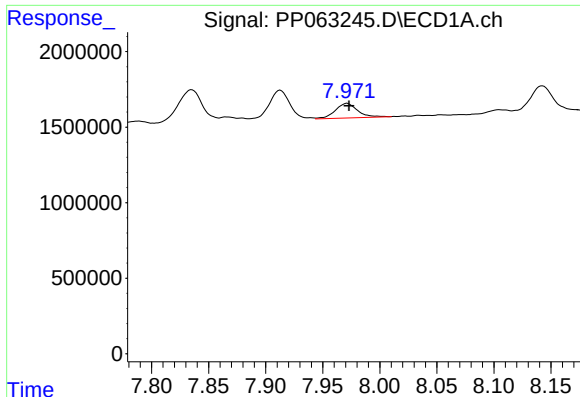

#36 AR-1262-1


R.T.: 7.971 min
Delta R.T.: -0.002 min
Response: 1450089
Conc: 22.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

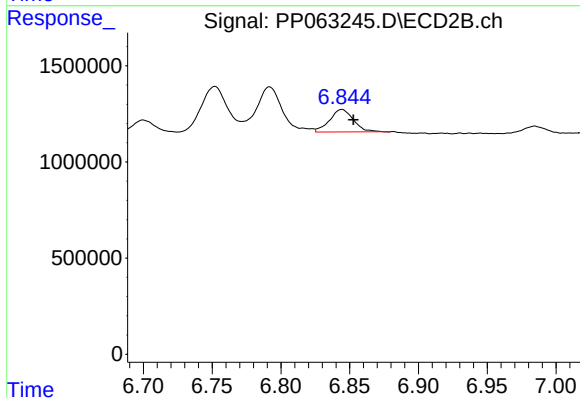


#36 AR-1262-1

R.T.: 6.844 min
Delta R.T.: -0.009 min
Response: 1403755
Conc: 19.78 ng/ml

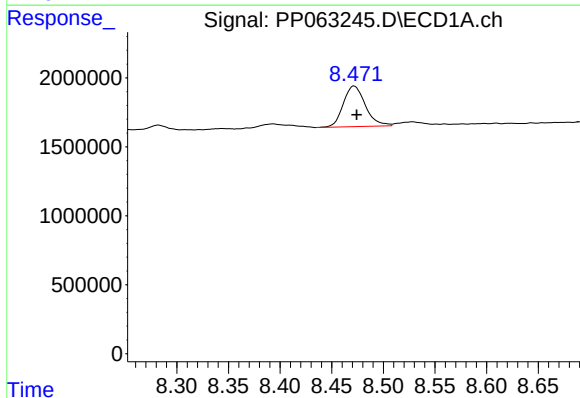


#37 AR-1262-2

R.T.: 8.472 min
Delta R.T.: -0.002 min
Response: 4394803
Conc: 19.07 ng/ml

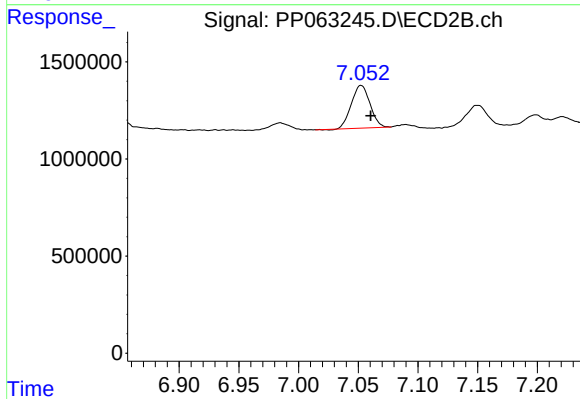

#37 AR-1262-2


R.T.: 7.052 min
Delta R.T.: -0.008 min
Response: 2387025
Conc: 14.57 ng/ml

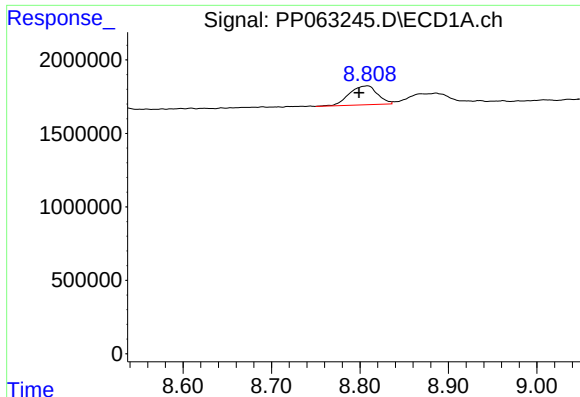

#38 AR-1262-3


R.T.: 8.809 min
Delta R.T.: 0.010 min
Response: 2860775
Conc: 17.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

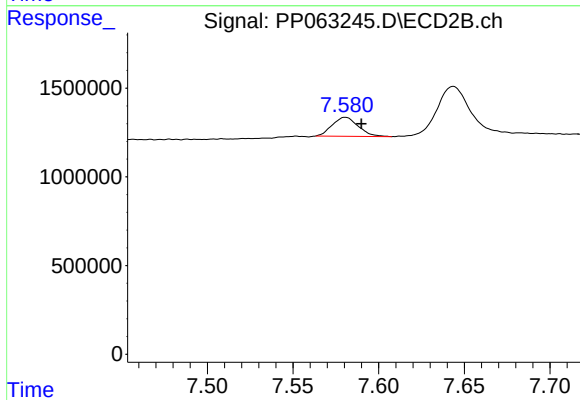


#38 AR-1262-3

R.T.: 7.581 min
Delta R.T.: -0.009 min
Response: 1127960
Conc: 9.33 ng/ml

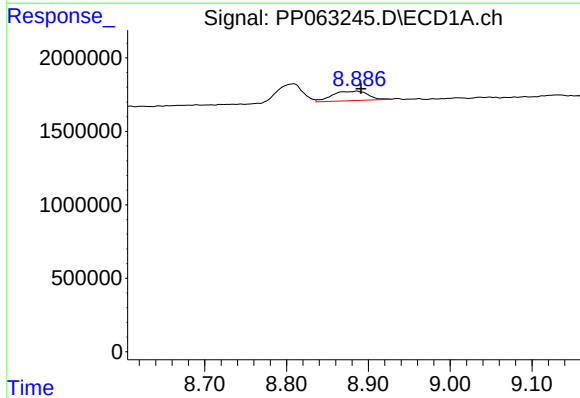


#39 AR-1262-4

R.T.: 8.886 min
Delta R.T.: -0.005 min
Response: 1960004
Conc: 14.51 ng/ml

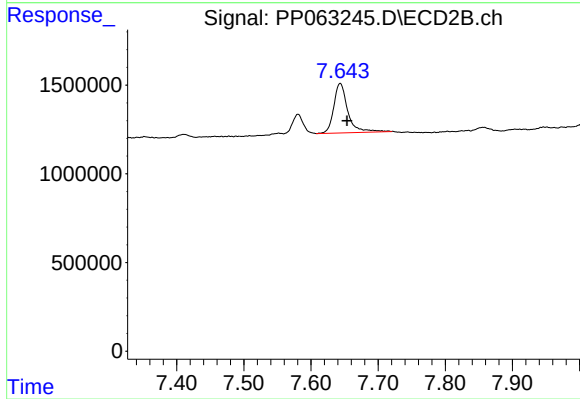

#39 AR-1262-4


R.T.: 7.644 min
Delta R.T.: -0.010 min
Response: 4034928
Conc: 19.15 ng/ml

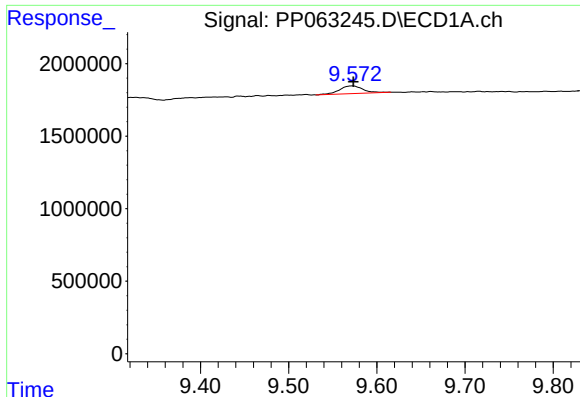

#40 AR-1262-5


R.T.: 9.573 min
Delta R.T.: 0.000 min
Response: 964654
Conc: 13.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

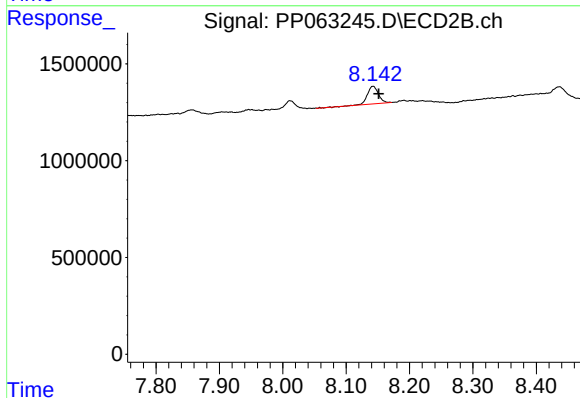


#40 AR-1262-5

R.T.: 8.142 min
Delta R.T.: -0.009 min
Response: 1091258
Conc: 13.37 ng/ml

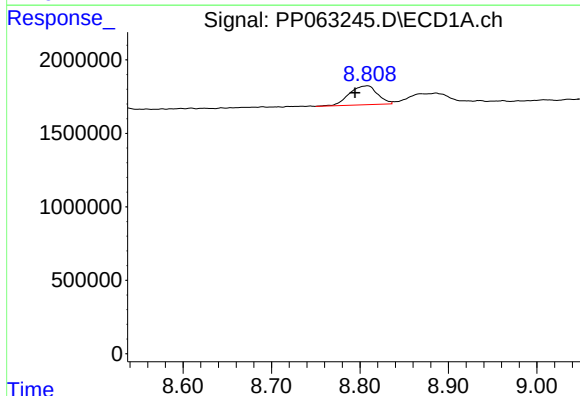


#41 AR-1268-1

R.T.: 8.809 min
Delta R.T.: 0.014 min
Response: 2860775
Conc: 9.82 ng/ml

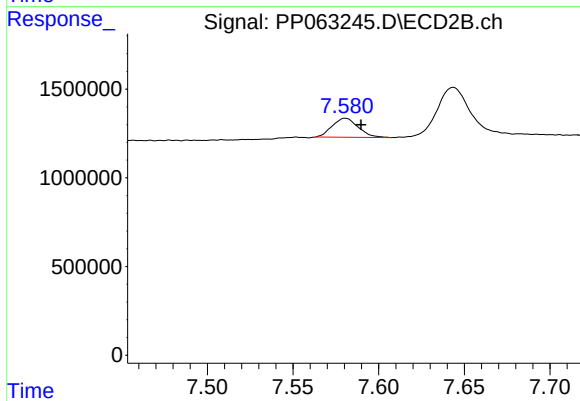

#41 AR-1268-1


R.T.: 7.581 min
Delta R.T.: -0.009 min
Response: 1127960
Conc: 3.51 ng/ml

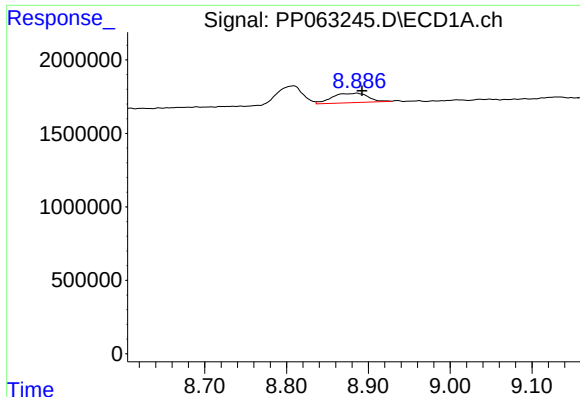

#42 AR-1268-2


R.T.: 8.886 min
Delta R.T.: -0.006 min
Response: 1960004
Conc: 7.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

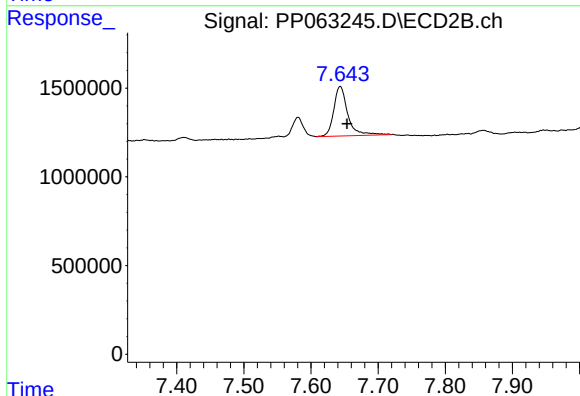


#42 AR-1268-2

R.T.: 7.644 min
Delta R.T.: -0.010 min
Response: 4034928
Conc: 13.50 ng/ml

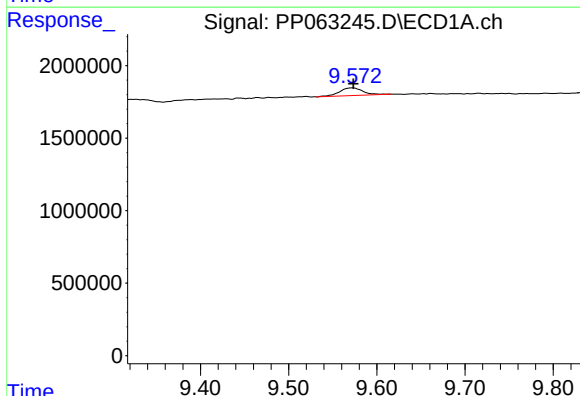


#44 AR-1268-4

R.T.: 9.573 min
Delta R.T.: 0.000 min
Response: 964654
Conc: 12.47 ng/ml

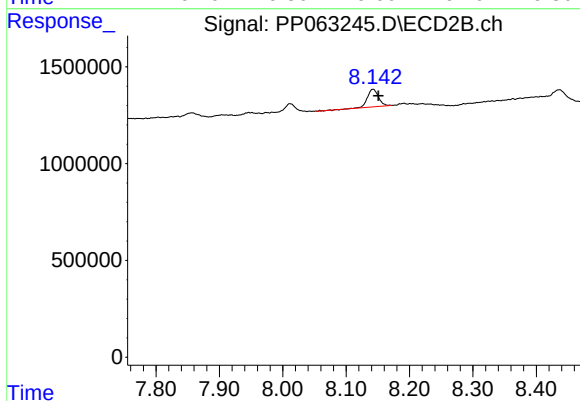

#44 AR-1268-4


R.T.: 8.142 min
Delta R.T.: -0.009 min
Response: 1091258
Conc: 12.43 ng/ml

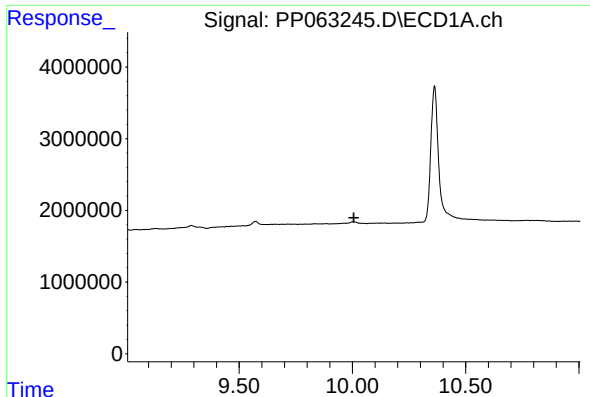

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.007 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

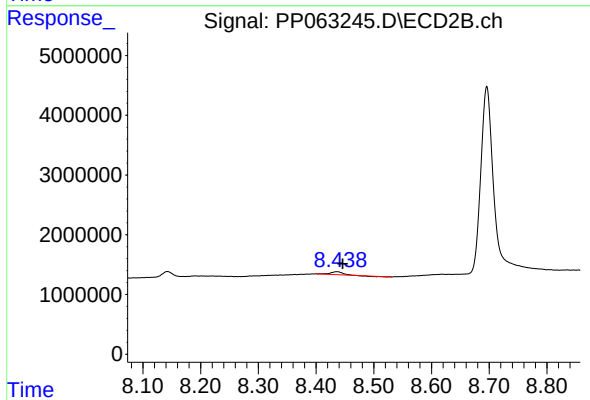

#45 AR-1268-5

R.T.: 8.436 min
Delta R.T.: -0.010 min
Response: 691001
Conc: 0.82 ng/ml