

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020124\
 Data File : PP063247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Feb 2024 11:11
 Operator : YP\AJ
 Sample : P1187-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 01:43:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 02 09:02:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.491	3.645	37294139	36153568	15.591	15.210
2)	SA Decachlor...	10.361	8.696	47569370	50138646	21.153	20.241
Target Compounds							
3)	L1 AR-1016-1	5.673	4.740	645934	753994	8.584	10.539
4)	L1 AR-1016-2	5.696	4.759	921551	858327	8.485	8.357
5)	L1 AR-1016-3	5.758	4.936	694468	707840	10.063	12.800 #
6)	L1 AR-1016-4	5.860	4.979	412147	282892	7.359	5.716
7)	L1 AR-1016-5	6.156	5.195	716800	884428	11.739	14.060
8)	L2 AR-1221-1	4.701	3.862	5082989	453968	182.673	17.168 #
9)	L2 AR-1221-2	4.801	3.948	1271108	600362	59.579	30.395 #
10)	L2 AR-1221-3	4.866	4.025	1086460	815108	17.637	13.388
11)	L3 AR-1232-1	4.866	4.025	1086460	815108	20.463	15.166 #
12)	L3 AR-1232-2	5.403	4.759	446044	858327	14.744	17.912
13)	L3 AR-1232-3	5.696	4.936	921551	707840	18.083	27.250 #
14)	L3 AR-1232-4	5.860	5.021	412147	399464	15.686	15.324
15)	L3 AR-1232-5	5.948	5.195	535071	884428	23.209	32.438 #
16)	L4 AR-1242-1	5.673	4.740	645934	753994	11.344	13.875
17)	L4 AR-1242-2	5.696	4.759	921551	858327	11.240	11.021
18)	L4 AR-1242-3	5.758	4.936	694468	707840	13.233	16.704 #
19)	L4 AR-1242-4	5.860	5.021	412147	399464	9.598	8.553
20)	L4 AR-1242-5	6.604	5.547	807914	695060	18.116	13.430 #
21)	L5 AR-1248-1	5.673	4.740	645934	753994	14.564	18.200
22)	L5 AR-1248-2	5.948	4.979	535071	282892	7.448	4.276 #
23)	L5 AR-1248-3	6.156	5.021	716800	399464	9.224	5.702 #
24)	L5 AR-1248-4	6.564	5.195	838080	884428	11.246	11.068
25)	L5 AR-1248-5	6.604	5.587	807914	811232	10.385	11.824
26)	L6 AR-1254-1	6.539	5.547	553661	695060	6.192	5.732
27)	L6 AR-1254-2	6.758	5.697	742357	299865	5.656	2.764 #
28)	L6 AR-1254-3	7.127	6.124f	861213	1624555	6.441	9.476 #
29)	L6 AR-1254-4	7.421	0.000	2406079	0	30.459	N.D. #
30)	L6 AR-1254-5	7.838	6.753	1136502	1658013	11.471	11.670
31)	L7 AR-1260-1	0.000	6.234	0	210000	N.D.	1.584 #
32)	L7 AR-1260-2	7.559	6.422	1878793	573004	14.773	3.879 #
33)	L7 AR-1260-3	7.912	6.571	412707	1062064	3.992	7.326 #
34)	L7 AR-1260-4	8.136	7.052	1066848	422243	9.086	3.464 #
35)	L7 AR-1260-5	8.476	7.295	2679731	2180674	13.655	8.777 #
36)	L8 AR-1262-1	7.995f	6.876f	510232	-459456	8.061	N.D. #
37)	L8 AR-1262-2	8.476	7.052	2679731	422243	11.628	2.577 #
38)	L8 AR-1262-3	8.810	7.576	1239876	515288	7.504	4.261 #
39)	L8 AR-1262-4	0.000	7.644	0	2056502	N.D.	9.759 #
40)	L8 AR-1262-5	9.571	8.143	583853	599720	8.011	7.346
41)	L9 AR-1268-1	8.810f	7.576	1239876	515288	4.257	1.602 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020124\
Data File : PP063247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Feb 2024 11:11
Operator : YP\AJ
Sample : P1187-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 78 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 01:43:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 02 09:02:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.644	0	2056502	N.D.	6.882 #
44) L9	AR-1268-4	9.571	8.143	583853	599720	7.550	6.832
45) L9	AR-1268-5	10.002	8.437	1483759	1805043	2.033	2.143


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020124\
Data File : PP063247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Feb 2024 11:11
Operator : YP\AJ
Sample : P1187-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 78 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 01:43:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 02 09:02:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

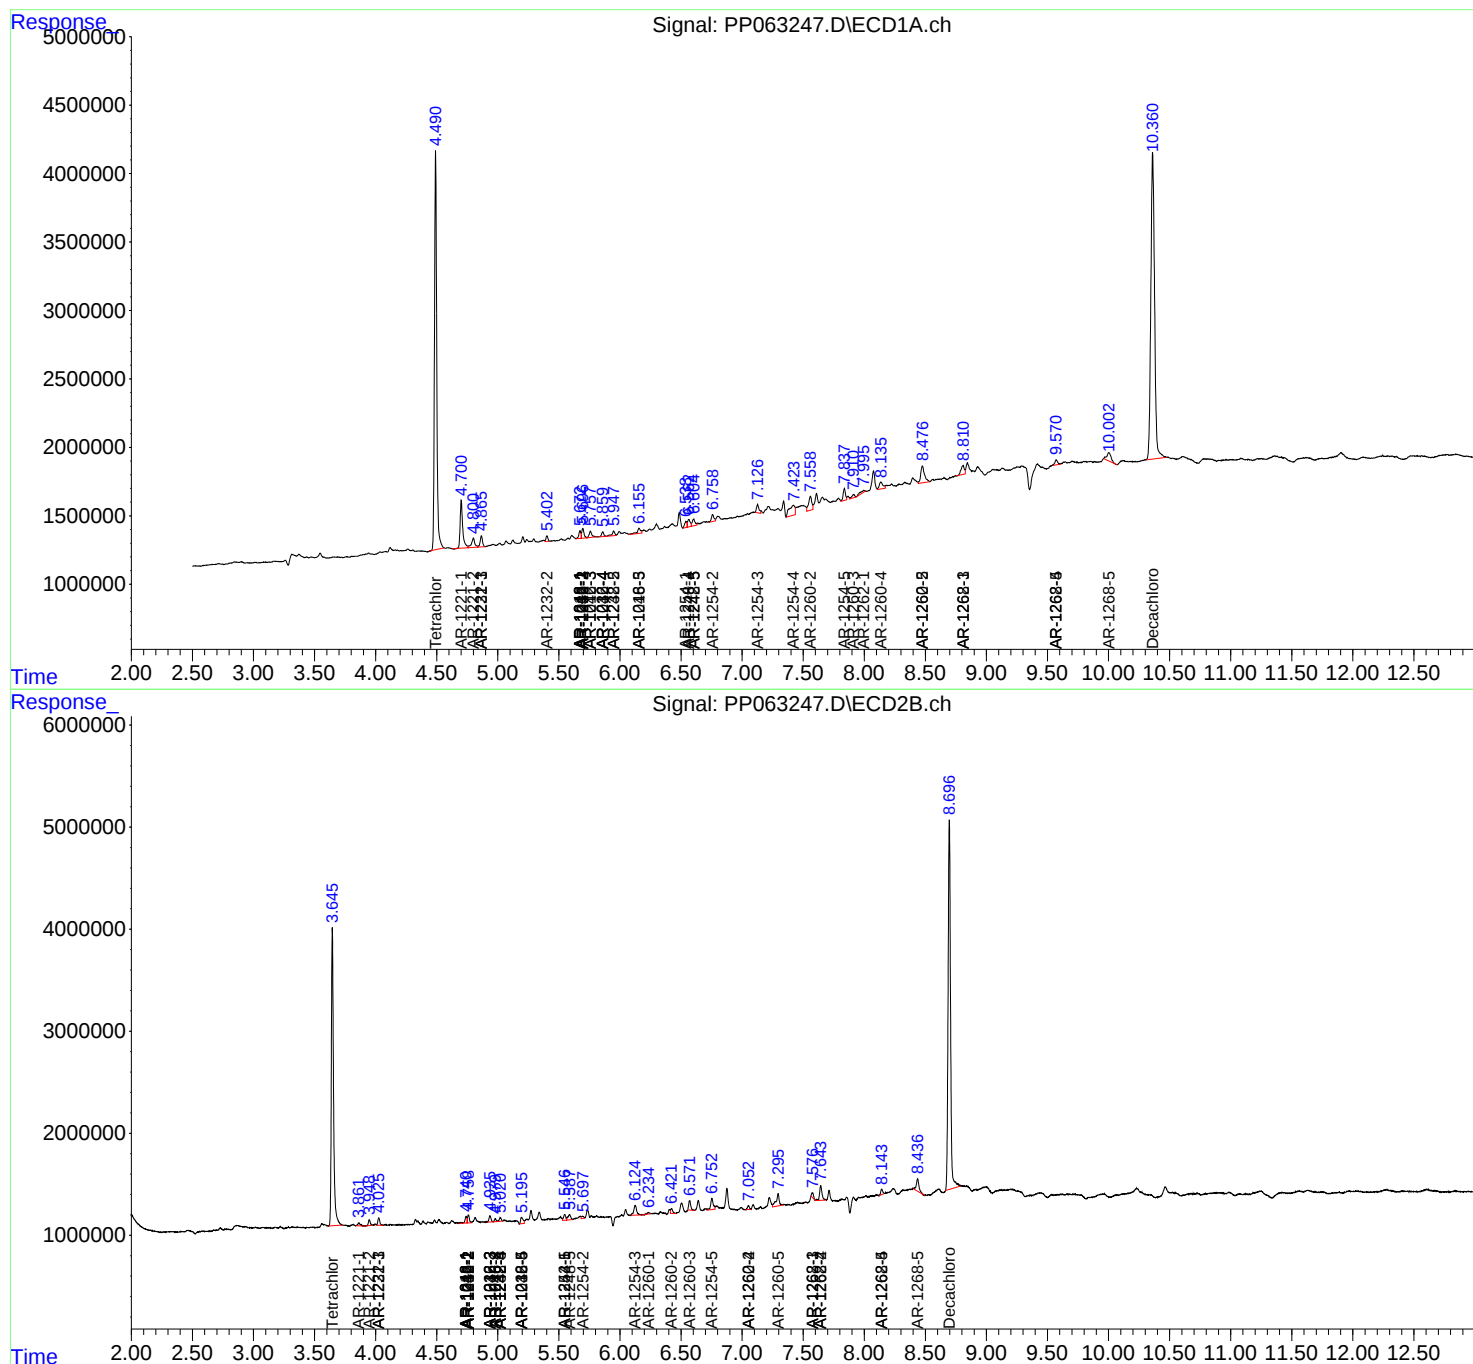


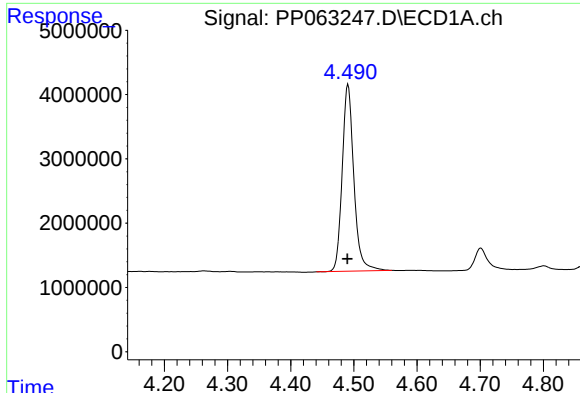

#1 Tetrachloro-m-xylene


R.T.: 4.491 min
Delta R.T.: 0.000 min
Response: 37294139
Conc: 15.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

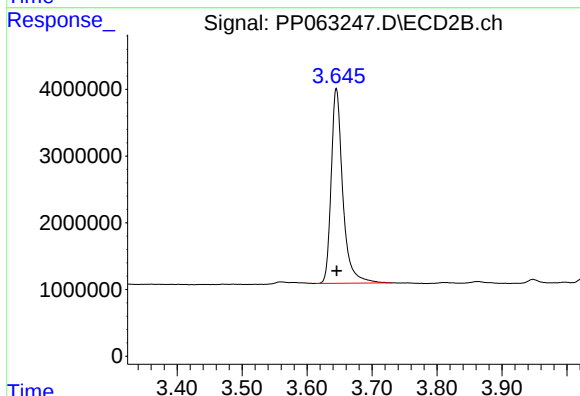


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: 0.000 min
Response: 36153568
Conc: 15.21 ng/ml

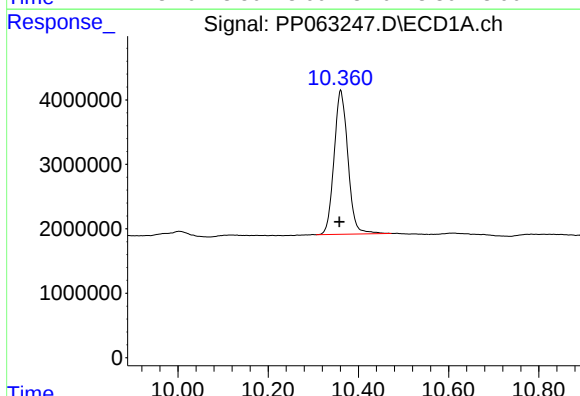


#2 Decachlorobiphenyl

R.T.: 10.361 min
Delta R.T.: 0.003 min
Response: 47569370
Conc: 21.15 ng/ml

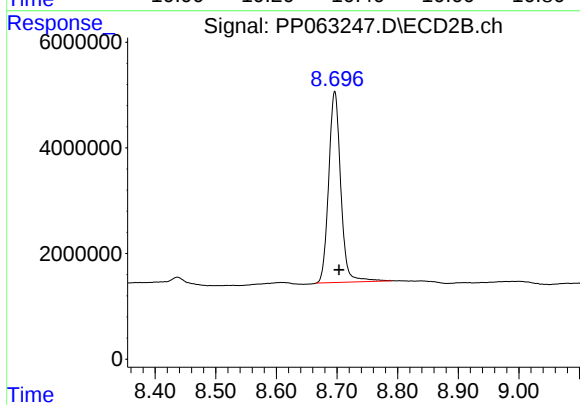

#2 Decachlorobiphenyl


R.T.: 8.696 min
Delta R.T.: -0.007 min
Response: 50138646
Conc: 20.24 ng/ml

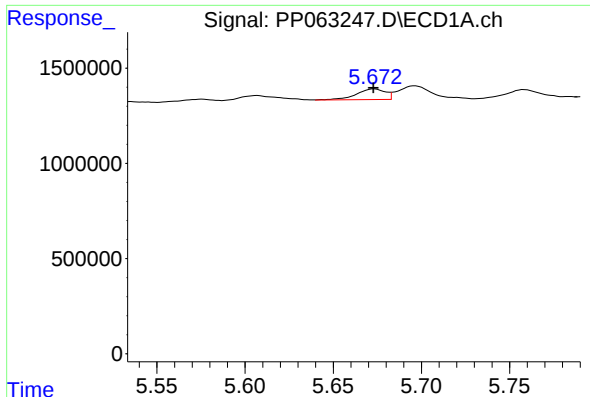

#3 AR-1016-1


R.T.: 5.673 min
Delta R.T.: 0.000 min
Response: 645934
Conc: 8.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

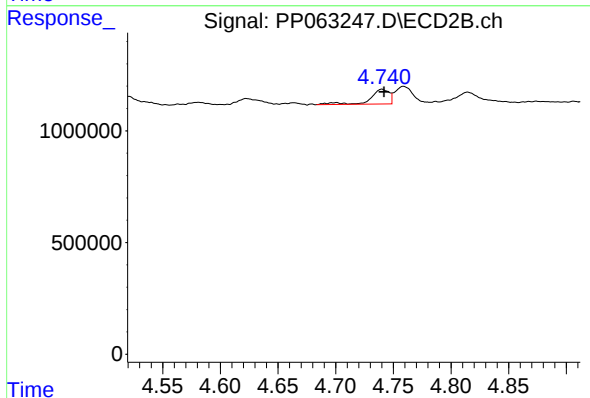


#3 AR-1016-1

R.T.: 4.740 min
Delta R.T.: -0.002 min
Response: 753994
Conc: 10.54 ng/ml

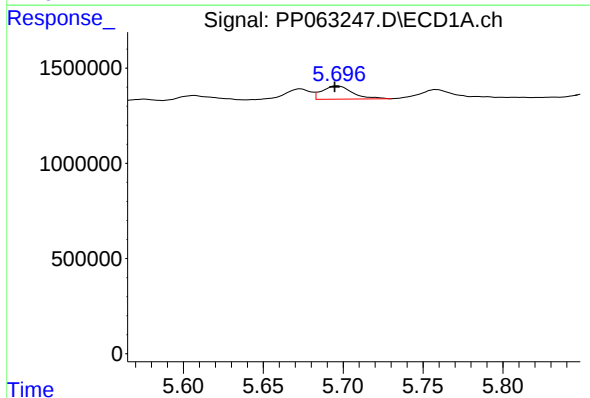


#4 AR-1016-2

R.T.: 5.696 min
Delta R.T.: 0.002 min
Response: 921551
Conc: 8.48 ng/ml

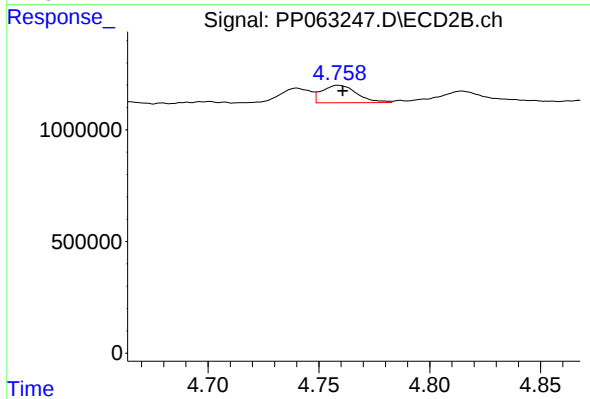

#4 AR-1016-2


R.T.: 4.759 min
Delta R.T.: -0.002 min
Response: 858327
Conc: 8.36 ng/ml

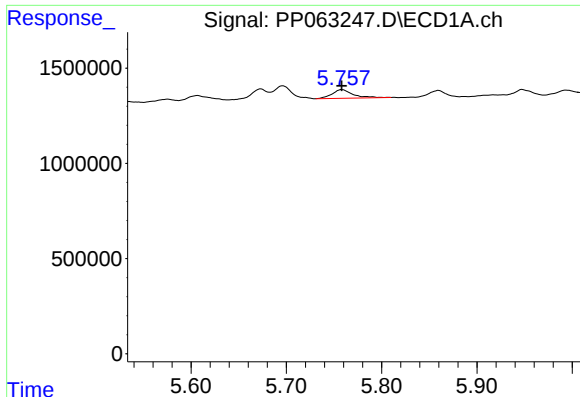

#5 AR-1016-3


R.T.: 5.758 min
Delta R.T.: 0.000 min
Response: 694468
Conc: 10.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

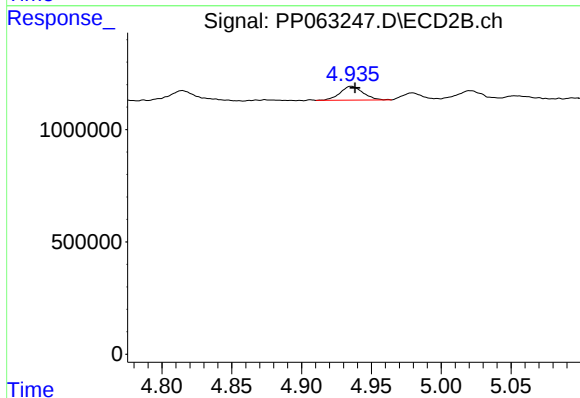


#5 AR-1016-3

R.T.: 4.936 min
Delta R.T.: -0.003 min
Response: 707840
Conc: 12.80 ng/ml

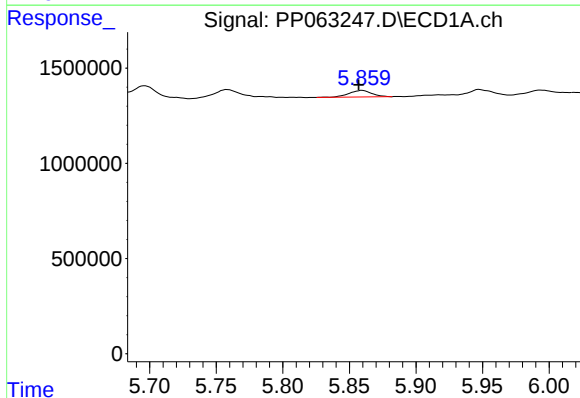


#6 AR-1016-4

R.T.: 5.860 min
Delta R.T.: 0.003 min
Response: 412147
Conc: 7.36 ng/ml

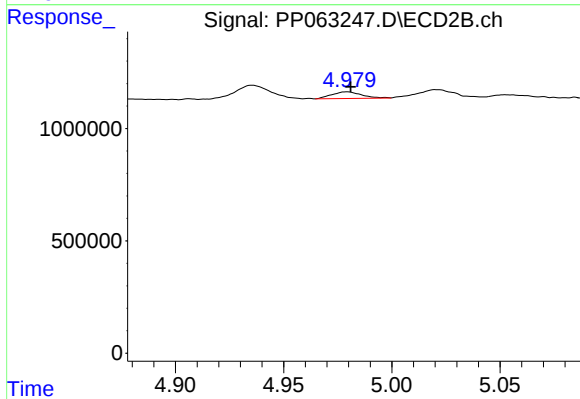

#6 AR-1016-4


R.T.: 4.979 min
Delta R.T.: -0.002 min
Response: 282892
Conc: 5.72 ng/ml

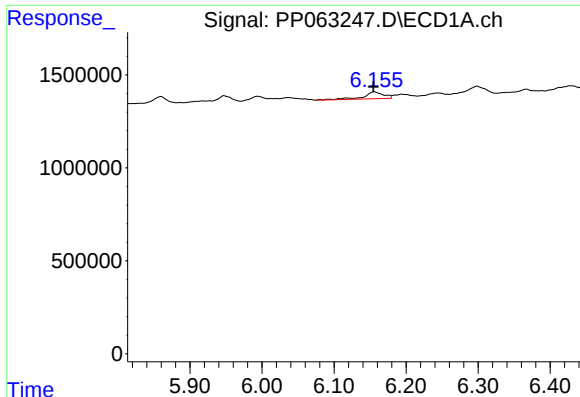

#7 AR-1016-5


R.T.: 6.156 min
Delta R.T.: 0.000 min
Response: 716800
Conc: 11.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

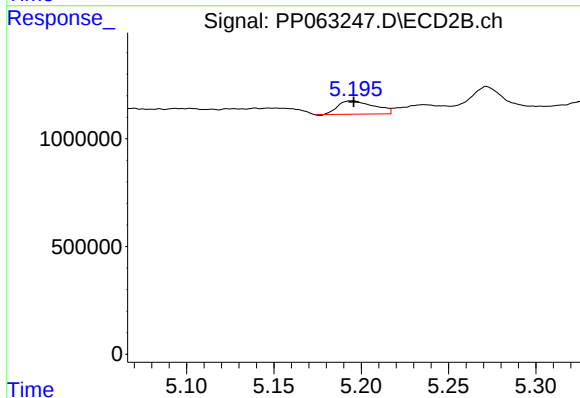


#7 AR-1016-5

R.T.: 5.195 min
Delta R.T.: -0.001 min
Response: 884428
Conc: 14.06 ng/ml

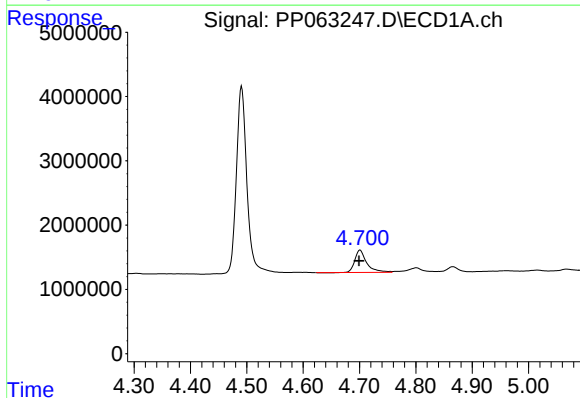


#8 AR-1221-1

R.T.: 4.701 min
Delta R.T.: 0.002 min
Response: 5082989
Conc: 182.67 ng/ml

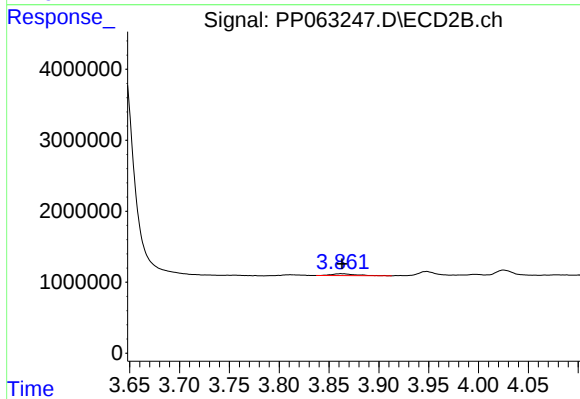

#8 AR-1221-1


R.T.: 3.862 min
Delta R.T.: -0.001 min
Response: 453968
Conc: 17.17 ng/ml

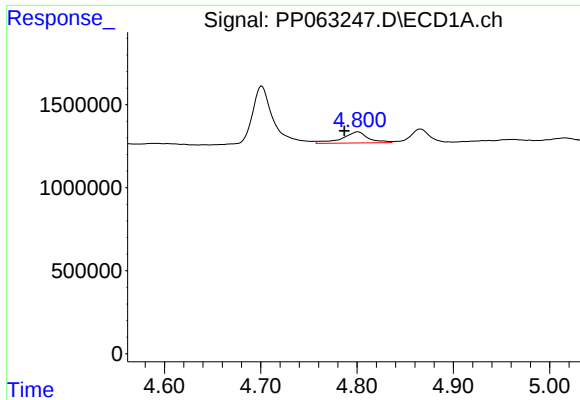

#9 AR-1221-2


R.T.: 4.801 min
Delta R.T.: 0.014 min
Response: 1271108
Conc: 59.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

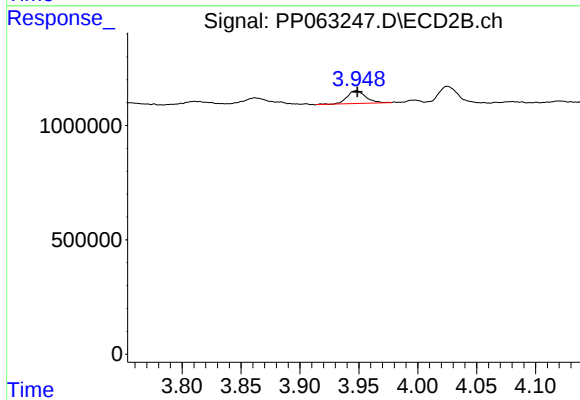


#9 AR-1221-2

R.T.: 3.948 min
Delta R.T.: 0.000 min
Response: 600362
Conc: 30.39 ng/ml

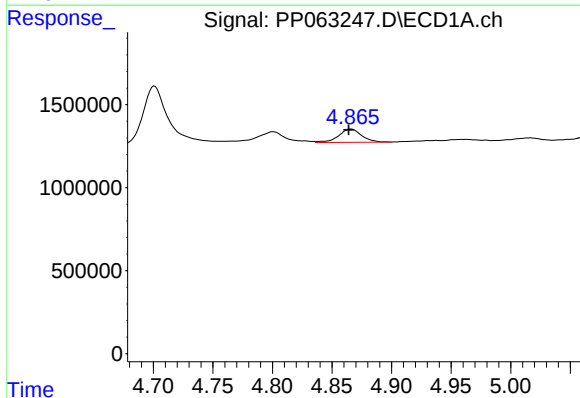


#10 AR-1221-3

R.T.: 4.866 min
Delta R.T.: 0.002 min
Response: 1086460
Conc: 17.64 ng/ml

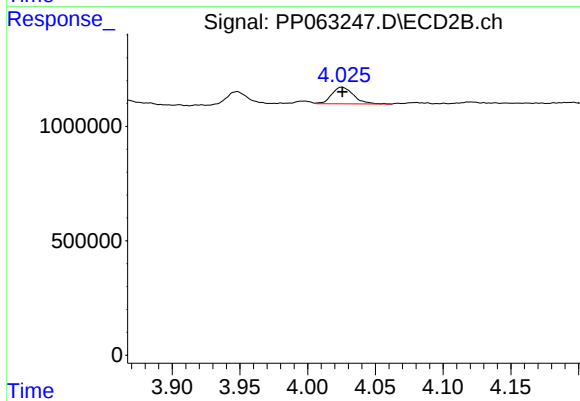

#10 AR-1221-3


R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 815108
Conc: 13.39 ng/ml

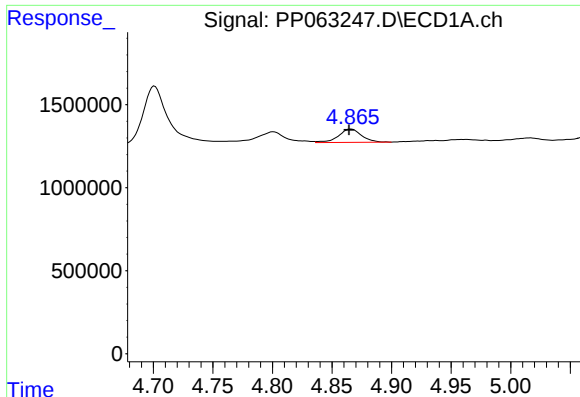

#11 AR-1232-1


R.T.: 4.866 min
Delta R.T.: 0.002 min
Response: 1086460
Conc: 20.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

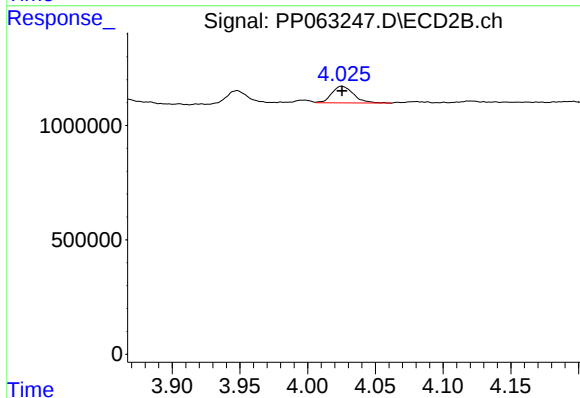


#11 AR-1232-1

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 815108
Conc: 15.17 ng/ml

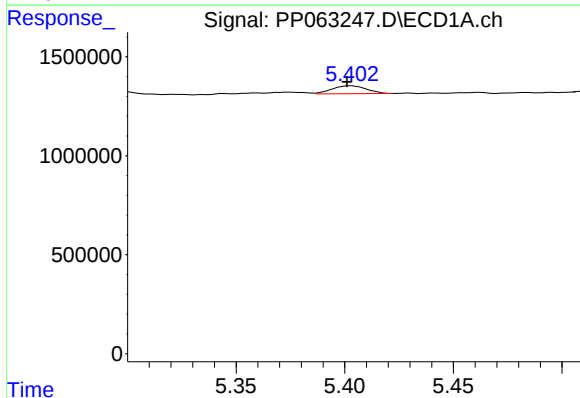


#12 AR-1232-2

R.T.: 5.403 min
Delta R.T.: 0.002 min
Response: 446044
Conc: 14.74 ng/ml

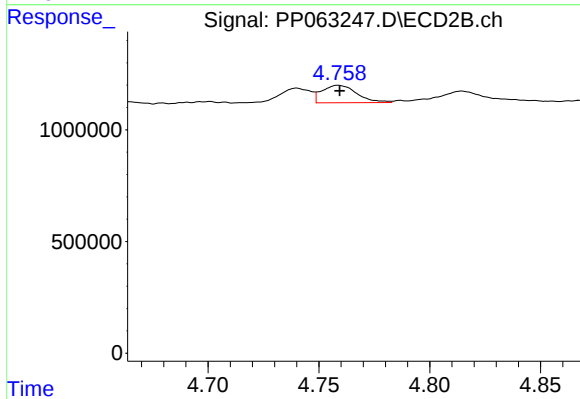

#12 AR-1232-2


R.T.: 4.759 min
Delta R.T.: 0.000 min
Response: 858327
Conc: 17.91 ng/ml

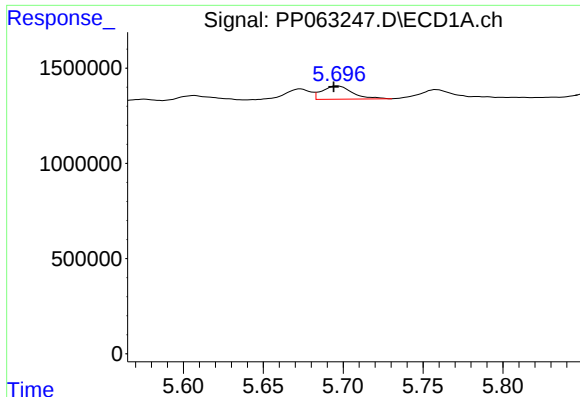

#13 AR-1232-3


R.T.: 5.696 min
Delta R.T.: 0.002 min
Response: 921551
Conc: 18.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

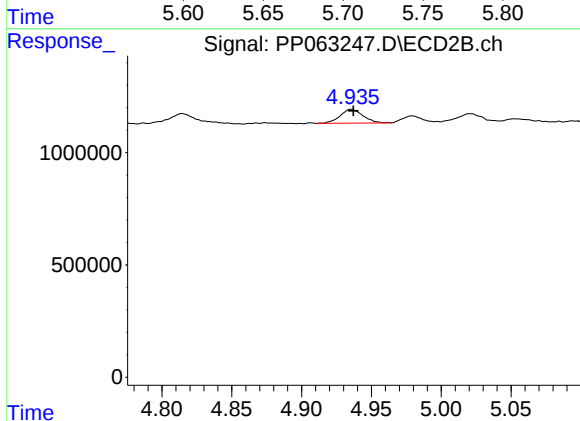


#13 AR-1232-3

R.T.: 4.936 min
Delta R.T.: -0.001 min
Response: 707840
Conc: 27.25 ng/ml

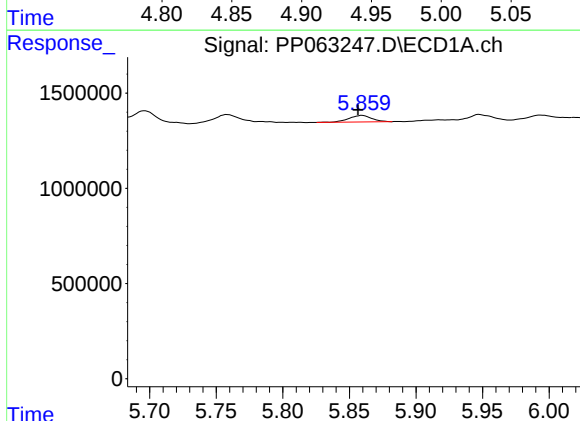


#14 AR-1232-4

R.T.: 5.860 min
Delta R.T.: 0.003 min
Response: 412147
Conc: 15.69 ng/ml

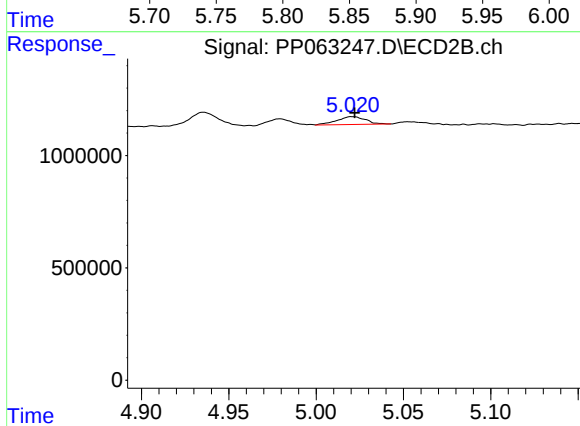

#14 AR-1232-4


R.T.: 5.021 min
Delta R.T.: -0.001 min
Response: 399464
Conc: 15.32 ng/ml

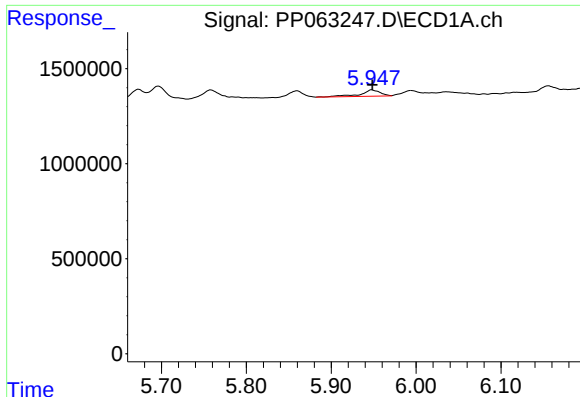

#15 AR-1232-5


R.T.: 5.948 min
Delta R.T.: 0.000 min
Response: 535071
Conc: 23.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

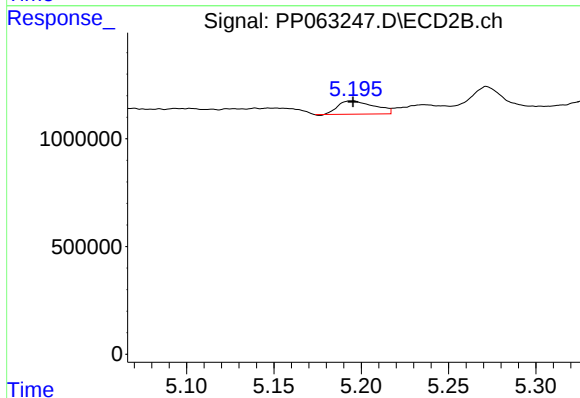


#15 AR-1232-5

R.T.: 5.195 min
Delta R.T.: 0.000 min
Response: 884428
Conc: 32.44 ng/ml

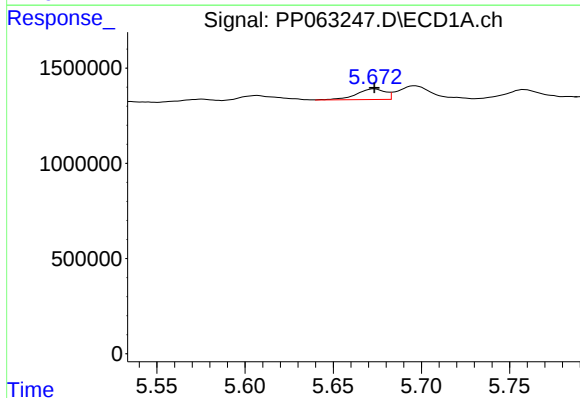


#16 AR-1242-1

R.T.: 5.673 min
Delta R.T.: 0.000 min
Response: 645934
Conc: 11.34 ng/ml

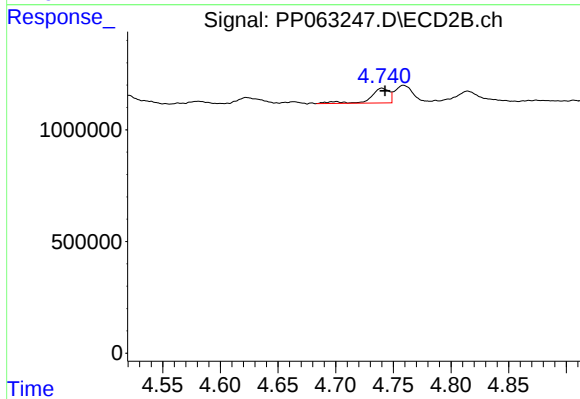

#16 AR-1242-1


R.T.: 4.740 min
Delta R.T.: -0.003 min
Response: 753994
Conc: 13.87 ng/ml

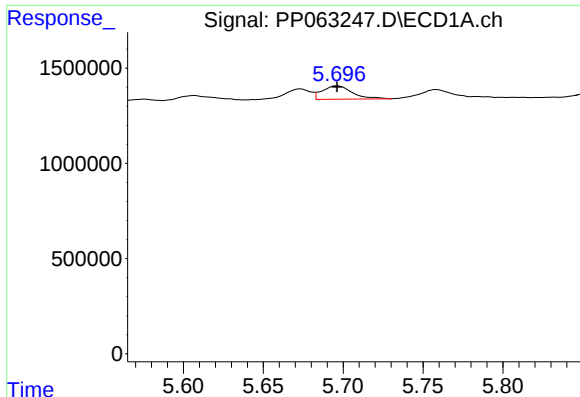

#17 AR-1242-2


R.T.: 5.696 min
Delta R.T.: 0.000 min
Response: 921551
Conc: 11.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

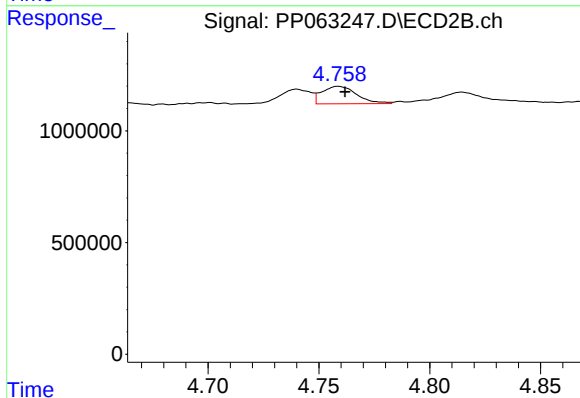


#17 AR-1242-2

R.T.: 4.759 min
Delta R.T.: -0.003 min
Response: 858327
Conc: 11.02 ng/ml

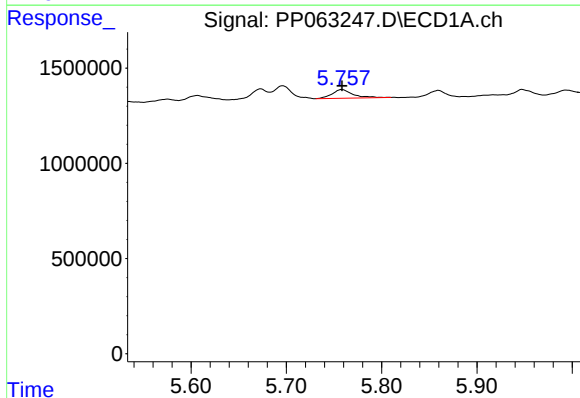


#18 AR-1242-3

R.T.: 5.758 min
Delta R.T.: 0.000 min
Response: 694468
Conc: 13.23 ng/ml

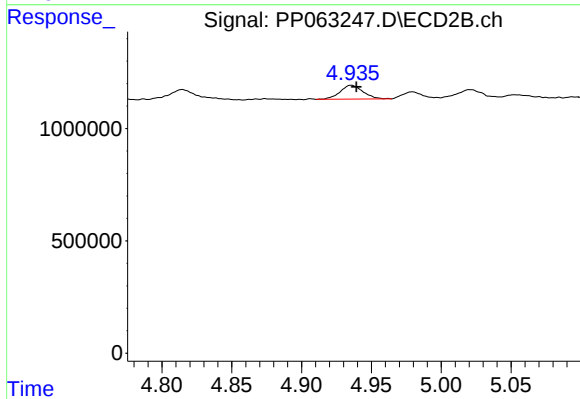

#18 AR-1242-3


R.T.: 4.936 min
Delta R.T.: -0.004 min
Response: 707840
Conc: 16.70 ng/ml

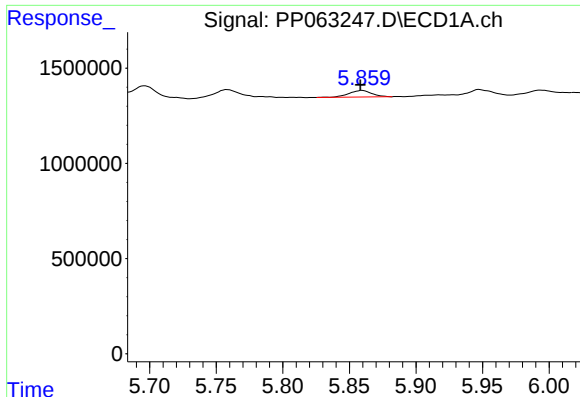

#19 AR-1242-4


R.T.: 5.860 min
Delta R.T.: 0.002 min
Response: 412147
Conc: 9.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

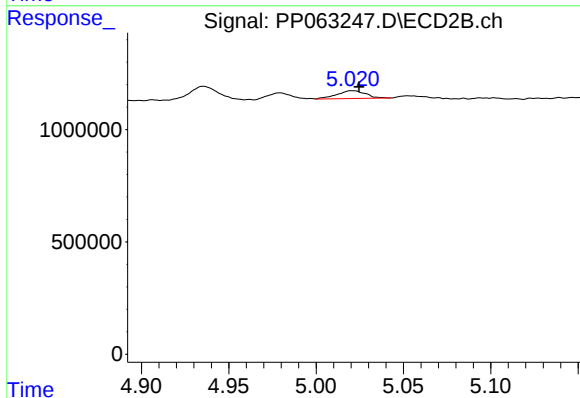


#19 AR-1242-4

R.T.: 5.021 min
Delta R.T.: -0.004 min
Response: 399464
Conc: 8.55 ng/ml

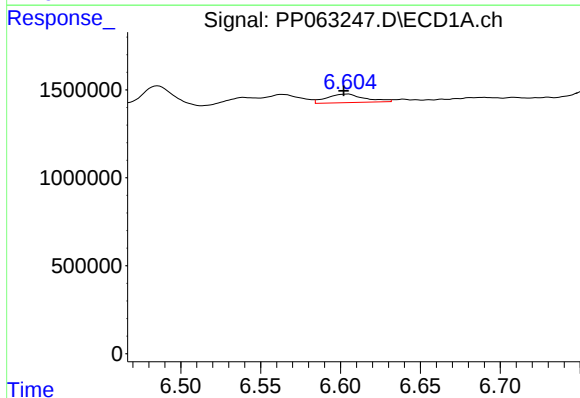


#20 AR-1242-5

R.T.: 6.604 min
Delta R.T.: 0.002 min
Response: 807914
Conc: 18.12 ng/ml

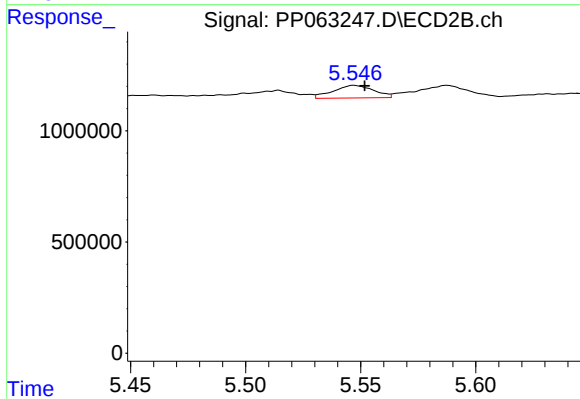

#20 AR-1242-5


R.T.: 5.547 min
Delta R.T.: -0.005 min
Response: 695060
Conc: 13.43 ng/ml

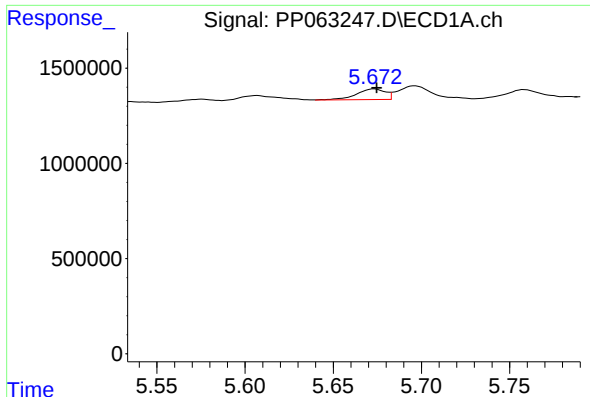

#21 AR-1248-1


R.T.: 5.673 min
Delta R.T.: -0.001 min
Response: 645934
Conc: 14.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

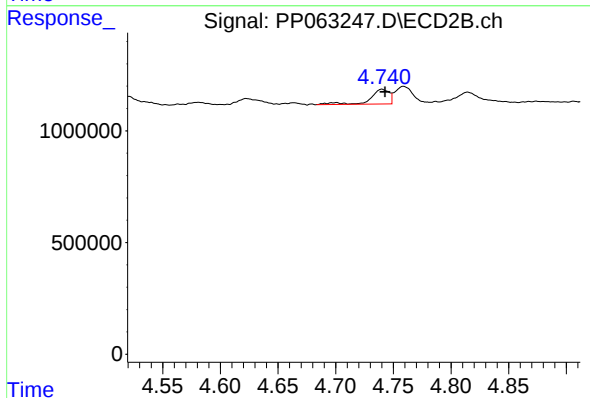


#21 AR-1248-1

R.T.: 4.740 min
Delta R.T.: -0.003 min
Response: 753994
Conc: 18.20 ng/ml

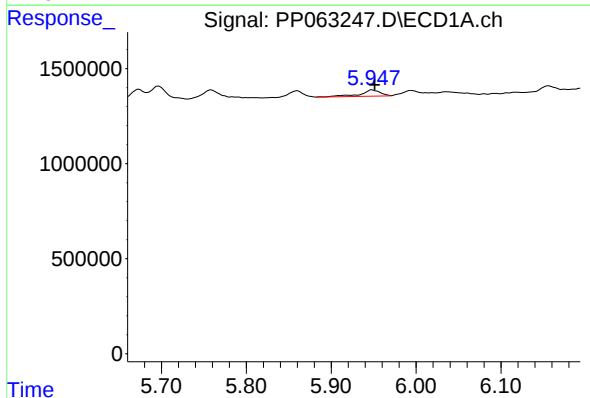


#22 AR-1248-2

R.T.: 5.948 min
Delta R.T.: -0.004 min
Response: 535071
Conc: 7.45 ng/ml

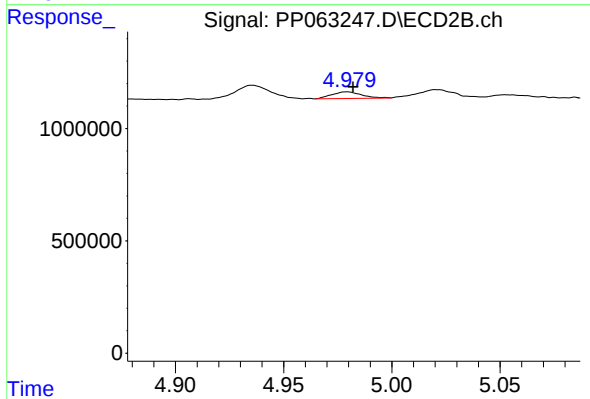

#22 AR-1248-2


R.T.: 4.979 min
Delta R.T.: -0.003 min
Response: 282892
Conc: 4.28 ng/ml

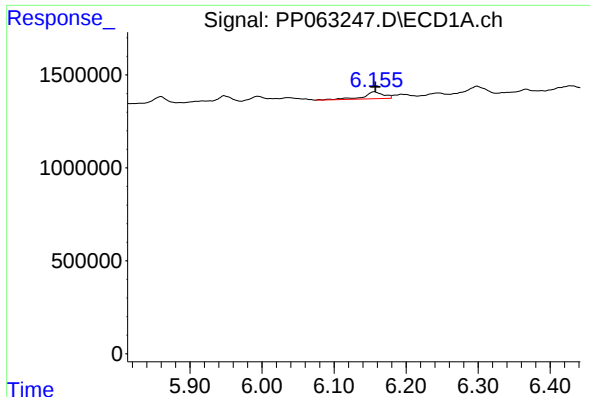

#23 AR-1248-3


R.T.: 6.156 min
Delta R.T.: -0.001 min
Response: 716800
Conc: 9.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

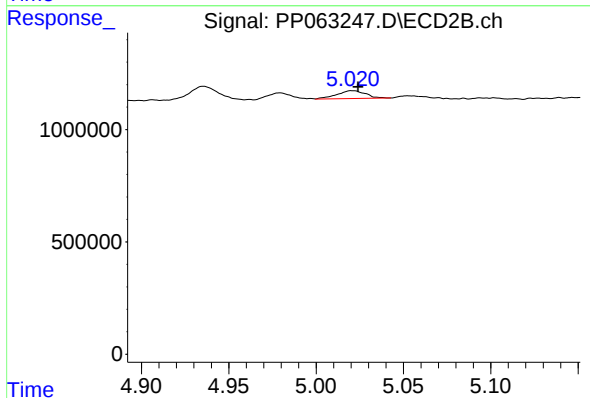


#23 AR-1248-3

R.T.: 5.021 min
Delta R.T.: -0.003 min
Response: 399464
Conc: 5.70 ng/ml

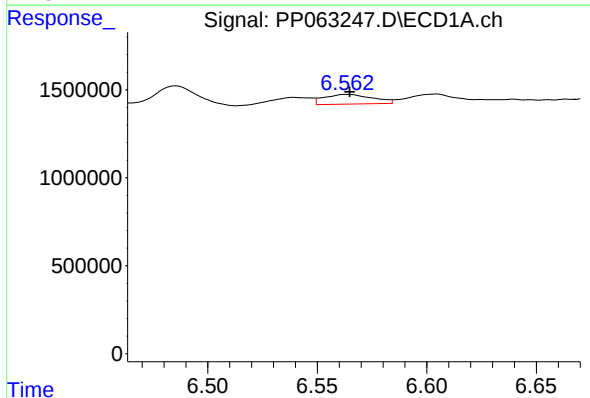


#24 AR-1248-4

R.T.: 6.564 min
Delta R.T.: -0.001 min
Response: 838080
Conc: 11.25 ng/ml

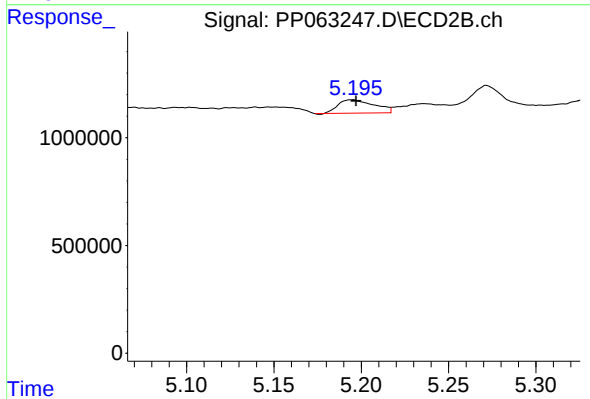

#24 AR-1248-4


R.T.: 5.195 min
Delta R.T.: -0.002 min
Response: 884428
Conc: 11.07 ng/ml

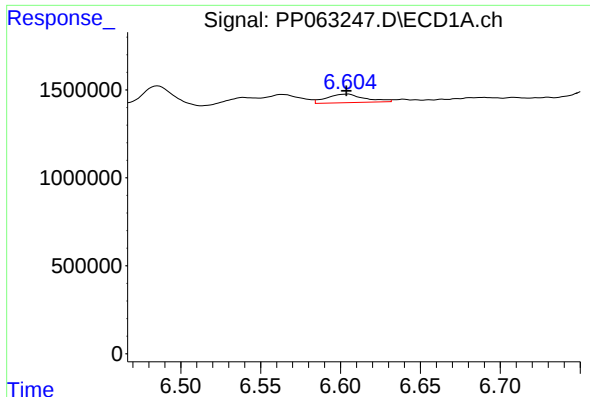

#25 AR-1248-5


R.T.: 6.604 min
Delta R.T.: 0.000 min
Response: 807914
Conc: 10.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

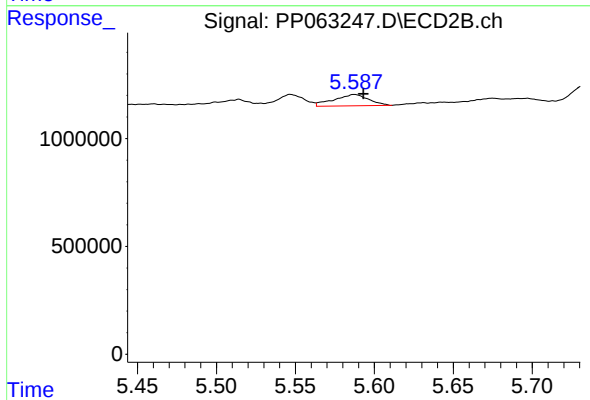


#25 AR-1248-5

R.T.: 5.587 min
Delta R.T.: -0.006 min
Response: 811232
Conc: 11.82 ng/ml

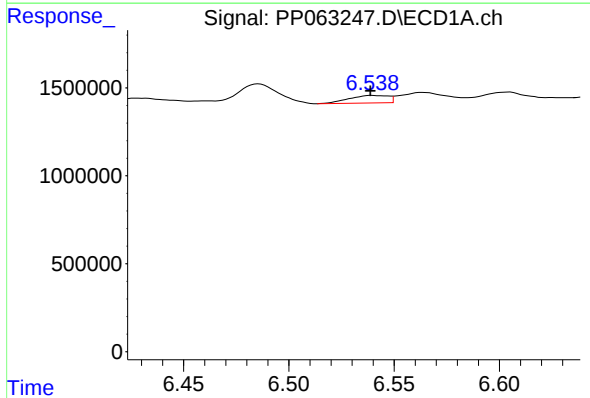


#26 AR-1254-1

R.T.: 6.539 min
Delta R.T.: 0.000 min
Response: 553661
Conc: 6.19 ng/ml

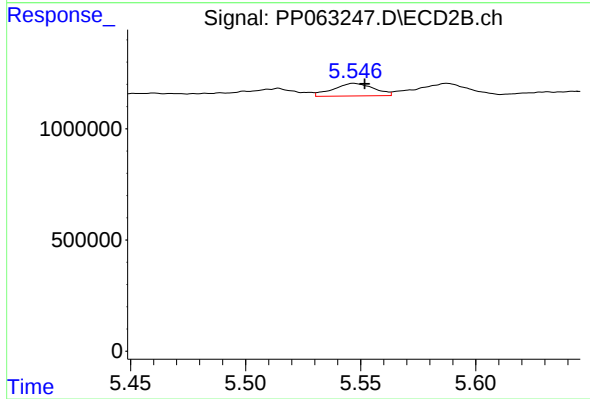

#26 AR-1254-1


R.T.: 5.547 min
Delta R.T.: -0.005 min
Response: 695060
Conc: 5.73 ng/ml

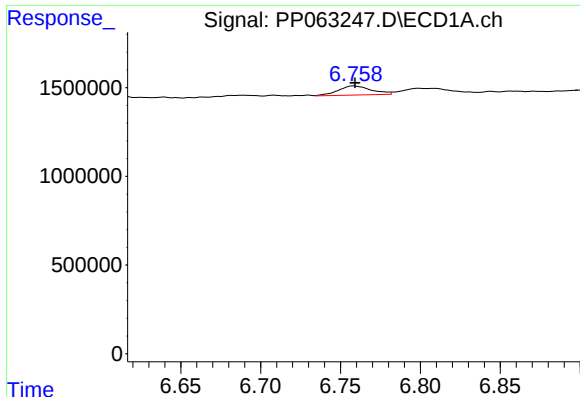

#27 AR-1254-2


R.T.: 6.758 min
Delta R.T.: 0.000 min
Response: 742357
Conc: 5.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

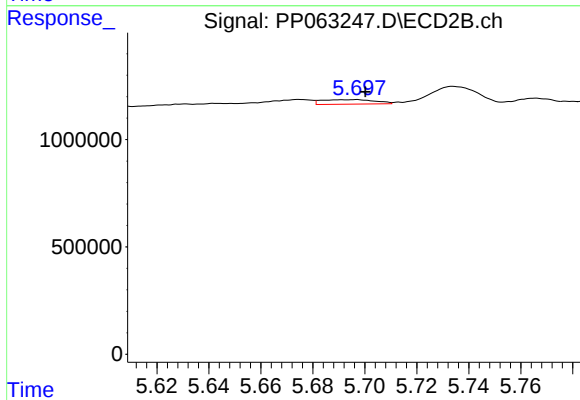


#27 AR-1254-2

R.T.: 5.697 min
Delta R.T.: -0.004 min
Response: 299865
Conc: 2.76 ng/ml

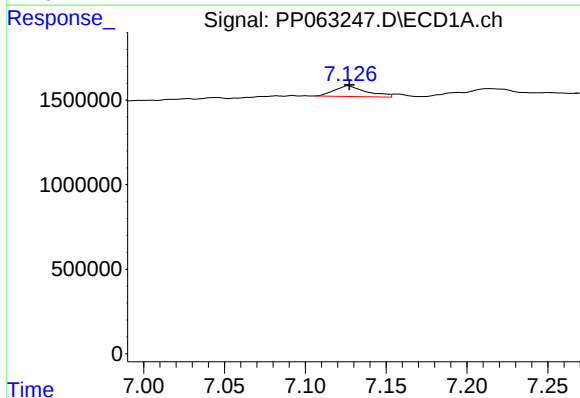


#28 AR-1254-3

R.T.: 7.127 min
Delta R.T.: 0.000 min
Response: 861213
Conc: 6.44 ng/ml

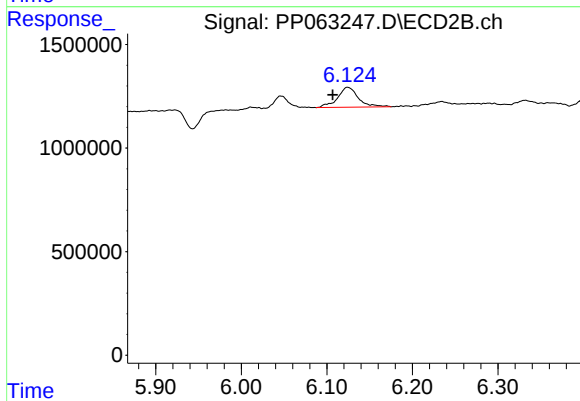

#28 AR-1254-3


R.T.: 6.124 min
Delta R.T.: 0.018 min
Response: 1624555
Conc: 9.48 ng/ml

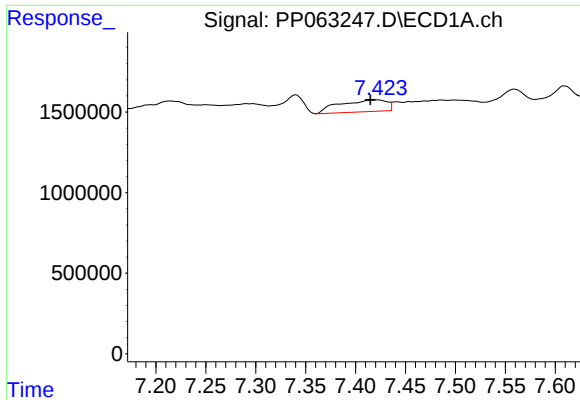

#29 AR-1254-4


R.T.: 7.421 min
Delta R.T.: 0.006 min
Response: 2406079
Conc: 30.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

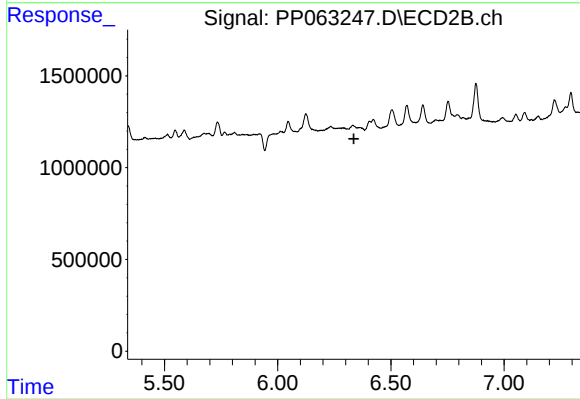


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.337 min
Response: 0
Conc: N.D.

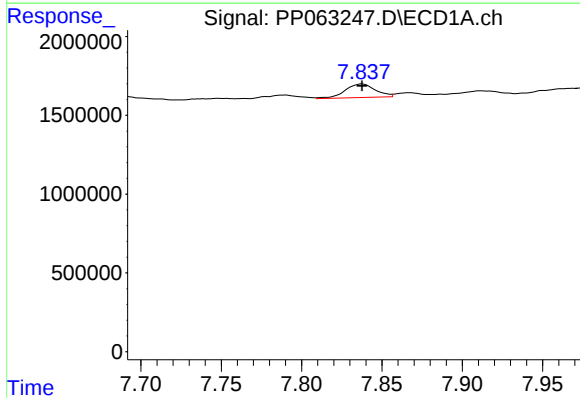


#30 AR-1254-5

R.T.: 7.838 min
Delta R.T.: 0.000 min
Response: 1136502
Conc: 11.47 ng/ml

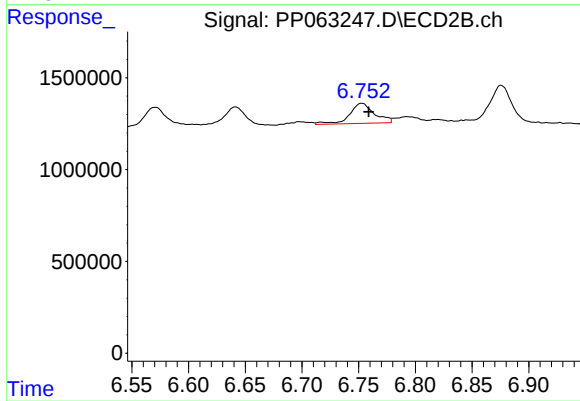

#30 AR-1254-5


R.T.: 6.753 min
Delta R.T.: -0.006 min
Response: 1658013
Conc: 11.67 ng/ml

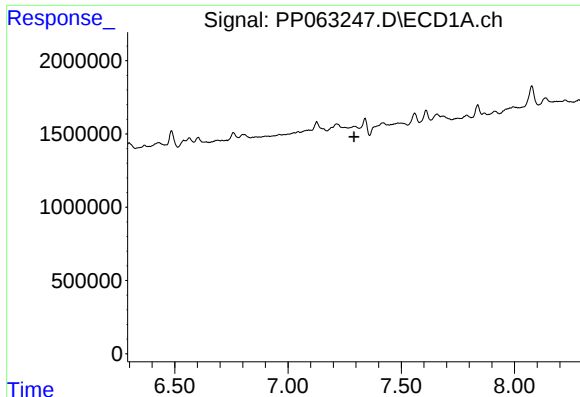

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

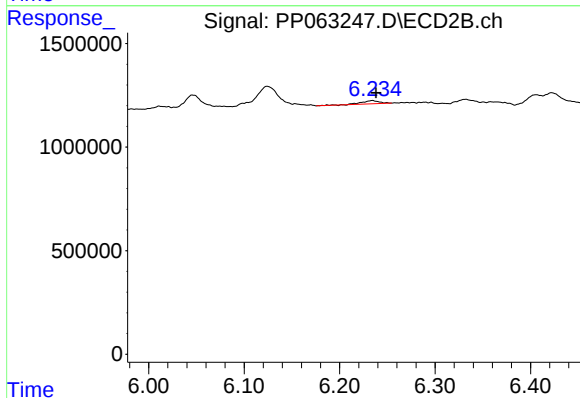


#31 AR-1260-1

R.T.: 6.234 min
Delta R.T.: -0.004 min
Response: 210000
Conc: 1.58 ng/ml

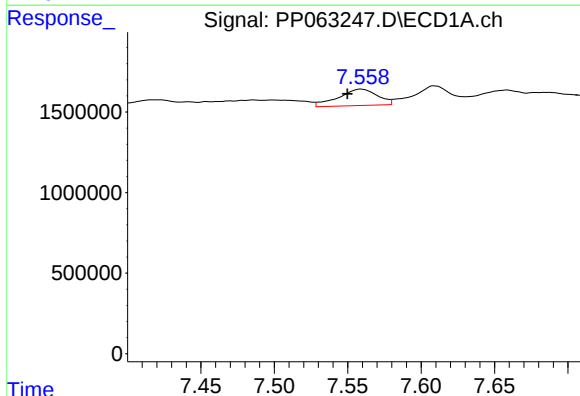


#32 AR-1260-2

R.T.: 7.559 min
Delta R.T.: 0.010 min
Response: 1878793
Conc: 14.77 ng/ml

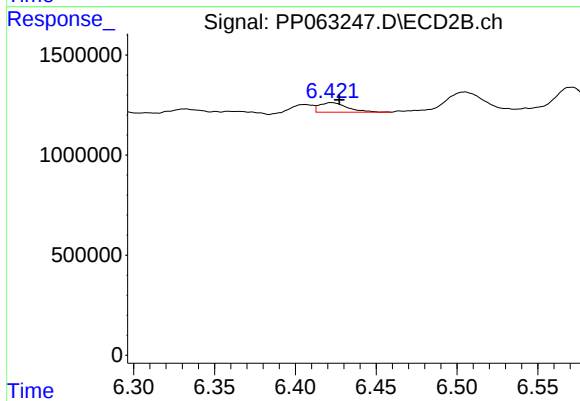

#32 AR-1260-2


R.T.: 6.422 min
Delta R.T.: -0.005 min
Response: 573004
Conc: 3.88 ng/ml

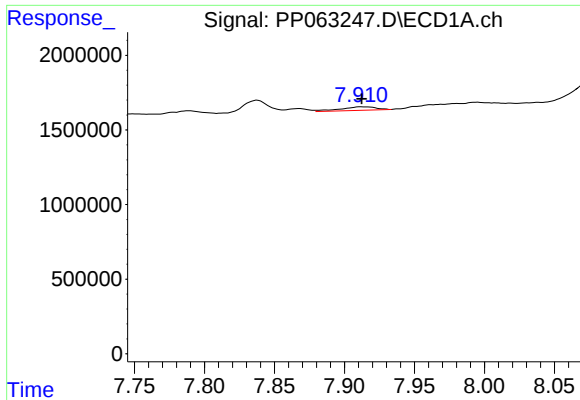

#33 AR-1260-3


R.T.: 7.912 min
Delta R.T.: 0.000 min
Response: 412707
Conc: 3.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

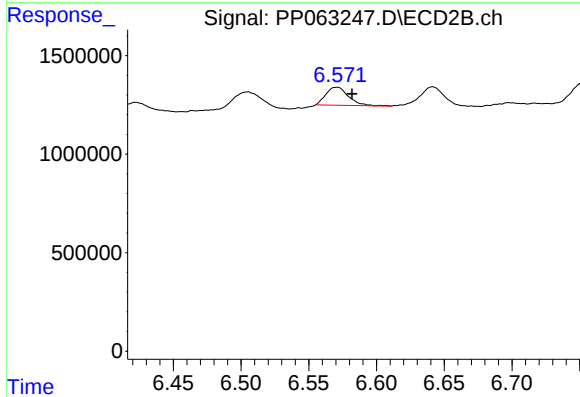


#33 AR-1260-3

R.T.: 6.571 min
Delta R.T.: -0.011 min
Response: 1062064
Conc: 7.33 ng/ml

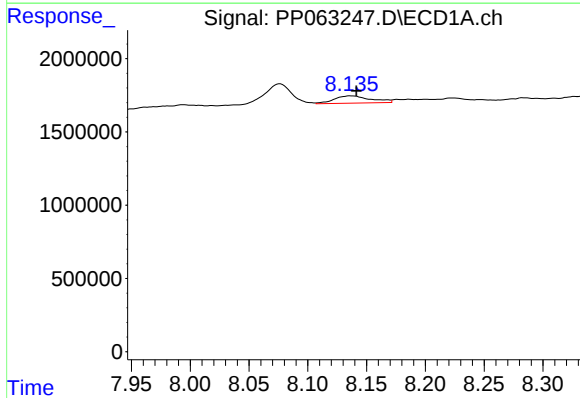


#34 AR-1260-4

R.T.: 8.136 min
Delta R.T.: -0.005 min
Response: 1066848
Conc: 9.09 ng/ml

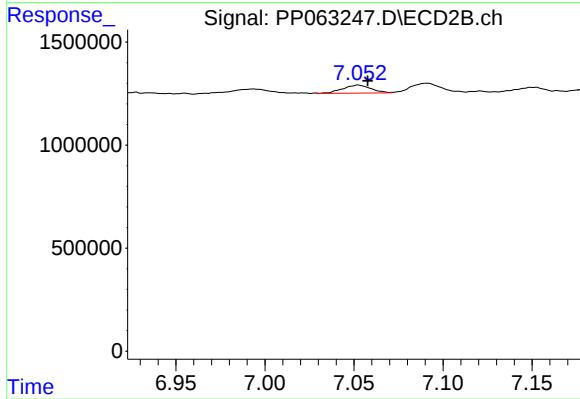

#34 AR-1260-4


R.T.: 7.052 min
Delta R.T.: -0.005 min
Response: 422243
Conc: 3.46 ng/ml

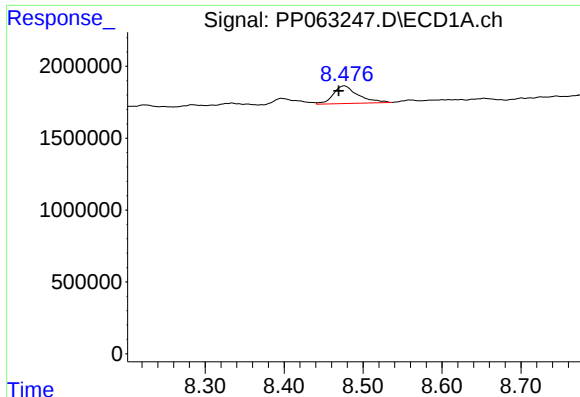

#35 AR-1260-5


R.T.: 8.476 min
Delta R.T.: 0.007 min
Response: 2679731
Conc: 13.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

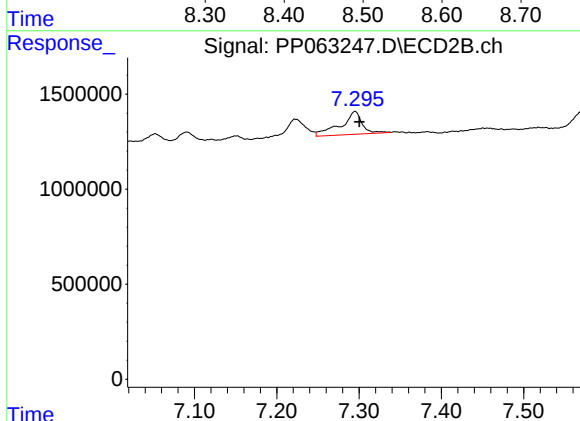


#35 AR-1260-5

R.T.: 7.295 min
Delta R.T.: -0.005 min
Response: 2180674
Conc: 8.78 ng/ml

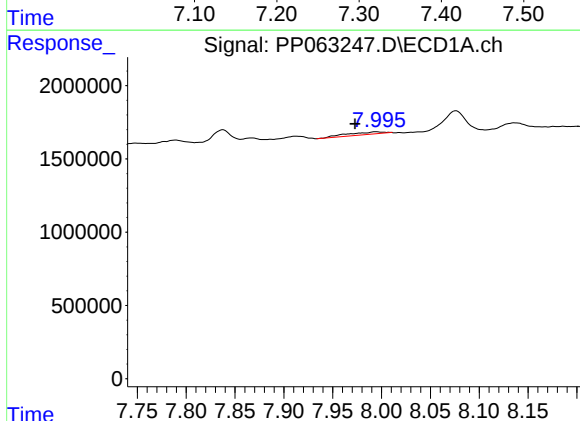


#36 AR-1262-1

R.T.: 7.995 min
Delta R.T.: 0.022 min
Response: 510232
Conc: 8.06 ng/ml

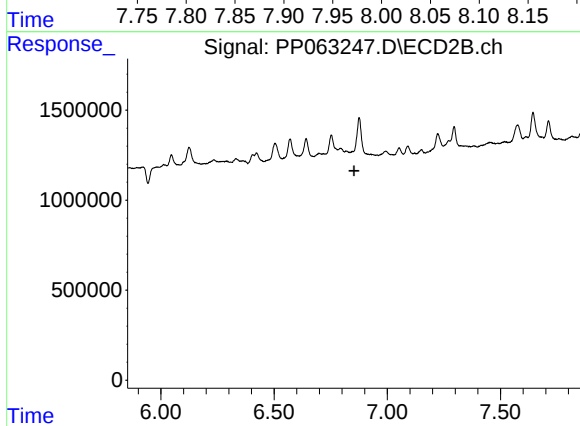

#36 AR-1262-1


R.T.: 6.876 min
Delta R.T.: 0.023 min
Response: -459456
Conc: N.D.

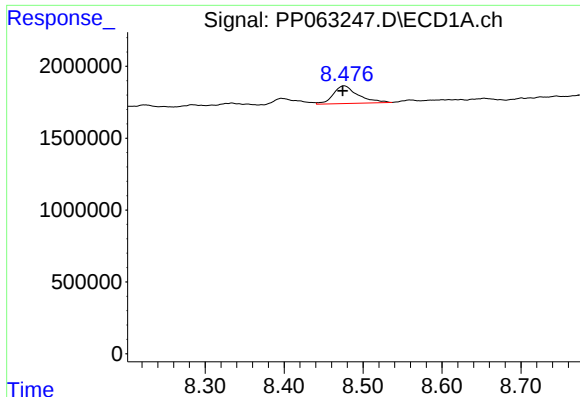

#37 AR-1262-2


R.T.: 8.476 min
Delta R.T.: 0.002 min
Response: 2679731
Conc: 11.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

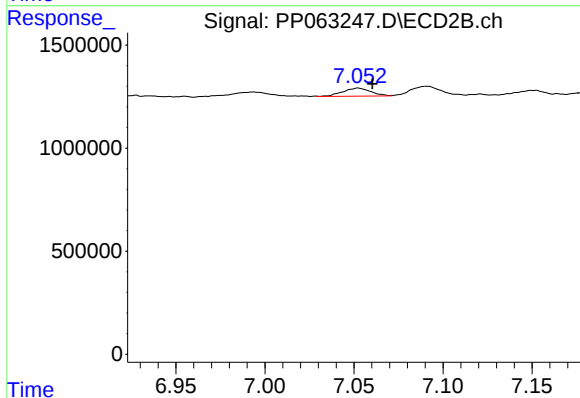


#37 AR-1262-2

R.T.: 7.052 min
Delta R.T.: -0.008 min
Response: 422243
Conc: 2.58 ng/ml

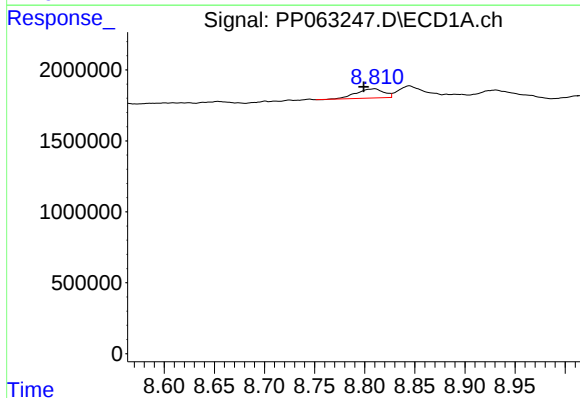


#38 AR-1262-3

R.T.: 8.810 min
Delta R.T.: 0.011 min
Response: 1239876
Conc: 7.50 ng/ml

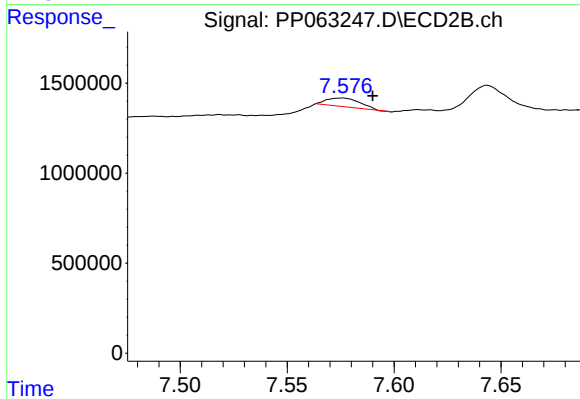

#38 AR-1262-3


R.T.: 7.576 min
Delta R.T.: -0.014 min
Response: 515288
Conc: 4.26 ng/ml

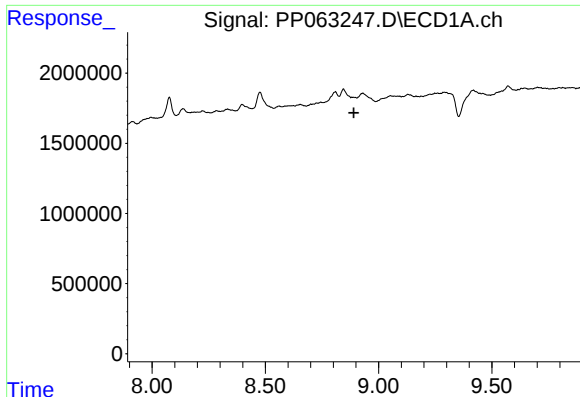

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.891 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

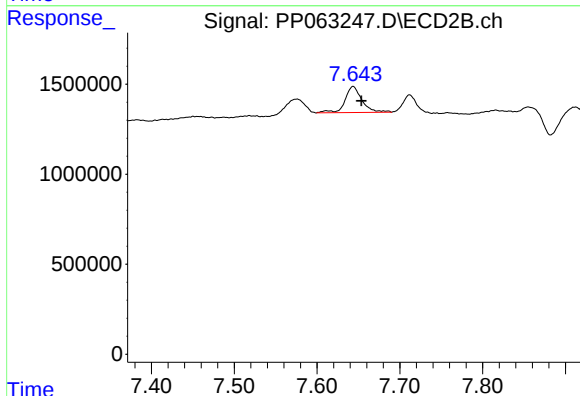


#39 AR-1262-4

R.T.: 7.644 min
Delta R.T.: -0.010 min
Response: 2056502
Conc: 9.76 ng/ml

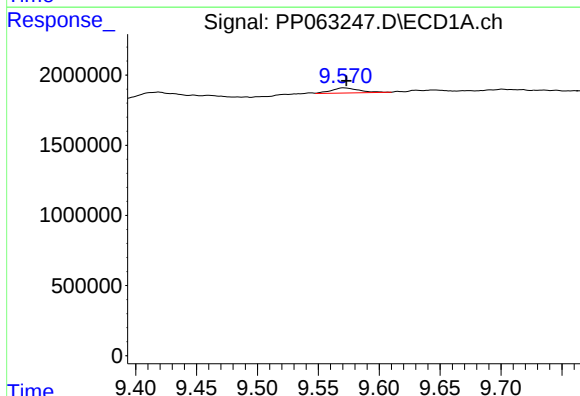


#40 AR-1262-5

R.T.: 9.571 min
Delta R.T.: -0.002 min
Response: 583853
Conc: 8.01 ng/ml

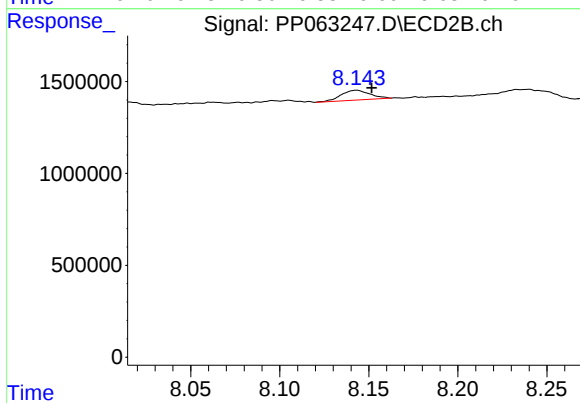

#40 AR-1262-5


R.T.: 8.143 min
Delta R.T.: -0.009 min
Response: 599720
Conc: 7.35 ng/ml

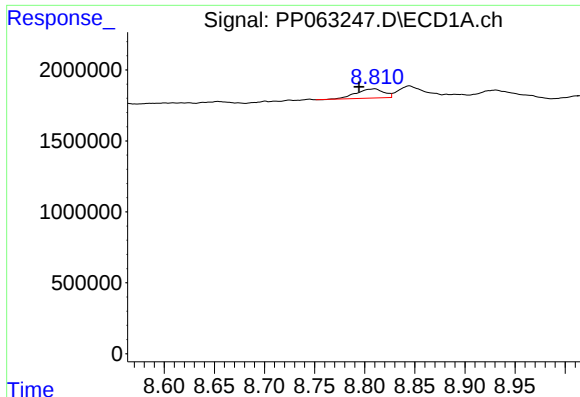

#41 AR-1268-1


R.T.: 8.810 min
Delta R.T.: 0.016 min
Response: 1239876
Conc: 4.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

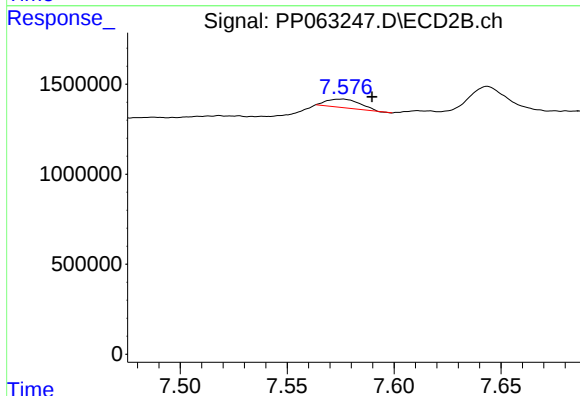


#41 AR-1268-1

R.T.: 7.576 min
Delta R.T.: -0.014 min
Response: 515288
Conc: 1.60 ng/ml

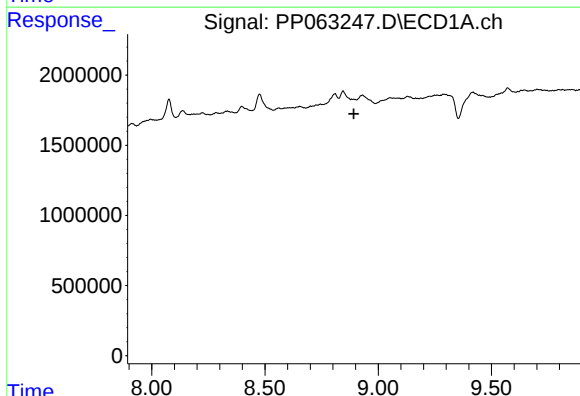


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.892 min
Response: 0
Conc: N.D.

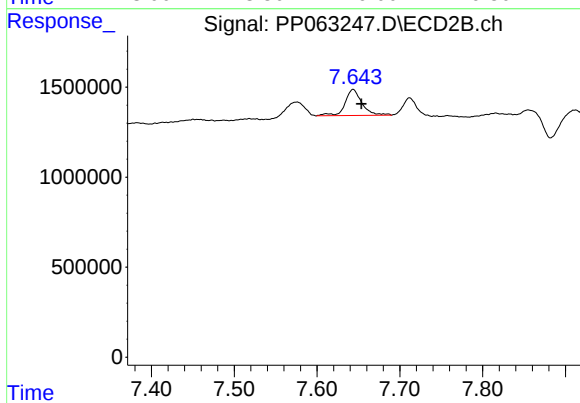

#42 AR-1268-2


R.T.: 7.644 min
Delta R.T.: -0.010 min
Response: 2056502
Conc: 6.88 ng/ml

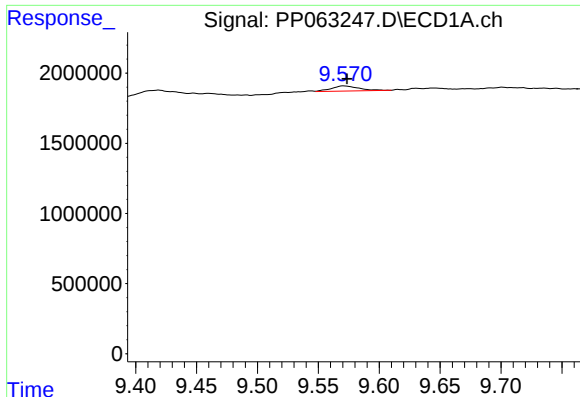

#44 AR-1268-4


R.T.: 9.571 min
Delta R.T.: -0.002 min
Response: 583853
Conc: 7.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

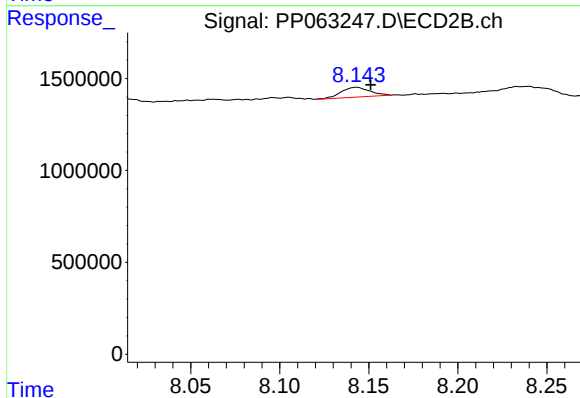


#44 AR-1268-4

R.T.: 8.143 min
Delta R.T.: -0.008 min
Response: 599720
Conc: 6.83 ng/ml

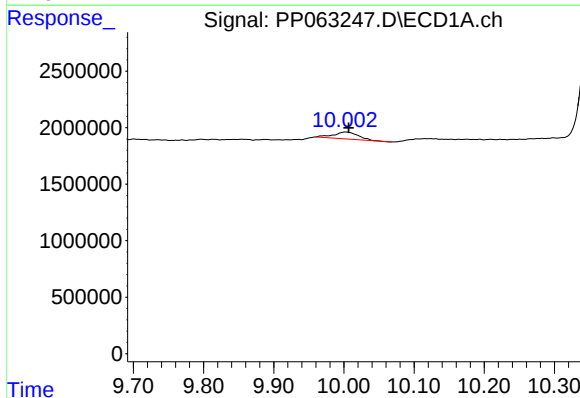

#45 AR-1268-5

R.T.: 10.002 min
Delta R.T.: -0.004 min
Response: 1483759
Conc: 2.03 ng/ml

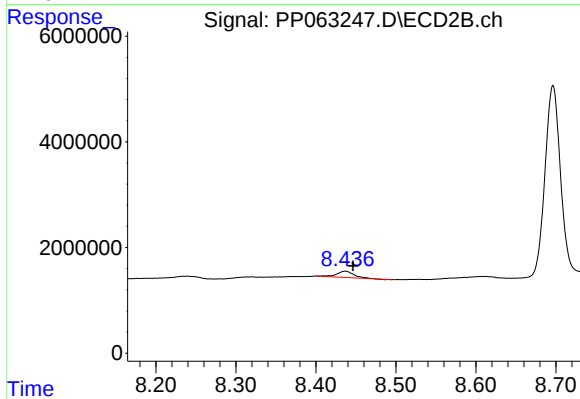

#45 AR-1268-5

R.T.: 8.437 min
Delta R.T.: -0.009 min
Response: 1805043
Conc: 2.14 ng/ml