

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020124\
 Data File : PP063250.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Feb 2024 11:59
 Operator : YP\AJ
 Sample : P1187-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 01:48:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 02 09:02:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.491	3.645	39804740	38919495	16.641	16.374
2) SA Decachlor...	10.362	8.696	42573463	45749342	18.931	18.469
Target Compounds						
26) L6 AR-1254-1	6.537	5.547	1952960	2673373	21.842	22.045
27) L6 AR-1254-2	6.757	5.696	3158035	2447588	24.059	22.557
28) L6 AR-1254-3	7.126	6.101	3734191	4012645	27.929	23.406
29) L6 AR-1254-4	7.414	6.331	1939783	1778865	24.556	21.861
30) L6 AR-1254-5	7.837	6.752	2291466	3151790	23.128	22.184



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020124\
Data File : PP063250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Feb 2024 11:59
Operator : YP\AJ
Sample : P1187-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 81 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 01:48:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 02 09:02:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

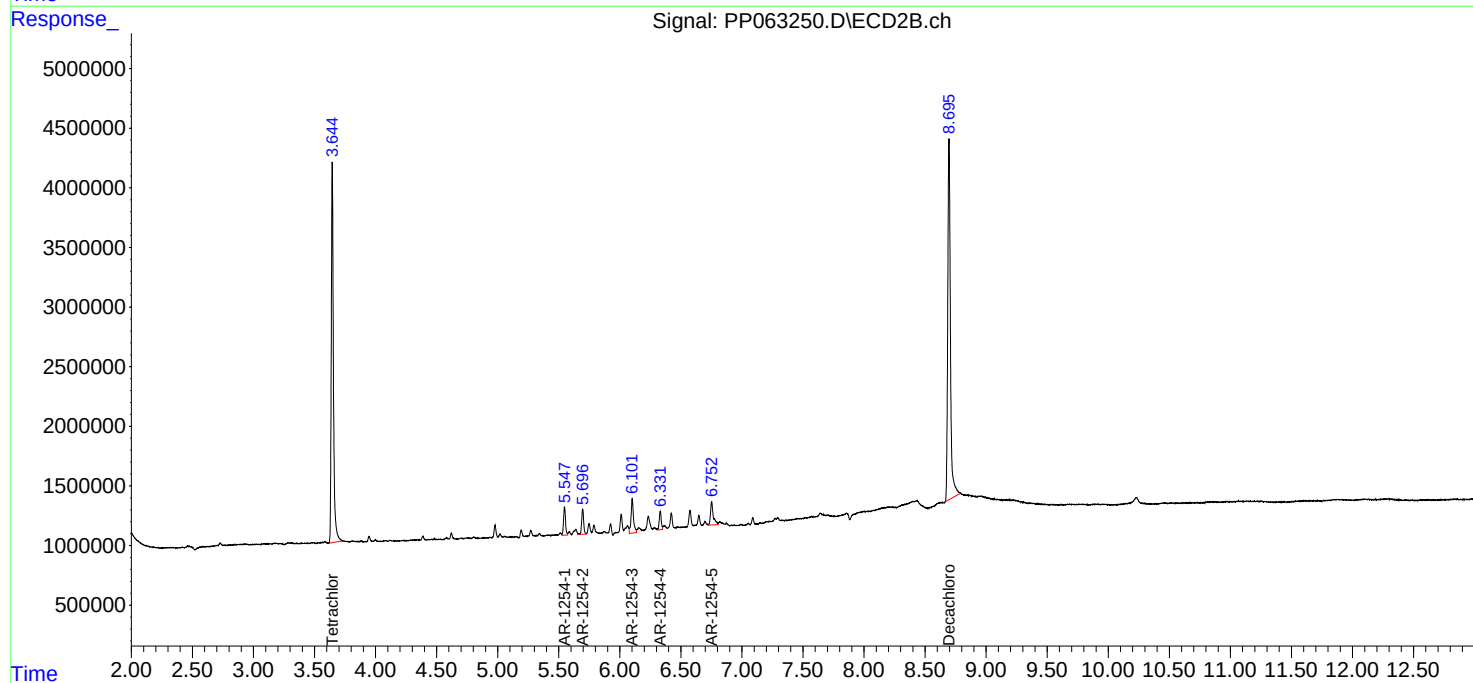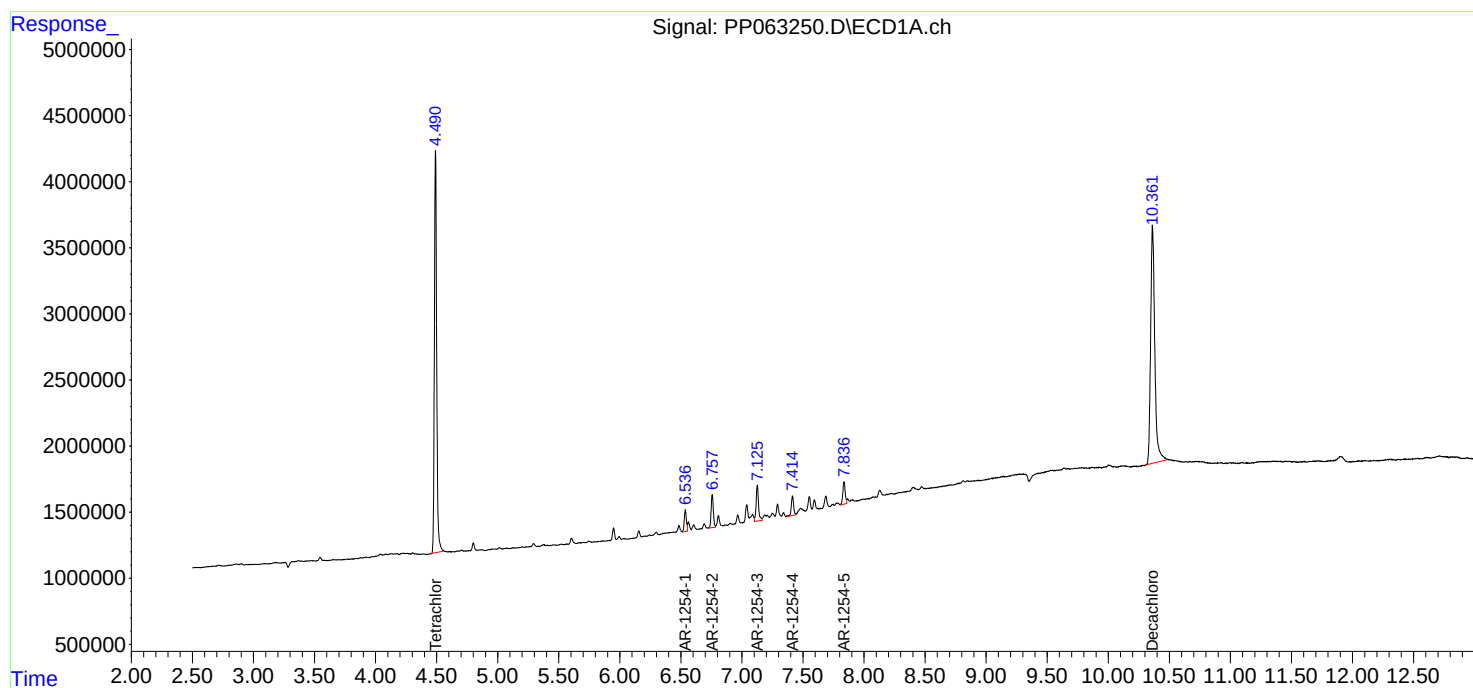


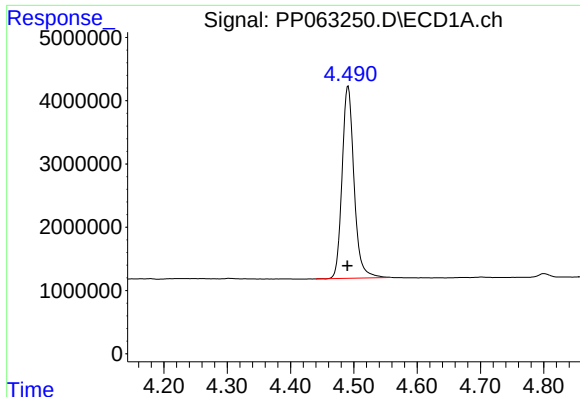

#1 Tetrachloro-m-xylene


R.T.: 4.491 min
Delta R.T.: 0.000 min
Response: 39804740
Conc: 16.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

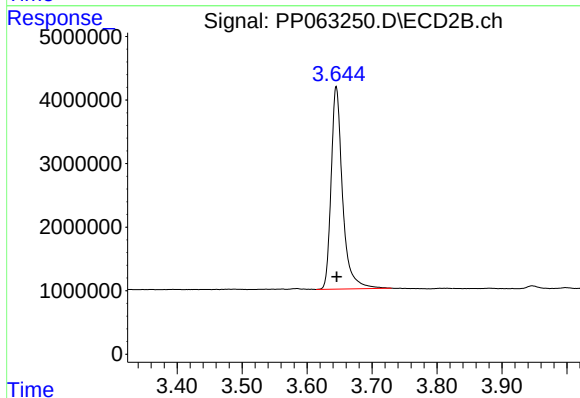


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: 0.000 min
Response: 38919495
Conc: 16.37 ng/ml

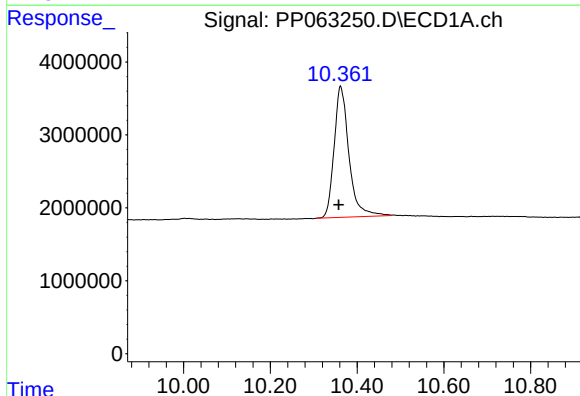


#2 Decachlorobiphenyl

R.T.: 10.362 min
Delta R.T.: 0.004 min
Response: 42573463
Conc: 18.93 ng/ml

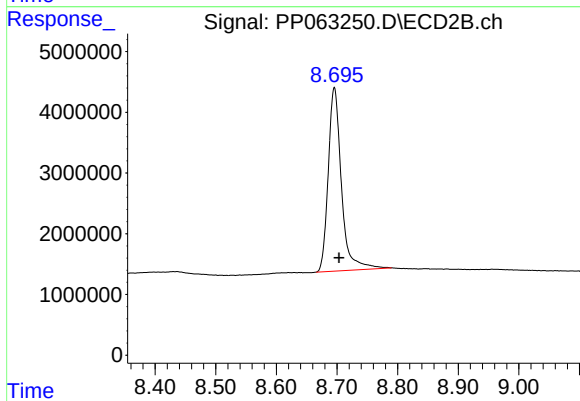

#2 Decachlorobiphenyl


R.T.: 8.696 min
Delta R.T.: -0.008 min
Response: 45749342
Conc: 18.47 ng/ml

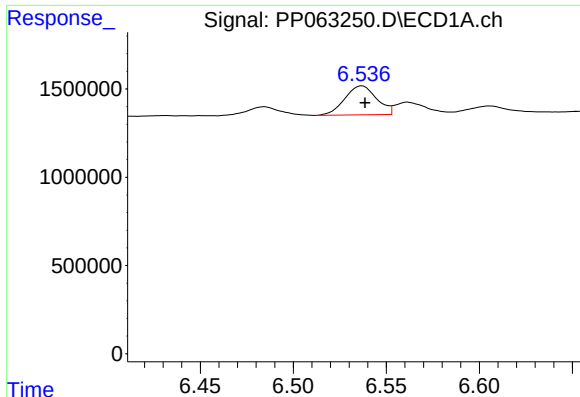

#26 AR-1254-1


R.T.: 6.537 min
Delta R.T.: -0.002 min
Response: 1952960
Conc: 21.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

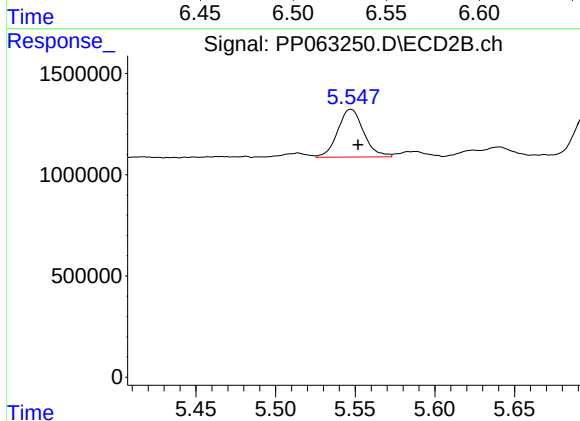


#26 AR-1254-1

R.T.: 5.547 min
Delta R.T.: -0.004 min
Response: 2673373
Conc: 22.04 ng/ml

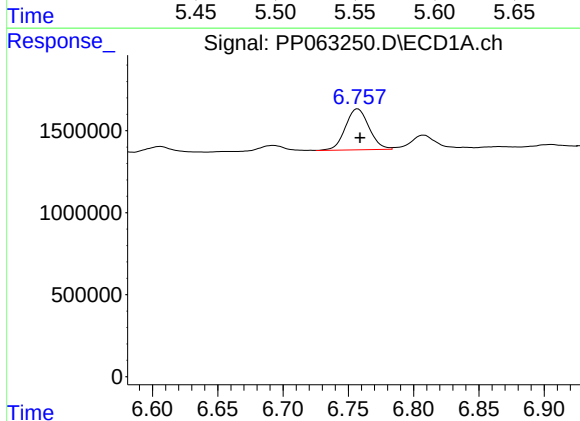


#27 AR-1254-2

R.T.: 6.757 min
Delta R.T.: -0.002 min
Response: 3158035
Conc: 24.06 ng/ml

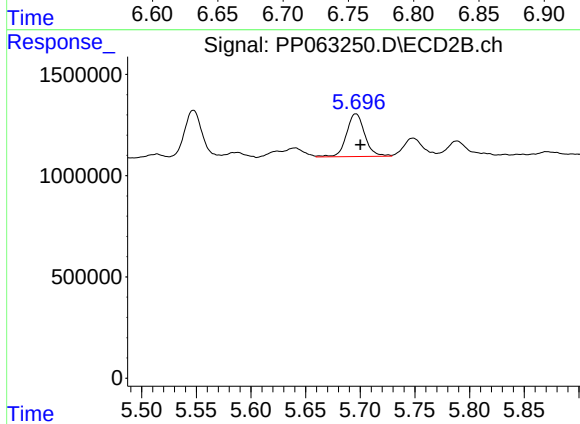

#27 AR-1254-2


R.T.: 5.696 min
Delta R.T.: -0.004 min
Response: 2447588
Conc: 22.56 ng/ml

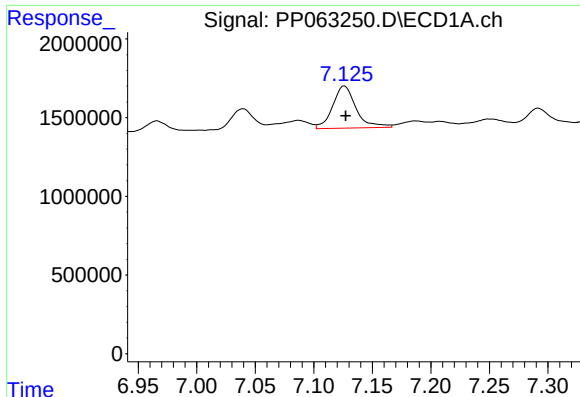

#28 AR-1254-3


R.T.: 7.126 min
Delta R.T.: -0.001 min
Response: 3734191
Conc: 27.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

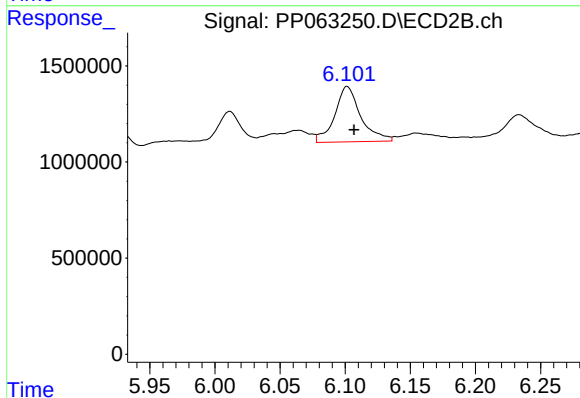


#28 AR-1254-3

R.T.: 6.101 min
Delta R.T.: -0.005 min
Response: 4012645
Conc: 23.41 ng/ml

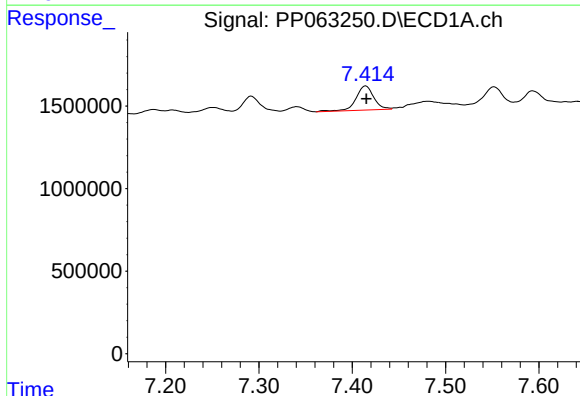


#29 AR-1254-4

R.T.: 7.414 min
Delta R.T.: 0.000 min
Response: 1939783
Conc: 24.56 ng/ml

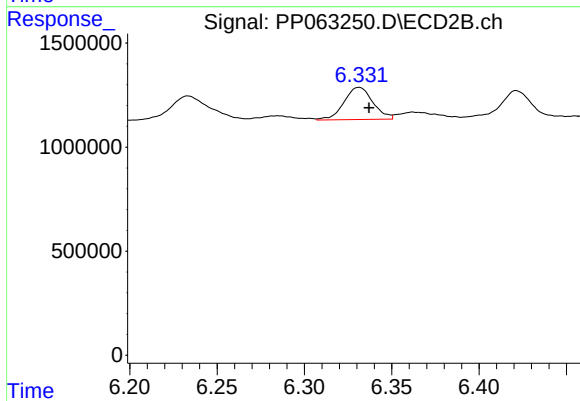

#29 AR-1254-4


R.T.: 6.331 min
Delta R.T.: -0.006 min
Response: 1778865
Conc: 21.86 ng/ml

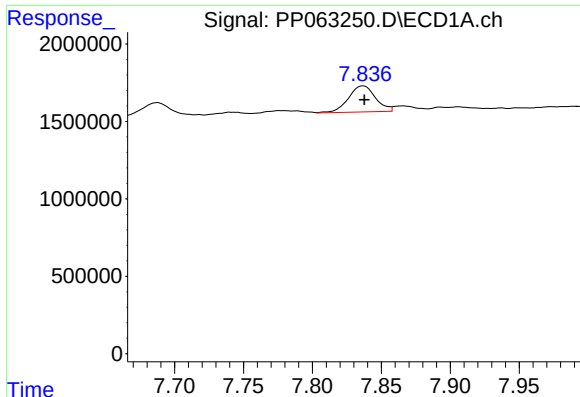

#30 AR-1254-5

R.T.: 7.837 min
Delta R.T.: 0.000 min
Response: 2291466
Conc: 23.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2024

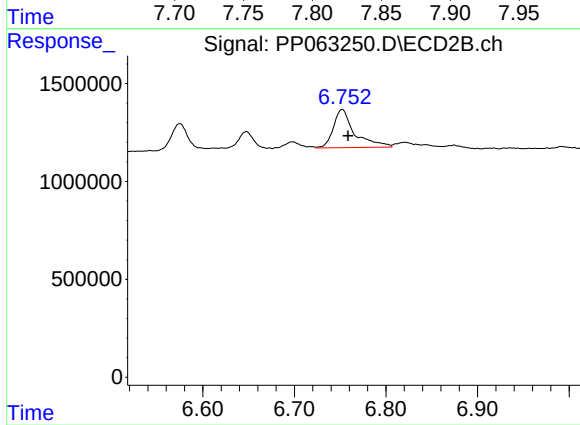

#30 AR-1254-5

R.T.: 6.752 min
Delta R.T.: -0.006 min
Response: 3151790
Conc: 22.18 ng/ml