

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020222\
 Data File : PP043451.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Feb 2022 18:44
 Operator : AJ\MA
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/03/2022
 Supervised By :Ankita Jodhani 02/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 09:07:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 03 09:04:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.865	4.024	147785	143208	4.948	5.738
2) SA Decachlor...	10.777	9.347	82520	111957	5.317m	5.641m
Target Compounds						
21) L5 AR-1248-1	6.169	5.288	25558	28520	53.893	59.081
22) L5 AR-1248-2	6.461	5.552	34237	42293	49.394m	61.889 #
23) L5 AR-1248-3	6.677	5.597	43616	42613	55.590	59.461
24) L5 AR-1248-4	7.100	5.784	39220	52283	50.829	60.891
25) L5 AR-1248-5	7.140	6.207	38087	49697	50.503	58.993m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020222\
Data File : PP043451.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Feb 2022 18:44
Operator : AJ\MA
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2022
Supervised By :Ankita Jodhani 02/03/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 09:07:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 03 09:04:44 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

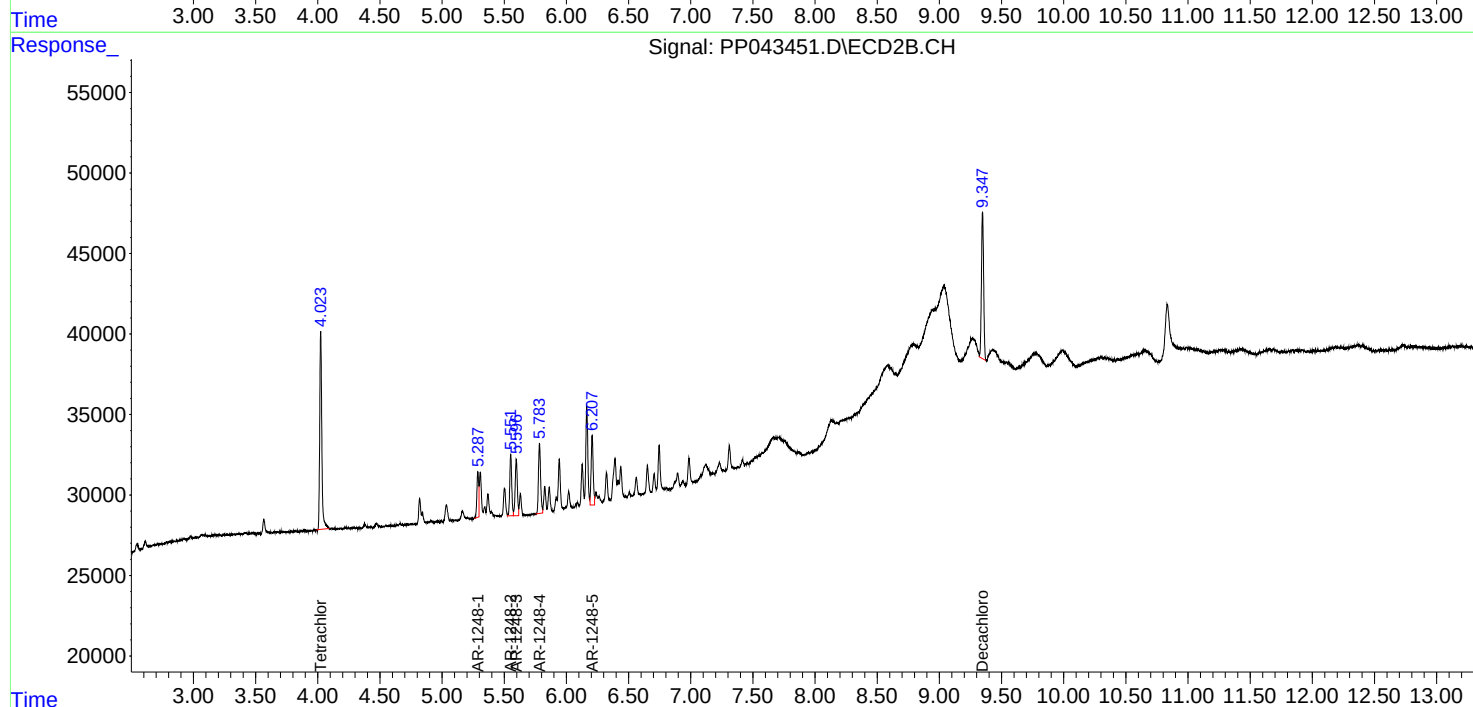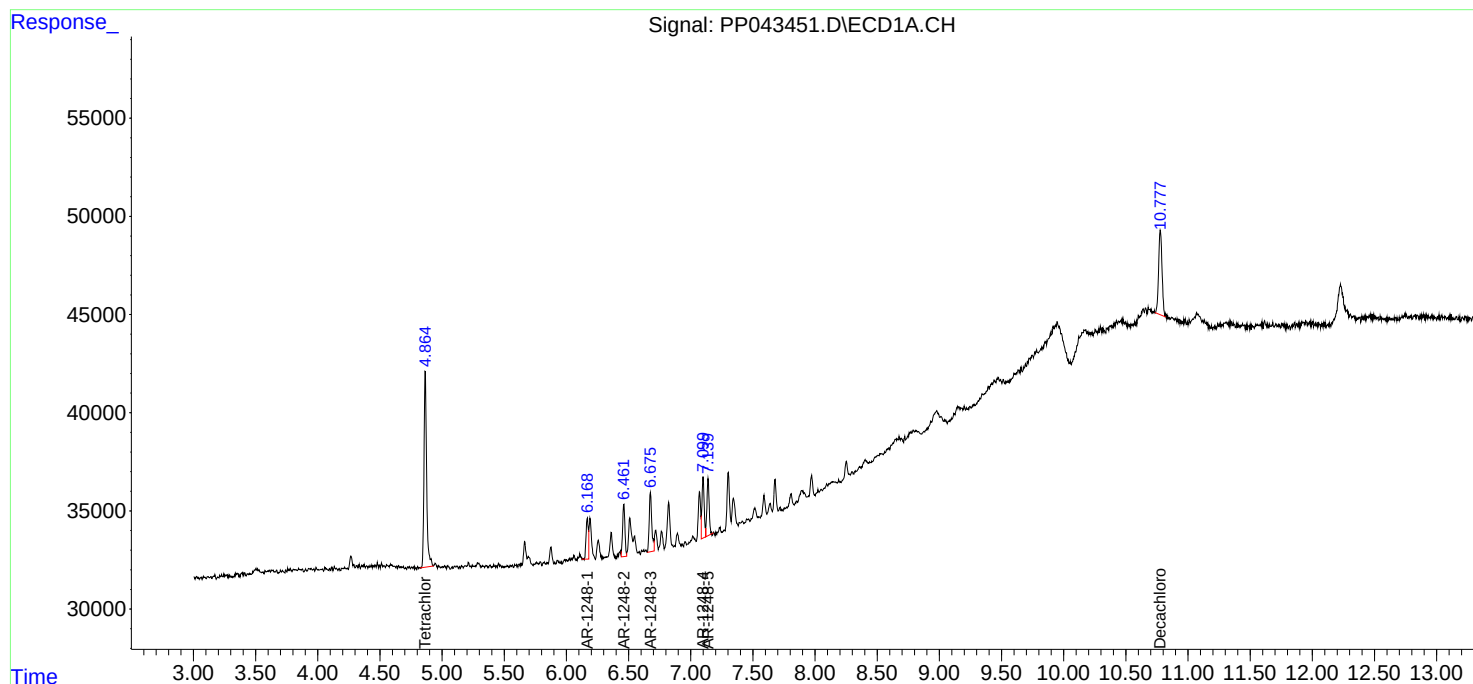

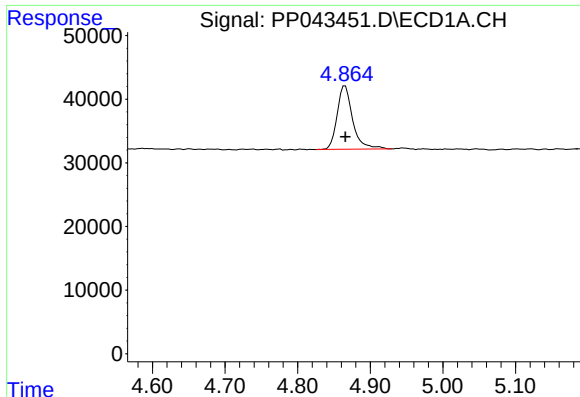


#1 Tetrachloro-m-xylene

R.T.: 4.865 min
Delta R.T.: 0.000 min
Response: 147785
Conc: 4.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2022
Supervised By :Ankita Jodhani 02/03/2022

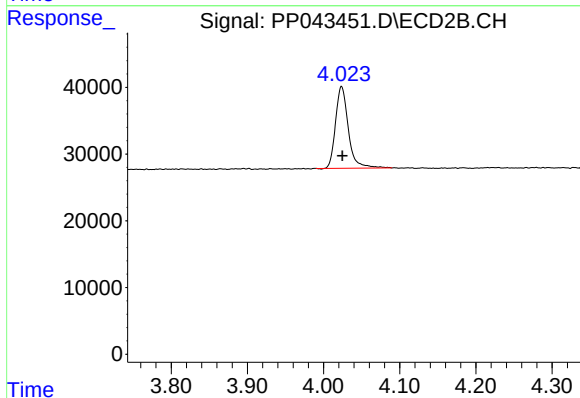


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: -0.001 min
Response: 143208
Conc: 5.74 ng/ml

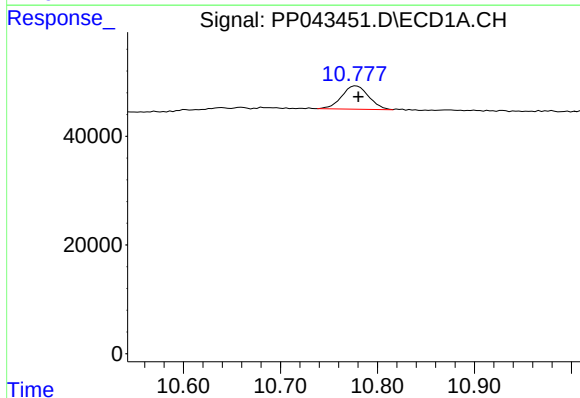


#2 Decachlorobiphenyl

R.T.: 10.777 min
Delta R.T.: -0.004 min
Response: 82520
Conc: 5.32 ng/ml m

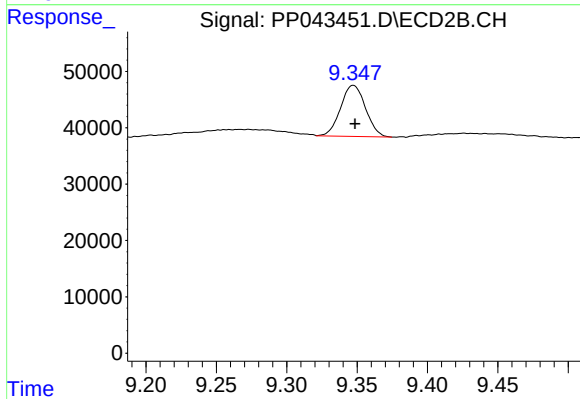

#2 Decachlorobiphenyl

R.T.: 9.347 min
Delta R.T.: -0.002 min
Response: 111957
Conc: 5.64 ng/ml m

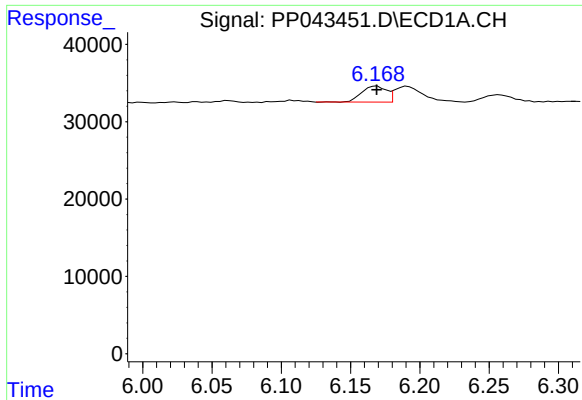


#21 AR-1248-1

R.T.: 6.169 min
Delta R.T.: 0.000 min
Response: 25558
Conc: 53.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2022
Supervised By :Ankita Jodhani 02/03/2022

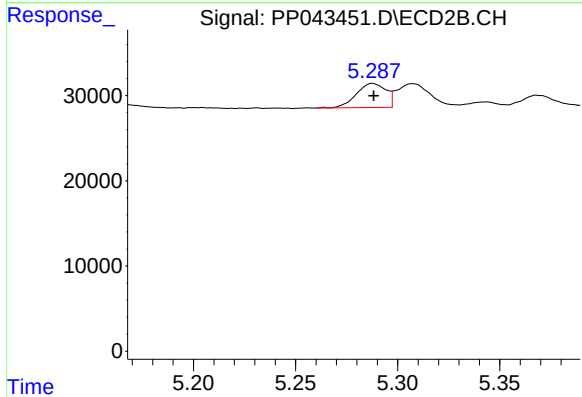


#21 AR-1248-1

R.T.: 5.288 min
Delta R.T.: 0.000 min
Response: 28520
Conc: 59.08 ng/ml

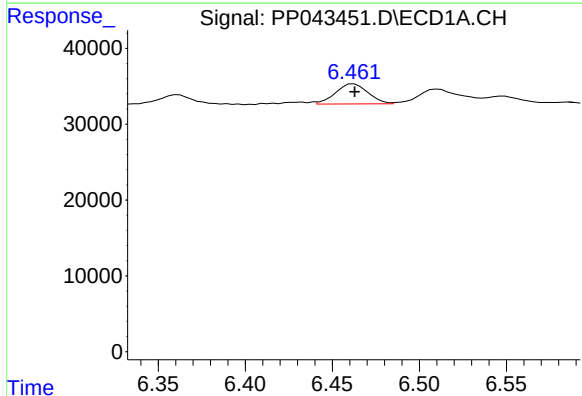


#22 AR-1248-2

R.T.: 6.461 min
Delta R.T.: -0.002 min
Response: 34237
Conc: 49.39 ng/ml m

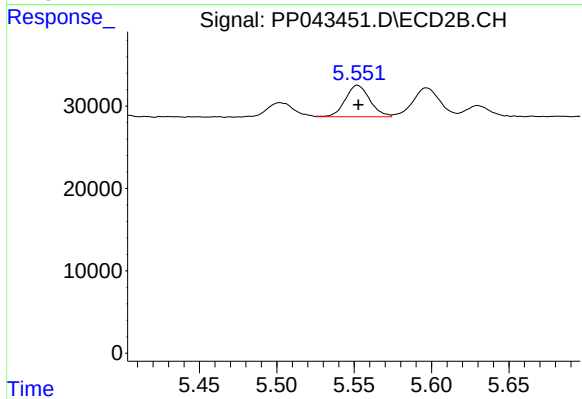

#22 AR-1248-2

R.T.: 5.552 min
Delta R.T.: 0.000 min
Response: 42293
Conc: 61.89 ng/ml

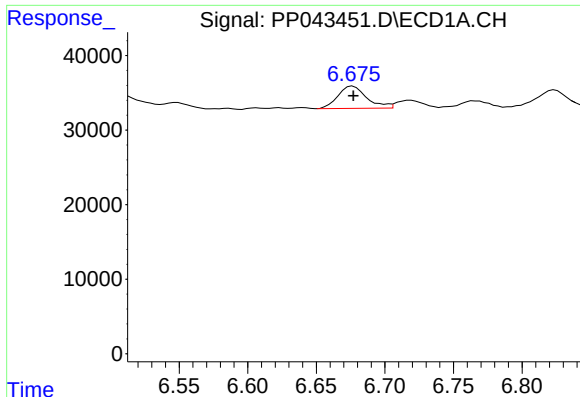


#23 AR-1248-3

R.T.: 6.677 min
Delta R.T.: 0.000 min
Response: 43616
Conc: 55.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2022
Supervised By :Ankita Jodhani 02/03/2022

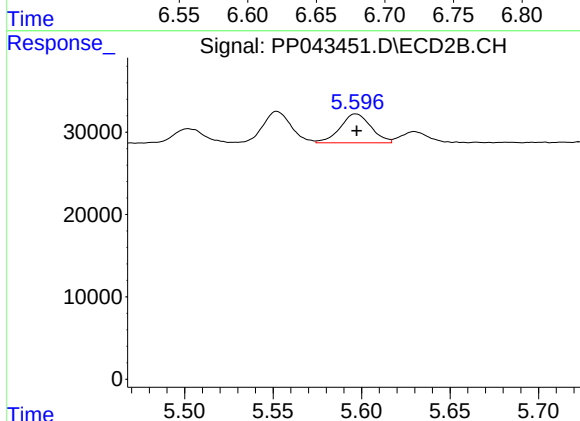


#23 AR-1248-3

R.T.: 5.597 min
Delta R.T.: 0.000 min
Response: 42613
Conc: 59.46 ng/ml

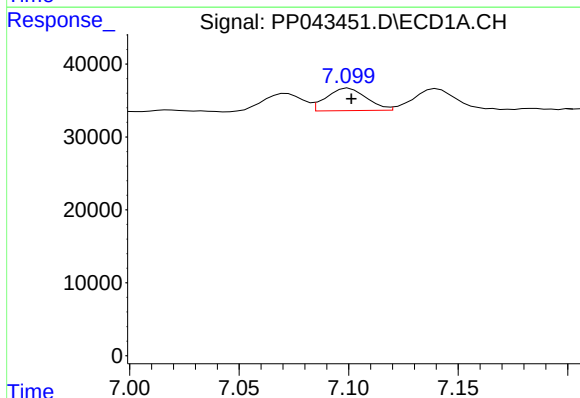


#24 AR-1248-4

R.T.: 7.100 min
Delta R.T.: -0.001 min
Response: 39220
Conc: 50.83 ng/ml

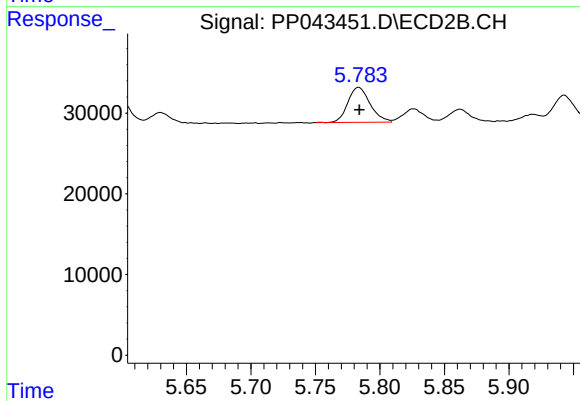

#24 AR-1248-4

R.T.: 5.784 min
Delta R.T.: 0.000 min
Response: 52283
Conc: 60.89 ng/ml

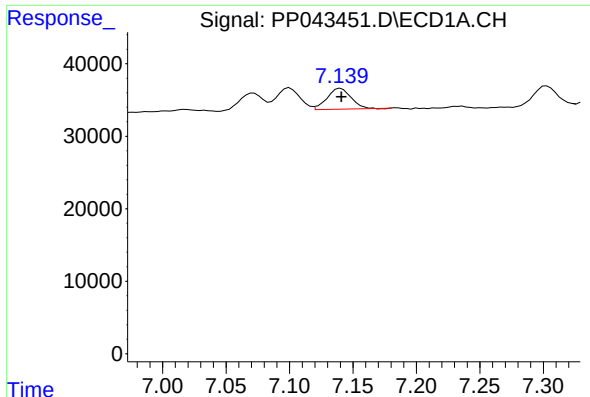


#25 AR-1248-5

R.T.: 7.140 min
Delta R.T.: 0.000 min
Response: 38087
Conc: 50.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2022
Supervised By :Ankita Jodhani 02/03/2022

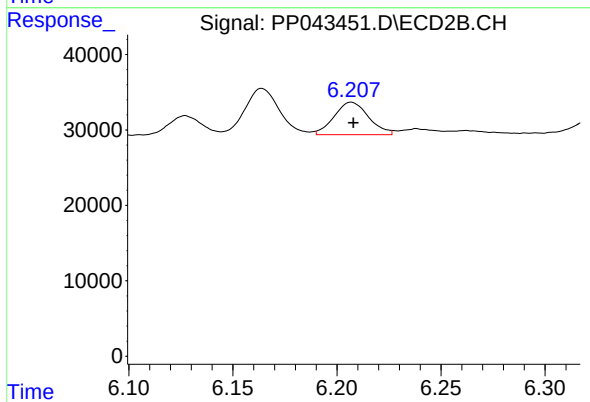

#25 AR-1248-5

R.T.: 6.207 min
Delta R.T.: -0.001 min
Response: 49697
Conc: 58.99 ng/ml m