

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020222\
 Data File : PP043456.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Feb 2022 20:07
 Operator : AJ\MA
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/03/2022
 Supervised By :Ankita Jodhani 02/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 09:30:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 03 09:30:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.866	4.024	154673	146522	5.171	5.770
2) SA Decachlor...	10.780	9.348	87164	113572	5.511	5.553
Target Compounds						
26) L6 AR-1254-1	7.073	6.165	46592	82138	53.813m	61.317
27) L6 AR-1254-2	7.302	6.323	72084	69427	56.166	59.550
28) L6 AR-1254-3	7.680	6.747	66527	106355	51.822	57.772
29) L6 AR-1254-4	7.973	6.987	46465	63477	54.079	57.451
30) L6 AR-1254-5	8.400	7.417	47674	87243	51.356	56.514

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020222\
Data File : PP043456.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Feb 2022 20:07
Operator : AJ\MA
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2022
Supervised By :Ankita Jodhani 02/03/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 09:30:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 03 09:30:16 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

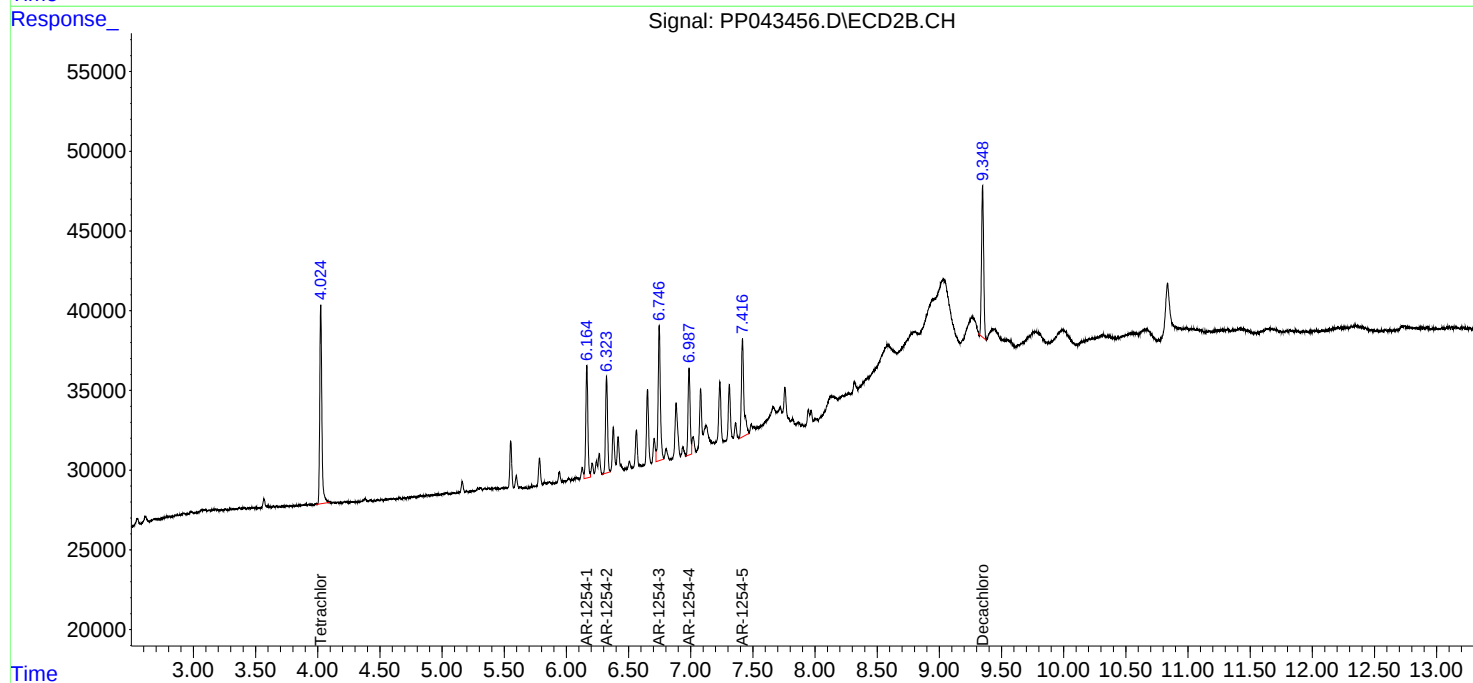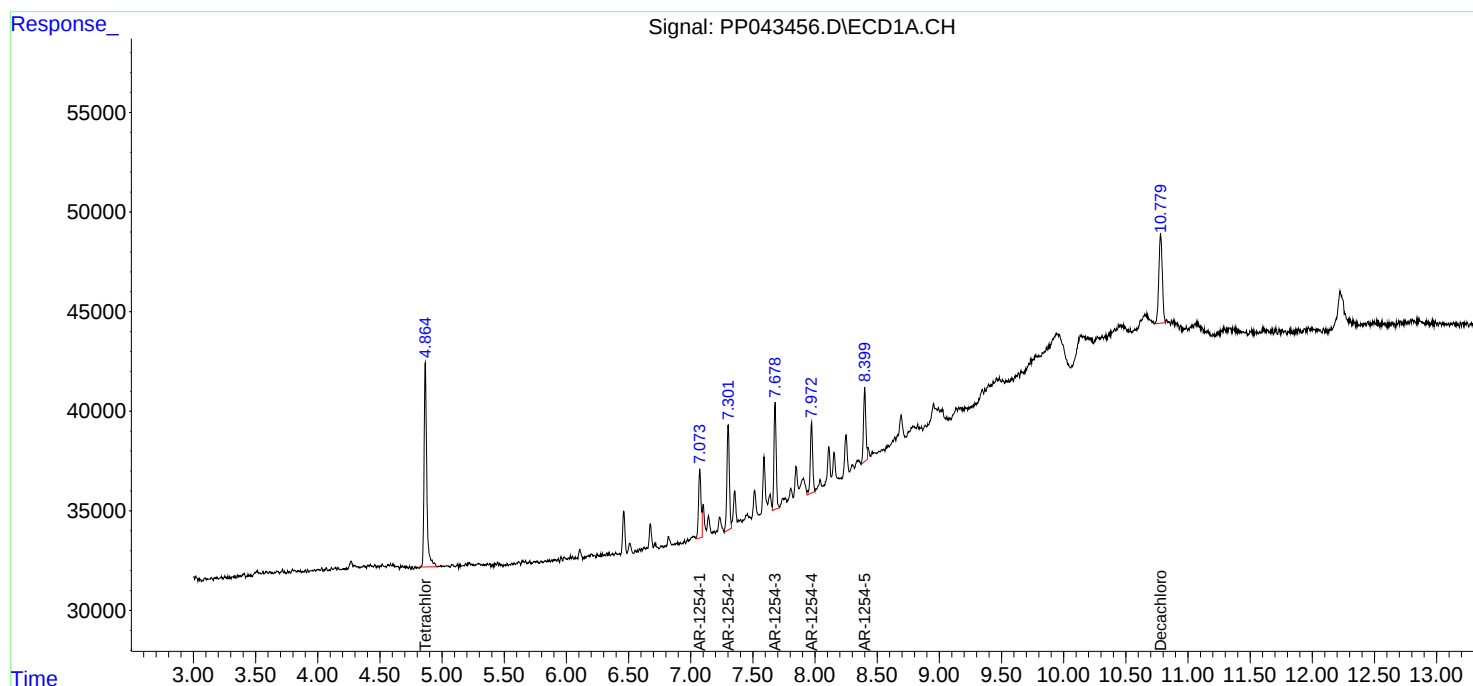

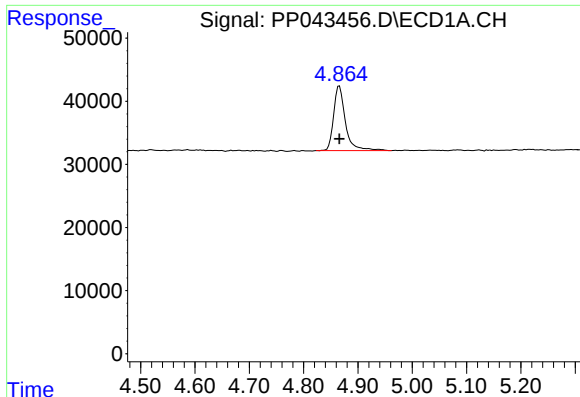


#1 Tetrachloro-m-xylene

R.T.: 4.866 min
Delta R.T.: 0.000 min
Response: 154673
Conc: 5.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2022
Supervised By :Ankita Jodhani 02/03/2022

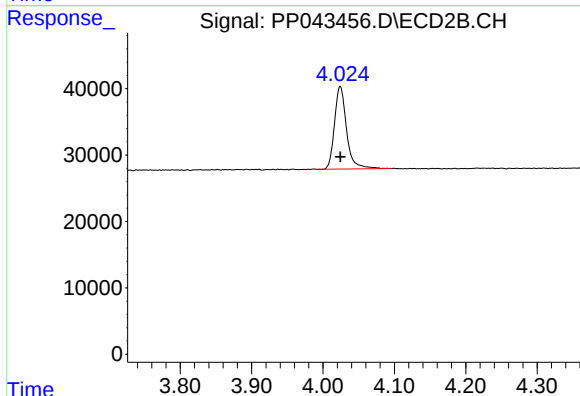


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 146522
Conc: 5.77 ng/ml

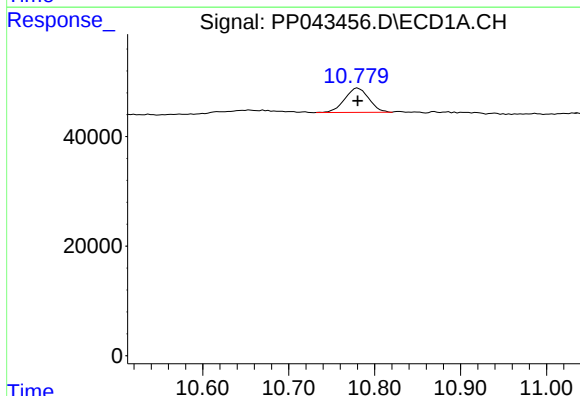


#2 Decachlorobiphenyl

R.T.: 10.780 min
Delta R.T.: 0.000 min
Response: 87164
Conc: 5.51 ng/ml

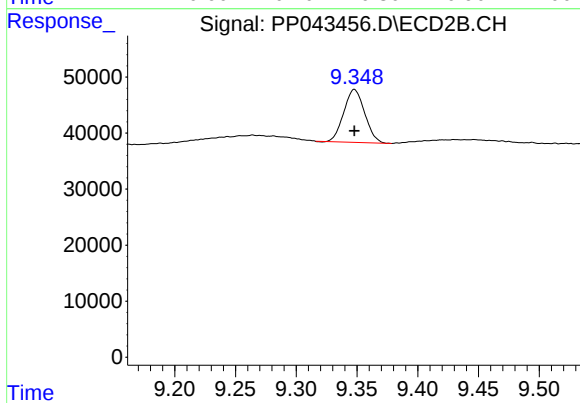

#2 Decachlorobiphenyl

R.T.: 9.348 min
Delta R.T.: 0.000 min
Response: 113572
Conc: 5.55 ng/ml

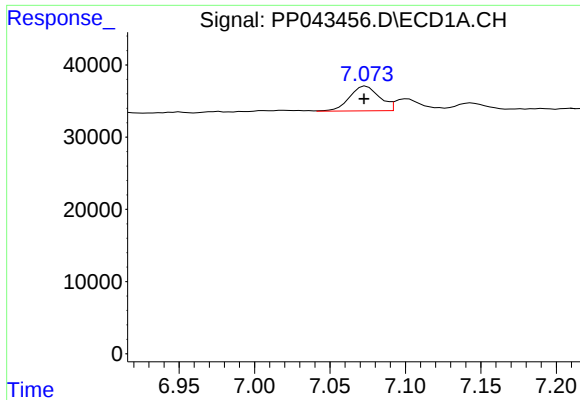


#26 AR-1254-1

R.T.: 7.073 min
Delta R.T.: 0.000 min
Response: 46592
Conc: 53.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254\ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2022
Supervised By :Ankita Jodhani 02/03/2022

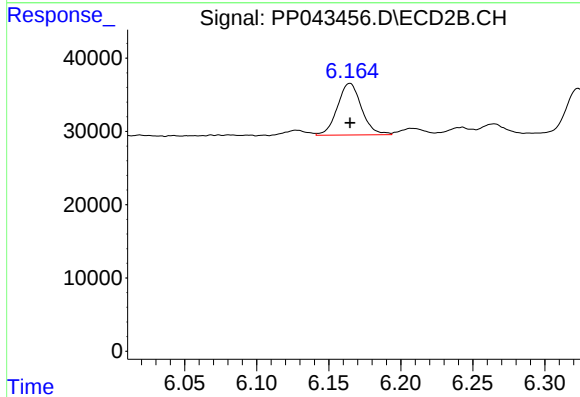


#26 AR-1254-1

R.T.: 6.165 min
Delta R.T.: 0.000 min
Response: 82138
Conc: 61.32 ng/ml

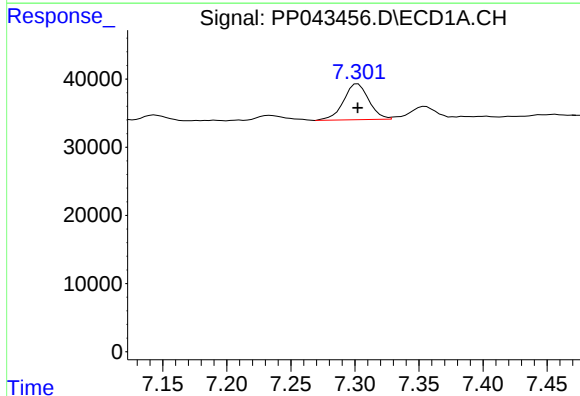


#27 AR-1254-2

R.T.: 7.302 min
Delta R.T.: 0.000 min
Response: 72084
Conc: 56.17 ng/ml

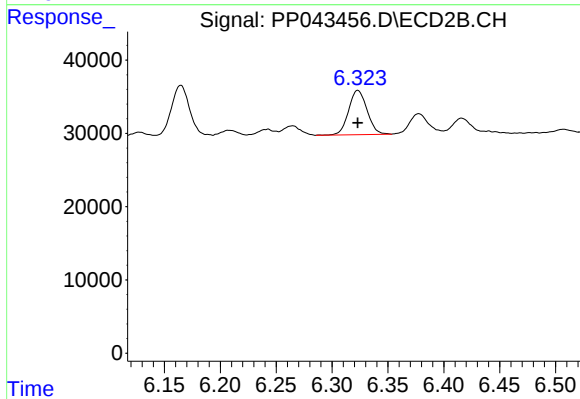

#27 AR-1254-2

R.T.: 6.323 min
Delta R.T.: 0.000 min
Response: 69427
Conc: 59.55 ng/ml

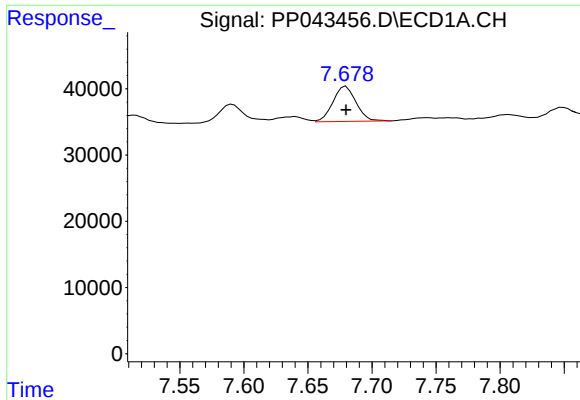


#28 AR-1254-3

R.T.: 7.680 min
Delta R.T.: 0.000 min
Response: 66527
Conc: 51.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254\ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2022
Supervised By :Ankita Jodhani 02/03/2022

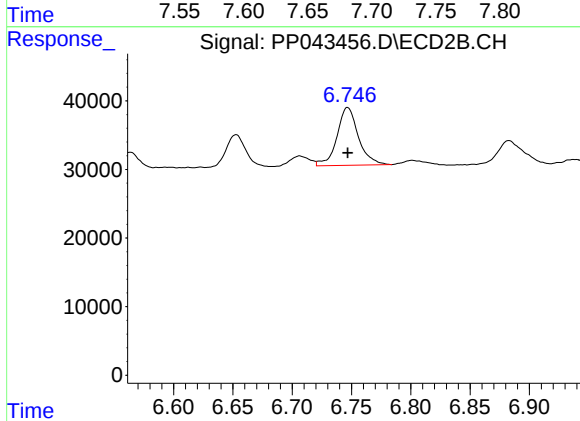


#28 AR-1254-3

R.T.: 6.747 min
Delta R.T.: 0.000 min
Response: 106355
Conc: 57.77 ng/ml

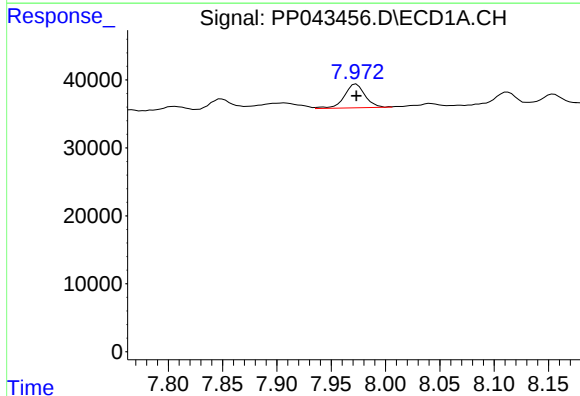


#29 AR-1254-4

R.T.: 7.973 min
Delta R.T.: 0.000 min
Response: 46465
Conc: 54.08 ng/ml

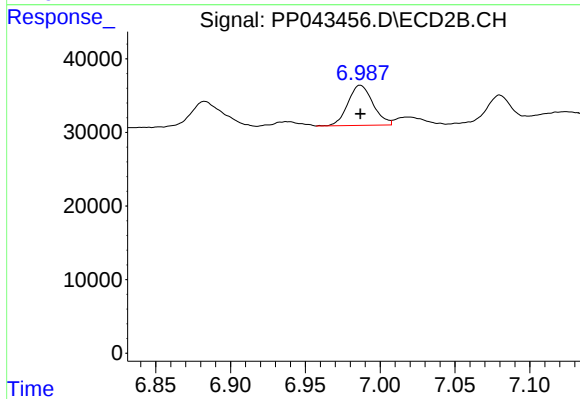

#29 AR-1254-4

R.T.: 6.987 min
Delta R.T.: 0.000 min
Response: 63477
Conc: 57.45 ng/ml

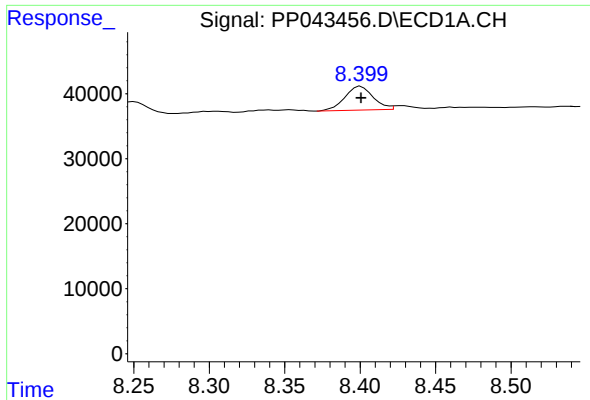


#30 AR-1254-5

R.T.: 8.400 min
Delta R.T.: 0.000 min
Response: 47674
Conc: 51.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2022
Supervised By :Ankita Jodhani 02/03/2022

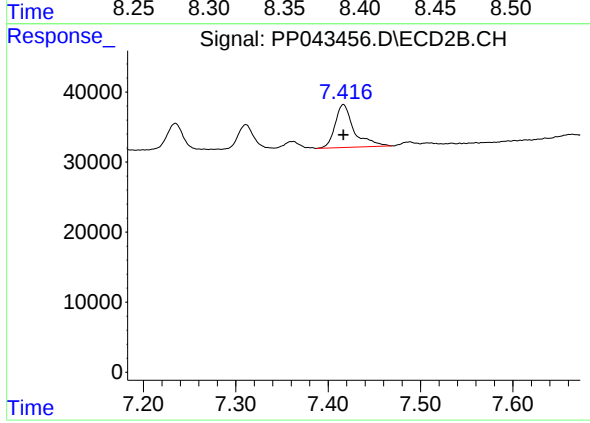

#30 AR-1254-5

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 87243
Conc: 56.51 ng/ml