

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020222\
 Data File : PP043462.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Feb 2022 21:47
 Operator : AJ\MA
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/03/2022
 Supervised By :Ankita Jodhani 02/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 09:15:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 03 09:01:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.867	4.026	121986	138592	4.416	5.668m#
2) SA Decachlor...	10.781	9.348	146219	195797	5.517	5.743
Target Compounds						
41) L9 AR-1268-1	9.328	8.254	122460	154113	55.589	54.388
42) L9 AR-1268-2	9.420	8.321	117153	155014	55.759	56.226
43) L9 AR-1268-3	9.641	8.527	97147	206315	53.837	77.578 #
44) L9 AR-1268-4	10.056	8.818	30663	53324	47.381	54.051
45) L9 AR-1268-5	10.456	9.102	361656	392194	62.206	55.510

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020222\
Data File : PP043462.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Feb 2022 21:47
Operator : AJ\MA
Sample : AR1268ICC050
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2022
Supervised By :Ankita Jodhani 02/03/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 09:15:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 03 09:01:44 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

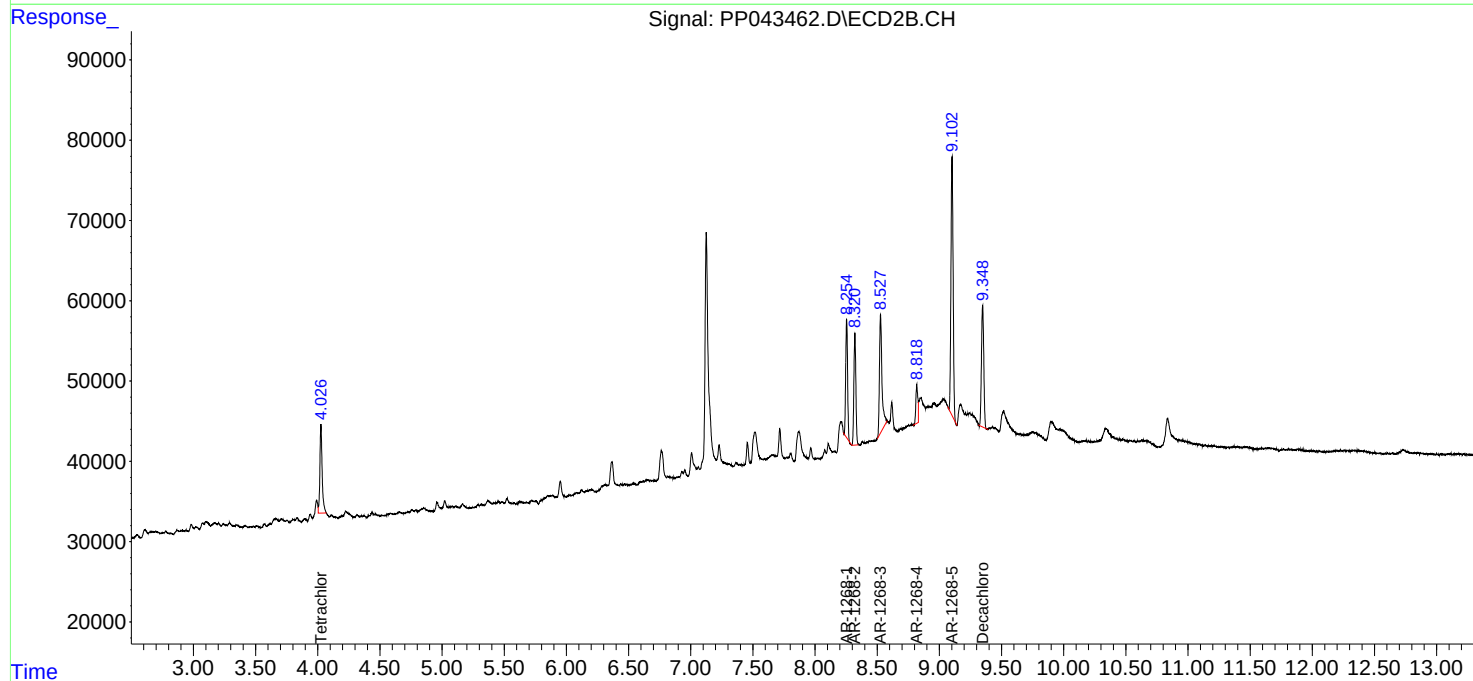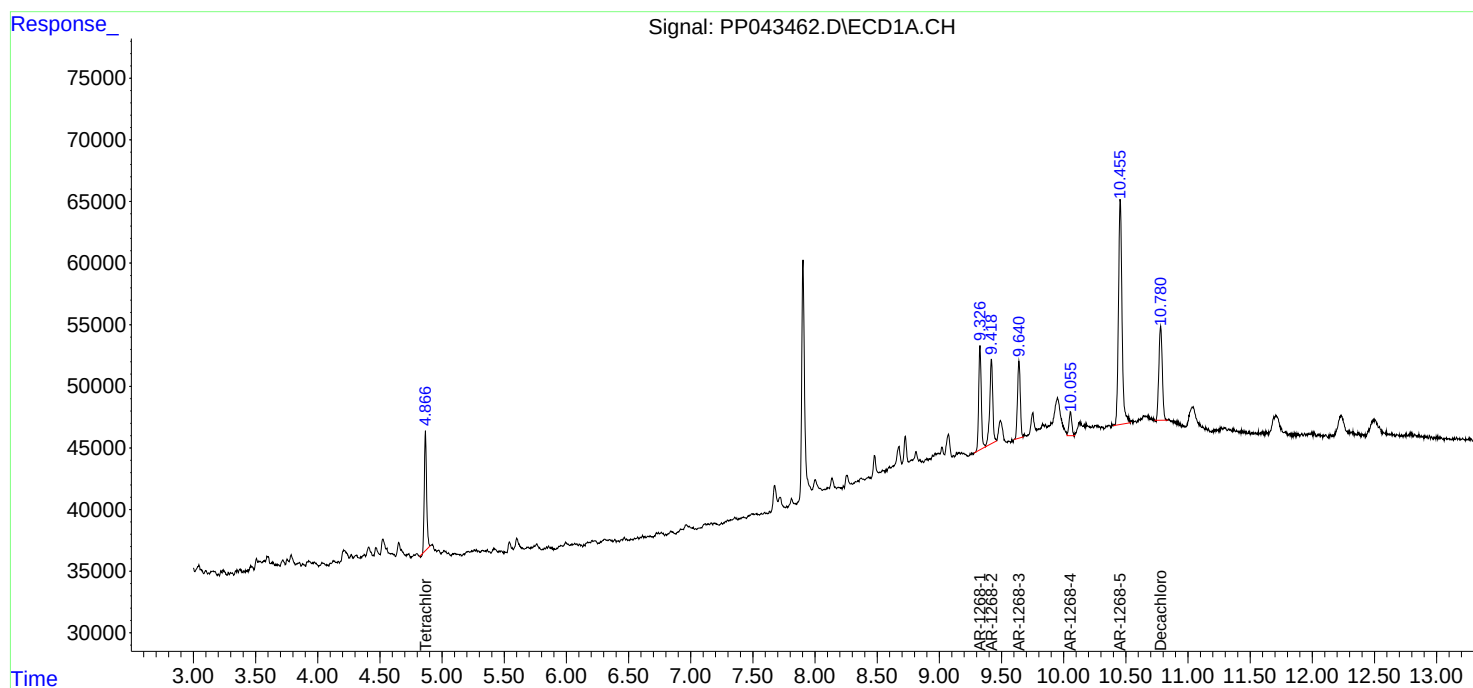

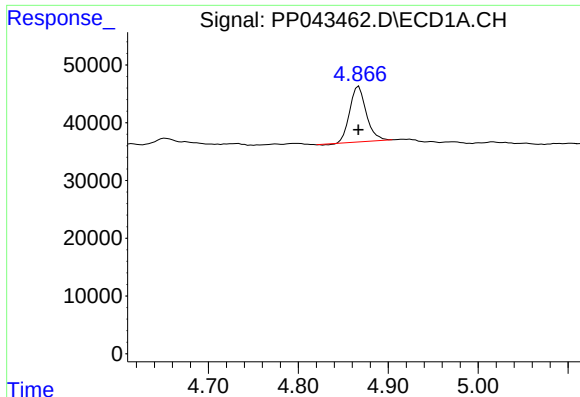


#1 Tetrachloro-m-xylene

R.T.: 4.867 min
Delta R.T.: 0.000 min
Response: 121986
Conc: 4.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2022
Supervised By :Ankita Jodhani 02/03/2022

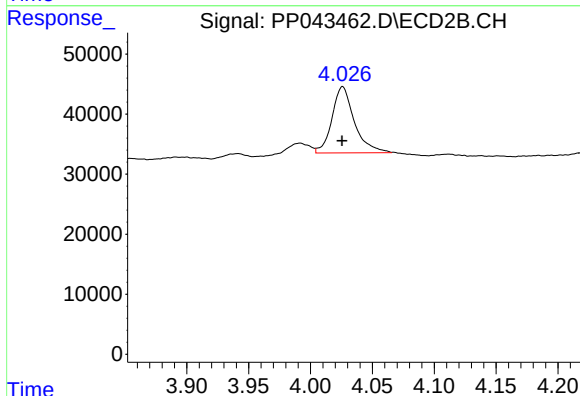


#1 Tetrachloro-m-xylene

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 138592
Conc: 5.67 ng/ml m

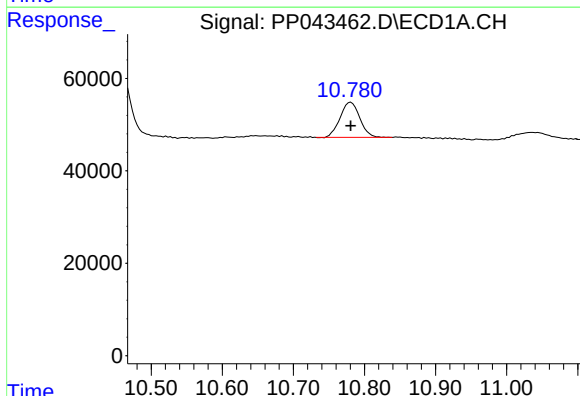


#2 Decachlorobiphenyl

R.T.: 10.781 min
Delta R.T.: 0.000 min
Response: 146219
Conc: 5.52 ng/ml

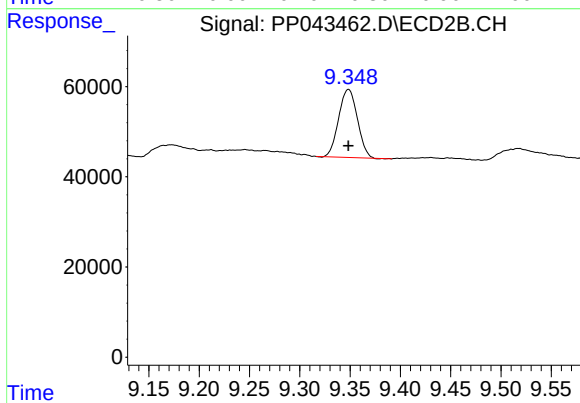

#2 Decachlorobiphenyl

R.T.: 9.348 min
Delta R.T.: 0.000 min
Response: 195797
Conc: 5.74 ng/ml

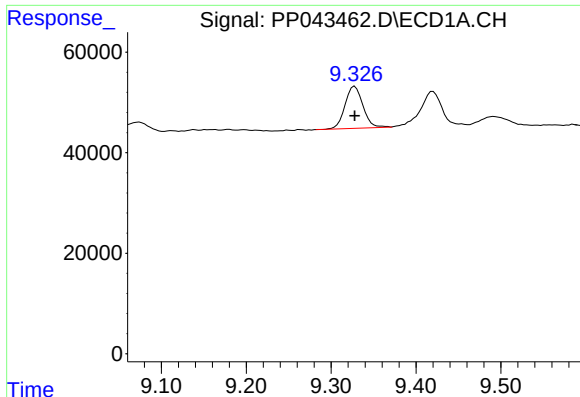


#41 AR-1268-1

R.T.: 9.328 min
Delta R.T.: 0.000 min
Response: 122460
Conc: 55.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2022
Supervised By :Ankita Jodhani 02/03/2022

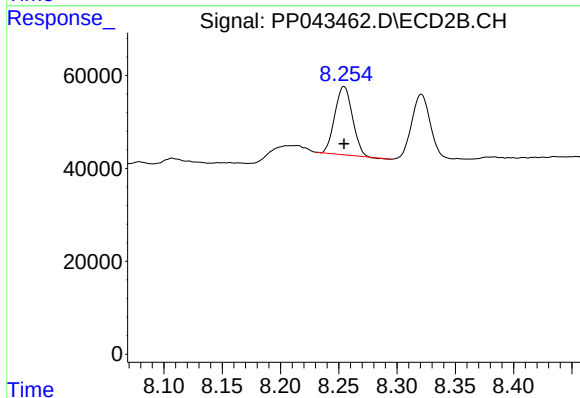


#41 AR-1268-1

R.T.: 8.254 min
Delta R.T.: 0.000 min
Response: 154113
Conc: 54.39 ng/ml

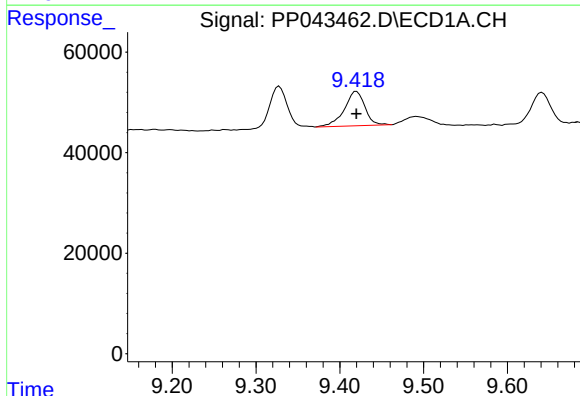


#42 AR-1268-2

R.T.: 9.420 min
Delta R.T.: 0.000 min
Response: 117153
Conc: 55.76 ng/ml

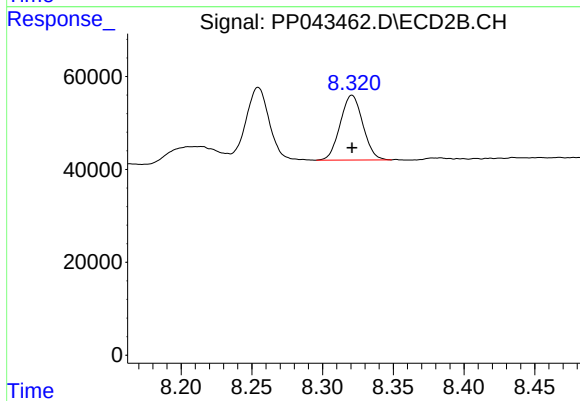

#42 AR-1268-2

R.T.: 8.321 min
Delta R.T.: 0.000 min
Response: 155014
Conc: 56.23 ng/ml

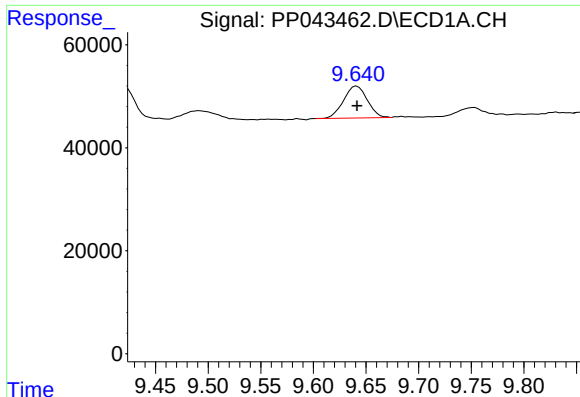


#43 AR-1268-3

R.T.: 9.641 min
Delta R.T.: 0.000 min
Response: 97147
Conc: 53.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2022
Supervised By :Ankita Jodhani 02/03/2022

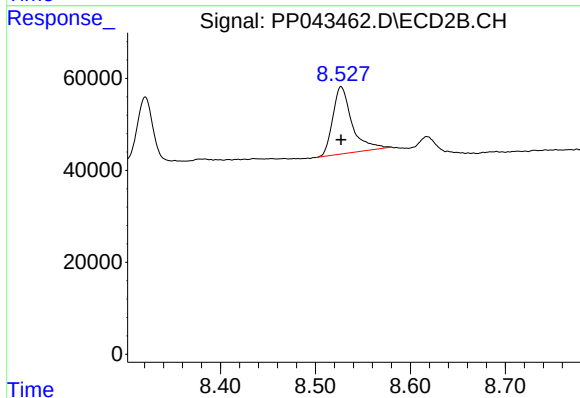


#43 AR-1268-3

R.T.: 8.527 min
Delta R.T.: 0.000 min
Response: 206315
Conc: 77.58 ng/ml

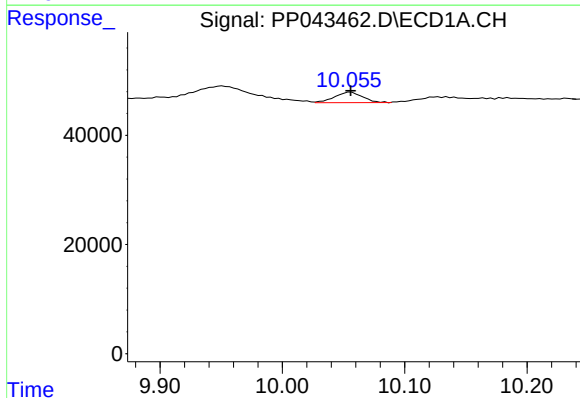


#44 AR-1268-4

R.T.: 10.056 min
Delta R.T.: 0.000 min
Response: 30663
Conc: 47.38 ng/ml

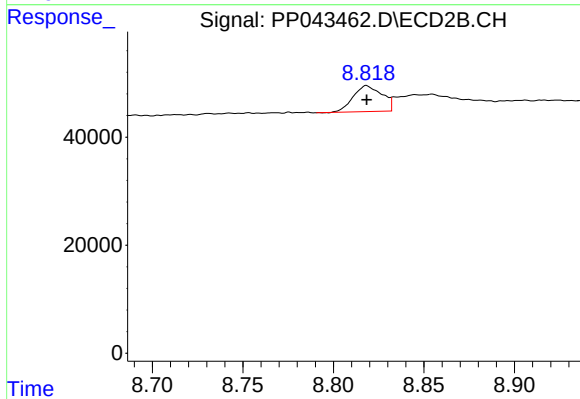

#44 AR-1268-4

R.T.: 8.818 min
Delta R.T.: 0.000 min
Response: 53324
Conc: 54.05 ng/ml

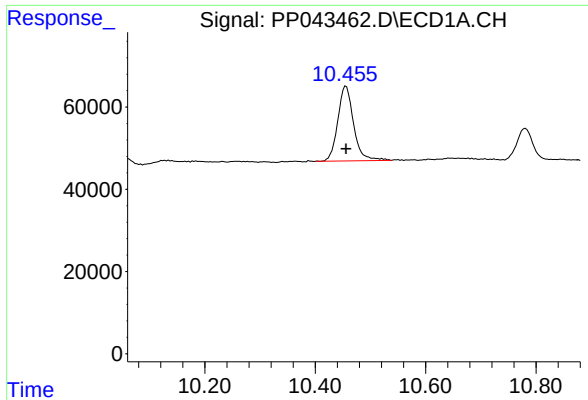


#45 AR-1268-5

R.T.: 10.456 min
Delta R.T.: 0.000 min
Response: 361656
Conc: 62.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2022
Supervised By :Ankita Jodhani 02/03/2022

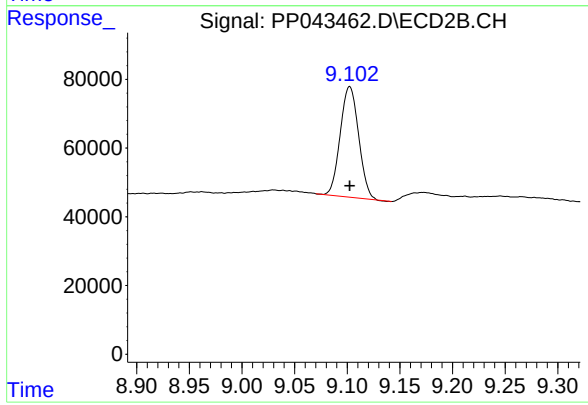

#45 AR-1268-5

R.T.: 9.102 min
Delta R.T.: 0.000 min
Response: 392194
Conc: 55.51 ng/ml