

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020322\
 Data File : PP043483.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Feb 2022 15:25
 Operator : AJ\MA
 Sample : N1382-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 00:53:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 03 10:01:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.867	4.025	583781	503813	21.271	22.245
2)	SA Decachlor...	10.781	9.348	300539	363561	19.592	19.231
Target Compounds							
8)	L2 AR-1221-1	5.102	0.000	17756	0	61.537	N.D. #
9)	L2 AR-1221-2	0.000	4.359f	0	6287	N.D.	27.677 #
12)	L3 AR-1232-2	5.857f	0.000	17388	0	66.066	N.D. #
39)	L8 AR-1262-4	9.428	0.000	8068	0	15.340	N.D. #
40)	L8 AR-1262-5	0.000	8.849f	0	24545	N.D.	28.525 #
42)	L9 AR-1268-2	9.428	0.000	8068	0	3.876	N.D. #
43)	L9 AR-1268-3	0.000	8.533	0	35518	N.D.	15.164 #
44)	L9 AR-1268-4	0.000	8.849f	0	24545	N.D.	24.804 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020322\
Data File : PP043483.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Feb 2022 15:25
Operator : AJ\MA
Sample : N1382-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 00:53:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 03 10:01:05 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

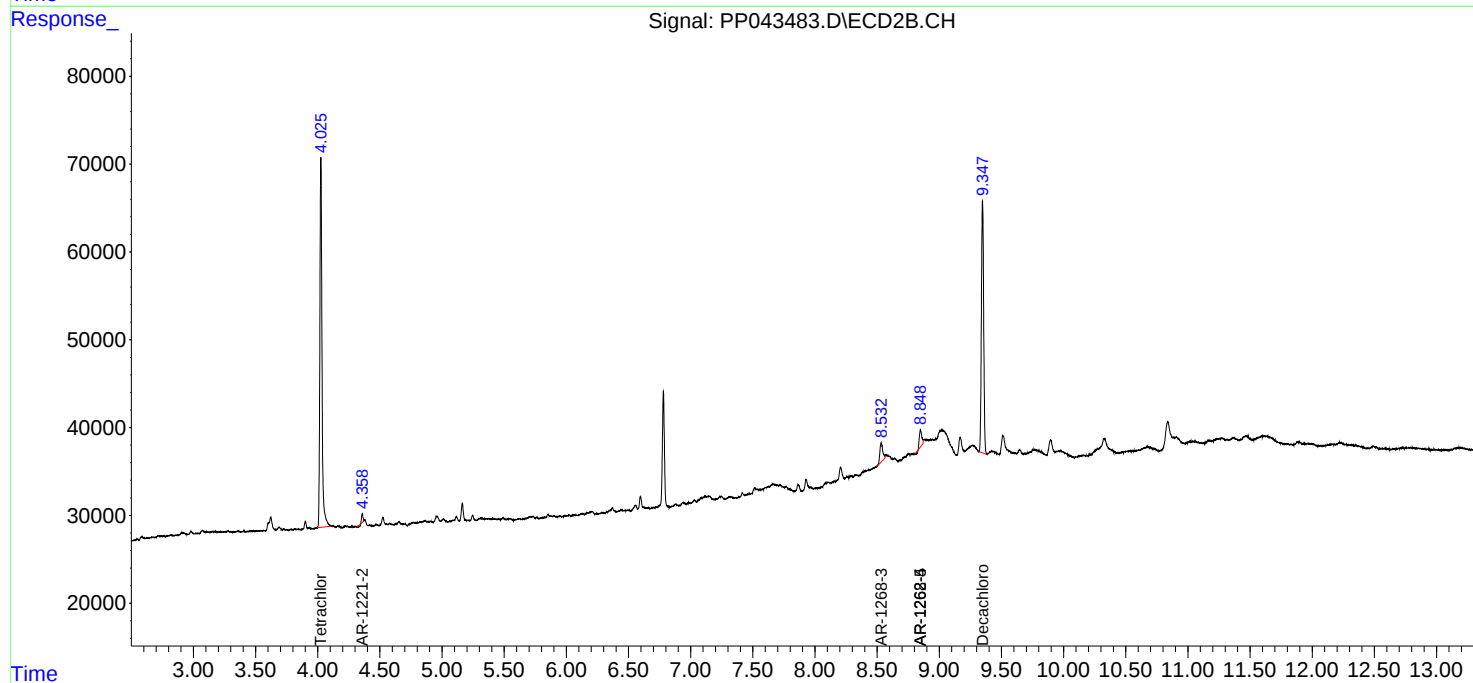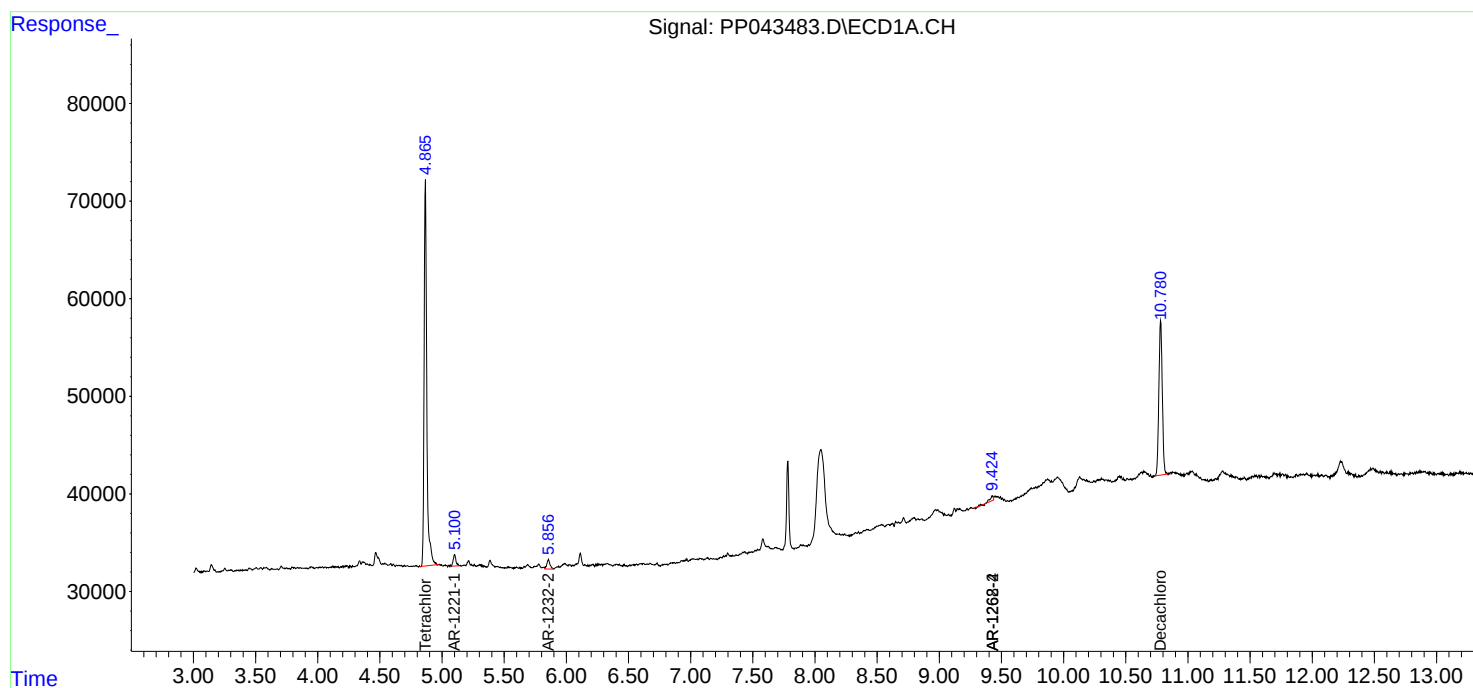


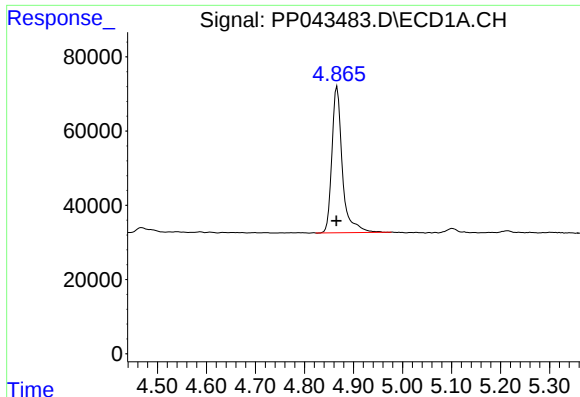

#1 Tetrachloro-m-xylene


R.T.: 4.867 min
Delta R.T.: 0.002 min
Response: 583781
Conc: 21.27 ng/ml

Instrument :
ECD_P
ClientSampleId :

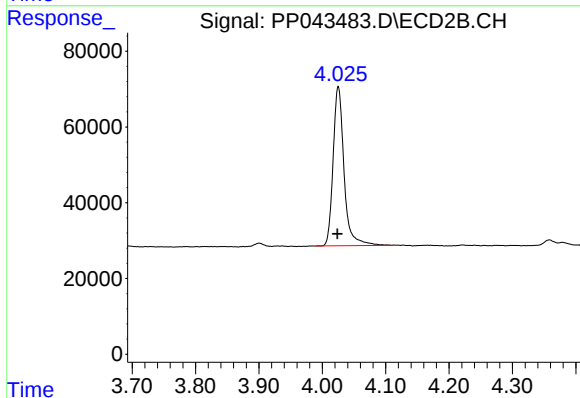


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.001 min
Response: 503813
Conc: 22.24 ng/ml

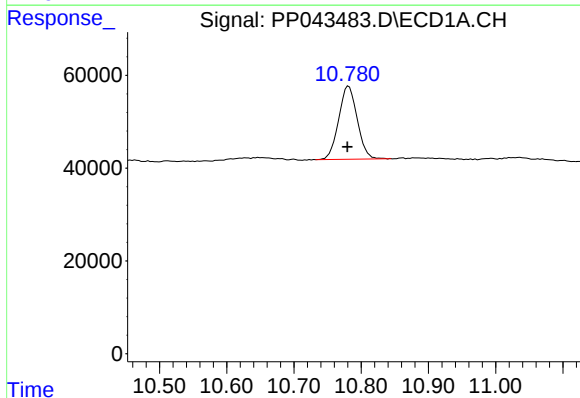


#2 Decachlorobiphenyl

R.T.: 10.781 min
Delta R.T.: 0.002 min
Response: 300539
Conc: 19.59 ng/ml

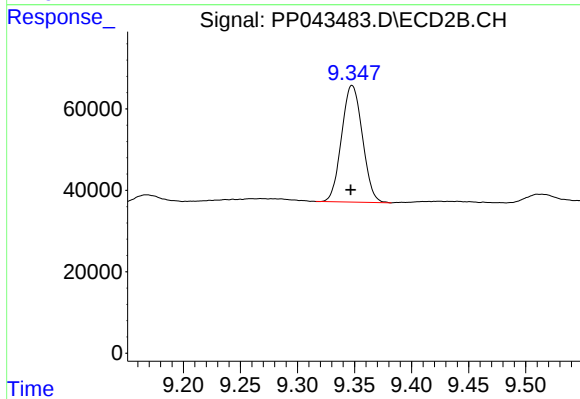

#2 Decachlorobiphenyl


R.T.: 9.348 min
Delta R.T.: 0.001 min
Response: 363561
Conc: 19.23 ng/ml

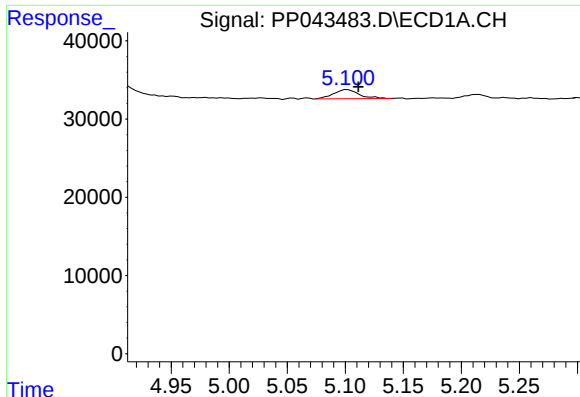

#8 AR-1221-1


R.T.: 5.102 min
Delta R.T.: -0.010 min
Response: 17756
Conc: 61.54 ng/ml

Instrument :
ECD_P
ClientSampleId :

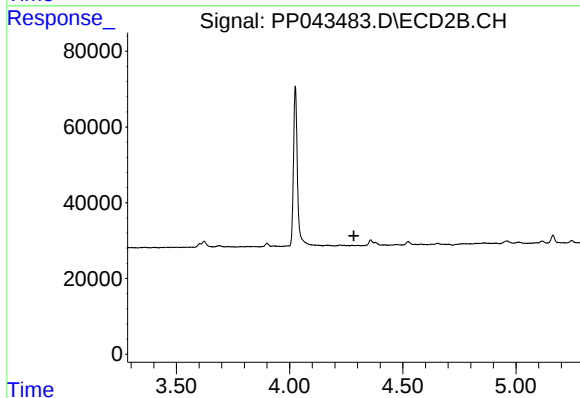


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.284 min
Response: 0
Conc: N.D.

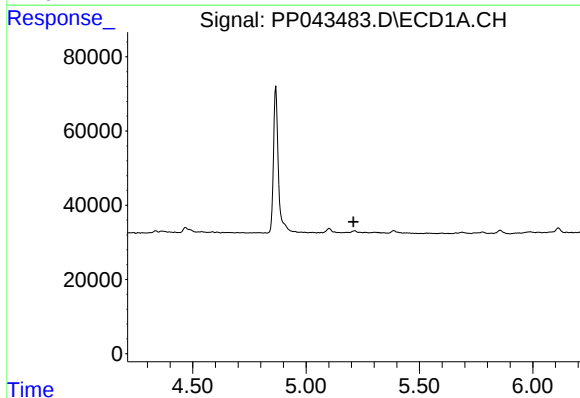


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.209 min
Response: 0
Conc: N.D.

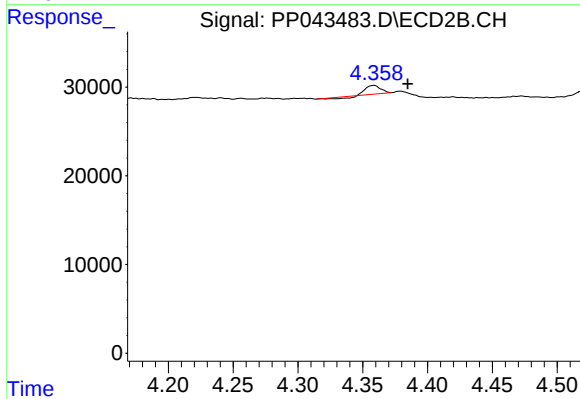

#9 AR-1221-2


R.T.: 4.359 min
Delta R.T.: -0.026 min
Response: 6287
Conc: 27.68 ng/ml

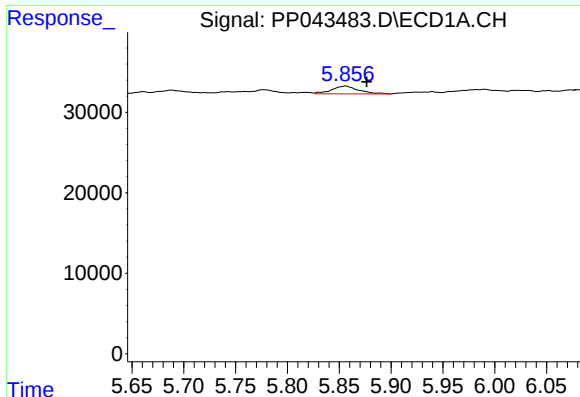

#12 AR-1232-2


R.T.: 5.857 min
Delta R.T.: -0.020 min
Response: 17388
Conc: 66.07 ng/ml

Instrument :
ECD_P
ClientSampleId :

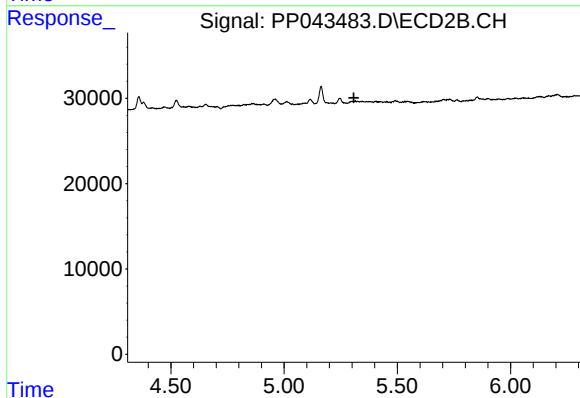


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.308 min
Response: 0
Conc: N.D.

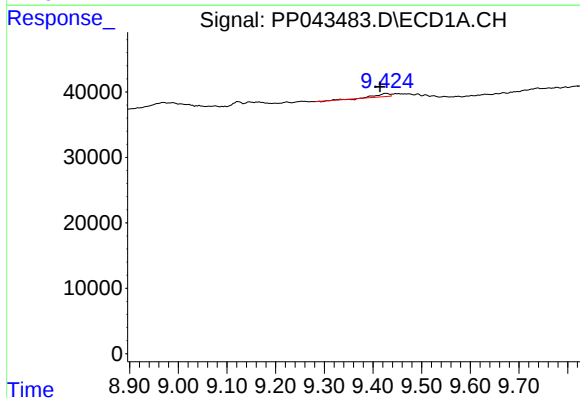


#39 AR-1262-4

R.T.: 9.428 min
Delta R.T.: 0.014 min
Response: 8068
Conc: 15.34 ng/ml

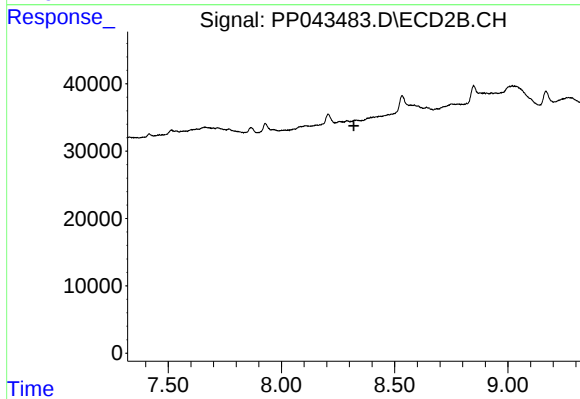

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.320 min
Response: 0
Conc: N.D.

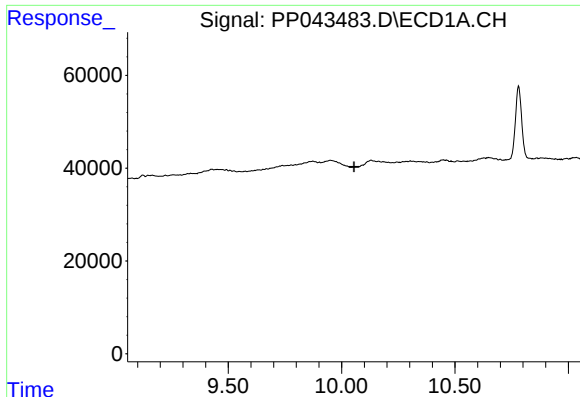

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 10.055 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

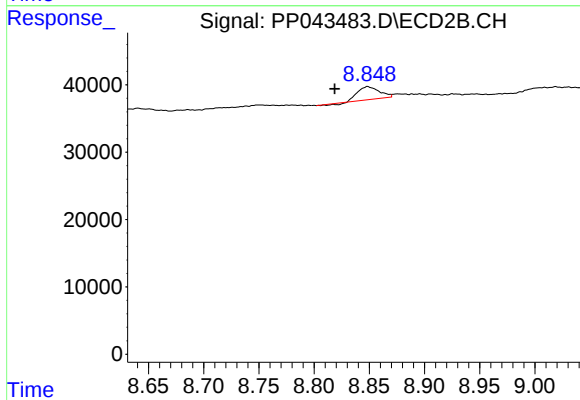


#40 AR-1262-5

R.T.: 8.849 min
Delta R.T.: 0.030 min
Response: 24545
Conc: 28.53 ng/ml

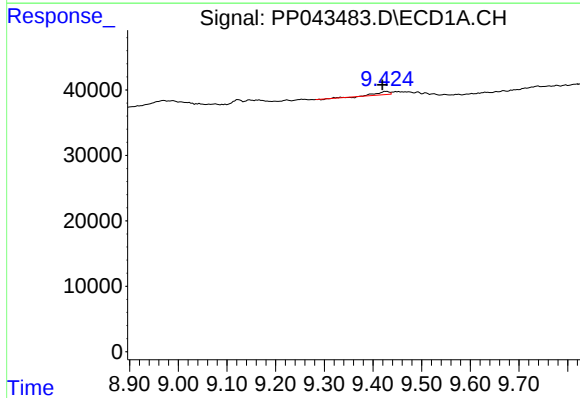


#42 AR-1268-2

R.T.: 9.428 min
Delta R.T.: 0.009 min
Response: 8068
Conc: 3.88 ng/ml

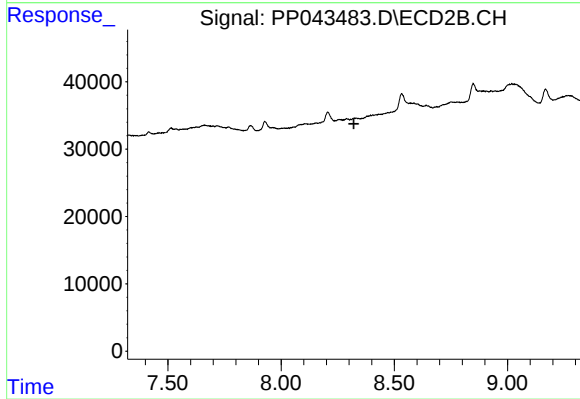

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 8.321 min
Response: 0
Conc: N.D.

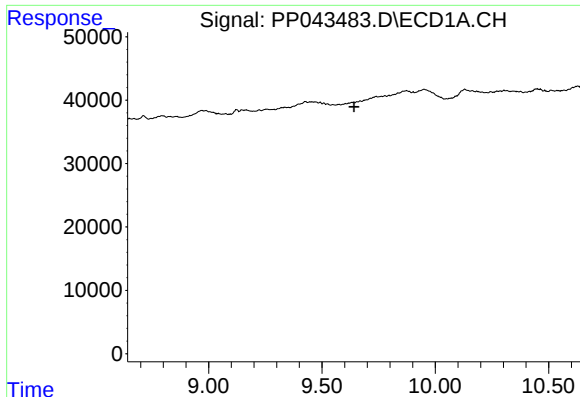

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.641 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

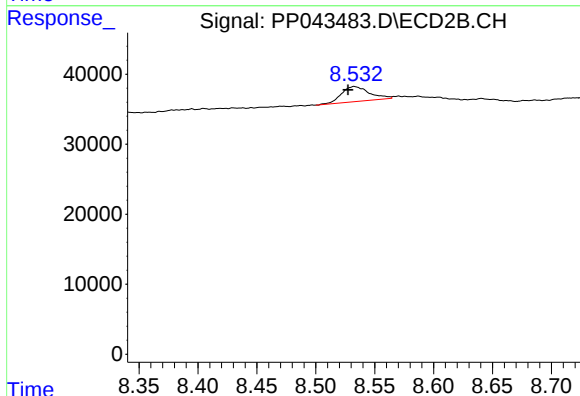


#43 AR-1268-3

R.T.: 8.533 min
Delta R.T.: 0.005 min
Response: 35518
Conc: 15.16 ng/ml

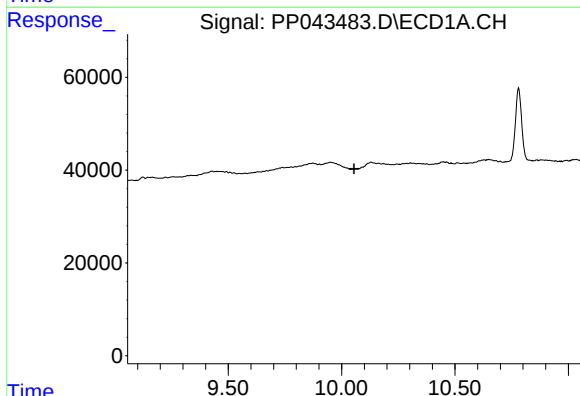

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 10.056 min
Response: 0
Conc: N.D.

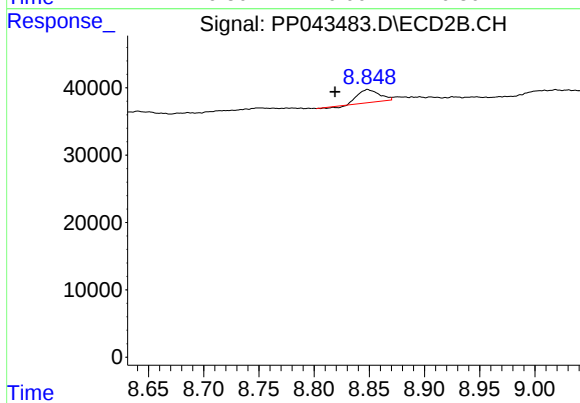

#44 AR-1268-4

R.T.: 8.849 min
Delta R.T.: 0.030 min
Response: 24545
Conc: 24.80 ng/ml