

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020325\
 Data File : PP069440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2025 01:41
 Operator : YP\AJ
 Sample : Q1269-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VNJ-231

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/04/2025
 Supervised By :Ankita Jodhani 02/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 03:31:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.537	3.840	16366600	13386032	11.433m	14.998 #
2) SA Decachlor...	10.277	8.907	10411193	10064164	9.526	8.998

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020325\
Data File : PP069440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2025 01:41
Operator : YP\AJ
Sample : Q1269-01
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
VNJ-231


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/04/2025
Supervised By :Ankita Jodhani 02/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 03:31:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

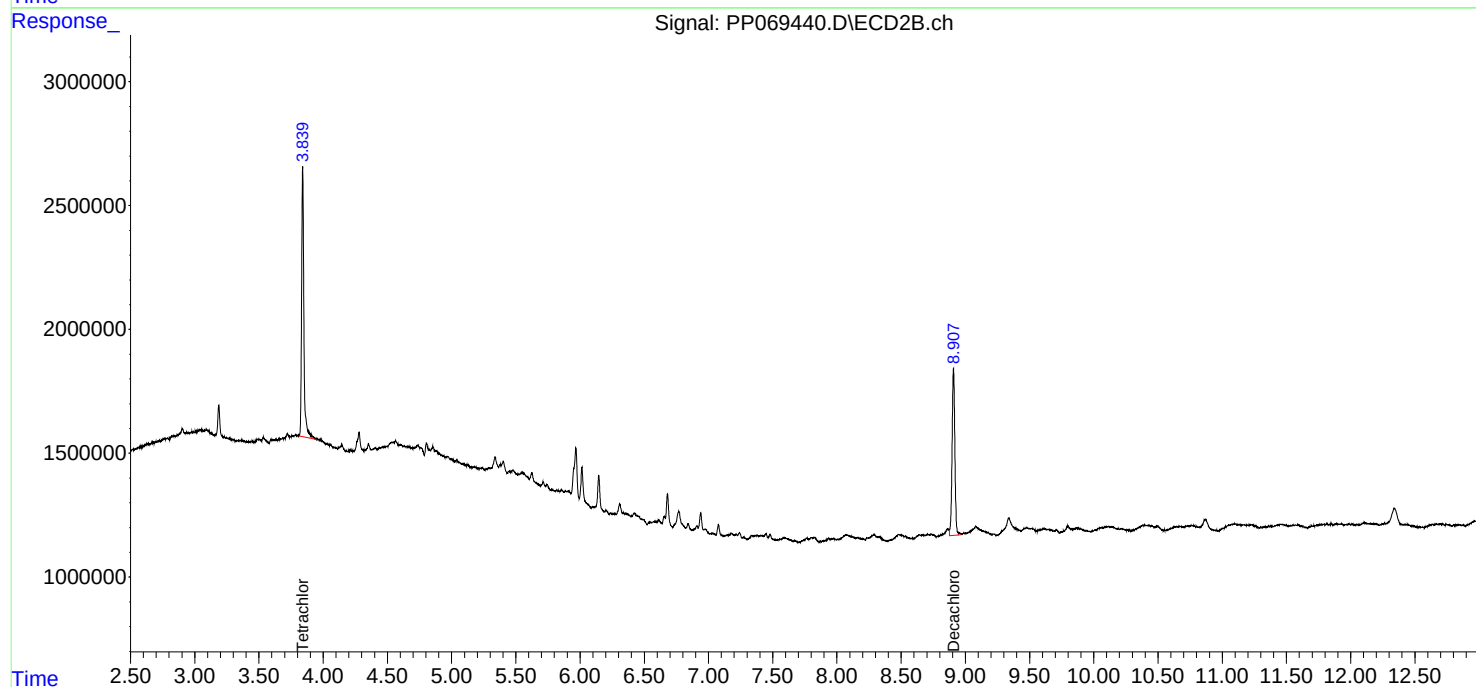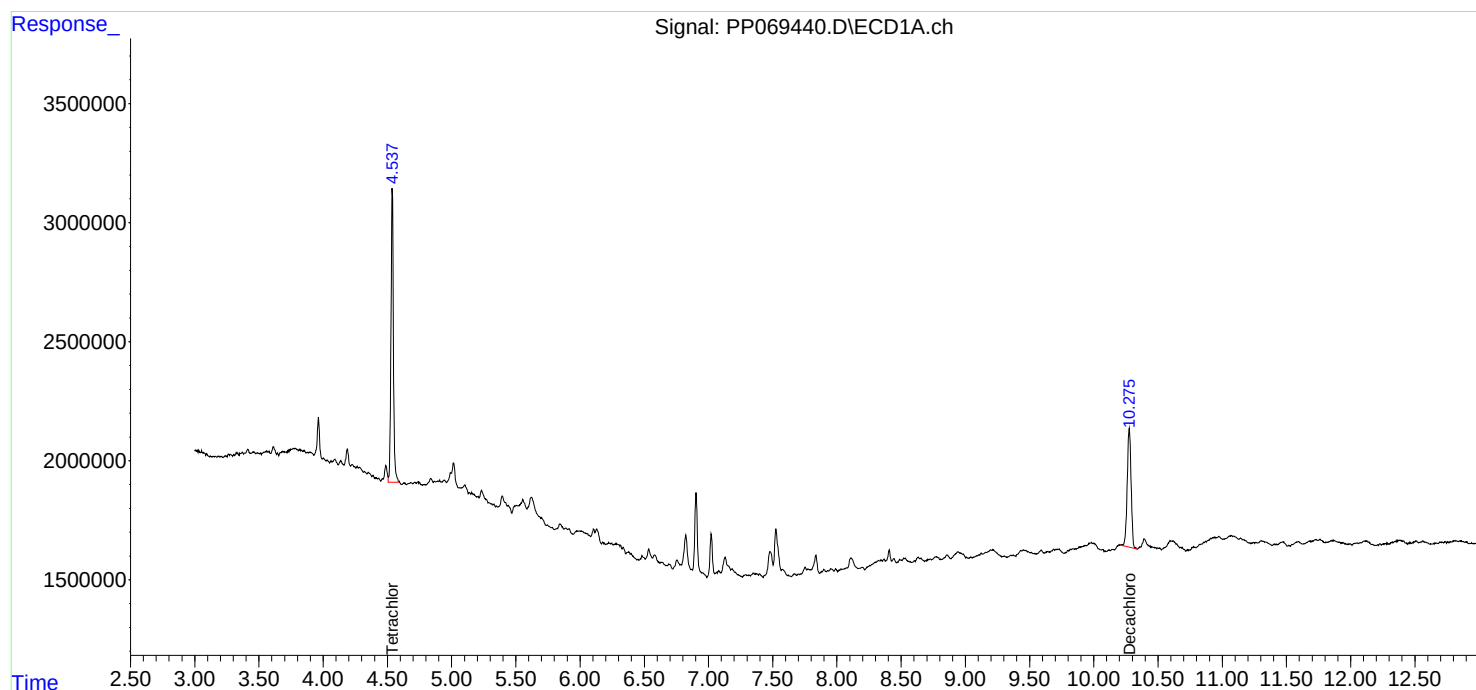

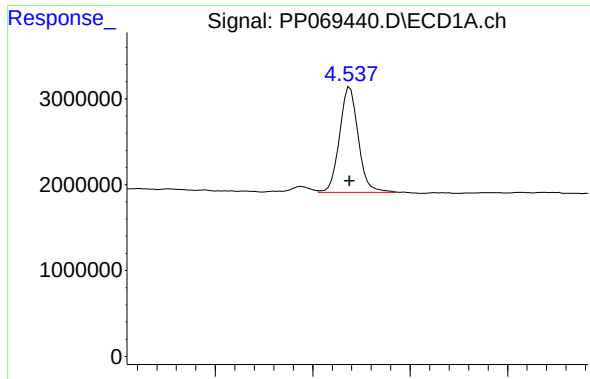


#1 Tetrachloro-m-xylene

R.T.: 4.537 min
Delta R.T.: -0.001 min
Response: 16366600
Conc: 11.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
VNJ-231


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/04/2025
Supervised By :Ankita Jodhani 02/04/2025

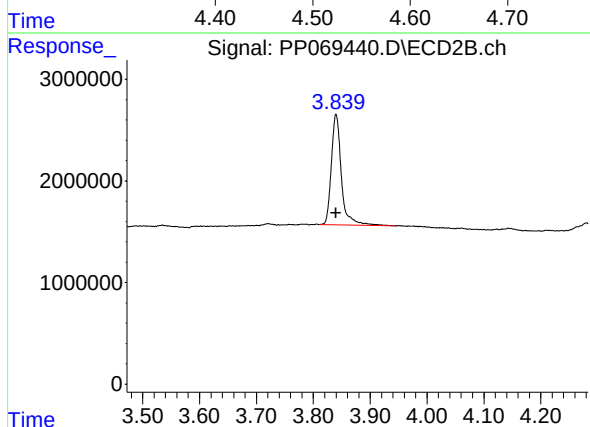


#1 Tetrachloro-m-xylene

R.T.: 3.840 min
Delta R.T.: 0.000 min
Response: 13386032
Conc: 15.00 ng/ml

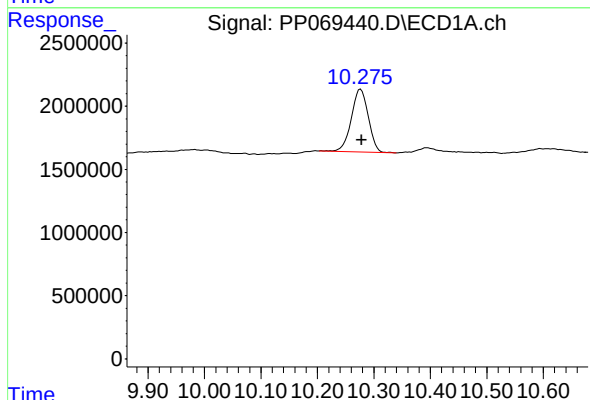

#2 Decachlorobiphenyl

R.T.: 10.277 min
Delta R.T.: -0.002 min
Response: 10411193
Conc: 9.53 ng/ml

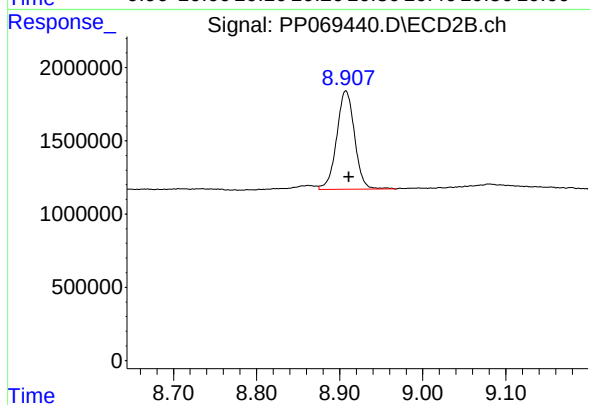

#2 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: -0.004 min
Response: 10064164
Conc: 9.00 ng/ml