

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020419\
 Data File : PP029095.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Feb 2019 21:36
 Operator : EI\MA
 Sample : K1360-04
 Misc : hexane
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 03:10:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012819.M
 Quant Title : 8080.M
 QLast Update : Mon Jan 28 11:24:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.002	12.156	169.9E6	235.2E6	670.879	571.032
Target Compounds							
1) T	Dalapon	0.000	2.951	0	142.3E6	N.D.	246.251 #
6) T	MCCP	12.692	0.000	22382492	0	53.848	N.D. #
8) T	DICHLORPROP	0.000	13.590	0	18365559	N.D.	48.025 #
9) T	2,4-D	13.870	0.000	8175869	0	23.852	N.D. #
11) T	2,4,5-TP ...	15.218	0.000	11428349	0	4.621	N.D. #
12) T	2,4,5-T	0.000	15.874	0	13690025	N.D.	6.271 #
13) T	2,4-DB	16.332	0.000	9274812	0	58.152	N.D. #
14) T	DINOSEB	0.000	16.944	0	5969444	N.D.	3.391 #
16) T	DCPA	18.111	0.000	32716756	0	9.489	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020419\
Data File : PP029095.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Feb 2019 21:36
Operator : EI\MA
Sample : K1360-04
Misc : hexane
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 03:10:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012819.M
Quant Title : 8080.M
QLast Update : Mon Jan 28 11:24:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

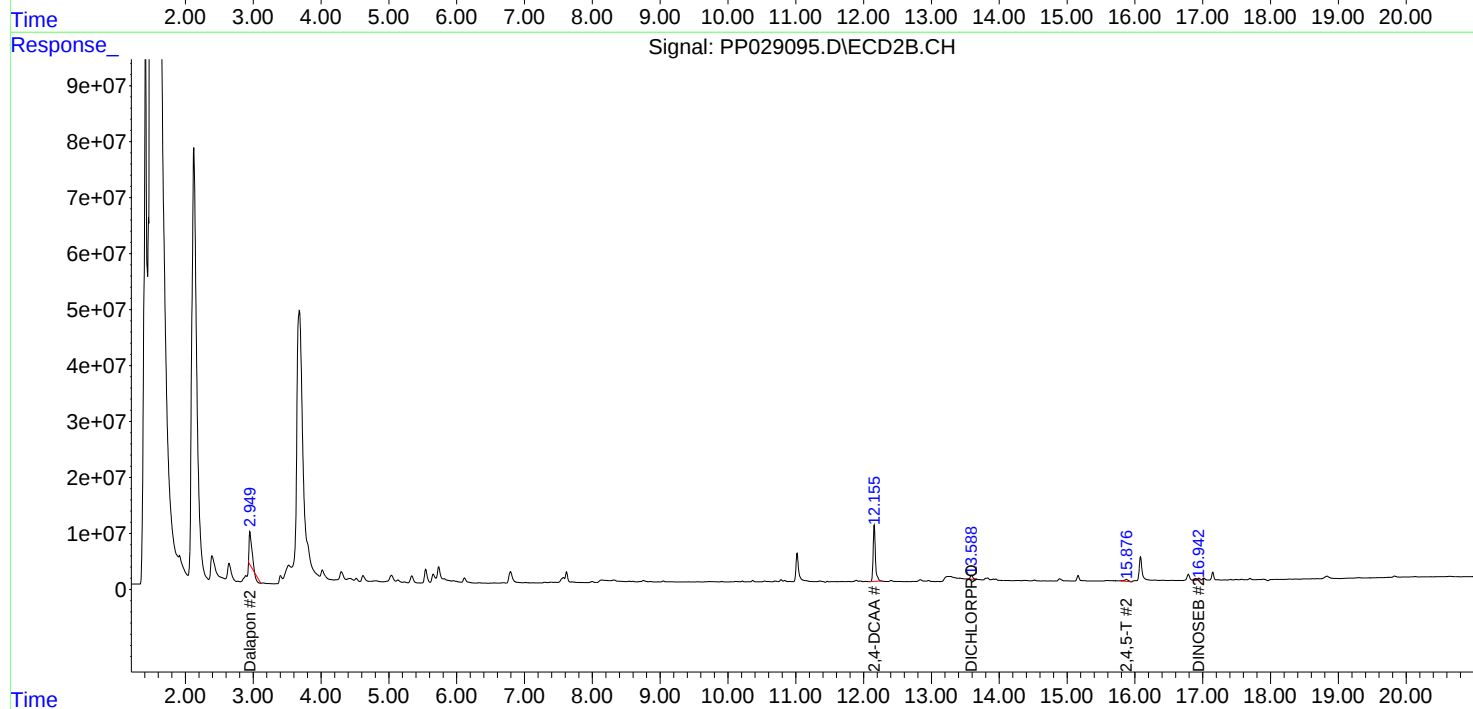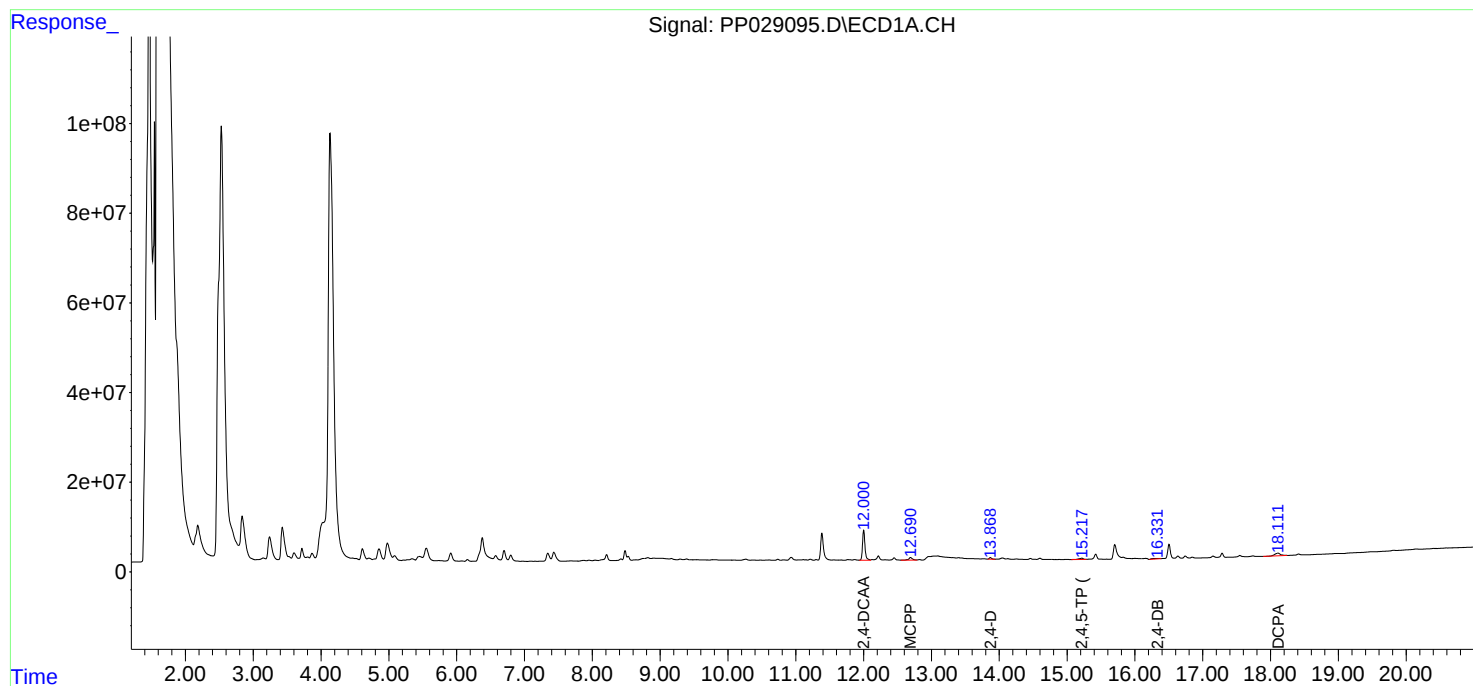


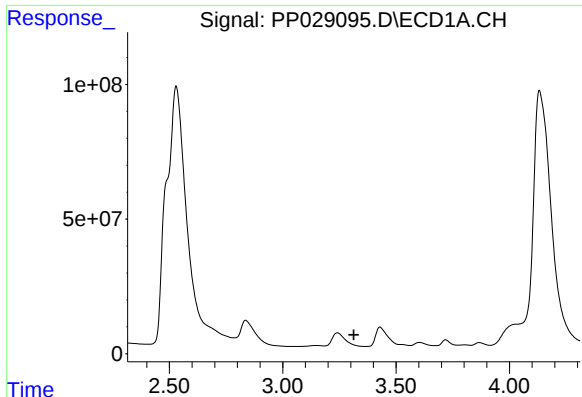

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

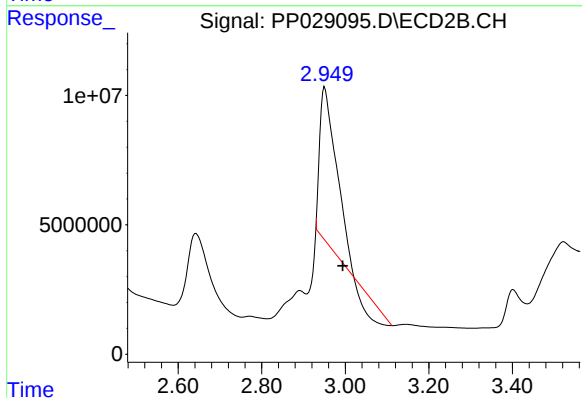


#1 Dalapon

R.T.: 2.951 min
Delta R.T.: -0.043 min
Response: 142271777
Conc: 246.25 ng/ml

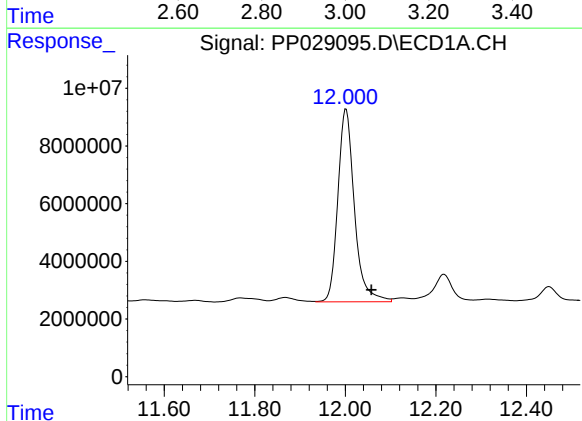


#4 2,4-DCAA

R.T.: 12.002 min
Delta R.T.: -0.056 min
Response: 169863954
Conc: 670.88 ng/ml

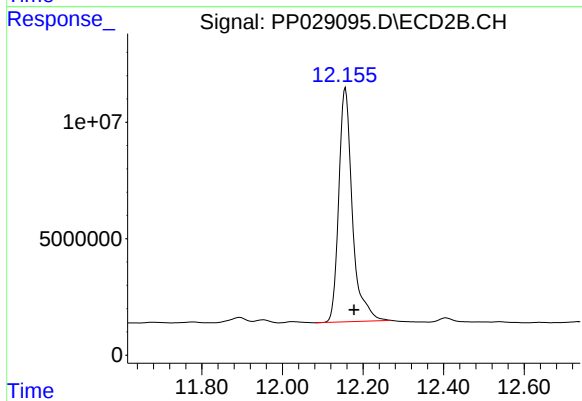

#4 2,4-DCAA


R.T.: 12.156 min
Delta R.T.: -0.021 min
Response: 235154287
Conc: 571.03 ng/ml

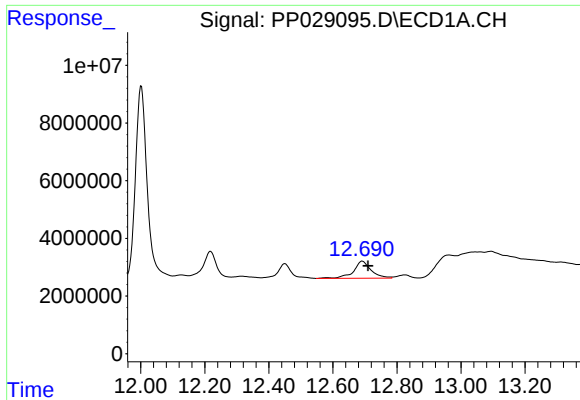

#6 MCP


R.T.: 12.692 min
Delta R.T.: -0.018 min
Response: 22382492
Conc: 53.85 ug/ml

Instrument :
ECD_P
ClientSampleId :

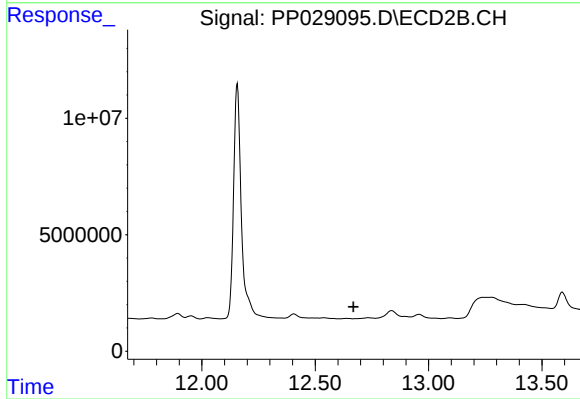


#6 MCP

R.T.: 0.000 min
Exp R.T. : 12.669 min
Response: 0
Conc: N.D.

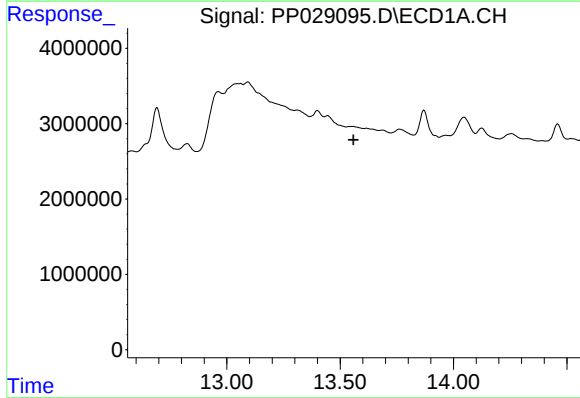


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.559 min
Response: 0
Conc: N.D.

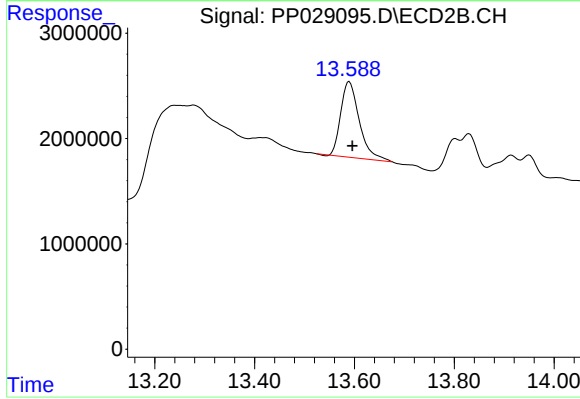

#8 DICHLORPROP


R.T.: 13.590 min
Delta R.T.: -0.006 min
Response: 18365559
Conc: 48.02 ng/ml

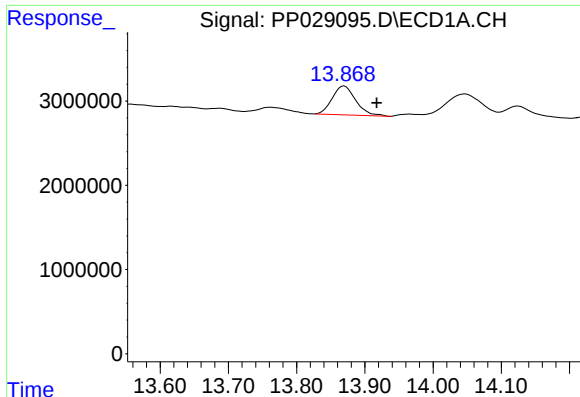

#9 2,4-D


R.T.: 13.870 min
Delta R.T.: -0.048 min
Response: 8175869
Conc: 23.85 ng/ml

Instrument :
ECD_P
ClientSampleId :

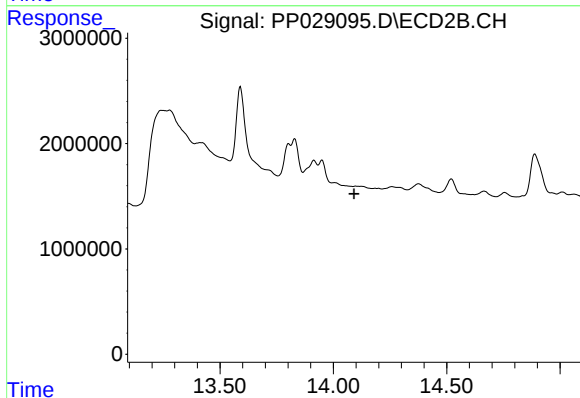


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 14.092 min
Response: 0
Conc: N.D.

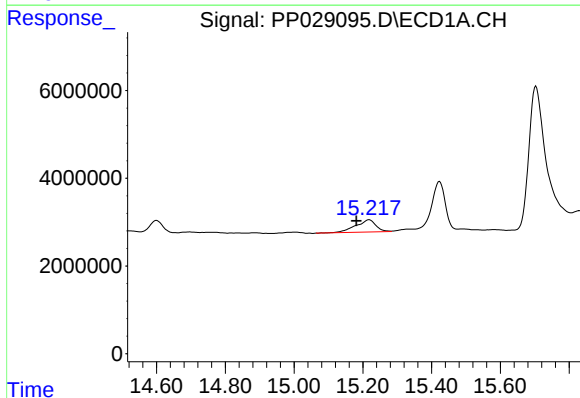


#11 2,4,5-TP (SILVEX)

R.T.: 15.218 min
Delta R.T.: 0.037 min
Response: 11428349
Conc: 4.62 ng/ml

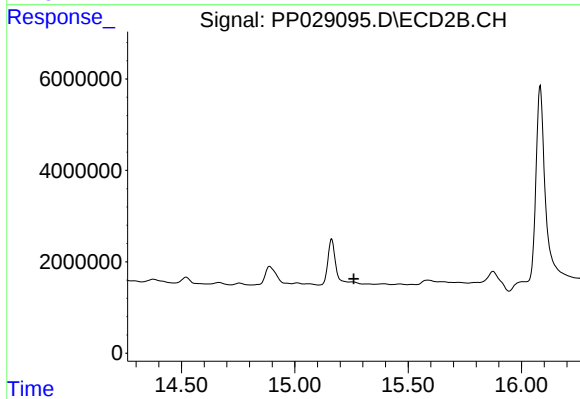

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 15.260 min
Response: 0
Conc: N.D.

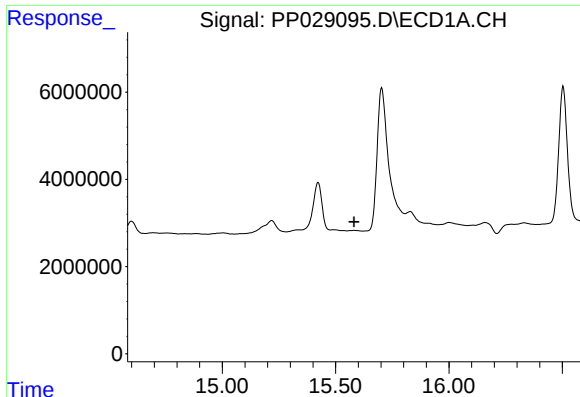

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.581 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

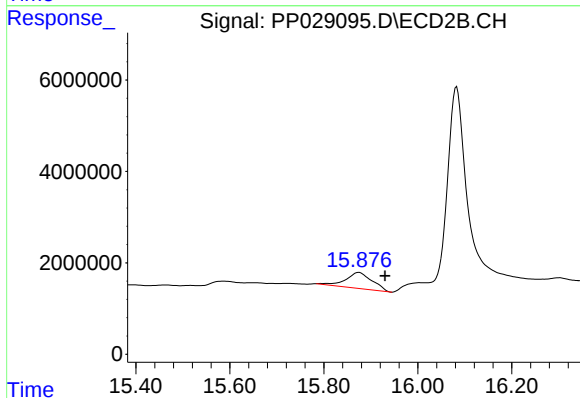


#12 2,4,5-T

R.T.: 15.874 min
Delta R.T.: -0.055 min
Response: 13690025
Conc: 6.27 ng/ml

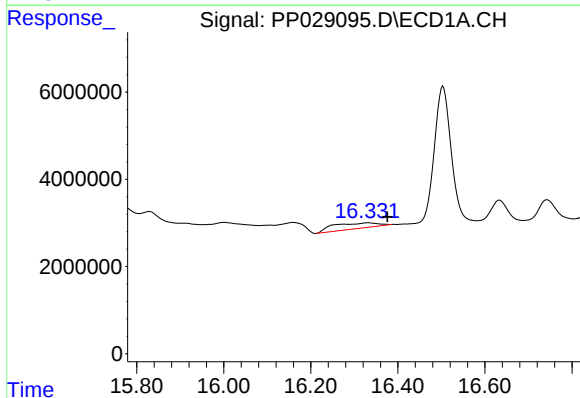


#13 2,4-DB

R.T.: 16.332 min
Delta R.T.: -0.045 min
Response: 9274812
Conc: 58.15 ng/ml

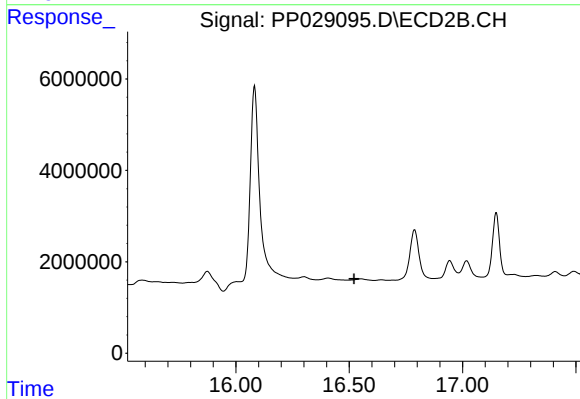

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.522 min
Response: 0
Conc: N.D.

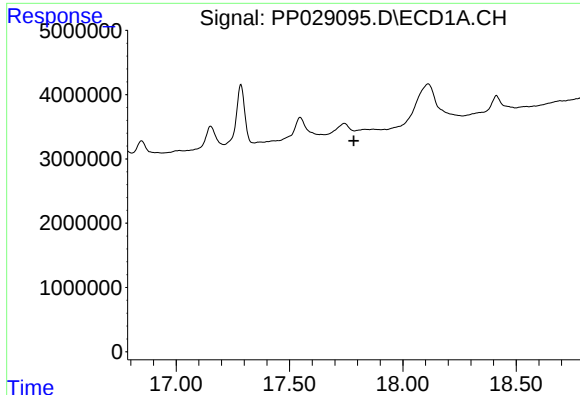

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.784 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

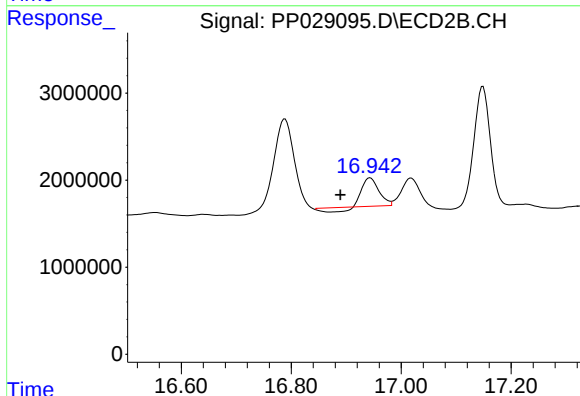


#14 DINOSEB

R.T.: 16.944 min
Delta R.T.: 0.054 min
Response: 5969444
Conc: 3.39 ng/ml

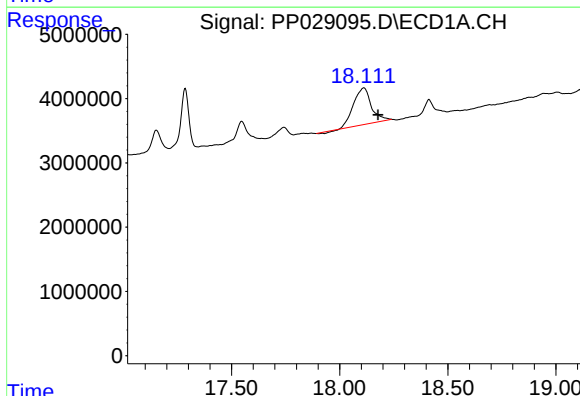

#16 DCPA

R.T.: 18.111 min
Delta R.T.: -0.066 min
Response: 32716756
Conc: 9.49 ng/ml

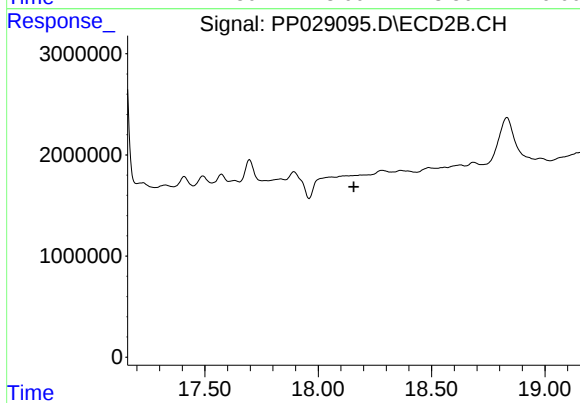

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 18.157 min
Response: 0
Conc: N.D.