

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020524\
 Data File : PP063273.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2024 15:05
 Operator : YP\AJ
 Sample : P1359-02 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC271332-1-2

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/06/2024
 Supervised By :Sohil Jodhani 02/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 21:06:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 05 12:13:11 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.492	3.646	3641399	3496904	1.522	1.471
2) SA Decachlor...	10.361	8.695	19095659	4724597	8.491m	1.907m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020524\
Data File : PP063273.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2024 15:05
Operator : YP\AJ
Sample : P1359-02 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC271332-1-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/06/2024
Supervised By :Sohil Jodhani 02/06/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 21:06:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 05 12:13:11 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

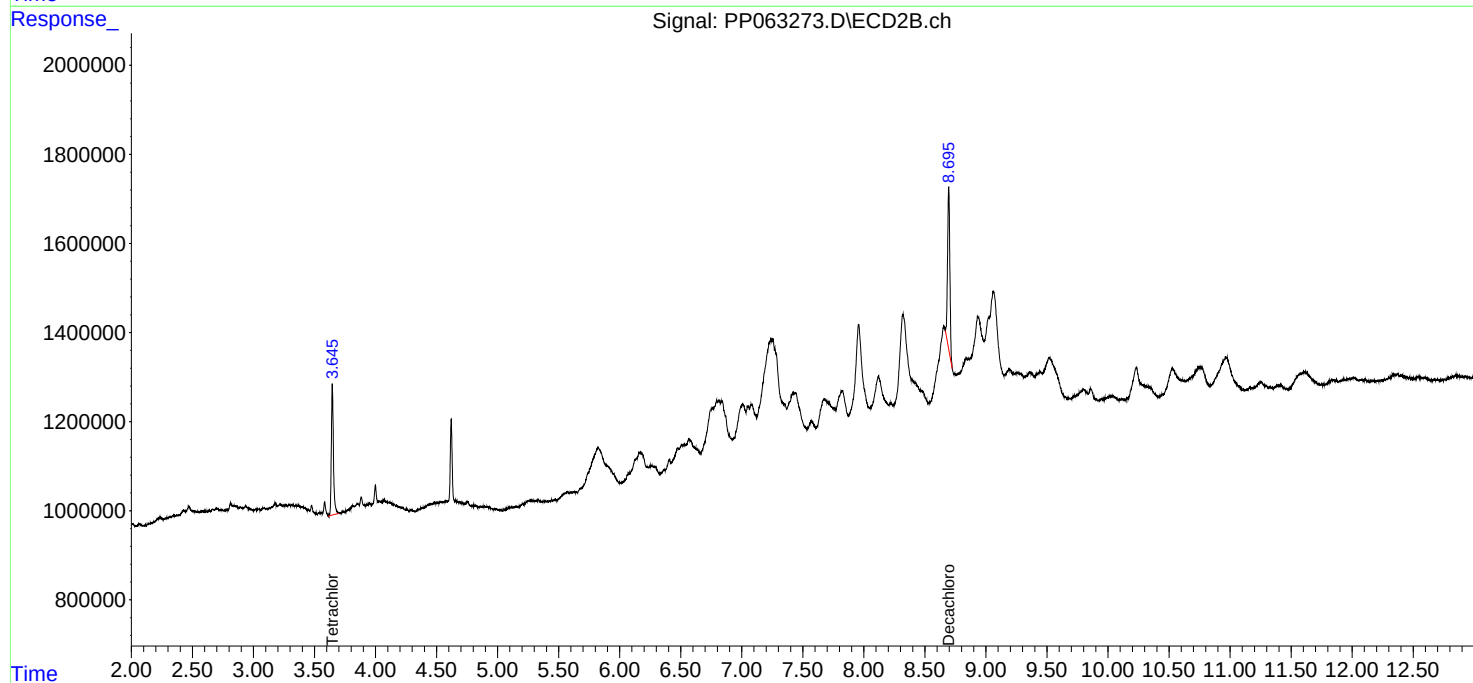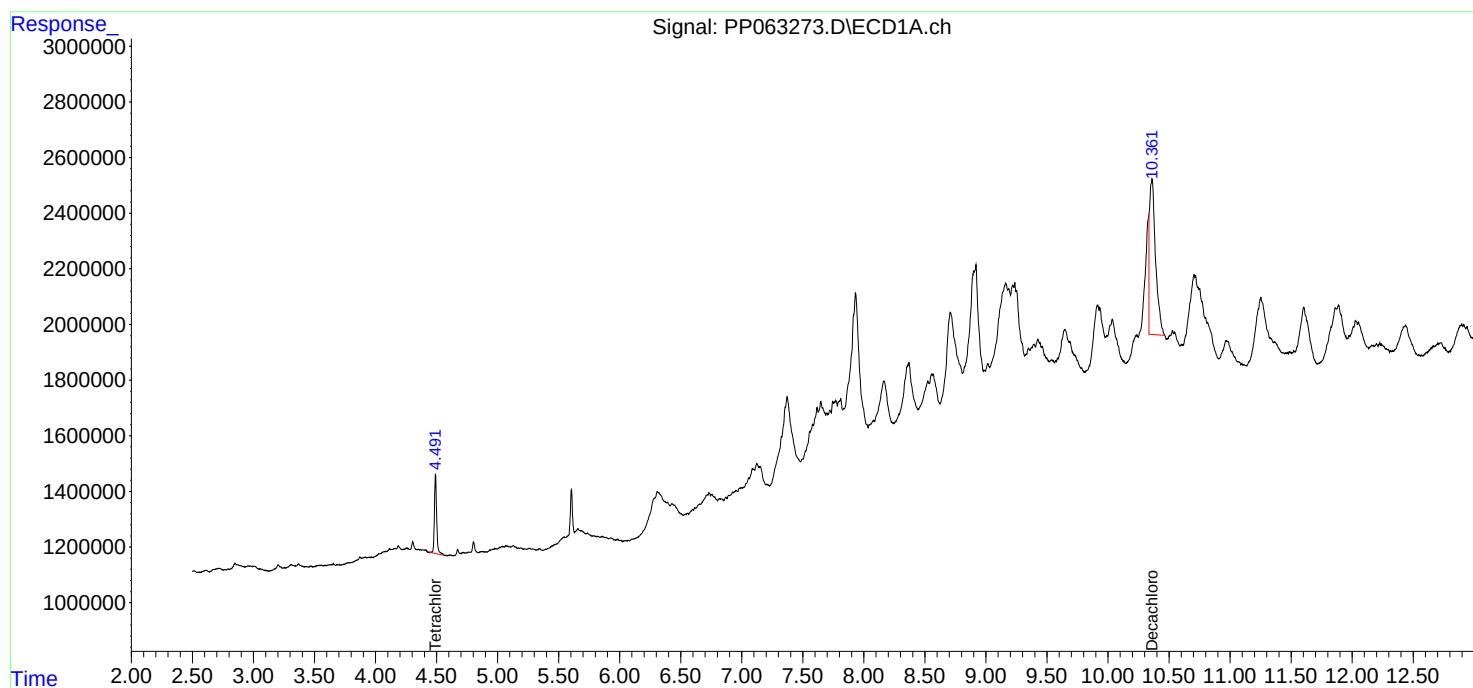

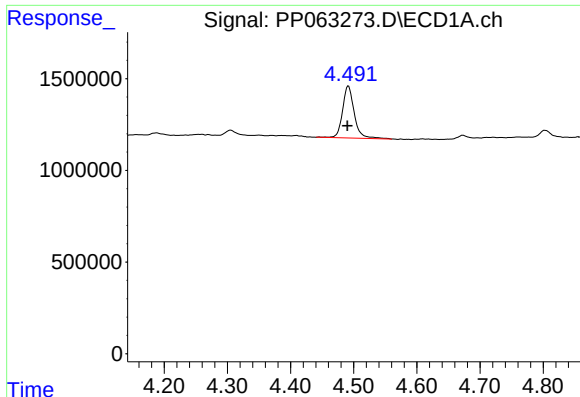


#1 Tetrachloro-m-xylene

R.T.: 4.492 min
Delta R.T.: 0.002 min
Response: 3641399
Conc: 1.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC271332-1-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/06/2024
Supervised By :Sohil Jodhani 02/06/2024

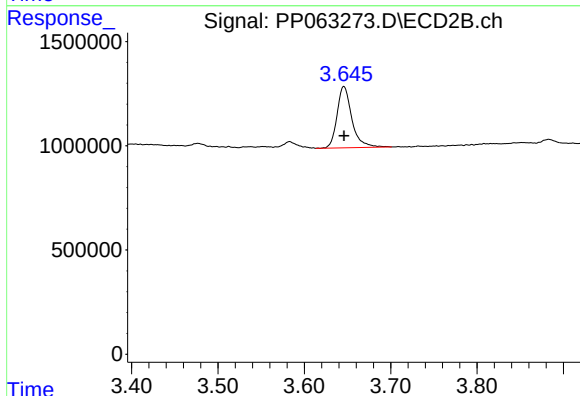


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 3496904
Conc: 1.47 ng/ml

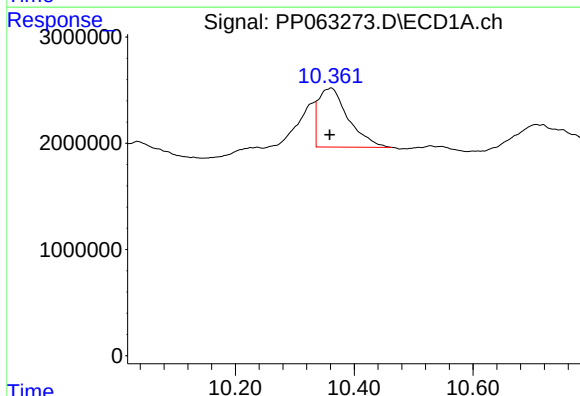

#2 Decachlorobiphenyl

R.T.: 10.361 min
Delta R.T.: 0.002 min
Response: 19095659
Conc: 8.49 ng/ml m

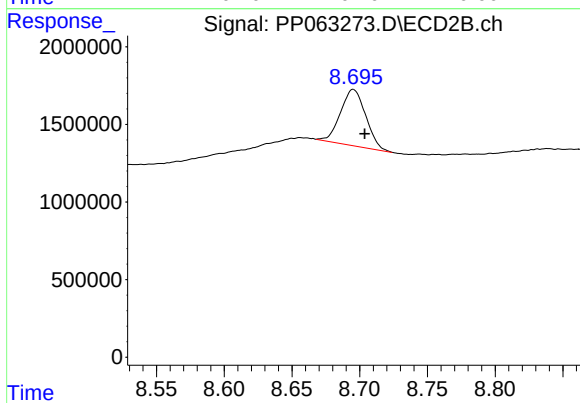

#2 Decachlorobiphenyl

R.T.: 8.695 min
Delta R.T.: -0.008 min
Response: 4724597
Conc: 1.91 ng/ml m