

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020524\
 Data File : PP063291.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2024 20:28
 Operator : YP\AJ
 Sample : P1333-12 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KMH382K-2-1

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/06/2024
 Supervised By :Sohil Jodhani 02/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 00:58:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 05 12:13:11 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.489	3.642	3464492	3463652	1.448m	1.457
2) SA Decachlor...	10.365	8.696	4521200	3799760	2.010	1.534

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020524\
Data File : PP063291.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2024 20:28
Operator : YP\AJ
Sample : P1333-12 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KMH382K-2-1


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/06/2024
Supervised By :Sohil Jodhani 02/06/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 00:58:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 05 12:13:11 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

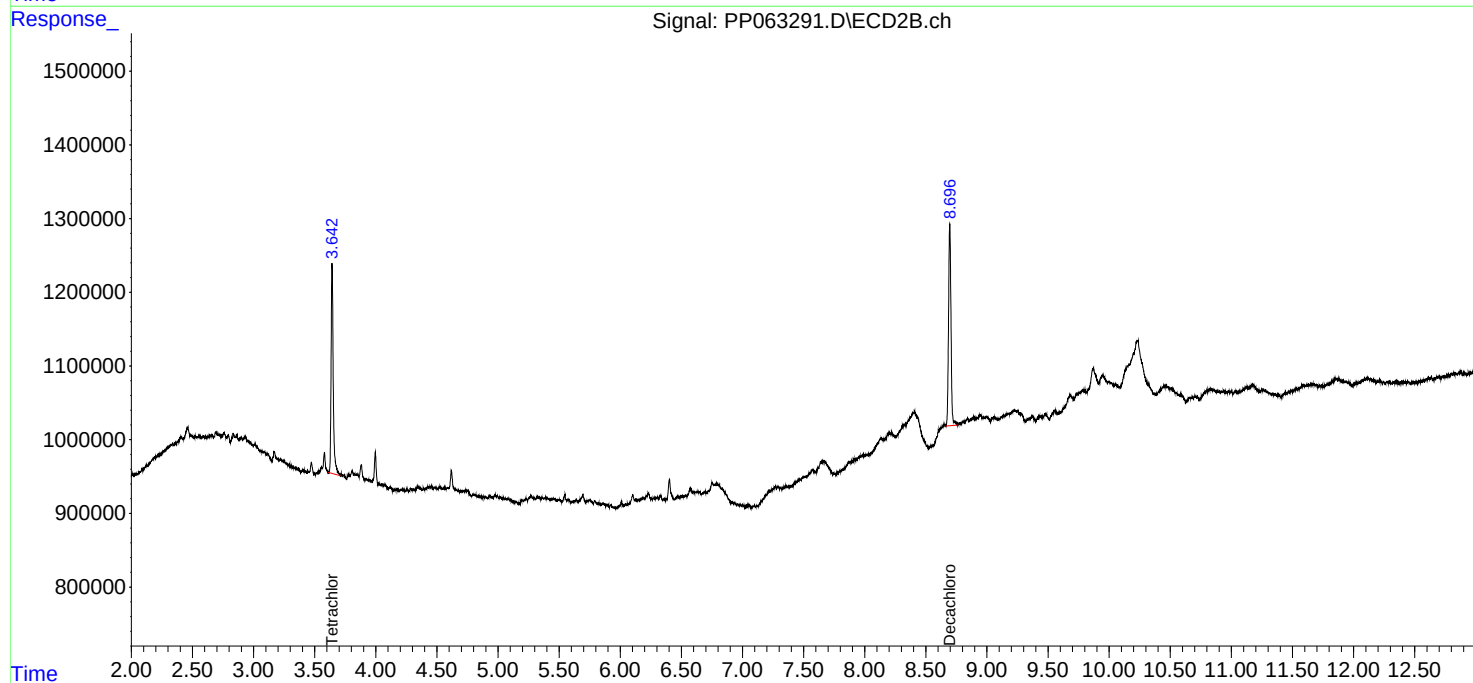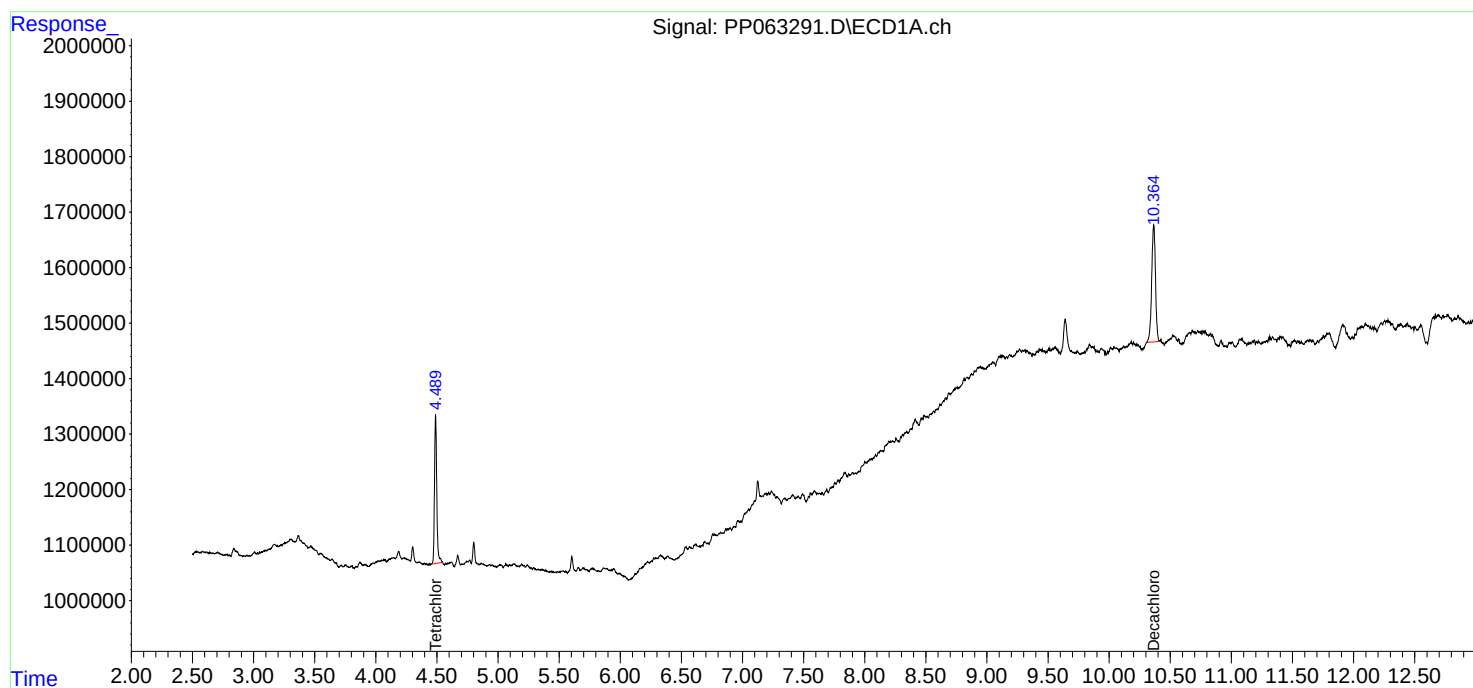

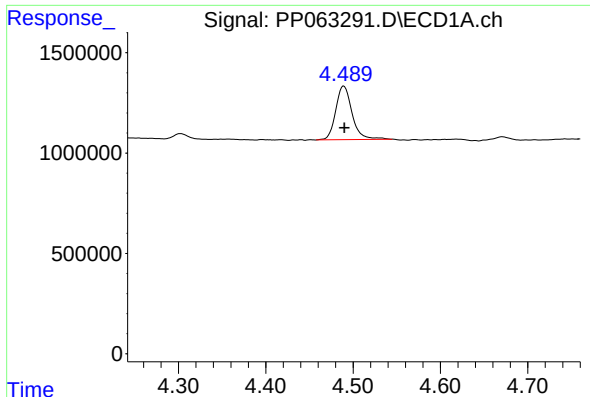


#1 Tetrachloro-m-xylene

R.T.: 4.489 min
Delta R.T.: -0.001 min
Response: 3464492
Conc: 1.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
KMH382K-2-1


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/06/2024
Supervised By :Sohil Jodhani 02/06/2024

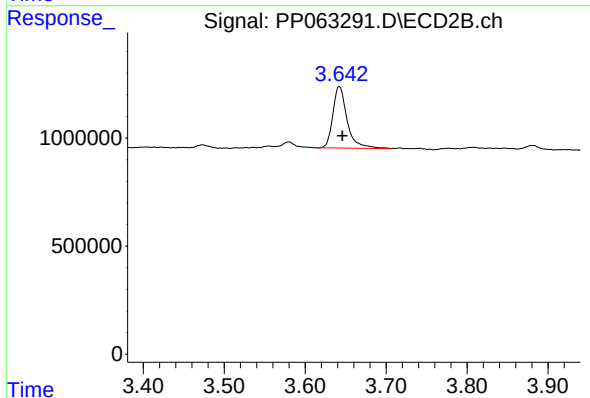


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.004 min
Response: 3463652
Conc: 1.46 ng/ml

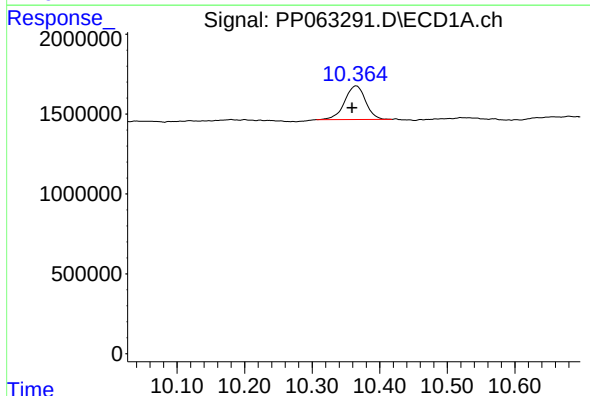

#2 Decachlorobiphenyl

R.T.: 10.365 min
Delta R.T.: 0.006 min
Response: 4521200
Conc: 2.01 ng/ml

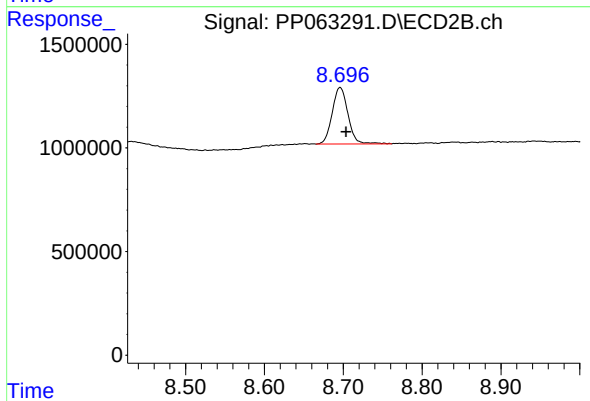

#2 Decachlorobiphenyl

R.T.: 8.696 min
Delta R.T.: -0.008 min
Response: 3799760
Conc: 1.53 ng/ml