

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020525\
 Data File : PP069498.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2025 14:16
 Operator : YP\AJ
 Sample : Q1287-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BAY-DRUMS-A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/06/2025
 Supervised By :Ankita Jodhani 02/06/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 02:21:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.531	3.837	30818561	23223812	21.529m	26.020
2) SA Decachlor...	10.261	8.900	20716216	16786748	18.955m	15.008

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020525\
Data File : PP069498.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2025 14:16
Operator : YP\AJ
Sample : Q1287-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BAY-DRUMS-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/06/2025
Supervised By :Ankita Jodhani 02/06/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 02:21:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

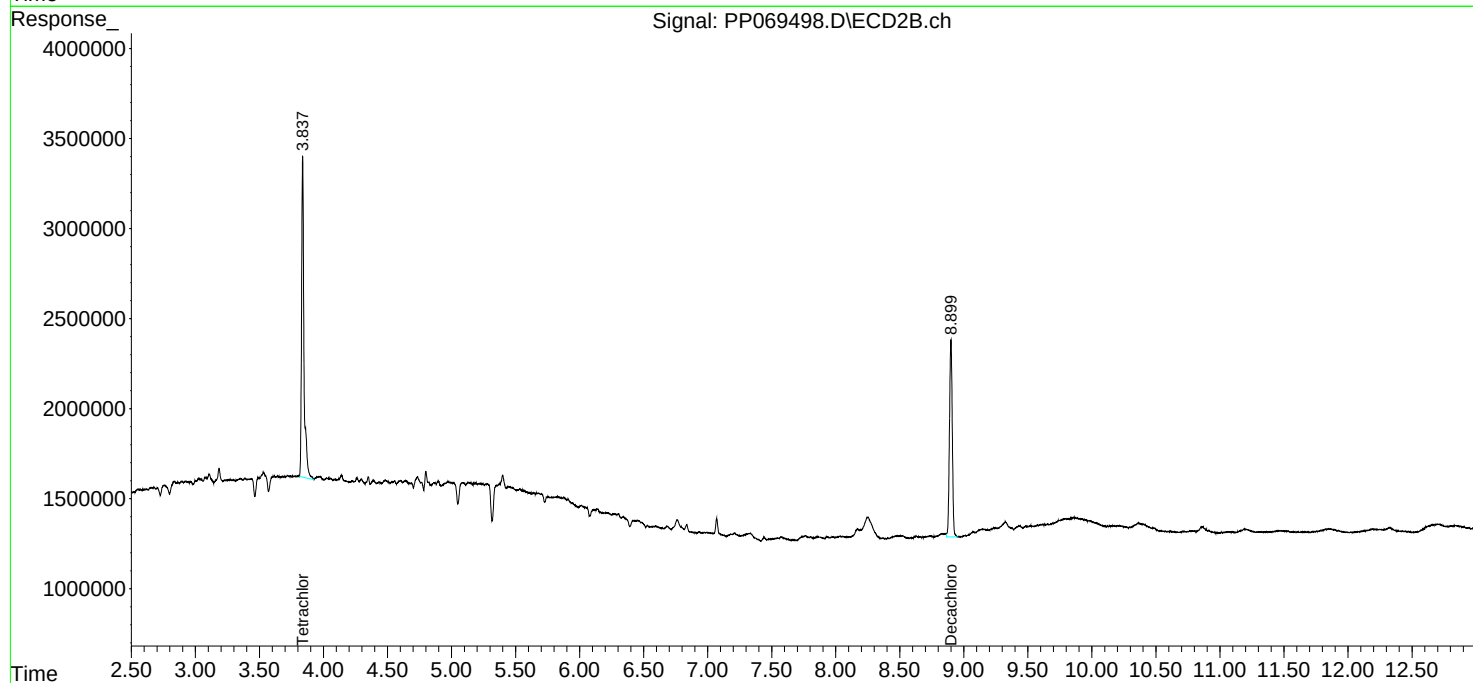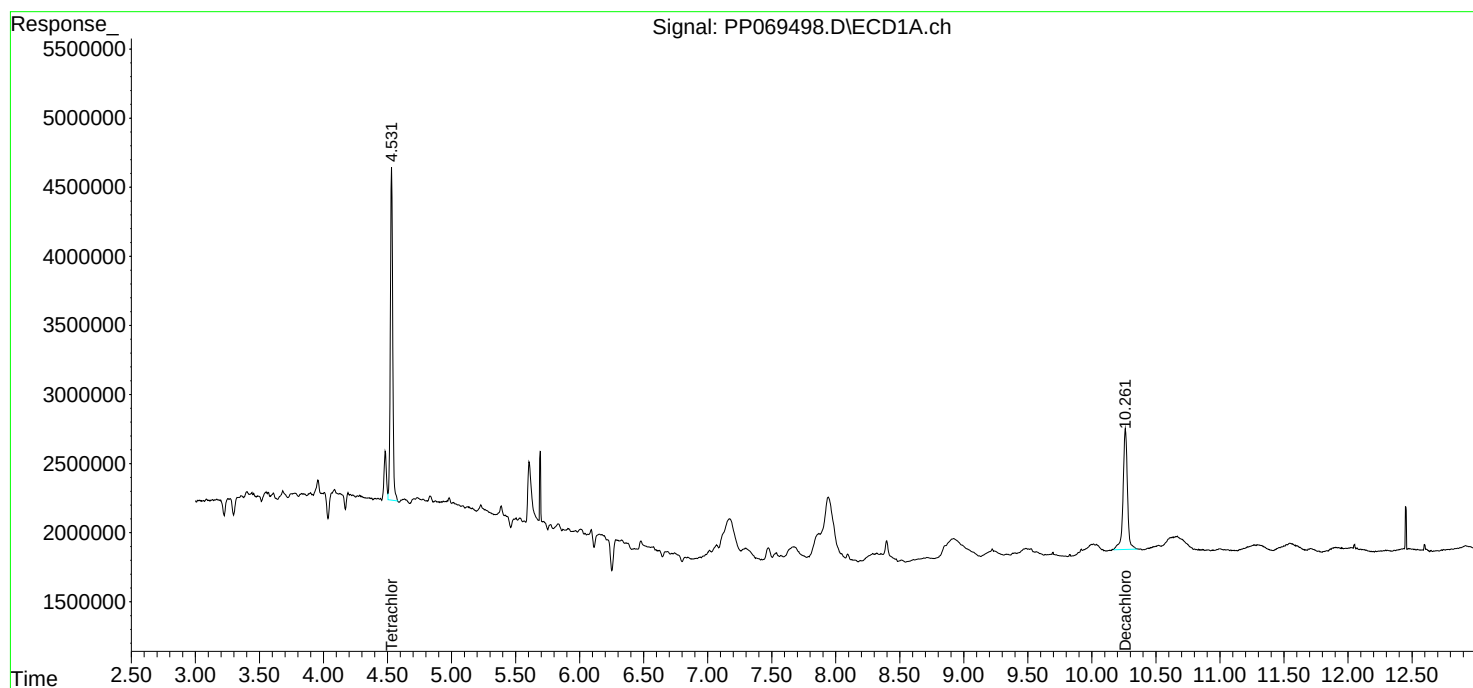

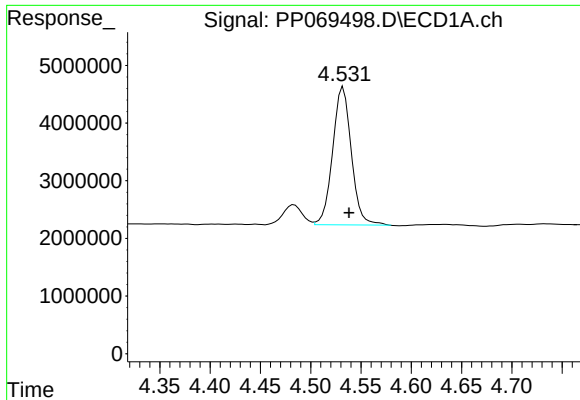


#1 Tetrachloro-m-xylene

R.T.: 4.531 min
Delta R.T.: -0.007 min
Response: 30818561
Conc: 21.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
BAY-DRUMS-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/06/2025
Supervised By :Ankita Jodhani 02/06/2025

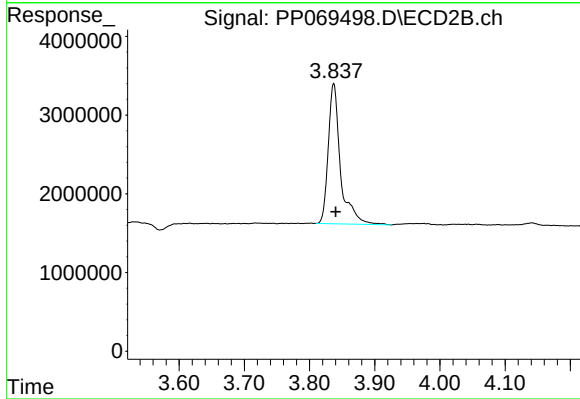


#1 Tetrachloro-m-xylene

R.T.: 3.837 min
Delta R.T.: -0.003 min
Response: 23223812
Conc: 26.02 ng/ml

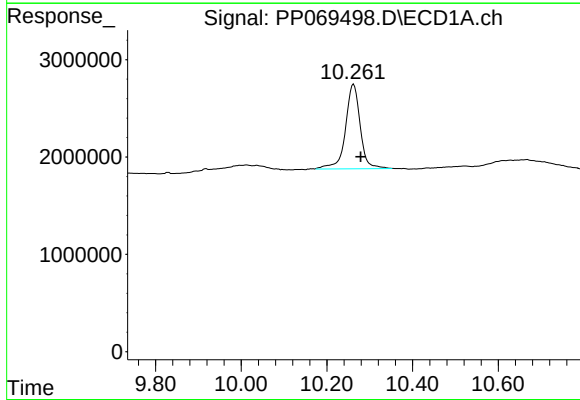

#2 Decachlorobiphenyl

R.T.: 10.261 min
Delta R.T.: -0.018 min
Response: 20716216
Conc: 18.96 ng/ml m

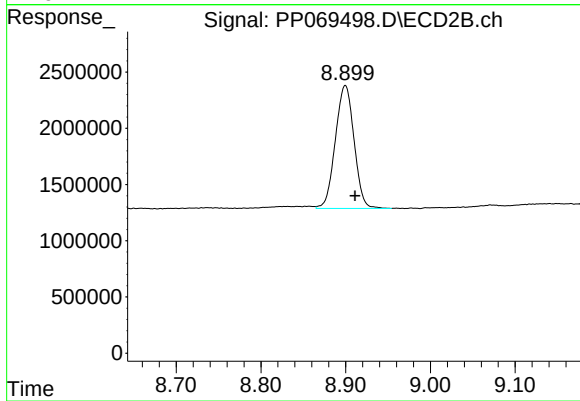

#2 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: -0.012 min
Response: 16786748
Conc: 15.01 ng/ml