

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020525\
 Data File : PP069530.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2025 00:00
 Operator : YP\AJ
 Sample : Q1305-05 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 Y2308-0040-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/06/2025
 Supervised By :Ankita Jodhani 02/06/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 02:30:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.531	3.838	3859107	2386089	2.696	2.673m
2) SA Decachlor...	10.262	8.900	3311605	2442119	3.030m	2.183m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020525\
Data File : PP069530.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2025 00:00
Operator : YP\AJ
Sample : Q1305-05 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
Y2308-0040-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/06/2025
Supervised By :Ankita Jodhani 02/06/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 02:30:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

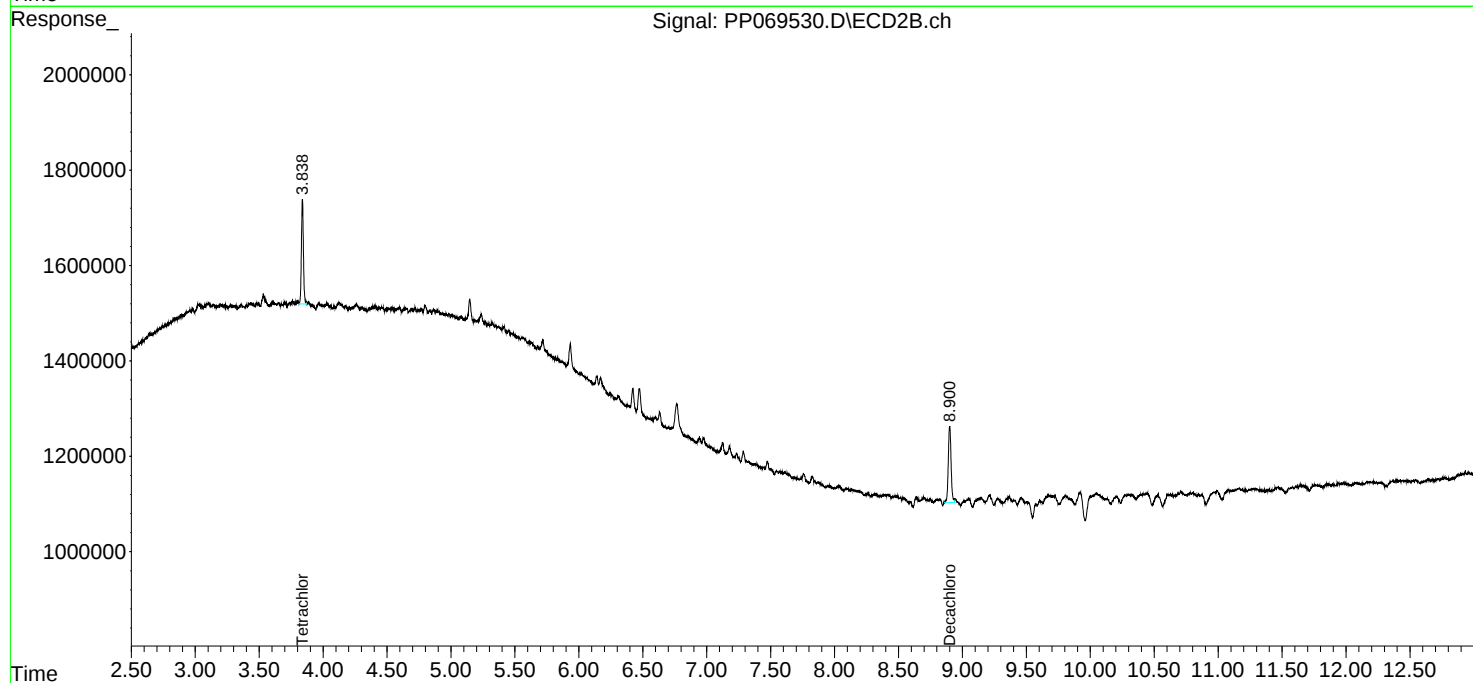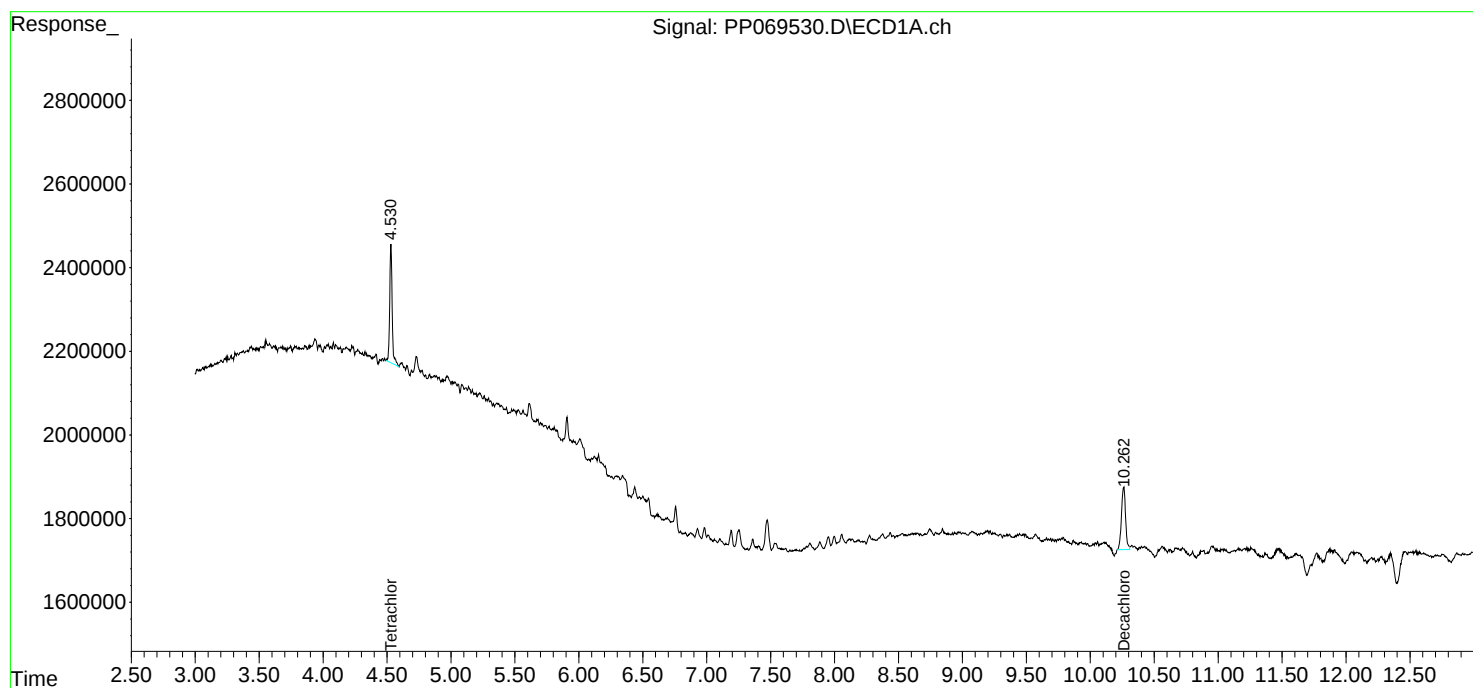

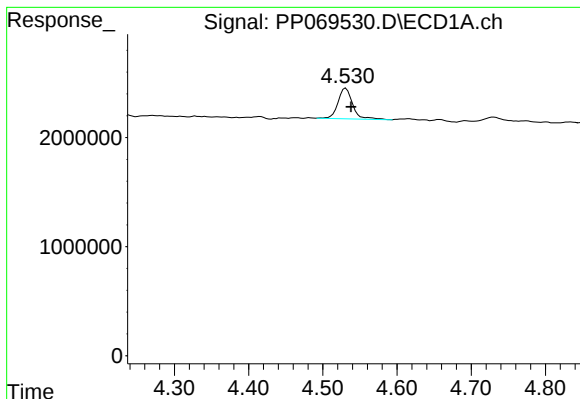


#1 Tetrachloro-m-xylene

R.T.: 4.531 min
Delta R.T.: -0.007 min
Response: 3859107
Conc: 2.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
Y2308-0040-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/06/2025
Supervised By :Ankita Jodhani 02/06/2025

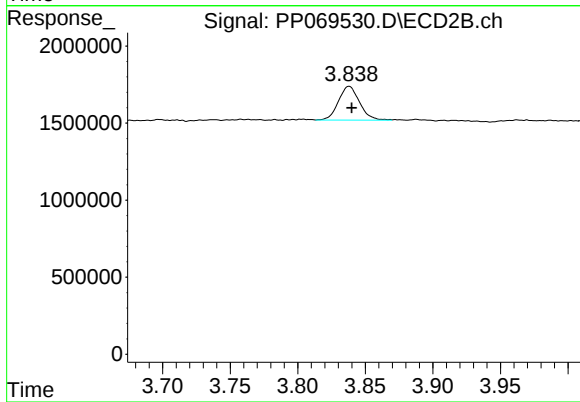


#1 Tetrachloro-m-xylene

R.T.: 3.838 min
Delta R.T.: -0.002 min
Response: 2386089
Conc: 2.67 ng/ml m

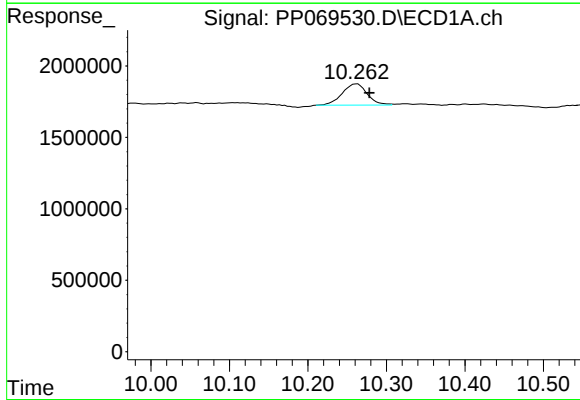

#2 Decachlorobiphenyl

R.T.: 10.262 min
Delta R.T.: -0.016 min
Response: 3311605
Conc: 3.03 ng/ml m

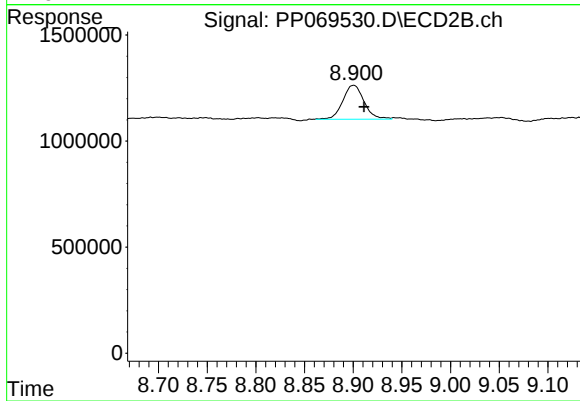

#2 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: -0.011 min
Response: 2442119
Conc: 2.18 ng/ml m